

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

CERTIFICATE OF CALIBRATION

Issued to: DIV20 B57 NARASI SRIDHAR

Device No: 2420

Manufacturer: BINKS

Model: 100 PSI

Nomenclature: PRESSURE GAUGE

Serial Number: 1593002

SwRI No: NONE

Cal interval 12 Mo.

Remarks

Accuracy: MFGR

Procedure: MFGR

ENVIRONMENT

Temperature: 0 Humidity: 0 Location: SWRI BLDG 145


CONCLUSION

Tolerance/Remarks: Received into the system, introduced or reactivated

Standard Reading:	Unit Under Test:
10 psi	10 psi
20 psi	20 psi
30 psi	30 psi
40 psi	40 psi
50 psi	50 psi
60 psi	60 psi
70 psi	70 psi
80 psi	80 psi
90 psi	90 psi
100 psi	100 psi

Calibration was in accord with requirements of MIL-STD-45662A. Measurements are traceable to the National Institute of Standards and Technology. Inspection and test data are on file and available for inspection.

Signed

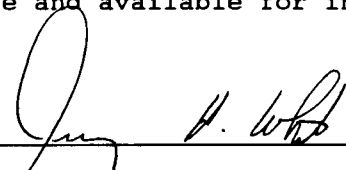

Calibration Date: 06/09/93

Cal interval: 12 Months

Record Number: 00011494

Next Calibration Due: 06/09/94

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

Device Serial No: 1593002

Calibration Date: 06/09/93

STANDARDS

Standard No: 1554 Manufacturer: AMETEK

Model: RK-300

Nomenclature: DEADWEIGHT TESTER

Serial No: 82167

Cal.Due: 03/26/94

Cal.Rec.No: 00010846

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

CERTIFICATE OF CALIBRATION

Issued to: DIV20 B57 RON GREEN

Device No: 2420

Manufacturer: BINKS

Model: 100 PSI

Nomenclature: PRESSURE GAUGE

Serial Number: 1593002

SwRI No: NONE

Cal interval 12 Mo.

Remarks

Accuracy: MFGR

Procedure: MFGR

ENVIRONMENT

Temperature:

Humidity:

Location: SWRI DIV04 BLDG. 145

CONCLUSION


Tolerance/Remarks: Received in tolerance, no adjustments made

Room Temperature.

Standard Reading:	Unit Under Test:
100 psi	100.1 psi
80 psi	80.0 psi
60 psi	60.0 psi
40 psi	40.0 psi
20 psi	20.0 psi

Calibration was in accord with requirements of MIL-STD-45662A. Measurements are traceable to the National Institute of Standards and Technology. Inspection and test data are on file and available for inspection.

Signed

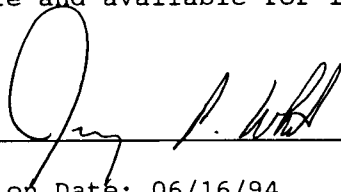

Calibration Date: 06/16/94

Cal interval: 12 Months

Record Number: 00014385

Next Calibration Due: 06/16/95

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

Device Serial No: 1593002

Calibration Date: 06/16/94

STANDARDS

Standard No: 1554 Manufacturer: AMETEK

Model: RK-300

Nomenclature: DEADWEIGHT TESTER

Serial No: 82167

Cal.Due: 02/18/95

Cal.Rec.No: 00013739

SOUTHWEST RESEARCH INSTITUTE
Department of Quality Assurance
Calibration Laboratory

CERTIFICATE OF CALIBRATION
06/21/95

Issued to: **RON GREEN** **DIV20** **,B57**
Manufacturer: **BINKS**
Nomenclature: **PRESSURE GAUGE**
Serial Number: **1593002**
Notes:

Asset Number: **002420**
Model Number: **100 PSI**

SwRI/Div. I.D. #: **NONE**

ENVIRONMENTAL CONDITIONS

Temperature: **65.0F**

Relative Humidity: **65%**

CALIBRATION INFORMATION


Procedure Number: **MFGR**
Remarks: **ERROR LESS THAN +/-1.0PSI**

Accuracy: **MFGR SPECS**
Received IN **Tolerance**

Calibration was in accordance with requirements of MIL-STD-45662A. Measurements are traceable to the National Institute of Standards and Technology. Inspection and test data are on file and available for inspection.

STANDARDS USED FOR CERTIFICATION

Asset #	Serial #	Mfg	Model #	Nomenclature	Cal Date	Int.	Cal Due
001554	82167	AMETE	RK-300	DEADWEIGHT TESTER	03/02/95	12	03/02/96

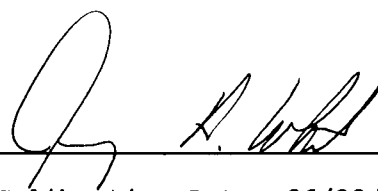Certified by : 

Certificate#: **17779**

Calibration Date: **06/20/95**
Interval: **12 months**
Next Calibration Due: **06/20/96**