

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

CERTIFICATE OF CALIBRATION

Issued to: DIV20 B51 KRISTI MEYER

Device No: 2867

Manufacturer: DWYER

Model: 475 MARKII

Nomenclature: DIGITAL MANOMETER

Serial Number: 356308

SwRI No: NONE

Cal interval 12 Mo.

Remarks

Accuracy: +/- .1 PSI

Procedure: SWRI

ENVIRONMENT

Temperature:

Humidity:

Location: SWRI BLDG. 145


CONCLUSION

Tolerance/Remarks: Received into the system, introduced or reactivated

Room Temperature.

Calibration was in accord with requirements of MIL-STD-45662A. Measurements are traceable to the National Institute of Standards and Technology. Inspection and test data are on file and available for inspection.

Signed

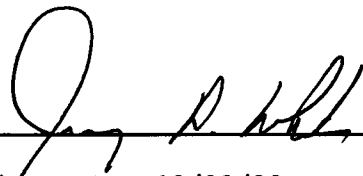

Calibration Date: 12/22/93

Cal interval: 12 Months

Record Number: 00013020

Next Calibration Due: 12/22/94

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

Device Serial No: 356308

Calibration Date: 12/22/93

STANDARDS

Standard No: 1554 Manufacturer: AMETEK

Model: RK-300

Nomenclature: DEADWEIGHT TESTER

Serial No: 82167

Cal.Due: 03/26/94

Cal.Rec.No: 00010846

SOUTHWEST RESEARCH INSTITUTE

**Department of Quality Assurance
Calibration Laboratory**

**CERTIFICATE OF CALIBRATION
12/19/94**

Issued to: KRISTI MEYER DIV20 ,B51
Manufacturer: DWYER
Nomenclature: DIGITAL MANOMETER
Serial Number: 356308

Asset Number: 002867
Model Number: 475 MARKII
SwRI Capital Number:

ENVIRONMENTAL CONDITIONS

Temperature: 69.0F

Relative Humidity: 75 %

CALIBRATION INFORMATION

Location: B184
Procedure Number: SWRI
Remarks: 5PSI READ 5.02, 10PSI READ 10.06, 15PSI READ
15.10, 19PSI READ 19.11.


Technician: 7213
Accuracy: +/- .1 PSI
Received IN Tolerance

**Calibration was in accordance with requirements of MIL-STD-45662A.
Measurements are traceable to the National Institute of Standards and Tech-
nology. Inspection and test data are on file and available for inspection.**

STANDARDS USED FOR CERTIFICATION

Asset #	Serial #	Mfg	Model #	Nomenclature	Cal Date	Int.	Cal Due
001554	82167	AMETE	RK-300	DEADWEIGHT TESTER	02/18/94	12	02/18/95

Certified by :

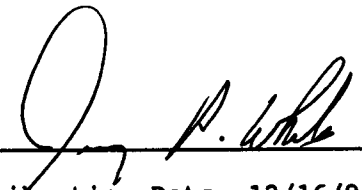

Certificate#: 16026

Calibration Date: 12/16/94
Interval: 12 months
Next Calibration Due: 12/16/95

SOUTHWEST RESEARCH INSTITUTE

**Department of Quality Assurance
Calibration Laboratory**

**CERTIFICATE OF CALIBRATION
02/13/96**

Issued to: RON GREEN DIV20 ,B57
Manufacturer/Model: DWYER/475 MARKII
Nomenclature: DIGITAL MANOMETER
Serial Number: 356308
Asset Number: 002867
Notes:

ENVIRONMENTAL CONDITIONS

Temperature: 69.0F

Relative Humidity: 27%

CALIBRATION INFORMATION

Procedure Number: SWRI
Remarks: PSI/READING, 19/19.00, 15/15.02, 10/10.01,
 5/5.00.


Accuracy: +/- .1 PSI
Received IN Tolerance

**Calibration was in accordance with requirements of MIL-STD-45662A.
Measurements are traceable to the National Institute of Standards and Tech-
nology. Inspection and test data are on file and available for inspection.**

STANDARDS USED FOR CERTIFICATION

Asset #	Serial #	Mfg	Model #	Nomenclature	Cal Date	Int.	Cal Due
004163	340119	MENSO	5000	FIELD PRESSURE STANDARD	12/06/95	3	03/06/96

Certified by :

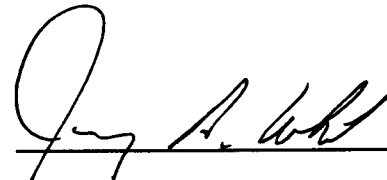

Calibration Date: 02/13/96
Interval: 12 months
Next Calibration Due: 02/13/97

Certificate#: 20202

