

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

CERTIFICATE OF CALIBRATION

Issued to: DIV20 B168 NARASI SRIDHAR

Device No: 2026

Manufacturer: PARR

Model: 4841

Nomenclature: TEMPERATURE CONTROLLER

Serial Number: 0690

SwRI No: NONE

Remarks

Accuracy: MFGR SPECS

Procedure: MFGR

ENVIRONMENT


Temperature: 72 Humidity: 35 Location: ROOM A11 B68 SWRI

CONCLUSION

Tolerance/Remarks: Received into the system, introduced or reactivated

Calibration was in accord with requirements of MIL-STD-45662A. Measurements are traceable to the National Institute of Standards and Technology. Inspection and test data are on file and available for inspection.

Signed



Calibration Date: 02/12/93

Record Number: 00010638

Next Calibration Due: 08/12/93

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

Device Serial No: 0690

Calibration Date: 02/12/93

STANDARDS

Standard No: 102 Manufacturer: ANALOGIC

Model: AN6520

Nomenclature: THERMOCOUPLE CALIBRATOR

Serial No: 9094

Cal.Due: 05/23/93

Cal.Rec.No: 00010131

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

CERTIFICATE OF CALIBRATION

Issued to: DIV20 B168 NARASI SRIDHAR

Device No: 2027

Manufacturer: PARR

Model: 4841

Nomenclature: TEMPERATURE CONTROLLER

Serial Number: 0690A

SwRI No: NONE

Remarks

Accuracy: MFGR SPECS

Procedure: SWRI

ENVIRONMENT


Temperature: 72 Humidity: 35 Location: ROOM A11 B68 SWRI

CONCLUSION

Tolerance/Remarks: Received into the system, introduced or reactivated

Calibration was in accord with requirements of MIL-STD-45662A. Measurements are traceable to the National Institute of Standards and Technology. Inspection and test data are on file and available for inspection.

Signed



Calibration Date: 02/12/93

Record Number: 00010639

Next Calibration Due: 08/12/93

S O U T H W E S T R E S E A R C H I N S T I T U T E

Department of Quality Assurance
Calibration Laboratory

Device Serial No: 0690A

Calibration Date: 02/12/93

STANDARDS

Standard No: 102 Manufacturer: ANALOGIC

Model: AN6520

Nomenclature: THERMOCOUPLE CALIBRATOR

Serial No: 9094

Cal.Due: 05/23/93

Cal.Rec.No: 00010131

SOUTHWEST RESEARCH INSTITUTE
Department of Quality Assurance
Calibration Laboratory

CERTIFICATE OF CALIBRATION
08/04/95

Issued to: DARRELL DUNN DIV20 ,B57
Manufacturer: PARR
Nomenclature: TEMPERATURE CONTROLLER
Serial Number: 0690A
Notes:

Asset Number: 002027
Model Number: 4841
SwRI/Div. I.D. #: NONE

ENVIRONMENTAL CONDITIONS

Temperature: 70.0F

Relative Humidity: 38%

CALIBRATION INFORMATION

Procedure Number: MFG
Remarks: CAL WITH "J" THERMOCOUPLE TO +/-2DEG. C.
LIMITED CALIBRATION -TEMP ONLY


Accuracy: MFRG SPECS
Received IN Tolerance

Calibration was in accordance with requirements of MIL-STD-45662A.
Measurements are traceable to the National Institute of Standards and Technology. Inspection and test data are on file and available for inspection.

STANDARDS USED FOR CERTIFICATION

Asset #	Serial #	Mfg	Model #	Nomenclature	Cal Date	Int.	Cal Due
000182	5200003	FLUKE	5700A	CALIBRATOR	06/07/95	3	09/07/95
002868	311210	KAYE	X0251	ICE POINT REFERENCE	01/03/95	12	01/03/96

Certified by :

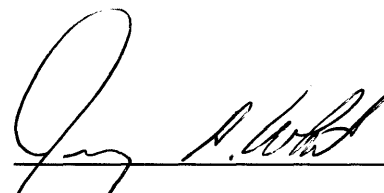

Calibration Date: 08/04/95
Interval: 6 months
Next Calibration Due: 02/02/96

Certificate#: 17596