



SOUTHWEST RESEARCH INSTITUTE®

6220 Culebra Road, P.O. Drawer 28510
Institute Quality Systems
Institute Calibration Laboratory
Phone: 210-522-5215 Fax 210-522-4834



Certificate of Calibration

0972-01

Submitted By: DIV20

Address: B57

Contact: DON BANNON

Manufacturer / Model: ORION / 720A

Description: PH/ION METER

Serial No: 003368

Asset No: 001441

Procedure: ORION 720A - 22 SEP, 2006

Work Order: 303072664

Date Issued: Jan 23, 2007

Calibration Date: Jan 23, 2007

***Calibration Due:** Jan 23, 2008

Calibration Location: Bldg. 64

Environment: Temp. 70.0°F Hum. 38 %RH

****Data Type:** FOUND-LEFT

DivID/Location:

This certificate documents traceability to the National Institute of Standards and Technology (NIST) and the International System of Units (SI). The Laboratory quality system conforms to ISO/IEC 17025, 2005, ANSI/NC SL Z540-1-1994 and relevant requirements of the ISO 9000-2000 standard. This certificate shall not be reproduced, except in full, without the written approval of the Southwest Research Institute Calibration Laboratory. This certificate shall not be used to claim product endorsement by Southwest Research Institute, American Association for Laboratory Accreditation (A2LA) or any agency of the U. S. Government. Results of this calibration relate only to the instrument described above at the time of calibration and does not imply any long term stability of the instrument.

*Determined by the customer, does not imply the instrument will remain within tolerance as any number of factors may cause an out-of-tolerance condition before this date. **Found/Left = adjustment and/or repair was not required, As Left = adjusted and/or repaired was required. The client has sole responsibility for determination of in-/out-of-tolerance or compliance/noncompliance. See Remarks or attached Measurement Report with the same Work Order number for data.

Reported uncertainty calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM) and represents an expanded uncertainty with a coverage factor of k=2 to approximate a 95% confidence level.

Remarks: mVolts Cal'd only

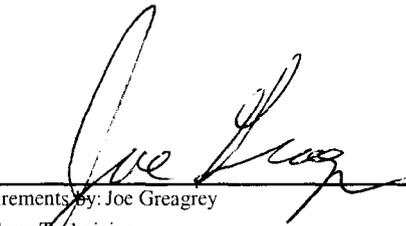
Standards Used

Asset No.	Serial No.	Manufacturer	Model	Description	Cal Due
006413	7085202	FLUKE	5520A/SC1100	MULTI-PRODUCT CALIBRATOR	Mar 16, 07

Reviewed by:  bit () jrg () pwc (→) wgh ()

Metrology Technician

m:\u2la1.rpt Rev date August 15, 2005

Measurements by:  Joe Greagrey

Metrology Technician

Southwest Research Institute
Calibration Laboratory
Measurement Report

Work Order:	303072664	Mfr.	Orion	Technician	JRG
Asset No.	001441	Model	720A		
Serial No.	003368	Type.	pH Meter	Cal Date.	23-Jan-07

Remarks:

LIMITED CAL: Millivolts Only

Function/Range	Test Point	TI Reading	Difference	+/-Limit	+/-Uncertainty	Found/Left
mVolts	mVolts	mVolts	mVolts	mVolts	mVolts	Result
Input 1	0.0	0.0	0.0	0.5	0.12	Pass
	1000.0	1000.1	0.1	1.0	0.12	Pass
	-1000.0	-1000.1	-0.1	1.0	0.12	Pass
END OF REPORT						
mVolts	mVolts	mVolts	mVolts	mVolts	mVolts	
Input 2	0.0	-0.1	-0.1	0.5	0.12	Pass
	1000.0	1000.0	0.0	1.0	0.12	Pass
	-1000.0	-1000.2	-0.2	1.0	0.12	Pass
END OF REPORT						