



SOUTHWEST RESEARCH INSTITUTE®

6220 Culebra Road, P.O. Drawer 28510
Institute Quality Systems
Institute Calibration Laboratory
Phone: 210-522-5215 Fax 210-522-4834



Calibration Laboratory
Certificate #0972-01

Certificate of Calibration

Submitted By: DIV20

Address: B57

Contact: DON BANNON

Manufacturer / Model: BIOS / DCL-M

Description: FLOW METER

Serial No: 1098

Asset No: 011734

Procedure: FLOW, GAS 0 TO 50 lpm - 16 MAR, 2006

Work Order: 303073681

Date Issued: Mar 22, 2007

Calibration Date: Mar 21, 2007

***Calibration Due:** Mar 21, 2008

Calibration Location: Bldg. 64

Environment: Temp. 68.0°F Hum. 40 %RH

****Data Type:** FOUND-LEFT

DivID/Location: N/A

This certificate documents traceability to the National Institute of Standards and Technology (NIST) and the International System of Units (SI). The Laboratory quality system conforms to ISO/IEC 17025, 2005, ANSI/NCSL Z540-1-1994 and relevant requirements of the ISO 9000-2000 standard. This certificate shall not be reproduced, except in full, without the written approval of the Southwest Research Institute Calibration Laboratory. This certificate shall not be used to claim product endorsement by Southwest Research Institute, American Association for Laboratory Accreditation (A2LA) or any agency of the U. S. Government. Results of this calibration relate only to the instrument described above at the time of calibration and does not imply any long term stability of the instrument.

*Determined by the customer, does not imply the instrument will remain within tolerance as any number of factors may cause an out-of-tolerance condition before this date. **Found/Left = adjustment and/or repair was not required, As Left = adjusted and/or repaired was required. The client has sole responsibility for determination of in-/out-of-tolerance or compliance/noncompliance. See Remarks or attached Measurement Report with the same Work Order number for data.

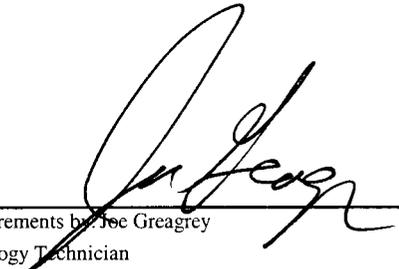
Reported uncertainty calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM) and represents an expanded uncertainty with a coverage factor of k=2 to approximate a 95% confidence level.

Remarks: STP 70 Deg F 29.92 InHg 30 PSI - Cal'd at 0.1SLM 0.3SLM, 1.0SLM, 2.5LPM, and 4.0LPM

Standards Used

Asset No.	Serial No.	Manufacturer	Model	Description	Cal Due
007502	1124	SIERRA	101 Cal Bench	GAS FLOW CALIBRATION SYSTEM	Dec 04, 07


Reviewed by: ~~dl~~ () jrg () pwc () wgh ()
Metrology Technician


Measurements by: Joe Greagrey
Metrology Technician

Southwest Research Institute
Calibration Laboratory
Measurement Report

Work Order:	303073681	Mfr.	Bios	Technician	JRG
Asset No.	011734	Model	DC-Lite		
Serial No.	1098	Type.	Flow Meter	Cal Date.	21-Mar-07
Remarks:		Pm=	741.69	mmHg	Pressure In 30 PSI
STP 70 Deg F		Tc=	20		
29.92 InHg		K=	21.111	Accuracy=	2 % Rdg

Function/Range	Test Point	TI Reading	Difference	+/-Limit	+/-Uncertainty	Found/Left
L/Min	L/Min	L/Min	L/Min	L/Min	L/Min	Result
	0.103	0.103	0.00	0.00	0.0084	Pass
	0.309	0.310	0.00	0.01	0.0084	Pass
	1.013	1.015	0.00	0.02	0.0084	Pass
	2.511	2.510	0.00	0.05	0.0084	Pass
	4.007	3.999	0.01	0.08	0.0084	Pass
END OF REPORT						