


ROOM WIPE TEST

Building 2

DATE 6-8-07

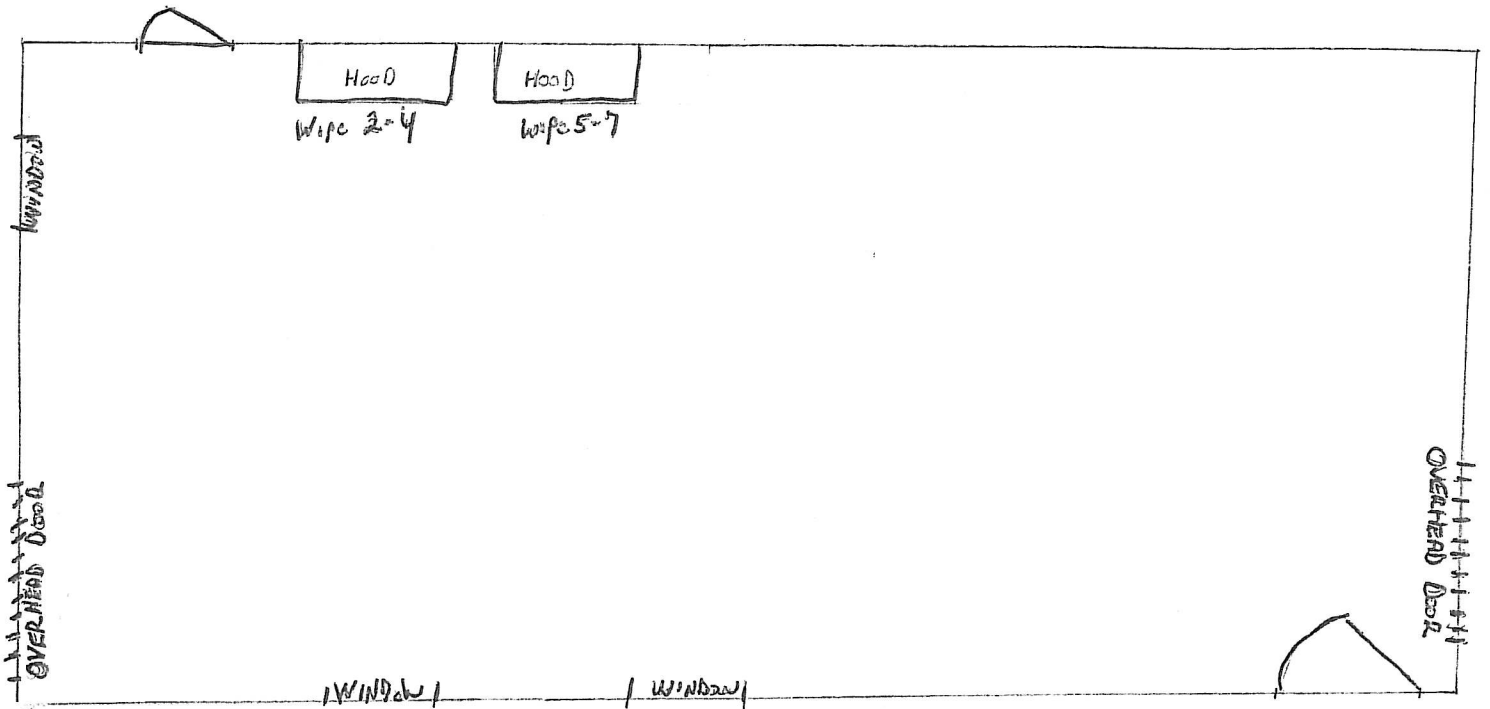

SEE READOUT DATA FOR COMPLETE ROOM RESULTS

MARK ADDITIONAL WIPE AREAS AS NEEDED.

HIGHEST READING AREA:

Wipe # <u>5</u>	<u>9</u> dpm	Wipe # _____	_____ dpm	Wipe # _____	_____ dpm
Wipe # <u>7</u>	<u>9</u> dpm	Wipe # _____	_____ dpm	Wipe # _____	_____ dpm
Wipe # _____	_____ dpm	Wipe # _____	_____ dpm	Wipe # _____	_____ dpm

results are in dpm per 100 cm

Room Activity: No Activity

Test sample taken by DE reviewed by AGL

Room declared: clean

Special Action: C

Room wipe #2

USER: 2 ID:ROOM WIPE 2 PRESET TIME: 2.00 FRI 08 JUN 2007 12:51
 SAMPLE REPEAT: 1 CYCLE REPEAT: 2 SCR:N RS232:N
 H#: 1 ADC:Y QCF:N RCM:Y
 RCM-TIME: 0.10 INT:999.95
 CHANNEL 1-LL: 1 UL: 400 2SIGMA: 1.00 BKG SUB: 10.00 BKG 2SIG: 2.00 LSR:
 CHANNEL 2-LL: 0 UL: 400 2SIGMA: 1.00 BKG SUB: 10.00 BKG 2SIG: 0.00 LSR:

SINGLE LABEL DPM SET UP ON 14 DEC 2005 16:03

UNKNOWN ID: UNKNOWN REPLICATES: 1
 UNKNOWN NORM FACTOR ISO1:0 1.00000
 UNKNOWN UNITS ISO1:DPM
 UNKNOWN HALF LIFE CORRECTION:N
 INDIVIDUAL UNKNOWN NORM FACTORS:N BACKGROUND QUENCH CURVES:N
 STANDARD ID:PACKARD 2005 QUENCH LIMITS LOW:44.00 HIGH:285.0
 HALF LIFE(DAYS) ISO1: 4511.000
 STANDARD DPM ISO1: 267800.0

BAM	POS	CH	CPM	2SIGZ	TIME	EL TIME	AVG H#	RCMZ	ERR
1	**	1	-0.50	*****	2.00	2.53	96.0	1.52	108
		2	-0.50	*****					
		ISO1 %EFF CH1:37.44					ISO1 DPM	: -1.33558	
2	**	1	-1.50	*****	2.00	5.18	93.0	2.80	108
		2	-1.50	*****					
		ISO1 %EFF CH1:38.10					ISO1 DPM	: -3.93673	
3	**	1	-1.50	*****	2.00	7.81	91.0	5.63	108
		2	-1.50	*****					
		ISO1 %EFF CH1:38.55					ISO1 DPM	: -3.89079	
4	**	1	0.50	917.4	2.00	10.46	124.0	8.35	
		2	0.50	916.5					
		ISO1 %EFF CH1:31.50					ISO1 DPM	: 1.587431	
5	**	1	3.50	148.6	2.00	13.10	94.0	4.66	
		2	3.50	148.5					
		ISO1 %EFF CH1:37.88					ISO1 DPM	: 9.239804	
6	**	1	-3.00	*****	2.00	15.73	92.0	1.97	108
		2	-3.00	*****					
		ISO1 %EFF CH1:38.33					ISO1 DPM	: -7.82739	
7	**	1	-0.50	*****	2.00	18.38	117.0	8.53	108
		2	-0.50	*****					
		ISO1 %EFF CH1:32.97					ISO1 DPM	: -1.51657	

CYCLE: 2

Pg 2

SAM	POS	CH	CPM	2SIG%	TIME	EL TIME	AVG H#	RCM%	ERR
1	**-	1	1.00	469.5	2.00	21.49	97.0	2.41	
		2	1.00	469.0					
		ISD1 %EFF CH1:37.22						ISD1 DPM :2.686911	
2	**-	1	0.50	917.4	2.00	24.14	93.0	1.24	
		2	0.50	916.5					
		ISD1 %EFF CH1:38.10						ISD1 DPM :1.312245	
3	**-	1	-3.50	*****	2.00	26.78	91.0	5.24	108
		2	-3.50	*****					
		ISD1 %EFF CH1:38.55						ISD1 DPM :-9.07855	
4	**-	1	-3.00	*****	2.00	29.41	126.0	10.57	108
		2	-3.00	*****					
		ISD1 %EFF CH1:31.07						ISD1 DPM :-9.65427	
5	**-	1	1.00	469.5	2.00	31.95	94.0	5.84	
		2	1.00	469.0					
		ISD1 %EFF CH1:37.88						ISD1 DPM :2.639958	
6	**-	1	-1.50	*****	2.00	34.59	93.0	1.57	108
		2	-1.50	*****					
		ISD1 %EFF CH1:38.10						ISD1 DPM :-3.93676	
7	**-	1	3.00	170.1	2.00	37.24	117.0	9.39	
		2	3.00	170.0					
		ISD1 %EFF CH1:32.97						ISD1 DPM :9.099470	