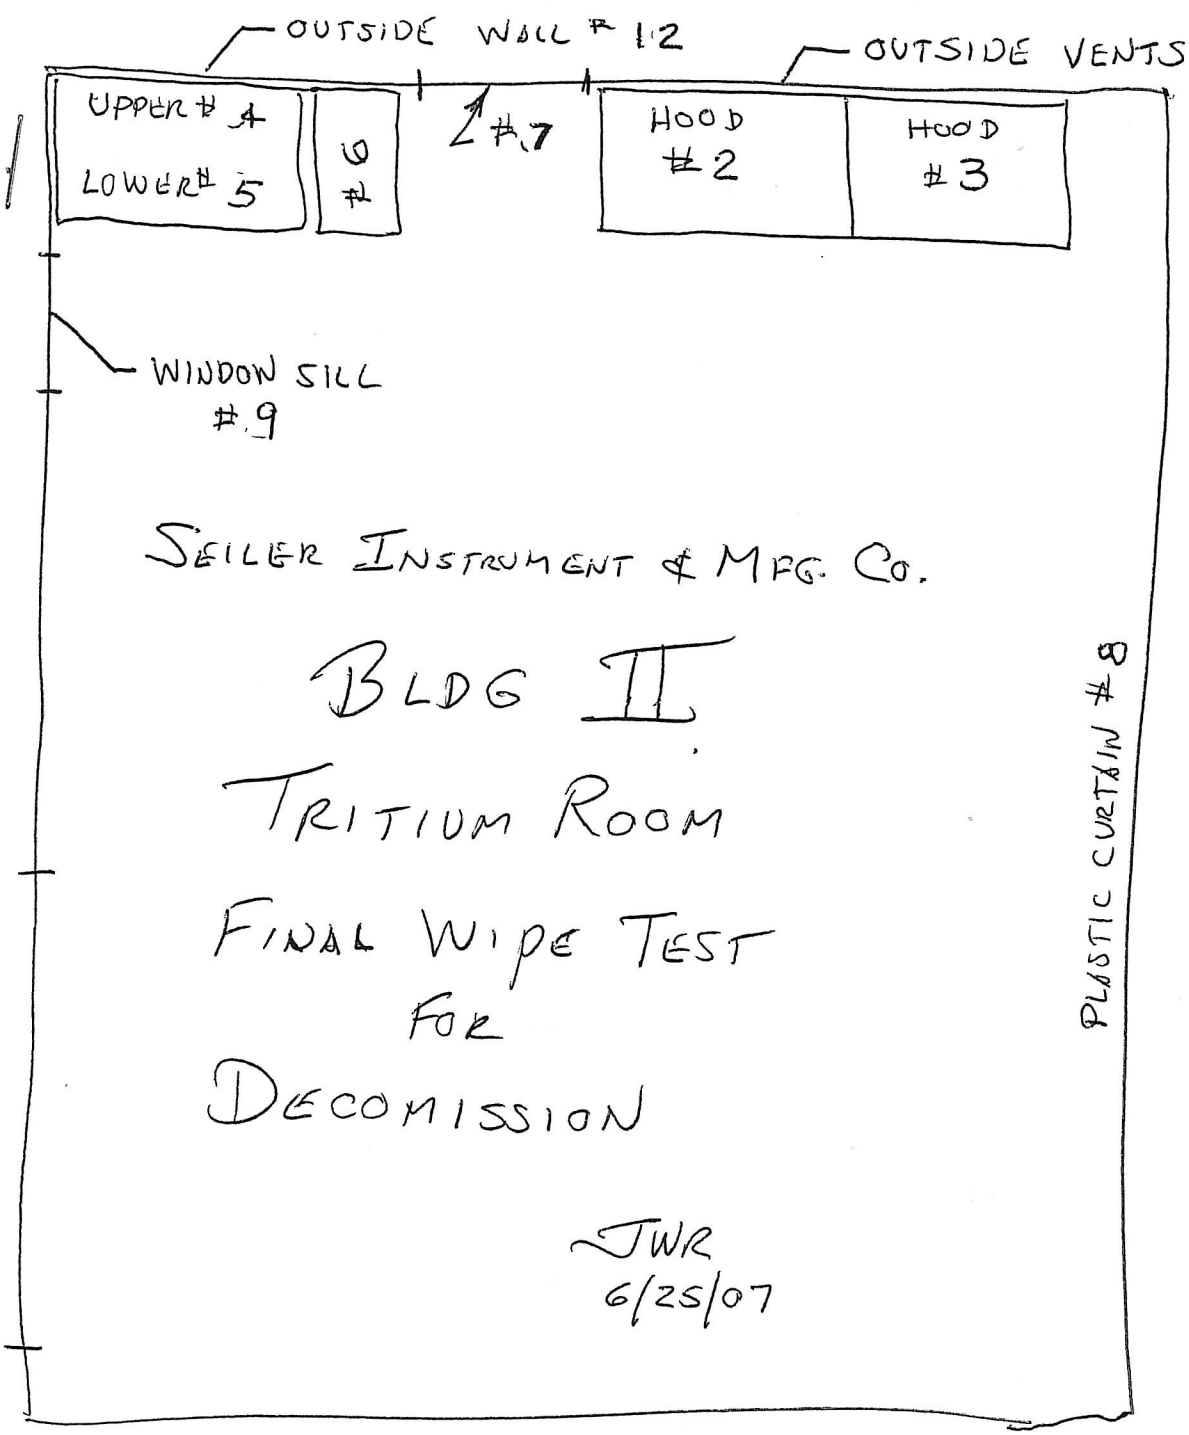
OUTSIDE WALL # 12
OUTSIDE VENTS #10 & #11
UPPER # 4
LOWER # 5
#6
#7
HOOD #2
HOOD #3
WINDOW SILL #9
SEILER INSTRUMENT & MFG. CO.
BLDG II
TRITIUM ROOM
FINAL WIPE TEST
FOR
DECOMISSION
JWR
6/25/07
PLASTIC CURTAIN #8

SAMPLE REPEAT: 1 CYCLE REPEAT: 2 SCR:N RS232:N
H#: 1 AQC:Y QCF:N RCM:Y
RCM-TIME: 0.10 INT:999.95
CHANNEL 1-LL: 1 UL: 400 2SIGMA: 1.00 BKG SUB: 10.00 BKG 2SIG: 2.00 LSR: 0
CHANNEL 2-LL: 0 UL: 400 2SIGMA: 1.00 BKG SUB: 10.00 BKG 2SIG: 0.00 LSR: 0

SINGLE LABEL DPM SET UP ON 14 DEC 2005 16:03

BLDG. II TRITIUM ROOM
FINAL WIPE PER LAYOUT
FOR DECOMMISSION
OK JWR 6/25/07

UNKNOWN ID: UNKNOWN REPLICATES: 1
UNKNOWN NORM FACTOR ISO1:@ 1.00000
UNKNOWN UNITS ISO1:DPM
UNKNOWN HALF LIFE CORRECTION:N
INDIVIDUAL UNKNOWN NORM FACTORS:N BACKGROUND QUENCH CURVES:N
STANDARD ID:PACKARD 2005 QUENCH LIMITS LOW:44.00 HIGH:285.0
HALF LIFE(DAYS) ISO1: 4511.000
STANDARD DPM ISO1: 267800.0

SAM	POS	CH	CPM	2SIG%	TIME	EL TIME	AVG H#	RCM%	ERR
1	**- 1	1	6.00	94.34	2.00	2.53	81.0	6.04	
		2	6.00	94.28					
	ISO1 %EFF CH1:40.89						ISO1 DPM	:14.67231	
2	**- 2	1	46.50	22.86	2.00	5.22	107.0	60.73	
		2	46.50	22.86					
	ISO1 %EFF CH1:35.07						ISO1 DPM	:132.5939	
3	**- 3	1	8.50	71.60	2.00	7.86	125.0	11.99	
		2	8.50	71.56					
	ISO1 %EFF CH1:31.29						ISO1 DPM	:27.16860	
4	**- 4	1	1.50	320.0	2.00	10.49	106.0	5.87	
		2	1.50	319.7					
	ISO1 %EFF CH1:35.28						ISO1 DPM	:4.251554	
5	**- 5	1	-1.50	*****	2.00	13.13	86.0	3.03	108
		2	-1.50	*****					
	ISO1 %EFF CH1:39.70						ISO1 DPM	:-3.77808	
6	**- 6	1	5.50	101.3	2.00	15.78	94.0	8.26	
		2	5.50	101.2					
	ISO1 %EFF CH1:37.88						ISO1 DPM	:14.51969	
7	**- 7	1	4.50	119.8	2.00	18.43	91.0	9.50	
		2	4.50	119.7					
	ISO1 %EFF CH1:38.55						ISO1 DPM	:11.67236	
8	**- 8	1	-1.00	*****	2.00	21.08	95.0	7.43	108
		2	-1.00	*****					
	ISO1 %EFF CH1:37.66						ISO1 DPM	:-2.65550	

```
 9 **- 9  1       11.00 58.94   2.00    23.72  98.0          8.42
          2       11.00 58.92
      ISO1 %EFF CH1:37.00                          ISO1 DPM  :29.73061

10 **-10  1        2.00 245.2   2.00    26.38  90.0         11.00
          2        2.00 244.9
      ISO1 %EFF CH1:38.78                          ISO1 DPM  :5.157371

11 **-11  1        6.50 88.43   2.00    29.03 100.0          9.02
          2        6.50 88.38
      ISO1 %EFF CH1:36.56                          ISO1 DPM  :17.77680

12 **-12  1        2.00 245.2   2.00    31.67  79.0          2.14
          2        2.00 244.9
      ISO1 %EFF CH1:41.38                          ISO1 DPM  :4.833189


CYCLE: 2

 1 **- 1  1        3.00 170.1   2.00    34.70  82.0          3.05
          2        3.00 170.0
      ISO1 %EFF CH1:40.65                          ISO1 DPM  :7.379757

 2 **- 2  1       17.00 43.24   2.00    37.36 123.0         17.71
          2       17.00 43.23
      ISO1 %EFF CH1:31.71                          ISO1 DPM  :53.61376

 3 **- 3  1        9.50 65.77   2.00    40.00 128.0          8.70
          2        9.50 65.74
      ISO1 %EFF CH1:30.65                          ISO1 DPM  :30.99489

 4 **- 4  1        1.00 469.5   2.00    42.64 107.0          2.90
          2        1.00 469.0
      ISO1 %EFF CH1:35.07                          ISO1 DPM  :2.851497

 5 **- 5  1        1.00 469.5   2.00    45.28  90.0          1.92
          2        1.00 469.0
      ISO1 %EFF CH1:38.78                          ISO1 DPM  :2.578686

 6 **- 6  1        4.00 132.4   2.00    47.92  98.0          5.22
          2        4.00 132.3
      ISO1 %EFF CH1:37.00                          ISO1 DPM  :10.81119

 7 **- 7  1        5.50 101.3   2.00    50.57  96.0          5.78
          2        5.50 101.2
      ISO1 %EFF CH1:37.44                          ISO1 DPM  :14.69141

 8 **- 8  1        3.50 148.6   2.00    53.21 102.0          2.81
          2        3.50 148.5
      ISO1 %EFF CH1:36.13                          ISO1 DPM  :9.686222
```

9	**- 9	1	4.00	132.4	2.00	55.85	104.0	7.37	
		2	4.00	132.3					
	ISO1	%EFF CH1:	35.71				ISO1 DPM	:11.20256	
10	**-10	1	2.00	245.2	2.00	58.48	93.0	4.79	
		2	2.00	244.9					
	ISO1	%EFF CH1:	38.10				ISO1 DPM	:5.249007	
11	**-11	1	5.50	101.3	2.00	61.12	105.0	7.56	
		2	5.50	101.2					
	ISO1	%EFF CH1:	35.49				ISO1 DPM	:15.49589	
12	**-12	1	-1.50	*****	2.00	63.76	83.0	3.82	108
		2	-1.50	*****					
	ISO1	%EFF CH1:	40.41				ISO1 DPM	:-3.71177	

Pg 4