

VIRGINIA DEPARTMENT OF HEALTH
DIVISION OF RADIOLOGICAL HEALTH



NRC AGREEMENT STATE APPLICATION



COMMONWEALTH of VIRGINIA

Office of the Governor

Timothy M. Kaine
Governor

June 12, 2008

The Honorable Dale E. Klein, Chairman
U.S. Nuclear Regulatory Commission
11555 Rockville Pike
Rockville, MD 20852

Dear Chairman Klein:

I am writing to formally request that an agreement be established between the United States Nuclear Regulatory Commission and the Commonwealth of Virginia as authorized under Section 274b of the Atomic Energy Act of 1954 (herein referred to as the Act), as amended and the Virginia Statutes Section 32.1-235.

Under this agreement the U.S. Nuclear Regulatory Commission will discontinue certain regulatory authority for radioactive materials now under federal jurisdiction and that authority will be assumed by the Commonwealth of Virginia. As provided by Virginia Statutes Section 32.1-228.1, the Virginia Department of Health is the agency responsible for the implementation of the agreement. The specific authority requested is for the following:

- A. By-product materials as defined in Section 11e. (1) of the Act;
- B. By-product materials as defined in Section 11e. (3) of the Act;
- C. By-product materials as defined in Section 11e. (4) of the Act;
- D. Source materials; and
- E. Special nuclear materials in quantities not sufficient to form a critical mass.


The Commonwealth of Virginia at this time is not requesting authority to regulate the extraction or concentration of source material from source material ore and the

The Honorable Dale E. Klein
June 12, 2008
Page 2

management and disposal of the resulting byproduct material; land disposal of byproduct, source, or special nuclear material waste received from other persons; or the evaluation of radiation safety information on sealed sources or devices containing byproduct, source, or special nuclear materials and the registration of the sealed sources or devices for distribution, as provided for in regulations or orders of the Commission.

I certify that the Commonwealth of Virginia desires to assume regulatory authority and oversight responsibility for such materials listed above, and that the Commonwealth of Virginia has an adequate program for the control of radiation hazards covered by this proposed agreement. Enclosed is the formal application, which contains information as required by the Office of Federal and State Materials and Environmental Management Programs (FSME) procedure; SA-700 'Processing an Agreement'.

Sincerely,

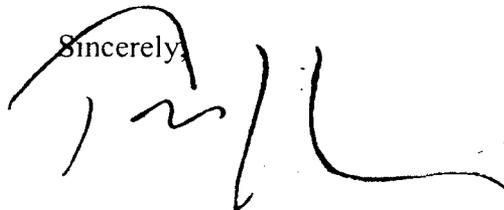A handwritten signature in black ink, appearing to read 'Timothy M. Kaine', written over the word 'Sincerely,'.

Timothy M. Kaine

AGREEMENT
BETWEEN
THE UNITED STATES NUCLEAR REGULATORY COMMISSION
AND
THE COMMONWEALTH OF VIRGINIA
FOR THE
DISCONTINUANCE OF CERTAIN COMMISSION REGULATORY AUTHORITY
AND RESPONSIBILITY WITHIN THE COMMONWEALTH PURSUANT TO
SECTION 274 OF THE ATOMIC ENERGY ACT OF 1954, AS AMENDED

WHEREAS, The United States Nuclear Regulatory Commission (hereinafter referred to as the Commission) is authorized under Section 274 of the Atomic Energy Act of 1954, as amended (hereinafter referred to as the Act), to enter into agreements with the Governor of the Commonwealth of Virginia providing for discontinuance of the regulatory authority of the Commission within the Commonwealth under Chapters 6, 7, and 8, and Section 161 of the Act with respect to byproduct materials as defined in Sections 11e. (1), (2), (3) and (4) of the Act, source materials, and special nuclear materials in quantities not sufficient to form a critical mass; and,

WHEREAS, The Governor of the Commonwealth of Virginia is authorized, under the Code of Virginia Section 32.1-235, to enter into this Agreement with the Commission; and,

WHEREAS, The Governor of the Commonwealth of Virginia certified on **[date?]** that the Commonwealth of Virginia (also referred to herein as the Commonwealth) has a program for the control of radiation hazards adequate to protect public health and safety with respect to the materials within the Commonwealth covered by this Agreement, and that the Commonwealth desires to assume regulatory authority for such materials; and,

WHEREAS, The Commission found on **[date?]** that the program of the Commonwealth for the regulation of the materials covered by this Agreement is compatible with the Commission's program for the regulation of such materials and is adequate to protect public health and safety; and,

WHEREAS, The Commonwealth and the Commission recognize the desirability and importance of cooperation between the Commission and the Commonwealth in the formulation of standards for protection against hazards of radiation and in assuring that Commonwealth and Commission programs for protection against hazards of radiation will be coordinated and compatible; and,

WHEREAS, The Commission and the Commonwealth recognize the desirability of the reciprocal recognition of licenses, and of the granting of limited exemptions from licensing of those materials subject to this Agreement; and,

WHEREAS, This Agreement is entered into pursuant to the provisions of the Atomic Energy Act of 1954, as amended;

NOW, THEREFORE, It is hereby agreed between the Commission and the Governor of the Commonwealth of Virginia, acting on behalf of the Commonwealth, as follows:

ARTICLE I

Subject to the exceptions provided in Articles II, IV, and V, the Commission shall discontinue, as of the effective date of this Agreement, the regulatory authority of the Commission in the Commonwealth under Chapters 6, 7, and 8, and Section 161 of the Act with respect to the following materials:

- A. By-product materials as defined in Section 11e. (1) of the Act;
- B. By-product materials as defined in Section 11e. (3) of the Act;
- C. By-product materials as defined in Section 11e. (4) of the Act;
- D. Source materials;
- E. Special nuclear materials in quantities not sufficient to form a critical mass.

ARTICLE II

This Agreement does not provide for discontinuance of any authority and the Commission shall retain authority and responsibility with respect to:

- A. The regulation of the construction and operation of any production or utilization facility or any uranium enrichment facility;
- B. The regulation of the export from or import into the United States of byproduct, source, or special nuclear material, or of any production or utilization facility;
- C. The regulation of the disposal into the ocean or sea of byproduct, source, or special nuclear material wastes as defined in the regulations or orders of the Commission;
- D. The regulation of the disposal of such other byproduct, source, or special nuclear material as the Commission from time to time determines by regulation or order should, because of the hazards or potential hazards thereof, not be so disposed without a license from the Commission;
- E. The evaluation of radiation safety information on sealed sources or devices containing byproduct, source, or special nuclear materials and the registration of the

sealed sources or devices for distribution, as provided for in regulations or orders of the Commission;

- F. The extraction or concentration of source material from source material ore and the management and disposal of the resulting byproduct material.
- G. The regulation of the land disposal of byproduct, source, or special nuclear material waste received from other persons;

ARTICLE III

With the exception of those activities identified in Article II, paragraphs A through D, this Agreement may be amended, upon application by the Commonwealth and approval by the Commission, to include the additional areas specified in Article II, paragraphs E, F and G, whereby the Commonwealth can exert regulatory authority and responsibility with respect to those activities and materials.

ARTICLE IV

Notwithstanding this Agreement, the Commission may from time to time by rule, regulation, or order, require that the manufacturer, processor, or producer of any equipment, device, commodity, or other product containing source, byproduct, or special nuclear material shall not transfer possession or control of such product except pursuant to a license or an exemption from licensing issued by the Commission.

ARTICLE V

This Agreement shall not affect the authority of the Commission under subsection 161b or 161i of the Act to issue rules, regulations, or orders to protect the common defense and security, to protect restricted data, or to guard against the loss or diversion of special nuclear material.

ARTICLE VI

The Commission will cooperate with the Commonwealth and other Agreement States in the formulation of standards and regulatory programs of the States and the Commission collectively for protection against hazards of radiation and to assure that Commission and Commonwealth programs for protection against hazards of radiation will be coordinated and compatible. The Commonwealth agrees to cooperate with the Commission and other Agreement States in the formulation of standards and regulatory programs of the Commonwealth and the Commission for protection against hazards of radiation and will

assure that the Commonwealth's program will continue to be compatible with the program of the Commission for the regulation of materials covered by this Agreement.

The Commonwealth and the Commission agree to keep each other informed of proposed changes in their respective rules and regulations, and to provide each other the opportunity for early and substantive contribution to the proposed changes.

The Commonwealth and the Commission agree to keep each other informed of events, accidents, and licensee performance that may have generic implication or otherwise be of regulatory interest.

ARTICLE VII

The Commission and the Commonwealth agree that it is desirable to provide reciprocal recognition of licenses for the materials listed in Article I licensed by the other party or by any other Agreement State. Accordingly, the Commission and the Commonwealth agree to develop appropriate rules, regulations, and procedures by which such reciprocity will be accorded.

ARTICLE VIII

The Commission, upon its own initiative after reasonable notice and opportunity for hearing to the Commonwealth, or upon request of the Governor of the Commonwealth of Virginia, may terminate or suspend all or part of this agreement and reassert the licensing and regulatory authority vested in it under the Act if the Commission finds that (1) such termination or suspension is required to protect public health and safety, or (2) the Commonwealth has not complied with one or more of the requirements of Section 274 of the Act. The Commission may also, pursuant to section 274j of the Act, temporarily suspend all or part of this agreement if, in the judgement of the Commission, an emergency situation exists requiring immediate action to protect public health and safety and the Commonwealth has failed to take necessary steps. The Commission shall periodically review this Agreement and actions taken by the Commonwealth under this Agreement to ensure compliance with Section 274 of the Act which requires a Commonwealth program to be adequate to protect public health and safety with respect to the materials covered by the Agreement and to be compatible with the Commission's program.

ARTICLE IX

This Agreement shall become effective on [date?] and shall remain in effect unless and until such time as it is terminated pursuant to Article VIII.

Done at Richmond, Virginia this [date?] day of [month?], [year?].

FOR THE UNITED STATES NUCLEAR
REGULATORY COMMISSION

, Chairman

FOR THE COMMONWEALTH OF
VIRGINIA

, Governor

Contact Information



Timothy Kaine

Governor

Office of the Governor
Patrick Henry Building, 3rd Floor
1111 East Broad Street
Richmond, Virginia 23219

Phone: (804) 786-2211
Fax: (804) 371-6351



Marilyn Tavenner
Secretary of Health and Human Resources

Office of the Secretary of Health and Human Resources

Patrick Henry Building
1111 East Broad Street
Richmond, VA 23219

For regular U.S. mail, please use the following address:

P.O. Box 1475
Richmond, VA 23218

Phone Numbers:

(804) 786-7765

Fax Line: (804) 371-6984



Karen Remley, M.D., M.B.A.

State Health Commissioner

VIRGINIA DEPARTMENT OF HEALTH

P.O. Box 2448

Richmond, Virginia 23218-2448

109 Governor Street

Richmond, Virginia 23219

(804) 864-7001

(804) 864-7022 FAX

VIRGINIA DIVISION OF RADIOLOGICAL HEALTH NARRATIVE

Table of Contents

I. HISTORY AND OVERVIEW

Introduction

History of Virginia Division of Radiological Health

Interest in Agreement State Status

II. DIVISION OF RADIOLOGICAL HEALTH AND SAFETY REGULATION DESCRIPTION

Organization, Mission, Staff Education & Experience, Training Activities and Overview

Environmental Radiation Monitoring

Radon Public Information and Outreach

Radiological Emergency Preparedness and Response

X-ray Registration; Mammography Inspection

Radiological Incident Response

III. RADIOACTIVE MATERIALS PROGRAM DESCRIPTION

Program Description

Accomplishments

Naturally Occurring and Accelerator Produced Radioactive Material (NARM)

Licensing and Inspection

Staff Designated for Training, Procedure & Regulation Development

Program Management

Licensing, Inspection & Enforcement, and Allegations & Incident Response

Administrative Tracking and Processing

Legal Assistance

Radioactive Materials Program Procedures

Staff Needs Analysis

I. HISTORY AND OVERVIEW

Introduction

The Commonwealth of Virginia seeks to enter into an Agreement with the Nuclear Regulatory Commission (NRC) for the purpose of assuming regulatory authority over reactor-produced (byproduct) radioactive materials, source materials and special nuclear materials in quantities not sufficient to form a critical mass. In addition the Commonwealth seeks to retain regulatory authority over those materials transferred to the NRC by the Energy Policy Act of 2005. The following Division of Radiological Health (DRH) history and overview has been developed to provide supporting information for the application to become an 'Agreement State'.

History of Virginia Division of Radiological Health

Protection against radiation hazards was first recognized as necessary in the late 1950's by the Virginia Department of Health (VDH). Personnel already on staff worked part-time performing safety surveys for medical and dental offices upon request.

In 1958 the Virginia Legislature passed a law limiting the use of shoe-fitting fluoroscopic machines. Also in 1958 the U.S. Public Health Service cooperated with Virginia in establishing air and water radiation monitoring programs which expanded in 1960 to include surveillance in the vicinity of the nuclear powered U.S.S Savannah and nuclear submarine activity in the Norfolk area.

In 1960, a Radiation Registration Law was passed by the Legislature. This law required the registration of all radiation-producing machines and all radioactive materials not licensed or controlled by the U.S. Atomic Energy Commission (AEC).

In 1964 the Legislature passed a comprehensive "Radiation Control Law" charging the State Department of Health with the protection of the health and safety of the citizens of Virginia from sources of ionizing radiation. The law was implemented by the preparation and promulgation of Rules and Regulations. It allowed for Virginia to eventually assume certain regulatory functions then carried out by the AEC for the control of by-product, source, and special nuclear materials. The Rules and Regulations adopted on April 1, 1973 were developed following the Model Regulations prepared by the Council of State Governments in cooperation with the AEC and U.S. Public Health Service. The Rules and Regulations promulgated since then were developed from the Suggested State Regulations published by the Conference of Radiation Control Program Directors. The Radiation Protection Regulations were revised again in 1980, 1985, 2006 and 2008.

The Radiation Control Law provided the Board of Health the authority to promulgate radiation protection rules and develop necessary policies and programs, plus established the requirement to register radiation producing machine and license non-AEC radioactive materials. In addition, the Radiation Control Law created a Radiation Advisory Board with responsibilities that included: review and evaluate policies and programs of the State relating to ionizing radiation,

and make recommendations to the State Health Commissioner and the Board of Health, and furnish such technical advice as may be required, on matters relating to development, utilization, and regulation of sources of ionizing radiation.

Initially the radiation control program was located in the Bureau of Industrial Hygiene. Later the Bureau of Industrial Hygiene was re-organized. The occupational health inspectors were transferred to the Department of Labor and Industry. The radiation control program was retained in the Department of Health and became the Bureau of Radiological Health (BRH) located in the Division of Health Hazards Control, along with the Toxic Substance Program, and the Bedding and Upholstery Inspection Program.

In the 1970's, the BRH began participating with the Food and Drug Administration (FDA) in numerous programs for the nationwide evaluation of x-ray trends (NEXT) and the dental evaluation of X-ray trends (DENT) to determine patient exposure from various radiological examinations. The compiled national data was used to establish exposure limits for various diagnostic examinations.

Other activities include: environmental monitoring of the North Anna and Surry Nuclear Power Stations, and the Babcock & Wilcox Naval Fuel Fabrication Facility under contract with the NRC and participation in the Environmental Protection Agency (EPA) Environmental Radiation Ambient Measurement System (ERAMS). The BRH also began conducting compliance inspections of newly installed x-ray systems under contract to the FDA.

Uranium exploration in Virginia became a significant legislative issue in the late 1970's. At the direction of a Virginia legislative committee, a feasibility study was conducted for mining uranium in Pittsylvania County by Marline Company, later to become Allied Chemical. Due to a drop in price and demand for uranium, the project did not proceed; however, recently there has been renewed interest in uranium mining in Virginia.

In response to the 1979 Three Mile Island accident, the BRH worked with the state emergency management agency to develop a radiological emergency preparedness and response (REP) capability to address incidents at the two nuclear power plants in Virginia. During the early-1980's the BRH expanded its REP capability to include a mobile radiological laboratory, with germanium analysis system, and increased field instrumentation. BRH also purchased an IBM personal computer and proprietary software, RADOSE, for atmospheric modeling of a nuclear power plant release. In 1984 several BRH staff traveled to the Nevada Test site for participation in the Nuclear Weapons Accident Exercise (NUWAX). The mobile lab was also transported by military air cargo to the test site. Beginning in the mid-1980s the utility also provided a technical consultant to assist BRH staff in the development of its emergency procedures in preparation for its first ingestion exercise.

During the mid-1980s numerous articles in the news media covering reports of elevated levels of radon in Pennsylvania appeared. The media attention began to generate inquiries from the public and legislators. In 1986 BRH was provided funding of \$75,000 to purchase Working Level Meters to conduct a study of radon in Virginia. The General Assembly called for a legislative committee to study radon levels in the Commonwealth. BRH conducted a study of 800 VDH

employee's homes located throughout the Commonwealth. Initial results indicated that about 10-12 percent of the homes tested had greater than 0.02 WL (equivalent to 4.0 picocuries per liter of radon). The General Assembly followed up with legislation that authorized VDH to create a program of technical assistance and radon information to the public. The legislation also provided \$54,000 annually to support the activity.

During the mid-1980s the Commonwealth of Virginia became a member of the Southeast Compact for the Disposal of Low Level Radioactive Waste and submitted a bid to host a low level waste facility. Most of the work was performed by another program in VDH, the Division of Waste Management, which later became a separate state agency. After the Commonwealth lost its bid to host a site, the program working on the activity was eliminated. BRH became the recipient of some of the equipment that was declared surplus, such as a portable germanium gamma spectroscopy system. VDH management has requested BRH staff to ensure regulations pertaining to land disposal of radioactive materials are kept current in the Radiation Protection Regulations in case a decision is made to add regulatory authority for land disposal to the agreement.

In 1986 the General Assembly passed legislation that required the registration of all X-ray producing machines as well as the inspection and certification of all X-ray machines used in the healing arts. The legislation also authorized the collection of registration fees for X-ray machines and fees for the inspection of X-ray machines by BRH inspectors. BRH staff revised the Radiation Protection Regulations in 1986 and created a fee schedule to implement the legislation. BRH staff also created a database which currently contains 17,000 X-ray machines and developed a fee collection system to implement the legislation. The workload quickly expanded and the staff installed the agency's first local area network (LAN) so multiple persons could make entries onto the system.

In the late 1980's BRH requested assistance from the Virginia Department of Emergency Services and Virginia Power, later Dominion Power, to replace the mobile radiation laboratory. A used vehicle, 1986 GMC truck, from another agency program that was being down sized was used as a mobile lab platform. Virginia Power provided \$120,000 to purchase new laboratory equipment, which included a new gamma spectroscopy system, an alpha/beta counter, and a liquid scintillation system. The previous laboratory was used primarily for the nuclear power plant exercises; however, it was used in several other incidents, such as the assessment of a transportation accident clean up in Christiansburg involving an overturned shipment of contaminated soil in October 1989. A year later during the first use of the new mobile lab at an evaluated plume and ingestion exercise at the Surry Nuclear Power Plant, a simultaneous real incident occurred involving an over-height vehicle on an I-64 underpass that was carrying a reactor coolant pump. The reactor coolant pump cracked the concrete payment and spilled about 10 gallons of primary coolant on I-64. The previous lab was pressed into service to handle the assessment of clean up activities during the week. The previous lab continued to provide service to scrap metal facilities and transportation incidents.

In 1990, the BRH applied for and was awarded one of the first State Indoor Radon Grants from the EPA. This grant allowed expansion of BRH's program of technical assistance and radon information to the public. BRH added an in-state toll-free telephone hotline so all citizens would

have access to radon information. The initial grant was a 75/25 percent match. Since BRH could not implement long term projects for the funds as the match would be reduced to a 50/50 match in succeeding grants, much of the initial federal funds were used to test for radon in schools in economically depressed areas of the Commonwealth. Later the General Assembly enacted legislation that all public schools will be tested for radon. BRH also conducted a more statistically powerful survey of radon homes in 1992 by conducting a survey of 1,600 homes. The survey confirmed the results of the previous survey of 800 homes and produced results for the four Health Districts.

Also in 1990, the BRH began participating in the Health Care Finance Administration (HCFA) mammography certification program. The HCFA program was superseded by the federal Mammography Quality Standards Act of 1992. The BRH subsequently entered into a contract with the Food and Drug Administration to conduct annual inspections of all mammography facilities in Virginia.

During the early 1990s, BRH staff initiated rulemaking to revise the Radiation Protection Regulations resulting from major changes by NRC to the Radiation Protection Standards (10 CFR 20). Unfortunately most rule making was suspended during the administration under then Governor George Allen. Promulgation of regulations was continued mid-term of the succeeding governor. The Administrative Process was also revised to include additional steps such as approval to initiate rule making by the Secretary and Governor, and a fiscal impact review by the State Department of Budget and Planning.

In 1997 NRC terminated its environmental monitoring contracts with the states for producing comparative annual environmental reports of utility data and that collected by the state radiation program. Unlike most states, Virginia did not have legislative authority to collect fees from the utility for the implementation of a state radiation environmental monitoring program for the nuclear power plants. FDA also decided not to renew the compliance contracts for the inspection new X-ray equipment with the states as well in the same year.

Interest in Agreement State Status

Interest in Agreement State status has been off and on for several decades. Historically the statutory authority for the Governor and VDH to enter into an agreement has been in place since 1964 when the Atomic Energy Commission was the cognizant federal agency. There were two major events during the 1980s that sparked renewed interest in Agreements State status, namely perspective uranium mining in Pittsylvania County, and Virginia's bid to host a low level radioactive waste site. Both of these activities failed to materialize, and thus interest in Agreement State status waned.

In the late 1980s the new Program Director for BRH invited representatives from NRC to speak to the Radiation Advisory Board and State Health Commissioner about the Agreement State Program. The presentation did not provide either the Advisory Board or VDH management sufficient motivation to pursue Agreement State status. Most NRC licensees were unaware or indifferent to the Agreement State Program.

In the following years the dynamics changed. NRC became more selective in who attended NRC training courses and eventually state programs had to pay registration and travel expenses for their employees. Many state programs used the five-week Health Physics course at Oak Ridge, TN to provide basic radiation training for their employees since few colleges include radiation physics or health physics in their curricula.

By the mid-1990s Congress required the NRC to be fully funded by fees. As a result NRC began collecting licensing fees from State agencies which had previously been exempt and increased fees to the materials licensees. This touched off a new round of states seeking Agreement State status and renewed interest by Virginia's Radiation Advisory Board and BRH staff. By 1997 Massachusetts had become an Agreement State; and Ohio, Oklahoma, and Pennsylvania had applied for Agreement State status.

On October 6, 1997, Virginia Senator Benedetti sent a letter to Governor George Allen suggesting his office consider entering into an Agreement. The Governor's reply suggested the Radiation Advisory Board would evaluate the feasibility of Virginia participating in the Agreement State Program and recognized that certain qualifying criteria had to be met. The Radiation Advisory Board quickly produced its recommendation in support of Agreement State status.

At a meeting of the Radiation Advisory Board on December 19, 1997, the Board recommended that it is advantageous for Virginia to participate in the Agreement State Program and submitted this recommendation to the State Board of Health.

In the 1999 session, the General Assembly enacted legislation authorizing VDH to implement civil penalties, fee schedule for radioactive materials licenses and inspections, and created a special fund for these fees. The intent of this legislation was to complete all statutory authority needed for the Commonwealth to enter into an agreement with the NRC.

In the meantime the agency had difficulty identifying a funding source to provide staffing during the transition of this activity until the agreement was signed. In the latter part of 2005 VDH considered taking a similar approach as some of the more recent Agreement States and collect a 30% surcharge from the NRC licensees in return for greatly reduced licensing fees after an agreement is signed. On October 24, 2005 Carl Armstrong, M.D., Director, Office of Epidemiology sent a letter to each of the NRC licensees in Virginia advising them of VDH's intentions to apply for NRC Agreement State status and collect a 33 per cent surcharge to support the transition. All of the responses from the licensees were either positive or neutral.

In December 2005 outgoing Governor Warner signed a letter of intent requesting NRC assistance in pursuing agreement state status. On September 8, 2006, Secretary of Health Marilyn Tavenner responded to the January 31, 2006 letter from the NRC regarding Virginia's letter of intent. Since then VDH management has decided to fund the transition to Agreement State status using specially designated funds for the next three state fiscal years, rather than collect the surcharge as originally intended. In April 2006 a letter was sent to the NRC licensees informing them that the Governor had submitted a letter of intent for NRC Agreement State status, and that VDH had decided not to collect a surcharge.

On April 25, 2006 NRC State Tribal Program (STP) Director, Janet Schluter, and staff meet with VDH staff to present information regarding the Agreement State Program and the application process. Based on the information provided, VDH management decided to proceed quickly with the application process and immediately began recruitment for the program staff. In addition, the program was elevated organizationally and is now the Division of Radiological Health and Safety Regulation (DRH)). The Division Director reports directly to a newly created Deputy Director position within the Office of Epidemiology and is a medical director position.

In September 2004, the DRH proposed creation of a new chapter of radiation protection regulations in the Virginia Administrative Code and abolish the existing Chapter since there were numerous changes since 1986 when the Radiation Protection regulations were last revised. The proposed regulations were based on the Suggested State Regulations for the Control of Radiation (SSRCR) developed by the Conference of Radiation Control Program Directors (CRCPD). The proposed regulation was published for public comment from June 27, 2005 through September 29, 2005 prior to the agency's decision to seek Agreement State status. After the public comment period, DRH staff did receive a public comment that suggested updating references to 10 CFR 35 and other federal sections. This allowed DRH staff to incorporate by reference missing sections or update NRC regulatory references. The final regulations were developed to make the Virginia radiation protection regulations current and compatible with applicable federal regulations. The final regulations became effective on September 20, 2006. These regulations were reviewed by the NRC in 2006. The NRC submitted a letter with 99 comments to VDH regarding these regulations. VDH staff reviewed these comments and made the necessary corrections. The amended regulations were submitted in October 2007 to the NRC for a final review. On December 19, 2007 the NRC submitted a letter with 31 comments regarding these regulations. These comments were reviewed and the appropriate amendments were made to the regulations. The revised regulations were submitted to the Virginia Registrar for review and approval following a fast track/exemption procedure. On April 14, 2008 the final draft regulations were delivered to the Virginia Legislative Services. The regulations were printed in the May 12, 2008 Virginia Register and became effective on June 12, 2008.

The Code of Virginia sections which corresponded with radiological health were submitted to the NRC in 2006 for review. In October of 2006 the NRC provided VDH a letter with 10 comments. These comments were reviewed with management and Virginia's Office of Attorney General (OAG) and a decision was made to amend these sections of the Code. On August 24, 2007 the proposed changes were submitted to the Secretary of Health and Human Services who in turn submitted them to the Governor's office. The Code of Virginia sections relating to radiation protection (32.1-227 through 32.1-238) were amended and reenacted on February 27, 2008. VDH is now designated as the state radiation control agency.

DRH staff also issued a Notice of Intended Regulatory Action (NOIRA) to create a fee schedule in 2006. The existing fee schedule contains fees only for the X-ray machine program. New sections will need to be developed for materials licensing and inspections, reciprocity, civil penalties, fiscal assurance, and exemptions and reductions for small business entities and others entities similar those NRC provides. The prescribed promulgation process for adopting and amending radiation control regulations entails 1) obtaining approval of the Department of

Health; Secretary of Health and Human Resources, and Governor; 2) submitting a NORIA for publication in the Virginia; 3) presenting the proposed rules to the Department of Planning and Budget for fiscal review; 4) presenting the proposed rules to the Board of Health for public review and comment, which may or may not include scheduled public hearings; 5) responding to each public comment and present modified regulations for approval as final regulations to the Board of Health; 6) submit the final rules to the Department of Planning and Budget for fiscal review again; 7) submit final regulation to Secretary and Governor for review; and 8) submit final regulation to Virginia Register for publication with effective date no less than 30 days from date of publication. The Board of Health approved the proposal fee schedule on July 20, 2007 the Governor approved the NOIRA on January 11, 2007 and the NOIRA was made available for public comment which ended on March 6, 2007. We received one comment from the public. The proposed fee schedule was printed in the Virginia Register on June 12, 2008 for a 60-day public comment period. The next step will be to respond to each comment and present to the Board of Health for final approval.

II. DIVISION OF RADIOLOGICAL HEALTH AND SAFETY REGULATION PROTECTION DESCRIPTION

Organization, Mission, Staff Education & Experience, Training Activities and Overview

The Division of Radiological Health (DRH) is located in the Department of Health (VDH). The Secretary of Health and Human Resources is Marilyn Tavenner, who was appointed by Governor Timothy Kaine. The State Health Commissioner, Karen Remley, M.D., reports to Secretary Tavenner. The Deputy Commissioner for Public Health, Jim Burns, M.D., MBA, reports to Ms. Remley. The Office of Epidemiology Director, Carl W. Armstrong, M.D., reports to Mr. Burns. The Deputy Director, Office of Epidemiology, (currently vacant), reports to Mr. Armstrong. The Division of Radiological Health and Safety Regulations Director, Les Foldesi, M.S., CHP, currently reports to Mr. Armstrong. The Director, Radioactive Materials Program (DRMP), Michael Welling reports to Mr. Foldesi. Currently four Radiation Safety Specialist positions are approved for the Radioactive Materials Program. These four positions are held by Charles Coleman, Kimberly Gilliam, Dante Laciste and Beth Schilke. Ms. Gilliam works from her home in Bristol, Ms. Schilke works from her home in Hampton while Mr. Coleman and Mr. Laciste work in the Richmond office. Organizational charts for these administrative levels within State government and VDH, as well as contact information, are included.

The mission of the DRH is to protect the public - both occupationally exposed and general - from unnecessary exposure to sources of radiation. To help accomplish this mission, the DRH has a staff of well-qualified personnel from a variety of academic and professional backgrounds. Currently, DRH employs 19 people with the following academic distribution:

- 2 staff with Master's degrees.
- 15 staff with Bachelor's degrees in various disciplines, including chemistry, biology and radiologic technology.
- 2 staff with Associate's degrees or equivalent in scientific specialties.
- 3 staff members certified in health physics.

DRH staff have wide ranging and extensive expertise in the areas of occupational health and safety, nuclear power plant operation, health physics, radon, training, environmental monitoring, radiochemistry, physics, emergency preparedness planning, geology, radiological incident response, dose assessment and radiation control.

Training activities are an important component of DRH activities. DRH and the Virginia Department of Emergency Management (VDEM) coordinate training for local emergency responders, state agency staff, DRH staff, county emergency government staff and utility personnel. VDH staff have participated in several tabletop exercises with other local and regional first responders. The recent heightened awareness of possible need to respond to a terrorist threat involving radioactive materials will present additional opportunities to provide training to regional and local emergency responders and train with military civilian support groups.

The primary responsibilities of the DRH are listed below and are discussed in further detail in subsequent sections:

- Environmental radiation monitoring
- Radon public information and outreach
- Radiological emergency preparedness and response
- X-ray registration and inspection; mammography facility inspection
- Radioactive materials licensing and inspection
- Radiological incident response

Environmental Radiation Monitoring

The DRH currently conducts environmental surveillance around each of the two nuclear power stations in Virginia – North Anna and Surry. Dominion Power, formerly Virginia Power operates two pressurized water reactors (PWR) at each power station. Dominion Power has submitted an application for an additional unit at the North Anna location. Dominion Power pioneered the development of the Interim Spent Fuel Storage facility at Surry and later installed another at North Anna. An extensive monitoring system was implemented for each of the two power stations during the pre-operational phase and continues today. The number of environmental samples were decreased from 1,000 to about 300 annually after the NRC canceled all state environmental monitoring contacts in 1997. Environmental monitoring activities include the following:

1. Passive TLD System

The passive TLD monitoring system utilizes thermo-luminescent dosimeters (TLDs) to measure the cumulative level of radiation around the plant sites. TLDs are exchanged quarterly and read on a Harshaw TLD reader, and then entered into the annual environmental report. Recently the software for the TLD system was upgraded to a Windows based software to make data archiving and reporting easier with the program's Windows based operating systems.

2. Environmental sampling (milk, water, vegetation, fish, shell fish, air particulate/air iodine)

Environmental sampling is conducted to monitor the air, terrestrial and aquatic environments for radioactivity content. Continuous air sampling is performed by air samplers placed in multiple locations around the plant sites. Milk, vegetation, soil, lake and river water, fish and shell fish are routinely collected, and analyzed by the VA Division of Consolidated Laboratories for radioactivity. Water samples are analyzed for tritium using DRH's liquid scintillation counter located in the mobile radiation laboratory. Sampling activities have been conducted continuously since the early 1970s.

3. Environmental Monitoring Reports

DRH compiles the analysis results of all environmental samples and TLDs collected around the plant sites into an annual report. Annual environmental monitoring reports are routinely provided to county, state and federal agencies and to public libraries, and other interested groups or individuals, upon request.

DRH also conducts environmental monitoring activities at BWXT's Naval Fuel Fabrication Facility, formerly Babcock & Wilcox, located near Lynchburg.

DRH collects split samples with the two major shipyards where naval nuclear re-fueling activities occur. The two shipyards are the Northrup Gruman Shipyard, formerly the Newport News Shipyard and Drydock Company, located in the City of Newport News and the Norfolk Naval Shipyard located in Portsmouth.

DRH participated in EPA's Environmental Radiation Ambient Measurement System (ERAMS). The EPA has modified the system and renamed it RADNET. Two locations have been identified in Virginia for the new monitoring system based on major population centers. The monitoring stations will be co-located with other monitoring equipment operated by the Virginia Department of Environmental Quality.

Radon Public Information and Outreach

The DRH has annually applied for and received a State Indoor Radon Grant from the EPA since the first grant award in 1990. This grant has been used to support a program of technical assistance and information to the public. DRH maintains an in-state toll-free radon hotline and maintains several web pages devoted to radon.

Radiological Emergency Preparedness and Response

The DRH is responsible for maintaining the state's technical response capability to an incident at a nuclear power facility impacting Virginia. Routine staff responsibilities consist of:

- a) Training annually and equipping a network of state and local field teams (first responders) located near each of the two nuclear plants in the state;

- b) Periodically training multi-agency ingestion sampling teams to sample the food supply for radiological contamination;
- c) Ensuring the operational readiness of a mobile radiological laboratory, radio-equipped response vehicles and field instrumentation;
- d) Providing radiation related training to local volunteer, state and county government staff;
- e) Calibrating and maintaining an intrinsic germanium analysis system, liquid scintillation and alpha/beta counter used in the mobile laboratory to quantify radioactive content in environmental samples; and
- f) Participating in all scheduled Radiological Emergency Preparedness (REP) exercises or real events.

Staff also routinely interact with VDEM to maintain the State Radiological Incident Response Plan and develop the technical portion of nuclear plant exercise scenarios. Two DRH staff members are trained to function as the State Radiological Coordinator responsible for coordinating the state technical response during the emergency phase of a power plant incident, developing protective action recommendations based on dose assessment and providing technical advice to the Governor or designee during all phases of the incident. Four DHF staff members are knowledgeable and capable of using the NRC's software, RASCAL, for modeling atmospheric releases from a nuclear power plant accident. DRH staff have participated in all REP exercises since the first exercise was held in the early 1980s. DRH experience also includes several federal exercises (NUWAX 84) and DISPLAY SELECT 95. DISPLAY SELECT 95 was a nuclear weapons accident exercise conducted at Yorktown Naval Weapons Station, VA in 1995 and involved the activation of a full FERMAC facility for one week of real time play.

The DRH's mobile radiological laboratory is equipped to prepare and analyze environmental samples collected by state field teams during a power plant incident or exercise. VDH Staff are trained to operate, maintain and calibrate an intrinsic germanium counting system, alpha/beta counter, and liquid scintillation counter used for radiological sample analysis. The mobile laboratory also functions as a communications center between the DRH and the field teams. Over the last two decades there have been at least four Alerts declared, three at North Anna and one at Surry. In all cases one of the mobile laboratories was deployed as specified in DRH's emergency procedures.

DRH retained the original mobile radiation laboratory, a 1982 Chevy cube van, for responding to transportation accidents, scrap metal facilities, and landfills since it was smaller and can be parked safely alongside the highway.

Both laboratories were damaged by flooding from the remnants of hurricane "*Gaston*" in August 2004. The 1982 Chevy was replaced by an ambulance type vehicle designed to respond to transportation emergency. It has Canberra's ISOCS gamma spectroscopy system which is

capable of *in situ* gamma analysis. This field laboratory also has a Ludlum Model 3030 alpha/beta counter, and field equipment to support several field teams.

The larger 1986 GMC truck with a van body was out of commission for a year to replace engine, transmission, and rear end; however, due to age of vehicle and continuous repairs the vehicle was permanently taken out of commission when it could not be used for a recent evaluated exercise. This vehicle is being replaced with a new incident command type vehicle which was delivered in January 2008. The incident command vehicle is a 42' 2007 Pierce Enforcer. It contains one high purity Germanium detector, one Sodium-Iodide detector, one alpha/beta counter and one liquid scintillation counter. The command vehicle also has a conference room and a state of the art communication center.

X-ray, and Mammography Inspection:

DRH registers approximately 17,000 X-ray machines that include simple dental X-ray machines to the more complex CT scanners and linear accelerators used for radiation therapy. Those X-ray machines used in the healing arts are also inspected and certified for use. There is a private inspector system in place for the inspection of X-ray machines used in the healing arts. DRH collects fees for registration and those inspections DRH inspectors perform. Three of the DRH inspectors work in different regions in the state based from their respective homes to reduce travel time and expenses.

DRH has a contract with the Food and Drug Administration for inspecting all mammography facilities annually. There are approximately 180 mammography machines used in Virginia.

The DRH has participated in the annual Nationwide Evaluation of X-ray Trends (NEXT) continuously for over 25 years.

Radiological Incident Response

The DRH routinely responds to all types of incidents within Virginia involving radioactive materials not of nuclear power plant origin. There are eight trained DRH staff members who are designated to serve as Duty Officer and are available on a 24-hour, rotating on-call basis to augment local resources and help safeguard public health and safety in the event of a radiological incident. Additional DRH staff are also trained and experienced in responding to radiological incidents.

DRH staff responded to many incidents involving radioactive materials. These incidents ranged from the detection of radioactive material at scrap facilities or landfills to a 1990 transportation accident that closed a portion of an interstate highway while an evaluated nuclear power plant was also underway.

III. RADIOACTIVE MATERIALS PROGRAM (RMP)

Program Description

The RMP is responsible for developing the radioactive materials regulatory structure needed for Virginia to become an agreement state with the NRC.

The program's activities will consist of, but not limited to:

- a) Attending NRC training courses required for Radiation Safety Specialists who will license and inspect the use of radioactive materials;
- b) Accompanying the NRC during their inspections in Virginia;
- c) Develop regulations consistent with NRC's requirements for an agreement;
- d) Develop a fee schedule to support the program;
- e) Develop a database and fee collection system for the licensing processes;
- f) Develop forms and regulatory guides;
- g) Develop procedures for licensing;
- h) Develop procedures for inspections;
- i) Develop procedures for allegations and investigations;
- j) Conducting inspections of NARM users in Virginia; and
- k) Developing the final application needed for Virginia to become an agreement state with the NRC.

Accomplishments

1. All NRC licensees in Virginia were informed of the Governor's letter of intent to participate in the agreement state program.
2. Operating funds to support program development are supplied by a special fund within VDH for a period of three years. This revenue source will fund development of a materials licensing and inspection program in the DRH, including salary and fringe expenses, travel, training, observation of NRC inspections, incident response, printing, equipment and administrative costs. When the agreement is signed, application and license fees will fund program operation.

3. A new Materials Licensing and Inspection Unit with a separate Director was authorized for DRH.
4. The RMP receives periodic updates of NRC licenses in Virginia from NRC Region I. A database has been compiled which contains all radioactive material users in Virginia, including all NRC licensees and current NARM licensees. This database contains basic information such as facility name, NRC license and/or NARM license number, location of material use, contact, license type, fee code, and inspection priority. Currently, the database is being used to determine future inspection and licensing workload. At present, the RMP estimates there are about 400 future Virginia licensees.
5. The RMP has a total of 5.0 FTE staff including 4.0 FTE Radiation Safety Specialists and 1.0 FTE Director. Currently there is also a 1.0 FTE Program Support Specialist in the business unit. A request for 2.0 more FTE for licensing and inspecting and 1.0 FTE program assistant will be provided to management in 2008.

Naturally Occurring and Accelerator Produced Radioactive Material (NARM) Licensing and Inspection

Radiation Safety Specialists conduct periodic inspections of NARM users. There are currently 215 NARM licenses of which 179 also possess an NRC license.

Staff Designated for Training, Procedure & Regulation Development

The RMP intends to utilize the Radiation Safety Specialists in all aspects of the program. All Radiation Safety Specialists will be trained to conduct licensing reviews, perform inspections and participate in enforcement activities. During the implementation phase, Radiation Safety Specialists who have completed the appropriate NRC training courses will be the lead inspector during inspections with newer, less trained Radiation Safety Specialists participating as observers to receive on-the-job experience. The DRMP will perform accompaniments in order to qualify each Radiation Safety Specialist for each type of inspection. Ultimately, all full-time Radiation Safety Specialists will receive the appropriate training for each of the various types of license inspections.

RMP staff have attended numerous NRC training classes to date and are being scheduled in 2008 to attend more NRC training classes. The following is a detailed description for each RMP staff member:

- Michael Welling:
1. Health Physics (H-109)
 2. Transportation (H-308)
 3. Diagnostic and Therapeutic Nuclear Medicine (H-304)
 4. Teletherapy and Brachytherapy (H-313)
 5. Industrial Radiography (H-305)
 6. Licensing Practices and Procedures (G-109)
 7. Inspections Procedures (G-108)
 8. Root Cause (G-205)

9. Inspection for Performance (G-304)
10. Irradiator Technology (H-315)
11. Well Logging (H-314)
12. Increased Controls

- Kim Gilliam:
1. Transportation (H-308)
 2. Industrial Radiography (H-305)
 3. Inspections Procedures (G-108)
 4. Well Logging (H-314)
 5. Irradiator Technology (H-315)
 6. Increased Controls
 7. Teletherapy and Brachytherapy (H-313)
 8. Environmental Monitoring (H-111)

- Dante Laciste:
1. Licensing Practices and Procedures (G-109)
 2. Inspections Procedures (G-108)
 3. Inspection for Performance (G-304)
 4. Increased Controls
 5. Transportation (H-308)
 6. Industrial Radiography (H-305)
 7. Irradiator Technology (H-315): Scheduled for 5/12/08
 8. Root Cause (G-205): Submitted for 5/19/08
 9. Diagnostic and Therapeutic Nuclear Medicine (H-304): Submitted for 7/27/08
 10. Well Logging (H-314): Submitted for 11/10/08

- Beth Schilke:
1. Licensing Practices and Procedures (G-109)
 2. Inspections Procedures (G-108)
 3. Inspection for Performance (G-304)
 4. Increased Controls
 5. Transportation (H-308)
 6. Diagnostic and Therapeutic Nuclear Medicine (H-304)
 7. Air Sampling (H-119)
 8. Industrial Radiography (H-305): Submitted for 10/20/08

- Charles Coleman:
1. Transportation (H-308)
 2. Inspection for Performance (G-304)
 3. Increased Controls
 4. Air Sampling (H-119)
 5. Industrial Radiography (H-305): Approved for 6/23/08
 6. Irradiator Technology (H-315): Submitted for 9/29/08
 8. Well Logging (H-314): Submitted for 11/10/08

Several RMP staff members have previous agreement state work. Mr. Welling worked in the Wisconsin program for almost 5 years. Ms. Gilliam worked for the Tennessee program for 6 years and Mr. Coleman worked for the Kentucky program for 10 years. Due to Ms. Gilliam and Mr. Coleman's extensive history with inspections of radioactive licensees, I have approved them to be qualified inspectors for all types of licensees. Due to Mr. Coleman's prior experience with licensing, I have approved him to be qualified as a license reviewer. Mr. Coleman was also provided on the job training with regards to Virginia's process for reviewing and creating a license. Mr. Welling performed all types of licensing and inspections while working in the Wisconsin program. Mr. Welling has attended the courses that were not provided during his tenure with the Wisconsin program.

All current staff members and future staff members will attend the core training courses as necessary to perform their duties. There are enough trained and proficient staff members for each license type to allow for licensing and inspecting. Other staff members will attend the necessary courses as approved by the NRC in 2009 and/or will be trained by proficient staff members.

To date over 80 inspections involving NARM have been performed and approximately 150 NARM licenses have been either amended or renewed by staff members.

Program Management

The DRMP will:

- Inform the DRH director on a quarterly basis concerning the status of overdue inspections, licensing actions which exceed the assigned 30-60-90 day time-frames, and staffing and training needs.
- Conduct supervisory accompaniments annually for all Radiation Safety Specialists conducting radioactive materials inspections.
- Ensure that survey instruments utilized by the RMP are calibrated annually.
- Ensure that notifications are made of reportable incidents to the NRC Operations Center and Region I Office for immediate and 24-hour reports, or the Region I Office and NMED for 30-day reports. See RMPP 4.2.
- Ensure Virginia's Radiation Protection Regulations are current with 10 CFR.
- Ensure all Radiation Safety Specialists receive the necessary NRC training or on the job experience.

Licensing, Inspection & Enforcement, and Allegations & Incident Response Program Description

The RMP will perform license reviews, conduct inspections and enforcement activities, notify licensees of generic problems, and respond to allegations and incidents involving radioactive materials. The routine activities for each aspect of the program are detailed in the RMPPs. An overview of the conduct of program activities is provided below.

License reviews will be conducted using Virginia Regulatory Guides (VAREG). The RMP has developed 'VAREGs' for Portable Gauges and XRFs, Fixed Gauges, Commercial Radiopharmacy, Medical, Radiography, Limited Scope, Broad Scope, Sealed Source Irradiators, Sealed Sources, Well Logging, and Pool Irradiator licensees. Likewise Application forms will be developed for the aforementioned licensees.

The close correlation between the application form and the VAREGs, will facilitate submittal of the needed information for new applications and renewals. Other forms including checklists, a Notice to Employees and information summaries have also been developed to assist licensees and registrants.

The RMP has the option to modify regulatory requirements through the use of legally binding requirements. These can take the form of orders, notices, or license conditions-or a combination of these. 12VAC5-481-90 gives VDH the authority to grant exemptions or exceptions. 12VAC5-481-490 and 580 grants VDH authority to incorporate additional requirements and conditions and modify license conditions. Other regulatory issues or problems that arise will be evaluated for the best approach.

Inspection checklists/reports have been developed for the same categories as licensing. Inspections will be performance-based, therefore, if any area on the checklist was not covered during the inspection the report will state 'not reviewed'. Inspection checklists/reports will be based on the information discussed in NRC's Manual Chapter 2800, Inspection Procedures and checklists will be modified as needed to reflect Virginia Rules and license conditions. Virginia's inspection procedures are documented in RMPP Section 2. A sample narrative report is included for review.

Enforcement actions are discussed in RMPP 2.5, "Enforcement, Escalated Enforcement and Administrative Actions" and include notices of violation, forfeitures and orders. The authority to issue orders is found in 12VAC5-481-110. A notice of violation will normally be issued by the Radiation Safety Specialists. Escalated enforcement actions must be issued by the DRMP or higher level manager. A designated attorney in the Office of the Attorney General is available to provide assistance with enforcement actions upon the request of the DRH Director.

Information Notices (INs) issued by the NRC will be evaluated for applicability to Virginia licensees. The RMP will also evaluate inspection findings for generic health and safety problems that are specific to Virginia licensees (e.g., NARM licensees). The RMP will forward applicable INs or generic health and safety information to affected licensees.

Response to allegations or incidents involving radioactive materials will be based on the RMPPs. The allegations procedure will be used by Radiation Safety Specialists to respond to allegations of impropriety or wrongdoing by licensees or registrants.

- 2.1 - Scheduling of Inspections
- 2.2 - Inspection Preparation
- 2.3 - Performance Based Inspection
- 2.4 - Documentation of Inspection Results
- 2.5 - Enforcement, Escalated Enforcement and Administrative Actions

Incidents and Allegations:

- 3.1 - Management of Allegations
- 3.2 - Incident Response
- 3.3 - Scrap Yard Incident Response

License Tracking

- 4.1 - Renewal Notices, Receipt and Tracking of Licensing Actions
- 4.2 - Tracking Inspection Reports and Correspondence

Qualifications and Training:

- 5.1 - Qualifications and Training

Staff Needs Analysis

A preliminary Staff Needs Analysis was performed to confirm that the current staff of 6.0 FTEs [4.0 FTE Radiation Safety Specialists, 1.0 FTE Supervisor, and 1.0 FTE Program Assistant], is adequate for transition to becoming an Agreement State.

A guide for the suggested number of technical FTEs was 1.0-1.5 FTEs per 100 licenses. Assuming 400 NRC licenses will transfer to the Commonwealth under the agreement, and there are no licensees that will take significant time to service than the average license, then the staffing level should be in the range of 4.0 to 6.0 FTEs.

Furthermore NRC Region I provided the following information:

Budgeted FTE for Region I Materials Program in FY2008

	Region I	Virginia ²
Materials Licensing ¹	6.2	1.5
Materials Inspection	9.9	2.3
Event Response and Response	0.7	0.2
Allegations	1.9	0.5
Training	0.4	0.1
Security	3.0	0.7
Enforcement	2.0	0.5
Agreement State Activities	1.9	0.5
Total FTE	26	6.3
Number of Licenses	1700	400
Budgeted Activity	Region I	Virginia ²

Notes:

1: Each budgeted activity is in FTE


2: The individual state FTE is based on percentage of state licenses compared to the Region

STAFF BALANCE ANALYSIS

License Category	Inspection staff days Needed	Licensing staff days Needed	VHD Staffing Current 5.0 FTE
Broadscope – Medical (I)	75	72	
Broadscope – Academic (I)	75	72	
Industrial Radiography (I)	160	32	
Nuclear Pharmacy (I)	114	24	
HDR (I)	10	2	
Mobile Nuc-Med (II)	40	18	
Gamma Knife – Teletherapy (III)	6	2	
Medical – Diagnostic (III)	54	54	
Medical – Therapy (III)	132	132	
Manufacturing with Distribution (III)	6	4	
IN-Vitro Testing (V)	2	2	
Fixed Gauges (V)	40	26	
Portable Gauges (V)	108	68	
Research & Development (V)	30	16	
Self Shielded Irradiators (V)	8	4	
Source Material (V)	3	2	
Other – NARM (V)	9	8	
Other (V)	24	20	
Reciprocity (V)	38		
Sum	934	558	
TOTAL		1,492 (5.96 FTE)	1,250

CLASS	Course #	Location	Michael Welling	Kimberly Gilliam	Florentino Laciste	Beth Schilke	Charles Coleman
BASICS							
Health Physics			N/A	N/A	N/A	N/A	N/A
Inspection Procedures	G-108	Chattanooga, TN	N/A	N/A	4/13/07	4/13/07	N/A
Licensing Procedures	G-109	Chattanooga, TN	N/A	N/A	3/9/07	3/9/07	N/A
Transportation of RAM	H-308	Chattanooga, TN	N/A	N/A	10/26/07	4/27/07	10/26/07
Nuclear Medicine	H-304	TBD	N/A			3/28/08	
Medical Therapy	H-313	TBD	N/A	4/4/08			
SPECIALIZED							
Increased Controls			N/A	12/14/07	8/10/07	12/14/07	4/18/08
Inspection for Performance	G-304	Chattanooga, TN	N/A	N/A	9/13/07	9/13/07	4/3/08
Radiography	H-305	TBD	N/A	N/A	4/4/08		
Well-Logging	H-314	Houston, TX		11/9/07			
Irradiator	H-315	Montreal, Canada		6/8/07	5/16/08		
Root Cause	G-205		N/A	N/A			5/23/08
Air Sampling	H-119	Oak Ridge				6/6/08	6/6/08
Environmental Monitoring	H-111	Oak Ridge					
RERO			N/A	N/A			

VIRGINIA DEPARTMENT OF HEALTH, OFFICE OF PUBLIC HEALTH

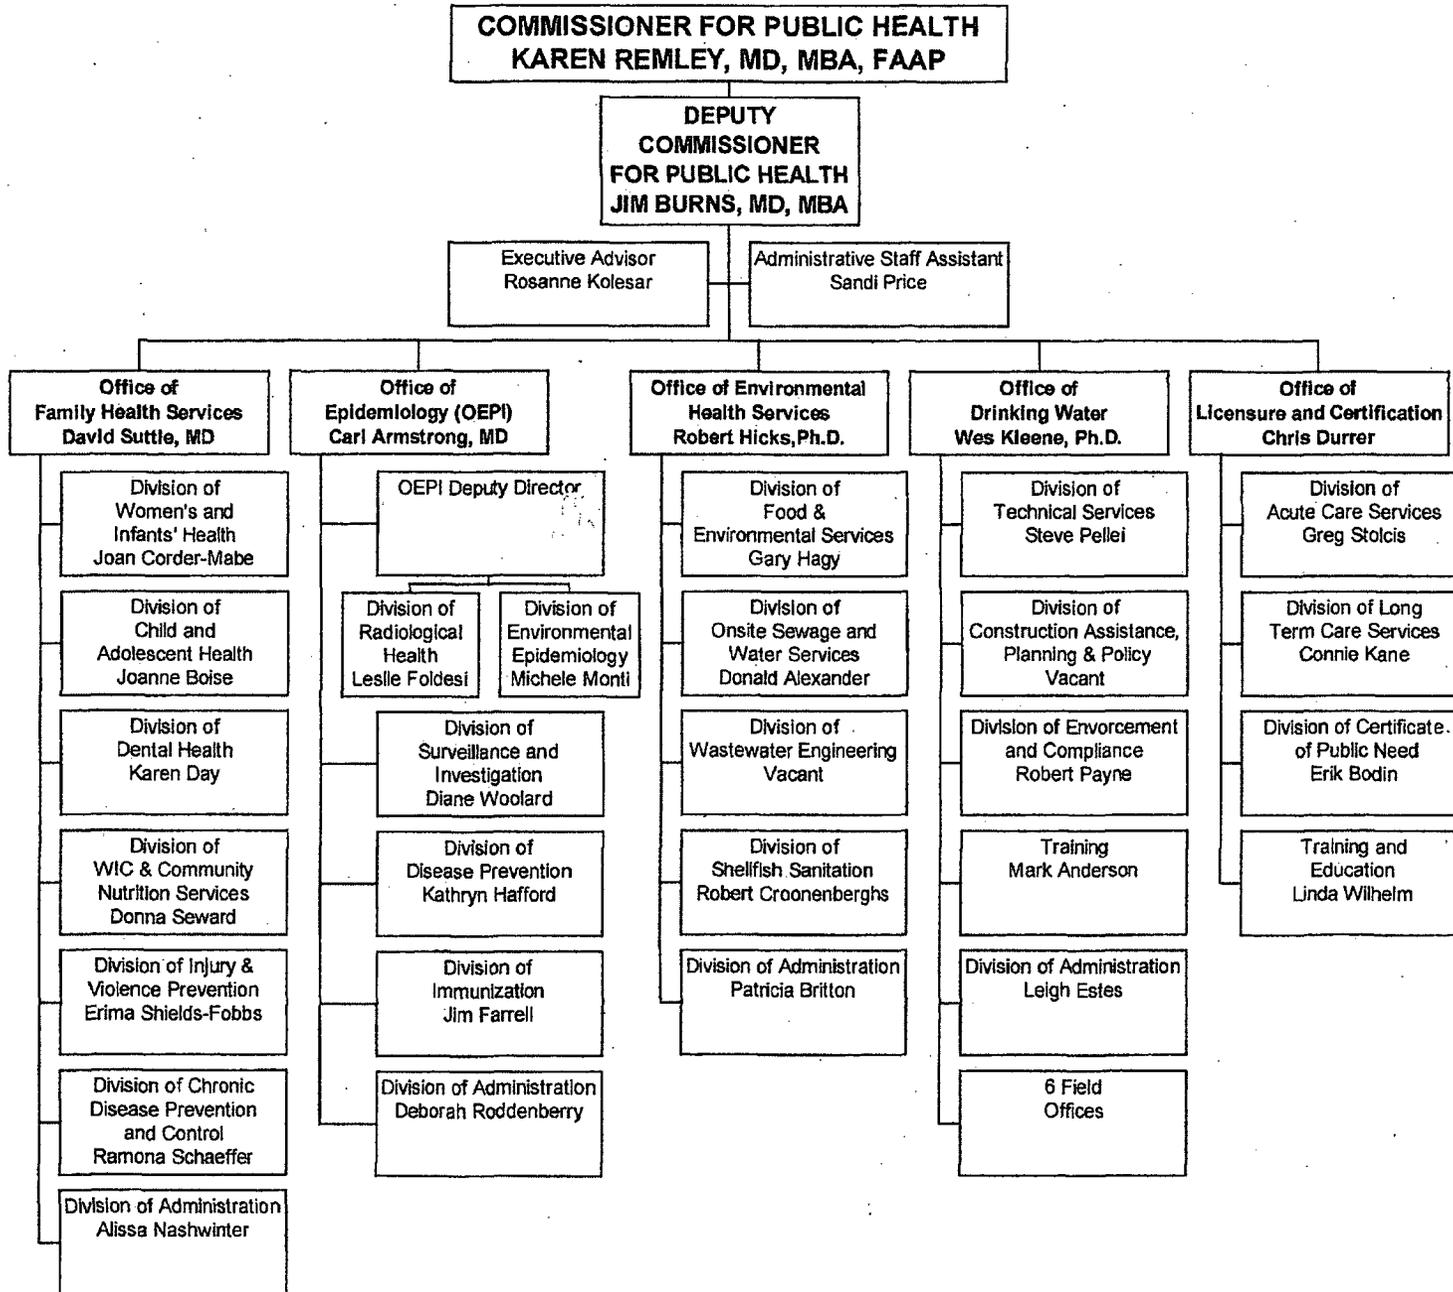

Radiation Safety Specialist

The position's purpose is to perform on-site inspections of licensed radioactive material facilities and file reports; operate analytical instrumentation; review license applications, license amendments, renewal applications and create the radioactive material license; respond to incidents involving radioactive material; participate in nuclear power plant exercises for emergency response preparedness; and interpret state regulations for licensees.

Director, Radioactive Materials Program

The focus of this position will be related to development and management of the Radioactive Materials Program. Supervise, train and evaluate Radiation Safety Specialist staff; review radioactive materials licensing and inspection activities; interpret the radioactive materials regulations and maintains a list of inaccuracies and issues for regulatory review; approve applications and license amendments for radioactive material licenses; review notices of violation and initiate enforcement activities if needed. Participate in the nuclear power plant exercises and other emergency preparedness activities as needed.

Director, Division of Radiological Health

Serve as Division Director of Radiological Health and Safety Regulation. Responsible for all senior-level leadership and management of the following statewide programs: x-ray (register, inspect and certify radiation producing machines), Radioactive Materials (inspect and license radioactive materials), education/technical assistance for indoor radon, environmental monitoring and radiological emergency planning and response. Works with staff, local, state, federal and international agencies, licensees, elected officials and the public.

Resume

Leslie P. Foldesi

Education

Post graduate work in Radiation Physics 1983-1984
Virginia Commonwealth University Richmond, VA

Master of Science- Biology 1982
Virginia Commonwealth University Richmond, VA

Bachelor of Science- Biology 1977
Virginia Commonwealth University Richmond, VA

Certification

American Board of Health Physics in 1993

National Registry of Radiological Radiation Protection Technologists in 1992

Work History

Program Director, Radiological Health Program in the Virginia Department of Health.
October 1988 to present.

Radiation Safety Specialist, Radiological Health Program in the Virginia Department of Health. May 1985 to October 1988.

Radiation Safety Specialist with Environmental Health & Safety, Virginia Commonwealth University. September 1984 to May 1985.

PROFESSIONAL AFFILIATIONS:

Conference of Radiation Control Program Directors

Health Physics Society

Virginia Chapter of the Health Physics Society

Former member of American Association of Physicists in Medicine

Former member of the Mid-Atlantic Chapter of the American Association of Physicists in Medicine

MICHAEL WELLING

2006 to Present: VIRGINIA DEPARTMENT OF HEALTH

Director, Radioactive Materials Program

Create the radioactive materials program in VDH to allow Virginia to become an agreement state.

2002 to 2006: WISCONSIN DEPARTMENT OF HEALTH AND FAMILY SERVICES:
Madison, Wisconsin

Nuclear Engineer

Perform licensing and inspections of radioactive material licensees.

2000 to 2001: LJNDBERG/BLUE M: Watertown, Wisconsin (Manufacturer of industrial heat treating equipment)

Quality Supervisor

Responsible for overseeing machinery testing. Supervised five quality testers.

Performed final machinery inspections prior to shipping.

Conducted vendor audits and coordinated defective material returns. .Handled in-process inspections.

Wrote quality documents and procedures.

2000: ROWLEY -SCHLIMGEN : Madison, Wisconsin (Office furniture design/installation)

Project Coordinator

Responsible for coordinating project installations and planning installation checks.

Reviewed parts orders.

Performed field installations.

Worked with customers to ensure acceptance of installation.

1999 to 2000: SUB-ZERO, INC.: Madison, Wisconsin (Manufacturer of freezers and refrigerators)

Data Management/Engineering

Responsible for the administration of the MAPICS system.

Trained employees.

Entered, audited, and reported data and bills of material.

1994 to 1999 MARQUIP , INC.: Madison, Wisconsin (Manufacturer of cardboard industry machinery)

Product Data Management (1997 -1999)

Responsible for overseeing and managing the entry and upkeep of part number databases.

Provide training and support.

MICHAEL WELLING

Page 2

Worked with engineering and manufacturing to ensure correct and timely entry of data.
Performed monthly queries and reports on the MAPICS database.
Instituted and maintained work instructions to adhere to ISO 9000 standards.

MARQUIP ,INC.: continued

Quality System Technician (1995-1997)

Responsible for inspecting incoming vendor products, inventory control of defective material, and weekly, monthly, quarterly, and yearly reports.
Performed in-process inspection of manufactured products.
Created and updated policies, procedures, and work instructions.

Production Assistant (1994-1995)

Responsible for assembling and wiring cabinets and panels. Supervised six part time employees, including conducting performance reviews.
Assisted engineering with the design and review of cabinets and panels.
Performed formal inspections of completed product.

MILITARY:

1988 to 1994 UNITED STATES NAVY: USS South Carolina (CGN-J7)

Electrical Control Shutdown Reactor Operator/Supply Petty Officer
Responsible for watchstanding, troubleshooting, and repairing generators, motors, and controllers. Supervised 10 electricians.
Maintained a supply budget of \$100,000.
Participated in the overhaul of two nuclear reactors.

EDUCATION:

LAKELAND COLLEGE: Madison, Wisconsin
B.A. in Business Administration

MADISON AREA TECHNICAL COLLEGE: Madison, Wisconsin
Associate Degree, Mid-Business Management

NAVY

Qualified Nuclear Power Plant Operator, SJG Naval Nuclear Prototype
Graduate, Naval Nuclear Power School
Nuclear Theory, Chemistry, Physics, Radiation, Electrical Theory
Graduate, Naval "A" School
Basic Electrical Theory, Motors, Generators

CHARLES COLEMAN

Job History Summary

US Ecology, Inc.

1998 to 2000 Programmer for Inventory Database/Health Physics Manager
US Ecology Oak Ridge Recycle Center

Duties:

- Develop new and conduct quality assurance of existing computer programming to track radioactive material inventory at the recycle facility (IBM AS400 and Microsoft Visual Basic).
- Develop radiation safety, quality assurance, and operating procedures for the facility.
- Prepare and review license application documents for submittal to the state of Tennessee.
- Oversight of the environmental monitoring, instrument calibration, and personnel dosimetry programs for the Recycle Facility.
- Evaluate and implement physical and operational constraints to ensure radiation exposures maintained as low as reasonably achievable.
- Act as Corporate Radiological Control and Safety Officer to assess compliance with radioactive material licenses issued to other US Ecology facilities.

1989 to 1998 Health Physics Manager
Nebraska Low-Level Radioactive Waste Disposal Facility Project

Duties:

- Prepare and review radioactive material license application documents for submittal to the state of Nebraska.
- Develop and implement the preoperational environmental monitoring program for the Nebraska Low-Level Radioactive Waste Facility.
- Develop radiation safety, quality assurance, and operating procedures for the facility.
- Public presentations relating to the project and responses to inquires.

1986 to 1989 Corporate Deputy Chief Radiological Control and Safety Officer
US Ecology Corporate Headquarters

Duties:

- Perform radiation safety, quality assurance, and compliance audits of US Ecology operations, including low-level radioactive waste disposal facilities.
- Prepare and review radiation safety, quality assurance, and operating procedures.
- Prepare and review of radioactive material license applications for submittal to regulatory bodies.
- Train personnel for the radiation safety qualification program, including the preparation of written examinations and acting as a member of oral examination boards.
- Assess personnel dosimetry records, environmental monitoring analytical results, and other records relating to radiation exposure.

Kentucky Cabinet of Human Resources , Radiation Control Branch
(Now Kentucky Cabinet for Health and Human Services, Radiation Health Branch)

1983 to 1986 Principal Technical Reviewer, Radioactive Material Unit

Duties:

- Approval of all radioactive material licenses issued by the state
- Approval of all inspections of radioactive material uses licensed by the state and implementation of regulatory enforcement actions.
- Schedule and oversight of other technical personnel in the unit.
- Review and update state regulations for radioactive material.
- Respond to incidents or accidents related to radioactive material within the state.
- Supervise, train, and evaluate job performance of state technical personnel.
- Develop criteria for the licensing of radioactive material.
- Represent the cabinet in the Kentucky Low-Level Radioactive Waste Task Group.
- Represent the cabinet in the Kentucky Fixed Facility Emergency Response Team.

1980 to 1983 Radioactive Material Specialist

Duties:

- Perform inspections of radioactive material uses.
- Review applications for radioactive material licenses.
- Train new staff members.
- Respond to incidents and accidents related to radioactive material.

1976 to 1980 Field Inspector

Duties:

- Inspect x-ray machine and radioactive and material uses.
- Response to incidents and accidents involving radioactive material.

Kimberly M. Gilliam, HP

Education

Bachelor of Science in Environmental Health, 1997
East Tennessee State University, Johnson City, Tennessee
Accreditation: Southern Association of Colleges and Schools and
National Environmental Health Science and Protection Council

Associate of Arts and Sciences, 1995
Virginia Highlands Community College, Abingdon, Virginia

PADI – Open Water Diver, 1997
Certification Number 9706154682

Certificate of Mechanical Measuring, 1986
Tri-City Technical College, Blountville, Tennessee

Professional experience

2000-present Tennessee Department of Environment and Conservation
Division of Radiological Health Knoxville, Tennessee

Health Physicist III

Inspection and enforcement of x-ray and radioactive material users
Respond to radiation incidents and accidents
Compose and process written reports and correspondence
Maintain radiological files and databases
Participate in emergency response drills at nuclear power plants
Environmental Radiation Ambient Monitoring Systems (ERAMS) for EPA
Training new employees for radioactive material and x-ray inspections

1998-1999 **Tri-State Environmental Lab**
Johnson City, Tennessee

Environmentalist / Organic Chemist
Extract organic compounds from soil, water sludge samples per EPA
Maintain records

1997 **State of Virginia Environmental Specialists**
Abingdon, Virginia

Environmentalist, Internship
Collected water samples for lab analysis
Conducted restaurant inspections
Rabies collection for state lab analysis
Solid Waste research (Virginia Department of Environmental Quality)
Planned and designed septic systems and soil analysis

1986-1992 **Bristol Compressors**
Bristol, Virginia

Machine shop inspector

1984-1986 **Sperry Univac**
Bristol, Tennessee

Incoming computer parts inspector

1980-1983 **Strong Robinette Company**
Bristol, Tennessee

Safety Program Coordinator
Establish safety goals and safe work practices
Conduct safety and first-aid classes
Safety inspection of machinery
Plan and design safety equipment for machinery
Sample/Sales Department

**Professional
Training Courses**

Safety Aspects of Industrial Radiography Course (H-305)
United States Nuclear Regulatory Commission
April 2006

Basic Environmental Crime Investigations
Southern Environmental Enforcement Network
February 2005

Diagnostic X-Ray Physics Course
Oak Ridge Associated Universities
July 2004

Health Physics Technology Course (H-201)
United States Nuclear Regulatory Commission
May 2004

Licensing Practices and Procedures Course (G-109)
United States Nuclear Regulatory Commission
September 2003

Root Cause/Incident Investigation Workshop (G-205)
United States Nuclear Regulatory Commission
July 2003

Nuclear Medicine and Brachytherapy Course
Oak Ridge Associated Universities
December 2002

Inspection Procedures Course (G-108)
United States Nuclear Regulatory Commission
September 2002

Air Sampling for Radioactive Materials (H-119)
United States Nuclear Regulatory Commission
June 2002

Environmental Monitoring for Radioactivity (H-111)
United States Nuclear Regulatory Commission
June 2002

Transportation of Radioactive Materials (H-308)
United States Nuclear Regulatory Commission
April 2002

Health Physics in Radiation Accidents
Radiation Emergency Assistance Center/Training Site (REAC/TS)
August 2001

Extraordinary Customer Service
State of Tennessee, Department of Environment and Conservation
June 2001

40-Hour Course for Hazardous Waste Site Personnel
The University of Tennessee Environmental, Health, and Safety Extension Services
The Midwest Consortium for Hazardous Waste Worker Training
June 2001

Applied Health Physics Course (H-109)
United States Nuclear Regulatory Commission
April/May 2001

ETTP Park Worker Access Training, Module No. 21221
East Tennessee Technology Park
April 2001

Inspecting for Performance Course – Materials Version (G-304)
United States Nuclear Regulatory Commission
February 2001

Training Course for the Use of Nuclear Testing Equipment
Troxler Electronic Laboratories, Inc.
November 2000

Affiliations

- East Tennessee Chapter of the Health Physics Society
- CRCPD

References

Excellent references and university transcript available upon request

Education 1973-1976 Middlesex County College Edison, NJ
 1979 - 1982 Manila Central University Philippines
 ■ Bachelor of Science, Chemistry

Interests Past member Alabama Health Physics Society, travel, golf, reading.

References

- Mr. Timothy Lawrence, Installation Radiation Safety Officer
U.S. Army Combined Arms Support Command Safety Office
ATTN: ATZN-SO
911 Bishop Loop, Bldg 837
Ft Lee, VA 23801-5141 Phone: (804) 765-3128

- Mr. Thomas Dougherty, Installation Radiation Safety Officer
Commander, I Corp & Ft Lewis Command Safety Office
ATTN: AFZH-SA (MS66)
Bldg 207A, Rm 210
Ft Lewis, WA 98433-9500 Phone: (253) 967-6764

- Mr. Jeffrey Harris, Radiation Safety Officer, 63rd Reserve Support Cmd
Occupational Health & Safety Office
ATTN: AFRC-CCA-SA
6235 Yorktown Ave.
Los Alamitos, CA 90720-5002 Phone: (562) 795-2251

Florentino A. Laciste, Jr.

Objective A 14 year radiation worker with 9 years experience in Health Physics seeking to exercise and expand my knowledge and experience in radiation safety. Security clearances were granted over the last 16 years by various agencies.

Experience 2000–2005 New World Technology Livermore, CA

Project Manager/Senior Health Physics Instructor

- Reduced Army-wide NRC violations from 45 violations in 2003 to 16 violations in 2004 through effective license management and comprehensive radiation safety training program.
- Administered and managed the U.S. Army's radiation safety program for Americium-241, Tritium, Promethium, and Nickel-63.
- Mitigated possible NRC violations through a comprehensive inspection and audit program.
- Monitored license initiatives and regulatory requirements to ensure compliance with all pertinent state, local, and federal regulations.
- Gained approval for NRC license amendment request for relief of wipe/leak test requirements for the Chemical Agent Monitor (CAM).

1999–2000 U.S. Army Chemical School Ft Leonard Wood, MO

Senior Instructor/Technical Writer

- U.S. Army Chemical School Alternate Radiation Safety Officer.
- Validated policies and procedures for the safe handling of radioactive material resulting in zero exposures to students and staff.
- Performed duties of Health Physics Technician for the Edwin R. Bradley Radiological Laboratories.
- Calibrated Army RADIACs and comparable civilian instruments using NIST traceable standards.
- Program of Instruction manager for three U.S. Army Radiation Safety Officer's qualifying courses.
- Instructed and qualified Radiation Safety Officers for U.S. Army and Department of Defense civilians.

1991–2000 U.S. Army Chemical School Ft McClellan, AL

Senior Instructor/Technical Writer

- Prepared radio-isotopes in excess of Type A quantities for shipment.
- Performed close-out surveys and decontamination of Ft McClellan sites to Multi Agency Radiation Site Investigation Manual (MARSIM) standards (1996 BRAC).
- Prepared and analyzed leak and survey wipe samples.
- Responsible for 9 certified radiological laboratories and over 35 licensed radio-isotopes ranging in activity from 0.75 micro curies to 137 Curies.

Education 1973-1976 Middlesex County College Edison, NJ
1979 - 1982 Manila Central University Philippines
▪ Bachelor of Science, Chemistry

Interests Past member Alabama Health Physics Society; travel, golf, reading.

References

- Mr. Timothy Lawrence, Installation Radiation Safety Officer
U.S. Army Combined Arms Support Command Safety Office
ATTN: ATZN-SO
911 Bishop Loop, Bldg 837
Ft Lee, VA 23801-5141 Phone: (804) 765-3128

- Mr. Thomas Dougherty, Installation Radiation Safety Officer
Commander, I Corp & Ft Lewis Command Safety Office
ATTN: AFZH-SA (MS66)
Bldg 207A, Rm 210
Ft Lewis, WA 98433-9500 Phone: (253) 967-6764

- Mr. Jeffrey Harris, Radiation Safety Officer, 63rd Reserve Support Cmd
Occupational Health & Safety Office
ATTN: AFRC-CCA-SA
6235 Yorktown Ave.
Los Alamitos, CA 90720-5002 Phone: (562) 795-2251

Beth McFadden Schilke

Objective: To obtain a rewarding career that will allow the implementation of the knowledge gained through studies and work experience.

Education *Environmental Studies, Bachelor of Science, May 2000.*
Southern Vermont College Bennington, VT

Relevant Experience

- Work previously in inspecting facilities and material and documenting any problems found
 - Currently hold a Confidential clearance
 - Experience with various radiacs including E140, E530-N, AN-PDR/27, etc
 - Supervise employees, both currently and in the past, to ensure proper work practices.
 - Provide assistance and follow directions from senior coworkers and supervisors and learn quickly through these situations how to handle any recurrence and other problems.
 - Current position requires maintaining the knowledge of current radiological control practices and basic knowledge required by the US Navy and the ability to interpret this knowledge into a real work practice through oversight of jobs, troubleshooting potential problems prior to starting work and helping to develop an alternative solution. Also required to response to drills and spills.
 - Proficient in Microsoft Word, Excel, and PowerPoint
-

Work Experience

Northrop Grumman
Newport News, VA 23607

Monitor I
(July 2004- present)

Kloke Group
Newport News, VA 23606

Relocation Coordinator
(Aug 2003 - July 2004)

Siracusa Moving & Storage
New Britain, CT 06050

Billing Clerk
(February 2001 - August 2003)

Southern Vermont College
Bennington, VT 05201

Work-Study Supervisor (May 1999 - May 2000)
Work-Study Security Officer (August 1997 - May 1999)

Beth McFadden Schilke

Code of Virginia

§ 32.1-227. Definitions.

As used in this article unless the context requires a different meaning:

1. "By-product material" means:

- a. Any radioactive material, except special nuclear material, yielded in or made radioactive by exposure to the radiation incident to the process of producing or utilizing special nuclear material;
- b. The tailings or wastes produced by the extraction or concentration of uranium or thorium from any ore processed primarily of its source material content;
- c. Any discrete source of radium-226 that is produced, extracted, or converted after extraction for use for a commercial, medical, or research activity;
- d. Any material that has been made radioactive by use of a particle accelerator and is produced, extracted, or converted after extraction for use for a commercial, medical, or research activity; and
- e. Any discrete source of naturally occurring radioactive material (NORM), other than source material that the Nuclear Regulatory Commission (NRC), in consultation with the Administrator of the Environmental Protection Agency, the Secretary of Energy, the Secretary of Homeland Security, and the head of any other appropriate federal agency, determines would pose a threat similar to the threat posed by a discrete source of radium-226 to the public health and safety or the common defense and security, that is extracted, or converted after extraction, for use for a commercial, medical, or research activity.

2. "General license" means a license effective under regulations promulgated by the Board without the filing of an application with the Department or the issuance of licensing documents to particular persons to transfer, acquire, own, possess, or use quantities of, or devices or equipment utilizing, radioactive material.

3. "Ionizing radiation" means gamma rays and X-rays, alpha and beta particles, high-speed electrons, neutrons, protons, and other nuclear particles.

4. "Person" means any individual, corporation, partnership, firm, association, trust, estate, public or private institution, group, department of the Commonwealth other than the Department of Health, political subdivision of the Commonwealth, any other state or political subdivision or department thereof, and any legal successor, representative, agent, or department of the foregoing, but not including federal government agencies.

5. "Radiation emergency" means any situation, excluding events resulting from nuclear warfare, which involves the possibility of accidental release of ionizing radiation that may pose a threat to the safety and health of any citizen of this Commonwealth.

6. "Radioactive material" means any material that emits ionizing radiation spontaneously.

7. "Source material" means uranium or thorium, or any combination thereof, in any physical or chemical form; or ores that contain by weight one-twentieth of one percent (0.05 percent) or more of uranium, thorium, or any combination thereof. Source material does not include special nuclear material.

8. "Special nuclear material" means (i) plutonium, uranium 233, uranium enriched in the isotope 233 or in the isotope 235, and any other material which the United States Nuclear Regulatory Commission or any successor thereto has determined to be such but does not include source material; or (ii) any material artificially enriched by any of the foregoing but not including source material.

9. "Specific license" means a license, issued to a named person upon application filed under the regulations promulgated pursuant to this article, to use, manufacture, produce, transfer, receive, acquire, or possess quantities of, or devices or equipment utilizing, radioactive material.

§ 32.1-228. Exemption.

The provisions of this article shall not apply to radioactive materials or facilities, including nuclear reactors that are subject to exclusive licensing and regulation by the United States Nuclear Regulatory Commission.

§ 32.1-228.1. Department designated state radiation control agency; powers and duties.

A. The Department of Health is hereby designated as the state radiation control agency. The Commissioner of Health may employ, compensate, and prescribe the duties of such individuals as may be necessary to discharge the responsibilities imposed by this article.

B. The Department shall:

1. Collect and disseminate information relating to control of sources of radiation including:
 - a. Establishing and maintaining a file of all applications for, issuances, denials, transfers, renewals, modifications, suspensions and revocations of, and amendments to all licenses;
 - b. Establishing and maintaining a file of registrants possessing sources of radiation requiring registration under the provisions of this article and any administrative or judicial action pertaining thereto; and
 - c. Establishing and maintaining a file of all agency rules and regulations related to regulation of sources of radiation, pending or promulgated, and proceedings thereon.
2. Establish a database of registered and certified X-ray machines, which shall include but not be limited to the name of the owner or operator and the location of the machine.
3. Pursuant to its powers enumerated in § 32.1-25, provide for scheduled and random unannounced inspections of facilities and physicians' offices that provide mammography services to ensure compliance with laws, regulations, or conditions specified by the Board.
4. Establish forms for the periodic Radiation Inspection Report.
5. Develop programs for responding adequately to radiation emergencies and coordinate such programs with the Department of Emergency Management.
6. Maintain, revise as needed, and make available to the public a list of persons who have been listed as proficient to offer screening, testing, or mitigation for radon by the United States Environmental Protection Agency, the National Radon Measurement Proficiency Program of the National Environmental Health Association, or the National Radon Safety Board Certified Radon Professional Program, or any other proficiency program acceptable to the Board of Health.
7. Publish and make available a list of qualified inspectors of X-ray machines.

§ 32.1-229. Powers and duties of the Board.

The Board shall:

1. Establish a program of effective regulation of sources of radiation for the protection of the public health and safety, including a program of education and technical assistance

relating to radon that is targeted to those areas of the Commonwealth known to have high radon levels.

2. Establish a program to promote the orderly regulation of radiation within the Commonwealth, among the states and between the federal government and the Commonwealth and to facilitate intergovernmental cooperation with respect to use and regulation of sources of radiation to the end that duplication of regulation may be minimized.
3. Establish a program to permit maximum utilization of sources of radiation consistent with the public health and safety.
4. Promulgate regulations providing for (i) general or specific licenses to use, manufacture, produce, transfer, receive, acquire, own or possess quantities of, or devices or equipment utilizing, by-product, source, special nuclear materials, or other radioactive material occurring naturally or produced artificially, (ii) registration of the possession of a source of radiation and of information with respect thereto, and (iii) regulation of by-product, source and special nuclear material.
5. Encourage, participate in and conduct studies, investigations, training, research and demonstrations relating to control of sources of radiation.
6. Establish fee schedules for the licensure of radioactive materials.
7. Establish guidelines to require the licensed facilities or physicians' offices where mammography services are performed to offer to the patient, prior to departure, development of such films to ensure integrity and quality of the film. When film developing is not available or the patient chooses not to wait, the patient shall be notified within two business days if another mammogram is necessary. This requirement does not imply or require that a diagnostic opinion be made at the time of the mammogram. The interpreting physician may require that the mammogram be retaken if, in the opinion of the physician, the study is of inadequate quality.
8. Issue such orders or modifications thereof as may be necessary in connection with proceedings under this title.

§ 32.1-229.01. Companies listed as proficient to perform radon screening, testing or mitigation; compliance.

A. No person shall conduct or offer to conduct any radon screening, testing or mitigation in the Commonwealth unless he has been listed as proficient by the United States Environmental Protection Agency, the National Radon Measurement Proficiency Program of the National Environmental Health Association or the National Radon Safety Board Certified Radon Professional Program or any other proficiency program acceptable to the Board of Health to offer such screening, testing or mitigation.

B. Radon professionals listed as proficient pursuant to subsection A shall comply with the radon mitigation and testing standards outlined in the Environmental Protection Agency's publication, EPA 402-R-93-078, as revised, or the American Society for Testing and Materials (ASTM International) Standard, E-2121-02, or any other radon testing and mitigation standards accepted by the Environmental Protection Agency and the Board.

§ 32.1-229.1. Inspections of X-ray machines required; Radiation Inspection Reports; fees; qualification of inspectors.

A. All X-ray machines shall be registered with the Department.

B. Every owner or operator of an X-ray machine used in the healing arts shall request an initial inspection by a private inspector or a Department inspector no later than 30 days after the installation of the equipment.

Inspections shall be performed periodically on a schedule prescribed by the Board. The Department may also require random, unannounced, follow-up inspections of machines that were inspected by private inspectors in order to maintain quality control. In the event of changes in or installations of new equipment during the last 90 days of a period for which an inspection has been made, no interim inspection shall be required. In addition, the Department may require the inspection and certification of other machines emitting radiation or utilizing radiation for patients, consumers, workers, or the general public. Inspections shall be performed by Department personnel or by private inspectors only. Inspections conducted by private inspectors shall be conducted in conformance with the regulations of the Board and reports on these inspections shall be filed by the registrant with the Department on forms prescribed by the Department. Results of all inspections shall be reviewed by the Department.

C. The Department shall issue a certificate for a diagnostic or therapeutic X-ray machine when the results of the inspection indicate the machine meets the Board's standards. If the machine does not meet the Board's standards, the certification may be denied. If the certification is denied, the machine shall not be used for treatment, diagnosis, or evaluation of patients, whether human or animal, until the standards of the Board have been met. A copy of the certificate shall be displayed by the registrant in a conspicuous place in close proximity to the X-ray machine.

D. The Board shall, in accordance with the Administrative Process Act (§ 2.2-4000 et seq.), promulgate such regulations as the Board deems necessary to protect the health and safety of health care workers, patients, and the general public, including but not limited to regulations to:

1. Fee schedules for registration of X-ray machines;
2. Schedule for inspections of X-ray machines;
3. Fee schedules for inspections of X-ray machines by Department personnel; however, no fee shall be charged for inspections initiated by the Department;
4. Standards for certification of X-ray machines; and
5. Qualifications for private inspectors.

E. The provisions of this section and of §§ 32.1-229 and 32.1-229.2 relating to X-ray machines and machines emitting or utilizing radiation shall not apply to devices purchased or used primarily for personal, family, or household purposes.

§ 32.1-229.2. Costs of inspection conducted by Health Department; fees to be used to support program.

In order to minimize competition with the private sector, the fee schedule developed by the Board for routine inspections of X-ray machines by Department of Health inspectors shall include all reasonable costs of such inspections

§ 32.1-229.3. Licensing of Radioactive Material.

A. All radioactive material not under the authority of the United States Nuclear Regulatory Commission, and devices or equipment utilizing such material, shall be licensed by the Board. The Board shall promulgate regulations that provide for general or

specific licenses. The Board may require registration or licensing of any other source of radiation and may exempt certain sources of radiation, uses of radiation, or users of radiation from the licensing and registration requirements set forth in this article when the Commissioner finds that the exemption of such sources, uses, or users of radiation will not constitute a significant risk to the health and safety of the public. The terms and conditions of all licenses shall be subject to amendment, revision, or modification by rules, regulations, or orders issued in accordance with the provisions of this article.

B. Regulations promulgated under this article should provide for recognition of other Agreement State or federal licenses, subject to such requirements as the Board may prescribe.

C. It shall be unlawful for any person to use, manufacture, produce, distribute, sell, transport, transfer, install, repair, receive, acquire, own, or possess any source of radiation unless licensed by or registered with the Department in conformance with this article and any regulations promulgated by the Board pursuant to this article.

§ 32.1-232.1. Special Trust Fund for Radioactive Materials Facility Licensure and Inspection created.

There is hereby created in the Department of the Treasury a special nonreverting fund known as the Special Trust Fund for Radioactive Materials Facility Licensure and Inspection, hereinafter referred to as the "Fund." The Fund shall be established on the books of the Comptroller, and any moneys remaining in the Fund at the end of the biennium shall not revert to the general fund but shall remain in the Fund. All deposits of fees collected pursuant to subdivision 6 of § 32.1-229 shall be paid into the Department of the Treasury and credited to the Fund; in addition, the Fund shall consist of such funds as may be appropriated for the purpose of licensure and inspection of radioactive materials facilities, and such gifts, donations, grants, bequests, and other funds as may be received on its behalf. Interest earned on such moneys shall remain in the Fund and be credited to it. Moneys in the Fund shall be used solely to support the Department of Health's program for licensure and inspection of radioactive materials facilities as provided in this article and Board of Health regulations. Disbursements from the Fund shall be made by the State Treasurer on warrants issued by the Comptroller upon written request of the Commissioner of Health.

§ 32.1-233. Radiation Advisory Board; composition; duties generally.

A. The Radiation Advisory Board shall consist of ten appointive members and the six ex officio members specified below. The Governor shall appoint to the Advisory Board individuals from industry, labor and agriculture as well as individuals with scientific training in one or more of the following fields: radiology, medicine, radiation or health physics, or related sciences, with specialization in ionizing radiation. Not more than two individuals shall be specialists in any one of the above-named fields. Members of the Advisory Board shall serve at the pleasure of the Governor. The Commissioner shall be an ex officio member and chairman of the Advisory Board. The Commissioner of Labor and Industry, the Commissioner of Agriculture and Consumer Services, the State Coordinator of Emergency Management, the Director of Environmental Quality, and the Director of the Virginia Institute of Marine Science shall be ex officio members of the Advisory Board.

B. The Advisory Board shall meet at least annually and shall:

1. Review and evaluate policies and programs of the Commonwealth relating to ionizing radiation; and
2. Make recommendations to the Commissioner and the Board of Health, the Director of Environmental Quality, and the Virginia Waste Management Board and furnish such technical advice as may be required, on matters relating to development, utilization and regulation of sources of ionizing radiation.

§ 32.1-234.1. Enforcement.

A. Whenever the Department finds, following inspection and examination, that a source of radiation as constructed, operated, or maintained results in a violation of this article or of any regulations promulgated pursuant to this article, the Department shall:

1. Notify the person in control of the source of radiation as to the nature of the violation; and
2. Specify a time frame for termination or abatement of the violation, including a deadline by which the source of the violation shall be reconstructed, operated, or maintained in compliance with this article and any regulations promulgated pursuant to this article.

B. Upon failure to comply with the time frame specified by the Department for termination or abatement of the violation, the Department may revoke the license, and pursue penalties or enforcement in accordance with § 32.1-27.

C. Whenever, in the judgment of the Department, any person has engaged in or is about to engage in any acts or practices that constitute or will constitute an emergency, hazard to health and safety, or a violation of any provision of this article or any rule, regulation, or order issued thereunder, and at the request of the Commissioner, the Attorney General may make application to the appropriate court for an order enjoining such acts or practices, or for an order directing compliance, and upon a showing by the Department that such person has engaged or is about to engage in any such acts or practices, a permanent or temporary injunction, restraining order, or other order may be granted.

D. In addition to the provisions of § 32.1-27, any person who violates the provisions of this article or any order or regulation adopted pursuant thereto shall, upon a finding by a court of competent jurisdiction, be assessed a civil penalty of not more than \$10,000 for each day of such violation. All penalties arising under this section shall be recovered in a civil action brought by the Attorney General in the name of the Commonwealth. Civil penalties collected pursuant to this section shall be paid into the state treasury and credited to the Radioactive Material Perpetual Care Trust Fund created pursuant to § 32.1-232.

E. In addition to the provisions of § 32.1-25, the Department shall have the power to enter at all reasonable times, or in cases of an emergency, upon any private or public property for the purpose of determining whether or not there is compliance with or violation of the provisions of this article and rules and regulations issued thereunder, except that entry into areas under the jurisdiction of the federal government shall be effected only with the concurrence of the federal government or its duly designated representative.

§ 32.1-235. Authority of Governor to enter into agreements with federal government; effect on federal licenses.

A. The Governor is authorized, subject to the appropriation of funds, to enter into agreements with the federal government providing for discontinuance of the federal government's responsibilities with respect to sources of ionizing radiation and the assumption thereof by this Commonwealth.

B. Any person who, on the effective date of an agreement under subsection A, except those exempted under § 32.1-228, possesses a license issued by the federal government shall be deemed to possess the same pursuant to this article. Such license shall expire either ninety days after receipt of a notice from the Department of expiration of such license or on the date of expiration specified in the federal license, whichever is earlier.

§ 32.1-238. Impounding sources of ionizing radiation.

The Department is authorized, in the event of an emergency or under other circumstances constituting a hazard to health and safety, to impound or order the impounding of sources of ionizing radiation in the possession of any person who is not equipped to observe or fails to observe the provisions of this article or any regulations issued thereunder.

Code of Virginia

§ 2.2-4000. Short title; purpose.

A. This chapter may be cited as the "Administrative Process Act."

B. The purpose of this chapter is to supplement present and future basic laws conferring authority on agencies either to make regulations or decide cases as well as to standardize court review thereof save as laws hereafter enacted may otherwise expressly provide. This chapter shall not supersede or repeal additional procedural requirements in such basic laws.

(1975, c. 503, §§ 9-6.14:1. 9-6.14:3; 1977, c. 647; 1984, c. 5; 2001, c. 844.)

§ 2.2-4001. Definitions.

As used in this chapter, unless the context requires a different meaning:

"Agency" means any authority, instrumentality, officer, board or other unit of the state government empowered by the basic laws to make regulations or decide cases.

"Agency action" means either an agency's regulation or case decision or both, any violation, compliance, or noncompliance with which could be a basis for the imposition of injunctive orders, penal or civil sanctions of any kind, or the grant or denial of relief or of a license, right, or benefit by any agency or court.

"Basic law" or "basic laws" means provisions of the Constitution and statutes of the Commonwealth authorizing an agency to make regulations or decide cases or containing procedural requirements therefor.

"Case" or "case decision" means any agency proceeding or determination that, under laws or regulations at the time, a named party as a matter of past or present fact, or of threatened or contemplated private action, either is, is not, or may or may not be (i) in violation of such law or regulation or (ii) in compliance with any existing requirement for obtaining or retaining a license or other right or benefit.

"Guidance document" means any document developed by a state agency or staff that provides information or guidance of general applicability to the staff or public to interpret or implement statutes or the agency's rules or regulations, excluding agency minutes or documents that pertain only to the internal management of agencies. Nothing in this definition shall be construed or interpreted to expand the identification or release of any document otherwise protected by law.

"Hearing" means agency processes other than those informational or factual inquiries of an informal nature provided in §§ 2.2-4007.01 and 2.2-4019 and includes only (i) opportunity for private parties to submit factual proofs in formal proceedings as provided in § 2.2-4009 in connection with the making of regulations or (ii) a similar right of private parties or requirement of public agencies as provided in § 2.2-4020 in connection with case decisions.

"Hearing officer" means an attorney selected from a list maintained by the Executive Secretary of the Supreme Court in accordance with § 2.2-4024.

"Public assistance and social services programs" means those programs specified in § 63.2-100.

"Rule" or "regulation" means any statement of general application, having the force of law, affecting the rights or conduct of any person, adopted by an agency in accordance with the authority conferred on it by applicable basic laws.

"Subordinate" means (i) one or more but less than a quorum of the members of a board constituting an agency, (ii) one or more of its staff members or employees, or (iii) any other person or persons designated by the agency to act in its behalf.

(1975, c. 503, § 9-6.14:4; 1977, cc. 377, 381; 1979, c. 613; 1984, c. 187; 1985, cc. 67, 602; 1997, c. 11; 2001, c. 844; 2002, c. 747; 2007, cc. 873, 916.)

§ 2.2-4002. Exemptions from chapter generally.

A. Although required to comply with § 2.2-4103 of the Virginia Register Act (§ 2.2-4100 et seq.), the following agencies shall be exempted from the provisions of this chapter, except to the extent that they are specifically made subject to §§ 2.2-4024, 2.2-4030 and 2.2-4031:

1. The General Assembly.
2. Courts, any agency of the Supreme Court, and any agency that by the Constitution is expressly granted any of the powers of a court of record.
3. The Department of Game and Inland Fisheries in promulgating regulations regarding the management of wildlife and for all case decisions rendered pursuant to any provisions of Chapters 2 (§ 29.1-200 et seq.), 3 (§ 29.1-300 et seq.), 4 (§ 29.1-400 et seq.), 5 (§ 29.1-500 et seq.), and 7 (§ 29.1-700 et seq.) of Title 29.1.
4. The Virginia Housing Development Authority.
5. Municipal corporations, counties, and all local, regional or multijurisdictional authorities created under this Code, including those with federal authorities.
6. Educational institutions operated by the Commonwealth, provided that, with respect to § 2.2-4031, such educational institutions shall be exempt from the publication requirements only with respect to regulations that pertain to (i) their academic affairs, (ii) the selection, tenure, promotion and disciplining of faculty and employees, (iii) the selection of students, and (iv) rules of conduct and disciplining of students.
7. The Milk Commission in promulgating regulations regarding (i) producers' licenses and bases, (ii) classification and allocation of milk, computation of sales and shrinkage, and (iii) class prices for producers' milk, time and method of payment, butterfat testing and differential.
8. The Virginia Resources Authority.
9. Agencies expressly exempted by any other provision of this Code.
10. The Department of General Services in promulgating standards for the inspection of buildings for asbestos pursuant to § 2.2-1164.
11. The State Council of Higher Education for Virginia, in developing, issuing, and revising guidelines pursuant to § 23-9.6:2.
12. The Commissioner of Agriculture and Consumer Services in adopting regulations pursuant to

subsection B of § 3.1-726 and in adopting regulations pursuant to § 3.1-741.6.

13. The Commissioner of Agriculture and Consumer Services and the Board of Agriculture and Consumer Services in promulgating regulations pursuant to subsections B and C of § 3.1-106.4, subsection B of § 3.1-126.12:1, §§ 3.1-271.1, 3.1-530.1, and 3.1-398, subsections B and C of § 3.1-828.4, and subsection A of § 3.1-884.21:1.

14. The Board of Optometry when specifying therapeutic pharmaceutical agents, treatment guidelines, and diseases and abnormal conditions of the human eye and its adnexa for TPA-certification of optometrists pursuant to Article 5 (§ 54.1-3222 et seq.) of Chapter 32 of Title 54.1.

15. The Virginia War Memorial Foundation.

16. The Virginia Medicaid Prior Authorization Advisory Committee in making recommendations to the Board of Medical Assistance Services regarding prior authorization for prescription drug coverage pursuant to Article 4 (§ 32.1-331.12 et seq.) of Chapter 10 of Title 32.1.

17. The State Board of Education, in developing, issuing, and revising guidelines pursuant to § 22.1-203.2.

18. The Virginia Racing Commission, (i) when acting by and through its duly appointed stewards or in matters related to any specific race meeting or (ii) in promulgating technical rules regulating actual live horse racing at race meetings licensed by the Commission.

19. The Virginia Small Business Financing Authority.

20. The Virginia Economic Development Partnership Authority.

21. The Board of Agriculture and Consumer Services in adopting, amending or repealing regulations pursuant to subsection A (ii) of § 59.1-156.

22. The Insurance Continuing Education Board pursuant to § 38.2-1867.

23. The Board of Health in promulgating the list of diseases that shall be reported to the Department of Health pursuant to § 32.1-35 and in adopting, amending or repealing regulations pursuant to subsection C of § 35.1-14 that incorporate the Food and Drug Administration's Food Code pertaining to restaurants or food service.

24. The nonprofit, nonstock corporation established by the Commissioner of Agriculture and Consumer Services pursuant to § 3.1-14.01.

25. (Expires December 31, 2010) The Secretary of Natural Resources in setting a date of closure for the Chesapeake Bay purse seine fishery for Atlantic menhaden for reduction purposes pursuant to § 28.2-1000.2.

B. Agency action relating to the following subjects shall be exempted from the provisions of this chapter:

1. Money or damage claims against the Commonwealth or agencies thereof.

2. The award or denial of state contracts, as well as decisions regarding compliance therewith.

3. The location, design, specifications or construction of public buildings or other facilities.
4. Grants of state or federal funds or property.
5. The chartering of corporations.
6. Customary military, naval or police functions.
7. The selection, tenure, dismissal, direction or control of any officer or employee of an agency of the Commonwealth.
8. The conduct of elections or eligibility to vote.
9. Inmates of prisons or other such facilities or parolees therefrom.
10. The custody of persons in, or sought to be placed in, mental, penal or other state institutions as well as the treatment, supervision, or discharge of such persons.
11. Traffic signs, markers or control devices.
12. Instructions for application or renewal of a license, certificate, or registration required by law.
13. Content of, or rules for the conduct of, any examination required by law.
14. The administration of pools authorized by Chapter 47 (§ 2.2-4700 et seq.) of this title.
15. Any rules for the conduct of specific lottery games, so long as such rules are not inconsistent with duly adopted regulations of the State Lottery Board, and provided that such regulations are published and posted.
16. Orders condemning or closing any shellfish, finfish, or crustacea growing area and the shellfish, finfish or crustacea located thereon pursuant to Article 2 (§ 28.2-803 et seq.) of Chapter 8 of Title 28.2.
17. Any operating procedures for review of child deaths developed by the State Child Fatality Review Team pursuant to § 32.1-283.1.
18. The regulations for the implementation of the Health Practitioners' Intervention Program and the activities of the Intervention Program Committee pursuant to Chapter 25.1 (§ 54.1-2515 et seq.) of Title 54.1.
19. The process of reviewing and ranking grant applications submitted to the Commonwealth Neurotrauma Initiative Advisory Board pursuant to Chapter 3.1 (§ 51.5-12.1 et seq.) of Title 51.5.
20. Loans from the Small Business Environmental Compliance Assistance Fund pursuant to Article 4 (§ 10.1-1197.1 et seq.) of Chapter 11.1 of Title 10.1.
21. The Virginia Breeders Fund created pursuant to § 59.1-372.
22. The types of pari-mutuel wagering pools available for live or simulcast horse racing.

23. The administration of medication or other substances foreign to the natural horse.

C. Minor changes to regulations published in the Virginia Administrative Code under the Virginia Register Act, Chapter 41 (§ 2.2-4100 et seq.) of this title, made by the Virginia Code Commission pursuant to § 30-150, shall be exempt from the provisions of this chapter.

(1985, c. 602, § 9-6.14:4.1; 1986, c. 615; 1987, cc. 375, 652; 1988, cc. 364, 424, 498, 723, 765, 820; 1989, cc. 54, 299, 478; 1990, cc. 721, 968; 1991, cc. 80, 294, 344; 1992, cc. 200, 409, 488, 592, 793; 1993, cc. 537, 669, 898; 1994, cc. 237, 577, 649, 740, 743, 801; 1995, cc. 103, 499, 516; 1996, cc. 51, 152, 158, 189, 205, 279, 320, 345, 573, 590, 598, 638, 705, 735, 818, 1012; 1997, cc. 87, 88, 109, 212, 390, 439, 567, 624, 785, 806, 845, 850, 861, 868; 1998, cc. 39, 619, 784; 1999, cc. 412, 421, 433, 603; 2000, cc. 382, 400, 924, 1011; 2001, cc. 465, 523, 688, 820, 844; 2003, cc. 639, 695; 2004, c. 802; 2006, c. 442; 2007, cc. 41, 870, 932.)

§ 2.2-4003. Venue.

In all proceedings under § 2.2-4019 or 2.2-4020 venue shall be in the city or county where the administrative agency maintains its principal office or as the parties may otherwise agree. In all proceedings under § 2.2-4026, venue shall be as specified in subdivision 1 of § 8.01-261.

(1975, c. 503, § 9-6.14:5; 1977, c. 624; 2001, c. 844; 2007, cc. 873, 916.)

§ 2.2-4004. Severability.

The provisions of regulations adopted under this chapter or the application thereof to any person or circumstances that are held invalid shall not affect the validity of other regulations, provisions or applications that can be given effect without the invalid provisions or applications. The provisions of all regulations are severable unless (i) the regulation specifically provides that its provisions are not severable or (ii) it is apparent that two or more regulations or provisions must operate in accord with one another.

(1987, c. 55, § 9-6.14:5.1; 2001, c. 844.)

§ 2.2-4005. Review of exemptions by Joint Legislative Audit and Review Commission.

The Joint Legislative Audit and Review Commission shall conduct a review periodically of the exemptions authorized by this chapter. The purpose of this review shall be to assess whether there are any exemptions that should be discontinued or modified.

(1985, c. 602, § 9-6.14:4.1; 1986, c. 615; 1987, cc. 375, 652; 1988, cc. 364, 424, 498, 723, 765, 820; 1989, cc. 54, 299, 478; 1990, cc. 721, 968; 1991, cc. 80, 294, 344; 1992, cc. 200, 409, 488, 592, 793; 1993, cc. 537, 669, 898; 1994, cc. 237, 577, 649, 740, 743, 801; 1995, cc. 103, 499, 516; 1996, cc. 51, 152, 158, 189, 205, 279, 320, 345, 573, 590, 598, 638, 705, 735, 818, 1012; 1997, cc. 87, 88, 109, 212, 390, 439, 567, 624, 785, 806, 845, 850, 861, 868; 1998, cc. 39, 619, 784; 1999, cc. 412, 421, 433, 603; 2000, cc. 382, 400, 924, 1011; 2001, c. 844.)

§ 2.2-4006. Exemptions from requirements of this article.

A. The following agency actions otherwise subject to this chapter and § 2.2-4103 of the Virginia Register Act shall be exempted from the operation of this article:

1. Agency orders or regulations fixing rates or prices.

2. Regulations that establish or prescribe agency organization, internal practice or procedures, including delegations of authority.
3. Regulations that consist only of changes in style or form or corrections of technical errors. Each promulgating agency shall review all references to sections of the Code of Virginia within their regulations each time a new supplement or replacement volume to the Code of Virginia is published to ensure the accuracy of each section or section subdivision identification listed.
4. Regulations that are:
 - a. Necessary to conform to changes in Virginia statutory law or the appropriation act where no agency discretion is involved;
 - b. Required by order of any state or federal court of competent jurisdiction where no agency discretion is involved; or
 - c. Necessary to meet the requirements of federal law or regulations, provided such regulations do not differ materially from those required by federal law or regulation, and the Registrar has so determined in writing. Notice of the proposed adoption of these regulations and the Registrar's determination shall be published in the Virginia Register not less than 30 days prior to the effective date of the regulation.
5. Preliminary program permit fees of the Department of Environmental Quality assessed pursuant to subsection C of § 10.1-1322.2.
6. Regulations of the Pesticide Control Board adopted pursuant to subsection B of § 3.1-249.51 or clause (v) or (vi) of subsection C of § 3.1-249.53 after having been considered at two or more Board meetings and one public hearing.
7. Regulations of the regulatory boards served by (i) the Department of Labor and Industry pursuant to Title 40.1 and (ii) the Department of Professional and Occupational Regulation or the Department of Health Professions pursuant to Title 54.1 that are limited to reducing fees charged to regulants and applicants.
8. The development and issuance of procedural policy relating to risk-based mine inspections by the Department of Mines, Minerals and Energy authorized pursuant to §§ 45.1-161.82 and 45.1-161.292:55.
9. General permits issued by the (a) State Air Pollution Control Board pursuant to Chapter 13 (§ 10.1-1300 et seq.) of Title 10.1 or (b) State Water Control Board pursuant to the State Water Control Law (§ 62.1-44.2 et seq.), Chapter 24 (§ 62.1-242 et seq.) of Title 62.1 and Chapter 25 (§ 62.1-254 et seq.) of Title 62.1, (c) Virginia Soil and Water Conservation Board pursuant to the Virginia Stormwater Management Act (§ 10.1-603.1 et seq.) of Title 10.1, and (d) the development and issuance of general wetlands permits by the Marine Resources Commission pursuant to subsection B of § 28.2-1307, if the respective Board or Commission (i) provides a Notice of Intended Regulatory Action in conformance with the provisions of § 2.2-4007.01, (ii) following the passage of 30 days from the publication of the Notice of Intended Regulatory Action forms a technical advisory committee composed of relevant stakeholders, including potentially affected citizens groups, to assist in the development of the general permit, (iii) provides notice and receives oral and written comment as provided in § 2.2-4007.03, and (iv) conducts at least one public hearing on the proposed general permit.
10. The development and issuance by the Board of Education of guidelines on constitutional

rights and restrictions relating to the recitation of the pledge of allegiance to the American flag in public schools pursuant to § 22.1-202.

11. Regulations of the Board of the Virginia College Savings Plan adopted pursuant to § 23-38.77.

12. Regulations of the Marine Resources Commission.

13. Regulations adopted by the Board of Housing and Community Development pursuant to (i) Statewide Fire Prevention Code (§ 27-94 et seq.), (ii) the Industrialized Building Safety Law (§ 36-70 et seq.), (iii) the Uniform Statewide Building Code (§ 36-97 et seq.), and (iv) § 36-98.3, provided the Board (a) provides a Notice of Intended Regulatory Action in conformance with the provisions of § 2.2-4007.01, (b) publishes the proposed regulation and provides an opportunity for oral and written comments as provided in § 2.2-4007.03, and (c) conducts at least one public hearing as provided in §§ 2.2-4009 and 36-100 prior to the publishing of the proposed regulations. Notwithstanding the provisions of this subdivision, any regulations promulgated by the Board shall remain subject to the provisions of § 2.2-4007.06 concerning public petitions, and §§ 2.2-4013 and 2.2-4014 concerning review by the Governor and General Assembly.

14. Amendments to the list of drugs susceptible to counterfeiting adopted by the Board of Pharmacy pursuant to subsection B of § 54.1-3307.

B. Whenever regulations are adopted under this section, the agency shall state as part thereof that it will receive, consider and respond to petitions by any interested person at any time with respect to reconsideration or revision. The effective date of regulations adopted under this subsection shall be in accordance with the provisions of § 2.2-4015, except in the case of emergency regulations, which shall become effective as provided in subsection B of § 2.2-4012.

C. A regulation for which an exemption is claimed under this section or § 2.2-4002, or 2.2-4011 and that is placed before a board or commission for consideration shall be provided at least two days in advance of the board or commission meeting to members of the public that request a copy of that regulation. A copy of that regulation shall be made available to the public attending such meeting.

(1985, c. 602, § 9-6.14:4.1; 1986, c. 615; 1987, cc. 375, 652; 1988, cc. 364, 424, 498, 723, 765, 820; 1989, cc. 54, 299, 478; 1990, cc. 721, 968; 1991, cc. 80, 294, 344; 1992, cc. 200, 409, 488, 592, 793; 1993, cc. 537, 669, 898; 1994, cc. 237, 577, 649, 740, 743, 801; 1995, cc. 103, 499, 516; 1996, cc. 51, 152, 158, 189, 205, 279, 320, 345, 573, 590, 598, 638, 705, 735, 818, 1012; 1997, cc. 87, 88, 109, 212, 390, 439, 567, 624, 785, 806, 845, 850, 861, 868; 1998, cc. 39, 619, 784; 1999, cc. 412, 421, 433, 603; 2000, cc. 382, 400, 924, 1011; 2001, c. 844; 2003, c. 436; 2005, c. 102; 2006, cc. 632, 719; 2007, cc. 873, 916.)

§ 2.2-4007. Petitions for new or amended regulations; opportunity for public comment.

A. Any person may petition an agency to request the agency to develop a new regulation or amend an existing regulation. The petition shall state (i) the substance and purpose of the rulemaking that is requested, including reference to any applicable Virginia Administrative Code sections, and (ii) reference to the legal authority of the agency to take the action requested.

B. Within 14 days of receiving a petition, the agency shall send a notice identifying the petitioner, the nature of the petitioner's request and the agency's plan for disposition of the petition to the Registrar for publication in the Virginia Register of Regulations in accordance with the provisions of subsection B of § 2.2-4031.

C. A 21-day period for acceptance of written public comment on the petition shall be provided after publication in the Virginia Register. The agency shall issue a written decision to grant or deny the petitioner's request within 90 days following the close of the comment period. However, if the rulemaking authority is vested in an entity that has not met within that 90-day period, the entity shall issue a written decision no later than 14 days after it next meets. The written decision issued by the agency shall include a statement of its reasons and shall be submitted to the Registrar for publication in the Virginia Register of Regulations. Agency decisions to initiate or not initiate rulemaking in response to petitions shall not be subject to judicial review.

(1984, c. 5, § 9-6.14:7.1; 1985, c. 602; 1989, c. 71; 1991, c. 488; 1993, cc. 898, 944; 1994, c. 938; 1995, cc. 25, 677, 717, 790; 1997, c. 87; 2001, c. 844; 2002, cc. 241, 391, 747; 2003, c. 224; 2005, cc. 619, 682; 2007, cc. 873, 916.)

§ 2.2-4007.01. Notice of intended regulatory action; public hearing.

A. In the case of all regulations, except those regulations exempted by § 2.2-4002, 2.2-4006, 2.2-4011, or 2.2-4012.1, an agency shall provide the Registrar of Regulations with a Notice of Intended Regulatory Action that describes the subject matter and intent of the planned regulation. At least 30 days shall be provided for public comment, to include an on-line public comment forum on the Virginia Regulatory Town Hall, after publication of the Notice of Intended Regulatory Action. An agency shall not file proposed regulations with the Registrar until the public comment period on the Notice of Intended Regulatory Action has closed.

B. Agencies shall state in the Notice of Intended Regulatory Action whether they plan to hold a public hearing on the proposed regulation after it is published. Agencies shall hold such public hearings if required by basic law. If the agency states an intent to hold a public hearing on the proposed regulation in the Notice of Intended Regulatory Action, then it shall hold the public hearing. If the agency states in its Notice of Intended Regulatory Action that it does not plan to hold a hearing on the proposed regulation, then no public hearing is required unless, prior to completion of the comment period specified in the Notice of Intended Regulatory Action, (i) the Governor directs the agency to hold a public hearing or (ii) the agency receives requests for a public hearing from at least 25 persons.

(2007, cc. 873, 916.)

§ 2.2-4007.02. Public participation guidelines.

A. Public participation guidelines for soliciting the input of interested parties in the formation and development of its regulations shall be developed, adopted, and used by each agency pursuant to the provisions of this chapter. The guidelines shall set out any methods for the identification and notification of interested parties and any specific means of seeking input from interested persons or groups that the agency intends to use in addition to the Notice of Intended Regulatory Action. The guidelines shall set out a general policy for the use of standing or ad hoc advisory panels and consultation with groups and individuals registering interest in working with the agency. Such policy shall address the circumstances in which the agency considers the panels or consultation appropriate and intends to make use of the panels or consultation.

B. In formulating any regulation, including but not limited to those in public assistance and social services programs, the agency pursuant to its public participation guidelines shall afford interested persons an opportunity to submit data, views, and arguments, either orally or in writing, to the agency, to include an on-line public comment forum on the Virginia Regulatory Town Hall, or other specially designated subordinate. However, the agency may begin drafting

the proposed regulation prior to or during any opportunities it provides to the public to submit comments.

(2007, cc. 873, 916.)

§ 2.2-4007.03. Informational proceedings; effect of noncompliance.

A. In the case of all regulations, except those regulations exempted by § 2.2-4002, 2.2-4006, or 2.2-4011, the proposed regulation and general notice of opportunity for oral or written submittals as to that regulation shall be posted on the Virginia Regulatory Town Hall and published in the Virginia Register of Regulations in accordance with the provisions of subsection B of § 2.2-4031. In addition, the agency may, in its discretion, (i) publish the notice in any newspaper and (ii) publicize the notice through press releases and such other media as will best serve the purpose and subject involved. The Register and any newspaper publication shall be made at least 60 days in advance of the last date prescribed in the notice for such submittals. All notices, written submittals, and transcripts and summaries or notations of oral presentations, as well as any agency action thereon, shall be matters of public record in the custody of the agency.

B. If an agency wishes to change a proposed regulation before adopting it as a final regulation, it may choose to publish a revised proposed regulation, provided the latter is subject to a public comment period of at least 30 additional days and the agency complies in all other respects with this section.

C. In no event shall the failure to comply with the requirements of this section be deemed mere harmless error for the purposes of § 2.2-4027.

(2007, cc. 873, 916.)

§ 2.2-4007.04. Economic impact analysis.

A. Before delivering any proposed regulation under consideration to the Registrar as required in § 2.2-4007.05, the agency shall submit on the Virginia Regulatory Town Hall a copy of that regulation to the Department of Planning and Budget. In addition to determining the public benefit, the Department of Planning and Budget in coordination with the agency shall, within 45 days, prepare an economic impact analysis of the proposed regulation, as follows:

1. The economic impact analysis shall include but need not be limited to the projected number of businesses or other entities to whom the regulation would apply; the identity of any localities and types of businesses or other entities particularly affected by the regulation; the projected number of persons and employment positions to be affected; the impact of the regulation on the use and value of private property, including additional costs related to the development of real estate for commercial or residential purposes; and the projected costs to affected businesses, localities, or entities of implementing or complying with the regulations, including the estimated fiscal impact on such localities and sources of potential funds to implement and comply with such regulation. A copy of the economic impact analysis shall be provided to the Joint Commission on Administrative Rules;

2. If the regulation may have an adverse effect on small businesses, the economic impact analysis shall also include (i) an identification and estimate of the number of small businesses subject to the regulation; (ii) the projected reporting, recordkeeping, and other administrative costs required for small businesses to comply with the regulation, including the type of professional skills necessary for preparing required reports and other documents; (iii) a statement of the probable effect of the regulation on affected small businesses; and (iv) a description of any

less intrusive or less costly alternative methods of achieving the purpose of the regulation. As used in this subdivision, "small business" has the same meaning as provided in subsection A of § 2.2-4007.1; and

3. In the event the Department cannot complete an economic impact statement within the 45-day period, it shall advise the agency and the Joint Commission on Administrative Rules as to the reasons for the delay. In no event shall the delay exceed 30 days beyond the original 45-day period.

B. Agencies shall provide the Department with such estimated fiscal impacts on localities and sources of potential funds. The Department may request the assistance of any other agency in preparing the analysis. The Department shall deliver a copy of the analysis to the agency drafting the regulation, which shall comment thereon as provided in § 2.2-4007.05, a copy to the Registrar for publication with the proposed regulation, and an electronic copy to each member of the General Assembly. No regulation shall be promulgated for consideration pursuant to § 2.2-4007.05 until the impact analysis has been received by the Registrar. For purposes of this section, the term "locality, business, or entity particularly affected" means any locality, business, or entity that bears any identified disproportionate material impact that would not be experienced by other localities, businesses, or entities. The analysis shall represent the Department's best estimate for the purposes of public review and comment on the proposed regulation. The accuracy of the estimate shall in no way affect the validity of the regulation, nor shall any failure to comply with or otherwise follow the procedures set forth in this subsection create any cause of action or provide standing for any person under Article 5 (§ 2.2-4025 et seq.) or otherwise to challenge the actions of the Department hereunder or the action of the agency in adopting the proposed regulation.

(2007, cc. 316, 561, 873, 916.)

§ 2.2-4007.05. Submission of proposed regulations to the Registrar.

Before promulgating any regulation under consideration, the agency shall deliver a copy of that regulation to the Registrar together with a summary of the regulation and a separate and concise statement of (i) the basis of the regulation, defined as the statutory authority for promulgating the regulation, including an identification of the section number and a brief statement relating the content of the statutory authority to the specific regulation proposed; (ii) the purpose of the regulation, defined as the rationale or justification for the new provisions of the regulation, from the standpoint of the public's health, safety, or welfare; (iii) the substance of the regulation, defined as the identification and explanation of the key provisions of the regulation that make changes to the current status of the law; (iv) the issues of the regulation, defined as the primary advantages and disadvantages for the public, and as applicable for the agency or the state, of implementing the new regulatory provisions; and (v) the agency's response to the economic impact analysis submitted by the Department of Planning and Budget pursuant to § 2.2-4007.04. Any economic impact estimate included in the agency's response shall represent the agency's best estimate for the purposes of public review and comment, but the accuracy of the estimate shall in no way affect the validity of the regulation. Staff as designated by the Code Commission shall review proposed regulation submission packages to ensure that the requirements of this subsection are met prior to publication of the proposed regulation in the Register. The summary; the statement of the basis, purpose, substance, and issues; the economic impact analysis; and the agency's response shall be published in the Virginia Register of Regulations and be available on the Virginia Regulatory Town Hall, together with the notice of opportunity for oral or written submittals on the proposed regulation.

(2007, cc. 873, 916.)

§ 2.2-4007.06. Changes between proposed and final regulations.

If one or more changes with substantial impact are made to a proposed regulation from the time that it is published as a proposed regulation to the time it is published as a final regulation, any person may petition the agency within 30 days from the publication of the final regulation to request an opportunity for oral and written submittals on the changes to the regulation. If the agency receives requests from at least 25 persons for an opportunity to submit oral and written comments on the changes to the regulation, the agency shall (i) suspend the regulatory process for 30 days to solicit additional public comment and (ii) file notice of the additional 30-day public comment period with the Registrar of Regulations, unless the agency determines that the changes made are minor or inconsequential in their impact. The comment period, if any, shall begin on the date of publication of the notice in the Register. Agency denial of petitions for a comment period on changes to the regulation shall be subject to judicial review.

(2007, cc. 873, 916.)

§ 2.2-4007.07. State Air Pollution Control Board; variances.

The provisions of §§ 2.2-4007 through 2.2-4007.06 shall not apply to the issuance by the State Air Pollution Control Board of variances to its regulations.

(2007, cc. 873, 916.)

§ 2.2-4007.1. Regulatory flexibility for small businesses; periodic review of regulations.

A. As used in this section, "small business" means a business entity, including its affiliates, that (i) is independently owned and operated and (ii) employs fewer than 500 full-time employees or has gross annual sales of less than \$6 million.

B. In addition to the requirements of §§ 2.2-4007 through 2.2-4007.06, prior to the adoption of any proposed regulation, the agency proposing a regulation shall prepare a regulatory flexibility analysis in which the agency shall consider utilizing alternative regulatory methods, consistent with health, safety, environmental, and economic welfare, that will accomplish the objectives of applicable law while minimizing the adverse impact on small businesses. The agency shall consider, at a minimum, each of the following methods of reducing the effects of the proposed regulation on small businesses:

1. The establishment of less stringent compliance or reporting requirements;
2. The establishment of less stringent schedules or deadlines for compliance or reporting requirements;
3. The consolidation or simplification of compliance or reporting requirements;
4. The establishment of performance standards for small businesses to replace design or operational standards required in the proposed regulation; and
5. The exemption of small businesses from all or any part of the requirements contained in the proposed regulation.

C. Prior to the adoption of any proposed regulation that may have an adverse effect on small businesses, each agency shall notify the Joint Commission on Administrative Rules, through the Virginia Regulatory Town Hall, of its intent to adopt the proposed regulation. The Joint

Commission on Administrative Rules shall advise and assist agencies in complying with the provisions of this section.

D. In addition to the requirements of § 2.2-4017, on or before July 1, 2009, an agency shall review its existing regulations to determine whether they should be continued without change or be amended or repealed, consistent with the stated objectives of applicable law, to minimize the economic impact of regulations on small businesses. If an agency head determines that completion of the review of existing regulations is not feasible by July 1, 2009, that agency shall publish a statement certifying that determination. An agency may extend the date required by this subsection in increments of one year, not to exceed a total of five years.

E. In addition to other requirements of § 2.2-4017, all final regulations adopted after July 1, 2005, shall be reviewed every five years to ensure that they minimize the economic impact on small businesses in a manner consistent with the stated objectives of applicable law.

F. The regulatory review required by this section shall include consideration of:

1. The continued need for the rule;
2. The nature of complaints or comments received concerning the regulation from the public;
3. The complexity of the regulation;
4. The extent to which the regulation overlaps, duplicates, or conflicts with federal or state law or regulation; and
5. The length of time since the regulation has been evaluated or the degree to which technology, economic conditions, or other factors have changed in the area affected by the regulation.

(2005, cc. 619, 682; 2007, cc. 873, 916.)

§ 2.2-4008. Availability of guidance documents.

It shall be the duty of every agency to annually file with the Registrar for publication in the Virginia Register of Regulations a list of any guidance documents upon which the agency currently relies. The filing shall be made on or before January 1 of each year in a format to be developed by the Registrar. Each agency shall also (i) maintain a complete list of all of its currently operative guidance documents and make the list available for public inspection, (ii) make available for public inspection the full texts of all guidance documents to the extent inspection is permitted by law, and (iii) upon request, make copies of such lists or guidance documents available without charge, at cost, or on payment of a reasonable fee.

(1997, c. 11, § 9-6.14:7.2; 2001, c. 844.)

§ 2.2-4009. Evidentiary hearings on regulations.

Where an agency proposes to consider the exercise of authority to promulgate a regulation, it may conduct or give interested persons an opportunity to participate in a public evidentiary proceeding; and the agency shall always do so where the basic law requires a hearing. Evidentiary hearings may be limited to the trial of factual issues directly related to the legal validity of the proposed regulation in any of the relevant respects outlined in § 2.2-4027 of this chapter.

General notice of the proceedings shall be published as prescribed in § 2.2-4007.01. In addition, where the proposed regulation is to be addressed to named persons, the latter shall also be given the same notice individually by mail or otherwise if acknowledged in writing. The proceedings may be conducted separately from, and in any event the record thereof shall be separate from, any other or additional proceedings the agency may choose or be required to conduct for the reception of general data, views, and argument pursuant to § 2.2-4007.02 or otherwise. Any probative evidence may be received except that the agency shall as a matter of efficiency exclude irrelevant, immaterial, insubstantial, privileged, or repetitive proofs, and may deny rebuttal, or cross-examination. Testimony may be admitted in written form provided those who have prepared it are made available for examination in person.

The agency or one or more of its subordinates specially designated for the purpose shall preside at the taking of evidence and may administer oaths and affirmations. The proceedings shall be recorded verbatim and the record thereof shall be made available to interested persons for transcription at their expense or, if transcribed by or for the agency, for inspection or purchase at cost.

Where subordinates preside at the taking of the evidence, they shall report their recommendations and proposed findings and conclusions that shall be made available upon request to the participants in the taking of evidence as well as other interested persons and serve as a basis for exceptions, briefs, or oral argument to the agency itself. Whether or not subordinates take the evidence, after opportunity for the submittal of briefs on request and such oral argument as may be scheduled, the agency may settle the terms of the regulation and shall promulgate it only upon (i) its findings of fact based upon the record of evidence made pursuant to this section and facts of which judicial notice may be taken, (ii) statements of basis and purpose as well as comment upon data received in any informational proceedings held under § 2.2-4007.01 and (iii) the conclusions required by the terms of the basic law under which the agency is operating.

(1975, c. 503, § 9-6.14:8; 1985, c. 602; 2001, c. 844; 2007, cc. 873, 916.)

§ 2.2-4010. Pilot programs for regulations imposing local government mandates.

Where an agency proposes to consider the exercise of authority to promulgate a regulation that will impose a statewide mandate on the Commonwealth's localities, the agency shall consider, where appropriate, implementing the regulation on a limited basis with a representative number of localities. An agency may use such a pilot program to determine the effectiveness or impact of proposed regulations prior to statewide adoption.

(1993, c. 168, § 9-6.14:8.1; 2001, c. 844.)

§ 2.2-4011. Emergency regulations; publication; exceptions.

A. Regulations that an agency finds are necessitated by an emergency situation may be adopted by an agency upon consultation with the Attorney General, which approval shall be granted only after the agency has submitted a request stating in writing the nature of the emergency, and the necessity for such action shall be at the sole discretion of the Governor.

B. Agencies may also adopt emergency regulations in situations in which Virginia statutory law or the appropriation act or federal law or federal regulation requires that a regulation be effective in 280 days or less from its enactment, and the regulation is not exempt under the provisions of subdivision A. 4. of § 2.2-4006. In such cases, the agency shall state in writing the nature of the emergency and of the necessity for such action and may adopt the regulations. Pursuant to § 2.2-

4012, such regulations shall become effective upon approval by the Governor and filing with the Registrar of Regulations.

C. All emergency regulations shall be limited to no more than twelve months in duration. During the twelve-month period, an agency may issue additional emergency regulations as needed addressing the subject matter of the initial emergency regulation, but any such additional emergency regulations shall not be effective beyond the twelve-month period from the effective date of the initial emergency regulation. If the agency wishes to continue regulating the subject matter governed by the emergency regulation beyond the twelve-month limitation, a regulation to replace the emergency regulation shall be promulgated in accordance with this article. The Notice of Intended Regulatory Action to promulgate a replacement regulation shall be filed with the Registrar within sixty days of the effective date of the emergency regulation and published as soon as practicable, and the proposed replacement regulation shall be filed with the Registrar within 180 days after the effective date of the emergency regulation and published as soon as practicable.

D. In the event that an agency concludes that despite its best efforts, a replacement regulation cannot be adopted before expiration of the 12-month period described in subsection C, it may seek the prior written approval of the Governor to extend the duration of the emergency regulation for a period of not more than six additional months. Any such request must be submitted to the Governor at least 30 days prior to the scheduled expiration of the emergency regulation and shall include a description of the agency's efforts to adopt a replacement regulation together with the reasons that a replacement regulation cannot be adopted before the expiration of the emergency regulation. Upon approval of the Governor, the duration of the emergency regulation shall be extended for a period of no more than six months. Such approval shall be in the sole discretion of the Governor and shall not be subject to judicial review. Agencies shall notify the Registrar of Regulations of the new expiration date of the emergency regulation as soon as practicable.

E. Emergency regulations shall be published as soon as practicable in the Register.

F. The Regulations of the Marine Resources Commission shall be excluded from the provisions of this section.

(1975, c. 503, § 9-6.14:9; 1977, cc. 450, 459; 1981, c. 387; 1982, c. 425; 1983, c. 295; 1984, c. 5; 1985, c. 602, § 9-6.14:4.1; 1986, c. 615; 1987, cc. 375, 652; 1988, cc. 364, 424, 498, 723, 765, 820; 1989, cc. 54, 71, 299, 478; 1990, cc. 721, 968; 1991, cc. 80, 294, 344; 1992, cc. 200, 409, 488, 592, 793, 829; 1993, cc. 537, 669, 898; 1994, cc. 237, 577, 649, 740, 743, 801, 938; 1995, cc. 103, 499, 516; 1996, cc. 51, 152, 158, 189, 205, 279, 320, 345, 573, 590, 598, 638, 705, 735, 818, 1012; 1997, cc. 87, 88, 109, 212, 390, 439, 567, 624, 785, 806, 845, 850, 861, 868; 1998, cc. 39, 619, 784; 1999, cc. 412, 421, 433, 603; 2000, cc. 382, 400, 924, 1011; 2001, c. 844; 2007, cc. 873, 916.)

§ 2.2-4012. Purpose; adoption; effective date; filing; duties of Registrar of Regulations.

A. The purpose of the regulatory procedures shall be to provide a regulatory plan that is predictable, based on measurable and anticipated outcomes, and is inclined toward conflict resolution.

B. Subject to the provisions of §§ 2.2-4013 and 2.2-4014, all regulations, including those that agencies, pursuant to § 2.2-4002, 2.2-4006, or 2.2-4011, may elect to dispense with the public procedures provided by §§ 2.2-4007.01 and 2.2-4009, may be formally and finally adopted by the signed order of the agency so stating. No regulation except an emergency regulation or a

noncontroversial regulation promulgated pursuant to § 2.2-4012.1 shall be effective until the expiration of the applicable period as provided in § 2.2-4015. In the case of an emergency regulation filed in accordance with § 2.2-4011, the regulation shall become effective upon its adoption and filing with the Registrar of Regulations, unless a later date is specified. The originals of all regulations shall remain in the custody of the agency as public records subject to judicial notice by all courts and agencies. They, or facsimiles thereof, shall be made available for public inspection or copying. Full and true copies shall also be additionally filed, registered, published, or otherwise made publicly available as required by other laws.

C. Prior to the publication for hearing of a proposed regulation, copies of the regulation and copies of the summary and statement as to the basis, purpose, substance, issues, and the economic impact estimate of the regulation submitted by the Department of Planning and Budget and the agency's response thereto as required by § 2.2-4007.04 shall be transmitted to the Registrar of Regulations, who shall retain these documents.

D. All regulations adopted pursuant to this chapter shall contain a citation to the section of the Code of Virginia that authorizes or requires the regulations and, where the regulations are required to conform to federal law or regulation in order to be valid, a citation to the specific federal law or regulation to which conformity is required.

E. Immediately upon the adoption by any agency of any regulation in final form, a copy of (i) the regulation, (ii) a then current summary and statement as to the basis, purpose, substance, issues, and the economic impact estimate of the regulation submitted by the Department of Planning and Budget, and (iii) the agency's summary description of the nature of the oral and written data, views, or arguments presented during the public proceedings and the agency's comments thereon shall be transmitted to the Registrar of Regulations, who shall retain these documents as permanent records and make them available for public inspection. A draft of the agency's summary description of public comment shall be sent by the agency to all public commenters on the proposed regulation at least five days before final adoption of the regulation.

(1975, c. 503, § 9-6.14:9; 1977, cc. 450, 459; 1981, c. 387; 1982, c. 425; 1983, c. 295; 1984, c. 5; 1989, c. 71; 1992, c. 829; 1993, c. 898; 1994, c. 938; 2001, c. 844; 2003, c. 224; 2007, cc. 873, 916.)

§ 2.2-4012.1. Fast-track rulemaking process.

Notwithstanding any other provision, rules that are expected to be noncontroversial may be promulgated or repealed in accordance with the process set out in this section. Upon the concurrence of the Governor, and after written notice to the applicable standing committees of the Senate of Virginia and the House of Delegates, and to the Joint Commission on Administrative Rules, the agency may submit a fast-track regulation without having previously published a Notice of Intended Regulatory Action. The fast-track regulation shall be published in the Virginia Register of Regulations and posted on the Virginia Regulatory Town Hall, along with an agency statement setting out the reasons for using the fast-track rulemaking process. Such regulations shall be subject to the requirements set out in §§ 2.2-4007.03, 2.2-4007.04, and 2.2-4007.05, except that the time for receiving public comment need not exceed 30 days after (i) publication of the regulation in the Virginia Register of Regulations and (ii) a public comment forum opens on the Virginia Regulatory Town Hall. The time for preparation of the economic impact analysis shall not exceed 30 days. If an objection to the use of the fast-track process is received within the public comment period from 10 or more persons, any member of the applicable standing committee of either house of the General Assembly or of the Joint Commission on Administrative Rules, the agency shall (i) file notice of the objection with the Registrar of Regulations for publication in the Virginia Register, and (ii) proceed with the

normal promulgation process set out in this article with the initial publication of the fast-track regulation serving as the Notice of Intended Regulatory Action. Otherwise, the regulation will become effective or shall be repealed as appropriate, 15 days after the close of the comment period, unless the regulation or repeal is withdrawn or a later effective date is specified by the agency.

(2003, c. 224; 2007, cc. 873, 916.)

§ 2.2-4013. Executive review of proposed and final regulations; changes with substantial impact.

A. The Governor shall adopt and publish procedures by executive order for review of all proposed regulations governed by this chapter by June 30 of the year in which the Governor takes office. The procedures shall include (i) review by the Attorney General to ensure statutory authority for the proposed regulations; and (ii) examination by the Governor to determine if the proposed regulations are (a) necessary to protect the public health, safety and welfare and (b) clearly written and easily understandable. The procedures may also include review of the proposed regulation by the appropriate Cabinet Secretary.

The Governor shall transmit his comments, if any, on a proposed regulation to the Registrar and the agency no later than fifteen days following the completion of the public comment period provided for in § 2.2-4007.01. The Governor may recommend amendments or modifications to any regulation that would bring that regulation into conformity with statutory authority or state or federal laws, regulations or judicial decisions.

Not less than fifteen days following the completion of the public comment period provided for in § 2.2-4007.01, the agency may (i) adopt the proposed regulation if the Governor has no objection to the regulation; (ii) modify and adopt the proposed regulation after considering and incorporating the Governor's objections or suggestions, if any; or (iii) adopt the regulation without changes despite the Governor's recommendations for change.

B. Upon final adoption of the regulation, the agency shall forward a copy of the regulation to the Registrar of Regulations for publication as soon as practicable in the Register. All changes to the proposed regulation shall be highlighted in the final regulation, and substantial changes to the proposed regulation shall be explained in the final regulation.

C. If the Governor finds that one or more changes with substantial impact have been made to the proposed regulation, he may require the agency to provide an additional thirty days to solicit additional public comment on the changes by transmitting notice of the additional public comment period to the agency and to the Registrar within the thirty-day adoption period described in subsection D, and publishing the notice in the Register. The additional public comment period required by the Governor shall begin upon publication of the notice in the Register.

D. A thirty-day final adoption period for regulations shall commence upon the publication of the final regulation in the Register. The Governor may review the final regulation during this thirty-day final adoption period and if he objects to any portion or all of a regulation, the Governor may file a formal objection to the regulation, suspend the effective date of the regulation in accordance with subsection B of § 2.2-4014, or both.

If the Governor files a formal objection to the regulation, he shall forward his objections to the Registrar and agency prior to the conclusion of the thirty-day final adoption period. The Governor shall be deemed to have acquiesced to a promulgated regulation if he fails to object to it or if he fails to suspend the effective date of the regulation in accordance with subsection B of

§ 2.2-4014 during the thirty-day final adoption period. The Governor's objection, or the suspension of the regulation, or both if applicable, shall be published in the Register.

A regulation shall become effective as provided in § 2.2-4015.

E. This section shall not apply to the issuance by the State Air Pollution Control Board of variances to its regulations.

(1984, c. 5, § 9-6.14:9.1; 1993, cc. 551, 772, 898; 1995, cc. 25, 736; 2001, c. 844; 2007, cc. 873, 916.)

§ 2.2-4014. Legislative review of proposed and final regulations.

A. After publication of the Register pursuant to § 2.2-4031, the standing committee of each house of the General Assembly to which matters relating to the content of the regulation are most properly referable or the Joint Commission on Administrative Rules may meet and, during the promulgation or final adoption process, file with the Registrar and the promulgating agency an objection to a proposed or final adopted regulation. The Registrar shall publish any such objection received by him as soon as practicable in the Register. Within 21 days after the receipt by the promulgating agency of a legislative objection, that agency shall file a response with the Registrar, the objecting legislative committee or the Joint Commission on Administrative Rules, and the Governor. If a legislative objection is filed within the final adoption period, subdivision A 1 of § 2.2-4015 shall govern.

B. In addition or as an alternative to the provisions of subsection A, the standing committee of both houses of the General Assembly to which matters relating to the content are most properly referable or the Joint Commission on Administrative Rules may suspend the effective date of any portion or all of a final regulation with the Governor's concurrence. The Governor and (i) the applicable standing committee of each house or (ii) the Joint Commission on Administrative Rules may direct, through a statement signed by a majority of their respective members and by the Governor, that the effective date of a portion or all of the final regulation is suspended and shall not take effect until the end of the next regular legislative session. This statement shall be transmitted to the promulgating agency and the Registrar within the 30-day adoption period, and shall be published in the Register.

If a bill is passed at the next regular legislative session to nullify a portion but not all of the regulation, then the promulgating agency (i) may promulgate the regulation under the provision of subdivision A 4 a of § 2.2-4006, if it makes no changes to the regulation other than those required by statutory law or (ii) shall follow the provisions of §§ 2.2-4007.01 through 2.2-4007.06, if it wishes to also make discretionary changes to the regulation. If a bill to nullify all or a portion of the suspended regulation, or to modify the statutory authority for the regulation, is not passed at the next regular legislative session, then the suspended regulation shall become effective at the conclusion of the session, unless the suspended regulation is withdrawn by the agency.

C. A regulation shall become effective as provided in § 2.2-4015.

D. This section shall not apply to the issuance by the State Air Pollution Control Board of variances to its regulations.

(1984, c. 5, § 9-6.14:9.2; 1993, cc. 551, 772; 2001, c. 844; 2002, c. 677; 2003, c. 212; 2004, c. 777; 2007, cc. 873, 916.)

§ 2.2-4015. Effective date of regulation; exception.

A. A regulation adopted in accordance with this chapter and the Virginia Register Act (§ 2.2-4100 et seq.) shall become effective at the conclusion of the thirty-day final adoption period provided for in subsection D of § 2.2-4013, or any other later date specified by the agency, unless:

1. A legislative objection has been filed in accordance with § 2.2-4014, in which event the regulation, unless withdrawn by the agency, shall become effective on a date specified by the agency that shall be after the expiration of the applicable twenty-one-day extension period provided in § 2.2-4014;
2. The Governor has exercised his authority in accordance with § 2.2-4013 to require the agency to provide for additional public comment, in which event the regulation, unless withdrawn by the agency, shall become effective on a date specified by the agency that shall be after the period for which the Governor has provided for additional public comment;
3. The Governor and (i) the appropriate standing committees of each house of the General Assembly or (ii) the Joint Commission on Administrative Rules have exercised their authority in accordance with subsection B of § 2.2-4014 to suspend the effective date of a regulation until the end of the next regular legislative session; or
4. The agency has suspended the regulatory process in accordance with § 2.2-4007.06, or for any reason it deems necessary or appropriate, in which event the regulation, unless withdrawn by the agency, shall become effective in accordance with subsection B.

B. Whenever the regulatory process has been suspended for any reason, any action by the agency that either amends the regulation or does not amend the regulation but specifies a new effective date shall be considered a readoption of the regulation for the purposes of appeal. If the regulation is suspended under § 2.2-4007.06, such readoption shall take place after the thirty-day public comment period required by that subsection. Suspension of the regulatory process by the agency may occur simultaneously with the filing of final regulations as provided in subsection B of § 2.2-4013.

When a regulation has been suspended, the agency must set the effective date no earlier than fifteen days from publication of the readoption action and any changes made to the regulation. During that fifteen-day period, if the agency receives requests from at least twenty-five persons for the opportunity to comment on new substantial changes, it shall again suspend the regulation pursuant to § 2.2-4007.06.

C. This section shall not apply to the issuance by the State Air Pollution Control Board of variances to its regulations.

(1984, c. 5, § 9-6.14:9.3; 1993, cc. 551, 772, 898; 1995, c. 25; 2001, c. 844; 2002, cc. 391, 677; 2004, c. 777; 2007, cc. 873, 916.)

§ 2.2-4016. Withdrawal of regulation.

Nothing in this chapter shall prevent any agency from withdrawing any regulation at any time prior to the effective date of that regulation. A regulation may be repealed after its effective date only in accordance with the provisions of this chapter that govern the adoption of regulations.

(1984, c. 5, § 9-6.14:9.4; 1985, c. 602; 2001, c. 844.)

§ 2.2-4017. Periodic review of regulations.

Each Governor shall mandate through executive order a procedure for periodic review during that Governor's administration of regulations of agencies within the executive branch of state government. The procedure shall include (i) a review by the Attorney General to ensure statutory authority for regulations and (ii) a determination by the Governor whether the regulations are (a) necessary for the protection of public health, safety and welfare and (b) clearly written and easily understandable.

The Governor may require each agency (i) to review all regulations promulgated by that agency to determine whether new regulations should be adopted and old regulations amended or repealed, and (ii) to prepare a written report summarizing the agency's findings about its regulations, its reasons for its findings and any proposed course of action.

(1984, c. 5, § 9-6.14:25; 2001, c. 844.)

§ 2.2-4018. Exemptions from operation of Article 3.

The following agency actions otherwise subject to this chapter shall be exempted from the operation of this article.

1. The assessment of taxes or penalties and other rulings in individual cases in connection with the administration of the tax laws.
2. The award or denial of claims for workers' compensation.
3. The grant or denial of public assistance or social services.
4. Temporary injunctive or summary orders authorized by law.
5. The determination of claims for unemployment compensation or special unemployment.
6. The suspension of any license, certificate, registration or authority granted any person by the Department of Health Professions or the Department of Professional and Occupational Regulation for the dishonor, by a bank or financial institution named, of any check, money draft or similar instrument used in payment of a fee required by statute or regulation.
7. The determination of accreditation or academic review status of a public school or public school division or approval by the Board of Education of a school division corrective action plan required by § 22.1-253.13:3.

(1985, c. 602, § 9-6.14:4.1; 1986, c. 615; 1987, cc. 375, 652; 1988, cc. 364, 424, 498, 723, 765, 820; 1989, cc. 54, 299, 478; 1990, cc. 721, 968; 1991, cc. 80, 294, 344; 1992, cc. 200, 409, 488, 592, 793; 1993, cc. 537, 669, 898; 1994, cc. 237, 577, 649, 740, 743, 801; 1995, cc. 103, 499, 516; 1996, cc. 51, 152, 158, 189, 205, 279, 320, 345, 573, 590, 598, 638, 705, 735, 818, 1012; 1997, cc. 87, 88, 109, 212, 390, 439, 567, 624, 785, 806, 845, 850, 861, 868; 1998, cc. 39, 619, 784; 1999, cc. 412, 421, 433, 603; 2000, cc. 382, 400, 924, 1011; 2001, c. 844; 2002, c. 747; 2004, c. 965.)

§ 2.2-4019. Informal fact finding proceedings.

A. Agencies shall ascertain the fact basis for their decisions of cases through informal conference or consultation proceedings unless the named party and the agency consent to waive such a

conference or proceeding to go directly to a formal hearing. Such conference-consultation procedures shall include rights of parties to the case to (i) have reasonable notice thereof, (ii) appear in person or by counsel or other qualified representative before the agency or its subordinates, or before a hearing officer for the informal presentation of factual data, argument, or proof in connection with any case, (iii) have notice of any contrary fact basis or information in the possession of the agency that can be relied upon in making an adverse decision, (iv) receive a prompt decision of any application for a license, benefit, or renewal thereof, and (v) be informed, briefly and generally in writing, of the factual or procedural basis for an adverse decision in any case.

B. Agencies may, in their case decisions, rely upon public data, documents or information only when the agencies have provided all parties with advance notice of an intent to consider such public data, documents or information. This requirement shall not apply to an agency's reliance on case law and administrative precedent.

(1975, c. 503, § 9-6.14:11; 1986, c. 615; 1989, c. 601; 1993, c. 898; 1994, c. 748; 1995, c. 398; 2001, c. 844.)

§ 2.2-4020. Formal hearings; litigated issues.

A. The agency shall afford opportunity for the formal taking of evidence upon relevant fact issues in any case in which the basic laws provide expressly for decisions upon or after hearing and may do so in any case to the extent that informal procedures under § 2.2-4019 have not been had or have failed to dispose of a case by consent.

B. Parties to formal proceedings shall be given reasonable notice of the (i) time, place, and nature thereof, (ii) basic law under which the agency contemplates its possible exercise of authority, and (iii) matters of fact and law asserted or questioned by the agency. Applicants for licenses, rights, benefits, or renewals thereof have the burden of approaching the agency concerned without such prior notice but they shall be similarly informed thereafter in the further course of the proceedings whether pursuant to this section or to § 2.2-4019.

C. In all such formal proceedings the parties shall be entitled to be accompanied by and represented by counsel, to submit oral and documentary evidence and rebuttal proofs, to conduct such cross-examination as may elicit a full and fair disclosure of the facts, and to have the proceedings completed and a decision made with dispatch. The burden of proof shall be upon the proponent or applicant. The presiding officers at the proceedings may (i) administer oaths and affirmations, (ii) receive probative evidence, exclude irrelevant, immaterial, insubstantial, privileged, or repetitive proofs, rebuttal, or cross-examination, rule upon offers of proof, and oversee a verbatim recording of the evidence, (iii) hold conferences for the settlement or simplification of issues by consent, (iv) dispose of procedural requests, and (v) regulate and expedite the course of the hearing. Where a hearing officer presides, or where a subordinate designated for that purpose presides in hearings specified in subsection F of § 2.2-4024, he shall recommend findings and a decision unless the agency shall by its procedural regulations provide for the making of findings and an initial decision by the presiding officers subject to review and reconsideration by the agency on appeal to it as of right or on its own motion. The agency shall give deference to findings by the presiding officer explicitly based on the demeanor of witnesses.

D. Prior to the recommendations or decisions of subordinates, the parties concerned shall be given opportunity, on request, to submit in writing for the record (i) proposed findings and conclusions and (ii) statements of reasons therefor. In all cases, on request, opportunity shall be afforded for oral argument (i) to hearing officers or subordinate presiding officers, as the case may be, in all cases in which they make such recommendations or decisions or (ii) to the agency

in cases in which it makes the original decision without such prior recommendation and otherwise as it may permit in its discretion or provide by general rule. Where hearing officers or subordinate presiding officers, as the case may be, make recommendations or decisions, the agency shall receive and act on exceptions thereto.

E. All decisions or recommended decisions shall be served upon the parties, become a part of the record, and briefly state or recommend the findings, conclusions, reasons, or basis therefor upon the evidence presented by the record and relevant to the basic law under which the agency is operating together with the appropriate order, license, grant of benefits, sanction, relief, or denial thereof.

(1975, c. 503, § 9-6.14:12; 1986, c. 615; 1991, c. 584; 1993, c. 898; 1995, c. 398; 2001, c. 844.)

§ 2.2-4020.1. Summary case decisions.

A. Any person who has (i) applied for a permit, certificate, or license from an agency or (ii) received written notice of a potential violation from an agency may request a summary case decision from the agency. The request for a summary case decision shall be in writing, signed by or on behalf of the requestor, and be submitted to the agency secretary as defined by the Rules of the Supreme Court of Virginia. The request shall include:

1. A statement that no material facts are in dispute;
2. A proposed stipulation of all such undisputed material facts concerning the application or notice;
3. A clear and concise statement of the questions of law to be decided by summary case decision; and
4. A statement that the requestor waives his right to any other administrative proceeding provided in this article by the agency on the questions of law to be decided by summary case decision.

B. Within 21 days of receipt of a complete request for summary case decision, the agency shall determine whether the matter in dispute properly may be decided by summary case decision and shall promptly notify the requestor of its determination in writing. If a request for summary case decision is not complete, the agency may request additional specific information from the requestor. The agency shall decide the matter by summary case decision if it determines that there are no disputed issues of material fact. However, if (i) an informal fact-finding proceeding as provided in § 2.2-4019, a formal hearing as provided in § 2.2-4020, or other proceeding authorized by the agency's basic law concerning the application or notice has been scheduled, the requestor has been notified; and the issues that are the subject of such proceeding or hearing include questions that are the subject of the request for summary case decision or (ii) the matter must be decided through any public participation requirements under this chapter or the agency's basic law, the agency shall not be required to decide the matter by summary case decision.

C. Denial of a request for summary case decision shall not be subject to judicial review in accordance with this chapter and the Rules of the Supreme Court of Virginia, and shall not prejudice any rights the requestor has or may have under this chapter or the agency's basic law. Nothing in this article shall prevent an agency from consolidating the summary case decision proceeding into, or proceeding with, a separate informal fact-finding proceeding, formal hearing, or other proceeding authorized by the agency's basic law concerning the matter in question.

D. Upon granting a request for summary case decision, the agency shall establish a schedule for the parties to submit briefs on the questions of law in dispute and may, by agreement of the parties, provide for oral argument.

E. All decisions or recommended decisions shall be served on the requestor, become a part of the record, and briefly state or recommend the findings, conclusions, reasons, or basis therefor upon the evidence contained in the record and relevant to the basic law under which the agency is operating, together with the appropriate order, license, grant of benefits, sanction, relief, or denial thereof.

(2006, c. 702.)

§ 2.2-4021. Timetable for decision; exemptions.

A. In cases where a board or commission meets to render (i) an informal fact-finding decision or (ii) a decision on a litigated issue, and information from a prior proceeding is being considered, persons who participated in the prior proceeding shall be provided an opportunity to respond at the board or commission meeting to any summaries of the prior proceeding prepared by or for the board or commission.

B. In any informal fact-finding, formal proceeding, or summary case decision proceeding in which a hearing officer is not used or is not empowered to recommend a finding, the board, commission, or agency personnel responsible for rendering a decision shall render that decision within 90 days from the date of the informal fact-finding, formal proceeding, or completion of a summary case decision proceeding, or from a later date agreed to by the named party and the agency. If the agency does not render a decision within 90 days, the named party to the case decision may provide written notice to the agency that a decision is due. If no decision is made within 30 days from agency receipt of the notice, the decision shall be deemed to be in favor of the named party. The preceding sentence shall not apply to case decisions before (i) the State Water Control Board or the Department of Environmental Quality to the extent necessary to comply with the federal Clean Water Act, (ii) the State Air Pollution Control Board or the Department of Environmental Quality to the extent necessary to comply with the federal Clean Air Act, or (iii) the Virginia Soil and Water Conservation Board or the Department of Conservation and Recreation to the extent necessary to comply with the federal Clean Water Act. An agency shall provide notification to the named party of its decision within five days of the decision.

C. In any informal fact-finding, formal proceeding, or summary case decision proceeding in which a hearing officer is empowered to recommend a finding, the board, commission, or agency personnel responsible for rendering a decision shall render that decision within 30 days from the date that the agency receives the hearing officer's recommendation. If the agency does not render a decision within 30 days, the named party to the case decision may provide written notice to the agency that a decision is due. If no decision is made within 30 days from agency receipt of the notice, the decision is deemed to be in favor of the named party. The preceding sentence shall not apply to case decisions before (i) the State Water Control Board or the Department of Environmental Quality to the extent necessary to comply with the federal Clean Water Act, (ii) the State Air Pollution Control Board or the Department of Environmental Quality to the extent necessary to comply with the federal Clean Air Act, or (iii) the Virginia Soil and Water Conservation Board or the Department of Conservation and Recreation to the extent necessary to comply with the federal Clean Water Act. An agency shall provide notice to the named party of its decision within five days of the decision.

D. The provisions of subsection B notwithstanding, if the board members or agency personnel

who conducted the informal fact-finding, formal proceeding, or summary case decision proceeding are unable to attend to official duties due to sickness, disability, or termination of their official capacity with the agency, then the timeframe provisions of subsection B shall be reset and commence from the date that either new board members or agency personnel are assigned to the matter or a new proceeding is conducted if needed, whichever is later. An agency shall provide notice within five days to the named party of any incapacity of the board members or agency personnel that necessitates a replacement or a new proceeding.

(1975, c. 503, §§ 9-6.14:11, 9-6.14:12; 1986, c. 615; 1989, c. 601; 1991, c. 584; 1993, c. 898; 1994, c. 748; 1995, c. 398; 2001, c. 844; 2005, c. 102; 2006, c. 702.)

§ 2.2-4022. Subpoenas, depositions and requests for admissions.

The agency or its designated subordinates may, and on request of any party to a case shall, issue subpoenas requiring testimony or the production of books, papers, and physical or other evidence. Any person so subpoenaed who objects may, if the agency does not quash or modify the subpoena at his timely request as illegally or improvidently granted, immediately procure by petition a decision on the validity thereof in the circuit court as provided in § 2.2-4003; and otherwise in any case of refusal or neglect to comply with an agency subpoena, unless the basic law under which the agency is operating provides some other recourse, enforcement, or penalty, the agency may procure an order of enforcement from such court. Depositions de bene esse and requests for admissions may be directed, issued, and taken on order of the agency for good cause shown; and orders or authorizations therefor may be challenged or enforced in the same manner as subpoenas. Nothing in this section shall be taken to authorize discovery proceedings.

(1975, c. 503, § 9-6.14:13; 2001, c. 844.)

§ 2.2-4023. Final orders.

The terms of any final agency case decision, as signed by it, shall be served upon the named parties by mail unless service otherwise made is duly acknowledged by them in writing. The signed originals shall remain in the custody of the agency as public records subject to judicial notice by all courts and agencies; and they, or facsimiles thereof, together with the full record or file in every case shall be made available for public inspection or copying except (i) so far as the agency may withhold the same in whole or part for the purpose of protecting individuals mentioned from personal embarrassment, obloquy, or disclosures of a private nature including statements respecting the physical, mental, moral, or financial condition of such individuals or (ii) for trade secrets or, so far as protected by other laws, other commercial or industrial information imparted in confidence.

(1975, c. 503, § 9-6.14:14; 2001, c. 844.)

§ 2.2-4024. Hearing officers.

A. In all formal hearings conducted in accordance with § 2.2-4020, the hearing shall be presided over by a hearing officer selected from a list prepared by the Executive Secretary of the Supreme Court and maintained in the Office of the Executive Secretary of the Supreme Court. Parties to informal fact-finding proceedings conducted pursuant to § 2.2-4019 may agree at the outset of the proceeding to have a hearing officer preside at the proceeding, such agreement to be revoked only by mutual consent. The Executive Secretary may promulgate rules necessary for the administration of the hearing officer system and shall have the authority to establish the number of hearing officers necessary to preside over administrative hearings in the Commonwealth.

Prior to being included on the list, all hearing officers shall meet the following minimum standards:

1. Active membership in good standing in the Virginia State Bar;
2. Active practice of law for at least five years; and
3. Completion of a course of training approved by the Executive Secretary of the Supreme Court. In order to comply with the demonstrated requirements of the agency requesting a hearing officer, the Executive Secretary may require additional training before a hearing officer shall be assigned to a proceeding before that agency.

B. On request from the head of an agency, the Executive Secretary shall name a hearing officer from the list, selected on a rotation system administered by the Executive Secretary. Lists reflecting geographic preference and specialized training or knowledge shall be maintained by the Executive Secretary if an agency demonstrates the need.

C. A hearing officer shall voluntarily disqualify himself and withdraw from any case in which he cannot accord a fair and impartial hearing or consideration, or when required by the applicable rules governing the practice of law in the Commonwealth. Any party may request the disqualification of a hearing officer by filing an affidavit, prior to the taking of evidence at a hearing, stating with particularity the grounds upon which it is claimed that a fair and impartial hearing cannot be accorded, or the applicable rule of practice requiring disqualification.

The issue shall be determined not less than ten days prior to the hearing by the Executive Secretary of the Supreme Court.

D. Any hearing officer empowered by the agency to provide a recommendation or conclusion in a case decision matter shall render that recommendation or conclusion within ninety days from the date of the case decision proceeding or from a later date agreed to by the named party and the agency. If the hearing officer does not render a decision within ninety days, then the named party to the case decision may provide written notice to the hearing officer and the Executive Secretary of the Supreme Court that a decision is due. If no decision is made within thirty days from receipt by the hearing officer of the notice, then the Executive Secretary of the Supreme Court shall remove the hearing officer from the hearing officer list and report the hearing officer to the Virginia State Bar for possible disciplinary action, unless good cause is shown for the delay.

E. The Executive Secretary shall remove hearing officers from the list, upon a showing of cause after written notice and an opportunity for a hearing. When there is a failure by a hearing officer to render a decision as required by subsection D, the burden shall be on the hearing officer to show good cause for the delay. Decisions to remove a hearing officer may be reviewed by a request to the Executive Secretary for reconsideration, followed by judicial review in accordance with this chapter.

F. This section shall not apply to hearings conducted by (i) any commission or board where all of the members, or a quorum, are present; (ii) the Alcoholic Beverage Control Board, the Virginia Workers' Compensation Commission, the State Corporation Commission, the Virginia Employment Commission, the Department of Motor Vehicles under Title 46.2 (§ 46.2-100 et seq.), § 58.1-2409, or Chapter 27 (§ 58.1-2700 et seq.) of Title 58.1, or the Motor Vehicle Dealer Board under Chapter 15 (§ 46.2-1500 et seq.) of Title 46.2; or (iii) any panel of a health regulatory board convened pursuant to § 54.1-2400, including any panel having members of a relevant advisory board to the Board of Medicine. All employees hired after July 1, 1986, pursuant to §§ 65.2-201 and 65.2-203 by the Virginia Workers' Compensation Commission to

conduct hearings pursuant to its basic laws shall meet the minimum qualifications set forth in subsection A. Agency employees who are not licensed to practice law in the Commonwealth, and are presiding as hearing officers in proceedings pursuant to clause (ii) shall participate in periodic training courses.

G. Notwithstanding the exemptions of subsection A of § 2.2-4002, this article shall apply to hearing officers conducting hearings of the kind described in § 2.2-4020 for the Department of Game and Inland Fisheries, the Virginia Housing Development Authority, the Milk Commission and the Virginia Resources Authority pursuant to their basic laws.

(1986, c. 615, § 9-6.14:14.1; 1988, c. 865; 1990, c. 219; 1991, c. 214; 1992, c. 659; 1993, c. 898; 1995, cc. 744, 776, 803, 805; 1996, cc. 189, 205, 639, 658; 2001, c. 844; 2002, cc. 448, 698.)

§ 2.2-4025. Exemptions operation of this article; limitations.

A. This article shall not apply to any agency action that (i) is placed beyond the control of the courts by constitutional or statutory provisions expressly precluding court review, (ii) involves solely the internal management or routine of an agency, (iii) is a decision resting entirely upon an inspection, test, or election save as to want of authority therefor or claim of arbitrariness or fraud therein, (iv) is a case in which the agency is acting as an agent for a court, or (v) encompasses matters subject by law to a trial de novo in any court.

B. The provisions of this article, however, shall apply to case decisions regarding the grant or denial of Temporary Assistance for Needy Families, Medicaid, food stamps, general relief, auxiliary grants, or state-local hospitalization. However, no appeal may be brought regarding the adequacy of standards of need and payment levels for public assistance and social services programs. Notwithstanding the provisions of § 2.2-4027, the review shall be based solely upon the agency record, and the court shall be limited to ascertaining whether there was evidence in the agency record to support the case decision of the agency acting as the trier of fact. If the court finds in favor of the party complaining of agency action, the court shall remand the case to the agency for further proceedings. The validity of any statute, regulation, standard or policy, federal or state, upon which the action of the agency was based shall not be subject to review by the court. No intermediate relief shall be granted under § 2.2-4028.

(1975, c. 503, §§ 9-6.14:4.1, 9-6.14:15, 9-6.14:16; 1986, c. 615; 1989, cc. 677, 734; 2001, c. 844; 2002, c. 747.)

§ 2.2-4026. Right, forms, venue.

Any person affected by and claiming the unlawfulness of any regulation, or party aggrieved by and claiming unlawfulness of a case decision and whether exempted from the procedural requirements of Article 2 (§ 2.2-4006 et seq.) or 3 (§ 2.2-4018 et seq.) of this chapter, shall have a right to the direct review thereof by an appropriate and timely court action against the agency or its officers or agents in the manner provided by the rules of the Supreme Court of Virginia. Actions may be instituted in any court of competent jurisdiction as provided in § 2.2-4003, and the judgments of the courts of original jurisdiction shall be subject to appeal to or review by higher courts as in other cases unless otherwise provided by law. In addition, when any regulation or case decision is the subject of an enforcement action in court, it shall also be reviewable by the court as a defense to the action, and the judgment or decree therein shall be appealable as in other cases.

(1975, c. 503, § 9-6.14:16; 1986, c. 615; 1989, cc. 677, 734; 2001, c. 844.)

§ 2.2-4027. Issues on review.

The burden shall be upon the party complaining of agency action to designate and demonstrate an error of law subject to review by the court. Such issues of law include: (i) accordance with constitutional right, power, privilege, or immunity, (ii) compliance with statutory authority, jurisdiction limitations, or right as provided in the basic laws as to subject matter, the stated objectives for which regulations may be made, and the factual showing respecting violations or entitlement in connection with case decisions, (iii) observance of required procedure where any failure therein is not mere harmless error, and (iv) the substantiality of the evidentiary support for findings of fact. The determination of such fact issue shall be made upon the whole evidentiary record provided by the agency if its proceeding was required to be conducted as provided in § 2.2-4009 or 2.2-4020 or, as to subjects exempted from those sections, pursuant to constitutional requirement or statutory provisions for opportunity for an agency record of and decision upon the evidence therein.

In addition to any other judicial review provided by law, a small business, as defined in subsection A of § 2.2-4007.1, that is adversely affected or aggrieved by final agency action shall be entitled to judicial review of compliance with the requirements of subdivision A 2 of § 2.2-4007.04 and § 2.2-4007.1 within one year following the date of final agency action.

When the decision on review is to be made on the agency record, the duty of the court with respect to issues of fact shall be limited to ascertaining whether there was substantial evidence in the agency record upon which the agency as the trier of the facts could reasonably find them to be as it did.

Where there is no agency record so required and made, any necessary facts in controversy shall be determined by the court upon the basis of the agency file, minutes, and records of its proceedings under § 2.2-4007.01 or 2.2-4019 as augmented, if need be, by the agency pursuant to order of the court or supplemented by any allowable and necessary proofs adduced in court except that the function of the court shall be to determine only whether the result reached by the agency could reasonably be said, on all such proofs, to be within the scope of the legal authority of the agency.

Whether the fact issues are reviewed on the agency record or one made in the review action, the court shall take due account of the presumption of official regularity, the experience and specialized competence of the agency, and the purposes of the basic law under which the agency has acted.

(1975, c. 503, § 9-6.14:17; 1989, c. 601; 2001, c. 844; 2005, cc. 619, 682; 2007, cc. 873, 916.)

§ 2.2-4028. Intermediate relief.

When judicial review is instituted or is about to be, the agency concerned may, on request of any party or its own motion, postpone the effective date of the regulation or decision involved where it deems that justice so requires. Otherwise the court may, on proper application and with or without bond, deposits in court, or other safeguards or assurances as may be suitable, issue all necessary and appropriate process to postpone the effective dates or preserve existing status or rights pending conclusion of the review proceedings if the court finds the same to be required to prevent immediate, unavoidable, and irreparable injury and that the issues of law or fact presented are not only substantial but that there is probable cause for it to anticipate a likelihood of reversible error in accordance with § 2.2-4027. Actions by the court may include (i) the stay of operation of agency decisions of an injunctive nature or those requiring the payment of money or suspending or revoking a license or other benefit and (ii) continuation of previous licenses in

effect until timely applications for renewal are duly determined by the agency.

(1975, c. 503, § 9-6.14:18; 2001, c. 844.)

§ 2.2-4029. Court judgments.

Unless an error of law as defined in § 2.2-4027 appears, the court shall dismiss the review action or affirm the agency regulation or decision. Otherwise, it may compel agency action unlawfully and arbitrarily withheld or unreasonably delayed except that the court shall not itself undertake to supply agency action committed by the basic law to the agency. Where a regulation or case decision is found by the court not to be in accordance with law under § 2.2-4027, the court shall suspend or set it aside and remand the matter to the agency for further proceedings, if any, as the court may permit or direct in accordance with law.

(1975, c. 503, § 9-6.14:19; 2001, c. 844.)

§ 2.2-4030. Recovery of costs and attorneys' fees from agency.

A. In any civil case brought under Article 5 (§ 2.2-4025 et seq.) of this chapter or §§ 2.2-4002, 2.2-4006, 2.2-4011, or § 2.2-4018, in which any person contests any agency action, such person shall be entitled to recover from that agency, including the Department of Game and Inland Fisheries, reasonable costs and attorneys' fees if such person substantially prevails on the merits of the case and the agency's position is not substantially justified, unless special circumstances would make an award unjust. The award of attorneys' fees shall not exceed \$25,000.

B. Nothing in this section shall be deemed to grant permission to bring an action against an agency if the agency would otherwise be immune from suit, or to grant a right to bring an action by a person who would otherwise lack standing to bring the action.

C. Any costs and attorneys' fees assessed against an agency under this section shall be charged against the operating expenses of the agency for the fiscal year in which the assessment is made, and shall not be reimbursed from any other source.

(1981, c. 446, § 9-6.14:21; 1997, c. 692; 2001, c. 844.)

§ 2.2-4031. Publication of Virginia Register of Regulations; exceptions; notice of public hearings of proposed regulations.

A. The Registrar shall publish every two weeks a Virginia Register of Regulations that shall include (i) proposed and final regulations; (ii) emergency regulations; (iii) executive orders; (iv) notices of all public hearings on regulations; (v) petitions for rulemaking made in accordance with § 2.2-4007; and (vi) tax bulletins. The entire proposed regulation shall be published in the Register; however, if an existing regulation has been previously published in the Virginia Administrative Code, then only those sections of regulations to be amended need to be published in the Register. If the length of the regulation falls within the guidelines established by the Registrar for the publication of a summary in lieu of the full text of the regulation, then, after consultation with the promulgating agency, the Registrar may publish only the summary of the regulation. In this event, the full text of the regulation shall be available for public inspection at the office of the Registrar and the promulgating agency.

If a proposed regulation is adopted as published or, in the sole discretion of the Registrar of Regulations, the only changes that have been made are those that can be clearly and concisely explained, the adopted regulation need not be published at length. Instead, the Register shall

contain a notation that the proposed regulation has been adopted as published as a proposed regulation without change or stating the changes made. The proposed regulation shall be clearly identified with a citation to the issue and page numbers where published.

A copy of all reporting forms the promulgating agency anticipates will be incorporated into or be used in administering the regulation shall be published with the proposed and final regulation in the Register.

B. Each regulation shall be prefaced with a summary explaining that regulation in plain and clear language. Summaries shall be prepared by the promulgating agency and approved by the Registrar prior to their publication in the Register. The notice required by § 2.2-4007.03 shall include (i) a statement of the date, time and place of the hearing at which the regulation is to be considered; (ii) a brief statement as to the regulation under consideration; (iii) reference to the legal authority of the agency to act; and (iv) the name, address and telephone number of an individual to contact for further information about that regulation. Agencies shall present their proposed regulations in a standardized format developed by the Virginia Code Commission in accordance with subdivision 1 of § 2.2-4104 of the Virginia Register Act (§ 2.2-4100 et seq.). Notwithstanding the exemptions allowed under § 2.2-4002, 2.2-4006 or 2.2-4011, the proposed and final regulations of all agencies shall be published in the Register. However, proposed regulations of the Marine Resources Commission and regulations exempted by subject from the provisions of this chapter by subsection B of § 2.2-4002 shall be exempt from this section.

C. The Virginia Register of Regulations shall be published by posting the Register on the Virginia Code Commission's website. The Virginia Code Commission may arrange for the printing of the Virginia Register as provided in § 30-146.

(1984, c. 5, § 9-6.14:22; 1985, cc. 67, 602; 1986, c. 615; 1988, c. 364; 1989, c. 71; 1992, c. 216; 2001, c. 844; 2002, c. 241; 2003, c. 212; 2007, cc. 300, 873, 916.)

§§ 2.2-4032. , 2.2-4033.

Repealed by Acts 2003, c. 212, cl. 2, effective March 16, 2003.

§ 8.01-581.17. Privileged communications of certain committees and entities.

A. For the purposes of this section:

"Centralized credentialing service" means (i) gathering information relating to applications for professional staff privileges at any public or licensed private hospital or for participation as a provider in any health maintenance organization, preferred provider organization or any similar organization and (ii) providing such information to those hospitals and organizations that utilize the service.

"Patient safety data" means reports made to patient safety organizations together with all health care data, interviews, memoranda, analyses, root cause analyses, products of quality assurance or quality improvement processes, corrective action plans or information collected or created by a health care provider as a result of an occurrence related to the provision of health care services.

"Patient safety organization" means any organization, group, or other entity that collects and analyzes patient safety data for the purpose of improving patient safety and health care outcomes and that is independent and not under the control of the entity that reports patient safety data.

B. The proceedings, minutes, records, and reports of any (i) medical staff committee, utilization review committee, or other committee, board, group, commission or other entity as specified in § 8.01-581.16; (ii) nonprofit entity that provides a centralized credentialing service; or (iii) quality assurance, quality of care, or peer review committee established pursuant to guidelines approved or adopted by (a) a national or state physician peer review entity, (b) a national or state physician accreditation entity, (c) a national professional association of health care providers or Virginia chapter of a national professional association of health care providers, (d) a licensee of a managed care health insurance plan (MCHIP) as defined in § 38.2-5800, (e) the Office of Emergency Medical Services or any regional emergency medical services council, or (f) a statewide or local association representing health care providers licensed in the Commonwealth, together with all communications, both oral and written, originating in or provided to such committees or entities, are privileged communications which may not be disclosed or obtained by legal discovery proceedings unless a circuit court, after a hearing and for good cause arising from extraordinary circumstances being shown, orders the disclosure of such proceedings, minutes, records, reports, or communications. Additionally, for the purposes of this section, accreditation and peer review records of the American College of Radiology and the Medical Society of Virginia are considered privileged communications. Oral communications regarding a specific medical incident involving patient care, made to a quality assurance, quality of care, or peer review committee established pursuant to clause (iii), shall be privileged only to the extent made more than 24 hours after the occurrence of the medical incident.

C. Nothing in this section shall be construed as providing any privilege to health care provider, emergency medical services agency, community services board, or behavioral health authority medical records kept with respect to any patient in the ordinary course of business of operating a hospital, emergency medical services agency, community services board, or behavioral health authority nor to any facts or information contained in such records nor shall this section preclude or affect discovery of or production of evidence relating to hospitalization or treatment of any patient in the ordinary course of hospitalization of such patient.

D. Notwithstanding any other provision of this section, reports or patient safety data in possession of a patient safety organization, together with the identity of the reporter and all related correspondence, documentation, analysis, results or recommendations, shall be privileged

and confidential and shall not be subject to a civil, criminal, or administrative subpoena or admitted as evidence in any civil, criminal, or administrative proceeding. Nothing in this subsection shall affect the discoverability or admissibility of facts, information or records referenced in subsection C as related to patient care from a source other than a patient safety organization.

E. Any patient safety organization shall promptly remove all patient-identifying information after receipt of a complete patient safety data report unless such organization is otherwise permitted by state or federal law to maintain such information. Patient safety organizations shall maintain the confidentiality of all patient-identifying information and shall not disseminate such information except as permitted by state or federal law.

F. Exchange of patient safety data among health care providers or patient safety organizations that does not identify any patient shall not constitute a waiver of any privilege established in this section.

G. Reports of patient safety data to patient safety organizations shall not abrogate obligations to make reports to health regulatory boards or other agencies as required by state or federal law.

H. No employer shall take retaliatory action against an employee who in good faith makes a report of patient safety data to a patient safety organization.

I. Reports produced solely for purposes of self-assessment of compliance with requirements or standards of the Joint Commission on Accreditation of Healthcare Organizations shall be privileged and confidential and shall not be subject to subpoena or admitted as evidence in a civil or administrative proceeding. Nothing in this subsection shall affect the discoverability or admissibility of facts, information, or records referenced in subsection C as related to patient care from a source other than such accreditation body. A health care provider's release of such reports to such accreditation body shall not constitute a waiver of any privilege provided under this section.

(Code 1950, § 8-654.10; 1976, c. 611; 1977, c. 617; 1995, c. 500; 1997, c. 292; 2001, c. 381; 2002, c. 675; 2004, c. 250; 2006, cc. 412, 678; 2007, c. 530.)

§ [19.2-393](#). Definitions.

An "inspection warrant" is an order in writing, made in the name of the Commonwealth, signed by any judge of the circuit court whose territorial jurisdiction encompasses the property or premises to be inspected or entered, and directed to a state or local official, commanding him to enter and to conduct any inspection, testing or collection of samples for testing required or authorized by state or local law or regulation in connection with the manufacturing, emitting or presence of a toxic substance, and which describes, either directly or by reference to any accompanying or attached supporting affidavit, the property or premises where the inspection, testing or collection of samples for testing is to occur. Such warrant shall be sufficiently accurate in description so that the official executing the warrant and the owner or custodian of the property or premises can reasonably determine from the warrant the activity, condition, circumstance, object or property of which inspection, testing or collection of samples for testing is authorized.

For the purposes of this chapter, "manufacturing" means producing, formulating, packaging, or diluting any substance for commercial sale or resale; "emitting" means the release of any substance, whether or not intentional or avoidable, into the work environment, into the air, into the water, or otherwise into the human environment; and "toxic substance" means any substance, including (i) any raw material, intermediate product, catalyst, final product and by-product of any operation conducted in a commercial establishment and (ii) any biological organism, that has the capacity, through its physical, chemical, or biological properties, to pose a substantial risk to humans, aquatic organisms or any other animal of illness, death or impairment of normal functions, either immediately or over a period of time.

(1976, c. 625; 1979, c. 122.)

§ [32.1-25](#). Right of entry to inspect, etc.; warrants.

Upon presentation of appropriate credentials and upon consent of the owner or custodian, the Commissioner or his designee shall have the right to enter at any reasonable time onto any property to inspect, investigate, evaluate, conduct tests or take samples for testing as he reasonably deems necessary in order to determine compliance with the provisions of any law administered by the Board, Commissioner or Department, any regulations of the Board, any order of the Board or Commissioner or any conditions in a permit, license or certificate issued by the Board or Commissioner. This right of entry shall not apply to privileged communications pursuant to § [8.01-581.17](#). If the Commissioner or his designee is denied entry, he may apply to an appropriate circuit court for an inspection warrant authorizing such investigation, evaluation, inspection, testing or taking of samples for testing as provided in Chapter 24 (§ [19.2-393](#) et seq.) of Title 19.2.

(1979, c. 711; 1998, c. 772.)

§ 32.1-27. Penalties, injunctions, civil penalties and charges for violations.

A. Any person willfully violating or refusing, failing or neglecting to comply with any regulation or order of the Board or Commissioner or any provision of this title shall be guilty of a Class 1 misdemeanor unless a different penalty is specified.

B. Any person violating or failing, neglecting, or refusing to obey any lawful regulation or order of the Board or Commissioner or any provision of this title may be compelled in a proceeding instituted in an appropriate court by the Board or Commissioner to obey such regulation, order or provision of this title and to comply therewith by injunction, mandamus, or other appropriate remedy or, pursuant to § 32.1-27.1, imposition of a civil penalty or appointment of a receiver.

C. Without limiting the remedies which may be obtained in subsection B of this section, any person violating or failing, neglecting or refusing to obey any injunction, mandamus or other remedy obtained pursuant to subsection B shall be subject, in the discretion of the court, to a civil penalty not to exceed \$25,000 for each violation, which shall be paid to the general fund, except that civil penalties for environmental pollution shall be paid into the state treasury and credited to the Water Supply Assistance Grant Fund created pursuant to § 32.1-171.2. Each day of violation shall constitute a separate offense.

D. With the consent of any person who has violated or failed, neglected or refused to obey any regulation or order of the Board or Commissioner or any provision of this title, the Board may provide, in an order issued by the Board against such person, for the payment of civil charges for past violations in specific sums, not to exceed the limits specified in § 32.1-27.1 and subsection C of this section. Such civil charges shall be instead of any appropriate civil penalty which could be imposed under § 32.1-27.1 and subsection C of this section. When civil charges are based upon environmental pollution, the civil charges shall be paid into the state treasury and credited to the Water Supply Assistance Grant Fund created pursuant to § 32.1-171.2.

(Code 1950, §§ 32-6.4, 32-15; 1975, c. 564; 1976, c. 623; 1979, c. 711; 1980, c. 378; 1989, c. 618; 1999, c. 786; 2003, cc. 753, 762.)

§ 32.1-27.1. Additional civil penalty or appointment of a receiver.

A. In addition to the remedies provided in § 32.1-27, the civil penalties set forth in this section may be imposed by the circuit court for the city or county in which the facility is located as follows:

1. A civil penalty for a Class I violation shall not exceed the lesser of \$25 per licensed or certified bed or \$1,000 for each day the facility is in violation, beginning on the date the facility was first notified of the violation.
2. A civil penalty for a Class II violation shall not exceed the lesser of \$5 per licensed or certified bed or \$250 per day for each day the facility is in violation, beginning on the date the facility was first notified of the violation.

In the event federal law or regulations require a civil penalty in excess of the amounts set forth above for Class I or Class II violations, then the lowest amounts required by such federal law or regulations shall become the maximum civil penalties under this section. The date of notification under this section shall be deemed to be the date of receipt by the facility of written notice of the alleged Class I or Class II violation, which notice shall include specifics of the violation charged and which notice shall be hand delivered or sent by overnight express mail or by registered or certified mail, return receipt requested.

All civil penalties received pursuant to this subsection shall be paid into a special fund of the Department for the cost of implementation of this section, to be applied to the protection of the health or property of residents or patients of facilities that the Commissioner or the United States Secretary of Health and Human Services finds in violation, including payment for the costs for relocation of patients, maintenance of temporary management or receivership to operate a facility pending correction of a violation, and for reimbursement to residents or patients of lost personal funds.

B. In addition to the remedies provided in § 32.1-27 and the civil penalties set forth in subsection A of this section, the Commissioner may petition the circuit court for the jurisdiction in which any nursing home or certified nursing facility as defined in § 32.1-123 is located for the appointment of a receiver in accordance with the provisions of this subsection whenever such nursing home or certified nursing facility shall (i) receive official notice from the Commissioner that its license has been or will be revoked or suspended, or that its Medicare or Medicaid certification has been or will be cancelled or revoked; or (ii) receive official notice from the United States Department of Health and Human Services or the Department of Medical Assistance Services that its provider agreement has been or will be revoked, cancelled, terminated or not renewed; or (iii) advise the Department of its intention to close or not to renew its license or Medicare or Medicaid provider agreement less than ninety days in advance; or (iv) operate at any time under conditions which present a major and continuing threat to the health, safety, security, rights or welfare of the patients, including the threat of imminent abandonment by the owner or operator, or a pattern of failure to meet ongoing financial obligations such as the inability to pay for essential food, pharmaceuticals, personnel, or required insurance; and (v) the Department is unable to make adequate and timely arrangements for relocating all patients who are receiving medical assistance under this chapter and Title XIX of the Social Security Act in order to ensure their continued safety and health care.

Upon the filing of a petition for appointment of a receiver, the court shall hold a hearing within ten days, at which time the Department and the owner or operator of the facility may participate

and present evidence. The court may grant the petition if it finds any one of the conditions identified in (i) through (iv) above to exist in combination with the condition identified in (v) and the court further finds that such conditions will not be remedied and that the patients will not be protected unless the petition is granted.

No receivership established under this subsection shall continue in effect for more than 180 days without further order of the court, nor shall the receivership continue in effect following the revocation of the nursing home's license or the termination of the certified nursing facility's Medicare or Medicaid provider agreement, except to enforce any post-termination duties of the provider as required by the provisions of the Medicare or Medicaid provider agreement.

The appointed receiver shall be a person licensed as nursing home administrator in the Commonwealth pursuant to Title 54.1 or, if not so licensed, shall employ and supervise a person so licensed to administer the day-to-day business of the nursing home or certified nursing facility.

The receiver shall have (i) such powers and duties to manage the nursing home or certified nursing facility as the court may grant and direct, including but not limited to the duty to accomplish the orderly relocation of all patients and the right to refuse to admit new patients during the receivership, (ii) the power to receive, conserve, protect and disburse funds, including Medicare and Medicaid payments on behalf of the owner or operator of the nursing home or certified nursing facility, (iii) the power to execute and avoid executory contracts, (iv) the power to hire and discharge employees, and (v) the power to do all other acts, including the filing of such reports as the court may direct, subject to accounting to the court therefor and otherwise consistent with state and federal law, necessary to protect the patients from the threat or threats set forth in the original petitions, as well as such other threats arising thereafter or out of the same conditions.

The court may grant injunctive relief as it deems appropriate to the Department or to its receiver either in conjunction with or subsequent to the granting of a petition for appointment of a receiver under this section.

The court may terminate the receivership on the motion of the Department, the receiver, or the owner or operator, upon finding, after a hearing, that either (i) the conditions described in the petition have been substantially eliminated or remedied, or (ii) all patients in the nursing home or certified nursing facility have been relocated. Within thirty days after such termination, the receiver shall file a complete report of his activities with the court, including an accounting for all property of which he has taken possession and all funds collected.

All costs of administration of a receivership hereunder shall be paid by the receiver out of reimbursement to the nursing home or certified nursing facility from Medicare, Medicaid and other patient care collections. The court, after terminating such receivership, shall enter appropriate orders to ensure such payments upon its approval of the receiver's reports.

A receiver appointed under this section shall be an officer of the court, shall not be liable for conditions at the nursing home or certified nursing facility which existed or originated prior to his appointment and shall not be personally liable, except for his own gross negligence and intentional acts which result in injuries to persons or damage to property at the nursing home or certified nursing facility during his receivership.

The provisions of this subsection shall not be construed to relieve any owner, operator or other party of any duty imposed by law or of any civil or criminal liability incurred by reason of any act or omission of such owner, operator, or other party.

(1989, c. 618; 1996, cc. 788, 797.)

[previous](#) | [next](#) | [new search](#) | [table of contents](#) | [home](#)

Virginia Administrative Code

Database updated through June 12, 2008

Part I

General Provisions

12VAC5-481-10. Definitions.

As used in these regulations, these terms have the definitions set forth below.

"A₁" means the maximum activity of special form radioactive material permitted in a Type A package. This value is listed in Table 1 of 12VAC5-481-3770.

"A₂" means the maximum activity of radioactive material, other than special form radioactive material, LSA, and SCO material, permitted in a Type A package. This value is listed in Table 1 of 12VAC5-481-3770.

"Absorbed dose" means the energy imparted by ionizing radiation per unit mass of irradiated material. The units of absorbed dose are the gray (Gy) and the rad.

"Absorbed dose rate" means absorbed dose per unit time, for machines with timers, or dose monitor unit per unit time for linear accelerators.

"Accelerator" means any machine capable of accelerating electrons, protons, deuterons, or other charged particles in a vacuum and of discharging the resultant particulate or other radiation into a medium at energies usually in excess of one MeV. For purposes of this definition, "particle accelerator" is an equivalent term.

"Accelerator-produced material" means any material made radioactive by a particle accelerator.

"Accessible surface" means the external surface of the enclosure or housing of the radiation producing machine as provided by the manufacturer. It also means surface of equipment or of an equipment part that can be easily or accidentally touched by persons without the use of a tool.

"Act" means §§32.1-227 through 32.1-238 of the Code of Virginia.

"Active maintenance" means any significant activity needed during the period of institutional control to maintain a reasonable assurance that the performance objectives

in 12VAC5-481-2490 and 12VAC5-481-2500 are met. Such active maintenance includes ongoing activities such as the pumping and treatment of water from a disposal unit or one-time measures such as replacement of a disposal unit cover. Active maintenance does not include custodial activities such as repair of fencing, repair or replacement of monitoring equipment, revegetation, minor additions to soil cover, minor repair of disposal unit covers, and general disposal site upkeep such as mowing grass.

"Activity" means the rate of disintegration or transformation or decay of radioactive material. The units of activity are the becquerel (Bq) and the curie (Ci).

"Acute" means a single radiation dose or chemical exposure event or multiple radiation dose or chemical exposure events occurring within a short time (24 hours or less).

"Added filtration" means any filtration that is in addition to the inherent filtration.

"Address of use" means the building or buildings that are identified on the license and where radioactive material may be produced, prepared, received, used, or stored.

"Adult" means an individual 18 or more years of age.

"Agency" means the Radiological Health Program of the Virginia Department of Health.

"Agreement state" means any state with which the NRC or the Atomic Energy Commission has entered into an effective agreement under subsection 274b of the Atomic Energy Act of 1954, as amended (73 Stat. 689).

"Airborne radioactive material" means any radioactive material dispersed in the air in the form of dusts, fumes, particulates, mists, vapors, or gases.

"Airborne radioactivity area" means a room, enclosure, or area in which airborne radioactive materials composed wholly or partly of licensed material exist in concentrations:

1. In excess of the derived air concentrations (DACs) specified in 12VAC5-481-3690; or
2. To such a degree that an individual present in the area without respiratory

Virginia Administrative Code

Database updated through June 12, 2008

Part I

General Provisions

12VAC5-481-10. Definitions.

As used in these regulations, these terms have the definitions set forth below.

"A₁" means the maximum activity of special form radioactive material permitted in a Type A package. This value is listed in Table 1 of 12VAC5-481-3770.

"A₂" means the maximum activity of radioactive material, other than special form radioactive material, LSA, and SCO material, permitted in a Type A package. This value is listed in Table 1 of 12VAC5-481-3770.

"Absorbed dose" means the energy imparted by ionizing radiation per unit mass of irradiated material. The units of absorbed dose are the gray (Gy) and the rad.

"Absorbed dose rate" means absorbed dose per unit time, for machines with timers, or dose monitor unit per unit time for linear accelerators.

"Accelerator" means any machine capable of accelerating electrons, protons, deuterons, or other charged particles in a vacuum and of discharging the resultant particulate or other radiation into a medium at energies usually in excess of one MeV. For purposes of this definition, "particle accelerator" is an equivalent term.

"Accelerator-produced material" means any material made radioactive by a particle accelerator.

"Accessible surface" means the external surface of the enclosure or housing of the radiation producing machine as provided by the manufacturer. It also means surface of equipment or of an equipment part that can be easily or accidentally touched by persons without the use of a tool.

"Act" means §§32.1-227 through 32.1-238 of the Code of Virginia.

"Active maintenance" means any significant activity needed during the period of institutional control to maintain a reasonable assurance that the performance objectives

in 12VAC5-481-2490 and 12VAC5-481-2500 are met. Such active maintenance includes ongoing activities such as the pumping and treatment of water from a disposal unit or one-time measures such as replacement of a disposal unit cover. Active maintenance does not include custodial activities such as repair of fencing, repair or replacement of monitoring equipment, revegetation, minor additions to soil cover, minor repair of disposal unit covers, and general disposal site upkeep such as mowing grass.

"Activity" means the rate of disintegration or transformation or decay of radioactive material. The units of activity are the becquerel (Bq) and the curie (Ci).

"Acute" means a single radiation dose or chemical exposure event or multiple radiation dose or chemical exposure events occurring within a short time (24 hours or less).

"Added filtration" means any filtration that is in addition to the inherent filtration.

"Address of use" means the building or buildings that are identified on the license and where radioactive material may be produced, prepared, received, used, or stored.

"Adult" means an individual 18 or more years of age.

"Agency" means the Radiological Health Program of the Virginia Department of Health.

"Agreement state" means any state with which the NRC or the Atomic Energy Commission has entered into an effective agreement under subsection 274b of the Atomic Energy Act of 1954, as amended (73 Stat. 689).

"Airborne radioactive material" means any radioactive material dispersed in the air in the form of dusts, fumes, particulates, mists, vapors, or gases.

"Airborne radioactivity area" means a room, enclosure, or area in which airborne radioactive materials composed wholly or partly of licensed material exist in concentrations:

1. In excess of the derived air concentrations (DACs) specified in 12VAC5-481-3690; or
2. To such a degree that an individual present in the area without respiratory

protective equipment could exceed, during the hours an individual is present in a week, an intake of 0.6% of the annual limit on intake (ALI) or 12 DAC-hours.

"Air kerma (K)" means the kinetic energy released in air by ionizing radiation. Kerma is determined as the quotient of D_e by D_m , where D_e is the sum of the initial kinetic energies of all the charged ionizing particles liberated by uncharged ionizing particles in air of mass D_m . The SI unit of air kerma is joule per kilogram and the special name for the unit of kerma is the gray (Gy).

"Air-purifying respirator" means a respirator with an air-purifying filter, cartridge, or canister that removes specific air contaminants by passing ambient air through the air-purifying element.

"Alert" means events may occur, are in progress, or have occurred that could lead to a release of radioactive material but that the release is not expected to require a response by offsite response organizations to protect persons offsite.

"Aluminum equivalent" means the thickness of type 1100 aluminum alloy affording the same attenuation, under specified conditions, as the material in question. The nominal chemical composition of type 100 aluminum is 99.00% minimum aluminum, 0.12% copper.

"Analytical X-ray equipment" means equipment used for X-ray diffraction or fluorescence analysis.

"Analytical X-ray system" means a group of components utilizing x- or gamma-rays to determine the elemental composition or to examine the microstructure of materials.

"Annual limit on intake" (ALI) means the derived limit for the amount of radioactive material taken into the body of an adult worker by inhalation or ingestion in a year. ALI is the smaller value of intake of a given radionuclide in a year by the reference man that would result in a committed effective dose equivalent of 0.05 Sv (5 rem) or a committed dose equivalent of 0.5 Sv (50 rem) to any individual organ or tissue. ALI values for intake by ingestion and by inhalation of selected radionuclides are given in Tables 1 and 2 in 12VAC5-481-3690.

"Annual refresher safety training" means a review conducted or provided by the

licensee or registrant for its employees on radiation safety aspects of industrial radiography. The review shall include, as a minimum, any results of internal inspections, new procedures or equipment, new or revised regulations, and accidents or errors that have been observed. The review shall also provide opportunities for employees to ask safety questions.

"Annually" means at intervals not to exceed one year.

"ANSI" means the American National Standards Institute.

"Area of use" means a portion of a physical structure that has been set aside for the purpose of producing, preparing, receiving, using, or storing radioactive material.

"Assigned protection factor (APF)" means the expected workplace level of respiratory protection that would be provided by a properly functioning respirator or a class of respirators to properly fitted and trained users. Operationally, the inhaled concentration can be estimated by dividing the ambient airborne concentration by the APF.

"As low as is reasonably achievable" (ALARA) means making every reasonable effort to maintain exposures to radiation as far below the dose limits in these regulations as is practical, consistent with the purpose for which the licensed or registered activity is undertaken, taking into account the state of technology, the economics of improvements in relation to state of technology, the economics of improvements in relation to benefits to the public health and safety, and other societal and socioeconomic considerations, and in relation to utilization of nuclear energy and licensed or registered sources of radiation in the public interest.

"Assembler" means any person engaged in the business of assembling, replacing, or installing one or more components into an X-ray system or subsystem. The term includes the owner of an X-ray system or his or her employee or agent who assembles components into an X-ray system that is subsequently used to provide professional or commercial services.

"Associated equipment" means equipment that is used in conjunction with a radiographic exposure device to make radiographic exposures that drive, guide, or

come in contact with the source.

"Atmosphere-supplying respirator" means a respirator that supplies the respirator user with breathing air from a source independent of the ambient atmosphere, and includes supplied-air respirators (SARs) and self-contained breathing apparatus (SCBA) units.

"Attenuation block" means a block or stack, having dimensions 20 centimeters by 20 centimeters by 3.8 centimeters, of type 1100 aluminum alloy or other materials having equivalent attenuation. The nominal chemical composition of type 100 aluminum is 99.00% minimum aluminum, 0.12% copper.

"Authorized medical physicist" means an individual who:

1. Meets the requirements in 12VAC5-481-1760 and 12VAC5-481-1790; or
2. Is identified as an authorized medical physicist or teletherapy physicist on:
 - a. A specific medical use license issued by the NRC or another agreement state;
 - b. A medical use permit issued by an NRC master material licensee;
 - c. A permit issued by an NRC or another agreement state broad scope medical use licensee; or
 - d. A permit issued by an NRC master material license broad scope medical use permittee.

"Authorized nuclear pharmacist" means a pharmacist who:

1. Meets the requirements in 12VAC5-481-1770 and 12VAC5-481-1790;
2. Is identified as an authorized nuclear pharmacist on:
 - a. A specific license issued by the NRC or another agreement state that authorizes medical use or the practice of nuclear pharmacy;
 - b. A permit issued by an NRC master material licensee that authorizes medical use or the practice of nuclear pharmacy;
 - c. A permit issued by an NRC or another agreement state broad scope medical use licensee that authorizes medical use or the practice of nuclear

pharmacy; or

- d. A permit issued by an NRC master material license broad scope medical use permittee that authorizes medical use or the practice of nuclear pharmacy;
3. Is identified as an authorized nuclear pharmacist by a commercial nuclear pharmacy that has been authorized to identify authorized nuclear pharmacists; or
4. Is designated as an authorized nuclear pharmacist in accordance with 12VAC5-481-440 I 2.

"Authorized user" means a practitioner of the healing arts who:

1. Meets the requirements in 12VAC5-481-1790 and any of the following:
 - a. 12VAC5-481-1910;
 - b. 12VAC5-481-1940;
 - c. 12VAC5-481-1980;
 - d. 12VAC5-481-1990;
 - e. 12VAC5-481-2000;
 - f. 12VAC5-481-2010;
 - g. 12VAC5-481-2030;
 - h. 12VAC5-481-2040; or
2. Is identified as an authorized user on:
 - a. A specific license issued by the NRC or another agreement state that authorizes medical use;
 - b. A permit issued by an NRC master material licensee that authorizes medical use;
 - c. A permit issued by an NRC or another agreement state broad scope medical use licensee that authorizes medical use; or
 - d. A permit issued by an NRC master material license broad scope medical use permittee that authorizes medical use.

"Automatic exposure control (AEC)" means a device that automatically controls one or more technique factors in order to obtain, at a preselected location(s), a required quantity of radiation (includes devices such as phototimers and ion chambers).

"Background radiation" means radiation from cosmic sources, naturally occurring radioactive materials, that have not been technologically enhanced, including radon, except as a decay product of source or special nuclear material, and including global fallout as it exists in the environment from the testing of nuclear explosive devices, or from past nuclear accidents such as Chernobyl that contribute to background radiation and are not under the control of the licensee or registrant. "Background radiation" does not include sources of radiation from radioactive materials regulated by the agency.

"Barrier" (See "Protective barrier").

"Beam axis" means a line from the source through the centers of the X-ray fields.

"Beam-limiting device" means a device that provides a means to restrict the dimensions of the X-ray field.

"Beam monitoring system" means a system designed and installed in the radiation head to detect and measure the radiation present in the useful beam.

"Beam scattering foil" means a thin piece of material (usually metallic) placed in the beam to scatter a beam of electrons in order to provide a more uniform electron distribution in the useful beam.

"Becquerel" (Bq) means the SI unit of activity. One becquerel is equal to one disintegration or transformation per second (dps or tps).

"Beneficial attribute" means, as used in Part XVI (12VAC5-481-3460 et seq.) of this chapter, the radioactivity of the product necessary to the use of the product.

"Beneficial to the product" see "Beneficial attribute."

"Bent beam linear accelerator" means a linear accelerator geometry in which the accelerated electron beam must change direction by passing through a bending magnet.

"Bioassay" means the determination of kinds, quantities or concentrations, and, in

some cases, the locations of radioactive material in the human body, whether by direct measurement, in-vivo counting, or by analysis and evaluation of materials excreted or removed from the human body. For purposes of these regulations, "radiobioassay" is an equivalent term.

"Board" means the State Board of Health.

"Brachytherapy" means a method of radiation therapy in which sealed sources are utilized to deliver a radiation dose at a distance of up to a few centimeters, by surface, intracavitary, or interstitial application.

"Buffer zone" means a portion of the disposal site that is controlled by the licensee and that lies under the disposal units and between the disposal units and the boundary of the site.

"Byproduct material" means:

1. Any radioactive material (except special nuclear material) yielded in, or made radioactive by, exposure to the radiation incident to the process of producing or using special nuclear material;
2. The tailings or wastes produced by the extraction or concentration of uranium or thorium from ore processed primarily for its source material content, including discrete surface wastes resulting from uranium solution extraction processes. Underground ore bodies depleted by these solution extraction operations do not constitute "byproduct material" within this definition;
3. a. Any discrete source of radium-226 that is produced, extracted, or converted after extraction, before, on, or after August 8, 2005, for use for a commercial, medical, or research activity; or
b. Any material that:
 - (1) Has been made radioactive by use of a particle accelerator; and
 - (2) Is produced, extracted, or converted after extraction, before, on, or after August 8, 2005, for use for a commercial, medical, or research activity; and
4. Any discrete source of naturally occurring radioactive material, other than

source material, that:

- a. The NRC, in consultation with the Administrator of the Environmental Protection Agency, the Secretary of Energy, the Secretary of Homeland Security, and the head of any other appropriate federal agency, determines would pose a threat similar to the threat posed by a discrete source of radium-226 to the public health and safety or the common defense and security; and
- b. Before, on, or after August 8, 2005, is extracted or converted after extraction for use in a commercial, medical, or research activity.

"C-arm X-ray system" means an X-ray system in which the image receptor and X-ray tube housing assembly are connected by a common mechanical support system in order to maintain a desired spatial relationship. This system is designed to allow a change in the projection of the beam through the patient without a change in the position of the patient.

"Cabinet radiography" means industrial radiography conducted in an enclosure or cabinet so shielded that every location on the exterior meets the dose limits for individual members of the public as specified in 12VAC5-481-720.

"Cabinet X-ray system" means an X-ray system with the X-ray tube installed in an enclosure independent of existing architectural structures except the floor on which it may be placed. The cabinet X-ray system is intended to contain at least that portion of a material being irradiated, provide radiation attenuation, and exclude personnel from its interior during generation of radiation. Included are all X-ray systems designed primarily for the inspection of carry-on baggage at airline, railroad, and bus terminals, and in similar facilities. An X-ray tube used within a shielded part of a building, or X-ray equipment that may temporarily or occasionally incorporate portable shielding, is not considered a cabinet X-ray system.

"Calendar quarter" means not less than 12 consecutive weeks nor more than 14 consecutive weeks. The first calendar quarter of each year shall begin in January and subsequent calendar quarters shall be so arranged such that no day is included in more

than one calendar quarter and no day in any one year is omitted from inclusion within a calendar quarter. The method observed by the licensee or registrant for determining calendar quarters shall only be changed at the beginning of a year.

"Calibration" means the determination of (i) the response or reading of an instrument relative to a series of known radiation values over the range of the instrument or (ii) the strength of a source of radiation relative to a standard.

"Camera" (See "Radiographic exposure device").

"Carrier" means a person engaged in the transportation of passengers or property by land or water as a common, contract, or private carrier, or by civil aircraft.

"Cephalometric device" means a device intended for the radiographic visualization and measurement of the dimensions of the human head.

"Certifiable cabinet X-ray system" means an existing uncertified X-ray system that has been modified to meet the certification requirements specified in 21 CFR 1020.40.

"Certificate holder" means a person who has been issued a certificate of compliance or other package approval by the NRC.

"Certificate of compliance (CoC)" means the certificate issued by the NRC that approves the design of a package for the transportation of radioactive material.

"Certified cabinet X-ray system" means an X-ray system that has been certified in accordance with 21 CFR 1010.2 as being manufactured and assembled pursuant to the provisions of 21 CFR 1020.40.

"Certified components" means components of X-ray systems that are subject to regulations promulgated under Pub.L. 90-602, the Radiation Control for Health and Safety Act of 1968 of the Food and Drug Administration.

"Certified system" means any X-ray system which has one or more certified component(s).

"Certifying entity" means an independent certifying organization meeting the agency's requirements for documenting applicant's training in topics set forth in 12VAC5-481-1320 or equivalent state or NRC regulations.

"CFR" means Code of Federal Regulations.

"Changeable filters" means any filter, exclusive of inherent filtration, that can be removed from the useful beam through any electronic, mechanical, or physical process.

"Chelating agent" means amine polycarboxylic acids, hydroxycarboxylic acids, gluconic acid, and polycarboxylic acids.

"Class" means a classification scheme for inhaled material according to its rate of clearance from the pulmonary region of the lung. Materials are classified as D, W, or Y, which applies to a range of clearance half-times: for Class D, Days, of less than 10 days; for Class W, Weeks, from 10 to 100 days; and for Class Y, Years, of greater than 100 days. For purposes of these regulations, "lung class" and "inhalation class" are equivalent terms.

"Closed transport vehicle" means a transport vehicle equipped with a securely attached exterior enclosure that during normal transportation restricts the access of unauthorized persons to the cargo space containing the radioactive material. The enclosure may be either temporary or permanent but shall limit access from top, sides, and ends. In the case of packaged materials, it may be of the "see-through" type.

"Coefficient of variation (C)" means the ratio of the standard deviation to the mean value of a set of observations. It is estimated using the following equation:

$$\frac{s}{\bar{x}}$$

where:

s = Standard deviation of the observed values;

\bar{x} = Mean value of observations in sample;

x_i = i_{th} observation in sample;

n = Number of observations in sample.

"Collective dose" means the sum of the individual doses received in a given period of time by a specified population from exposure to a specified source of radiation.

"Collimator" means a device used to limit the size, shape, and direction of the primary radiation beam. For industrial radiography it means a radiation shield that is

placed on the end of the guide tube or directly onto a radiographic exposure device to restrict the size of the radiation beam when the sealed source is cranked into position to make a radiographic exposure.

"Commencement of construction" means any clearing of land, excavation, or other substantial action that would adversely affect the environment of a land disposal facility. The term does not mean disposal site exploration, necessary roads for disposal site exploration, borings to determine foundation conditions, or other preconstruction monitoring or testing to establish background information related to the suitability of the disposal site or the protection of environmental values.

"Committed dose equivalent" ($H_{T,50}$) means the dose equivalent to organs or tissues of reference (T) that will be received from an intake of radioactive material by an individual during the 50-year period following the intake.

"Committed effective dose equivalent" ($H_{E,50}$) is the sum of the products of the weighting factors (w_T) applicable to each of the body organs or tissues that are irradiated and the committed dose equivalent to each of these organs or tissues ($H_{E,50} = \sum (w_T H_{T,50})$).

"Computed tomography" means the production of a tomogram by the acquisition and computer processing of X-ray transmission data.

"Computed tomography dose index" means the integral from $-7T$ to $+7T$ of the dose profile along a line perpendicular to the tomographic plane divided by the product of the nominal tomographic section thickness and the number of tomograms produced in a single scan, that is:

$$\int_{-7T}^{+7T} D(z) dz$$

where:

z = Position along a line perpendicular to the tomographic plane;

$D(z)$ = Dose at position z ;

T = Nominal tomographic section thickness;

n = Number of tomograms produced in a single scan.

This definition assumes that the dose profile is centered around $z = 0$ and that, for a multiple tomogram system, the scan increment between adjacent scans is nT .

"Consignment" means each shipment of a package or groups of packages or load of radioactive material offered by a shipper for transport.

"Consortium" means an association of medical use licensees and a PET radionuclide production facility in the same geographical area that jointly own or share in the operation and maintenance cost of the PET radionuclide production facility that produces PET radionuclides for use in producing radioactive drugs within the consortium for noncommercial distributions among its associated members for medical use. The PET radionuclide production facility within the consortium must be located at an educational institution or a federal facility or a medical facility.

"Constraint" means each shipment of a package or groups of packages or load of radioactive material offered by a shipper for transport.

"Constraint (dose constraint)" means a value above which specified licensee actions are required.

"Contact therapy system" means a therapeutic radiation machine with a short target to skin distance (TSD), usually less than five centimeters.

"Contrast scale" means the change in the linear attenuation coefficient per CTN relative to water, that is:



where:

μ = Linear attenuation coefficient of the material of interest;

μ_w = Linear attenuation coefficient of water;

ρ = of the material of interest;

ρ_w = of water.

"Control (drive) cable" means the cable that is connected to the source assembly and used to drive the source to and from the exposure location.

"Control drive mechanism" means a device that enables the source assembly to be

moved into and out of the exposure device.

"Control panel" means that part of the X-ray control upon which are mounted the switches, knobs, pushbuttons, and other hardware necessary for manually setting the technique factors.

"Control tube" means a protective sheath for guiding the control cable. The control tube connects the control drive mechanism to the radiographic exposure device.

"Controlled area" means an area, outside of a restricted area but inside the site boundary, access to which can be limited by the licensee for any reason.

"Conveyance" means:

1. For transport by public highway or rail any transport vehicle or large freight container;
2. For transport by water any vessel, or any hold, compartment, or defined deck area of a vessel including any transport vehicle on board the vessel; and
3. For transport by any aircraft.

"Cooling curve" means the graphical relationship between heat units stored and cooling time.

"Critical group" means the group of individuals reasonably expected to receive the greatest exposure to residual radioactivity for any applicable set of circumstances.

"Criticality safety index (CSI)" means the dimensionless number (rounded up to the next tenth) assigned to and placed on the label of a fissile material package, to designate the degree of control of accumulation of packages containing fissile material during transportation. Determination of the criticality safety index is described in Part XIII (12VAC5-481-2950 et seq.).

"CS" (See "Contrast scale").

"CT" (See "Computed tomography").

"CT conditions of operation" means all selectable parameters governing the operation of a CT X-ray system including, but not limited to, nominal tomographic section thickness, filtration, and the technique factors as defined in these regulations.

"CTDI" (See "Computed tomography dose index").

"CT gantry" means the tube housing assemblies, beam-limiting devices, detectors, and the supporting structures and frames which hold these components.

"CTN" (See "CT number").

"CT Number" means the number used to represent the X-ray attenuation associated with each elemental area of the CT image.



where:

\square = A constant, a normal value of 1,000 when the Hounsfield scale of CTN is used;

Γ = Linear attenuation coefficient of the material of interest;

Γ_w = Linear attenuation coefficient of water.

"Curie" means a unit of quantity of activity. One curie (Ci) is that quantity of radioactive material that decays at the rate of $3.7E+10$ disintegrations or transformations per second (dps or tps).

"Custodial agency" means an agency of the government designated to act on behalf of the government owner of the disposal site.

"Dead-man switch" means a switch so constructed that a circuit closing contact can be maintained only by continuous pressure on the switch by the operator.

"Declared pregnant woman" means a woman who has voluntarily informed the licensee, in writing, of her pregnancy and the estimated date of conception. The declaration remains in effect until the declared pregnant woman withdraws the declaration in writing or is no longer pregnant.

"Decommission" means to remove a facility or site safely from service and reduce residual radioactivity to a level that permits release of the property for unrestricted use and termination of the license or release of the property under restricted conditions and termination of the license.

"Dedicated check source" means a radioactive source that is used to assure the

constant operation of a radiation detection or measurement device over several months or years. This source may also be used for other purposes.

"Deep dose equivalent" (H_D), which applies to external whole body exposure, means the dose equivalent at a tissue depth of one centimeter (1000 mg/cm^2).

"Demand respirator" means an atmosphere-supplying respirator that admits breathing air to the facepiece only when a negative pressure is created inside the facepiece by inhalation.

"Department of Energy" means the Department of Energy established by Pub. L. 95-91, August 4, 1977, 91 Stat. 565, 42 USC §7101 et seq., to the extent that the Department exercises functions formerly vested in the Atomic Energy Commission, its Chairman, members, officers and components and transferred to the Energy Research and Development Administration and to the Administrator thereof pursuant to sections 104(b), (c) and (d) of the Energy Reorganization Act of 1974 (Pub. L. 93-438, October 11, 1974, 88 Stat. 1233 at 1237, 42 USC §5814, effective January 19, 1975) and retransferred to the Secretary of Energy pursuant to section 301(a) of the Department of Energy Organization Act (Pub. L. 95-91, August 4, 1977, 91 Stat. 565 at 577-578, 42 USC §7151, effective October 1, 1977.)

"Depleted uranium" means the source material uranium in which the isotope uranium-235 is less than 0.711 weight percentage of the total uranium present. Depleted uranium does not include special nuclear material.

"Derived air concentration" (DAC) means the concentration of a given radionuclide in air which, if breathed by the reference man for a working year of 2,000 hours under conditions of light work, results in an intake of one ALI. For purposes of these regulations, the condition of light work is an inhalation rate of 1.2 cubic meters of air per hour for 2,000 hours in a year. DAC values are given in 12VAC5-481-3690.

"Derived air concentration-hour" (DAC-hour) means the product of the concentration of radioactive material in air, expressed as a fraction or multiple of the derived air concentration for each radionuclide, and the time of exposure to that radionuclide, in hours. A licensee or registrant may take 2,000 DAC-hours to represent one ALI,

equivalent to a committed effective dose equivalent of 0.05 Sv (5 rem).

"Detector" (See "Radiation detector").

"Deuterium" means, for the purposes of Part XIII (12VAC5-481-2950 et seq.) deuterium and any deuterium compounds, including heavy water, in which the ratio of deuterium atoms to hydrogen atoms exceeds 1:5000.

"Diagnostic clinical procedures manual" means a collection of written procedures that describes each method (and other instructions and precautions) by which the licensee performs diagnostic clinical procedures, where each diagnostic clinical procedure has been approved by the authorized user and includes the radiopharmaceutical, dosage, and route of administration.

"Diagnostic source assembly" means the tube housing assembly with a beam-limiting device attached.

"Diagnostic X-ray system" means an X-ray system designed for irradiation of any part of the human or animal body for the purpose of diagnosis or visualization.

"Diagnostic X-ray imaging system" means an assemblage of components for the generation, emission and reception of X-rays and the transformation, storage and visual display of the resultant X-ray image.

"Direct scattered radiation" means that scattered radiation that has been deviated in direction only by materials irradiated by the useful beam (See "Scattered radiation").

"Discrete source" means a radionuclide that has been processed so that its concentration within a material has been purposely increased for use for commercial, medical, or research activities.

"Disposable respirator" means a respirator for which maintenance is not intended and that is designed to be discarded after excessive breathing resistance, sorbent exhaustion, physical damage, or end-of-service-life renders it unsuitable for use. Examples of this type of respirator are a disposable half-mask respirator or a disposable escape-only self-contained breathing apparatus (SCBA).

"Disposal" means the isolation of wastes from the biosphere inhabited by man and

his food chains by emplacement in a land disposal facility.

"Disposal site" means that portion of a land disposal facility that is used for disposal of waste. It consists of disposal units and a buffer zone.

"Disposal unit" means a discrete portion of the disposal site into which waste is placed for disposal. For near-surface disposal, the unit is usually a trench.

"Distinguishable from background" means that the detectable concentration of a radionuclide is statistically different from the background concentration of that radionuclide in the vicinity of the site or, in the case of structures, in similar materials using adequate measurement technology, survey, and statistical techniques.

"Dose" is a generic term that means absorbed dose, dose equivalent, effective dose equivalent, committed dose equivalent, committed effective dose equivalent, total organ dose equivalent, or total effective dose equivalent. For purposes of these regulations, "radiation dose" is an equivalent term.

"Dose commitment" means the total radiation dose to a part of the body that will result from retention in the body of radioactive material. For purposes of estimating the dose commitment, it is assumed that from the time of intake the period of exposure to retained material will not exceed 50 years.

"Dose equivalent (H_T)" means the product of the absorbed dose in tissue, quality factor, and all other necessary modifying factors at the location of interest. The units of dose equivalent are the sievert (Sv) and rem.

"Dose limits" means the permissible upper bounds of radiation doses established in accordance with these regulations. For purposes of these regulations, "limits" is an equivalent term.

"Dose monitor unit (DMU)" means a unit response from the beam monitoring system from which the absorbed dose can be calculated.

"Dose profile" means the dose as a function of position along a line.

"Dosimetry processor" means an individual or an organization that processes and evaluates individual monitoring devices in order to determine the radiation dose

delivered to the monitoring devices.

"Doubly encapsulated sealed source" means a sealed source in which the radioactive material is sealed within an inner capsule and that capsule is sealed within an outer capsule.

"Drive cable" (See "Control cable").

"Effective dose equivalent (H_E)" means the sum of the products of the dose equivalent (H_T) to each organ or tissue and the weighting factor (w_T) applicable to each of the body organs or tissues that are irradiated ($H_E = \sum w_T H_T$).

"Elemental area" means the smallest area within a tomogram for which the X-ray attenuation properties of a body are depicted. (See also "Picture element").

"Embryo/fetus" means the developing human organism from conception until the time of birth.

"Energy compensation source (ECS)" means a small sealed source, with an activity not exceeding 3.7 MBq (100 μ Ci), used within a logging tool, or other tool components, to provide a reference standard to maintain the tool's calibration when in use.

"Engineered barrier" means a manmade structure or device that is intended to improve the land disposal facility's ability to meet the performance objectives in these regulations.

"Enriched uranium" (See "Uranium – natural, depleted, enriched").

"Entrance exposure rate" means the exposure free in air per unit time at the point where the center of the useful beam enters the patient.

"Entrance or access point" means any opening through which an individual or extremity of an individual could gain access to radiation areas or to licensed or registered radioactive materials. This includes entry or exit portals of sufficient size to permit human entry, irrespective of their intended use.

"Equipment" (See "X-ray equipment").

"Exclusive use" means the sole use by a single consignor of a conveyance for which all initial, intermediate, and final loading and unloading are carried out in accordance

with the direction of the consignor or consignee. The consignor and the carrier must ensure that any loading or unloading is performed by personnel having radiological training and resources appropriate for safe handling of the consignment. The consignor must issue specific instructions, in writing, for maintenance of exclusive use shipment controls, and include them with the shipping paper information provided to the carrier by the consignor.

"Explosive material" means any chemical compound, mixture, or device that produces a substantial instantaneous release of gas and heat spontaneously or by contact with sparks or flame.

"Exposure" means being exposed to ionizing radiation or to radioactive material.

"Exposure head" means a device that locates the gamma radiography sealed source in the selected working position.

"Exposure rate" means the exposure per unit of time, such as roentgen per minute and milliroentgen per hour.

"External beam radiation therapy" means therapeutic irradiation in which the source of radiation is at a distance from the body.

"External dose" means that portion of the dose equivalent received from any source of radiation outside the body.

"Extremity" means hand, elbow, arm below the elbow, foot, knee, and leg below the knee.

"Facility" means the location, building, vehicle, or complex under one administrative control, at which one or more radiation machines are installed, located and/or used.

"Fail-safe characteristics" mean a design feature that causes beam port shutters to close, or otherwise prevents emergence of the primary beam, upon the failure of a safety or warning device.

"Field emission equipment" means equipment that uses an X-ray tube in which electron emission from the cathode is due solely to the action of an electric field.

"Field-flattening filter" means a filter used to homogenize the absorbed dose rate

over the radiation field.

"Field station" means a facility where radioactive sources may be stored or used and from which equipment is dispatched to temporary jobsites.

"Filter" means material placed in the useful beam to preferentially absorb selected radiations. It also means material placed in the useful beam to change beam quality in therapeutic radiation machines subject to Part XV (12VAC5-481-3380 et seq.) of this chapter.

"Filtering facepiece (dusk mask)" means a negative pressure particulate respirator with a filter as an integral part of the facepiece or with the entire facepiece composed of the filtering medium, not equipped with elastomeric sealing surfaces and adjustable straps.

"Fissile material" means the radionuclides uranium-233, uranium-235, plutonium-239, and plutonium-241, or any combination of these radionuclides. "Fissile material" means the fissile nuclides themselves, not material containing fissile nuclides. Unirradiated natural uranium and depleted uranium and natural uranium or depleted uranium, that has been irradiated in thermal reactors only, are not included in this definition. Certain exclusions from fissile material controls are provided in 10 CFR 71.15.

1. Fissile Class I: A package that may be transported in unlimited numbers and in any arrangement, and that requires no nuclear criticality safety controls during transportation. A transport index is not assigned for purposes of nuclear criticality safety but may be required because of external radiation levels.
2. Fissile Class II: A package that may be transported together with other packages in any arrangement but, for criticality control, in numbers that do not exceed an aggregate transport index of 50. These shipments require no other nuclear criticality safety control during transportation. Individual packages may have a transport index not less than 0.1 and not more than 10.

"Fissile material package" means a fissile material packaging together with its fissile material contents.

"Fit factor" means a quantitative estimate of the fit of a particular respirator to a specific individual, and typically estimates the ratio of the concentration of a substance in ambient air to its concentration inside the respirator when worn.

"Fit test" means the use of a protocol to qualitatively or quantitatively evaluate the fit of a respirator on an individual.

"Fluoroscopic imaging assembly" means a subsystem in which X-ray photons produce a visible image. It includes the image receptor(s) such as the image intensifier and spot-film device, electrical interlocks, if any, and structural material providing linkage between the image receptor and diagnostic source assembly.

"Focal spot (actual)" means the area projected on the anode of the X-ray tube bombarded by the electrons accelerated from the cathode and from which the useful beam originates.

"Former Atomic Energy Commission or NRC licensed facilities" means nuclear reactors, nuclear fuel reprocessing plants, uranium enrichment plants, or critical mass experimental facilities where Atomic Energy Commission or NRC licenses have been terminated.

"Gantry" means that part of a radiation therapy system supporting and allowing movements of the radiation head about a center of rotation.

"Generally applicable environmental radiation standards" means standards issued by the Environmental Protection Agency under the authority of the Atomic Energy Act of 1954, as amended, that impose limits on radiation exposures or levels, or concentrations or quantities of radioactive material, in the general environment outside the boundaries of locations under the control of persons possessing or using radioactive material.

"General environment" means, as used in Part XVI (12VAC5-481-3460 et seq.) of this chapter, the total terrestrial, atmospheric, and aquatic environments outside the site boundary within which any activity, operation, or process authorized by a general or specific license issued under Part XVI, is performed.

"General purpose radiographic X-ray system" means any radiographic X-ray system which, by design, is not limited to radiographic examination of specific anatomical regions.

"Gonad shield" means a protective barrier for the testes or ovaries.

"Gray (Gy)" means the SI unit of absorbed dose. One gray is equal to an absorbed dose of one joule per kilogram (100 rad).

"Guide tube (protection sheath)" means a flexible or rigid tube, or "J" tube, for guiding the source assembly and the attached control cable from the exposure device to the exposure head. The guide tube may also include the connections necessary for attachment to the exposure device and to the exposure head.

"Half-value layer (HVL)" means the thickness of a specified material that attenuates X-radiation or gamma radiation to an extent such that the air kerma rate, exposure rate or absorbed dose rate is reduced to one-half of the value measured without the material at the same point.

"Hands-on experience" means experience in all of those areas considered to be directly involved in the radiography process, and includes taking radiographs, calibration of survey instruments, operational and performance testing of survey instruments and devices, film development, posting of radiation areas, transportation of radiography equipment, posting of records and radiation area surveillance, etc., as applicable. Excessive time spent in only one or two of these areas, such as film development or radiation area surveillance, should not be counted toward the 2,000 hours of hands-on experience required for a radiation safety officer in 12VAC5-481-1310 A 2 or the hands-on experience for a radiographer as required by 12VAC5-481-1320 A.

"Hazardous waste" means those wastes designated as hazardous by the Environmental Protection Agency regulations in 40 CFR Part 261.

"Healing arts" means the art or science or group of arts or sciences dealing with the prevention and cure or alleviation of ailments, diseases or infirmities, and has the same meaning as "medicine" when the latter term is used in its comprehensive sense.

"Healing arts screening" means the testing of human beings using X-ray machines for the detection or evaluation of health indications when such tests are not specifically and individually ordered by a licensed practitioner of the healing arts legally authorized to prescribe such X-ray tests for the purpose of diagnosis or treatment.

"Heat unit" means a unit of energy equal to the product of the peak kilovoltage, milliamperes, and seconds, such as (kVp) times (mA) times (seconds).

"Helmet" means a rigid respiratory inlet covering that also provides head protection against impact and penetration.

"High radiation area" means an area, accessible to individuals, in which radiation levels from radiation sources external to the body could result in an individual receiving a dose equivalent in excess of one mSv (0.1 rem) in one hour at 30 centimeters from any source of radiation or 30 centimeters from any surface that the radiation penetrates.

"Hood" means a respiratory inlet covering that completely covers the head and neck and may also cover portions of the shoulders and torso.

"Human use" means the internal or external administration of radiation or radioactive material to human beings.

"HVL" (See "Half-value layer").

"Hydrogeologic unit" means any soil or rock unit or zone which by virtue of its porosity or permeability, or lack thereof, has a distinct influence on the storage or movement of groundwater.

"Image intensifier" means a device, installed in its housing, that instantaneously converts an X-ray pattern into a corresponding light image of higher intensity.

"Image receptor" means any device, such as a fluorescent screen or radiographic film, that transforms incident X-ray photons either into a visible image or into another form that can be made into a visible image by further transformations.

"Image receptor support" means, for mammographic systems, that part of the system designed to support the image receptor during mammography.

"Inadvertent intruder" means a person who might occupy the disposal site after

closure and engage in normal activities, such as agriculture, dwelling construction, or other pursuits in which an individual might be unknowingly exposed to radiation from the waste.

"Independent certifying organization" means an independent organization that meets the agency's criteria for documenting applicant's training in topics set forth in 12VAC5-481-1320 or equivalent agreement state or NRC regulations.

"Individual" means any human being.

"Individual monitoring" means the assessment of:

1. Dose equivalent (i) by the use of individual monitoring devices or (ii) by the use of survey data; or
2. Committed effective dose equivalent (i) by bioassay or (ii) by determination of the time-weighted air concentrations to which an individual has been exposed, that is, DAC-hours. (See the definition of DAC)

"Individual monitoring devices" means devices designed to be worn by a single individual for the assessment of dose equivalent. For purposes of these regulations, "personnel dosimeter" and "dosimeter" are equivalent terms. Examples of individual monitoring devices are film badges, thermoluminescent dosimeters (TLDs), pocket ionization chambers, optically stimulated luminescence (OSL) dosimeters and personal air sampling devices.

"Industrial radiography" means an examination of the structure of materials by the nondestructive method of utilizing ionizing radiation to make radiographic images.

"Inhalation class" (See "Class").

"Inherent filtration" means the filtration of the useful beam provided by the permanently installed components of the tube housing assembly.

"Injection tool" means a device used for controlled subsurface injection of radioactive tracer material.

"Inspection" means an official examination or observation including, but not limited to, tests, surveys, and monitoring to determine compliance with rules, regulations,

orders, requirements, and conditions of the agency.

"Institutional controls" means: (i) permanent markers placed at a disposal site, (ii) public records and archives, (iii) government ownership and regulations regarding land or resource use, and (iv) other methods of preserving knowledge about the location, design, and contents of a disposal system.

"Instrument traceability" (for ionizing radiation measurements) means the ability to show that an instrument has been calibrated at specified time intervals using a national standard or a transfer standard. If a transfer standard is used, the calibration must be at a laboratory accredited by a program that requires continuing participation in measurement quality assurance with the National Institute of Standards and Technology or other equivalent national or international program.

"Interlock" means a device arranged or connected such that the occurrence of an event or condition is required before a second event or condition can occur or continue to occur.

"Internal dose" means that portion of the dose equivalent received from radioactive material taken into the body.

"Interruption of irradiation" means the stopping of irradiation with the possibility of continuing irradiation without resetting of operating conditions at the control panel.

"Intruder barrier" means a sufficient depth of cover over the waste that inhibits contact with waste and helps to ensure that radiation exposures to an inadvertent intruder will meet the performance objectives set forth in these regulations, or engineered structures that provide equivalent protection to the inadvertent intruder.

"Irradiation" means the exposure of matter to ionizing radiation.

"Irradiator" means a facility that uses radioactive sealed sources for the irradiation of objects or materials and in which radiation dose rates exceeding five grays (500 rads) per hour exist at one meter from the sealed radioactive sources in air or water, as applicable for the irradiator type, but does not include irradiators in which both the sealed source and the area subject to irradiation are contained within a device and are not accessible to personnel.

"Irradiator operator" means an individual who has successfully completed the training and testing described in 12VAC5-481-2830 and is authorized by the terms of the license to operate the irradiator without a supervisor present.

"Irradiator operator supervisor" means an individual who meets the requirements for an irradiator operator and who physically oversees operation of the irradiator by an individual who is currently receiving training and testing described in 12VAC5-481-2830.

"Isocenter" means the center of the sphere through which the useful beam axis passes while the gantry moves through its full range of motions.

"kBq" means kilobecquerels.

"Kilovolt (kV) (kilo electron volt (keV))" means the energy equal to that acquired by a particle with one electron charge in passing through a potential difference of 1,000 volts in a vacuum. Current convention is to use kV for photons and keV for electrons.

"Kilovolts peak" (See "Peak tube potential").

"kV" means kilovolts.

"kVp" (See "Peak tube potential").

"kWs" means kilowatt second.

"Land disposal facility" means the land, buildings, structures and equipment that is intended to be used for the disposal of wastes into the subsurface of the land. For purposes of this chapter, a "geologic repository" as defined in 10 CFR Part 60 or 10 CFR Part 63 is not considered a land disposal facility.

"Lay-barge radiography" means industrial radiography performed on any water vessel used for laying pipe.

"Lead equivalent" means the thickness of the material in question affording the same attenuation, under specified conditions, as lead.

"Leakage radiation" means radiation emanating from the diagnostic source assembly except for:

1. The useful beam; and
2. Radiation produced when the exposure switch or timer is not activated.

"Leakage technique factors" means the technique factors associated with the diagnostic source assembly that are used in measuring leakage radiation. They are defined as follows:

1. For diagnostic source assemblies intended for capacitor energy storage equipment, the maximum-rated peak tube potential and the maximum-rated number of exposures in an hour for operation at the maximum-rated peak tube potential with the quantity of charge per exposure being 10 millicoulombs, i.e., 10 milliamperere seconds, or the minimum obtainable from the unit, whichever is larger;
2. For diagnostic source assemblies intended for field emission equipment rated for pulsed operation, the maximum-rated peak tube potential and the maximum-rated number of X-ray pulses in an hour for operation at the maximum-rated peak tube potential;
3. For all other diagnostic source assemblies, the maximum-rated peak tube potential and the maximum-rated continuous tube current for the maximum-rated peak tube potential.

"Lens dose equivalent (LDE)" applies to the external exposure of the lens of the eye and is taken as the dose equivalent at a tissue depth of 0.3 cm (300 mg/cm^2).

"License" means a license issued by the agency in accordance with the regulations adopted by the board.

"Licensed material" means radioactive material received, possessed, used, transferred or disposed of under a general or specific license issued by the agency.

"Licensee" means any person who is licensed by the agency in accordance with these regulations and the Act.

"Light field" means that area of the intersection of the light beam from the beam-limiting device and one of the set of planes parallel to and including the plane of the image receptor, whose perimeter is the locus of points at which the illumination is one-fourth of the maximum in the intersection.

"Limits" (See "Dose limits").

"Line-voltage regulation" means the difference between the no-load and the load line potentials expressed as a percentage of the load line potential. It is calculated using the following equation:

$$\text{Percent line-voltage regulation} = 100 (V_n - V_l) / V_l$$

where:

V_n = No-load line potential; and

V_l = Load line potential.

"Lixiscope" means a portable light-intensified imaging device using a sealed source.

"Local components" mean part of an analytical X-ray system and include areas that are struck by X-rays such as radiation source housings, port and shutter assemblies, collimators, sample holders, cameras, goniometers, detectors, and shielding, but do not include power supplies, transformers, amplifiers, readout devices, and control panels.

"Logging assistant" means any individual who, under the personal supervision of a logging supervisor, handles sealed sources or tracers that are not in logging tools or shipping containers or who performs surveys required by Part XIV (12VAC5-481-3140 et seq.) of this chapter.

"Logging supervisor" means the individual who uses sources of radiation or provides personal supervision of the utilization of sources of radiation at the well site.

"Logging tool" means a device used subsurface to perform well-logging.

"Loose-fitting facepiece" means a respiratory inlet covering that is designed to form a partial seal with the face.

"Lost or missing licensed material" means licensed (or registered) source of radiation whose location is unknown. This definition includes, but is not limited to, radioactive material that has been shipped but has not reached its planned destination and whose location cannot be readily traced in the transportation system.

"Lot tolerance percent defective" means, expressed in percent defective, the poorest quality in an individual inspection lot that should be accepted.

"Low specific activity (LSA) material" means radioactive material with limited specific activity that is nonfissile or is excepted under 12VAC5-481-2970 C, and that satisfies the descriptions and limits set forth below. Shielding materials surrounding the LSA material may not be considered in determining the estimated average specific activity of the package contents. LSA material must be in one of three groups:

1. LSA-I

- a. Uranium and thorium ores, concentrates of uranium and thorium ores, and other ores containing naturally occurring radioactive radionuclide that are not intended to be processed for the use of these radionuclides;
- b. Solid unirradiated natural uranium or depleted uranium or natural thorium or their solid or liquid compounds or mixtures;
- c. Radioactive material, for which the A_2 value is unlimited; or
- d. Other radioactive material in which the activity is distributed throughout and the estimated average specific activity does not exceed 30 times the value for exempt material activity concentration determined in accordance with 12VAC5-481-3720.

2. LSA-II

- a. Water with tritium concentration up to 0.8 terabecquerel per liter (20.0 Ci/L); or
- b. Other material in which the activity is distributed throughout, and the average specific activity does not exceed $1.0 \text{ E-}04 \text{ A}_2/\text{g}$ for solids and gases, and $1.0 \text{ E-}05 \text{ A}_2/\text{g}$ for liquids.

3. LSA-III

Solids (e.g., consolidated wastes, activated materials), excluding powders, that satisfy the requirements of 10 CFR 71.77) in which:

- a. The radioactive material is distributed throughout a solid or a collection of solid objects, or is essentially uniformly distributed in a solid compact binding agent (for example: concrete, bitumen, or ceramic);

b. The radioactive material is relatively insoluble, or it is intrinsically contained in a relatively insoluble material, so that, even under loss of packaging, the loss of radioactive material per package by leaching, when placed in water for seven days, would not exceed $0.1 A_2$; and

c. The estimated average specific activity of the solid does not exceed $2.0 E-03 A_2/g$.

"Low toxicity alpha emitters" means natural uranium, depleted uranium, natural thorium; uranium-235, uranium-238, thorium-232, thorium-228 or thorium-230 when contained in ores or physical or chemical concentrates or tailings; or alpha emitters with a half-life of less than 10 days.

"Lung class" (See "Class").

"mA" means milliamperere.

"mAs" means milliamperere second.

"Major processor" means a user processing, handling, or manufacturing radioactive material exceeding Type A quantities as unsealed sources or material, or exceeding four times Type B quantities as sealed sources, but does not include nuclear medicine programs, universities, industrial radiographers, or small industrial programs. Type A and B quantities are defined in this section.

"Maximum line current" means the root-mean-square current in the supply line of an X-ray machine operating at its maximum rating.

"Management" means the chief executive officer or that individual's designee.

"MBq" means megabecquerels.

"Medical event" means an event that meets the criteria in 12VAC5-481-2080.

"Medical institution" means an organization in which several medical disciplines are practiced.

"Medical use" means the intentional internal or external administration of radioactive material or the radiation from radioactive material to patients or human research subjects under the supervision of an authorized user.

"Megavolt (MV) (mega electron volt (MeV))" means the energy equal to that acquired by a particle with one electron charge in passing through a potential difference of one million volts in a vacuum. (Note: current convention is to use MV for photons and MeV for electrons.)

"Member of the public" means an individual except when that individual is receiving an occupational dose.

"Mineral logging" means any logging performed for the purpose of mineral exploration other than oil or gas.

"Minor" means an individual less than 18 years of age.

"Mobile nuclear medicine service" means the transportation and medical use of radioactive material.

"Mobile X-ray equipment" (See "X-ray equipment").

"Monitor unit (MU)" (See "Dose monitor unit").

"Monitoring" means the measurement of radiation, radioactive material concentrations, surface area activities or quantities of radioactive material and the use of the results of these measurements to evaluate potential exposures and doses. For purposes of these regulations, "radiation monitoring" and "radiation protection monitoring" are equivalent terms. For Part XI (12VAC5-481-2330 et seq.) of this chapter, it means observing and making measurements to provide data to evaluate the performance and characteristics of the disposal site.

"Moving beam radiation therapy" means radiation therapy with any planned displacement of radiation field or patient relative to each other, or with any planned change of absorbed dose distribution. It includes arc, skip, conformal, intensity modulation and rotational therapy.

"Multiple tomogram system" means a computed tomography X-ray system that obtains X-ray transmission data simultaneously during a single scan to produce more than one tomogram.

"NARM" means any naturally occurring or accelerator-produced radioactive material.

It does not include byproduct, source, or special nuclear material.

"Nationally tracked source" means a sealed source containing a quantity equal to or greater than Category 1 or Category 2 levels of any radioactive material listed in 12VAC5-481-3780. In this context a sealed source is defined as radioactive material that is sealed in a capsule or closely bonded, in a solid form and that is not exempt from regulatory control. It does not mean material encapsulated solely for disposal, or nuclear material contained in any fuel assembly, subassembly, fuel rod, or fuel pellet. Category 1 nationally tracked sources are those containing radioactive material at a quantity equal to or greater than the Category 1 threshold. Category 2 nationally tracked sources are those containing radioactive material at a quantity equal to or greater than the Category 2 threshold but less than the Category 1 threshold.

"Natural radioactivity" means radioactivity of naturally occurring nuclides.

"Natural thorium" means thorium with the naturally occurring distribution of thorium isotopes, which is essentially 100 weight percent thorium-232.

"Natural uranium" (See "Uranium – natural, depleted, enriched").

"Near-surface disposal facility" means a land disposal facility in which waste is disposed of within approximately the upper 30 meters of the earth's surface.

"Negative pressure respirator (tight fitting)" means a respirator in which the air pressure inside the facepiece is negative during inhalation with respect to the ambient air pressure outside the respirator.

"Noise" means the standard deviation of the fluctuations in CTN expressed as a percentage of the attenuation coefficient of water. Its estimate (S_n) is calculated using the following expression:

$$\boxed{\times}$$

where:

μ = Linear attenuation coefficient of the material of interest.

μ_w = Linear attenuation coefficient of water.

S_n = Standard deviation of the CTN of picture elements in a specified area of

the CT image.

"Nominal tomographic section thickness" means the full width at half-maximum of the sensitivity profile taken at the center of the cross-sectional volume over which X-ray transmission data are collected.

"Nonstochastic effect" means a health effect, the severity of which varies with the dose and for which a threshold is believed to exist. Radiation-induced cataract formation is an example of a nonstochastic effect. For purposes of these regulations, "deterministic effect" is an equivalent term.

"NORM" means any naturally occurring radioactive material. It does not include accelerator produced, byproduct, source, or special nuclear material.

"Normal form radioactive material" means radioactive material that has not been demonstrated to qualify as special form radioactive material.

"Normal operating procedures" mean step-by-step instructions necessary to accomplish the analysis. These procedures shall include sample insertion and manipulation, equipment alignment, routine maintenance by the registrant (or licensee), and data recording procedures, which are related to radiation safety.

"Nominal treatment distance" means:

1. For electron irradiation, the distance from the scattering foil, virtual source, or exit window of the electron beam to the entrance surface of the irradiated object along the central axis of the useful beam.
2. For X-ray irradiation, the virtual source or target to isocenter distance along the central axis of the useful beam. For nonisocentric equipment, this distance shall be that specified by the manufacturer.

"Nuclear Regulatory Commission (NRC)" means the NRC or its duly authorized representatives.

"Nuclear waste" means a quantity of source, byproduct or special nuclear material (the definition of nuclear waste in this part is used in the same way as in 49 CFR 173.403) required to be in NRC-approved specification packaging while transported to,

through or across a state boundary to a disposal site, or to a collection point for transport to a disposal site.

"Occupational dose" means the dose received by an individual in the course of employment in which the individual's assigned duties for the licensee or registrant involve exposure to sources of radiation, whether or not the sources of radiation are in the possession of the licensee, registrant, or other person. Occupational dose does not include doses received from background radiation, from any medical administration the individual has received, from exposure to individuals administered radioactive material and released in accordance with 12VAC5-481-1870, from voluntary participation in medical research programs, or as a member of the public.

"Offshore platform radiography" means industrial radiography conducted from a platform over a body of water.

"Offshore waters" means that area of land and water, beyond the Commonwealth of Virginia's jurisdiction, on or above the U.S. Outer Continental Shelf.

"Open-beam configuration" means an analytical X-ray system in which an individual could accidentally place some part of his body in the primary beam path during normal operation.

"Output" means the exposure rate, dose rate, or a quantity related in a known manner to these rates from a teletherapy unit for a specified set of exposure conditions.

"Package" means the packaging together with its radioactive contents as presented for transport.

1. Fissile material package or Type AF package, Type BF package, Type B(U)F package, or Type B(M)F package means a fissile material packaging together with its fissile material contents.

2. Type A package means a Type A packaging together with its radioactive contents. A Type A package is defined and must comply with the DOT regulations in 49 CFR Part 173.

3. Type B package means a Type B packaging together with its radioactive

contents. On approval, a Type B package design is designated by NRC as B(U) unless the package has a maximum normal operating pressure of more than 700 kPa (100 lbs/in²) gauge or a pressure relief device that would allow the release of radioactive material to the environment under the tests specified in 10 CFR 71.73 (hypothetical accident conditions), in which case it will receive a designation B (M). B(U) refers to the need for unilateral approval of international shipments; B (M) refers to the need for multilateral approval of international shipments. There is no distinction made in how packages with these designations may be used in domestic transportation. To determine their distinction for international transportation, see DOT regulations in 49 CFR Part 173. A Type B package approved before September 6, 1983, was designated only as Type B. Limitations on its use are specified in 10 CFR 71.19.

"Packaging" means the assembly of components necessary to ensure compliance with the packaging requirements of these regulations. It may consist of one or more receptacles, absorbent materials, spacing structures, thermal insulation, radiation shielding, and devices for cooling or absorbing mechanical shocks. The vehicle, tie-down system, and auxiliary equipment may be designated as part of the packaging.

"Panoramic dry-source-storage irradiator" means an irradiator in which the irradiations occur in air in areas potentially accessible to personnel and in which the sources are stored in shields made of solid materials. The term includes beam-type dry-source-storage irradiators in which only a narrow beam of radiation is produced for performing irradiations.

"Panoramic irradiator" means an irradiator in which the irradiations are done in air in areas potentially accessible to personnel. The term includes beam-type irradiators.

"Panoramic wet-source-storage irradiator" means an irradiator in which the irradiations occur in air in areas potentially accessible to personnel and in which the sources are stored under water in a storage pool.

"Particle accelerator" (See "Accelerator").

"Patient" means an individual or animal subjected to healing arts examination,

diagnosis, or treatment.

"PBL" (See "Positive beam limitation").

"Peak tube potential" means the maximum value of the potential difference across the X-ray tube during an exposure.

"Periodic quality assurance check" means a procedure that is performed to ensure that a previous calibration continues to be valid.

"Permanent radiographic installation" means an enclosed shielded room, cell, or vault, not located at a temporary jobsite, in which radiography is performed.

"Person" means any individual, corporation, partnership, firm, association, trust, estate, public or private institution, group, department of the Commonwealth other than the Department of Health, political subdivision of the Commonwealth, any other state or political subdivision or department thereof, and any legal successor, representative, agent, or department of the foregoing, but not including federal government agencies.

"Personal supervision" means guidance and instruction by the supervisor who is physically present at the jobsite and watching the performance of the operation in such proximity that contact can be maintained and immediate assistance given as required. In radiography it means guidance and instruction provided to a radiographer trainee by a radiographer instructor who is present at the site, in visual contact with the trainee while the trainee is using sources of radiation, and in such proximity that immediate assistance can be given if required.

"Personnel monitoring equipment" (See "Individual monitoring devices").

"Phantom" means a volume of material behaving in a manner similar to tissue with respect to the attenuation and scattering of radiation. This requires that both the atomic number (Z) and the density of the material be similar to that of tissue.

"Pool irradiator" means any irradiator at which the sources are stored or used in a pool of water including panoramic wet-source-storage irradiators and underwater irradiators.

"Pharmacist" means an individual licensed by this state to compound and dispense

drugs, prescriptions, and poisons.

"Physician" means an individual licensed by this state to prescribe drugs in the practice of medicine.

"Picture element" means an elemental area of a tomogram.

"PID" (See "Position indicating device").

"Pigtail" (See "Source assembly").

"Pill" (See "Sealed source").

"Planned special exposure" means an infrequent exposure to radiation, separate from and in addition to the annual occupational dose limits.

"Portable X-ray equipment" (See "X-ray equipment").

"Position indicating device" means a device on dental X-ray equipment used to indicate the beam position and to establish a definite source-surface (skin) distance. It may or may not incorporate or serve as a beam-limiting device.

"Positive beam limitation" means the automatic or semi-automatic adjustment of an X-ray beam to the size of the selected image receptor, whereby exposures cannot be made without such adjustment.

"Positive emission tomography (PET) radionuclide production facility" means a facility operating a cyclotron or accelerator for the purpose of producing PET radionuclides.

"Positive pressure respirator" means a respirator in which the pressure inside the respiratory inlet covering exceeds the ambient air pressure outside the respirator.

"Powered air-purifying respirator (PAPR)" means an air-purifying respirator that uses a blower to force the ambient air through air-purifying elements to the inlet covering.

"Practical examination" means a demonstration through application of the safety rules and principles in industrial radiography including use of all procedures and equipment to be used by radiographic personnel.

"Practical range of electrons" corresponds to classical electron range where the only remaining contribution to dose is from bremsstrahlung X-rays. A further explanation may

be found in "Clinical Electron Beam Dosimetry: Report of AAPM Radiation Therapy Committee Task Group 25" (Medical Physics 18(1): 73-109, Jan/Feb. 1991) and ICRU Report 35, "Radiation Dosimetry: Electron Beams with Energies Between 1 and 50 MeV", International Commission on Radiation Units and Measurements, September 15, 1984.

"Preceptor" means an individual who provides, directs, or verifies training and experience required for an individual to become an authorized user, an authorized medical physicist, an authorized nuclear pharmacist, or a radiation safety officer.

"Prescribed dosage" means the quantity of radiopharmaceutical activity as documented:

1. In a written directive; or
2. Either in the diagnostic clinical procedures manual or in any appropriate record in accordance with the directions of the authorized user for diagnostic procedures.

"Prescribed dose" means:

1. For gamma stereotactic radiosurgery, the total dose as documented in the written directive; or
2. For teletherapy, the total dose and dose per fraction as documented in the written directive; or
3. For brachytherapy, either the total source strength and exposure time, or the total dose, as documented in the written directive.

"Pressure demand respirator" means a positive pressure atmosphere-supplying respirator that admits breathing air to the facepiece when the positive pressure is reduced inside the facepiece by inhalation.

"Primary beam" means radiation that passes through an aperture of the source housing by a direct path from the X-ray tube or a radioactive source located in the radiation source housing.

"Primary dose monitoring system" means a system that will monitor the useful beam

during irradiation and that will terminate irradiation when a preselected number of dose monitor units have been delivered.

"Primary protective barrier" (See "Protective barrier").

"Principal activities," as used in this chapter, means activities authorized by the license that are essential to achieving the purpose(s) for which the license was issued or amended. Storage during which no licensed material is accessed for use or disposal and activities incidental to decontamination or decommissioning are not principal activities.

"Private inspector" means an individual who meets the requirements set forth in 12VAC5-481-340 and who has demonstrated to the satisfaction of the agency that such individual possesses the knowledge, training and experience to measure ionizing radiation, to evaluate safety techniques, and to advise regarding radiation protection needs.

"Product" means, as used in Part XVI (12VAC5-481-3460 et seq.) of this chapter, something produced, made, manufactured, refined, or benefited.

"Product conveyor system" means a system for moving the product to be irradiated to, from, and within the area where irradiation takes place.

"Projection sheath" (See "Guide tube").

"Projector" (See "Radiographic exposure device").

"Protective apron" means an apron made of radiation-attenuating or absorbing materials used to reduce exposure to radiation.

"Protective barrier" means a barrier of radiation absorbing material(s) used to reduce radiation exposure. The types of protective barriers are as follows:

1. "Primary protective barrier" means the material, excluding filters, placed in the useful beam;
2. "Secondary protective barrier" means the material that attenuates stray radiation.

"Protective glove" means a glove made of radiation absorbing materials used to

reduce radiation exposure.

"Public dose" means the dose received by a member of the public from exposure to sources of radiation released by the licensee or registrant, or to any other source of radiation under the control of the licensee or registrant. Public dose does not include occupational dose, or doses received from background radiation, from any medical administration the individual has received, from exposure to individuals administered radioactive material and released in accordance with 12VAC5-481-1870, or from voluntary participation in medical research programs.

"Pyrophoric material" means any liquid that ignites spontaneously in dry or moist air at or below 130°F (54.4°C) or any solid material, other than one classed as an explosive, which under normal conditions is liable to cause fires through friction, retained heat from manufacturing or processing, or that can be ignited readily and, when ignited, burns so vigorously and persistently as to create a serious transportation, handling, or disposal hazard. Included are spontaneously combustible and water-reactive materials.

"Qualitative fit test (QLFT)" means a pass/fail fit test to assess the adequacy of respirator fit that relies on the individual's response to the test agent.

"Quality factor" (Q) means the modifying factor, that is referenced in 12VAC5-481-240, that is used to derive dose equivalent from absorbed dose.

"Quantitative fit test (QNFT)" means an assessment of the adequacy of respirator fit by numerically measuring the amount of leakage into the respirator.

"Quarter" means a period of time equal to one-fourth of the year observed by the licensee, approximately 13 consecutive weeks, providing that the beginning of the first quarter in a year coincides with the starting date of the year and that no day is omitted or duplicated in consecutive quarters.

"Rad" means the special unit of absorbed dose. One rad is equal to an absorbed dose of 100 erg per gram or 0.01 joule per kilogram (0.01 gray).

"Radiation" means alpha particles, beta particles, gamma rays, X-rays, neutrons, high-speed electrons, high-speed protons, and other particles capable of producing

ions. For purposes of these regulations, ionizing radiation is an equivalent term. Radiation, as used in these regulations, does not include nonionizing radiation, such as radiowaves or microwaves, visible, infrared, or ultraviolet light.

"Radiation area" means any area, accessible to individuals, in which radiation levels could result in an individual receiving a dose equivalent in excess of 0.05 mSv (0.005 rem) in one hour at 30 centimeters from the source of radiation or from any surface that the radiation penetrates.

"Radiation dose" (See "Dose").

"Radiation field" (See "Useful beam").

"Radiation head" means the structure from which the useful beam emerges.

"Radiation machine" means any device capable of producing radiation except those devices with radioactive material as the only source of radiation.

"Radiation room" means a shielded room in which irradiations take place. Underwater irradiators do not have radiation rooms.

"Radiation safety officer (RSO)" means an individual who has the knowledge and responsibility to apply appropriate radiation protection regulations and has been assigned such responsibility by the licensee or registrant.

"Radiation safety officer for industrial radiography" means an individual with the responsibility for the overall radiation safety program on behalf of the licensee or registrant and who meets the requirements of 12VAC5-481-1310.

"Radiation safety officer for medical" means an individual who meets the requirements of 12VAC5-481-1750 and 12VAC5-481-1790 and is identified as an RSO on: a medical use license issued by the agency, NRC or another agreement state, or a medical use permit issued by an NRC masters material licensee.

"Radiation therapy physicist" means an individual qualified in accordance with 12VAC5-481-340.

"Radiation therapy simulation system" means a radiographic or fluoroscopic X-ray system intended for localizing the volume to be exposed during radiation therapy and

confirming the position and size of the therapeutic irradiation field.

"Radioactive material" means any solid, liquid, or gas which emits radiation spontaneously.

"Radioactive marker" means radioactive material placed subsurface or on a structure intended for subsurface use for the purpose of depth determination or direction orientation.

"Radioactivity" means the transformation of unstable atomic nuclei by the emission of radiation.

"Radiobioassay" (See "Bioassay").

"Radiograph" means an image receptor on which the image is created directly or indirectly by an X-ray pattern and results in a permanent record.

"Radiographer" means any individual who performs or who, in attendance at the site where the sources of radiation are being used, personally supervises industrial radiographic operations and who is responsible to the licensee or registrant for assuring compliance with the requirements of the agency's regulations and the conditions of the license or registration.

"Radiographer certification" means written approval received from a certifying entity stating that an individual has satisfactorily met the radiation safety, testing, and experience criteria in 12VAC5-481-1320.

"Radiographer instructor" means any radiographer who has been authorized by the agency to provide on-the-job training to radiographer trainees in accordance with Part V (12VAC5-481-1170 et seq.) of this chapter.

"Radiographer trainee" means any individual who, under the personal supervision of a radiographer instructor, uses sources of radiation, related handling tools, or radiation survey instruments during the course of his instruction.

"Radiographer's assistant" means any individual who under the direct supervision of a radiographer, uses radiographic exposure devices, sources of radiation, related handling tools, or radiation survey instruments in industrial radiography.

"Radiographic exposure device" means any instrument containing a sealed source fastened or contained therein, in which the sealed source or shielding thereof may be moved, or otherwise changed, from a shielded to unshielded position for purposes of making a radiographic exposure.

"Radiographic imaging system" means any system whereby a permanent or semi-permanent image is recorded on an image receptor by the action of ionizing radiation.

"Radiographic operations" means all activities performed with a radiographic exposure device, or with a radiation machine. Activities include using, transporting except by common or contract carriers, or storing at a temporary job site, performing surveys to confirm the adequacy of boundaries, setting up equipment, and any activity inside restricted area boundaries. Transporting a radiation machine is not considered a radiographic operation.

"Radiographic personnel" means any radiographer, radiographer instructor, or radiographer trainee.

"Radiography" (See "Industrial radiography").

"Rating" means the operating limits as specified by the component manufacturer.

"Reasonably maximally exposed individual" means, as used in Part XVI (12VAC5-481-3460 et seq.) of this chapter, a representative of a population who is exposed to TENORM at the maximum TENORM concentration measured in environmental media found at a site along with reasonable maximum case exposure assumptions. The exposure is determined by using maximum values for one or more of the most sensitive parameters affecting exposure, based on cautious but reasonable assumptions, while leaving the others at their mean value.

"Recording" means producing a permanent form of an image resulting from X-ray photons.

"Redundant beam monitoring system" means a combination of two dose monitoring systems in which each system is designed to terminate irradiation in accordance with a preselected number of dose monitor units.

"Reference man" means a hypothetical aggregation of human physical and physiological characteristics determined by international consensus. These characteristics may be used by researchers and public health employees to standardize results of experiments and to relate biological insult to a common base. A description of the reference man is contained in the International Commission on Radiological Protection report, ICRP Publication 23, "Report of the Task Group on Reference Man."

"Reference plane" means a plane that is displaced from and parallel to the tomographic plane.

"Registrant" means any person who is registered with the agency and is legally obligated to register with the agency pursuant to these regulations and the Act.

"Registration" means registration with the agency in accordance with the regulations adopted by the agency.

"Regulations of the United States Department of Transportation" means the regulations in 49 CFR Parts 100-189.

"Rem" means the special unit of any of the quantities expressed as dose equivalent. The dose equivalent in rems is equal to the absorbed dose in rad multiplied by the quality factor (1 rem = 0.01 Sv).

"Research and development" means (i) theoretical analysis, exploration, or experimentation; or (ii) the extension of investigative findings and theories of a scientific or technical nature into practical application for experimental and demonstrative purposes, including the experimental production and testing of models, devices, equipment, materials, and processes. Research and development does not include the internal or external administration of radiation or radioactive material to human beings.

"Residential location" means any area where structures in which people lodge or live are located, and the grounds on which such structures are located including, but not limited to, houses, apartments, condominiums, and garages.

"Residual radioactive material" means (i) waste (that the Secretary of Energy determines to be radioactive) in the form of tailings resulting from the processing of ores

for the extraction of uranium and other valuable constituents of the ores and (ii) other waste (that the Secretary of Energy determines to be radioactive) at a processing site that relates to such processing, including any residual stock of unprocessed ores or low-grade materials. This term is used only with respect to materials at sites subject to remediation under Title I of the Uranium Mill Tailings Radiation Control Act of 1978, as amended.

"Residual radioactivity" means radioactivity in structures, materials, soils, groundwater, and other media at a site resulting from activities under the licensee's control. This includes radioactivity from all licensed and unlicensed sources used by the licensee, but excludes background radiation. It also includes radioactive materials remaining at the site as a result of routine or accidental releases of radioactive materials at the site and previous burials at the site, even if those burials were made in accordance with the provisions of Part IV (12VAC5-481-600 et seq.) of this chapter.

"Respiratory protective device" means an apparatus, such as a respirator, used to reduce an individual's intake of airborne radioactive materials.

"Restricted area" means an area, access to which is limited by the licensee or registrant for the purpose of protecting individuals against undue risks from exposure to radiation and radioactive materials. Restricted area does not include areas used as residential quarters, but separate rooms in a residential building may be set apart as a restricted area.

"Roentgen" means the special unit of exposure. One roentgen (R) equals $2.58E-4$ coulombs per kilogram of air (see "Exposure" and 12VAC5-481-240).

"S-tube" means a tube through which the radioactive source travels when inside a radiographic exposure device.

"Sanitary sewerage" means a system of public sewers for carrying off waste water and refuse, but excluding sewage treatment facilities, septic tanks, and leach fields owned or operated by the licensee or registrant.

"Scan" means the complete process of collecting X-ray transmission data for the production of a tomogram. Data can be collected simultaneously during a single scan

for the production of one or more tomograms.

"Scan increment" means the amount of relative displacement of the patient with respect to the CT X-ray system between successive scans measured along the direction of such displacement.

"Scan sequence" means a preselected set of two or more scans performed consecutively under preselected CT conditions of operation.

"Scan time" means the period of time between the beginning and end of X-ray transmission data accumulation for a single scan.

"Scattered radiation" means ionizing radiation emitted by interaction of ionizing radiation with matter, the interaction being accompanied by a change in direction of the radiation. Scattered primary radiation means that scattered radiation which has been deviated in direction only by materials irradiated by the useful beam.

"Sealed source" means any radioactive material that is encased in a capsule designed to prevent leakage or escape of any radioactive material.

"Sealed Source and Device Registry (SSD)" means the national registry that contains the registration certificates, maintained by the NRC, that summarize the radiation safety information for sealed sources and devices, and describes the licensing and use conditions approved for the product.

"Secondary dose monitoring system" means a system which will terminate irradiation in the event of failure of the primary dose monitoring system.

"Secondary protective barrier" (See "Protective barrier").

"Seismic area" means any area where the probability of a horizontal acceleration in rock of more than 0.3 times the acceleration of gravity in 250 years is greater than 10%, as designated by the United States Geological Survey.

"Self-contained breathing apparatus (SCBA)" means an atmosphere-supplying respirator for which the breathing air source is designed to be carried by the user.

"Shadow tray" means a device attached to the radiation head to support auxiliary beam blocking material.

"Shallow dose equivalent (H_s)," which applies to the external exposure of the skin or an extremity, means the dose equivalent at a tissue depth of 0.007 centimeter (7 mg/cm²).

"Shielded position" means the location within the radiographic exposure device or storage container which, by manufacturer's design, is the proper location for storage of the sealed source.

"Shielded-room radiography" means industrial radiography conducted in a room shielded so that radiation levels at every location on the exterior meet the limitations specified in 12VAC5-481-640.

"Shutter" means a device attached to the tube housing assembly which can intercept the entire cross sectional area of the useful beam and which has a lead equivalency not less than that of the tube housing assembly.

"SI" means the abbreviation for the International System of Units.

"SID" (See "Source-image receptor distance").

"Sievert" (Sv) means the SI unit of any of the quantities expressed as dose equivalent. The dose equivalent in sievert is equal to the absorbed dose in gray multiplied by the quality factor (1 Sv = 100 rem).

"Simulator (radiation therapy simulation system)" means any X-ray system intended for localizing the volume to be exposed during radiation therapy and reproducing the position and size of the therapeutic irradiation field.

"Single tomogram system" means a CT X-ray system that obtains X-ray transmission data during a scan to produce a single tomogram.

"Site area emergency" means events may occur, are in progress, or have occurred that could lead to a significant release of radioactive material and that could require a response by offsite response organizations to protect persons offsite.

"Site boundary" means that line beyond which the land or property is not owned, leased, or otherwise controlled by the licensee.

"Site closure and stabilization" means those actions that are taken upon completion

of operations that prepare the disposal site for custodial care and that assure that the disposal site will remain stable and will not need ongoing active maintenance.

"Source" means the focal spot of the X-ray tube.

"Source assembly" means an assembly that consists of the sealed source and a connector that attaches the source to the control cable. The source assembly may include a ballstop to secure the source in the shielded position.

"Source changer" means a device designed and used for replacement of sealed sources in radiographic exposure devices, including those source changers also used for transporting and storage of sealed sources.

"Source holder" means a housing or assembly into which a radioactive source is placed for the purpose of facilitating the handling and use of the source in well-logging operations.

"Source-image receptor distance" means the distance from the source to the center of the input surface of the image receptor.

"Source material" means:

1. Uranium or thorium, or any combination thereof, in any physical or chemical form; or
2. Ores that contain by weight one-twentieth of 1.0% (0.05%) or more of uranium, thorium or any combination of uranium and thorium. Source material does not include special nuclear material.

"Source of radiation" means any radioactive material or any device or equipment emitting, or capable of producing, radiation.

"Source-skin distance (SSD)" means the distance between the source and the skin entrance plane of the patient.

"Source traceability" means the ability to show that a radioactive source has been calibrated either by the national standards laboratory of the National Institute of Standards and Technology, or by a laboratory that participates in a continuing measurement quality assurance program with National Institute of Standards and

Technology or other equivalent national or international program.

"Special form radioactive material" means radioactive material that satisfies the following conditions:

1. It is either a single solid piece or is contained in a sealed capsule that can be opened only by destroying the capsule;
2. The piece or capsule has at least one dimension not less than five millimeters (0.2 in.); and
3. It satisfies the test requirements specified by the NRC. A special form encapsulation designed in accordance with the NRC requirements in effect on June 30, 1983, and constructed prior to July 1, 1985, may continue to be used. A special form encapsulation either designed or constructed after April 1, 1998, must meet requirements of this definition applicable at the time of its design or construction.

"Special nuclear material" means:

1. Plutonium, uranium-233, uranium enriched in the isotope 233 or in the isotope 235, and any other material the NRC, pursuant to the provisions of section 51 of the Atomic Energy Act of 1954, as amended, determines to be special nuclear material, but does not include source material; or
2. Any material artificially enriched by any of the foregoing but does not include source material.

"Special nuclear material in quantities not sufficient to form a critical mass" means uranium enriched in the isotope U-235 in quantities not exceeding 350 grams of contained U-235; uranium-233 in quantities not exceeding 200 grams; plutonium in quantities not exceeding 200 grams; or any combination of them in accordance with the following formula: For each kind of special nuclear material, determine the ratio between the quantity of that special nuclear material and the quantity specified above for the same kind of special nuclear material. The sum of such ratios for all of the kinds of special nuclear material in combination shall not exceed 1. For example, the following quantities in combination would not exceed the limitation and are within the formula:

"Specific activity" of a radionuclide means the radioactivity of a radionuclide per unit mass of that nuclide. The specific activity of a material in which the radionuclide is essentially uniformly distributed is the radioactivity per unit mass of the material.

"Spot film" means a radiograph that is made during a fluoroscopic examination to permanently record conditions that exist during that fluoroscopic procedure.

"Spot-film device" means a device intended to transport and/or position a radiographic image receptor between the X-ray source and fluoroscopic image receptor. It includes a device intended to hold a cassette over the input end of an image intensifier for the purpose of making a radiograph.

"Stability" means structural stability.

"State inspector" means an employee of the Virginia Department of Health designated to perform those duties or functions assigned the Radiological Health Program.

"Stationary beam radiation therapy" means radiation therapy without displacement of one or more mechanical axes relative to the patient during irradiation.

"Stationary X-ray equipment" (See "X-ray equipment").

"Stochastic effect" means a health effect that occurs randomly and for which the probability of the effect occurring, rather than its severity, is assumed to be a linear function of dose without threshold. Hereditary effects and cancer incidence are examples of stochastic effects. For purposes of these regulations, "probabilistic effect" is an equivalent term.

"Storage" means a condition in which a device or source is not being used for an extended period of time, and has been made inoperable.

"Storage area" means any location, facility, or vehicle that is used to store and secure a radiographic exposure device, a radiation machine, or a storage container when it is not used for radiographic operations. Storage areas are locked or have a physical barrier to prevent accidental exposure, tampering, or unauthorized removal of

the device, machine, or container.

"Storage container" means a device in which sealed sources or radiation machines are secured and stored.

"Stray radiation" means the sum of leakage and scattered radiation.

"Subsurface tracer study" means the release of a substance tagged with radioactive material for the purpose of tracing the movement or position of the tagged substance in the well-bore or adjacent formation.

"Supplied-air respirator (SAR) or airline respirator" means an atmosphere-supplying respirator for which the source of breathing air is not designed to be carried by the user.

"Surface contaminated object" (SCO) means a solid object that is not itself classed as radioactive material, but that has radioactive material distributed on any of its surfaces. An SCO must be in one of two groups with surface activity not exceeding the following limits:

1. SCO-I: A solid object on which:

- a. The nonfixed contamination on the accessible surface averaged over 300 cm², or the area of the surface if less than 300 cm², does not exceed four becquerel per cm² (1 E-04 μCi/cm²) for beta and gamma and low toxicity alpha emitters, or 0.4 becquerel per cm² (1 E-05 μCi/cm²) for all other alpha emitters;
- b. The fixed contamination on the accessible surface averaged over 300 cm², or the area of the surface if less than 300 cm², does not exceed 4 E+04 becquerel per cm² (1.0 μCi/cm²) for beta and gamma and low toxicity alpha emitters, or 4 E+03 becquerel per cm² (0.1 μCi/cm²) for all other alpha emitters; and
- c. The nonfixed contamination plus the fixed contamination on the inaccessible surface averaged over 300 cm², or the area of the surface if less than 300 cm², does not exceed 4 E+04 becquerel per cm² (1 μCi/cm²) for beta and gamma and low toxicity alpha emitters, or 4 E+03 Becquerel per cm² (0.1

$\mu\text{Ci}/\text{cm}^2$) for all other alpha emitters.

2. SCO-II: A solid object on which the limits for SCO-I are exceeded and on which:

a. The nonfixed contamination on the accessible surface averaged over 300 cm^2 , or the area of the surface if less than 300 cm^2 , does not exceed 400 becquerel per cm^2 ($1 \text{ E-}02 \mu\text{Ci}/\text{cm}^2$) for beta and gamma and low toxicity alpha emitters or 40 becquerel per cm^2 ($1 \text{ E-}03 \mu\text{Ci}/\text{cm}^2$) for all other alpha emitters;

b. The fixed contamination on the accessible surface averaged over 300 cm^2 , or the area of the surface if less than 300 cm^2 , does not exceed $8 \text{ E+}05$ becquerel per cm^2 ($20 \mu\text{Ci}/\text{cm}^2$) for beta and gamma and low toxicity alpha emitters, or $8 \text{ E+}04$ becquerel per cm^2 ($2 \mu\text{Ci}/\text{cm}^2$) for all other alpha emitters; and

c. The nonfixed contamination plus the fixed contamination on the inaccessible surface averaged over 300 cm^2 , or the area of the surface if less than 300 cm^2 , does not exceed $8 \text{ E+}05$ becquerel per cm^2 ($20 \mu\text{Ci}/\text{cm}^2$) for beta and gamma and low toxicity alpha emitters, or $8 \text{ E+}04$ becquerel per cm^2 ($2 \mu\text{Ci}/\text{cm}^2$) for all other alpha emitters.

"Surveillance" means monitoring and observation of the disposal site for purposes of visual detection of need for maintenance, custodial care, evidence of intrusion, and compliance with other license and regulatory requirements.

"Survey" means an evaluation of the radiological conditions and potential hazards incident to the production, use, transfer, release, disposal, or presence of radioactive material or other sources of radiation. When appropriate, such an evaluation includes a physical survey of the location of radioactive material and measurements or calculations of levels of radiation, or concentrations or quantities of radioactive material present.

"Target" means that part of an X-ray tube or accelerator onto which a beam of accelerated particles is directed to produce ionizing radiation or other particles.

"Technologically Enhanced Naturally Occurring Radioactive Material (TENORM)"

means, as used in Part XVI (12VAC5-481-3460 et seq.) of this chapter, naturally occurring radionuclides whose concentrations are increased by or as a result of past or present human practices. TENORM does not include background radiation or the natural radioactivity of rocks or soils. TENORM does not include uranium or thorium in "source material" as defined in the AEA and NRC regulations.

"Technique factors" means the following conditions of operation:

1. For capacitor energy storage equipment, peak tube potential in kV and quantity of charge in mAs;
2. For field emission equipment rated for pulsed operation, peak tube potential in kV, and number of X-ray pulses;
3. For CT X-ray systems designed for pulsed operation, peak tube potential in kV, scan time in seconds, and either tube current in Ma, X-ray pulse width in seconds, and the number of X-ray pulses per scan, or the product of tube current, X-ray pulse width, and the number of X-ray pulses in mAs;
4. For CT X-ray systems not designed for pulsed operation, peak tube potential in kV, and either tube current in Ma and scan time in seconds, or the product of tube current and exposure time in mAs and the scan time when the scan time and exposure time are equivalent; and
5. For all other equipment, peak tube potential in kV, and either tube current in Ma and exposure time in seconds, or the product of tube current and exposure time in mAs.

"Teletherapy physicist" means an individual identified as a qualified teletherapy physicist on an agency license.

"Teletherapy" means therapeutic irradiation in which the source of radiation is at a distance from the body.

"Temporary job site" means any location where industrial radiography, wireline service, well-logging, portable gauge or XRF use is performed and where licensed material may be stored other than those location(s) of use authorized on the license.

"Tenth-value layer (TVL)" means the thickness of a specified material that attenuates X-radiation or gamma radiation to an extent such that the air kerma rate, exposure rate, or absorbed dose rate is reduced to one-tenth of the value measured without the material at the same point.

"Termination of irradiation" means the stopping of irradiation in a fashion that will not permit continuance of irradiation without the resetting of operating conditions at the control panel.

"Test" means the process of verifying compliance with an applicable regulation.

"Therapeutic radiation machine" means X-ray or electron-producing equipment designed and used for external beam radiation therapy.

"These regulations" mean all parts of these regulations.

"Tight-fitting facepiece" means a respiratory inlet covering that forms a complete seal with the face.

"Tomogram" means the depiction of the X-ray attenuation properties of a section through the body.

"Tomographic plane" means that geometric plane which is identified as corresponding to the output tomogram.

"Tomographic section" means the volume of an object whose X-ray attenuation properties are imaged in a tomogram.

"Total effective dose equivalent" (TEDE) means the sum of the effective dose equivalent for external exposures and the committed effective dose equivalent for internal exposures.

"Total organ dose equivalent" (TODE) means the sum of the deep dose equivalent and the committed dose equivalent to the organ receiving the highest dose as described in 12VAC5-481-1040.

"Traceable to a National Standard" (See "Instrument traceability" or "Source traceability").

"Transfer" means, as used in Part XVI (12VAC5-481-3460 et seq.) of this chapter,

the physical relocation of NORM containing materials not directly associated with commercial distribution within a business's operation or between general or specific licensees. This term does not include a change in legal title to NORM containing materials that does not involve physical movement of those materials.

"Transport container" means a package that is designed to provide radiation safety and security when sealed sources are transported and which meets all applicable requirements of the United States Department of Transportation.

"Transport index (TI)" means the dimensionless number, rounded up to the next tenth, placed on the label of a package to designate the degree of control to be exercised by the carrier during transportation. The transport index is the number determined by multiplying the maximum radiation level in millisievert (mSv) per hour at one meter (3.3 feet) from the external surface of the package by 100 (equivalent to the maximum radiation level in millirem per hour at one meter (3.3 ft)).

"Treatment site" means the correct anatomical description of the area intended to receive a radiation dose, as described in a written directive.

"Tritium neutron generator target source" means a tritium source used within a neutron generator tube to produce neutrons for use in well-logging applications.

"Tube" means an X-ray tube, unless otherwise specified.

"Tube housing assembly" means the tube housing with tube installed. It includes high-voltage and/or filament transformers and other appropriate elements when such are contained within the tube housing.

"Tube rating chart" means the set of curves which specify the rated limits of operation of the tube in terms of the technique factors.

"Type A quantity" means a quantity of radioactive material, the aggregate radioactivity of which does not exceed A_1 for special form radioactive material or A_2 for normal form radioactive material, where A_1 and A_2 are given in Table A-1 of 12VAC5-481-3770 or may be determined by procedures described in Table A-1 of 12VAC5-481-3770.

"Type B quantity" means a quantity of radioactive material greater than a Type A quantity.

"Underwater irradiator" means an irradiator in which the sources always remain shielded under water and humans do not have access to the sealed sources or the space subject to irradiation without entering the pool.

"Underwater radiography" means radiographic operations performed when the radiographic exposure device or radiation machine and/or related equipment are beneath the surface of the water.

"Unirradiated uranium" means uranium containing not more than 2×10^3 Bq of plutonium per gram of uranium-235, not more than 9×10^6 Bq of fission products per gram of uranium-235, and not more than 5×10^{-3} g of uranium-236 per gram of uranium-235.

"Unrefined and unprocessed ore" means ore in its natural form prior to any processing, such as grinding, roasting, beneficiating, or refining.

"Unrestricted area" means an area, access to which is neither limited nor controlled by the licensee or registrant. For purposes of these regulations, "uncontrolled area" is an equivalent term.

"Uranium—natural, depleted, enriched"

1. "Natural uranium" means uranium with the naturally occurring distribution of uranium isotopes, which is approximately 0.711 weight percent uranium-235, and the remainder by weight essentially uranium-238.
2. "Depleted uranium" means uranium containing less uranium-235 than the naturally occurring distribution of uranium isotopes.
3. "Enriched uranium" means uranium containing more uranium-235 than the naturally occurring distribution of uranium isotopes.

"Uranium sinker bar" means a weight containing depleted uranium used to pull a logging tool down toward the bottom of a well.

"Useful beam" means the radiation emanating from the tube housing port or the

radiation head and passing through the aperture of the beam limiting device when the exposure controls are in a mode to cause the system to produce radiation.

"User seal check (fit check)" means an action conducted by the respirator user to determine if the respirator is properly seated to the face. Examples include negative pressure check, positive pressure check, irritant smoke check, or isoamyl acetate check.

"Variable-aperture beam-limiting device" means a beam-limiting device which has capacity for stepless adjustment of the X-ray field size at a given SID.

"Very high radiation area" means an area, accessible to individuals, in which radiation levels from radiation sources external to the body could result in an individual receiving an absorbed dose in excess of five Gy (500 rad) in one hour at one meter from a source of radiation or one meter from any surface that the radiation penetrates.

"Virtual source" means a point from which radiation appears to originate.

"Visible area" means that portion of the input surface of the image receptor over which incident X-ray photons are producing a visible image.

"Visiting authorized user" means an authorized user who is not identified on the license of the licensee being visited.

"Waste" means those low-level radioactive wastes containing source, special nuclear, or byproduct material that are acceptable for disposal in a land disposal facility. For the purposes of this definition, low-level radioactive waste means radioactive waste not classified as high-level radioactive waste, transuranic waste, spent nuclear fuel, or byproduct material as defined in subdivisions 2, 3, and 4 of the definition of byproduct material.

"Waste handling licensees" mean persons licensed to receive and store radioactive wastes prior to disposal and/or persons licensed to dispose of radioactive waste.

"Wedge filter" means a filter that effects continuous change in transmission over all or a part of the useful beam.

"Week" means seven consecutive days starting on Sunday.

"Weighting factor (w_T)" for an organ or tissue (T) means the proportion of the risk of stochastic effects resulting from irradiation of that organ or tissue to the total risk of stochastic effects when the whole body is irradiated uniformly. For calculating the effective dose equivalent, the values of w_T are:

Organ Dose Weighting Factors	
Organ or Tissue	w_T
Gonads	0.25
Breast	0.15
Red bone marrow	0.12
Lung	0.12
Thyroid	0.03
Bone surfaces	0.03
Remainder	0.30 ^{a/}
Whole Body	1.00 ^{b/}

^{a/}0.30 results from 0.06 for each of five "remainder" organs, excluding the skin and the lens of the eye, that receive the highest doses.

^{b/}For the purpose of weighting the external whole body dose for adding it to the internal dose, a single weighting factor, $w_T = 1.0$, has been specified. The use of other weighting factors for external exposure will be approved on a case-by-case basis until such time as specific guidance is issued.

"Well-bore" means a drilled hole in which wireline service operations or subsurface tracer studies are performed.

"Well-logging" means all operations involving the lowering and raising of measuring devices or tools that may contain sources of radiation into well-bores or cavities for the purpose of obtaining information about the well or adjacent formations.

"Whole body" means, for purposes of external exposure, head, trunk including male gonads, arms above the elbow, or legs above the knee.

"Wireline" means a cable containing one or more electrical conductors that is used to lower and raise logging tools in the well-bore.

"Wireline service operation" means any evaluation or mechanical service that is performed in the well-bore using devices on a wireline.

"Worker" means an individual engaged in work under a license or registration issued by the agency and controlled by a licensee or registrant but does not include the

licensee or registrant.

"Working level (WL)" means any combination of short-lived radon daughters in one liter of air that will result in the ultimate emission of $1.3E+5$ MeV of potential alpha particle energy. The short-lived radon daughters of radon-222 are polonium-218, lead-214, bismuth-214, and polonium-214; and those of radon-220 are polonium-216, lead-212, bismuth-212, and polonium-212.

"Working level month" (WLM) means an exposure to one working level for 170 hours. Two thousand working hours per year divided by 12 months per year is approximately equal to 170 hours per month.

"Written directive" means an order in writing for a specific patient, dated and signed by an authorized user prior to the administration of a radiopharmaceutical or radiation, except as specified in subdivision 6 below, containing the following information:

1. For any administration of quantities greater than 1.11 megabecquerels (30 mCi) of sodium iodide I-125 or I-131: the radionuclide, and dosage; or
2. For a therapeutic administration of a radiopharmaceutical other than sodium iodide I-125 or I-131: the radiopharmaceutical, dosage, and route of administration; or
3. For gamma stereotactic radiosurgery: target coordinates, collimator size, plug pattern, and total dose; or
4. For teletherapy: the total dose, dose per fraction, treatment site, and overall treatment period; or
5. For high-dose-rate remote afterloading brachytherapy: the radionuclide, treatment site, and total dose; or
6. For all other brachytherapy,
 - a. Prior to implantation: the radionuclide, number of sources, and source strengths; and
 - b. After implantation but prior to completion of the procedure: the radionuclide, treatment site, and total source strength and exposure time (or,

equivalently, the total dose).

"X-ray exposure control" means a device, switch, button or other similar means by which an operator initiates and/or terminates the radiation exposure. The X-ray exposure control may include such associated equipment as timers and back-up timers.

"X-ray equipment" means an X-ray system, subsystem, or component thereof.

Types of X-ray equipment are as follows:

1. "Mobile X-ray equipment" means X-ray equipment mounted on a permanent base with wheels and/or casters for moving while completely assembled.
2. "Portable X-ray equipment" means X-ray equipment designed to be hand-carried.
3. "Stationary X-ray equipment" means X-ray equipment that is installed in a fixed location.

"X-ray field" means that area of the intersection of the useful beam and any one of the sets of planes parallel to and including the plane of the image receptor, whose perimeter is the locus of points at which the exposure rate is one-fourth of the maximum in the intersection.

"X-ray high-voltage generator" means a device which transforms electrical energy from the potential supplied by the X-ray control to the tube operating potential. The device may also include means for transforming alternating current to direct current, filament transformers for the X-ray tube(s), high-voltage switches, electrical protective devices, and other appropriate elements.

"X-ray system" means an assemblage of components for the controlled production of X-rays. It includes minimally an X-ray high-voltage generator, an X-ray control, a tube housing assembly, a beam-limiting device, and the necessary supporting structures. Additional components that function with the system are considered integral parts of the system.

"X-ray table" means a patient support device with its patient support structure (tabletop) interposed between the patient and the image receptor during radiography

and/or fluoroscopy. This includes, but is not limited to, any stretcher equipped with a radiolucent panel and any table equipped with a cassette tray (or bucky), cassette tunnel, image intensifier, or spot-film device beneath the tabletop.

"X-ray tube" means any electron tube that is designed for the conversion of electrical energy into X-ray energy.

"Year" means the period of time beginning in January used to determine compliance with the provisions of these regulations. The licensee or registrant may change the starting date of the year used to determine compliance by the licensee or registrant provided that the change is made at the beginning of the year. If a licensee or registrant changes in a year, the licensee or registrant shall assure that no day is omitted or duplicated in consecutive years.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-20. Scope.

Except as otherwise specifically provided, these regulations apply to all persons who receive, possess, use, transfer, own, or acquire any source of radiation; provided, however, that nothing in these regulations shall apply to any person to the extent such person is subject to regulation by the NRC. Attention is directed to the fact that regulation by the state of source material, byproduct material, and special nuclear material in quantities not sufficient to form a critical mass is subject to the provisions of the agreement between the state and the NRC and to 10 CFR Part 150 of the commission's regulations.

To reconcile differences between this chapter and the incorporated sections of federal regulations and to effectuate their joint enforcement, the following words and phrases shall be substituted for the language of the federal regulations:

1. A reference to "NRC" or "Commission" means agency.
2. A reference to "NRC or agreement state" means agency, NRC or another agreement state.
3. The definition of "sealed source" includes NARM.
4. A reference to "byproduct material" includes NARM.
5. Notifications, reports and correspondence referenced in the incorporated parts of 10 CFR shall be directed to the agency and, for NRC licenses, to the NRC until agreement state status is in effect.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-30. Deliberate misconduct.

A. No person may do any of the following:

1. Engage in deliberate misconduct that causes or would have caused, if not detected, a licensee, registrant or applicant under this chapter to be in violation of any rule or order of the agency; or any term, condition or limitation of any license or registration issued by the agency under this chapter.
2. Deliberately submit to the agency, a licensee, registrant or applicant under this chapter; or a contractor or subcontractor of a licensee, registrant or applicant under this chapter; any information that the person knows to be incomplete or inaccurate.

B. Deliberate misconduct by a person means an intentional act or omission that the person knows:

1. Would cause a licensee, certificate of registration holder or applicant to be in violation of any rule, regulation, or order; or any term, condition, or limitation, of any license issued by the agency; or

2. Constitutes a violation of a requirement, procedure, instruction, contract, purchase order, or policy of a licensee; certificate of registration holder, applicant, contractor, or subcontractor.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Reserved, Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-40. (Reserved.)**Statutory Authority**

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-50. (Reserved.)**Statutory Authority**

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-60. (Reserved.)**Statutory Authority**

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-70. (Reserved.)**Statutory Authority**

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-80. (Reserved.)

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-90. Exemptions from regulatory requirements.

A. The agency may, upon application or upon its own initiative, grant such exemptions or exceptions from the requirements of these regulations as it determines are authorized by law and will not result in undue hazard to public health and safety or property.

B. Any Department of Energy contractor or subcontractor and any NRC contractor or subcontractor of the following categories operating within this state is exempt from these regulations to the extent that such contractor or subcontractor under his contract receives, possesses, uses, transfers, or acquires sources of radiation:

1. Prime contractors performing work for the Department of Energy at United States government-owned or controlled sites, including the transportation of sources of radiation to or from such sites and the performance of contract services during temporary interruptions of such transportation;
2. Prime contractors of the Department of Energy performing research in, or development, manufacture, storage, testing, or transportation of, atomic weapons or components thereof;
3. Prime contractors of the Department of Energy using or operating nuclear reactors or other nuclear devices in a United States Government-owned vehicle or vessel; and
4. Any other prime contractor or subcontractor of the Department of Energy or of the NRC when the state and the NRC jointly determine:
 - a. That the exemption of the prime contractor or subcontractor is authorized

by law; and

b. That, under the terms of the contract or subcontract, there is adequate assurance that the work thereunder can be accomplished without undue risk to the public health and safety.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-100. Records.

A. Each licensee and registrant shall maintain records showing the receipt, transfer, and disposal of all sources of radiation as follows:

1. As long as the material is possessed and for three years following transfer or disposition of the radioactive material.
2. Until the agency terminates the license for the licensee who transferred the material.
3. Until the agency terminates the license for the licensee who disposes the material.

B. If radioactive material is combined or mixed with other licensed material and subsequently treated in a manner that makes direct correlation of a receipt record with a transfer, export, or disposition record impossible, the licensee may use evaluative techniques (such as first-in-first-out) to make the records that are required by this section account for 100% of the material received.

C. Additional record requirements are specified elsewhere in these regulations. If the record retention period is not specified, the record shall be maintained for a period of three years.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-110. Inspections and enforcement.

A. Each licensee and registrant shall afford the agency at all reasonable times opportunity to inspect sources of radiation and the premises and facilities wherein such sources of radiation are used or stored.

B. Each licensee and registrant shall make available to the agency for inspection, upon reasonable notice, records maintained pursuant to these regulations.

C. Enforcement.

1. Whenever the department finds, following inspection and examination, that a source of radiation as constructed, operated or maintained results in a violation of this article or of any rules promulgated under this article, the department shall:

a. Notify the person in control of the source of radiation as to the nature of the violation; and

b. Specify a time frame for termination or abatement of the violation, including a deadline by which the source of the violation shall be reconstructed, operated, or maintained in compliance with this article and any regulations promulgated pursuant to this article.

2. Upon failure to comply within the time frame specified by the department for termination or abatement of the violation, the department may revoke the license, and pursue penalties or enforcement in accordance with §32.1-27 of the Code of Virginia.

3. Whenever, in the judgment of the department, any person has engaged in or is about to engage in any acts or practices that constitute or will constitute an emergency, hazard to health and safety, or a violation of any provision of this article, or any rule, regulation or order issued thereunder, and at the request of the commissioner, the Attorney General may make application to the appropriate

court for an order enjoining such acts or practices, or for an order directing compliance, and upon a showing by the department that such person has engaged or is about to engage in any such acts or practices, a permanent or temporary injunction, restraining order, or other order may be granted.

4. In addition to the provisions of §32.1-27 of the Code of Virginia, any person who violates any provisions of this article or any order or regulation adopted pursuant thereto shall, upon such finding by a court of competent jurisdiction, be assessed a civil penalty of not more than \$10,000 for each day of such violation. All penalties under this section shall be recovered in a civil action brought by the Attorney General in the name of the Commonwealth. Civil penalties collected pursuant to this section shall be paid into the state treasury and credited to the Radioactive Material Perpetual Care Trust Fund created pursuant to §32.1-232 of the Code of Virginia.

5. In addition to the provisions of §32.1-25 of the Code of Virginia, the department shall have the power to enter at all reasonable times, or in cases of an emergency, upon any private or public property for the purpose of determining whether or not there is compliance with or violation of the provisions of this article and rules and regulations issued thereunder, except that entry into areas under the jurisdiction of the federal government shall be effected only with the concurrence of the federal government or its duly designated representative.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-120. [Reserved]

12VAC5-481-130. Impounding.

Sources of radiation shall be subject to impounding pursuant to §32.1-238 of the

Code of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-140. Prohibited uses.

A. A hand-held fluoroscopic screen shall not be used with X-ray equipment unless it has been listed in the Registry of Sealed Source and Devices or accepted for certification by the Food and Drug Administration, Center for Devices and Radiological Health.

B. Shoe-fitting fluoroscopic devices shall not be used.

C. No person shall intentionally apply or allow to be applied, either directly or indirectly, radiation to human beings except by, or under the supervision of, a practitioner of the healing arts licensed by this state, except in the case of healing arts screening programs approved in advance by the commissioner. Supervision, as used in this subsection, means the responsibility for and control of quality, radiation safety and technical aspects of the application of radiation to human beings for diagnostic or therapeutic purposes. This prohibition does not apply to persons who are occupationally exposed to radiation or as otherwise provided in these regulations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-150. Communications.

All communications and reports concerning this chapter, and applications filed thereunder, should be addressed to the agency at the following address: Virginia Department of Health, Radioactive Materials Program, 109 Governor Street, Room 730,

Richmond, VA 23219.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-160. Effective date.

The application of these regulations to possess by-product materials, source and special nuclear materials shall not become operative until 30 days after publication in the Virginia Register of a notice of an agreement executed by the Commonwealth of Virginia and the Federal Government under the provisions of Section 274b of the Atomic Energy Act of 1954, as amended (73 Statute 689). All other applications of the provisions of this chapter shall become effective September 20, 2006.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-170. Removal of notices posted by agency prohibited.

Any sign, notice, warning or label affixed by the agency to equipment or facilities of any registrant or licensee shall not be removed, defaced or concealed by any person other than the agency without written permission.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-180. Tests.

Each licensee and registrant shall perform upon instructions from the agency, or

shall permit the agency to perform, such reasonable tests as the agency deems appropriate or necessary including, but not limited to, tests of:

1. Sources of radiation;
2. Facilities wherein sources of radiation are used or stored;
3. Radiation detection and monitoring instruments; and
4. Other equipment and devices used in connection with utilization or storage of licensed or registered sources of radiation.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-190. Additional regulatory requirements.

The agency may, by rule, regulation, or order, impose upon any licensee or registrant such requirements in addition to those established in these regulations as it deems appropriate or necessary to minimize danger to public health and safety or property.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-200. (Repealed.)

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; repealed, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-210. Types of hearings.

Hearings before the board, the commissioner, or their designees shall include any of the following forms depending upon the nature of the controversy and the interests of

the parties involved. All concerned parties will be provided with a reasonable notice of any intent to consider any public data, documents or information in making case decisions.

1. Informal conference. An informal conference is a conference with the commissioner or his designee with concerned parties, in person, with counsel or other representatives held in accordance with §2.2-4019 of the Code of Virginia.

2. Hearing. A hearing is a formal, public proceeding before the commissioner or a designated hearing officer and held in conformance with §2.2-4020 of the Code of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-220. Hearing as a matter of right.

Any licensee or registrant whose licensure, certification or registration has been, or may be affected by any decision of the board or its subordinates in the administration of this chapter shall have a right to both informal and adjudicatory hearings. The commissioner may require participation in an informal hearing before granting the request for a full adjudicatory hearing.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-230. Appeal.

A. Any appeal from a denial of a license or certification must be made in writing and received by the agency within 30 days of the date of receipt of notice of the denial.

B. Any request for hearing on the findings on a Notice of Violation pursuant to this regulation must be made in writing and received within 30 days of receipt of the final

Notice of Violation.

C. Pursuant to the Administrative Process Act (§2.2-4000 et seq. of the Code of Virginia), an aggrieved licensee or registrant may appeal a final decision of the commissioner to an appropriate circuit court.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-240. Units of exposure and dose.

The following regulation, Units of radiation dose (10 CFR 20.1004) is applicable and identical in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-250. Units of radioactivity.

The following regulation, Units of radioactivity (10 CFR 20.1005) is applicable and identical in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part II

Registration of Radiation Machine Facilities and Services

12VAC5-481-260. Purpose and scope.

A. This part provides for the registration of ionizing radiation machine facilities.

B. In addition to the requirements of this part, all registrants are subject to the applicable provisions of Part 1 (12VAC5-481-10 et seq.), Part IV (12VAC5-481-600 et seq.) and Part X (12VAC5-481-2250 et seq.) of this chapter. In addition, some registrants are subject to provisions of the regulations for Part V (12VAC5-481-1170 et seq.), Part VI (12VAC5-481-1580 et seq.), Part VIII (12VAC5-481-2090 et seq.) and Part IX (12VAC5-481-2140 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-270. Exemptions.

A. Electronic equipment that produces radiation incidental to its operation is exempt from the registration and notification requirements of this part, provided that the dose equivalent rate averaged over an area of 10 square centimeters does not exceed 5 μ Sv (0.5 mrem) per hour at five centimeters from any accessible surface of such equipment. The production, testing, or factory servicing of such equipment shall not be exempt.

B. Radiation machines while in transit or storage incident thereto are exempt from the requirements of this part.

C. Domestic television receivers are exempt from the requirements of this part.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-280. Shielding plan review.

A. Prior to construction, the floor plans, shielding specifications and equipment arrangement of all new installations, or modifications of existing installations, utilizing ionizing radiation machines shall be available to the agency for review. The required information is found in 12VAC5-481-280 E.

B. The agency may require the applicant to utilize the services of a private inspector to determine the shielding requirements prior to the plan review.

C. The review of such plans shall not preclude the requirement of additional modifications should a subsequent analysis of operating conditions indicate the possibility of an individual receiving a dose in excess of the limits prescribed in 12VAC5-481-640 and 12VAC5-481-680 through 12VAC5-481-730.

D. After installation of a radiation machine, the registrant shall maintain for inspection by the agency:

1. The maximum rated technique factors of each machine;
2. A scale drawing of the room in which a stationary radiation machine system is located with such drawing indicating the use of areas adjacent to the room and an estimation of the extent of occupancy by an individual in such areas. In addition, the drawing shall include:
 - a. The results of a survey for radiation levels present at the operator's position and at pertinent points outside the room at specified test conditions; or
 - b. The type and thickness of materials, or lead equivalency, of each protective barrier.

E. In order for the private inspector to provide an evaluation, technical advice, and approval on shielding requirements for a radiation installation, the following information shall be required.

1. The plans showing, as a minimum, the following:
 - a. The normal location of the system's radiation port; the port's travel and traverse limits; general direction(s) of the useful beam; locations of any windows and doors or other openings; the location of the operator's booth;

and the location of the control panel;

b. The structural composition and thickness or lead equivalent of all walls, doors, partitions, floor, and ceiling of the room(s) concerned;

c. The dimensions of the room(s) concerned;

d. The type of occupancy of all adjacent areas inclusive of space above and below the room(s) concerned. If there is an exterior wall, show distance to the closest area(s) where it is likely that individuals may be present;

e. The make and model of the equipment, the maximum technique factors, and the energy waveform (single phase, three phase, etc.);

f. The type of examination(s) or treatment(s) that will be performed with the equipment.

2. Information on the anticipated workload of the system(s) in Ma-minutes per week.

3. A report showing all basic assumptions used in the development of the shielding specifications.

F. The following requirements shall be used in the design for an operator's booth:

1. Space requirements:

a. The operator shall be allotted not less than 0.70 square meter (7.5 square feet) of unobstructed floor space in the booth;

b. The operator's booth may be any geometric configuration with no dimension of less than 0.6 m (2 feet);

c. The space shall be allotted excluding any encumbrance by the X-ray control panel, such as overhang, cables, or other similar encroachments;

d. The booth shall be located or constructed such that unattenuated direct scatter radiation originating on the examination table or at the wall-mounted image receptor will not reach the operator's position in the booth.

2. Structural requirements:

a. The booth walls shall be permanently fixed barriers of at least 2 m (7 feet)

high;

b. When a door or movable panel is used as an integral part of the booth structure, it must have an interlock which will prevent an exposure when the door or panel is not closed;

c. Shielding shall be provided to meet the requirements of Part IV (12VAC5-481-600 et seq.) of this chapter.

3. Radiation exposure control placement: The radiation exposure control for the system shall be fixed within the booth and:

a. Shall allow the operator to remain in the protected area and not be exposed to direct scatter, leakage or primary beam radiation;

b. Shall allow the operator to use the majority of the available viewing windows.

4. Viewing system requirements:

a. Each booth shall have at least one viewing device that will:

(1) Be so placed that the operator can view the patient during any exposure; and

(2) Be so placed that the operator can have full view of any occupant of the room and should be so placed that the operator can view any entry into the room. If any door that allows access to the room cannot be seen from the booth, then outside that door there shall be an "X-ray on" warning sign that will be lighted anytime the rotor of the X-ray tube is activated. Alternatively, an interlock shall be present such that exposures are prevented unless the door is closed.

b. When the viewing system is a window, the following requirements also apply:

(1) The window shall have a viewing area of at least 0.09 square meter (1 square foot); Regardless of size or shape, at least 0.09 square meter (1 square foot) of the window area must be centered no less than 0.6 meter (2

feet) from the open edge of the booth and no less than 1.5 meter (5.0 feet) from the floor;

(2) The window shall have at least the same lead equivalence as that required in the booth's wall in which it is mounted.

c. When the viewing system is by mirrors, the mirror(s) shall be so located as to accomplish the general requirements of subdivision 1 of this subsection.

d. When the viewing system is by electronic means:

(1) The camera shall be so located as to accomplish the general requirements of subdivision 1 of this subsection; and

(2) There shall be an alternate viewing system as a backup for the primary system.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-290. Registration of radiation machine facilities.

Each person having a radiation machine facility shall:

1. Apply for registration of such facility with the agency within 30 days following installation of equipment. Application for registration shall be completed on forms furnished by the agency and shall contain all the information required by the form and accompanying instructions. Registrations filed with the agency prior to September 20, 2006, shall remain in effect until a renewal notice is issued by the agency pursuant to 12VAC5-481-310.

2. Designate on the application form an individual to be responsible for radiation protection;

3. Submit to the agency as part of any application for registration or renewal of registration one copy of each radiation survey or calibration report for which records are required to be maintained pursuant to 12VAC5-481-1590 A 12 c.

Records submitted once need not be submitted again for renewal of registration.

4. Have an initial inspection by a private or state inspector no later than 30 days after the registration of the equipment. Subsequent inspections shall be made periodically in accordance with other parts of these regulations or whenever the equipment is moved to a new location. The agency shall furnish a list of private inspectors.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-300. Issuance of registration certificate.

A. Upon a determination that an applicant meets the requirements of this chapter and has paid the appropriate registration fee, the agency shall issue a registration certificate.

B. The agency may incorporate in the registration certificate at the time of issuance or thereafter by appropriate rule, regulation or order, such additional requirements and conditions with respect to the registrant's receipt, possession, use and transfer of radiation machines as he deems appropriate or necessary.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-310. Renewal of registration and approval not implied.

A. Application for renewal of registration shall be filed in accordance with 12VAC5-481-290.

B. In any case in which a registrant not less than 30 days prior to the expiration of his existing registration certificate has filed an application in proper form for renewal, such existing registration certificate shall not expire until the application status has been

finally determined by the agency.

C. No person, in any advertisement, shall refer to the fact that he or his facility is registered with the agency pursuant to the provisions of 12VAC5-481-290, and no person shall state or imply that any activity under such registration has been approved by the agency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-320. Expiration of registration certificate.

Except as provided by 12VAC5-481-310 B, each registration certificate shall expire at the end of the specified day in the month and year stated therein or upon notice issued to the registrant by the agency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-330. Report of changes.

The registrant shall notify the agency in writing before making any change that would render the information contained in the application for registration and/or the notice of registration no longer accurate.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-340. Private inspector qualifications.

Any person desiring designation as a private inspector for diagnostic X-ray,

mammographic or therapeutic X-ray and teletherapy machines must be qualified by training and experience to perform inspections or calibrations according to the following criteria and must submit to the agency a statement on the appropriate form certifying his specific qualifications. In order to maintain designation as a private inspector, the individual must maintain satisfactory performance of work performed in that capacity. The agency shall disqualify individuals from this designation for just cause provided that a show-cause hearing has been held and the agency has determined that the individual has demonstrated unsatisfactory performance as a private inspector.

A. Private inspector, diagnostic X-ray (except mammography). The person must have adequate knowledge, training and experience to measure ionizing radiation, evaluate safety techniques, and advise regarding radiation protection needs to assure compliance with Virginia Rules and Regulations for Ionizing Radiation as evidenced by all of the following:

1. Initial qualifications: evidenced by one or more of the following:

a. Certification by one of the following: American Board of Radiology either in diagnostic or radiological physics, American Board of Health Physics in comprehensive practice, or the American Board of Medical Physics in diagnostic imaging physics.

b. Bachelor's degree in one of the physical sciences or engineering and three years of full-time experience in radiation safety including at least one year in diagnostic X-ray safety. Advanced degrees in related areas may be substituted for experience on an equal time basis, except that no substitution shall be allowed for the required one year of experience in diagnostic X-ray safety.

c. Those individuals listed as private inspectors immediately prior to September 20, 2006, shall be considered grandfathered.

2. Continuing qualifications:

a. Continuing education. Private inspectors must participate in continuing education programs relating to diagnostic X-ray, either by teaching or

completing at least 15 continuing education units (CMEs) every three years.

b. Continuing experience. The private inspector must have inspected at least 10 diagnostic X-ray machines within the preceding 12 months.

3. Reestablishing qualifications. Private inspectors who fail to maintain the required continuing qualifications of this section may not perform the inspections without the supervision of a qualified private inspector. Before independently inspecting another facility, private inspectors must reestablish their qualifications, as follows:

a. Private inspectors who fail to meet the continuing educational requirements of this section shall obtain a sufficient number of continuing education units to bring their total units up to five continuing education units during the preceding 12 months.

b. Private inspectors who fail to meet the continuing experience requirement of this section shall complete a satisfactory inspection of a sufficient number of facilities and machines under the direct supervision of a private inspector who meets the qualifications of this section to bring the number to the required level.

B. Private inspector, therapeutic X-ray and teletherapy machines. The person must have adequate knowledge, training, and experience to calibrate a therapeutic X-ray machine or teletherapy machine, perform inspections and to establish procedures for (and review the results of) spot-check measurements as evidenced by all of the following:

1. Initial qualifications: evidenced by one or more of the following:

a. Be certified by the American Board of Radiology in:

- (1) Therapeutic radiological physics;
- (2) Roentgen-ray and gamma-ray physics;
- (3) X-ray and radium physics;
- (4) Radiological physics;

- b. Be certified by the American Board of Medical Physics in Radiation Oncology Physics;
- c. Be certified by the Canadian College of Medical Physics; or
- d. Hold a master's or doctor's degree in physics, biophysics, radiological physics, or health physics, and have completed one year of full time training in therapeutic radiological physics and also one year of full time work experience under the supervision of a radiation therapy physicist at a medical institution. To meet this requirement, the individual shall have performed the tasks listed in 12VAC5-481-3400 A; 12VAC5-481-3420 P; 12VAC5-481-3430 T; 12VAC5-481-3420 Q; and 12VAC5-481-3430 U under the supervision of a radiation therapy physicist during the year of work experience.

Notwithstanding the provisions of 12VAC5-481-3390 D, certification pursuant to subdivisions B 1 a, b or c of this section shall be required on or before July 1, 2007, for all persons currently qualifying as a radiation therapy physicist pursuant to subdivision B 1 d of this section.

2. Continuing qualifications.

a. Continuing education: Private inspectors must participate in continuing education programs relating to therapeutic X-ray and teletherapy machines, either by teaching or completing at least 15 continuing education units (CEUs) every three years.

b. Continuing experience: The private inspector must have inspected at least one therapeutic X-ray or teletherapy facilities and at least one therapeutic X-ray or teletherapy machine within the preceding 12 months.

3. Reestablishing qualifications. Private inspectors who fail to maintain the required continuing qualifications of this section may not perform an inspection without the supervision of a qualified private inspector. Before independently inspecting another facility, private inspectors must reestablish their qualifications, as follows:

a. Private inspectors who fail to meet the continuing educational requirements of this section shall obtain a sufficient number of continuing education units to bring their total units up to five continuing education units during the preceding 12 months.

b. Private inspectors who fail to meet the continuing experience requirement of this section shall complete a satisfactory inspection of a sufficient number of facilities and machines under the direct supervision of a private inspector who meets the qualifications of this section to bring the number to the required level.

C. Private inspector, mammography. The person must have adequate knowledge, training, and experience to inspect mammography X-ray machines and facilities. All mammography private inspector conducting inspections of mammography facilities and providing oversight of the facility quality assurance program must meet one of the following tracks, either through the initial master's degree of higher route or the alternative initial bachelor's degree route:

1. Initial qualifications:

Master Route:

a. Be certified by the American Board of Radiology (ABR) or the American Board of Medical Physics (ABMP) in:

(1) Diagnostic radiological physics;

(2) Radiological physics; or

(3) Diagnostic imaging physics;

b. A master's degree or higher in a physical science with at least 20 semester hours or equivalent of graduate or undergraduate physics; and

c. Twenty contact hours of mammography facility training; and

d. The experience of conducting inspections of at least one mammography facility and a total of at least 10 mammography units.

Bachelor Route (must have been qualified before April 28, 1999):

- a. A bachelor's degree in a physical science with at least 10 semester hours or equivalent of college level physics;
- b. Forty contact hours of documented specialized training in conducting inspections of mammography facilities; and
- c. The experience of conducting inspections of at least one mammography facility and a total of at least 20 mammography units. The training and experience requirements must be met after fulfilling the degree requirement.

2. Continuing qualifications.

a. Continuing education. At all times after the third anniversary of completion of the initial requirements of this section, the private inspector shall have taught or completed at least 15 continuing education units in mammography during the preceding three years.

b. Continuing experience. At all times after the first anniversary of the completion of the initial requirements of this section, the private inspector shall have inspected at least two mammography facilities and six machines in 24 months.

c. Before a private inspector may begin independently performing mammographic examinations using a new modality, that is, a modality other than one for which the physicist received training to qualify under this section, the inspector must receive at least eight hours of training in inspecting units with the new modality.

3. Reestablishing qualifications. Private inspectors who fail to maintain the required continuing qualifications of this section may not perform the mammography inspections without the supervision of a qualified private inspector. Before independently inspecting another facility, private inspectors must reestablish their qualifications as follows:

- a. Private inspectors who fail to meet the continuing educational requirements of this section shall obtain a sufficient number of continuing education units to

bring their total units up to the required 15 in the previous three years.

b. Private inspectors who fail to meet the continuing experience requirement of this section shall complete a satisfactory inspection of three mammography facilities under the direct supervision of a private inspector who meets the qualifications of this section.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-350. Assembler or transfer obligation.

A. Any person who sells, leases, transfers, lends, disposes, assembles, or installs radiation machines or upon significant service or modification thereof of any radiation machine (such as tube inserts, generators or collimators) in this state shall notify the agency within 15 days of:

1. The name and address of persons who have received these machines;
2. The manufacturer, model, and serial number of each radiation machine transferred; and
3. The date of transfer of each radiation machine.

B. No person shall make, sell, lease, transfer, lend, assemble, or install radiation machines or the supplies used in connection with such machines unless such supplies and equipment when properly placed in operation and used shall meet the requirements of these regulations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-360. Reciprocal recognition of out-of-state radiation machines.

A. Whenever any radiation machine is to be brought into the state, for any temporary use, the person proposing to bring such machine into the state shall give written notice to the agency at least two working days before such machine is to be used in the state.

The notice shall include:

1. The type of radiation machine;
2. The nature, duration, and scope of use;
3. The exact location(s) where the radiation machine is to be used; and
4. States in which this machine is registered.

B. If, for a specific case, the two-working-day period would impose an undue hardship on the person, upon application to the agency, permission to proceed sooner may be granted.

C. The person referred to in subsection A of this section shall:

1. Comply with all applicable regulations of the agency;
2. Supply the agency with such other information as the agency may reasonably request; and
3. Not operate within the state on a temporary basis in excess of 180 calendar days per year.
4. Supply the agency a copy of a medical physicist or private inspector report not less than one year old indicating the equipment is certified by another state.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-370. Certification of X-ray systems.

A. Every owner or operator of an X-ray machine shall:

1. Have the machine certified by the agency within 60 days of the date of installation and thereafter according to the inspection schedule in Part VI

(12VAC5-481-1580 et seq.) of this chapter; and

2. Have the machine inspected whenever the machine is moved to a new location or according to the schedule in Part VI (12VAC5-481-1580 et seq.) of this chapter, whichever occurs first, by a private or state inspector; and

3. Submit to the agency one copy of each inspection or calibration report for which records are required to be maintained pursuant to Part VI (12VAC5-481-1580 et seq.) of this chapter. If the inspection was performed by a state inspector and the inspection was not initiated by the agency pay the appropriate fee as established by the board.

B. Certification may be denied if any noncompliances are not corrected within 45 days from the date of inspection.

C. The agency shall issue a certificate when the data indicates the machine meets the board's standards. A copy of the certificate shall be displayed by the registrant in a conspicuous place in close proximity to the X-ray machine.

D. Certification may be denied if the machine does not meet the standards set forth in these regulations. If the certification is denied, the machine shall not be used for treatment, diagnosis, or evaluation of patients, whether human or animal, until the standards of the board have been met.

E. Final disposition of the machine, including electrical disconnection or storage, will be made within 90 days of agency review.

F. For facilities providing mammography services, the agency may conduct scheduled and random unannounced inspections, to ensure compliance with laws, regulations, or conditions specified by the board.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part III

Licensing of Radioactive Material

Article 1

Purpose and Scope

12VAC5-481-380. Purpose and scope.

A. This part, and Parts V (12VAC5-481-1170 et seq.), VII (12VAC5-481-1660 et seq.), XI (12VAC5-481-2330 et seq.), XIII (12VAC5-481-2950 et seq.), XIV (12VAC5-481-3140 et seq.) and XVI (12VAC5-481-3460 et seq.) of this chapter, provide for the licensing of radioactive material. No person shall receive, possess, use, transfer, own, or acquire radioactive material except as authorized pursuant to this part or Parts V (12VAC5-481-1170 et seq.), VII (12VAC5-481-1660 et seq.), XI (12VAC5-481-2330 et seq.), XII (12VAC5-481-2660 et seq.), XIII (12VAC5-481-2950 et seq.), XIV (12VAC5-481-3140 et seq.) and XVI (12VAC5-481-3460 et seq.) of this chapter, or as otherwise provided in these parts.

B. In addition to the requirements of this part, all licensees are subject to the requirements of Parts I (12VAC5-481-10 et seq.), IV (12VAC5-481-600 et seq.), X (12VAC5-481-2250 et seq.), and XIII (12VAC5-481-2950 et seq.) of this chapter. Furthermore, licensees engaged in industrial radiographic operations are subject to the requirements of Part V (12VAC5-481-1170 et seq.) of this chapter, licensees using radionuclides in the healing arts are subject to the requirements of Part VII (12VAC5-481-1660 et seq.) of this chapter, licensees engaged in irradiator operations are subject to the requirements of Part XII (12VAC5-481-2660 et seq.) of this chapter, and licensees engaged in wireline and subsurface tracer studies are subject to the requirements of Part XIV (12VAC5-481-3140 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 2

Exemptions from the Regulatory Requirements

12VAC5-481-390. Source material.

The following regulations, Carriers (10 CFR 40.12) and Unimportant quantities of source material (10 CFR 40.13) are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-400. Radioactive material other than source material.

A. Exempt concentrations. The following regulation, Exempt concentrations (10 CFR 30.14) is applicable in the Commonwealth of Virginia and include the regulation of natural occurring and accelerator produced radioactive materials (NARM).

B. Exempt quantities. The following regulation, Exempt quantities (10 CFR 30.18) is applicable in the Commonwealth of Virginia and include the regulation of NARM. The exemption stated in paragraph (b) of 10 CFR 30.18 does not apply for radium-226.

C. Exempt items. The following regulation, Certain items containing byproduct material (10 CFR 30.15) is applicable in the Commonwealth of Virginia and include the regulation of NARM. The following item is specifically included: 37 kBq (1 μ Ci) of radium-226 per timepiece in timepieces acquired prior to September 1, 1980.

D. Self-luminous products containing radioactive material. The following regulation, Self-luminous products containing tritium, krypton-85, or promethium-147 (10 CFR 30.19) is applicable in the Commonwealth of Virginia and includes the regulation of NARM. In addition, any person is exempt from these regulations to the extent that such person receives, possesses, uses, transfers, or owns articles containing less than 3.7 kBq (0.1 μ Ci) of radium-226 that were acquired prior to September 1, 1980.

E. Gas and aerosol detectors containing radioactive material.

1. The following regulation, Gas and aerosol detectors containing byproduct material (10CFR 30.20) is applicable in the Commonwealth of Virginia and include the regulation of NARM.

2. Gas and aerosol detectors previously manufactured and distributed to general licensees in accordance with a specific license issued by an agreement state shall be considered exempt under subdivision 1 of this subsection, provided that the device is labeled in accordance with the specific license authorizing distribution of the generally licensed device, and provided further that they meet the requirements of 12VAC5-481-480 C.

3. Gas and aerosol detectors containing NARM previously manufactured and distributed in accordance with a specific license issued by a licensing state shall be considered exempt under subdivision 1 of this subsection, provided that the device is labeled in accordance with the specific license authorizing distribution, and provided further that they meet the requirements of 12VAC5-481-480 C.

F. Resins containing Scandium-46 and designed for sand consolidation in oil wells.

The following regulations, Resins containing Scandium-46 and designed for sand consolidation in oil wells (10 CFR 30.16) is applicable in the Commonwealth of Virginia.

G. Radioactive drug: Capsules containing carbon-14 urea for "in-vivo" diagnostic use for humans. The following regulation, Capsules containing carbon-14 urea for "in-vivo" diagnostic use for humans (10 CFR 30.21) is applicable in the Commonwealth of Virginia.

H. Special nuclear material. The following regulations, Carriers (10 CFR 70.12) and Department of Defense (10 CFR 70.13) are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 3

Licenses

12VAC5-481-410. Types of licenses.

The following regulations, Types of licenses (10 CFR 30.31, 10 CFR 40.20(a) and 10 CFR 70.18) are applicable in the Commonwealth of Virginia, and include the regulation of NARM.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-420. General licenses -- source material.

A. Small quantities of source material. The following regulation, Small quantities of source material (10 CFR 40.22) is applicable in the Commonwealth of Virginia.

B. General license to receive title to source or byproduct material. The following regulation, General license to receive title to source or byproduct material (10 CFR 40.21) is applicable in the Commonwealth of Virginia.

C. Depleted uranium in industrial products and devices. The following regulation, General license for use of certain industrial products or devices (10 CFR 40.25) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-430. General licenses -- radioactive material other than source material.

A. Certain devices and equipment. The following regulations, Certain devices and equipment (10 CFR 31.3) and Terms and Conditions (10 CFR 31.2) are applicable in the Commonwealth of Virginia.

B. Certain detecting, measuring, gauging or controlling devices and certain devices for producing light or an ionized atmosphere. The following regulations, Certain detecting, measuring, gauging, or controlling devices and certain devices for producing light or an ionized atmosphere (10 CFR 31.5) and Terms and Conditions (10 CFR 31.2) are applicable in the Commonwealth of Virginia. In addition, any person who owns, receives, acquires, possesses, uses, or transfers radioactive material in a device pursuant to the general license in this subsection, shall comply with the provisions of 12VAC5-481-1090 and 12VAC5-481-1100 for reporting radiation incidents, theft, or loss of licensed material, but shall be exempt from the other requirements of Parts IV (12VAC5-481-600 et seq.) and X (12VAC5-481-2250 et seq.) of this chapter. The registration required by 10 CFR 31.5(c)(13)(i) shall be made to the agency. A registration invoice will be provided by the agency. The registration fee will be \$50 per device.

C. The general license provided in 12VAC5-481-420 B is subject to the provisions of 12VAC5-481-100 through 12VAC5-481-210, 12VAC5-481-500, 12VAC5-481-570, 12VAC5-481-580 and Part XIII (12VAC5-481-2950 et seq.) of this chapter.

D. Luminous safety devices for use in aircraft. The following regulations, Luminous safety devices for use in aircraft (10 CFR 31.7) and Terms and Conditions (10 CFR 31.2) are applicable in the Commonwealth of Virginia. In addition, this general license is subject to the provisions of 12VAC5-481-100 through 12VAC5-481-210, 12VAC5-481-500, 12VAC5-481-570, 12VAC5-481-580, and Part XIII (12VAC5-481-2950 et seq.) of this chapter.

E. General license to own byproduct material. The following regulations, General license to own byproduct material (10 CFR 31.9), Terms and Conditions (10 CFR 31.2)

and General license to own special nuclear material (10 CFR 70.20) are applicable in the Commonwealth of Virginia and includes NARM.

F. Calibration and reference sources.

1. The following regulations, Americium-241 in the form of calibration or reference sources (10 CFR 31.8), Terms and Conditions (10 CFR 31.2) and General license for calibration or reference sources (10 CFR 70.19) are applicable in the Commonwealth of Virginia and include NARM.

2. A general license is hereby issued to own, receive, possess, use, and transfer plutonium in the form of calibration or reference sources in accordance with the provisions of subdivisions 4 and 5 of this subsection to any person who holds a specific license issued by the agency that authorizes him to receive, possess, use, and transfer radioactive material.

3. A general license is hereby issued to own, receive, possess, use, and transfer radium-226 in the form of calibration or reference sources in accordance with the provisions of subdivisions 4 and 5 of this subsection to any person who holds a specific license issued by the agency which authorizes him to receive, possess, use, and transfer radioactive material.

4. The general licenses in subdivisions 1 through 3 of this subsection apply only to calibration or reference sources that have been manufactured in accordance with the specifications contained in a specific license issued to the manufacturer or importer of the sources by the NRC pursuant to 10 CFR 32.57 or 10 CFR 70.39, or that have been manufactured in accordance with the specifications contained in a specific license issued to the manufacturer by the agency, any agreement state or licensing state pursuant to licensing requirements equivalent to those contained in 10 CFR 32.57 or 10 CFR Part 70.39.

5. The general licenses provided in subdivisions 1 through 3 of this subsection are subject to the provisions of 12VAC5-481-100 through 12VAC5-481-210, 12VAC5-481-500, 12VAC5-481-570, 12VAC5-481-580 and Parts IV (12VAC5-481-600 et seq.); X (12VAC5-481-2250 et seq.); and XIII (12VAC5-481-2950 et

seq.) of this chapter. In addition, persons who own, receive, acquire, possess, use, or transfer one or more calibration or reference sources pursuant to these general licenses:

a. Shall not possess at any one time, at any one location of storage or use, more than 185 kBq (5 μ Ci) of americium-241, 185 kBq (5 μ Ci) of plutonium, or 185 kBq (5 μ Ci) of radium-226 in such sources;

b. Shall not receive, possess, use, or transfer such source unless the source, or the storage container, bears a label that includes one of the following statements, as appropriate, or a substantially similar statement that contains the information called for in one of the following statements, as appropriate:

(1) The receipt, possession, use and transfer of this source,

 Model _____, Serial No. _____, are subject to a general license and the regulations of the Nuclear Regulatory Commission or of a state with which the Nuclear Regulatory Commission has entered into an agreement for the exercise of regulatory authority. Do not remove this label.

CAUTION—RADIOACTIVE MATERIAL

THIS SOURCE CONTAINS (AMERICIUM-241).

(PLUTONIUM) (Showing only the name of the appropriate material.)

DO NOT TOUCH RADIOACTIVE PORTION OF THIS SOURCE.

_____ Name of manufacturer or importer

(2) The receipt, possession, use and transfer of this source, Model _____, Serial No. _____, are subject to a general license and the regulations of a licensing state. Do not remove this label.

CAUTION—RADIOACTIVE MATERIAL

THIS SOURCE CONTAINS RADIUM-226.

DO NOT TOUCH RADIOACTIVE PORTION OF THIS SOURCE.

_____ Name of manufacturer or importer

c. Shall not transfer, abandon, or dispose of such source except by transfer to a person authorized by a license from the agency, the NRC, or another agreement state to receive the source;

d. Shall store such source, except when the source is being used, in a closed container adequately designed and constructed to contain americium-241, plutonium, or radium-226 that might otherwise escape during storage; and

e. Shall not use such source for any purpose other than the calibration of radiation detectors or the standardization of other sources.

6. These general licenses do not authorize the manufacture of calibration or reference sources containing americium-241, plutonium, or radium-226.

G. General license for use of radioactive material for certain in vitro clinical or laboratory testing.

The following regulations, General license for use of byproduct material for certain in vitro clinical or laboratory testing (10 CFR 31.11) and Terms and Conditions (10 CFR 31.2) are applicable in the Commonwealth of Virginia and include NARM.

H. Ice detection devices. The following regulations, General license for use strontium-90 in ice detection devices (10 CFR 31.10) and Terms and Conditions (10 CFR 31.2) are applicable in the Commonwealth of Virginia.

I. Certain items and self-luminous products containing radium-226. The following regulations, General license for certain items and self-luminous products containing radium-226 (10 CFR 31.12) and Terms and Conditions (10 CFR 31.2) are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Specific Licenses

12VAC5-481-440. Filing application for specific licenses.

A. Applications for specific licenses shall be filed on a form prescribed by the agency.

B. The agency may at any time after the filing of the original application, and before the expiration of the license, require further statements in order to enable the agency to determine whether the application should be granted or denied or whether a license should be modified or revoked.

C. Each application shall be signed by the applicant or licensee or a person duly authorized to act for and on his behalf.

D. An application for a license may include a request for a license authorizing one or more activities.

E. Applications and documents submitted to the agency may be made available for public inspection in accordance with the Virginia Freedom of Information Act (§2.2-3700 et seq. of the Code of Virginia). The agency may withhold records in accordance with specific exemptions in the Virginia Freedom of Information Act or as otherwise specified by law.

F. An application for a specific license to use radioactive material in the form of a sealed source or in a device that contains the sealed source must either:

1. Identify the source or device by manufacturer and model number as registered with the NRC under 10 CFR 32.210 or an agreement state under equivalent regulations;
2. Contain the information in 10 CFR 32.210(c); or
3. For sources or devices containing NARM manufactured prior to November 30, 2007, that are not registered with the NRC under 10 CFR 32.210 or with an agreement state, and for which the applicant is unable to provide all categories of information specified in 10 CFR 32.210(c), the applicant must provide:
 - a. All available information identified in 10 CFR 32.210(c) concerning the

source, and, if applicable, the device; and

b. Sufficient additional information to demonstrate that there is reasonable assurance that the radiation safety properties of the source or device are adequate to protect health and minimize danger to life and property. Such information must include a description of the source or device, a description of radiation safety features, the intended use and associated operating experience, and the results of a recent leak test.

G. Each application to possess radioactive material in unsealed form, on a foil or plated source, or sealed in glass in excess of the quantities in 12VAC5-481-3740 shall contain one of the following:

1. An evaluation showing that the projected dose to a person offsite due to a release of radioactive material would not exceed 0.01 Sv (1 rem) total effective dose equivalent or 0.05 Sv (5 rem) to the thyroid; or

2. An emergency plan, reviewed and commented on by offsite response organizations expected to respond in the event of an accident that contains the following information:

a. Facility description. A brief description of the licensee or applicant's facility and surroundings.

b. Types of accidents. An identification of each type of radioactive materials accident for which actions by licensee staff or offsite response organizations will be needed to protect members of the public.

c. Classification of accidents. A method for classifying and declaring an accident as alert or site area emergency.

d. Detection of accidents. Identification of the means for detecting each type of alert or site area emergency in a timely manner.

e. Mitigation of consequences. A brief description of the means and equipment that are available for mitigating the consequences of each type of accident, including those provided to protect workers onsite, and a description of the

program for maintaining the equipment.

f. Assessment of releases. A brief description of the methods and equipment available to assess releases of radioactive material.

g. Responsibilities. A brief description of the responsibilities of the licensee or applicant's personnel who will respond if an accident occurs, including identification of personnel responsible for promptly notifying offsite response organizations, including the agency.

h. Plan maintenance. A brief description of the positions assigned and methods to develop, maintain and update the plan.

i. A list of offsite response organizations, description of their responsibilities and anticipated actions, and copy of formal commitments, if any.

j. Notification and coordination. A brief description of the means to promptly notify the offsite response organizations and request offsite assistance including medical assistance for the treatment of contaminated injured onsite workers. The notification and coordination must include alternate provisions in case key personnel, parts of the facility, or some equipment are unavailable. The licensee shall also commit to notify the agency immediately after notification of the appropriate offsite response organizations and not later than one hour after the licensee declares an emergency.

k. Information to be communicated. A brief description of the types of information on facility status, radioactive releases and recommended protective actions, if necessary, to be given to offsite response organizations and the agency. A licensee shall allow the offsite response organizations expected to respond in case of an accident 60 days to comment on the licensee's emergency plan before submitting it to the agency. A licensee shall provide any comments received within the 60 days to the agency with the emergency plan.

l. Training. A brief description of the frequency, performance objectives and plan for training that the licensee or applicant will provide workers on how to respond to an emergency, including any special instructions and orientation tours that the

licensee or applicant will offer to fire, police, medical and other emergency personnel. The training shall familiarize personnel with site-specific hazards and emergency procedures. The training shall also prepare site personnel for their responsibilities in the event of accident scenarios postulated as most probable for the specific site, including the use of drills, exercises and team training for such scenarios.

m. Drills and exercises. Provisions for conducting quarterly communications checks with offsite response organizations and biennial onsite exercises to test response to simulated emergencies. The licensee or applicant shall invite offsite response organizations to participate in biennial exercises. The exercises shall use accident scenarios postulated as the most probable for the specific site and the scenarios may not be known to most exercise participants. Critiques of exercises must evaluate the appropriateness of the plan, emergency procedures, facilities, equipment, training of personnel and overall effectiveness of the response. Deficiencies found by the critiques must be corrected.

n. Safe condition. A brief description of the means of restoring the facility and surroundings to a safe condition after an accident.

o. Hazardous chemicals. A certification that the applicant has met its responsibilities under the Emergency Planning and Community Right-To-Know Act of 1986, Title III, P.L. 99-499, if applicable to the applicant's activities at the proposed place of use of the radioactive material.

H. An application from a medical facility or educational institution to produce PET radioactive drugs for noncommercial transfer to licensees in its consortium authorized for medical use under Part VII (12VAC5-481-1660 et seq.) of this chapter shall include:

1. A request for authorization for the production of PET radionuclides or evidence of an existing license issued under Part III (12VAC5-481-380 et seq.) of this chapter for a PET radionuclide production facility within its consortium from which it receives PET radionuclides.

2. Evidence that the applicant is qualified to produce radioactive drugs for

medical use by meeting one of the criteria in 12VAC5-481-480 I.

3. Identification of individual(s) authorized to prepare the PET radioactive drugs if the applicant is a pharmacy, and documentation that each individual meets the requirements of an ANP as specified in 12VAC5-481-480 I 2.

4. Information identified in 12VAC5-481-480 I 1 c on the PET drugs to be noncommercially transferred to members of its consortium.

I. Manufacture, preparation, or transfer for commercial distribution of drugs containing radioactive material for medical use under Part VII (12VAC5-481-1660 et seq.).

1. An application for a specific license to manufacture, prepare, or transfer for commercial distribution drugs containing radioactive material for use by persons authorized pursuant to Part VII (12VAC5-481-1660 et seq.) will be approved if:

a. The applicant satisfies the general requirements specified in 12VAC5-481-450;

b. The applicant submits evidence that the applicant is at least one of the following:

(1) Registered or licensed with the U.S. Food and Drug Administration (FDA) as a drug manufacturer;

(2) Registered or licensed with a state agency as a drug manufacturer;

(3) Licensed as a pharmacy by the Virginia Board of Pharmacy;

(4) Operating as a nuclear pharmacy within a federal medical institution; or

(5) A PET drug production facility registered with a state agency.

c. The applicant submits information on the radionuclide; the chemical and physical form; the maximum activity per vial, syringe, generator, or other container of the radioactive drug; and the shielding provided by the packaging to show it is appropriate for the safe handling and storage of the radioactive drugs by medical use licensees; and

d. The applicant satisfies the following labeling requirements:

(1) A label is affixed to each transport radiation shield, whether it is constructed of lead, glass, plastic, or other material, of a radioactive drug to be transferred for commercial distribution. The label must include the radiation symbol and the words "CAUTION, RADIOACTIVE MATERIAL" or "DANGER, RADIOACTIVE MATERIAL"; the name of the radioactive drug or its abbreviation; and the quantity of radioactivity at a specified date and time. For radioactive drugs with a half life greater than 100 days, the time may be omitted.

(2) A label is affixed to each syringe, vial, or other container used to hold a radioactive drug to be transferred for commercial distribution. The label must include the radiation symbol and the words "CAUTION, RADIOACTIVE MATERIAL" or "DANGER, RADIOACTIVE MATERIAL" and an identifier that ensures that the syringe, vial, or other container can be correlated with the information on the transport radiation shield label.

2. A licensee authorized to manufacture, prepare or transfer for commercial distribution radioactive drugs shall ensure that any individual preparing the drugs is one of the following:

- a. An authorized nuclear pharmacist (ANP) as defined in 12VAC5-481-10;
- b. An individual that meets the requirements specified in 12VAC5-481-1770 and 12VAC5-481-1790, and the licensee has received an approved license amendment identifying this individual as an ANP;

c. A pharmacist, as defined in 12VAC5-481-10, designated as an ANP if:

(1) The individual was a nuclear pharmacist preparing only radioactive drugs containing accelerator-produced radioactive material; and

(2) The individual practiced at a pharmacy at a government agency or federally recognized Indian Tribe before November 30, 2007, or at all other pharmacies before August 8, 2009, or an earlier date as noticed by the NRC;

or

- d. An individual under the supervision of an ANP as specified in 12VAC5-481-1710.
3. Shall provide to the agency no later than 30 days after the date that the licensee allows, under subdivision 2 a or c of this subsection, the individual to work as an ANP:
 - a. The individual's certification by a specialty board whose certification process has been recognized by the NRC with the written attestation signed by a preceptor as required by 12VAC5-481-1770;
 - b. An NRC or another agreement state license;
 - c. NRC master materials licensee permit;
 - d. The permit issued by a licensee or NRC master materials permittee of broad scope or the authorization from a commercial nuclear pharmacy authorized to list its own authorized nuclear pharmacist; or
 - e. Documentation that only accelerator-produced radioactive materials were used in the practice of nuclear pharmacy at a government agency or federally recognized Indian Tribe before November 30, 2007, or at all other locations of use before August 8, 2009, or an earlier date as noticed by the NRC; and
 - f. The Virginia Board of Pharmacy's license.
 4. A licensee shall possess and use instrumentation to measure the radioactivity of radioactive drugs. The licensee shall have procedures for use of the instrumentation. The licensee shall measure, by direct measurement or by combination of measurements and calculations, the amount of radioactivity in dosages of alpha, beta, or photon-emitting radioactive drugs prior to transfer for commercial distribution. In addition, the licensee shall:
 - a. Perform tests before initial use, periodically, and following repair, on each instrument for accuracy, linearity, and geometry dependence, as appropriate for the use of the instrument; and make adjustments when necessary; and
 - b. Check each instrument for constancy and proper operation at the

beginning of each day of use.

5. Nothing in this subsection relieves the licensee from complying with applicable FDA, other federal, and state requirements governing radioactive drugs.

6. Each licensee preparing technetium-99m radiopharmaceuticals from molybdenum-99/technetium-99m generators or rubidium-82 from strontium-82/rubidium-82 generators shall test the generator eluates for molybdenum-99 breakthrough or strontium-82 and strontium-85 contamination in accordance with 12VAC5-481-1930. The licensee shall record the results of each test and retain each record for three years after the record is made.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-450. General requirements for the issuance of specific licenses.

A. A license application will be approved if the agency determines that:

1. The applicant is qualified by reason of training and experience to use the material in question for the purpose requested in accordance with these regulations in such a manner as to minimize danger to public health and safety or property;
2. The applicant's proposed equipment, facilities, and procedures are adequate to minimize danger to public health and safety or property;
3. The issuance of the license will not be inimical to the health and safety of the public;
4. The applicant has described in the application how facility design and procedures for operation will minimize, to the extent practicable, contamination of the facility and the environment, facilitate eventual decommissioning, and minimize, to the extent practicable, the generation of radioactive waste; and

5. The applicant satisfies any applicable special requirements in 12VAC5-481-460, 12VAC5-481-470, 12VAC5-481-480, Part V (12VAC5-481-1170 et seq.), Part VII (12VAC5-481-1660 et seq.), Part XI (12VAC5-481-2330 et seq.), Part XII (12VAC5-481-2660 et seq.), Part XIV (12VAC5-481-3140 et seq.) or Part XVI (12VAC5-281-3460 et seq.) of this chapter.

B. Environmental report, commencement of construction. In the case of an application for a license to receive and possess radioactive material for commercial waste disposal by land burial, or for the conduct of any other activity that the agency determines will significantly affect the quality of the environment, the agency, before commencement of construction of the plant or facility in which the activity will be conducted, has concluded, after weighing the environmental, economic, technical and other benefits against environmental costs and considering available alternatives, that the action called for is the issuance of the proposed license, with any appropriate conditions to protect environmental values. Commencement of construction prior to such conclusion shall be grounds for denial of a license to receive and possess radioactive material in such plant or facility. As used in this subsection the term "commencement of construction" means any clearing of land, excavation, or other substantial action that would adversely affect the environment of a site. The term does not mean site exploration, necessary roads for site exploration, borings to determine foundation conditions, or other preconstruction monitoring or testing to establish background information related to the suitability of the site or the protection of environmental values.

C. Financial assurance and records for decommissioning.

1. A person applying for a specific license authorizing the possession and use of unsealed radioactive material shall submit a decommissioning funding plan as described in subdivision 6 of this subsection with the license application for any of the following types of materials:

a. Unsealed radioactive material with a half-life greater than 120 days and in quantities greater than 10^5 times the applicable quantities listed in 12VAC5-

481-3750.

b. Unsealed radioactive material involving a combination of isotopes with R divided by 10^5 being greater than one, where R is defined as the sum of the ratios of the quantity of each isotope to the applicable value in 12VAC5-481-3750.

2. A person applying for a specific license authorizing the possession and use of radioactive material not covered by subdivision 1 of this subsection with a half-life greater than 120 days and in quantities specified in subdivision 5 of this subsection shall do either of the following:

a. Submit a decommissioning funding plan as described in subdivision 6 of this subsection.

b. Submit a written certification, signed by the chief financial officer or other individual designated by management to represent the licensee, that financial assurance has been provided in the amount prescribed in subdivision 5 of this subsection using one of the methods described in subdivision 6 of this subsection and a signed original of the financial instrument obtained to satisfy the requirements of subdivision 7 of this subsection. The written certification may state that the appropriate assurance will be obtained after the application has been approved and the license issued by the agency but before receipt of radioactive material by the applicant. If the applicant defers execution of the financial instrument until after the license has been issued, the applicant shall submit to the agency a signed original of the financial instrument obtained before receipt of licensed material.

3. The following are exempt from the requirements of this subsection:

a. A state, local or other government agency, except for a government agency licensed to handle or process radioactive waste.

b. A person authorized to possess only radioactive materials with a half-life of 65 days or less.

c. Other persons exempted by the agency based on a review of the license

application.

4. Implementation.

a. A person who possesses a specific license authorizing the possession and use of radioactive material issued on or after the effective date as stated in 12VAC5-481-160 that is of a type described in subdivision 1 of this subsection, shall provide financial assurance for decommissioning under this section.

b. A person who possesses a specific license issued before the effective date as stated in 12VAC5-481-160 shall do one of the following:

(1) For a license authorizing the use of radioactive material meeting the criteria of subdivision 1 of this subsection, submit a decommissioning funding plan as described in subdivision 6 of this subsection and a certification of financial assurance for at least \$1,125,000, under the criteria in subdivision 5 of this subsection, with any application for license renewal.

(2) For a license authorizing the use of radioactive material meeting the criteria of subdivision 2 of this subsection, submit a decommissioning funding plan as described in subdivision 6 of this subsection or a certification of financial assurance for decommissioning according to the criteria of subdivision 5 of this subsection with any application for license renewal.

c. The term of the financial assurance shall be from the issuance or renewal of the license until the agency terminates the license.

d. A licensee's financial assurance arrangements may be reviewed annually by the agency to recognize any increases or decreases resulting from inflation or deflation, changes in engineering plans, activities performed or any other condition affecting costs for decommissioning to ensure that sufficient funding is available to cover liability that remains until license termination.

5. Required amounts for financial assurance.

a. A licensee shall provide the following minimum amounts of financial assurance for decommissioning, unless otherwise specified by the agency:

(1) \$1,125,000 if the quantity of material is greater than 10^4 but less than or equal to 10^5 times the applicable quantities of 12VAC5-481-3750 in unsealed form. For a combination of isotopes, R divided by 10^4 is greater than one but R divided by 10^5 is less than or equal to one.

(2) \$225,000 if the quantity of material is greater than 10^3 but less than or equal to 10^4 times the applicable quantities of 12VAC5-481-3750 in unsealed form. For a combination of isotopes, R divided by 10^3 is greater than one but R divided by 10^4 is less than or equal to one.

(3) \$113,000 if the quantity of material is greater than 10^{10} times the applicable quantities of 12VAC5-481-3750 in sealed sources or plated foils. For a combination of isotopes, R divided by 10^{10} is greater than one.

b. The agency may eliminate, reduce or raise the required amount of financial assurance under subdivision 5 a of this subsection for an individual applicant or licensee based on the cost estimate for decommissioning included in the decommissioning funding plan required under subdivision 6 a of this subsection.

6. Decommissioning funding plan.

a. A decommissioning funding plan shall include all the following information:

(1) A cost estimate for decommissioning that considers all of the following:

(a) Probable extent of contamination through the use or possession of radioactive material at the facility or site and the projected cost of removal of the contamination to a level specified by the agency. The evaluation shall encompass probable contaminating events associated with the licensee's or applicant's operation and shall be based on factors such as quantity, half-life, radiation hazard, toxicity and chemical and physical forms.

(b) The extent of possible offsite property damage caused by operation of the

facility or site.

(c) The cost of removal and disposal of radiation sources that are or would be generated, stored, processed or otherwise present at the licensed facility or site.

(d) The costs involved in reclaiming the property on which the facility or site is located and all other properties contaminated by radioactive material authorized under the license.

(2) A description of the method of assuring funds for decommissioning according to subdivision 7 of this subsection.

(3) A description of the method for adjusting cost estimates and associated funding levels periodically over the life of the facility.

b. The decommissioning funding plan shall also contain the licensee's certification that financial assurance has been provided in the amount of the cost estimate for decommissioning and a signed original of the financial instrument obtained to satisfy the requirements of subdivision 7 of this subsection.

7. A licensee may use any of the following methods to provide financial assurance for decommissioning:

a. Prepayment. Prepayment is the deposit prior to operation into an account segregated from licensee assets and outside the licensee's administrative control of cash or liquid assets in an amount sufficient to pay decommissioning costs. Prepayment may be in the form of a trust, escrow account, government fund, certificate of deposit or deposit of government securities.

b. Surety method, insurance or other guarantee. Payment of future decommissioning costs shall be guaranteed by a surety method, insurance or other guarantee. A surety method may be in the form of a surety bond, letter of credit or line of credit. Self insurance, or any method that essentially constitutes self-insurance, may not be used as a method of providing financial

assurance. Any surety method or insurance used to provide financial assurance for decommissioning must meet all of the following criteria:

(1) The surety method or insurance shall be open-ended or, if written for a specified term, renewed automatically unless 90 days or more prior to the renewal date, the issuer notifies the agency, the beneficiary and the licensee of its intention not to renew. The surety method or insurance shall also provide that the full face amount be paid to the beneficiary automatically prior to the expiration without proof of forfeiture if the licensee fails to provide a replacement acceptable to the agency within 30 days after receipt of notification of cancellation.

(2) The surety method or insurance shall be payable to a trust established for decommissioning costs. The agency shall approve the trustee and the trust.

(3) The surety method or insurance shall remain in effect until the agency terminates the license.

c. External sinking fund. An external sinking fund may be used in which deposits are made at least annually, coupled with a surety method or insurance, the value of which may decrease by the amount being accumulated in the sinking fund. An external sinking fund may be in the form of a trust, escrow account, government fund, certificate of deposit or deposit of government securities. The surety or insurance provisions shall meet the requirements of subdivision 7 b of this subsection.

d. Statement of intent. A state or local government licensee exempt under subdivision 3 of this subsection shall submit a written statement of intent containing a cost estimate for decommissioning or an amount based on subdivision 5 of this subsection. The cost estimate shall indicate that funds for decommissioning will be obtained when necessary.

8. A licensee shall keep the following records of information related to decommissioning of a facility in an identified location until the site is released for unrestricted use:

a. Records of spills or other unusual occurrences involving the spread of radioactive contamination in and around the facility, equipment or site. The records may be limited to instances where contamination remains after any cleanup procedures or when there is reasonable likelihood that radioactive contaminants may have spread to inaccessible areas or into porous materials such as concrete. The records shall include any known information on identification of involved nuclides, quantities, forms and concentrations.

b. As-built drawings and modifications of structures and equipment in restricted areas where radioactive materials are used or stored, and of locations of possible inaccessible contamination such as buried pipes that may contain radioactive contaminants. If required drawings are referenced, each relevant document does not need to be indexed individually. If drawings are not available, a licensee shall substitute appropriate records of available information concerning the areas and locations of inaccessible contamination.

Note: As-built architectural and engineering drawings need to reflect the final details of the structures and equipment as they were constructed.

c. Except for areas containing only sealed sources that have not leaked or where no contamination remains after a leak, or byproduct materials with half-lives of less than 65 days, a list containing all the following:

- (1) All areas currently and formerly designated as restricted areas.
- (2) All areas outside of restricted areas that require documentation under subdivision 8 (c) 1 of this subsection.
- (3) All areas outside of restricted areas where current and previous wastes have been buried as documented under 12VAC5-481-1060.
- (4) All areas outside of restricted areas that contain radioactive material such that, if the license expired, the licensee would be required to either decontaminate the area to meet the criteria for decommissioning in 12VAC5-481-510 or apply for approval for disposal under 12VAC5-481-920.

d. Records of the cost estimate performed for the decommissioning funding plan or the amount certified for decommissioning and records of the funding method used for assuring funds.

9. A licensee shall keep the records in subdivision 8 of this subsection until the site is decommissioned and approved by the agency for unrestricted use.

10. Prior to a licensed activity being transferred to another licensee under 12VAC5-481-500 B, the original licensee shall transfer all records under subdivision 8 of this subsection to the new licensee. The new licensee shall be responsible for maintaining the records until their license is terminated by the agency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-460. (Repealed.)

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; repealed, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-470. Special requirements for specific licenses of broad scope.

This section prescribes requirements for the issuance of specific licenses of broad scope for radioactive material and certain regulations governing holders of such licenses. (Authority to transfer possession or control by the manufacturer, processor, or producer of any equipment, device, commodity, or other product containing byproduct material whose subsequent possession, use, transfer, and disposal by all other persons are exempted from regulatory requirements may be obtained only from the Nuclear Regulatory Commission, Washington, D.C. 20555-0001.)

A. The different types of broad scope licenses are set forth below:

1. A "Type A specific license of broad scope" is a specific license authorizing receipt, acquisition, ownership, possession, use and transfer of any chemical or physical form of the radioactive material specified in the license, but not exceeding quantities specified in the license, for any authorized purpose. The quantities specified are usually in the multicurie range.

2. A "Type B specific license of broad scope" is a specific license authorizing receipt, acquisition, ownership, possession, use and transfer of any chemical or physical form of radioactive material specified in 12VAC5-481-3760, for any authorized purpose. The possession limit for a Type B license of broad scope, if only one radionuclide is possessed thereunder, is the quantity specified for that radionuclide in 12VAC5-481-3760, Column I. If two or more radionuclides are possessed thereunder, the possession limit for each is determined as follows: for each radionuclide, determine the ratio of the quantity possessed to the applicable quantity specified in 12VAC5-481-3760, Column I, for that radionuclide. The sum of the ratios for all radionuclides possessed under the license shall not exceed unity.

3. A "Type C specific license of broad scope" is a specific license authorizing receipt, acquisition, ownership, possession, use, and transfer of any chemical or physical form of radioactive material specified in 12VAC5-481-3760, for any authorized purpose. The possession limit for a Type C license of broad scope, if only one radionuclide is possessed thereunder, is the quantity specified for that radionuclide in 12VAC5-481-3760, Column II. If two or more radionuclides are possessed thereunder, the possession limit is determined for each as follows: for each radionuclide, determine the ratio of the quantity possessed to the applicable quantity specified in 12VAC5-481-3760, Column II, for that radionuclide. The sum of the ratios for all radionuclides possessed under the license shall not exceed unity.

B. An application for a Type A specific license of broad scope will be approved if:

1. The applicant satisfies the general requirements specified in 12VAC5-481-450;

2. The applicant has engaged in a reasonable number of activities involving the use of radioactive material; and

3. The applicant has established administrative controls and provisions relating to organization and management, procedures, recordkeeping, material control and accounting, and management review that are necessary to assure safe operations, including:

a. The establishment of a radiation safety committee composed of such persons as a radiation safety officer, a representative of management, and persons trained and experienced in the safe use of radioactive material;

b. The appointment of a radiation safety officer who is qualified by training and experience in radiation protection, and who is available for advice and assistance on radiation safety matters; and

c. The establishment of appropriate administrative procedures to assure:

(1) Control of procurement and use of radioactive material;

(2) Completion of safety evaluations of proposed uses of radioactive material that take into consideration such matters as the adequacy of facilities and equipment, training and experience of the user, and the operating or handling procedures; and

(3) Review, approval, and recording by the radiation safety committee of safety evaluations of proposed uses prepared in accordance with subdivision 3 c (2) of this subsection prior to use of the radioactive material.

C. An application for a Type B specific license of broad scope will be approved if:

1. The applicant satisfies the general requirements specified in 12VAC5-481-450; and

2. The applicant has established administrative controls and provisions relating to organization and management, procedures, recordkeeping, material control and accounting, and management review that are necessary to assure safe operations, including:

a. The appointment of a radiation safety officer who is qualified by training and experience in radiation protection, and who is available for advice and assistance on radiation safety matters, and

b. The establishment of appropriate administrative procedures to assure,

(1) Control of procurement and use of radioactive material,

(2) Completion of safety evaluations of proposed uses of radioactive material that take into consideration such matters as the adequacy of facilities and equipment, training and experience of the user, and the operating or handling procedures, and

(3) Review, approval, and recording by the radiation safety officer of safety evaluations of proposed uses prepared in accordance with subdivision 2 b (2) of this subsection prior to use of the radioactive material.

D. An application for a Type C specific license of broad scope will be approved if:

1. The applicant satisfies the general requirements specified in 12VAC5-481-450;

2. The applicant submits a statement that radioactive material will be used only by, or under the direct supervision of, individuals who have received:

a. A college degree at the bachelor level, or equivalent training and experience, in the physical or biological sciences or in engineering, and

b. At least 40 hours of training and experience in the safe handling of radioactive material, and in the characteristics of ionizing radiation, units of radiation dose and quantities, radiation detection instrumentation, and biological hazards of exposure to radiation appropriate to the type and forms of radioactive material to be used; and

3. The applicant has established administrative controls and provisions relating to procurement of radioactive material, procedures, recordkeeping, material control and accounting, and management review necessary to assure safe operations.

E. Specific licenses of broad scope are subject to the following conditions:

1. Unless specifically authorized, persons licensed pursuant to 12VAC5-481-470

shall not:

- a. Conduct tracer studies in the environment involving direct release of radioactive material;
 - b. Receive, acquire, own, possess, use, or transfer devices containing 3.7 PBq (100,000 Ci) or more of radioactive material in sealed sources used for irradiation of materials;
 - c. Conduct activities for which a specific license issued by the agency under Part III (12VAC5-481-380 et seq.), Part V (12VAC5-481-1170 et seq.) or Part VII (12VAC5-481-1660 et seq.) of this chapter is required; or
 - d. Add or cause the addition of radioactive material to any food, beverage, cosmetic, drug, or other product designed for ingestion or inhalation by, or application to, a human being.
2. Each Type A specific license of broad scope issued under this part shall be subject to the condition that radioactive material possessed under the license may only be used by, or under the direct supervision of, individuals approved by the licensee's radiation safety committee.
 3. Each Type B specific license of broad scope issued under this part shall be subject to the condition that radioactive material possessed under the license may only be used by, or under the direct supervision of, individuals approved by the licensee's radiation safety officer.
 4. Each Type C specific license of broad scope issued under this part shall be subject to the condition that radioactive material possessed under the license may only be used by, or under the direct supervision of, individuals who satisfy the requirements of subsection D of this section.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-480. Special requirements for a specific license to manufacture, assemble, repair, or distribute commodities, products, or devices that contain radioactive material.

A. Reserved.

B. Licensing the distribution of radioactive material in exempt quantities. (Authority to transfer possession or control by the manufacturer, processor, or producer of any equipment, device, commodity, or other product containing radioactive material whose subsequent possession, use, transfer, and disposal by all other persons are exempted from regulatory requirements may be obtained only from the Nuclear Regulatory Commission, Washington, D.C. 20555-0001.)

C. Licensing the manufacture or initial transfer of devices to persons generally licensed under 12VAC5-481-430 B.

1. An application for a specific license to manufacture or initially transfer devices containing radioactive material, excluding special nuclear material, to persons generally licensed under 12VAC5-481-430 B or equivalent regulations of the NRC, or another agreement state will be approved if:

a. The applicant satisfies the general requirements of 12VAC5-481-450;

b. The applicant submits sufficient information relating to the design, manufacture, prototype testing, quality control, labels, proposed uses, installation, servicing, leak testing, operating and safety instructions, and potential hazards of the device to provide reasonable assurance that:

(1) The device can be safely operated by persons not having training in radiological protection,

(2) Under ordinary conditions of handling, storage, and use of the device, the radioactive material contained in the device will not be released or inadvertently removed from the device, and it is unlikely that any person will receive in any period of one calendar quarter a dose in excess of 10% of the

limits specified in 12VAC5-481-640, and

(3) Under accident conditions such as fire and explosion associated with handling, storage, and use of the device, it is unlikely that any person would receive an external radiation dose or dose commitment in excess of the dose to the appropriate organ as specified in 12VAC5-481-3580, Column IV; and

c. Each device bears a durable, legible, clearly visible label or labels approved by the agency, which contain in a clearly identified and separate statement:

(1) Instructions and precautions necessary to assure safe installation, operation, and servicing of the device; documents such as operating and service manuals may be identified in the label and used to provide this information;

(2) The requirement, or lack of requirement, for leak testing, or for testing any "on-off" mechanism and indicator, including the maximum time interval for such testing, and the identification of radioactive material by isotope, quantity of radioactivity, and date of determination of the quantity, and

(3) The information called for in one of the following statements, as appropriate, in the same or substantially similar form:

(a) The receipt, possession, use, and transfer of this device, Model _____, Serial No. _____, are subject to a general license or the equivalent and the regulations of the Nuclear Regulatory Commission or a state with which the Nuclear Regulatory Commission has entered into an agreement for the exercise of regulatory authority. This label shall be maintained on the device in a legible condition. Removal of this label is prohibited.

CAUTION—RADIOACTIVE MATERIAL

_____ Name of manufacturer or initial transferor

(b) The receipt, possession, use, and transfer of this device, Model _____, Serial No. _____, are subject to a general license or the equivalent, and the regulations of a licensing state. This label shall be maintained on the device in a legible condition. Removal of this label is prohibited. (The model, serial number, and name of the manufacturer or distributor may be omitted from this label provided the information is elsewhere specified in labeling affixed to the device.)

CAUTION—RADIOACTIVE MATERIAL

_____ Name of manufacturer or initial transferor

2. In the event the applicant desires that the device be required to be tested at intervals longer than six months, either for proper operation of the "on-off" mechanism and indicator, if any, or for leakage of radioactive material or for both, the applicant shall include in the application sufficient information to demonstrate that such longer interval is justified by performance characteristics of the device or similar devices and by design features that have a significant bearing on the probability or consequences of leakage of radioactive material from the device or failure of the "on-off" mechanism and indicator. In determining the acceptable interval for the test for leakage of radioactive material, the agency will consider information that includes, but is not limited to:

- a. Primary containment or source capsule;
- b. Protection of primary containment;
- c. Method of sealing containment;
- d. Containment construction materials;
- e. Form of contained radioactive material;
- f. Maximum temperature withstood during prototype tests;
- g. Maximum pressure withstood during prototype tests;
- h. Maximum quantity of contained radioactive material;

- i. Radiotoxicity of contained radioactive material; and
 - j. Operating experience with identical devices or similarly designed and constructed devices.
3. In the event the applicant desires that the general licensee under 12VAC5-481-430 B, or under equivalent regulations of the NRC, or another agreement state, be authorized to install the device, collect the sample to be analyzed by a specific licensee for leakage of radioactive material, service the device, test the "on-off" mechanism and indicator, or remove the device from installation, the applicant shall include in the application written instructions to be followed by the general licensee, estimated calendar quarter doses associated with such activity or activities, and basis for such estimates. The submitted information shall demonstrate that performance of such activity or activities by an individual untrained in radiological protection, in addition to other handling, storage, and use of devices under the general license, is unlikely to cause that individual to receive a calendar quarter dose in excess of 10% of the limits specified in 12VAC5-481-640.
4. Each person licensed under this subsection to distribute devices to generally licensed persons shall:
- a. Furnish a copy of the general license contained in 12VAC5-481-430 B to each person to whom he directly or through an intermediate person transfers radioactive material in a device for use pursuant to the general license contained in 12VAC5-481-430 B;
 - b. Furnish a copy of the general license contained in the NRC's, or another agreement state's, regulation equivalent to 12VAC5-481-430 B, or alternatively, furnish a copy of the general license contained in 12VAC5-481-430 B to each person to whom he directly or through an intermediate person transfers radioactive material in a device for use pursuant to the general license of the NRC, or another agreement state. If a copy of the general license in 12VAC5-481-430 B is furnished to such a person, it shall be

accompanied by a note explaining that the use of the device is regulated by the NRC, or another agreement state, under requirements substantially the same as those in 12VAC5-481-430 B;

c. Report to the agency all transfers of such devices to persons for use under the general license in 12VAC5-481-430 B. Such report shall identify each general licensee by name and address, an individual by name and/or position who may constitute a point of contact between the agency and the general licensee, the type and model number of device transferred, and the quantity and type of radioactive material contained in the device. If one or more intermediate persons will temporarily possess the device at the intended place of use prior to its possession by the user, the report shall include identification of each intermediate person by name, address, contact, and relationship to the intended user. If no transfers have been made to persons generally licensed under 12VAC5-481-430 B during the reporting period, the report shall so indicate. The report shall cover each calendar quarter and shall be filed within 30 days thereafter;

d. Furnish reports to other agencies.

(1) Report to the NRC all transfers of such devices to persons for use under the NRC's general license in 10 CFR 31.5.

(2) Report to the responsible state agency all transfers of devices manufactured and distributed pursuant to this subsection for use under a general license in that state's regulations equivalent to 12VAC5-481-430 B.

(3) Such reports shall identify each general licensee by name and address, an individual by name and/or position who may constitute a point of contact between the agency and the general licensee, the type and model of the device transferred, and the quantity and type of radioactive material contained in the device. If one or more intermediate persons will temporarily possess the device at the intended place of use prior to its possession by the user, the report shall include identification of each intermediate person by name,

address, contact, and relationship to the intended user. The report shall be submitted within 30 days after the end of each calendar quarter in which such a device is transferred to the generally licensed person.

(4) If no transfers have been made to NRC general licensees during the reporting period, this information shall be reported to the NRC.

(5) If no transfers have been made to general licensees within a particular state during the reporting period, this information shall be reported to the responsible state agency upon request of that agency; and

e. Keep records showing the name, address, and the point of contact for each general licensee to whom he directly or through an intermediate person transfers radioactive material in devices for use pursuant to the general license provided in 12VAC5-481-430 B, or equivalent regulations of the NRC or another agreement state. The records shall show the date of each transfer, the radionuclide and the quantity of radioactivity in each device transferred, the identity of any intermediate person, and compliance with the report requirements of subdivision 4 of this subsection.

f. If a notification of bankruptcy has been made under 12VAC5-481-500 E or the license is to be terminated, each person licensed under this section shall provide, upon request, to the agency, the NRC and to any appropriate agreement state, records of final disposition required under subdivision 4 e of this subsection.

g. The licensee shall maintain all information concerning transfers and receipts of devices that supports the reports required by this section. Records required by this section must be maintained for a period of three years following the date of the recorded event.

D. Special requirements for the manufacture, initially transfer, assembly, or repair of luminous safety devices for use in aircraft. An application for a specific license to manufacture, assemble, or repair luminous safety devices containing tritium or promethium-147 for use in aircraft, for distribution to persons generally licensed under

12VAC5-481-430 D will be approved if:

1. The applicant satisfies the general requirements specified in 12VAC5-481-450; and
2. The applicant satisfies the requirements of 10 CFR 32.53, 32.54, 32.55, 32.56, 32.101 and 32.110, or their equivalent.

E. Special requirements for license to manufacture or initially transfer calibration sources containing americium-241, plutonium or radium-226 for distribution to persons generally licensed under 12VAC5-481-430 F. An application for a specific license to manufacture calibration and reference sources containing americium-241, plutonium or radium-226 to persons generally licensed under 12VAC5-481-430 F will be approved if:

1. The applicant satisfies the general requirement of 12VAC5-481-450; and
2. The applicant satisfies the requirements of 10 CFR 32.57, 32.58, 32.59, 32.102 and 10 CFR 70.39 or their equivalent.

F. Reserved.

G. Manufacture and distribution of radioactive material for certain in vitro clinical or laboratory testing under general license. An application for a specific license to manufacture or distribute radioactive material for use under the general license of 12VAC5-481-430 G will be approved if:

1. The applicant satisfies the general requirements specified in 12VAC5-481-450.
2. The radioactive material is to be prepared for distribution in prepackaged units of:
 - a. Carbon-14 in units not exceeding 370 kBq (10 μ Ci) each.
 - b. Cobalt-57 in units not exceeding 370 kBq (10 μ Ci) each.
 - c. Hydrogen-3 (tritium) in units not exceeding 1.85 MBq (50 μ Ci) each.
 - d. Iodine-125 in units not exceeding 370 kBq (10 μ Ci) each.
 - e. Mock iodine-125 in units not exceeding 1.85 kBq (0.05 μ Ci) of iodine-129 and 185 Bq (0.005 μ Ci) of americium-241 each.
 - f. Iodine-131 in units not exceeding 370 kBq (10 μ Ci) each.

- g. Iron-59 in units not exceeding 740 kBq (20 μ Ci) each.
 - h. Selenium-75 in units not exceeding 370 kBq (10 μ Ci) each.
3. Each prepackaged unit bears a durable, clearly visible label:
- a. Identifying the radioactive contents as to chemical form and radionuclide, and indicating that the amount of radioactivity does not exceed 370 kBq (10 μ Ci) of iodine-125, iodine-131, carbon-14, cobalt-57, or selenium-75; 1.85 MBq (50 μ Ci) of hydrogen-3 (tritium); 740 kBq (20 μ Ci) of iron-59; or mock iodine-125 in units not exceeding 1.85 kBq (0.05 μ Ci) of iodine-129 and 185 Bq (0.005 μ Ci) of americium-241 each; and
 - b. Displaying the radiation caution symbol described in 12VAC5-481-850 and the words, "CAUTION, RADIOACTIVE MATERIAL," and "Not for Internal or External Use in Humans or Animals."
4. One of the following statements, as appropriate, or a substantially similar statement that contains the information called for in one of the following statements, appears on a label affixed to each prepackaged unit or appears in a leaflet or brochure that accompanies the package:
- a. This radioactive material may be received, acquired, possessed, and used only by physicians, veterinarians, clinical laboratories or hospitals and only for in vitro clinical or laboratory tests not involving internal or external administration of the material, or the radiation therefrom, to human beings or animals. Its receipt, acquisition, possession, use, and transfer are subject to the regulations and a general license of the Nuclear Regulatory Commission or of a state with which the Nuclear Regulatory Commission has entered into an agreement for the exercise of regulatory authority.

_____ Name of manufacturer
 - b. This radioactive material may be received, acquired, possessed, and used only by physicians, veterinarians, clinical laboratories or hospitals and only for in vitro clinical or laboratory tests not involving internal or external

administration of the material, or the radiation therefrom, to human beings or animals. Its receipt, acquisition, possession, use, and transfer are subject to the regulations and a general license of a licensing state.

_____ Name of manufacturer

5. The label affixed to the unit, or the leaflet or brochure which accompanies the package, contains adequate information as to the precautions to be observed in handling and storing such radioactive material. In the case of the Mock Iodine-125 reference or calibration source, the information accompanying the source must also contain directions to the licensee regarding the waste disposal requirements set out in 12VAC5-481-910.

H. Licensing the manufacture and distribution of ice detection devices. An application for a specific license to manufacture and distribute ice detection devices to persons generally licensed under 12VAC5-481-430 H will be approved if:

1. The applicant satisfies the general requirements of 12VAC5-481-450; and
2. The criteria of 10 CFR 32.61, 32.62, 32.103 and 32.110 are met.

I. Manufacture, preparation, or transfer for commercial distribution of drugs containing radioactive material for medical use under Part VII (12VAC5-481-1660 et seq.).

1. An application for a specific license to manufacture, prepare, or transfer for commercial distribution drugs containing radioactive material for use by persons authorized pursuant to Part VII (12VAC5-481-1660 et seq.) will be approved if:

- a. The applicant satisfies the general requirements specified in 12VAC5-481-450;
- b. The applicant submits evidence that the applicant is at least one of the following:
 - (1) Registered or licensed with the U.S. Food and Drug Administration (FDA) as a drug manufacturer;
 - (2) Registered or licensed with a state agency as a drug manufacturer;

- (3) Licensed as a pharmacy by the Virginia Board of Pharmacy;
- (4) Operating as a nuclear pharmacy within a federal medical institution; or
- (5) A PET drug production facility registered with a state agency.

c. The applicant submits information on the radionuclide; the chemical and physical form; the maximum activity per vial, syringe, generator, or other container of the radioactive drug; and the shielding provided by the packaging to show it is appropriate for the safe handling and storage of the radioactive drugs by medical use licensees; and

d. The applicant satisfies the following labeling requirements:

(1) A label is affixed to each transport radiation shield, whether it is constructed of lead, glass, plastic, or other material, of a radioactive drug to be transferred for commercial distribution. The label must include the radiation symbol and the words "CAUTION, RADIOACTIVE MATERIAL" or "DANGER, RADIOACTIVE MATERIAL"; the name of the radioactive drug or its abbreviation; and the quantity of radioactivity at a specified date and time. For radioactive drugs with a half life greater than 100 days, the time may be omitted.

(2) A label is affixed to each syringe, vial, or other container used to hold a radioactive drug to be transferred for commercial distribution. The label must include the radiation symbol and the words "CAUTION, RADIOACTIVE MATERIAL" or "DANGER, RADIOACTIVE MATERIAL" and an identifier that ensures that the syringe, vial, or other container can be correlated with the information on the transport radiation shield label.

2. A licensee authorized to manufacture, prepare or transfer for commercial distribution radioactive drugs shall ensure that any individual preparing the drugs is one of the following:

- a. An authorized nuclear pharmacist (ANP) as defined in 12VAC5-481-10;
- b. An individual that meets the requirements specified in 12VAC5-481-1770

and 12VAC5-481-1790, and the licensee has received an approved license amendment identifying this individual as an ANP;

c. A pharmacist, as defined in 12VAC5-481-10, designated as an ANP if:

(1) The individual was a nuclear pharmacist preparing only radioactive drugs containing accelerator-produced radioactive material, and

(2) The individual practiced at a pharmacy at a government agency or federally recognized Indian Tribe before November 30, 2007, or at all other pharmacies before August 8, 2009, or an earlier date as noticed by the NRC;

or

d. An individual under the supervision of an ANP as specified in 12VAC5-481-1710.

3. Shall provide to the agency no later than 30 days after the date that the licensee allows, under subdivision 2 a or c in this subsection, the individual to work as an ANP:

a. The individual's certification by a specialty board whose certification process has been recognized by the NRC with the written attestation signed by a preceptor as required by 12VAC5-481-1770;

b. An NRC or another agreement state license;

c. NRC master materials licensee permit;

d. The permit issued by a licensee or NRC master materials permittee of broad scope or the authorization from a commercial nuclear pharmacy authorized to list its own authorized nuclear pharmacist; or

e. Documentation that only accelerator-produced radioactive materials were used in the practice of nuclear pharmacy at a government agency or federally recognized Indian Tribe before November 30, 2007, or at all other locations of use before August 8, 2009, or an earlier date as noticed by the NRC; and

f. The Virginia Board of Pharmacy's license.

4. A licensee shall possess and use instrumentation to measure the radioactivity

of radioactive drugs. The licensee shall have procedures for use of the instrumentation. The licensee shall measure, by direct measurement or by combination of measurements and calculations, the amount of radioactivity in dosages of alpha, beta, or photon-emitting radioactive drugs prior to transfer for commercial distribution. In addition, the licensee shall:

- a. Perform tests before initial use, periodically, and following repair, on each instrument for accuracy, linearity, and geometry dependence, as appropriate for the use of the instrument; and make adjustments when necessary; and
- b. Check each instrument for constancy and proper operation at the beginning of each day of use.

5. Nothing in this subsection relieves the licensee from complying with applicable FDA, other federal, and state requirements governing radioactive drugs.

6. Each licensee preparing technetium-99m radiopharmaceuticals from molybdenum-99/technetium-99m generators or rubidium-82 from strontium-82/rubidium-82 generators shall test the generator eluates for molybdenum-99 breakthrough or strontium-82 and strontium-85 contamination in accordance with 12VAC5-481-1930. The licensee shall record the results of each test and retain each record for three years after the record is made.

J. Manufacture and distribution of sources or devices containing radioactive material for medical use. An application for a specific license to manufacture and distribute sources and devices containing radioactive material to persons licensed pursuant to Part VII (12VAC5-481-1660 et seq.) of this chapter for use as a calibration or reference source or for the uses listed in 12VAC5-481-2010, 12VAC5-481-2020, 12VAC5-481-2040 and 12VAC5-481-2060 will be approved if:

1. The applicant satisfies the general requirements in 12VAC5-481-450;
2. The applicant submits sufficient information regarding each type of source or device pertinent to an evaluation of its radiation safety, including:
 - a. The radioactive material contained, its chemical and physical form, and amount,

- b. Details of design and construction of the source or device,
 - c. Procedures for, and results of, prototype tests to demonstrate that the source or device will maintain its integrity under stresses likely to be encountered in normal use and accidents,
 - d. For devices containing radioactive material, the radiation profile of a prototype device,
 - e. Details of quality control procedures to assure that production sources and devices meet the standards of the design and prototype tests,
 - f. Procedures and standards for calibrating sources and devices,
 - g. Legend and methods for labeling sources and devices as to their radioactive content, and
 - h. Instructions for handling and storing the source or device from the radiation safety standpoint; these instructions are to be included on a durable label attached to the source or device or attached to a permanent storage container for the source or device provided, that instructions that are too lengthy for such label may be summarized on the label and printed in detail on a brochure that is referenced on the label;
3. The label affixed to the source or device, or to the permanent storage container for the source or device, contains information on the radionuclide, quantity, and date of assay, and a statement that the source or device is licensed by the agency for distribution to persons licensed pursuant to 12VAC5-481-1830, 12VAC5-481-2010, 12VAC5-481-2020 and 12VAC5-481-2040 or under equivalent licenses of the NRC, or another agreement state, provided that such labeling for sources that do not require long term storage may be on a leaflet or brochure that accompanies the source;
4. In the event the applicant desires that the source or device be required to be tested for leakage of radioactive material at intervals longer than six months, the applicant shall include sufficient information to demonstrate that such longer

interval is justified by performance characteristics of the source or device or similar sources or devices and by design features that have a significant bearing on the probability or consequences of leakage of radioactive material from the source; and

5. In determining the acceptable interval for test of leakage of radioactive material, the agency will consider information that includes, but is not limited to:

- a. Primary containment or source capsule,
- b. Protection of primary containment,
- c. Method of sealing containment,
- d. Containment construction materials,
- e. Form of contained radioactive material,
- f. Maximum temperature withstood during prototype tests,
- g. Maximum pressure withstood during prototype tests,
- h. Maximum quantity of contained radioactive material,
- i. Radiotoxicity of contained radioactive material, and
- j. Operating experience with identical sources or devices or similarly designed and constructed sources or devices.

K. Requirements for license to manufacture and distribute industrial products containing depleted uranium for mass-volume applications.

1. An application for a specific license to manufacture industrial products and devices containing depleted uranium for use pursuant to 12VAC5-481-420 C or equivalent regulations of the NRC or another agreement state will be approved if:

- a. The applicant satisfies the general requirements specified in 12VAC5-481-450;
- b. The applicant submits sufficient information relating to the design, manufacture, prototype testing, quality control procedures, labeling or marking, proposed uses, and potential hazards of the industrial product or device to provide reasonable assurance that possession, use, or transfer of

the depleted uranium in the product or device is not likely to cause any individual to receive in any period of one calendar quarter a radiation dose in excess of 10% of the limits specified in 12VAC5-481-640; and

c. The applicant submits sufficient information regarding the industrial product or device and the presence of depleted uranium for a mass-volume application in the product or device to provide reasonable assurance that unique benefits will accrue to the public because of the usefulness of the product or device.

2. In the case of an industrial product or device whose unique benefits are questionable, the agency will approve an application for a specific license under this subsection only if the product or device is found to combine a high degree of utility and low probability of uncontrolled disposal and dispersal of significant quantities of depleted uranium into the environment.

3. The agency may deny any application for a specific license under this subsection if the end use(s) of the industrial product or device cannot be reasonably foreseen.

4. Each person licensed pursuant to subdivision 1 of this subsection shall:

a. Maintain the level of quality control required by the license in the manufacture of the industrial product or device, and in the installation of the depleted uranium into the product or device;

b. Label or mark each unit to:

(1) Identify the manufacturer or initial transferor of the product or device and the number of the license under which the product or device was manufactured or initially transferred, the fact that the product or device contains depleted uranium, and the quantity of depleted uranium in each product or device; and

(2) State that the receipt, possession, use, and transfer of the product or device are subject to a general license or the equivalent and the regulations of the NRC or another agreement state;

c. Assure that the depleted uranium before being installed in each product or device has been impressed with the following legend clearly legible through any plating or other covering: "Depleted Uranium";

d. Do the following:

(1) Furnish a copy of the general license contained in 12VAC5-481-420 C and a copy of agency form "Certificate - Use of Depleted Uranium under a General License" to each person to whom depleted uranium in a product or device for use pursuant to the general license contained in 12VAC5-481-420 C is transferred, or

(2) Furnish a copy of the general license contained in the NRC's or another agreement state's regulation equivalent to 12VAC5-481-420 B and a copy of the NRC's or another agreement state's certificate, or alternatively, furnish a copy of the general license contained in 12VAC5-481-420 C and a copy of agency form "Certificate - Use of Depleted Uranium under a General License" to each person to whom depleted uranium in a product or device for use pursuant to the general license of the NRC or another agreement state is transferred, with a note explaining that use of the product or device is regulated by the NRC or another agreement state under requirements substantially the same as those in 12VAC5-481-420 C;

e. Report to the agency all transfers of industrial products or devices to persons for use under the general license in 12VAC5-481-420 C. Such report shall identify each general licensee by name and address, an individual by name and/or position who may constitute a point of contact between the agency and the general licensee, the type and model number of device transferred, and the quantity of depleted uranium contained in the product or device. The report shall be submitted within 30 days after the end of each calendar quarter in which such a product or device is transferred to the generally licensed person. If no transfers have been made to persons generally licensed under 12VAC5-481-420 C during the reporting period, the

report shall so indicate;

f. Do the following:

(1) Report to the NRC all transfers of industrial products or devices to persons for use under the NRC general license in 10 CFR 40.25,

(2) For devices transferred to another agreement state, report to the responsible state agency all transfers of devices manufactured and distributed pursuant to this subsection for use under a general license in that state's regulations equivalent to 12VAC5-481-420 C,

(3) Such report shall identify each general licensee by name and address, an individual by name and/or position who may constitute a point of contact between the agency and the general licensee, the type and model number of the device transferred, and the quantity of depleted uranium contained in the product or device. The report shall be submitted within 30 days after the end of each calendar quarter in which such product or device is transferred to the generally licensed person,

(4) If no transfers have been made to NRC licensees during the reporting period, this information shall be reported to the NRC, and

(5) If no transfers have been made to general licensees within another agreement state during the reporting period, this information shall be reported to the responsible state agency upon the request of that agency; and keep records showing the name, address, and point of contact for each general licensee to whom he transfers depleted uranium in industrial products or devices for use pursuant to the general license provided in 12VAC5-481-420 C or equivalent regulations of the NRC or another agreement state. The records shall be maintained for a period of two years and shall show the date of each transfer, the quantity of depleted uranium in each product or device transferred, and compliance with the report requirements of this section.

L. An application for a specific license to manufacture, or initially transfer for sale or distribution, synthetic plastic resins containing scandium-46 for use pursuant to

12VAC5-481-400 F will be approved if:

1. The applicant satisfies the general requirements specified in 12VAC5-481-450 of this chapter;
2. The product is designed to be used only for sand-consolidation in oil wells;
3. The applicant submits the following information:
 - a. The general description of the product to be manufactured or initially transferred.
 - b. A description of control procedures to be used to assure that the concentration of scandium-46 in the final product at the time of distribution will not exceed 1.4×10^{-3} $\mu\text{Ci/ml}$.
4. Each container of such product will bear a durable, legible label approved by the agency, which contains the following information:
 - a. The product name;
 - b. A statement that the product contains radioactive scandium and is designed and manufactured only for sand-consolidation in oil wells;
 - c. Instructions necessary for proper use; and
 - d. The manufacturer's name.

M. Serialization of nationally tracked sources. Each licensee who manufactures a nationally tracked source shall assign a unique serial number to each nationally tracked source. Serial numbers must be composed only of alpha-numeric characters.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-490. Issuance of specific licenses.

- A. Upon a determination that an application meets the requirements of the Act and

the regulations of the agency, the agency will issue a specific license authorizing the proposed activity in such form and containing such conditions and limitations as it deems appropriate or necessary.

B. The agency may incorporate in any license at the time of issuance, or thereafter by appropriate rule, regulation, or order, such additional requirements and conditions with respect to the licensee's receipt, possession, use, and transfer of radioactive material subject to this part as it deems appropriate or necessary in order to:

1. Minimize danger to public health and safety or property;
2. Require such reports and the keeping of such records, and to provide for such inspections of activities under the license as may be appropriate or necessary; and
3. Prevent loss or theft of material subject to this part.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-500. Specific terms and conditions of licenses.

A. Each license issued pursuant to this part shall be subject to all the provisions of the Act, now or hereafter in effect, and to all rules, regulations, and orders of the agency.

B. No license issued or granted under this part and no right to possess or utilize radioactive material granted by any license issued pursuant to this part shall be transferred, assigned, or in any manner disposed of, either voluntarily or involuntarily, directly or indirectly, through transfer of control of any license to any person unless the agency shall, after securing full information find that the transfer is in accordance with the provisions of the Act, now or hereafter in effect, and to all valid rules, regulations, and orders of the agency, and shall give its consent in writing.

C. Each person licensed by the agency pursuant to this part shall confine use and

possession of the material licensed to the locations and purposes authorized in the license.

D. Each licensee shall notify the agency in writing when the licensee decides to permanently discontinue all activities involving materials authorized under the license.

E. Each licensee shall notify the agency in writing immediately following the filing of a voluntary or involuntary petition for bankruptcy under any Chapter of Title 11 (Bankruptcy) of the United States Code by or against:

1. The licensee;
2. An entity (as that term is defined in 11 USC §101(15)) controlling the licensee or listing the license or licensee as property of the estate; or
3. An affiliate (as that term is defined in 11 USC §101(2)) of the licensee.

F. The notification specified in subsection E of this section shall indicate the bankruptcy court in which the petition for bankruptcy was filed and the date of the filing of the petition.

G. PET Distribution.

1. Authorization under 12VAC5-481-440 H to produce PET radioactive drugs for noncommercial transfer to medical use licensees in its consortium does not relieve the licensee from complying with applicable FDA, other state or local requirements governing radioactive drugs.

2. Each licensee authorized under 12VAC5-481-440 H to produce PET radioactive drugs for noncommercial transfer to medical use licensees in its consortium shall:

- a. Satisfy the labeling requirements in 12VAC5-481-480 I 1 d for each PET radioactive drug transport radiation shield and each syringe, vial, or other container used to hold a PET radioactive drug intended for noncommercial distribution to members of its consortium.
- b. Possess and use instrumentation to measure the radioactivity of the PET radioactive drugs intended for noncommercial distribution to members of its

consortium and meet the procedural, radioactivity measurement, instrument test, instrument check, and instrument adjustment requirements in 12VAC5-481-480 I 3.

3. A licensee that is a pharmacy authorized under 12VAC5-481-440 H to produce PET radioactive drugs for noncommercial transfer to medical use licensees in its consortium shall require that any individual that prepares PET radioactive drugs shall be:

- a. An ANP that meets the requirements in 12VAC5-481-480 I 2; or
- b. An individual under the supervision of an ANP as specified in 12VAC5-481-1710.

4. A pharmacy, authorized under 12VAC5-481-440 H to produce PET radioactive drugs for noncommercial transfer to medical use licensees in its consortium that allows an individual to work as an ANP, shall meet the requirements of 12VAC5-481-480 I 2.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-510. Expiration and termination of licenses and decommissioning of sites and separate building or outdoor areas.

A. Except as provided in 12VAC5-481-520, a specific license shall expire at the end of the specified day in the month and year stated in the license. If an application for license renewal has been filed at least 30 days prior to the expiration date stated in the existing license and the agency denies the renewal application, the license shall expire on the date as stated in the determination of denial. If an application for license renewal is filed less than 30 days from the expiration date stated in the existing license, the agency may deny the renewal application and the license shall expire on the expiration

date stated in the license.

B. A specific license revoked by the agency expires at the end of the day on the date of the agency's final determination, or on the expiration date stated in the determination, or as otherwise provided by an agency order.

C. A specific license remains valid, with respect to possession of radioactive material, until the agency notifies the licensee in writing that the license is terminated.

While the license is valid, the licensee shall do all of the following:

1. Limit actions involving radioactive material to those related to decommissioning and other activities related to preparation for release for unrestricted use.
2. Continue to control entry to restricted areas until they are suitable for release for unrestricted use and the agency notifies the licensee in writing that the license is terminated.

D. A licensee shall do all of the following:

1. Notify the agency within 60 days of any of the following:
 - a. Expiration of the license pursuant to subsections A or B of this section.
 - b. The licensee's deciding to permanently cease principal activities at the entire site or in any separate building or outdoor area that contains residual radioactivity such that the building or outdoor area is unsuitable for release in accordance with agency requirements.
 - c. The absence of conduct of any principal activities under the license for a period of 24 months.
 - d. The absence of conduct of any principal activities for a period of 24 months in any separate building or outdoor area that contains residual radioactivity such that the building or outdoor area is unsuitable for release in accordance with agency requirements.
2. If any separate building or outdoor area contains residual radioactivity so that the building or outdoor area is unsuitable for release, do one of the following:

- a. Begin decommissioning its site, separate building or outdoor area if a decommissioning plan has been previously approved by the agency.
- b. Submit a decommissioning plan within 12 months if required by subsection F of this section and begin decommissioning upon approval of that plan.

E. Concurrent with the notification required by subsection D of this section, the licensee shall maintain in effect all decommissioning financial assurances established by the licensee pursuant to 12VAC5-481-450 C in conjunction with a license issuance or renewal or as required by this section. The amount of the financial assurance shall be increased, or may be decreased, as appropriate, to cover the detailed cost estimate for decommissioning established pursuant to subdivision H 5 of this section. Following approval of the decommissioning plan and with the agency's approval, a licensee may reduce the amount of the financial assurance as decommissioning proceeds and radiological contamination is reduced at the site.

F. A licensee shall submit a decommissioning plan to the agency if required by license condition or if the procedures and activities necessary to carry out decommissioning of the site, separate building or outdoor area have not been previously approved by the agency and the procedures and activities may adversely effect the health and safety of workers or the public. The procedures may not be carried out prior to the agency's approval of the decommissioning plan. Examples of applicable procedures and activities include any of the following cases:

1. Procedures that would involve techniques not applied routinely during cleanup or maintenance operations.
2. Procedures by which workers would be entering areas not normally occupied where surface contamination and radiation levels are significantly higher than routinely encountered during operation.
3. Procedures that could result in significantly greater airborne concentrations of radioactive materials than are present during operation.
4. Procedures that could result in significantly greater releases of radioactive material to the environment than those associated with operation.

G. The agency may approve an alternate schedule for submittal of a decommissioning plan required pursuant to subsection D of this section if the agency determines that the alternative schedule is necessary to the effective conduct of decommissioning operations and presents no undue risk from radiation to the public health and safety and is otherwise in the public interest.

H. The proposed decommissioning plan for the site or separate building or outdoor area shall include all of the following elements:

1. A description of the conditions of the site, separate building or outdoor area sufficient to evaluate the acceptability of the plan.
2. A description of planned decommissioning activities.
3. A description of methods used to ensure protection of workers and the environment against radiation hazards during decommissioning.
4. A description of the planned final radiation survey.
5. An updated detailed cost estimate for decommissioning, comparison of that estimate with present funds set aside for decommissioning, and a plan for assuring the availability of adequate funds for completion of decommissioning.
6. For decommissioning plans calling for completion of decommissioning later than 24 months after plan approval, a justification for the delay based on the criteria in subsection J of this section.

I. Except as provided in subsection H of this section, a licensee shall complete decommissioning of the site or separate building or outdoor area no later than 24 months following the initiation of decommissioning. When decommissioning involves the entire site, a licensee shall request license termination no later than 24 months following the initiation of decommissioning.

J. The agency may approve a request for an alternative schedule for completion of decommissioning of the site, separate building or outdoor area, and license termination if appropriate, if the agency determines that the alternative is warranted after consideration of all the following:

1. Whether it is technically feasible to complete decommissioning within the allotted 24-month period.
 2. Whether sufficient waste disposal capacity is available to allow completion of decommissioning within the allotted 24-month period.
 3. Whether a significant volume reduction in wastes requiring disposal will be achieved by allowing short-lived radionuclides to decay.
 4. Whether a significant reduction in radiation exposure to workers may be achieved by allowing short-lived radionuclides to decay.
 5. Other site-specific factors which the agency may consider appropriate on a case-by-case basis, such as the regulatory requirements of other government agencies, court decisions, ground-water treatment activities, monitored natural ground-water restoration, actions that could result in more environmental harm than deferred cleanup, and other factors beyond the control of the licensee.
- K. As the final step in decommissioning, a licensee shall do all the following:
1. Certify the disposition of all licensed material, including accumulated wastes, by submitting a completed agency form for disposition of radioactive materials or equivalent information.
 2. Conduct a radiation survey of the premises where the licensed activities were carried out and submit a report of the results of this survey, unless the licensee demonstrates in some other manner that the premises are suitable for release in accordance with the criteria for decommissioning in 12VAC5-481-1161.
 3. Report levels of gamma radiation in units of millisieverts (microrentgen) per hour at one meter from surfaces, and report levels of radioactivity, including alpha and beta, in units of megabecquerels per 100 square centimeters, disintegrations per minute per 100 square centimeters or microcuries per 100 square centimeters - removable and fixed - for surfaces, megabecquerels (microcuries) per milliliter for water, and becquerels (picocuries) per gram for solids such as soils or concrete.

4. Specify the survey instruments used and certify that each instrument is properly calibrated and tested.

L. The agency shall terminate a specific license, including an expired license, by written notice to the licensee when the agency determines all of the following have occurred:

1. Radioactive material has been properly disposed of.
2. Reasonable effort has been made to eliminate residual radioactive contamination, if present.
3. The licensee has filed with the agency sufficient information, including a radiation survey, to demonstrate that the premises are suitable for release in accordance with the criteria for decommissioning in 12VAC5-481-1161.
4. The licensee has submitted records required under 12VAC5-481-571 to the agency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-520. Renewal of licenses.

A. Applications for renewal of specific licenses shall be filed in accordance with 12VAC5-481-440.

B. In any case in which a licensee, not less than 30 days prior to expiration of his existing license, has filed an application in proper form for renewal or for a new license authorizing the same activities, such existing license shall not expire until final action by the agency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-530. Amendment of licenses at request of licensee.

Amendment requests for a license shall be filed in accordance with 12VAC5-481-440 and shall specify the respects in which the licensee desires the license to be amended and the grounds for such amendment.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-540. Agency action on applications to renew or amend.

In considering an application by a licensee to renew or amend the license, the agency will apply the criteria set forth in 12VAC5-481-450 through 12VAC5-481-480 and in Parts V (12VAC5-481-1170 et seq.), VII (12VAC5-481-1660 et seq.), XI (12VAC5-481-2330 et seq.), XII (12VAC5-481-2660 et seq.), XIV (12VAC5-481-3140 et seq.), or XVI (12VAC5-481-3460 et seq.) of this chapter, as applicable.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 5

Licenses Held at the Time of the Effective Date of These Regulations

12VAC5-481-550. Persons possessing a license for source, byproduct, or special nuclear material in quantities not sufficient to form a critical mass on effective date of these regulations.

Any person who, on the effective date as stated in 12VAC5-481-160, possesses a general or specific license for source, byproduct, or special nuclear material in

quantities not sufficient to form a critical mass, issued by the NRC, shall be deemed to possess a like license issued under this part and the Act, such license to expire either 90 days after receipt from the agency of a notice of expiration of such license, or on the date or expiration specified in the NRC license, whichever is earlier.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-560. Persons possessing NARM on effective date of these regulations.

Any person who, on September 20, 2006, possesses NARM for which a specific license is required by the Act or this part shall be deemed to possess such a license issued under the Act and this part. Such license shall expire 90 days after September 20, 2006; provided, however, that if within the 90 days the person possessing such material files an application in proper form for a license, such existing license shall not expire until the application has been finally determined by the agency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 6

Transfer of Material

12VAC5-481-570. Transfer of material.

A. No licensee shall transfer radioactive material except as authorized pursuant to this section.

B. Except as otherwise provided in the license and subject to the provisions of

subsections C and D of this section, any licensee may transfer radioactive material:

1. To the agency only after receiving prior approval from the agency.
2. To the United States Department of Energy;
3. To any person exempt from these regulations to the extent permitted under such exemption;
4. To any person authorized to receive such material under terms of a general license or its equivalent, or a specific license or equivalent licensing document, issued by the agency, the NRC, or another agreement state, or to any person otherwise authorized to receive such material by the federal government or any agency thereof, the agency, or another agreement state; or
5. As otherwise authorized by the agency in writing.

C. Before transferring radioactive material to a specific licensee of the agency, the NRC, or another agreement state, or to a general licensee who is required to register with the agency, the NRC, or another agreement state prior to receipt of the radioactive material, the licensee transferring the material shall verify that the transferee's license authorizes the receipt of the type, form, and quantity of radioactive material to be transferred.

D. Any of the following methods for the verification required by subsection C of this section is acceptable:

1. The transferor may possess and read a current copy of the transferee's specific license or registration certificate.
2. The transferor may possess a written certification by the transferee that the transferee is authorized by license or registration certificate to receive the type, form, and quantity of radioactive material to be transferred, specifying the license or registration certificate number, issuing agency, and expiration date.
3. For emergency shipments, the transferor may accept oral certification by the transferee that the transferee is authorized by license or registration certificate to receive the type, form, and quantity of radioactive material to be transferred,

specifying the license or registration certificate number, issuing agency, and expiration date; provided that the oral certification is confirmed in writing within 10 days.

4. The transferor may obtain other information compiled by a reporting service from official records of the agency, the NRC, or another agreement state, regarding the identity of licensees and the scope and expiration dates of licenses and registration.

5. When none of the methods of verification described in subdivisions 1 through 4 of this subsection are readily available or when a transferor desires to verify that information received by one of such methods is correct or up to date, the transferor may obtain and record confirmation from the agency, the NRC, or another agreement state, that the transferee is licensed to receive the radioactive material.

E. Shipment and transport of radioactive material shall be in accordance with the provisions of Part XIII (12VAC5-481-2950 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 7

Records

12VAC5-481-571. Receipt, transfer and disposal records.

A. Record retention. A licensee shall retain records required by 12VAC5-481-100 or by license condition. If a retention period is not otherwise specified by this chapter or license condition, the record shall be retained until the agency terminates each license.

B. Transfer of records to the agency. Prior to license termination, a licensee authorized to possess radioactive material, in an unsealed form, with a half-life greater

than 120 days, shall forward to the agency all records of disposal of licensed material made under 12VAC5-481-910 to 12VAC5-481-950, including burials authorized before January 28, 1981, and the results of measurements and calculations required by 12VAC5-481-1000.

C. Transfer of records to new licensee.

1. If licensed activities are transferred or assigned in accordance with 12VAC5-481-570, each licensee authorized to possess radioactive material in unsealed form, with a half-life greater than 120 days, shall transfer the following records to the new licensee:

a. Records of disposal of licensed material made under 12VAC5-481-910 to 12VAC5-481-950, including burials authorized before January 28, 1981.

b. Records of the results of measurements and calculations required by 12VAC5-481-1000.

2. The new licensee shall be responsible for maintaining the records required in subdivision C 1 of this section until the license is terminated.

D. Transfer of records of decommissioning activities. A licensee shall forward the records required by 12VAC5-481-450 C to the agency prior to license termination.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 8

Modification and Revocation of Licenses

12VAC5-481-580. Modification and revocation of licenses.

A. The terms and conditions of all licenses shall be subject to amendment, revision, or modification or the license may be suspended or revoked by reason of amendments to the Act, or by reason of rules, regulations, and orders issued by the agency.

B. Any license may be revoked, suspended, or modified, in whole or in part, for any

false statement in the application or any statement of fact required under provisions of the Act, or because of conditions revealed by such application or statement of fact or any report, record, or inspection or other means that would warrant the agency to refuse to grant a license on an original application, or for violation of, or failure to observe any of the terms and conditions of the Act, or of the license, or of any rule, regulation, or order of the agency.

C. Except in cases of willfulness or those in which the public health, interest or safety requires otherwise, no license shall be modified, suspended, or revoked unless, prior to the institution of proceedings therefor, facts or conduct that may warrant such action shall have been called to the attention of the licensee in writing and the licensee shall have been accorded an opportunity to demonstrate or achieve compliance with all lawful requirements.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 9

Reciprocity

12VAC5-481-590. Reciprocal recognition of licenses.

A. Licenses of byproduct, source, and special nuclear material in quantities not sufficient to form a critical mass.

1. Subject to these regulations, any person who holds a specific license from the NRC or another agreement state, and issued by the agency having jurisdiction where the licensee maintains an office for directing the licensed activity and at which radiation safety records are normally maintained, is hereby granted a general license to conduct the activities authorized in such licensing document within this state for a period not in excess of 180 days in any calendar year.

provided that:

- a. The licensing document does not limit the activity authorized by such document to specified installations or locations;
 - b. The out-of-state licensee notifies the agency in writing at least three days prior to engaging in such activity. Such notification shall indicate the location, period, and type of proposed possession and use within the state, and shall be accompanied by a copy of the pertinent licensing document. If, for a specific case, the three-day period would impose an undue hardship on the out-of-state licensee, the licensee may, upon application to the agency, obtain permission to proceed sooner. The agency may waive the requirement for filing additional written notifications during the remainder of the calendar year following the receipt of the initial notification from a person engaging in activities under the general license provided in this subdivision;
 - c. The out-of-state licensee complies with all applicable regulations of the agency and with all the terms and conditions of the licensing document, except any such terms and conditions that may be inconsistent with applicable regulations of the agency;
 - d. The out-of-state licensee supplies such other information as the agency may request; and
 - e. The out-of-state licensee shall not transfer or dispose of radioactive material possessed or used under the general license provided in this subdivision except by transfer to a person:
 - (1) Specifically licensed by the agency, the NRC or another agreement state to receive such material, or
 - (2) Exempt from the requirements for a license for such material under 12VAC5-481-400 A.
2. Notwithstanding the provisions of subdivision A 1 of this section, any person who holds a specific license issued by the NRC or another agreement state authorizing the holder to manufacture, transfer, install, or service a device

described in 12VAC5-481-430 B within areas subject to the jurisdiction of the licensing body is hereby granted a general license to install, transfer, demonstrate, or service such a device in this state provided that:

a. Such person shall file a report with the agency within 30 days after the end of each calendar quarter in which any device is transferred to or installed in this state. Each such report shall identify each general licensee to whom such device is transferred by name and address, the type of device transferred, and the quantity and type of radioactive material contained in the device;

b. The device has been manufactured, labeled, installed, and serviced in accordance with applicable provisions of the specific license issued to such person by the NRC or another agreement state;

c. Such person shall assure that any labels required to be affixed to the device under regulations of the authority which licensed manufacture of the device bear a statement that "Removal of this label is prohibited"; and

d. The holder of the specific license shall furnish to each general licensee to whom he transfers such device or on whose premises he installs such device a copy of the general license contained in 12VAC5-481-430 B or in equivalent regulations of the agency having jurisdiction over the manufacture and distribution of the device.

3. The agency may withdraw, limit, or qualify its acceptance of any specific license or equivalent licensing document issued by the NRC or another agreement state, or any product distributed pursuant to such licensing document, upon determining that such action is necessary in order to prevent undue hazard to public health and safety or property.

B. Licenses of NARM.

1. Subject to these regulations, any person who holds a specific license from the NRC or another agreement state, and issued by the agency having jurisdiction where the licensee maintains an office for directing the licensed activity and at which radiation safety records are normally maintained, is hereby granted a

general license to conduct the activities authorized in such licensing document within this state for a period not in excess of 180 days in any calendar year provided that:

- a. The licensing document does not limit the activity authorized by such document to specified installations or locations;
- b. The out-of-state licensee notifies the agency in writing at least three days prior to engaging in such activity. Such notification shall indicate the location, period, and type of proposed possession and use within the state, and shall be accompanied by a copy of the pertinent licensing document. If, for a specific case, the three-day period would impose an undue hardship on the out-of-state licensee, the licensee may, upon application to the agency, obtain permission to proceed sooner. The agency may waive the requirement for filing additional written notifications during the remainder of the calendar year following the receipt of the initial notification from a person engaging in activities under the general license provided in subdivision 1 of this subsection;
- c. The out-of-state licensee complies with all applicable regulations of the agency and with all the terms and conditions of the licensing document, except any such terms and conditions which may be inconsistent with applicable regulations of the agency;
- d. The out-of-state licensee supplies such other information as the agency may request; and
- e. The out-of-state licensee shall not transfer or dispose of radioactive material possessed or used under the general license provided in subdivision 1 of this subsection except by transfer to a person:
 - (1) Specifically licensed by the agency, the NRC or another agreement state to receive such material, or
 - (2) Exempt from the requirements for a license for such material under 12VAC5-481-400.

2. Notwithstanding the provisions of subdivision 1 of this subsection, any person who holds a specific license issued by the NRC or another agreement state authorizing the holder to manufacture, transfer, install, or service a device described in 12VAC5-481-430 B within areas subject to the jurisdiction of the licensing body is hereby granted a general license to install, transfer, demonstrate or service such a device in this state provided that:

a. Such person shall file a report with the agency within 30 days after the end of each calendar quarter in which any device is transferred to or installed in this state. Each such report shall identify each general licensee to whom such device is transferred by name and address, the type of device transferred, and the quantity and type of radioactive material contained in the device;

b. The device has been manufactured, labeled, installed, and serviced in accordance with applicable provisions of the specific license issued to such person by the NRC or another agreement state;

c. Such person shall assure that any labels required to be affixed to the device under regulations of the authority which licensed manufacture of the device bear a statement that "Removal of this label is prohibited"; and

d. The holder of the specific license shall furnish to each general licensee to whom he transfers such device or on whose premises he installs such device a copy of the general license contained in 12VAC5-481-430 B or in equivalent regulations of the agency having jurisdiction over the manufacture and distribution of the device.

3. The agency may withdraw, limit, or qualify its acceptance of any specific license or equivalent licensing document issued by the NRC or another agreement state, or any product distributed pursuant to such licensing document, upon determining that such action is necessary in order to prevent undue hazard to public health and safety or property.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part IV

Standards For Protection Against Radiation

Article 1

General Provisions

12VAC5-481-600. Purpose.

A. Part IV (12VAC5-481-600 et seq.) of this chapter establishes standards for protection against ionizing radiation resulting from activities conducted pursuant to licenses or registrations issued by the agency. These regulations are issued pursuant to the Act, as amended.

B. The requirements of Part IV (12VAC5-481-600 et seq.) of this chapter are designed to control the receipt, possession, use, transfer, and disposal of sources of radiation by any licensee or registrant so the total dose to an individual, including doses resulting from all sources of radiation other than background radiation, does not exceed the standards for protection against radiation prescribed in Part IV (12VAC5-481-600 et seq.) of this chapter. However, nothing in Part IV (12VAC5-481-600 et seq.) of this chapter shall be construed as limiting actions that may be necessary to protect health and safety in an emergency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-610. Scope.

Except as specifically provided in other parts of these regulations, Part IV (12VAC5-481-600 et seq.) of this chapter applies to persons licensed or registered by the agency to receive, possess, use, transfer, or dispose of sources of radiation. The limits in Part

IV (12VAC5-481-600 et seq.) of this chapter do not apply to doses due to background radiation, to exposure of patients to radiation for the purpose of medical diagnosis or therapy, or to voluntary participation in medical research programs.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-620. Implementation.

A. Any existing license or registration condition that is more restrictive than Part IV (12VAC5-481-600 et seq.) of this chapter remains in force until there is an amendment or renewal of the license or registration.

B. If a license or registration condition exempts a licensee or registrant from a provision of Part IV (12VAC5-481-600 et seq.) of this chapter in effect on or before September 20, 2006, it also exempts the licensee or registrant from the corresponding provision of Part IV (12VAC5-481-600 et seq.) of this chapter.

C. If a license or registration condition cites provisions of Part IV (12VAC5-481-600 et seq.) of this chapter in effect prior to September 20, 2006, which do not correspond to any provisions of Part IV (12VAC5-481-600 et seq.) of this chapter, the license or registration condition remains in force until there is an amendment or renewal of the license or registration that modifies or removes this condition.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 2

Radiation Protection Programs

12VAC5-481-630. Radiation protection programs.

The following regulation, Radiation protection programs (10 CFR 20.1101) is

applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 3

Occupational Dose Limits

12VAC5-481-640. Occupational dose limits for adults.

The following regulation, Occupational dose limits for adults (10 CFR 20.1201) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-650. Compliance with requirements for summation of external and internal doses.

The following regulation, Compliance with requirements for summation of external and internal doses (10 CFR 20.1202) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-660. Determination of external dose from airborne radioactive material.

The following regulation, Determination of external dose from airborne radioactive material (10 CFR 20.1203) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-670. Determination of internal exposure.

The following regulation, Determination of internal exposure (10 CFR 20.1204) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-680. Determination of prior occupational dose.

A. For each individual who may enter the licensee's or registrant's restricted area and is likely to receive, in a year, an occupational dose requiring monitoring pursuant to 12VAC5-481-760, the licensee or registrant shall determine the occupational radiation dose received during the current year.

B. Prior to permitting an individual to participate in a planned special exposure, the licensee or registrant shall determine:

1. The internal and external doses from all previous planned special exposures; and
2. All doses in excess of the limits, including doses received during accidents and emergencies, received during the lifetime of the individual.

C. In complying with the requirements of subsection A or B of this section, a licensee

or registrant may:

1. Accept, as a record of the occupational dose that the individual received during the current year, a written signed statement from the individual, or from the individual's most recent employer for work involving radiation exposure, that discloses the nature and the amount of any occupational dose that the individual received during the current year;
2. Accept, as the record of lifetime cumulative radiation dose, an up-to-date occupational radiation exposure form provided by the agency or equivalent, signed by the individual and countersigned by an appropriate official of the most recent employer for work involving radiation exposure, or the individual's current employer, if the individual is not employed by the licensee or registrant; and
3. Obtain reports of the individual's dose equivalent from the most recent employer for work involving radiation exposure, or the individual's current employer, if the individual is not employed by the licensee or registrant, by telephone, telegram, facsimile, or letter. The licensee or registrant shall request a written verification of the dose data if the authenticity of the transmitted report cannot be established.

D. Do the following:

1. The licensee or registrant shall record the exposure history, as required by this section on an occupational radiation exposure form provided by the agency, or other clear and legible record, of all the information required on that form. The form or record shall show each period in which the individual received occupational exposure to radiation or radioactive material and shall be signed by the individual who received the exposure. For each period for which the licensee or registrant obtains reports, the licensee or registrant shall use the dose shown in the report in preparing the occupational radiation exposure form provided by the agency or equivalent. For any period in which the licensee or registrant does not obtain a report, the licensee or registrant shall place a notation on the occupational radiation exposure form provided by the agency or equivalent

indicating the periods of time for which data are not available.

2. Licensees or registrants are not required to partition historical dose between external dose equivalent(s) and internal committed dose equivalent(s). Further, occupational exposure histories obtained and recorded on the occupational radiation exposure form provided by the agency or equivalent before September 20, 2006, might not have included effective dose equivalent, but may be used in the absence of specific information on the intake of radionuclides by the individual.

E. If the licensee or registrant is unable to obtain a complete record of an individual's current and previously accumulated occupational dose, the licensee or registrant shall assume:

1. In establishing administrative controls pursuant to 12VAC5-481-640 for the current year, that the allowable dose limit for the individual is reduced by 12.5 mSv (1.25 rem) for each quarter for which records were unavailable and the individual was engaged in activities that could have resulted in occupational radiation exposure; and

2. That the individual is not available for planned special exposures.

F. The licensee or registrant shall retain the records on an occupational radiation exposure form provided by the agency or equivalent until the agency terminates each pertinent license or registration requiring this record. The licensee or registrant shall retain records used in preparing the occupational radiation exposure form provided by the agency or equivalent for three years after the record is made.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-690. Planned special exposures.

The following regulation, Planned special exposures (10 CFR 20.1206) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-700. Occupational dose limits for minors.

The following regulation, Occupational dose limits for minors (10 CFR 20.1207) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-710. Dose to an embryo/fetus.

The following regulation, Dose to an embryo/fetus (10 CFR 20.1208) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 4

Radiation Dose Limits for Individual Members of the Public

12VAC5-481-720. Dose limits for individual members of the public.

The following regulation, Dose limits for individual members of the public (10

CFR20.1301) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-730. Compliance with dose limits for individual members of the public.

The following regulation, Compliance with dose limits for individual members of the public (10 CFR 20.1302) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 5

Testing for Leakage or Contamination of Sealed Sources

12VAC5-481-740. Testing for leakage or contamination of sealed sources.

- A. The licensee or registrant in possession of any sealed source shall assure that:
1. Each sealed source, except as specified in subsection B of this section, is tested for leakage or contamination and the test results are received before the sealed source is put into use unless the licensee or registrant has a certificate from the transferor indicating that the sealed source was tested within six months before transfer to the licensee or registrant;
 2. Each sealed source that is not designed to emit alpha particles is tested for leakage or contamination at intervals not to exceed six months or at alternative intervals approved by the agency; after evaluation of information specified by 12VAC5-481-480 J 4 and 5, the NRC or another agreement state;

3. Each sealed source that is designed to emit alpha particles is tested for leakage or contamination at intervals not to exceed three months or at alternative intervals approved by the agency, after evaluation of information specified by 12VAC5-481-480 J 4 and 5, the NRC or another agreement state;

4. For each sealed source that is required to be tested for leakage or contamination, at any other time there is reason to suspect that the sealed source might have been damaged or might be leaking, the licensee or registrant shall assure that the sealed source is tested for leakage or contamination before further use;

5. Tests for leakage for all sealed sources, except brachytherapy sources manufactured to contain radium, shall be capable of detecting the presence of 185 Bq (0.005 μ Ci) of radioactive material on a test sample. Test samples shall be taken from the sealed source or from the surfaces of the container in which the sealed source is stored or mounted on which one might expect contamination to accumulate. For a sealed source contained in a device, test samples are obtained when the source is in the "off" position;

6. The test for leakage for brachytherapy sources manufactured to contain radium shall be capable of detecting an absolute leakage rate of 37 Bq (0.001 μ Ci) of radon-222 in a 24-hour period when the collection efficiency for radon-222 and its daughters has been determined with respect to collection method, volume and time;

7. Tests for contamination from radium daughters shall be taken on the interior surface of brachytherapy source storage containers and shall be capable of detecting the presence of 185 Bq (0.005 μ Ci) of a radium daughter which has a half-life greater than four days.

B. A licensee or registrant need not perform test for leakage or contamination on the following sealed sources:

1. Sealed sources containing only radioactive material with a half-life of less than 30 days;

2. Sealed sources containing only radioactive material as a gas;
3. Sealed sources containing 3.7 MBq (100 μ Ci) or less of beta or photon-emitting material or 370 kBq (10 μ Ci) or less of alpha-emitting material;
4. Sealed sources containing only hydrogen-3;
5. Seeds of iridium-192 encased in nylon ribbon; and
6. Sealed sources that are stored, not being used and identified as in storage.

The licensee or registrant shall, however, test each such sealed source for leakage or contamination and receive the test results at intervals not to exceed five years and within six months before the date of use or transfer.

C. Tests for leakage or contamination from sealed sources shall be performed by persons specifically authorized by the agency, the NRC or another agreement state to perform such services.

D. Test results shall be kept in units of becquerel or microcurie and maintained for inspection by the agency. Records of test results for sealed sources shall be made pursuant to 12VAC5-481-1010.

E. The following shall be considered evidence that a sealed source is leaking:

1. The presence of 185 Bq (0.005 μ Ci) or more of removable contamination on any test sample;
2. Leakage of 37 Bq (0.001 μ Ci) of radon-222 per 24 hours for brachytherapy sources manufactured to contain radium;
3. The presence of removable contamination resulting from the decay of 185 Bq (0.005 μ Ci) or more of radium.

F. The licensee or registrant shall immediately withdraw a leaking sealed source from use and shall take action to prevent the spread of contamination. The leaking sealed source shall be repaired or disposed of in accordance with this part.

G. Reports of test results for leaking or contaminated sealed sources shall be made pursuant to 12VAC5-481-1150.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 6

Surveys and Monitoring

12VAC5-481-750. General.

The following regulation, (10 CFR 20.1501) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-760. Conditions requiring individual monitoring of external and internal occupational dose.

The following regulation, Conditions requiring individual monitoring of external and internal occupational dose (10 CFR 20.1502) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-770. Location of individual monitoring devices.

Each licensee or registrant shall ensure that individuals who are required to monitor occupational doses in accordance with 12VAC5-481-760 wear individual monitoring

devices as follows:

1. An individual monitoring device used for monitoring the dose to the whole body shall be worn at the unshielded location of the whole body likely to receive the highest exposure. When a protective apron is worn, the location of the individual monitoring device is typically at the neck (collar);
2. An individual monitoring device used for monitoring the dose to an embryo/fetus of a declared pregnant woman, pursuant to 12VAC5-481-710, shall be located at the waist under any protective apron being worn by the woman;
3. An individual monitoring device used for monitoring the eye dose equivalent, to demonstrate compliance with 12VAC5-481-640, shall be located at the neck (collar), outside any protective apron being worn by the monitored individual, or at an unshielded location closer to the eye;
4. An individual monitoring device used for monitoring the dose to the extremities, to demonstrate compliance with 12VAC5-481-640, shall be worn on the extremity likely to receive the highest exposure. Each individual monitoring device shall be oriented to measure the highest dose to the extremity being monitored.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 7

Control of Exposure from External Sources in Restricted Areas

12VAC5-481-780. Control of access to high radiation areas.

A. The following regulation, Control of access to high radiation areas (10 CFR 20.1601) is applicable in the Commonwealth of Virginia.

B. The licensee or registrant is not required to control entrance or access to rooms or other areas containing sources of radiation capable of producing a high radiation

area as described in this section if the licensee or registrant has met all the specific requirements for access and control specified in other applicable parts of this chapter, such as Part V (12VAC5-481-1170 et seq.) for industrial radiography, Part VI (12VAC5-481-1580 et seq.) for X-rays in the healing arts, Part IX (12VAC5-481-2140 et seq.) for particle accelerators and Part XII (12VAC5-481-2660 et seq.) for irradiators.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-790. Control of access to very high radiation areas.

A. In addition to the requirements in 12VAC5-481-780, the licensee or registrant shall institute measures to ensure that an individual is not able to gain unauthorized or inadvertent access to areas in which radiation levels could be encountered at 5 Gy (500 rad) or more in one hour at one meter from a source of radiation or any surface through which the radiation penetrates. This requirement does not apply to rooms or areas in which diagnostic X-ray systems are the only source of radiation, or to nonself-shielded irradiators.

B. The licensee or registrant is not required to control entrance or access to rooms or other areas containing sources of radiation capable of producing a very high radiation area as described in subsection A of this section if the registrant has met all the specific requirements for access and control specified in other applicable parts of these regulations, such as Part V (12VAC5-481-1170 et seq.) for industrial radiography, Part VI (12VAC5-481-1580 et seq.) for X-rays in the healing arts, Part IX (12VAC5-481-2140 et seq.) for particle accelerators, and Part XII (12VAC5-481-2660 et seq.) for irradiators.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-800. (Repealed.)

Historical Notes

Derived from Virginia Register Volume 22, Issue 25; eff. September 20, 2006; repealed, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 8

Respiratory Protection and Controls to Restrict Internal Exposure in Restricted Areas

12VAC5-481-810. Use of process or other engineering controls.

The following regulation, Use of process or other engineering controls (10 CFR 20.1701) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-820. Use of other controls.

The following regulation, Use of other controls (10 CFR 20.1702) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-830. Use of individual respiratory protection equipment.

The following regulations, Use of individual respiratory protection equipment (10 CFR 20.1703), Further restrictions on the use of respiratory protection equipment, (10

CFR 20.1704), and Applications for use of higher assigned protection factors (10 CFR 20.1705) are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 9

Security and Control of Licensed or Registered Sources of Radiation

12VAC5-481-840. Security and control of licensed or registered sources of radiation.

A. The following regulations, Security of stored materials (10 CFR 20.1801), and Control of material not in storage (10 CFR 20.1802) are applicable in the Commonwealth of Virginia.

B. The registrant shall secure registered radiation machines from unauthorized removal.

C. The registrant shall use devices or administrative procedures to prevent unauthorized use of registered radiation machines.

D. Security requirements for portable gauges. Each portable gauge licensee shall use a minimum of two independent physical controls that form tangible barriers to secure portable gauges from unauthorized removal, whenever portable gauges are not under the control and constant surveillance of the licensee.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 10

Precautionary Procedures

12VAC5-481-850. Caution signs.

The following regulation, Caution signs (10 CFR 20.1901) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-860. Posting requirements.

The following regulation, Posting requirements (10 CFR 20.1902) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-870. Exceptions to posting requirements.

The following regulation, Exceptions to posting requirements (10 CFR 20.1903) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-880. Labeling containers and radiation machines.

A. The following regulation, Labeling containers (10 CFR 20.1904) is applicable in

the Commonwealth of Virginia.

B. Each registrant shall ensure that each radiation machine is labeled in a conspicuous manner that cautions individuals that radiation is produced when it is energized.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-890. Exemptions to labeling requirements.

The following regulation, Exemptions to labeling requirements (10 CFR 20.1905) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-900. Procedures for receiving and opening packages.

The following regulation, Procedures for receiving and opening packages (10 CFR 20.1906) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 11

Waste Disposal

12VAC5-481-910. General requirements.

The following regulation, General requirements (10 CFR 20.2001) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-920. Method for obtaining approval of proposed disposal procedures.

A licensee or registrant or applicant for a license or registration may apply to the agency for approval of proposed procedures, not otherwise authorized in these regulations, to dispose of licensed or registered material generated in the licensee's or registrant's operations. Each application shall include:

1. A description of the waste containing licensed or registered material to be disposed of, including the physical and chemical properties that have an impact on risk evaluation, and the proposed manner and conditions of waste disposal;
2. An analysis and evaluation of pertinent information on the nature of the environment;
3. The nature and location of other potentially affected facilities; and
4. Analyses and procedures to ensure that doses are maintained ALARA and within the dose limits in Part IV (12VAC5-481-600 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-930. Disposal by release into sanitary sewerage.

The following regulation, Disposal by release into sanitary sewerage (10 CFR 20.2003) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-940. Treatment or disposal by incineration.

The following regulation, Treatment or disposal by incineration (10 CFR 20.2004) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-950. Disposal of specific wastes.

The following regulation, Disposal of specific wastes (10 CFR 20.2005) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-960. Transfer for disposal and manifests.

The following regulation, Transfer for disposal and manifests (10 CFR 20.2006) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-970. Compliance with environmental and health protection regulations.

The following regulation, Compliance with environmental and health protection regulations (10 CFR 20.2007) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-971. Disposal of certain byproduct material.

The following regulation, Disposal of certain byproduct material (10 CFR 20.2008) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 12

Records

12VAC5-481-980. General provisions.

The following regulation, General Provisions (10 CFR 20.2101) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-990. Records of radiation protection programs.

The following regulation, Records of radiation protection programs (10 CFR 20.2102) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1000. Records of surveys.

The following regulation, Records of surveys (10 CFR 20.2103) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1010. Records of tests for leakage or contamination of sealed sources.

Records of tests for leakage or contamination of sealed sources (required by 12VAC5-481-740) shall be kept in units of becquerel or microcurie and maintained for five years after the records are made.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1020. Records of prior occupational dose.

The licensee or registrant shall retain the records of prior occupational dose and exposure history as specified in 12VAC5-481-680 on an occupational radiation exposure form provided by the agency or equivalent until the agency terminates each pertinent license or registration requiring this record. The licensee or registrant shall retain records used in preparing an occupational radiation exposure form provided by the agency or equivalent for three years after the record is made.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1030. Records of planned special exposures.

The following regulation, Records of planned special exposures (10 CFR 20.2105) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1040. Records of individual monitoring results.

The following regulation, Records of individual monitoring results (10 CFR 20.2106) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1050. Records of dose to individual members of the public.

A. Each licensee or registrant shall maintain records sufficient to demonstrate compliance with the dose limit for individual members of the public per 12VAC5-481-720.

B. The licensee or registrant shall retain the records required by subsection A of this section until the agency terminates each pertinent license or registration requiring the record.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1060. Records of waste disposal.

A. Each licensee or registrant shall maintain records of the disposal of licensed or registered materials made pursuant to 12VAC5-481-920 through 12VAC5-481-950, Part XI (12VAC5-481-2330 et seq.) of this chapter, and disposal by burial in soil, including burials authorized before, September 1, 1980, of the rule that removed the authorization.

B. The licensee or registrant shall retain the records required by subsection A of this section until the agency terminates each pertinent license or registration requiring the record.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1070. Records of testing entry control devices for very high radiation areas.

A. Each licensee or registrant shall maintain records of tests made on entry control devices for very high radiation areas. These records must include the date, time, and results of each such test of function.

B. The licensee or registrant shall retain the records required by subsection A of this section for three years after the record is made.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1080. Form of records.

Each record required by Part IV (12VAC5-481-600 et seq.) of this chapter shall be legible throughout the specified retention period. The record shall be the original or a reproduced copy or a microform, provided that the copy or microform is authenticated by authorized personnel and that the microform is capable of producing a clear copy throughout the required retention period or the record may also be stored in electronic media with the capability for producing legible, accurate, and complete records during the required retention period. Records, such as letters, drawings, and specifications, shall include all pertinent information, such as stamps, initials, and signatures. The licensee shall maintain adequate safeguards against tampering with and loss of records.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Reports

12VAC5-481-1090. Reports of stolen, lost, or missing licensed or registered sources of radiation.

A. Telephone reports. Each licensee or registrant shall report to the agency by telephone as follows:

1. Immediately after its occurrence becomes known to the licensee or registrant, stolen, lost, or missing licensed or registered radioactive material in an aggregate quantity equal to or greater than 1,000 times the quantity specified in 12VAC5-481-3700 under such circumstances that it appears to the licensee or registrant that an exposure could result to individuals in unrestricted areas;
2. Within 30 days after its occurrence becomes known to the licensee or registrant, lost, stolen, or missing licensed or registered radioactive material in an aggregate quantity greater than 10 times the quantity specified in 12VAC5-481-3700 that is still missing; or
3. Immediately after its occurrence becomes known to the registrant, a stolen, lost, or missing radiation machine.

B. Written reports. Each licensee or registrant required to make a report pursuant to subsection A of this section shall, within 30 days after making the telephone report, make a written report to the agency setting forth the following information:

1. A description of the licensed or registered source of radiation involved, including, for radioactive material, the kind, quantity, and chemical and physical form; and, for radiation machines, the manufacturer, model and serial number, type and maximum energy of radiation emitted;
2. A description of the circumstances under which the loss or theft occurred;
3. A statement of disposition, or probable disposition, of the licensed or registered source of radiation involved;
4. Exposures of individuals to radiation, circumstances under which the exposures occurred, and the possible total effective dose equivalent to persons

in unrestricted areas;

5. Actions that have been taken, or will be taken, to recover the source of radiation; and

6. Procedures or measures that have been, or will be, adopted to ensure against a recurrence of the loss or theft of licensed or registered sources of radiation.

C. Subsequent to filing the written report, the licensee or registrant shall also report additional substantive information on the loss or theft within 30 days after the licensee or registrant learns of such information.

D. The licensee or registrant shall prepare any report filed with the agency pursuant to this section so that names of individuals who may have received exposure to radiation are stated in a separate and detachable portion of the report.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1100. Notification of incidents.

The following regulation, Notification of incidents (10 CFR 20.2202) is applicable in the Commonwealth of Virginia, and notifications are made by telephone to the agency during normal business hours at (804) 864-8150, and after business hours to the State Emergency Operations Center (804) 674-2400.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1110. Reporting requirements.

The following regulations, Reports of exposures, radiation levels, and concentrations

of radioactive material exceeding the constraints or limits (10 CFR 20.2203 (a) and (b)) and Reporting requirements (10 CFR 30.50, 10 CFR 40.60, and 10 CFR 70.50(a) (b)(c)) are applicable in the Commonwealth of Virginia, and reports are submitted to the agency at the following address: 109 Governor Street, Room 730, Richmond, VA 23219.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1120. Reports of planned special exposures.

The licensee or registrant shall submit a written report to the agency within 30 days following any planned special exposure conducted in accordance with 12VAC5-481-690, informing the agency that a planned special exposure was conducted and indicating the date the planned special exposure occurred and the information required by 12VAC5-481-1030.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1130. Reports of individual monitoring.

A. This section applies to each person licensed or registered by the agency to:

1. Possess or use sources of radiation for purposes of industrial radiography pursuant to Parts III (12VAC5-481-380 et seq.) and V (12VAC5-481-1170 et seq.) of this chapter; or
2. Receive radioactive waste from other persons for disposal pursuant to Part XI (12VAC5-481-2330 et seq.) of this chapter; or
3. Possess or use at any time, for processing or manufacturing for distribution

pursuant to Part III (12VAC5-481-380 et seq.) or VII (12VAC5-481-1660 et seq.) of this chapter, radioactive material in quantities exceeding any one of the following quantities:

Radionuclide	Activity ^a	
	GBq	Ci
Cesium-137	37	1
Cobalt-60	37	1
Gold-98	3,700	100
Iodine-131	37	1
Iridium-192	270	10
Krypton-85	37,000	1,000
Promethium-147	370	10
Technecium-99m	37,000	1,000

^aThe agency may require as a license condition, or by rule, regulation, or an order pursuant to 12VAC5-481-190, reports from licensees or registrants who are licensed or registered to use radionuclides not on this list, in quantities sufficient to cause comparable radiation levels.

B. Each licensee or registrant in a category listed in subsection A of this section shall submit an annual report of the results of individual monitoring carried out by the licensee or registrant for each individual for whom monitoring was required by 12VAC5-481-760 during that year. The licensee or registrant may include additional data for individuals for whom monitoring was provided but not required. The licensee or registrant shall use the agency's record of individual monitoring results form or equivalent or electronic media containing all the information required by the agency's record of individual monitoring results form.

C. The licensee or registrant shall file the report required by subsection B of this section, covering the preceding year, on or before April 30 of each year. The licensee or registrant shall submit the report to the agency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1140. Notifications and reports to individuals.

A. Requirements for notification and reports to individuals of exposure to radiation or radioactive material are specified in 12VAC5-481-2280.

B. When a licensee or registrant is required pursuant to 12VAC5-481-1110 to report to the agency any exposure of an individual to radiation or radioactive material, the licensee or registrant shall also notify the individual. Such notice shall be transmitted at a time not later than the transmittal to the agency, and shall comply with the provisions of 12VAC5-481-2280 A.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1150. Reports of leaking or contaminated sealed sources.

The licensee or registrant shall file a report within five days with the agency if the test for leakage or contamination required pursuant to 12VAC5-481-740 indicates a sealed source is leaking or contaminated. The report shall include the equipment involved, the test results and the corrective action taken.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1151. Reports of transactions involving nationally tracked sources.

A. Each licensee who manufactures a nationally tracked source shall complete and submit a National Source Tracking Transaction Report. The report must include the following information:

1. The name, address, and license number of the reporting licensee;
2. The name of the individual preparing the report;

3. The manufacturer, model, and serial number of the source;
4. The radioactive material in the source;
5. The initial source strength in becquerels (curies) at the time of manufacture; and
6. The manufacture date of the source.

B. Each licensee that transfers a nationally tracked source to another person shall complete and submit a National Source Tracking Transaction Report. The report must include the following information:

1. The name, address, and license number of the reporting licensee;
2. The name of the individual preparing the report;
3. The name and license number of the recipient facility and the shipping address;
4. The manufacturer, model, and serial number of the source or, if not available, other information to uniquely identify the source;
5. The radioactive material in the source;
6. The initial or current source strength in becquerels (curies);
7. The date for which the source strength is reported;
8. The shipping date;
9. The estimated arrival date; and
10. For nationally tracked sources transferred as waste under a Uniform Low-Level Radioactive Waste Manifest, the waste manifest number and the container identification of the container with the nationally tracked source.

C. Each licensee that receives a nationally tracked source shall complete and submit a National Source Tracking Transaction Report. The report must include the following information:

1. The name, address, and license number of the reporting licensee;
2. The name of the individual preparing the report;

3. The name, address, and license number of the person that provided the source;
4. The manufacturer, model, and serial number of the source or, if not available, other information to uniquely identify the source;
5. The radioactive material in the source;
6. The initial or current source strength in becquerels (curies);
7. The date for which the source strength is reported;
8. The date of receipt; and
9. For material received under a Uniform Low-Level Radioactive Waste Manifest, the waste manifest number and the container identification with the nationally tracked source.

D. Each licensee that disassembles a nationally tracked source shall complete and submit a National Source Tracking Transaction Report. The report must include the following information:

1. The name, address, and license number of the reporting licensee;
2. The name of the individual preparing the report;
3. The manufacturer, model, and serial number of the source or, if not available, other information to uniquely identify the source;
4. The radioactive material in the source;
5. The initial or current source strength in becquerels (curies);
6. The date for which the source strength is reported; and
7. The disassemble date of the source.

E. Each licensee who disposes of a nationally tracked source shall complete and submit a National Source Tracking Transaction Report. The report must include the following information:

1. The name, address, and license number of the reporting licensee;
2. The name of the individual preparing the report;

3. The waste manifest number;
4. The container identification with the nationally tracked source;
5. The date of disposal; and
6. The method of disposal.

F. The reports discussed in subsections A through E of this section must be submitted by the close of the next business day after the transaction. A single report may be submitted for multiple sources and transactions. The reports must be submitted to the National Source Tracking System by using:

1. The online National Source Tracking System;
2. Electronically using a computer-readable format;
3. By facsimile;
4. By mail to the address on the National Source Tracking Transaction Report Form (NRC Form 748); or
5. By telephone with followup by facsimile or mail.

G. Each licensee shall correct any error in previously filed reports or file a new report for any missed transaction within five business days of the discovery of the error or missed transaction. Such errors may be detected by a variety of methods such as administrative reviews or by physical inventories required by regulation. In addition, each licensee shall reconcile the inventory of nationally tracked sources possessed by the licensee against that licensee's data in the National Source Tracking System. The reconciliation must be conducted during the month of January in each year. The reconciliation process must include resolving any discrepancies between the National Source Tracking System and the actual inventory by filing the reports identified by subsections A through E of this section. By January 31 of each year, each licensee must submit to the National Source Tracking System confirmation that the data in the National Source Tracking System is correct.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 14

Additional Requirements

12VAC5-481-1160. (Repealed.)

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; repealed, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1161. Radiological criteria for license termination.

A. General provisions and applicability.

1. This part applies to the decommissioning of facilities licensed under this chapter.
2. This part does not apply to sites that:
 - a. Have been decommissioned before the effective date as stated in 12VAC5-481-160; or
 - b. Have previously submitted and received NRC's approval on a license termination plan or decommissioning plan.
3. After a site has been decommissioned and the license terminated according to this section, the agency shall require additional cleanup only if, based on new information, the agency determines that the criteria of this part were not met and residual radioactivity remaining at the site could result in a significant threat to public health and safety.
4. When calculating the Total Effective Dose Equivalent (TEDE) to the average member of the critical group, the licensee must determine the peak annual TEDE expected within the first 1,000 years after decommissioning.

B. Radiological criteria for unrestricted use. A site is considered acceptable for unrestricted use if the residual radioactivity that is distinguishable from background radiation results in a TEDE to an average member of the critical group that does not

exceed 0.25 mSv (25 mrem) per year, including that from groundwater sources of drinking water; and the residual radioactivity has been reduced to levels that are ALARA. Determination of levels that are ALARA must take into account consideration of any detriments, such as deaths from transportation accidents, expected to potentially result from decontamination and waste disposal.

C. Criteria for termination under restricted conditions. A site is considered acceptable for license termination under restricted conditions, if the licensee:

1. Can demonstrate that further reductions in residual radioactivity necessary to comply with subsection B of this section would result in net public or environmental harm or are not being made because the residual levels associated with restricted conditions are ALARA. Determination of the levels that are ALARA must take into account consideration of any detriments, such as traffic accidents, expected to potentially result from decontamination and waste disposal;

2. Has made provisions for legally enforceable institutional controls that provide reasonable assurance that the TEDE from residual radioactivity, distinguishable from background radiation, will not exceed 0.25 mSv (25 mrem) per year to the average member of the critical group;

3. Has provided sufficient financial assurance to enable an independent third party, including a governmental custodian of a site, to assume and carry out responsibilities for any necessary control and maintenance of the site.

Acceptable financial assurance mechanisms are:

- a. Funds placed into an account segregated from the licensee's assets and outside the licensee's administrative control as described under 12VAC5-481-450 C 7 a;

- b. Surety method, insurance, or other guarantee method as described under part 12VAC5-481-450 C 7 b;

- c. A statement of intent, in the case of federal, state, or local government licensees, as described in 12VAC5-481-450 C 7 d; or

- d. When a governmental entity is assuming custody and ownership of a site, an arrangement that is deemed acceptable by the governmental entity;
4. Has submitted a decommissioning plan or a license termination plan to the agency indicating the licensee's intent to decommission according to 12VAC5-481-510 and specifying that the licensee intends to decommission by restricting use of the site. The licensee must document in the license termination plan or decommissioning plan how the advice of individuals and institutions in the community has been sought according to subdivisions 5 and 6 of this subsection and incorporated, as appropriate, following analysis of that advice;
5. If proposing to decommission by restricting use of the site, seeks advice from individuals and institutions in the community who may be affected by the decommissioning regarding whether:
 - a. Institutional controls proposed by the licensee:
 - (1) Will provide reasonable assurance that the TEDE from residual radioactivity distinguishable from background radiation to the average member of the critical group will not exceed 0.25 mSv (25 mrem) TEDE per year;
 - (2) Will be enforceable; and
 - (3) Will not impose undue burdens on the local community or other affected parties; and
 - b. The licensee has provided sufficient financial assurance to enable an independent third party, including a governmental custodian of a site, to assume and carry out responsibilities for any necessary control and maintenance of the site;
6. While seeking advice under subdivision 5 of this subsection, provides for:
 - a. Participation by representatives of a broad cross section of community interests who may be affected by the decommissioning;
 - b. An opportunity for a comprehensive, collective discussion on the issues by

the participants represented; and

c. A publicly available summary of the results of all such discussions, including a description of the individual viewpoints of the participants on the issues and the extent of agreement and disagreement among the participants on the issues; and

7. Reduces residual radioactivity at the site so that if the institutional controls were no longer in effect, there is reasonable assurance that the TEDE from residual radioactivity distinguishable from background radiation to the average member of the critical group is ALARA and would not exceed:

a. 1 mSv (100 mrem) per year; or

b. 5 mSv (500 mrem) per year, if the licensee:

(1) Demonstrates that further reductions in residual radioactivity necessary to comply with subdivision C 7 a of this section are not technically achievable, would be prohibitively expensive, or would result in net public or environmental harm;

(2) Makes provisions for durable institutional controls; and

(3) Provides sufficient financial assurance, according to subdivision C 3 of this section, to enable a responsible governmental entity or independent third party, including a governmental custodian of a site, to carry out periodic rechecks of the site no less frequently than every five years to ensure that the institutional controls remain in place as necessary to meet the criteria of subdivision C 2 of this section, and to assume and carry out responsibilities for any necessary control and maintenance of those controls.

D. Alternative criteria for license termination.

1. The agency may terminate a license using alternative criteria greater than the dose criterion of subsection B and subdivision C 5 a (1) of this section, if the licensee:

a. Provides assurance that public health and safety would continue to be

protected and that it is unlikely that the dose from all manmade sources combined, other than medical, would be more than the 1 mSv (100 mrem) per year limit under 12VAC5-481-720, by submitting an analysis of possible sources of exposure;

b. Employs, to the extent practical, restrictions on site use according to subsection C of this section, in minimizing exposures at the site;

c. Reduces doses to ALARA levels, taking into consideration any detriments, such as traffic accidents, expected to potentially result from decontamination and waste disposal; and

d. Submits a decommissioning plan or license termination plan to the agency indicating the licensee's intent to decommission according to 12VAC5-481-510, and specifying that the licensee proposes to decommission by use of alternate criteria. The licensee must document in the decommissioning plan or license termination plan how the advice of individuals and institutions in the community who may be affected by the decommissioning has been sought and addressed, as appropriate, following analysis of that advice. In seeking such advice, the licensee must provide for:

(1) Participation by representatives of a broad cross section of community interests who may be affected by the decommissioning;

(2) An opportunity for a comprehensive, collective discussion on the issues by the participants represented; and

(3) A publicly available summary of the results of all such discussions, including a description of the individual viewpoints of the participants on the issues and the extent of agreement and disagreement among the participants on the issues.

2. The use of alternate criteria to terminate a license requires the approval of the agency after consideration of staff recommendations of the agency that address any comments provided by federal, state and local governments and any public comments submitted pursuant under subsection E of this section.

E. Public notification and public participation. Upon receipt of a license termination plan or decommissioning plan from a licensee or a proposal by a licensee for release of a site according to subsection C or D of this section, or whenever the agency deems such notice to be in the public interest, the agency must:

1. Notify and solicit comments from:

a. Local and state governments in the vicinity of the site and any Indian Nation or other indigenous people that have treaty or statutory rights that could be affected by the decommissioning; and

b. The US Environmental Protection Agency and Virginia Department of Environmental Quality for cases when the licensee proposes to release a site according to subsection D of this section; and

2. Publish a notice in the State Register and in a forum, such as local newspapers, letters to state and local organizations, or other appropriate forum, that is readily accessible to individuals in the vicinity of the site and solicit comments from affected parties.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part V

Radiation Safety Requirements For Industrial Radiographic Operations

Article 1

General Requirements

12VAC5-481-1170. Purpose.

This part prescribes requirements for the issuance of licenses or registrations for the industrial use of sources of radiation and radiation safety requirements for persons using these sources of radiation in industrial radiography.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1180. Scope.

The provisions and requirements of this part are in addition to, and not in substitution for, other requirements of these regulations. In particular, the general requirements and provisions of Parts I (12VAC5-481-10 et seq.); II (12VAC5-481-260 et seq.); III (12VAC5-481-380 et seq.); IV (12VAC5-481-600 et seq.); X (12VAC5-481-2250 et seq.) and XIII (12VAC5-481-2950 et seq.), of this chapter apply to applicants, licensees and registrants subject to this part. Parts III (12VAC5-481-380 et seq.) and XIII (12VAC5-481-2950 et seq.) of this chapter apply to licensing and transportation of radioactive material and Part II (12VAC5-481-260 et seq.) of this chapter applies to the registration of radiation machines. Except for sections that are applicable only to sealed radioactive sources, radiation machines and sealed radioactive sources are both covered by this part. This regulation does not apply to medical uses of sources of radiation that are addressed in Parts VII (12VAC5-481-1660 et seq.) and XV (12VAC5-481-3380 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1190. Exemptions.

A. Uses of certified and certifiable cabinet X-ray systems are exempt from the requirements of this part except for 12VAC5-481-1200 and the following:

1. For certified and certifiable cabinet X-ray systems, including those designed to allow admittance of individuals:

- a. No registrant shall permit any individual to operate a cabinet X-ray system until the individual has received a copy of and instruction in the operating

procedures for the unit. Records that demonstrate compliance with this subdivision shall be maintained for agency inspection until disposal is authorized by the agency.

b. Tests for proper operation of interlocks must be conducted and recorded at intervals not to exceed six months. Records of these tests shall be maintained for agency inspection until disposal is authorized by the agency.

c. The registrant shall perform an evaluation of the radiation dose limits to determine compliance with 12VAC5-481-720 and 21 CFR 1020.40, Cabinet X-ray Systems, at intervals not to exceed one year. Records of these evaluations shall be maintained for agency inspection for two years after the evaluation.

2. Certified cabinet X-ray systems shall be maintained in compliance with 21 CFR 1020.40, Cabinet X-ray Systems, and no modification shall be made to the system unless prior agency approval has been granted.

B. Industrial uses of hand-held light intensified imaging devices are exempt from the requirements of exceed 0.2 mSv (2 mrem) per hour. Devices that exceed this limit shall meet the applicable requirements of this part and the licensing or registration requirements of Part II (12VAC5-481-260 et seq.) or Part III (12VAC5-481-380 et seq.) of this chapter, as applicable.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1200. Licensing and registration requirements for industrial radiography operations.

A. The agency will approve an application for a specific license for the use of licensed material or a registration for use of radiation machines if the applicant meets

the following requirements:

1. The applicant satisfies the general requirements specified in Part II (12VAC5-481-260 et seq.) for radiation machine facilities or Part III (12VAC5-481-380 et seq.) for radioactive material, as applicable, and any special requirements contained in this part;
2. The applicant submits an adequate program for training radiographers and radiographer's assistants that meets the requirements of 12VAC5-481-1320;
3. The applicant submits procedures for verifying and documenting the certification status of radiographers and for ensuring that the certification of individuals acting as radiographers remains valid;
4. The applicant submits written operating and emergency procedures as described in 12VAC5-481-1330;
5. The applicant submits a description of a program for inspections of the job performance of each radiographer and radiographer's assistant at intervals not to exceed six months as described in 12VAC5-481-1320 E;
6. The applicant submits a description of the applicant's overall organizational structure as it applies to the radiation safety responsibilities in industrial radiography, including specified delegation of authority and responsibility;
7. The applicant submits the qualifications of the individual(s) designated as the radiation safety officer as described in 12VAC5-481-1310 A 1;
8. If an applicant intends to perform leak testing of sealed sources or exposure devices containing depleted uranium (DU) shielding, the applicant must describe the procedures for performing the test. The description must include the:
 - a. Methods of collecting the samples;
 - b. Qualifications of the individual who analyzes the samples;
 - c. Instruments to be used; and
 - d. Methods of analyzing the samples;
9. If the applicant intends to perform calibrations of survey instruments and

alarming ratemeters, the applicant must describe methods to be used and the experience of the person(s) who will perform the calibrations. All calibrations must be performed according to the procedures described and at the intervals prescribed in 12VAC5-481-1240 and 12VAC5-481-1350 G 4;

10. The applicant identifies and describes the location(s) of all field stations and permanent radiographic installations;

11. The applicant identifies the location(s) where all records required by this and other parts of these regulations will be maintained;

12. If a license application includes underwater radiography, a description of:

a. Radiation safety procedures and radiographer responsibilities unique to the performance of underwater radiography;

b. Radiographic equipment and radiation safety equipment unique to underwater radiography; and

c. Methods for gas-tight encapsulation of equipment; and

13. If an application includes offshore platform and/or lay-barge radiography, a description of:

a. Transport procedures for radioactive material to be used in industrial radiographic operations;

b. Storage facilities for radioactive material; and

c. Methods for restricting access to radiation areas.

B. A license or registration will be issued if the requirements of subsection A of this section, as applicable, are met.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1210. Performance requirements for industrial radiography

equipment.

A. Equipment used in industrial radiographic operations must meet the following minimum criteria:

Each radiographic exposure device, source assembly or sealed source, and all associated equipment must meet the requirements specified in American National Standard Institute, N432-1980 "Radiological Safety for the Design and Construction of Apparatus for Gamma Radiography," (published as NBS Handbook 136, issued January 1981);

B. In addition to the requirements specified in this section the following requirements apply to radiographic exposure devices, source changers, source assemblies and sealed sources;

1. The licensee shall ensure that each radiographic exposure device has attached to it a durable, legible, clearly visible label bearing the:

- a. Chemical symbol and mass number of the radionuclide in the device;
- b. Activity and the date on which this activity was last measured;
- c. Model or product code and serial number of the sealed source;
- d. Name of the manufacturer of the sealed source; and
- e. Licensee's name, address, and telephone number.

2. Radiographic exposure devices intended for use as Type B packages must meet the applicable transportation requirements of Part XIII (12VAC5-481-2950 et seq.) of this chapter.

3. Modification of radiographic exposure devices, source changers, and source assemblies and associated equipment is prohibited, unless approved by the agency or other approval body.

C. In addition to the requirements specified in subsections A and B of this section, the following requirements apply to radiographic exposure devices, source assemblies, and associated equipment that allow the source to be moved out of the device for radiographic operations or to source changers;

1. The coupling between the source assembly and the control cable must be designed in such a manner that the source assembly will not become disconnected if cranked outside the guide tube. The coupling must be such that it cannot be unintentionally disconnected under normal and reasonably foreseeable abnormal conditions.
2. The device must automatically secure the source assembly when it is cranked back into the fully shielded position within the device. This securing system may only be released by means of a deliberate operation on the exposure device.
3. The outlet fittings, lock box, and drive cable fittings on each radiographic exposure device must be equipped with safety plugs or covers that must be installed during storage and transportation to protect the source assembly from water, mud, sand or other foreign matter.
4. Each sealed source or source assembly must have attached to it or engraved on it, a durable, legible, visible label with the words:

"DANGER—RADIOACTIVE."

The label may not interfere with the safe operation of the exposure device or associated equipment.

5. The guide tube must be able to withstand a crushing test that closely approximates the crushing forces that are likely to be encountered during use, and be able to withstand a kinking resistance test that closely approximates the kinking forces that are likely to be encountered during use.
6. Guide tubes must be used when moving the source out of the device.
7. An exposure head or similar device designed to prevent the source assembly from passing out of the end of the guide tube must be attached to the outermost end of the guide tube during industrial radiography operations.
8. The guide tube exposure head connection must be able to withstand the tensile test for control units specified in ANSI N432-1980.
9. Source changers must provide a system for ensuring that the source will not

be accidentally withdrawn from the changer when connecting or disconnecting the drive cable to or from a source assembly.

D. All radiographic exposure devices and associated equipment in use after January 10, 1996, must comply with the requirements of this section; and

E. As an exception to subsection A of this section, equipment used in industrial radiographic operations need not comply with 8.9.2(c) of the Endurance Test in American National Standards Institute N432-1980, if the prototype equipment has been tested using a torque value representative of the torque that an individual using the radiography equipment can reasonably exert on the lever or crankshaft of the drive mechanism.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1220. Limits on external radiation levels from storage containers and source changers.

The maximum exposure rate limits for storage containers and source changers are 2 mSv (200 mrem) per hour at any exterior surface, and 0.1 mSv (10 mrem) per hour at one meter from any exterior surface with the sealed source in the shielded position.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1230. Locking of sources of radiation, storage containers and source changers.

A. Each radiographic exposure device must have a lock or outer locked container designed to prevent unauthorized or accidental removal of the sealed source from its

shielded position. The exposure device and/or its container must be kept locked, and if a keyed-lock, with the key removed at all times, when not under the direct surveillance of a radiographer or a radiographer's assistant except at permanent radiographic installations as stated in 12VAC5-481-1370. In addition, during radiographic operations the sealed source assembly must be secured in the shielded position each time the source is returned to that position.

B. Each sealed source storage container and source changer must have a lock or outer locked container designed to prevent unauthorized or accidental removal of the sealed source from its shielded position. Storage containers and source changers must be kept locked, and if a keyed-lock, with the key removed at all times, when containing sealed sources except when under the direct surveillance of a radiographer or a radiographer's assistant.

C. The control panel of each radiation machine shall be equipped with a lock that will prevent the unauthorized use of an X-ray system or the accidental production of radiation. The radiation machine shall be kept locked and the key removed at all times except when under the direct visual surveillance of a radiographer or a radiographer's assistant.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1240. Radiation survey instruments.

A. The licensee or registrant shall keep sufficient calibrated and operable radiation survey instruments at each location where sources of radiation are present to make the radiation surveys required by this part and by Part IV (12VAC5-481-600 et seq.) of this chapter. Instrumentation required by this section must be capable of measuring a range from 0.02 mSv (2 mrem) per hour through 0.01 Sv (1 rem) per hour.

B. The licensee or registrant shall have each radiation survey instrument required under subsection A of this section calibrated:

1. At energies appropriate for use and at intervals not to exceed six months or after instrument servicing, except for battery changes;
2. For linear scale instruments, at two points located approximately one-third and two-thirds of full-scale on each scale; for logarithmic scale instruments, at mid-range of each decade, and at two points of at least one decade; and for digital instruments, at three points between 0.02 and 10 mSv (2 and 1000 mrem) per hour; and
3. So that an accuracy within plus or minus 20% of the true radiation dose rate can be demonstrated at each point checked.

C. The licensee or registrant shall maintain records of the results of the instrument calibrations in accordance with 12VAC5-481-1410.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1250. Leak testing and replacement of sealed sources.

A. The replacement of any sealed source fastened to or contained in a radiographic exposure device and leak testing of any sealed source must be performed by persons authorized to do so by the agency, the NRC, or another agreement state.

B. The opening, repair, or modification of any sealed source must be performed by persons specifically authorized to do so by the agency, the NRC, or another agreement state.

C. Testing and recordkeeping requirements.

1. Each licensee who uses a sealed source shall have the source tested for leakage at intervals not to exceed six months. The leak testing of the source

must be performed using a method approved by the agency, the NRC, or by another agreement state. The wipe sample should be taken from the nearest accessible point to the sealed source where contamination might accumulate. The wipe sample must be analyzed for radioactive contamination. The analysis must be capable of detecting the presence of 185 Bq (0.005 μ Ci) of radioactive material on the test sample and must be performed by a person specifically authorized by the agency, the NRC, or another agreement state to perform the analysis.

2. The licensee shall maintain records of the leak tests in accordance with 12VAC5-481-1420.

3. Unless a sealed source is accompanied by a certificate from the transferor that shows that it has been leak tested within six months before the transfer, it may not be used by the licensee until tested for leakage. Sealed sources that are in storage and not in use do not require leak testing, but must be tested before use or transfer to another person if the interval of storage exceeds six months.

D. Any test conducted pursuant to subsections B and C of this section that reveals the presence of 185 Bq (0.005 μ Ci) or more of removable radioactive material must be considered evidence that the sealed source is leaking. The licensee shall immediately withdraw the equipment involved from use and shall have it decontaminated and repaired or disposed of in accordance with agency regulations. A report must be filed with the agency within five days of any test with results that exceed the threshold in this paragraph, describing the equipment involved, the test results, and the corrective action taken.

E. Each exposure device using depleted uranium (DU) shielding and an "S" tube configuration must be tested for DU contamination at intervals not to exceed 12 months. The analysis must be capable of detecting the presence of 185 Bq (0.005 μ Ci) of radioactive material on the test sample and must be performed by a person specifically authorized by the agency, the NRC, or another agreement state to perform the analysis. Should such testing reveal the presence of DU contamination, the exposure device

must be removed from use until an evaluation of the wear of the S-tube has been made. Should the evaluation reveal that the S-tube is worn through, the device may not be used again. DU shielded devices do not have to be tested for DU contamination while not in use and in storage. Before using or transferring such a device, however, the device must be tested for DU contamination, if the interval of storage exceeds 12 months. A record of the DU leak test must be made in accordance with 12VAC5-481-1420.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1260. Quarterly inventory.

A. Each licensee or registrant shall conduct a quarterly physical inventory to account for all sources of radiation, and for devices containing depleted uranium received and possessed under the license.

B. The licensee or registrant shall maintain records of the quarterly inventory in accordance with 12VAC5-481-1430.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1270. Inspection and maintenance of radiation machines, radiographic exposure devices, transport and storage containers, associated equipment, source changers, and survey instruments.

A. The licensee or registrant shall perform visual and operability checks on survey meters, radiation machines, radiographic exposure devices, transport and storage containers, associated equipment and source changers before each day's use, or work

shift, to ensure that:

1. The equipment is in good working condition;
2. The sources are adequately shielded; and
3. Required labeling is present.

B. Survey instrument operability must be performed using check sources or other appropriate means.

C. If equipment problems are found, the equipment must be removed from service until repaired.

D. Each licensee or registrant shall have written procedures for and perform inspection and routine maintenance of radiation machines, radiographic exposure devices, source changers, associated equipment, transport and storage containers, and survey instruments at intervals not to exceed three months or before the first use thereafter to ensure the proper functioning of components important to safety. If equipment problems are found, the equipment must be removed from service until repaired. Replacement components shall meet design requirements.

E. The licensee's inspection and maintenance program must include procedures to assure that Type B packages are shipped and maintained in accordance with the certificate of compliance or other approval.

F. Records of equipment problems and of any maintenance performed under this section must be made in accordance with 12VAC5-481-1450.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1280. Permanent radiographic installations.

A. Each entrance that is used for personnel access to the high radiation area in a permanent radiographic installation must have either:

1. An entrance control of the type described in 12VAC5-481-780 that causes the radiation level upon entry into the area to be reduced; or
2. Both conspicuous visible and audible warning signals to warn of the presence of radiation. The visible signal must be actuated by radiation whenever the source is exposed or the machine is energized. The audible signal must be actuated when an attempt is made to enter the installation while the source is exposed or the machine is energized.

B. The alarm system must be tested for proper operation with a radiation source each day before the installation is used for radiographic operations. The test must include a check of both the visible and audible signals. Entrance control devices that reduce the radiation level upon entry as designated in subdivision A 1 of this section must be tested monthly. If an entrance control device or an alarm is operating improperly, it must be immediately labeled as defective and repaired within seven calendar days. The facility may continue to be used during this seven-day period, provided the licensee or registrant implements the continuous surveillance requirements of 12VAC5-481-1370 and uses an alarming ratemeter. Test records for entrance controls and audible and visual alarms must be maintained in accordance with 12VAC5-481-1460.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1290. Labeling, storage, and transportation.

A. The licensee may not use a source changer or a container to store radioactive material unless the source changer or the storage container has securely attached to it a durable, legible, and clearly visible label bearing the standard trefoil radiation caution symbol conventional colors, i.e., magenta, purple or black on a yellow background, having a minimum diameter of 25 mm, and the wording:

CAUTION *

RADIOACTIVE MATERIAL

NOTIFY CIVIL AUTHORITIES (or "NAME OF COMPANY")

* ———or "DANGER"

B. The licensee may not transport radioactive material unless the material is packaged, and the package is labeled, marked, and accompanied with appropriate shipping papers in accordance with regulations set out in Part XIII (12VAC5-481-2950 et seq.) of this chapter.

C. Radiographic exposure devices, source changers, storage containers, and radiation machines, must be physically secured to prevent tampering or removal by unauthorized personnel. The licensee shall store radioactive material in a manner that will minimize danger from explosion or fire.

D. The licensee shall lock and physically secure the transport package containing radioactive material in the transporting vehicle to prevent accidental loss, tampering, or unauthorized removal.

E. The licensee's or registrant's name and city or town where the main business office is located shall be prominently displayed with a durable, clearly visible label(s) on both sides of all vehicles used to transport radioactive material or radiation machines for temporary job site use.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 2

Radiation Safety Requirements

12VAC5-481-1300. Conducting industrial radiographic operations.

A. Whenever radiography is performed at a location other than a permanent radiographic installation, the radiographer must be accompanied by at least one other

qualified radiographer or an individual who has at a minimum met the requirements of 12VAC5-481-1320 C. The additional qualified individual shall observe the operations and be capable of providing immediate assistance to prevent unauthorized entry. Radiography may not be performed if only one qualified individual is present.

B. All radiographic operations must be conducted in a permanent radiographic installation unless otherwise specifically authorized by the agency.

C. Except when physically impossible, collimators shall be used in industrial radiographic operations that use radiographic exposure devices that allow the source to be moved out of the device.

D. A licensee or registrant may conduct lay-barge, offshore platform, or underwater radiography only if procedures have been approved by the agency, the NRC, or by another agreement state.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1310. Radiation safety officer.

A. The radiation safety officer shall ensure that radiation safety activities are being performed in accordance with approved procedures and regulatory requirements in the daily operation of the licensee's or registrant's program.

B. The minimum qualifications, training, and experience for radiation safety officers for industrial radiography are as follows:

1. Completion of the training and testing requirements of 12VAC5-481-1320 A;
2. 2000 hours of hands-on experience as a qualified radiographer in industrial radiographic operations; and
3. Formal training in the establishment and maintenance of a radiation protection program.

C. The agency will consider alternatives when the radiation safety officer has appropriate training and experience in the field of ionizing radiation, and in addition, has adequate formal training with respect to the establishment and maintenance of a radiation safety protection program.

D. The specific duties and authorities of the radiation safety officer include:

1. Establishing and overseeing all operating, emergency, and ALARA procedures as required by Part IV (12VAC5-481-600 et seq.) of this chapter and reviewing them regularly to ensure that they conform to agency regulations and to the license or registration conditions;
2. Overseeing and approving the training program for radiographic personnel to ensure that appropriate and effective radiation protection practices are taught;
3. Ensuring that required radiation surveys and leak tests are performed and documented in accordance with the regulations, including any corrective measures when levels of radiation exceed established limits;
4. Ensuring that personnel monitoring devices are calibrated, if applicable, and used properly; that records are kept of the monitoring results; and that timely notifications are made as required by Part IV of this chapter; and
5. Ensuring that operations are conducted safely and for implementing corrective actions including terminating operations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1320. Training.

A. The licensee or registrant may not permit any individual to act as a radiographer until the individual has received at least 40 hours of training in the subjects outlined in subsection G of this section in addition to on the job training consisting of hands-on

experience under the supervision of a radiographer and is certified through a radiographer certification program by a certifying entity meeting the requirements of 10 CFR Part 34, Appendix A. The on-the-job training shall include a minimum of two months (320 hours) of active participation in the performance of industrial radiography utilizing radioactive material and/or one month (160 hours) of active participation in the performance of industrial radiography utilizing radiation machines. Individuals performing industrial radiography utilizing radioactive materials and radiation machines must complete both segments of the on-the-job training (3 months or 480 hours).

B. In addition, the licensee or registrant may not permit any individual to act as a radiographer until the individual:

1. Has received copies of and instruction in the requirements described in the regulations contained in this part, 12VAC5-481-30 and applicable sections of Parts IV (12VAC5-481-600 et seq.), X (12VAC5-481-2250 et seq.), and XIII (12VAC5-481-2950 et seq.) of this chapter, in the license or registration under which the radiographer will perform industrial radiography, and the licensee's or registrant's operating and emergency procedures;
2. Has demonstrated an understanding of items in subdivision 1 of this subsection by successful completion of a written examination;
3. Has received training in the use of the registrant's radiation machines, or the licensee's radiographic exposure devices, sealed sources, in the daily inspection of devices and associated equipment, and in the use of radiation survey instruments; and
4. Has demonstrated understanding of the use of the equipment described in subdivision 3 of this subsection by successful completion of a practical examination.

C. The licensee or registrant may not permit any individual to act as a radiographer's assistant until the individual:

1. Has received copies of and instruction in the requirements described in the regulations contained in this part, 12VAC5-481-30 and applicable sections of

Parts IV (12VAC5-481-600 et seq.), X (12VAC5-481-2250 et seq.), and XIII (12VAC5-481-2950 et seq.) of this chapter, in the license or registration under which the radiographer's assistant will perform industrial radiography, and the licensee's or registrant's operating and emergency procedures;

2. Has demonstrated an understanding of items in subdivision 1 of this subsection by successful completion of a written examination;

3. Under the personal supervision of a radiographer, has received training in the use of the registrant's radiation machines, or the licensee's radiographic exposure devices and sealed sources, in the daily inspection of devices and associated equipment, and in the use of radiation survey instruments; and

4. Has demonstrated understanding of the use of the equipment described in subdivision 3 of this subsection by successful completion of a practical examination.

D. The licensee or registrant shall provide annual refresher safety training for each radiographer and radiographer's assistant at intervals not to exceed 12 months.

E. Except as provided in subdivision 4 of this subsection, the RSO or designee shall conduct an inspection program of the job performance of each radiographer and radiographer's assistant to ensure that the agency's regulations, license or registration requirements, and operating and emergency procedures are followed. The inspection program must:

1. Include observation of the performance of each radiographer and radiographer's assistant during an actual industrial radiographic operation, at intervals not to exceed six months;

2. Provide that, if a radiographer or a radiographer's assistant has not participated in an industrial radiographic operation for more than six months since the last inspection, the radiographer must demonstrate knowledge of the training requirements of subdivision B 3 of this section and the radiographer's assistant must demonstrate knowledge of the training requirements of subdivision C 3 of this section by a practical examination before these individuals

can next participate in a radiographic operation;

3. The agency may consider alternatives in those situations where the individual serves as both radiographer and radiation safety officer; and

4. In those operations where a single individual serves as both radiographer and radiation safety officer, and performs all radiography operations, an inspection program is not required;

F. The licensee or registrant shall maintain records of the above training to include certification documents, written and practical examinations, refresher safety training and inspections of job performance in accordance with 12VAC5-481-1470.

G. The licensee or registrant shall include the following subjects required in subsection A of this section:

1. Fundamentals of radiation safety including:

- a. Characteristics of gamma and x-radiation;
- b. Units of radiation dose and quantity of radioactivity;
- c. Hazards of exposure to radiation;
- d. Levels of radiation from sources of radiation; and
- e. Methods of controlling radiation dose (time, distance, and shielding);

2. Radiation detection instruments including:

- a. Use, operation, calibration, and limitations of radiation survey instruments;
- b. Survey techniques; and
- c. Use of personnel monitoring equipment;

3. Equipment to be used including:

- a. Operation and control of radiographic exposure equipment, remote handling equipment, and storage containers, including pictures or models of source assemblies (pigtailed);
- b. Operation and control of radiation machines;
- c. Storage, control, and disposal of sources of radiation; and

- d. Inspection and maintenance of equipment.
4. The requirements of pertinent state and federal regulations; and
5. Case histories of accidents in radiography.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1330. Operating and emergency procedures.

A. Operating and emergency procedures must include, as a minimum, instructions in the following:

1. Appropriate handling and use of sources of radiation so that no person is likely to be exposed to radiation doses in excess of the limits established in Part IV (12VAC5-481-600 et seq.) of this chapter;
2. Methods and occasions for conducting radiation surveys;
3. Methods for posting and controlling access to radiographic areas;
4. Methods and occasions for locking and securing sources of radiation;
5. Personnel monitoring and the use of personnel monitoring equipment;
6. Transporting equipment to field locations, including packing of radiographic exposure devices and storage containers in the vehicles, placarding of vehicles when required, and control of the equipment during transportation as described in Part XIII (12VAC5-481-2950 et seq.) of this chapter;
7. The inspection, maintenance, and operability checks of radiographic exposure devices, radiation machines, survey instruments, alarming ratemeters, transport containers, and storage containers;
8. Steps that must be taken immediately by radiography personnel in the event a pocket dosimeter is found to be off-scale or an alarming ratemeter alarms

unexpectedly;

9. The procedure(s) for identifying and reporting defects and noncompliance, as required by 12VAC5-481-1530;

10. The procedure for notifying proper persons in the event of an accident or incident;

11. Minimizing exposure of persons in the event of an accident or incident, including a source disconnect, a transport accident, or loss of a source of radiation;

12. Source recovery procedure if licensee will perform source recoveries; and

13. Maintenance of records.

B. The licensee or registrant shall maintain copies of current operating and emergency procedures in accordance with 12VAC5-481-1480 and 12VAC5-481-1520.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1340. Supervision of radiographer's assistants.

The radiographer's assistant shall be under the personal supervision of a radiographer when using sources of radiation or conducting radiation surveys required by subdivision 2 of 12VAC5-481-1360 to determine that the sealed source has returned to the shielded position or the radiation machine is off after an exposure. The personal supervision must include:

1. The radiographer's physical presence at the site where the sources of radiation are being used;

2. The availability of the radiographer to give immediate assistance if required; and

3. The radiographer's direct observation of the assistant's performance of the operations referred to in this section.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1350. Personnel monitoring.

A. The licensee or registrant may not permit any individual to act as a radiographer or a radiographer's assistant unless, at all times during radiographic operations, each individual wears, on the trunk of the body, a combination of direct reading dosimeter, an alarming ratemeter, and either a film badge, an optically stimulated luminescence (OSL) dosimeter or a thermoluminescent dosimeter (TLD). At permanent radiographic installations where other appropriate alarming or warning devices are in routine use, or during radiographic operations using radiation machines, the use of an alarming ratemeter is not required.

1. Pocket dosimeters must have a range from 0 to 2 mSv (200 mrem) and must be recharged at the start of each shift. Electronic personal dosimeters may only be used in place of ion-chamber pocket dosimeters.
2. Each film badge, OSL or TLD must be assigned to and worn by only one individual.
3. Film badges must be exchanged monthly. OSLs or TLDs must be exchanged at periods not to exceed three months.
4. After replacement, each film badge, OSL or TLD must be returned to the supplier for processing within 14 calendar days of the end of the monitoring period, or as soon as practicable. In circumstances that make it impossible to return each film badge, OSL or TLD in 14 calendar days, such circumstances must be documented and available for review by the agency.

B. Direct reading dosimeters, such as pocket dosimeters or electronic personal dosimeters, must be read and the exposures recorded at the beginning and end of each shift, and records must be maintained in accordance with 12VAC5-481-1490.

C. Pocket dosimeters, or electronic personal dosimeters, must be checked at periods not to exceed 12 months for correct response to radiation, and records must be maintained in accordance with 12VAC5-481-1490. Acceptable dosimeters must read within plus or minus 20% of the true radiation exposure.

D. If an individual's pocket dosimeter is found to be off-scale, or the electronic personal dosimeter reads greater than 2 mSv (200 mrem), the individual's film badge, OSL or TLD must be sent for processing within 24 hours. In addition, the individual may not resume work associated with the use of sources of radiation until a determination of the individual's radiation exposure has been made. This determination must be made by the radiation safety officer or the radiation safety officer's designee. The results of this determination must be included in the records maintained in accordance with 12VAC5-481-1490.

E. If a film badge, OSL or TLD is lost or damaged, the worker shall cease work immediately until a replacement film badge, OSL or TLD is provided and the exposure is calculated for the time period from issuance to loss or damage of the film badge, OSL or TLD. The results of the calculated exposure and the time period for which the film badge, OSL or TLD was lost or damaged must be included in the records maintained in accordance with 12VAC5-481-1490.

F. Reports received from the film badge, OSL or TLD processor must be retained in accordance with 12VAC5-481-1490.

G. Each alarming ratemeter must:

1. Be checked to ensure that the alarm functions properly before using at the start of each shift;
2. Be set to give an alarm signal at a preset dose rate of 5 mSv (500 mrem) per hour with an accuracy of plus or minus 20% of the true radiation dose rate;
3. Require special means to change the preset alarm function; and
4. Be calibrated at periods not to exceed 12 months for correct response to radiation. The licensee shall maintain records of alarming ratemeter calibrations

in accordance with 12VAC5-481-1490.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1360. Radiation surveys.

The licensee or registrant shall:

1. Conduct all surveys with a calibrated and operable radiation survey instrument that meets the requirements of 12VAC5-481-1240;
2. Conduct a survey of the radiographic exposure device and the guide tube after each exposure when approaching the device or the guide tube. The survey must determine that the sealed source has returned to its shielded position before exchanging films, repositioning the exposure head, or dismantling equipment. Radiation machines shall be surveyed after each exposure to determine that the machine is off;
3. Conduct a survey of the radiographic exposure device whenever the source is exchanged and whenever a radiographic exposure device is placed in a storage area, as defined in 12VAC5-481-10, to ensure that the sealed source is in its shielded position; and
4. Maintain records in accordance with 12VAC5-481-1500.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1370. Surveillance.

During each radiographic operation, the radiographer shall ensure continuous direct visual surveillance of the operation to protect against unauthorized entry into a radiation

area or a high radiation area, as defined in Part I (12VAC5-481-10 et seq.) of this chapter, except at permanent radiographic installations where all entryways are locked and the requirements of 12VAC5-481-1280 are met.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1380. Posting.

All areas in which industrial radiography is being performed must be conspicuously posted as required by 12VAC5-481-860. The exceptions listed in 12VAC5-481-870 do not apply to industrial radiographic operations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 3

Recordkeeping Requirements

12VAC5-481-1390. Records for industrial radiography.

Each licensee or registrant shall maintain a copy of its license or registration, documents incorporated by reference, and amendments to each of these items until superseded by new documents approved by the agency, or until the agency terminates the license or registration.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1400. Records of receipt and transfer of sources of radiation.

A. Each licensee or registrant shall maintain records showing the receipts and transfers of sealed sources, devices using DU for shielding, and radiation machines, and retain each record for three years after it is made.

B. These records must include the date, the name of the individual making the record, radionuclide, number of becquerels (curies) or mass (for DU), and manufacturer, model, and serial number of each source of radiation and/or device, as appropriate.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1410. Records of radiation survey instruments.

Each licensee or registrant shall maintain records of the calibrations of its radiation survey instruments that are required under 12VAC5-481-1240 and retain each record for three years after it is made.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1420. Records of leak testing of sealed sources and devices containing DU.

Each licensee shall maintain records of leak test results for sealed sources and for devices containing DU. The results must be stated in units of becquerels (microcuries). The licensee shall retain each record for three years after it is made or until the source in storage is removed.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1430. Records of quarterly inventory.

A. Each licensee or registrant shall maintain records of the quarterly inventory of sources of radiation, including devices containing depleted uranium as required by 12VAC5-481-1260, and retain each record for three years.

B. The record must include the date of the inventory, name of the individual conducting the inventory, radionuclide, number of becquerels (curies) or mass (for DU) in each device, location of sources of radiation and/or devices, and manufacturer, model, and serial number of each source of radiation and/or device, as appropriate.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1440. Utilization logs.

A. Each licensee or registrant shall maintain utilization logs showing for each source of radiation the following information:

1. A description, including the make, model, and serial number of the radiation machine or the radiographic exposure device, transport, or storage container in which the sealed source is located;
2. The identity and signature of the radiographer to whom assigned;
3. The location and dates of use, including the dates removed and returned to storage; and
4. For permanent radiographic installations, the dates each radiation machine is energized.

B. The licensee or registrant shall retain the logs required by subsection A of this section for three years.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1450. Records of inspection and maintenance of radiation machines, radiographic exposure devices, transport and storage containers, associated equipment, source changers, and survey instruments.

A. Each licensee or registrant shall maintain records specified in 12VAC5-481-1270 of equipment problems found in daily checks and quarterly inspections of radiation machines, radiographic exposure devices, transport and storage containers, associated equipment, source changers, and survey instruments, and retain each record for three years after it is made.

B. The record must include the date of check or inspection, name of inspector, equipment involved, any problems found, and what repair and/or maintenance, if any, was performed.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1460. Records of alarm system and entrance control checks at permanent radiographic installations.

Each licensee or registrant shall maintain records of alarm system and entrance control tests required by 12VAC5-481-1280 and retain each record for three years after it is made.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1470. Records of training and certification.

Each licensee or registrant shall maintain the following records for three years:

1. Records of training of each radiographer and each radiographer's assistant.

The record must include radiographer certification documents and verification of certification status, copies of written tests, dates of oral and practical examinations, the names of individuals conducting and receiving the oral and practical examinations, and a list of items tested and the results of the oral and practical examinations; and

2. Records of annual refresher safety training and semi-annual inspections of job performance for each radiographer and each radiographer's assistant. The records must list the topics discussed during the refresher safety training, the dates the annual refresher safety training was conducted, and names of the instructors and attendees. For inspections of job performance, the records must also include a list showing the items checked and any noncompliance observed by the radiation safety officer or designee.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1480. Copies of operating and emergency procedures.

Each licensee or registrant shall maintain a copy of current operating and emergency procedures until the agency terminates the license or registration.

Superseded material must be retained for three years after the change is made.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1490. Records of personnel monitoring.

Each licensee or registrant shall maintain the following exposure records specified in 12VAC5-481-1350:

1. Direct reading dosimeter readings and yearly operability checks required by 12VAC5-481-1350 B and 12VAC5-481-1350 C for three years after the record is made;
2. Records of alarming ratemeter calibrations for three years after the record is made;
3. Reports received from the film badge, OSL or TLD processor until the agency terminates the license or registration; and
4. Records of estimates of exposures as a result of off-scale personal direct reading dosimeters, or lost or damaged film badges, OSL or TLD's, until the agency terminates the license or registration.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1500. Records of radiation surveys.

Each licensee shall maintain a record of each exposure device survey conducted before the device is placed in storage as specified in subdivision 3 of 12VAC5-481-1360. Each record must be maintained for three years after it is made.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1510. Form of records.

Each record required by this part must be legible throughout the specified retention period. The record may be the original or a reproduced copy or a microform provided that the copy or microform is authenticated by authorized personnel and that the microform is capable of reproducing a clear copy throughout the required retention period. The record may also be stored in electronic media with the capability for producing legible, accurate, and complete records during the required retention period. Records, such as letters, drawings, and specifications, must include all pertinent information, such as stamps, initials, and signatures. The licensee or registrant shall maintain adequate safeguards against tampering with and loss of records.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1520. Location of documents and records.

A. Each licensee or registrant shall maintain copies of records required by this part and other applicable parts of these regulations at the location specified in 12VAC5-481-1200 A 11.

B. Each licensee or registrant shall also maintain current copies of the following documents and records sufficient to demonstrate compliance at each applicable field station and each temporary jobsite;

1. The license or registration authorizing the use of sources of radiation;
2. A copy of Parts I (12VAC5-481-10 et seq.); IV (12VAC5-481-600 et seq.); V (12VAC5-481-1170 et seq.); and X (12VAC5-481-2250 et seq.) of this chapter;
3. Utilization logs for each source of radiation dispatched from that location as required by 12VAC5-481-1440.
4. Records of equipment problems identified in daily checks of equipment as required by 12VAC5-481-1450 A;
5. Records of alarm system and entrance control checks required by 12VAC5-

481-1460, if applicable;

6. Records of dosimeter readings as required by 12VAC5-481-1490;

7. Operating and emergency procedures as required by 12VAC5-481-1480;

8. Evidence of the latest calibration of the radiation survey instruments in use at the site, as required by 12VAC5-481-1410;

9. Evidence of the latest calibrations of alarming ratemeters and operability checks of dosimeters as required by 12VAC5-481-1490;

10. Survey records as required by 12VAC5-481-1500 and 12VAC5-481-1000 as applicable, for the period of operation at the site;

11. The shipping papers for the transportation of radioactive materials required by Part XIII (12VAC5-481-2950 et seq.) of this chapter; and

12. When operating under reciprocity pursuant to Part III (12VAC5-481-380 et seq.) of this chapter, a copy of the applicable state license or registration, or NRC license authorizing the use of sources of radiation.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 4

Notifications

12VAC5-481-1530. Notifications.

A. In addition to the reporting requirements specified in 10 CFR 30.50 and in Part IV (12VAC5-481-600 et seq.) of this chapter, each licensee or registrant shall provide a written report to the agency within 30 days of the occurrence of any of the following incidents involving radiographic equipment:

1. Unintentional disconnection of the source assembly from the control cable;

2. Inability to retract the source assembly to its fully shielded position and secure

it in this position;

3. Failure of any component, which is critical to safe operation of the device, to properly perform its intended function; or

4. An indicator on a radiation machine fails to show that radiation is being produced, an exposure switch fails to terminate production of radiation when turned to the off position, or a safety interlock fails to terminate X-ray production.

B. The licensee or registrant shall include the following information in each report submitted under subsection A of this section, and in each report of overexposure submitted under 12VAC5-481-1110 that involves failure of safety components of radiography equipment:

1. Description of the equipment problem;

2. Cause of each incident, if known;

3. Name of the manufacturer and model number of equipment involved in the incident;

4. Place, date, and time of the incident;

5. Actions taken to establish normal operations;

6. Corrective actions taken or planned to prevent recurrence; and

7. Names and qualifications of personnel involved in the incident.

C. Any licensee or registrant conducting radiographic operations or storing sources of radiation at any location not listed on the license or registration for a period in excess of 180 days in a calendar year, shall notify the agency prior to exceeding the 180 days.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 5

Jobsite Requirements

12VAC5-481-1540. (Repealed.)

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; repealed, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1550. (Repealed.)

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; repealed, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1560. Reciprocity.

A. All reciprocal recognition of licenses and registrations by the agency will be granted in accordance with Part III (12VAC5-481-380 et seq.) of this chapter.

B. Reciprocal recognition by the agency of an individual radiographer certification will be granted provided that:

1. The individual holds a valid certification in the appropriate category issued by a certifying entity, as defined in 12VAC5-481-10;
2. The requirements and procedures of the certifying entity issuing the certification affords the same or comparable certification standards as those afforded by 12VAC5-481-1320 A;
3. The applicant presents the certification to the agency prior to entry into the state; and
4. No escalated enforcement action is pending with the NRC or in any other agreement state.

C. Certified individuals who are granted reciprocity by the agency shall maintain the certification upon which the reciprocal recognition was granted, or prior to the expiration of such certification, shall meet the requirements of 12VAC5-481-1320 A.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1570. Specific requirements for radiographic personnel performing industrial radiography.

A. At a job site, the following shall be supplied by the licensee or registrant:

1. At least one operable, calibrated survey instrument for each exposure device or radiation machine in use;
2. A current whole body personnel monitor (TLD, OSL or film badge) for each person performing radiographic operations;
3. An operable, calibrated pocket dosimeter with a range of 0 to 2 mSv (200 mrem) for each person performing radiographic operations;
4. An operable, calibrated, alarming ratemeter for each person performing radiographic operations using a radiographic exposure device; and
5. The appropriate barrier ropes and signs.

B. Each radiographer at a job site shall have on their person a valid certification ID card issued by a certifying entity.

C. Industrial radiographic operations shall not be performed if any of the items in subsections A and B of this section are not available at the job site or are inoperable.

D. During an inspection, the agency may terminate an operation if any of the items in subsections A and B of this section are not available or operable, or if the required number of radiographic personnel are not present. Operations shall not be resumed until all required conditions are met.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part VI

Use Of Diagnostic X-Rays In The Healing Arts

12VAC5-481-1580. Purpose and scope.

This part establishes requirements, for which a registrant is responsible, for use of diagnostic X-ray equipment by, or under the supervision of, an individual authorized by and licensed in accordance with state statutes to engage in the healing arts or veterinary medicine. The provisions of this part are in addition to, and not in substitution for, other applicable provisions of Parts I (12VAC5-481-10 et seq.); II (12VAC5-481-260 et seq.); IV (12VAC5-481-600 et seq.); and X (12VAC5-481-2250 et seq.) of this chapter. Some registrants may also be subject to the requirements of Parts IX (12VAC5-481-2140 et seq.) and XV (12VAC5-481-3380 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1590. General and administrative requirements.

A. Radiation safety requirements. The registrant shall be responsible for directing the operation of the X-ray system(s) under his administrative control. The registrant or the registrant's agent shall assure that the requirements of these regulations are met in the operation of the X-ray system(s).

1. An X-ray system that does not meet the provisions of these regulations shall not be operated for diagnostic purposes.
2. Individuals who will be operating the X-ray systems shall be adequately instructed in the safe operating procedures and be competent in the safe use of the equipment. The agency may use interview, observation and/or testing to determine compliance. The following are areas in which the agency considers it important that an individual have expertise for the competent operation of X-ray equipment:

a. Familiarization with equipment

- (1) Identification of controls
- (2) Function of each control
- (3) How to use a technique chart

b. Radiation protection

- (1) Collimation
- (2) Filtration
- (3) Gonad shielding and other patient protection devices, if used
- (4) Restriction of X-ray tube radiation to the image receptor
- (5) Personnel protection
- (6) Grids

c. Image processing

- (1) Film speed as related to patient exposure
- (2) Image processing parameters
- (3) Quality assurance program

d. Emergency procedures—termination of exposure in event of automatic timing device failure

e. Proper use of personnel dosimetry, if required

f. Understanding units of radiation

3. A chart shall be provided in the vicinity of the diagnostic X-ray system's control panel that specifies, for all examinations performed with that system, the following information:

- a. Patient's body part and anatomical size, or body part thickness, or age (for pediatrics), versus technique factors to be utilized;
- b. Reserved;
- c. Reserved;
- d. Source to image receptor distance to be used (except for dental intra-oral

radiography);

e. Type and location of placement of patient shielding (e.g., gonad, etc.) to be used; and

f. For mammography, indication of kVp/target/filter combination.

4. The registrant of a facility shall create and make available to X-ray operators written safety procedures, including patient holding and any restrictions of the operating technique required for the safe operation of the particular X-ray system. The operator shall be able to demonstrate familiarity with these procedures. A copy of the written safety procedures shall be posted near each X-ray machine.

5. Except for patients who cannot be moved out of the room, only the staff, ancillary personnel or other persons required for the medical procedure or training shall be in the room during the radiographic exposure. Other than the patient being examined:

a. All individuals shall be positioned such that no part of the body will be struck by the useful beam unless protected by not less than 0.5 millimeter lead equivalent material;

b. The X-ray operator, other staff, ancillary personnel, and other persons required for the medical procedure shall be protected from the direct scatter radiation by protective aprons or whole body protective barriers of not less than 0.25 millimeter lead equivalent material;

c. Human patients who cannot be removed from the room shall be protected from the direct scatter radiation by whole body protective barriers, or protective aprons of not less than 0.25 millimeter lead equivalent material or shall be so positioned that the nearest portion of the body is at least two meters from both the tube head and the nearest edge of the image receptor.

6. Gonad shielding of not less than 0.5 millimeter lead equivalent material shall be used for human patients, who have not passed the reproductive age, during radiographic procedures in which the gonads are in the useful beam, except for

cases in which this would interfere with the diagnostic procedure.

7. Individuals shall not be exposed to the useful beam except for healing arts purposes and unless such exposure has been authorized by a licensed practitioner of the healing arts. This provision specifically prohibits deliberate exposure for the following purposes:

- a. Exposure of an individual for training, demonstration, or other nonhealing arts purposes; and
- b. Exposure of an individual for the purpose of healing arts screening except as authorized by subdivision A 11 of this section.

8. When a patient or film must be provided with auxiliary support during a radiation exposure:

- a. Mechanical holding devices shall be used when the technique permits. The written safety procedures, required by subdivision A 4 of this section, shall list individual projections where holding devices cannot be utilized;
- b. Written safety procedures, as required by subdivision A 4 of this section, shall indicate the requirements for selecting a holder and the procedure the holder shall follow;
- c. The human holder shall be instructed in personal radiation safety and protected as required by subdivision A 5 of this section;
- d. No individual shall be used routinely to hold film or patients;
- e. In those cases where the patient must hold the film, except during intraoral examinations, any portion of the body other than the area of clinical interest struck by the useful beam shall be protected by not less than 0.5 millimeter lead equivalent material; and
- f. Each facility shall have leaded aprons and gloves available in sufficient numbers to provide protection to all personnel who are involved with X-ray operations and who are otherwise not shielded.
- g. When an animal must be held in position during radiography, mechanical

supporting or restraining devices should be used. If the animal must be held by an individual, that individual shall be protected by appropriate shielding devices, such as protective glove and apron, and he shall be so positioned that no part of his body will be struck by the useful beam. The radiation exposure of and individual used for this purpose shall be monitored and recorded. These records of radiation exposure must be maintained indefinitely for inspection by the agency.

9. Procedures and auxiliary equipment designed to minimize patient and personnel exposure commensurate with the needed diagnostic information shall be utilized.

a. The speed of the screen and film combinations used shall be the fastest speed consistent with the diagnostic objective of the examinations. Film cassettes without intensifying screens shall not be used for any routine diagnostic radiological imaging, with the exception of veterinary radiography and standard film packets for intra-oral use in dental radiography.

b. The radiation exposure to the patient shall be the minimum exposure required to produce images of good diagnostic quality and, where applicable, shall not exceed the following standards:

EXPOSURE LIMITS FOR SELECTED PROJECTIONS

Using a method acceptable to the agency, the exposure measurement shall be determined in the center of the X-ray field at the location of the entrance skin of a standard patient, except for dental intraoral X-ray machines in which case the measurement shall be determined at the conetip. The technique factors selected shall be those used for routine radiography for an average size adult patient at that facility for that X-ray machine. At least one projection must be tested for each X-ray machine unless none of the projections listed are used. If an X-ray machine is used in both the manual and phototimed modes, then only the manual mode shall be tested. If the machine is used only in the phototimed mode, then this test is not required. An average size adult, for purposes of these regulations, is defined as a 5'8", 164 lb. adult male

meeting the following anthropometric guidelines for the radiographic examination projection specified: PA Chest—Thorax—23 cm thickness; AP Abdomen and AP Lumbar Spine—Abdomen—23 cm thickness.

The exposure shall not exceed the following maximum exposure limits for the projections below:

Projection	Maximum Exposure
------------	------------------

PA Chest	50 mR
AP Lumbar Spine	1400 mR
AP Abdomen	1100 mR

Dental Bitewing

Using D Speed Film

50 kVp	575 mR
55 kVp	500 mR
60 kVp	440 mR
65 kVp	400 mR
70 kVp	350 mR
75 kVp	260 mR
80 kVp	230 mR
85 kVp	200 mR
90 kVp	180 mR
95 kVp	160 mR

100 kVp

140 mR

Using E Speed Film

50 kVp	320 mR
55 kVp	270 mR
60 kVp	230 mR
65 kVp	200 mR
70 kVp	170 mR
75 kVp	140 mR
80 kVp	120 mR
85 kVp	105 mR
90 kVp	90 mR
95 kVp	80 mR
100 kVp	70 mR

c. Portable or mobile X-ray equipment shall be used only for examinations where it is impractical to transfer the patient(s) to a stationary X-ray installation.

d. X-ray systems subject to 12VAC5-481-1620 shall not be utilized in procedures where the source to patient distance is less than 30 centimeters, except for veterinary systems.

e. If grids are used between the patient and the image receptor to decrease scatter to the film and improve contrast, the grid shall:

- (1) Be positioned properly, i.e., tube side facing the right direction, and grid centered to the central ray;
- (2) If of the focused type, be of the proper focal distance for the SID's being

used.

10. All individuals who are associated with the operation of an X-ray system are subject to the requirements of 12VAC5-481-640, 12VAC5-481-680, 12VAC5-481-700 and 12VAC5-481-710.

11. Healing arts screening. Any person proposing to conduct a healing arts screening program shall not initiate such a program without prior approval of the agency. When requesting such approval, that person shall submit the following information. If any information submitted to the agency becomes invalid or outdated, the agency shall be immediately notified.

INFORMATION TO BE SUBMITTED BY PERSONS PROPOSING TO CONDUCT
HEALING ARTS SCREENING

Persons requesting that the agency approve a healing arts screening program shall submit the following information and evaluation:

- a. Name and address of the applicant and, where applicable, the names and addresses of agents within this state;
- b. Diseases or conditions for which the X-ray examinations are to be used in diagnoses;
- c. A detailed description of the X-ray examinations proposed in the screening program;
- d. Description of the population to be examined in the screening program, i.e., age, sex, physical condition, and other appropriate information;
- e. An evaluation of any known alternate methods not involving ionizing radiation that could achieve the goals of the screening program and why these methods are not used instead of the X-ray examinations;
- f. An evaluation by a private inspector of the X-ray system(s) to be used in the screening program. The evaluation by the private inspector shall show that such system(s) do satisfy all requirements of these regulations. The evaluation shall include a measurement of patient exposures from the X-ray

examinations to be performed;

g. A description of the diagnostic X-ray quality control program;

h. A copy of the technique chart for the X-ray examination procedures to be used;

i. The qualifications of each individual who will be operating the X-ray system (s);

j. The qualifications of the individual who will be supervising the operators of the X-ray system(s). The extent of supervision and the method of work performance evaluation shall be specified;

k. The name and address of the individual who will interpret the radiograph(s);

l. A description of the procedures to be used in advising the individuals screened and their private practitioners of the healing arts of the results of the screening procedure and any further medical needs indicated;

m. A description of the procedures for the retention or disposition of the radiographs and other records pertaining to the X-ray examinations;

n. An indication of the frequency of screening and the duration of the entire screening program.

12. Information and maintenance record and associated information. The registrant shall maintain the following information for each X-ray system for inspection by the agency:

a. Model and serial numbers of all major components, and user's manuals for those components;

b. Tube rating charts and cooling curves;

c. Records of surveys, calibrations, maintenance, and modifications performed on the X-ray system(s); and

d. A copy of all correspondence with this agency regarding that X-ray system.

13. X-ray utilization log. Except for veterinary facilities, each facility shall maintain a record containing the patient's name, the type of examinations, and the dates

the examinations were performed. When the patient or film must be provided with human auxiliary support, the name of the human holder shall be recorded.

14. The registrant shall maintain a list of X-ray machine operators for each facility. The following information will be maintained on the list:

The name of the X-ray machine operator. Operators must be licensed by the Department of Health Professions where X-rays are used within the scope of practice or be certified by the ARRT, or an individual enrolled in an accredited program for radiologic technology and under the supervision of a licensed or certified radiological technologist, and if a dental assistant, comply with the Board of Dentistry's radiation certification requirements in 18VAC60-20-195.

B. X-ray film processing facilities and practices.

1. Each installation using a radiographic X-ray system and using analog image receptors (e.g. radiographic film) shall have available suitable equipment for handling and processing radiographic film in accordance with the following provisions:

a. Manually developed film:

(1) Processing tanks shall be constructed of mechanically rigid, corrosion resistant material; and

(2) The temperature of solutions in the tanks shall be maintained within the range of 60°F to 80°F (16°C to 27°C). Film shall be developed in accordance with the time-temperature relationships recommended by the film manufacturer, or, in the absence of such recommendations, with the following time-temperature chart that must be posted in the darkroom:

Thermometer Reading (Degrees) Minimum Developing Time (Minutes)

C

F

26.7	80	2

26.1	79	2

25.6	78	22

25.0	77	22

24.4	76	3

23.9	75	3

23.3	74	32

22.8	73	32

22.2	72	4

21.7	71	4

21.1	70	42

20.6	69	42

20.0	68	5

19.4	67	52
18.9	66	52
18.3	65	6
17.8	64	62
17.2	63	7
16.7	62	8
16.1	61	82
15.6	60	92

(3) Devices shall be utilized which will indicate the actual temperature of the developer and signal the passage of a preset time appropriate to the developing time required.

b. Automatic processors and other closed processing systems:

(1) Films shall be developed in accordance with the time-temperature relationships recommended by the film manufacturer; in the absence of such recommendations, the film shall be developed using the following chart:

Developer Temperature Minimum Immersion Time (Seconds)

<input type="checkbox"/> C	<input type="checkbox"/> F	
35.5	96	19
35	95	20
34.5	94	21
34	93	22
33.5	92	23
33	91	24
32	90	25
31.5	89	26
31	88	27
30.5	87	28
30	86	29
29.5	85	30

Immersion time only, no crossover time included.

(2) The specified developer temperature and immersion time shall be posted in the darkroom or on the automatic processor.

c. Processing deviations from the requirements of subdivision 1 of this subsection shall be documented by the registrant in such manner that the requirements are shown to be met or exceeded (e.g., extended processing, and special rapid chemistry).

2. Other requirements.

a. Pass boxes, if provided, shall be so constructed as to exclude light from the darkroom when cassettes are placed in or removed from the boxes, and shall incorporate adequate shielding from stray radiation to prevent exposure of undeveloped film.

b. The darkroom shall be light tight and use proper safelighting such that any film type in use exposed in a cassette to x-radiation sufficient to produce an optical density from one to two when processed shall not suffer an increase in density greater than 0.1 (0.05 for mammography) when exposed in the darkroom for two minutes with all safelights on. If used, daylight film handling boxes shall preclude fogging of the film.

c. Darkrooms typically used by more than one individual shall be provided a method to prevent accidental entry while undeveloped films are being handled or processed.

d. Film shall be stored in a cool, dry place and shall be protected from exposure to stray radiation. Film in open packages shall be stored in a light tight container.

e. Film cassettes and intensifying screens shall be inspected periodically and shall be cleaned and replaced as necessary to best assure radiographs of good diagnostic quality.

f. Outdated X-ray film shall not be used for diagnostic radiographs, unless the film has been stored in accordance with the manufacturer's recommendations and a sample of the film passes a sensitometric test for normal ranges of base plus fog and speed.

g. Film developing solutions shall be prepared in accordance with the directions given by the manufacturer, and shall be maintained in strength by replenishment or renewal so that full development is accomplished within the time specified by the manufacturer.

h. Living and deceased patient's films (diagnostic images) shall be maintained for a minimum of five years. Films for minors shall be maintained for a minimum of five years beyond their 18th birthday.

C. Information to be submitted to the agency. The registrant shall submit to the agency a copy of all surveys, calibrations and inspections performed by a private inspector within 30 days of completion of the survey or calibration.

D. Information to be submitted by the private inspector to the registrant. The private inspector shall provide the inspection report to the registrant within 14 days of the completion of the inspection. A summary and/or recommendations shall be included with this report. The private inspector shall notify the registrant of any noncompliances that need corrective action.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1600. General requirements for all diagnostic X-ray systems.

In addition to other requirements of this part, all diagnostic X-ray systems shall meet the following requirements:

1. Warning label. The control panel containing the main power switch shall bear the warning statement, legible and accessible to view: "WARNING: This X-ray

unit may be dangerous to patient and operator unless safe exposure factors and operating instructions are observed."

2. Battery charge indicator. On battery-powered X-ray generators, visual means shall be provided on the control panel to indicate whether the battery is in a state of charge adequate for proper operation.

3. Leakage radiation from the diagnostic source assembly. The leakage radiation from the diagnostic source assembly measured at a distance of one meter in any direction from the source shall not exceed 25.8 $\mu\text{C}/\text{kg}$ (100 milliroentgens) in one hour when the X-ray tube is operated at its leakage technique factors. Compliance shall be determined by measurements averaged over an area of 100 square centimeters with no linear dimension greater than 20 centimeters.

4. Radiation from components other than the diagnostic source assembly. The radiation emitted by a component other than the diagnostic source assembly shall not exceed 0.5 $\mu\text{C}/\text{kg}$ (2 milliroentgens) in one hour at five centimeters from any accessible surface of the component when it is operated in an assembled X-ray system under any conditions for which it was designed. Compliance shall be determined by measurements averaged over an area of 100 square centimeters with no linear dimension greater than 20 centimeters.

5. Beam quality.

a. Half-value layer.

(1) The half-value layer of the useful beam for a given X-ray tube potential shall not be less than the values shown in Table I. If it is necessary to determine such half-value layer at an X-ray tube potential that is not listed in Table I, linear interpolation or extrapolation may be made.

TABLE I

Design Operating Range (kVp)	Measured Potential (kVp)	Half-Value Layer In mm Aluminum	
		Dental Intra-Oral Manufactured Before Aug. 1, 1974, and on or After Dec. 1, 1980	All Other Diagnostic X-ray Systems
Below 51	30	N/A	0.3

	40	N/A	0.4
	50	1.5	0.5
51 to 70	51	1.5	1.2
	60	1.5	1.3
	70	1.5	1.5
Above 70	71	2.1	2.1
	80	2.3	2.3
	90	2.5	2.5
	100	2.7	2.7
	110	3.0	3.0
	120	3.2	3.2
	130	3.5	3.5
	140	3.8	3.8
	150	4.1	4.1

(2) For capacitor energy storage equipment, compliance with the requirements of subdivision 5 a of this section shall be determined with the system fully charged and a setting of 10 mAs for each exposure.

(3) The required minimal half-value layer of the useful beam shall include the filtration contributed by all materials which are permanently between the source and the patient.

b. Filtration controls. For X-ray systems that have variable kVp and variable filtration for the useful beam, a device shall link the kVp selector with the filter (s) and shall prevent an exposure unless the minimum amount of filtration necessary to produce the HVL required by subdivision 5 a of this section is in the useful beam for the given kVp that has been selected.

6. Multiple tubes. Where two or more radiographic tubes are controlled by one exposure switch, the tube or tubes that have been selected shall be clearly indicated prior to initiation of the exposure. This indication shall be both on the X-ray control panel and at or near the tube housing assembly that has been selected.

7. Mechanical support of tube head. The tube housing assembly supports shall be adjusted such that the tube housing assembly will remain stable during an exposure unless tube housing movement is a designed function of the X-ray

system.

8. Technique indicators.

a. The technique factors to be used during an exposure shall be indicated before the exposure begins. If automatic exposure controls are used, the technique factors which are set prior to the exposure shall be indicated.

b. The requirement of subdivision 8 a of this section may be met by permanent markings on equipment having fixed technique factors. Indication of technique factors shall be visible from the operator's position except in the case of spot films made by the fluoroscopist.

9. Maintaining compliance. Diagnostic X-ray systems and their associated components used on humans and certified pursuant to the federal X-ray Equipment Performance Standard (21 CFR Part 1020) shall be maintained in compliance with applicable requirements of that standard.

10. Locks. All position locking, holding, and centering devices on X-ray system components and systems shall function as intended.

11. Mechanical timers. The use of a mechanical timer is prohibited.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1610. Fluoroscopic X-ray systems.

All fluoroscopic X-ray systems used shall be image intensified and meet the following requirements:

1. Limitation of useful beam.

a. Primary barrier.

(1) The fluoroscopic imaging assembly shall be provided with a primary protective barrier that intercepts the entire cross section of the useful beam at any SID.

(2) The X-ray tube used for fluoroscopy shall not produce X-rays unless the barrier is in position to intercept the entire useful beam.

b. Fluoroscopic beam limitation.

(1) For certified fluoroscopic systems with or without a spot film device, neither the length nor the width of the X-ray field in the plane of the image receptor shall exceed that of the visible area of the image receptor by more than 3.0% of the SID. The sum of the excess length and the excess width shall be no greater than 4.0% of the SID.

(2) For uncertified fluoroscopic systems with a spot film device, the X-ray beam with the shutters fully opened (during fluoroscopy or spot filming) shall be no larger than the largest spot film size for which the device is designed. Measurements shall be made at the minimum SID available but at no less than 20 centimeters table top to the film plane distance.

(3) For uncertified fluoroscopic systems without a spot film device, the requirements of subdivision b (1) of this section apply.

(4) Other requirements for fluoroscopic beam limitation:

(a) Means shall be provided to permit further limitation of the field. Beam-limiting devices manufactured after May 22, 1979, and incorporated in equipment with a variable SID and/or a visible area of greater than 300 square centimeters shall be provided with means for stepless adjustment of the X-ray field;

(b) All equipment with a fixed SID and a visible area of 300 square centimeters or less shall be provided with either stepless adjustment of the X-ray field or with means to further limit the X-ray field size at the plane of the image receptor to 125 square centimeters or less;

(c) If provided, stepless adjustment shall, at the greatest SID, provide continuous field sizes from the maximum attainable to a field size of five centimeters by five centimeters or less;

(d) For equipment manufactured after February 25, 1978, when the angle between the image receptor and beam axis is variable, means shall be provided to indicate when the axis of the X-ray beam is perpendicular to the plane of the image receptor;

(e) For noncircular X-ray fields used with circular image receptors, the error in alignment shall be determined along the length and width dimensions of the X-ray field that pass through the center of the visible area of the image receptor.

c. Spot-film beam limitation. Spot-film devices shall meet the following requirements:

(1) Means shall be provided between the source and the patient for adjustment of the X-ray field size in the plane of the film to the size of that portion of the film that has been selected on the spot film selector. Such adjustment shall be automatically accomplished except when the X-ray field size in the plane of the film is smaller than that of the selected portion of the film. For spot film devices manufactured after June 21, 1979, if the X-ray field size is less than the size of the selected portion of the film, the means for adjustment of the field size shall be only at the operator's option;

(2) Neither the length nor the width of the X-ray field in the plane of the image receptor shall differ from the corresponding dimensions of the selected portion of the image receptor by more than 3.0% of the SID when adjusted for full coverage of the selected portion of the image receptor. The sum, without regard to sign, of the length and width differences shall not exceed 4.0% of the SID;

(3) It shall be possible to adjust the X-ray field size in the plane of the film to a size smaller than the selected portion of the film. The minimum field size at the greatest SID shall be equal to, or less than, five centimeters by five centimeters;

(4) The center of the X-ray field in the plane of the film shall be aligned with

the center of the selected portion of the film to within 2.0% of the SID; and

(5) On spot-film devices manufactured after February 25, 1978, if the angle between the plane of the image receptor and beam axis is variable, means shall be provided to indicate when the axis of the X-ray beam is perpendicular to the plane of the image receptor, and compliance shall be determined with the beam axis indicated to be perpendicular to the plane of the image receptor.

d. Override. If a means exists to override any of the automatic X-ray field size adjustments required in subdivisions 1 b and c of this section that means:

(1) Shall be designed for use only in the event of system failure;

(2) Shall incorporate a signal visible at the fluoroscopist's position that will indicate whenever the automatic field size adjustment is overridden; and

(3) Shall be clearly and durably labeled as follows:

FOR X-RAY FIELD LIMITATION SYSTEM FAILURE

2. Activation of the fluoroscopic tube. X-ray production in the fluoroscopic mode shall be controlled by a device that requires continuous pressure by the fluoroscopist for the entire time of any exposure. When recording serial fluoroscopic images, the fluoroscopist shall be able to terminate the X-ray exposure(s) at any time, but means may be provided to permit completion of any single exposure of the series in process.

3. Exposure rate limits.

a. Entrance exposure rate allowable limits.

(1) Fluoroscopic equipment which is provided with automatic exposure rate control shall not be operable at any combination of tube potential and current which will result in an exposure rate in excess of 2.6 mC/kg (10 roentgens) per minute at the point where the center of the useful beam enters the patient, except:

(a) During recording of fluoroscopic images; or

(b) When an optional high level control is provided. When so provided, the equipment shall not be operable at any combination of tube potential and current that will result in an exposure rate in excess of 5.2 mC/kg-min (20 R/min) at the point where the center of the useful beam enters the patient unless the high level control is activated. Special means of activation of high level controls shall be required. The high level control shall only be operable when continuous manual activation is provided by the operator. A continuous signal audible to the fluoroscopist shall indicate that the high level control is being employed.

(2) Fluoroscopic equipment that is not provided with automatic exposure rate control shall not be operable at any combination of tube potential and current that will result in a exposure rate in excess of 1.3 mC/kg (5 roentgens) per minute at the point where the center of the useful beam enters the patient, except:

(a) During recording of fluoroscopic images; or

(b) When an optional high level control is activated. Special means of activation of high level controls shall be required. The high level control shall only be operable when continuous manual activation is provided by the operator. A continuous signal audible to the fluoroscopist shall indicate that the high level control is being employed.

(3) Compliance with the requirements of subdivision 3 of this section shall be determined as follows:

(a) If the source is below the X-ray table, the exposure rate shall be measured one centimeter above the tabletop or cradle;

(b) If the source is above the X-ray table, the exposure rate shall be measured at 30 centimeters above the tabletop with the end of the beam-limiting device or spacer positioned as closely as possible to the point of measurement;

(c) For a C-arm type of fluoroscope, the exposure rate shall be measured 30

centimeters from the input surface of the fluoroscopic imaging assembly, with the source positioned at any available SID, provided that the end of the beam-limiting device or spacer is no closer than 30 centimeters from the input surface of the fluoroscopic imaging assembly;

(d) For a lateral type fluoroscope, the exposure rate shall be measured at a point 15 centimeters from the centerline of the X-ray table and in the direction of the X-ray source with the end of the beam-limiting device or spacer positioned as closely as possible to the point of measurement. If the tabletop is movable, it shall be positioned as closely as possible to the lateral X-ray source, with the end of the beam-limiting device or spacer no closer than 15 centimeters to the centerline of the X-ray table.

b. Periodic measurement of entrance exposure rate shall be performed by a private inspector for both typical and maximum values as follows:

(1) Such measurements shall be made annually or after any maintenance of the system that might affect the exposure rate;

(2) Results of these measurements shall be posted where any fluoroscopist may have ready access to such results while using the fluoroscope and in the record required in 12VAC5-481-1590 A 12 c. The measurement results shall be stated in coulombs per kilogram (roentgens) per minute and include the technique factors used in determining such results. The name of the individual performing the measurements and the date the measurements were performed shall be included in the results;

(3) Conditions of periodic measurement of typical entrance exposure rate are as follows:

(a) The measurement shall be made under the conditions that satisfy the requirements of subdivision 3 a (3) of this section;

(b) The kVp, mA, and/or other selectable parameters shall be adjusted to those settings typical of clinical use on a 23 cm thick abdominal patient;

(c) The X-ray system that incorporates automatic exposure rate control shall

have sufficient attenuative material placed in the useful beam to produce a milliamperage and/or kilovoltage to satisfy the conditions of subdivision 3 b (3) (b) of this section.

(4) Conditions of periodic measurement of maximum entrance exposure rate are as follows:

(a) The measurement shall be made under the conditions that satisfy the requirements of subdivision 3 a (3) of this section;

(b) The kVp, mA and/or other selectable parameters shall be adjusted to those settings which give the maximum entrance exposure rate;

(c) The X-ray system(s) that incorporates automatic exposure rate control shall have sufficient attenuative material placed in the useful beam to produce the maximum entrance exposure rate of the system.

4. Barrier transmitted radiation rate limits.

a. The exposure rate due to transmission through the primary protective barrier with the attenuation block in the useful beam, combined with radiation from the image intensifier, if provided, shall not exceed 0.5 mR/hr (2 milliroentgens) per hour at 10 centimeters from any accessible surface of the fluoroscopic imaging assembly beyond the plane of the image receptor for each mC/kg (roentgen) per minute of entrance exposure rate.

b. Measuring compliance of barrier transmission.

(1) The exposure rate due to transmission through the primary protective barrier combined with radiation from the image intensifier shall be determined by measurements averaged over an area of 100 square centimeters with no linear dimension greater than 20 centimeters.

(2) If the source is below the tabletop, the measurement shall be made with the input surface of the fluoroscopic imaging assembly positioned 30 centimeters above the tabletop.

(3) If the source is above the tabletop and the SID is variable, the

measurement shall be made with the end of the beam-limiting device or spacer as close to the tabletop as it can be placed, provided that it shall not be closer than 30 centimeters.

(4) Movable grids and compression devices shall be removed from the useful beam during the measurement.

5. Indication of potential and current. During fluoroscopy and cinefluorography, the kV and the mA shall be continuously indicated.

6. Source-to-skin distance. The SSD shall not be less than:

a. Thirty-eight centimeters on stationary fluoroscopic systems manufactured on or after August 1, 1974;

b. Thirty-five and one-half centimeters on stationary fluoroscopic systems manufactured prior to August 1, 1974;

c. Thirty centimeters on all mobile fluoroscopes;

d. Twenty centimeters for all mobile fluoroscopes when used for specific surgical applications; or

e. Nine centimeters for all portable fluoroscopes when used for special applications.

7. Fluoroscopic timer.

a. Means shall be provided to preset the cumulative on-time of the fluoroscopic X-ray tube. The maximum cumulative time of the timing device shall not exceed five minutes without resetting.

b. A signal audible to the fluoroscopist shall indicate the completion of any preset cumulative on-time. Such signal shall continue to sound while X-rays are produced until the timing device is reset.

8. Control of scattered radiation.

a. Fluoroscopic table designs when combined with procedures utilized shall be such that no unprotected part of any staff or ancillary individual's body shall be exposed to unattenuated scattered radiation that originates from

under the table. The attenuation required shall be not less than 0.25 millimeter lead equivalent.

b. Equipment configuration when combined with procedures shall be such that no portion of any staff or ancillary individual's body, except the extremities, shall be exposed to the unattenuated scattered radiation emanating from above the tabletop unless that individual:

(1) Is at least 120 centimeters from the center of the useful beam; or

(2) The radiation has passed through not less than 0.25 millimeter lead equivalent material including, but not limited to, drapes, Bucky-slot cover panel, or self-supporting curtains, in addition to any lead equivalency provided by the protective apron referred to in 12VAC5-481-1590 A 5.

c. The agency may grant exemptions to subdivision 8 b of this section where a sterile field will not permit the use of the normal protective barriers. Where the use of prefitted sterilized covers for the barriers is practical, the agency shall not permit such exemption. The following is a suggested list of fluoroscopic procedures where such exemptions will be automatically granted: angiograms, arthrograms, biliary drainage procedures, fluoroscopic biopsy procedures, myelograms, percutaneous cholangiograms, percutaneous nephrostomies, sinograms or fistulograms, t-tube cholangiograms, interventional cardiac catheterization, and interventional special procedures.

9. Spot-film exposure reproducibility. Fluoroscopic systems equipped with spot-film (radiographic) mode shall meet the exposure reproducibility requirements of 12VAC5-481-1620 D when operating in the spot film mode.

10. Radiation therapy simulation systems. Radiation therapy simulation systems shall be exempt from all the requirements of subdivision 3 of this section. In addition, these systems shall be exempt from:

a. The requirements of subdivisions 1 and 4 of this section provided such systems are designed and used in such a manner that no individual other

than the patient is in the X-ray room during periods of time when the system is producing X-rays; and

b. The requirements of subdivision 7 of this section if such systems are provided with a means of indicating the cumulative time that an individual patient has been exposed to X-rays. Procedures shall require in such cases that the timer be reset between examinations.

11. Surveys. Radiation safety and equipment performance surveys shall be performed annually on all fluoroscopic X-ray systems by or under the direct supervision of a private or state inspector who is physically present at the facility during the inspection in order to assure compliance with these regulations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1620. Radiographic systems other than fluoroscopic, dental intraoral, or computed tomography X-ray systems.

A. Beam limitation, except mammographic systems. The useful beam shall be limited to the area of clinical interest. This shall be deemed to have been met if a positive beam limiting device meeting manufacturer's specifications and the requirements of 12VAC5-481-1620 H 2 has been properly used or if evidence of collimation is shown on at least three sides or three corners of the film (for example, projections from the shutters of the collimator, cone cutting at the corners, or borders at the film's edge).

1. General purpose stationary and mobile X-ray systems, including veterinary systems (other than portable) installed after September 20, 2006.

a. Only X-ray systems provided with means for independent stepless adjustment of at least two dimensions of the X-ray field shall be used.

b. A method shall be provided for visually defining the perimeter of the X-ray

field. The total misalignment of the edges of the visually defined field with the respective edges of the X-ray field along either the length or width of the visually defined field shall not exceed 2.0% of the distance from the source to the center of the visually defined field when the surface upon which it appears is perpendicular to the axis of the X-ray beam.

c. The agency may grant an exemption on noncertified X-ray systems to subdivisions 1 a and b of this subsection provided the registrant makes a written application for such exemption and in that application:

(1) Demonstrates it is impractical to comply with subdivisions 1 a and b of this subsection; and

(2) The purpose of subdivisions 1 a and b of this subsection will be met by other methods.

2. Additional requirements for stationary general purpose X-ray systems. In addition to the requirements of subdivision 1 of this subsection, stationary general purpose X-ray systems, both certified and noncertified, shall meet the following requirements:

a. A method shall be provided to indicate when the axis of the X-ray beam is perpendicular to the plane of the image receptor, to align the center of the X-ray field with respect to the center of the image receptor to within 2.0% of the SID, and to indicate the SID to within 2.0%;

b. The beam-limiting device shall indicate numerically the field size in the plane of the image receptor to which it is adjusted; and

c. Indication of field size dimensions and SID's shall be specified in inches and/or centimeters, and shall be such that aperture adjustments result in X-ray field dimensions in the plane of the image receptor that correspond to those indicated by the beam-limiting device to within 2.0% of the SID when the beam axis is indicated to be perpendicular to the plane of the image receptor.

3. X-ray systems designed for one image receptor size. Radiographic equipment

designed for only one image receptor size at a fixed SID shall be provided with means to limit the field at the plane of the image receptor to dimensions no greater than those of the image receptor, and to align the center of the X-ray field with the center of the image receptor to within 2.0% of the SID, or shall be provided with means to both size and align the X-ray field such that the X-ray field at the plane of the image receptor does not extend beyond any edge of the image receptor.

4. X-ray systems other than those described in subdivisions 1 through 3 of this subsection, and veterinary systems installed prior to September 20, 2006, and all portable veterinary X-ray systems.

a. Means shall be provided to limit the X-ray field in the plane of the image receptor so that such field does not exceed each dimension of the image receptor by more than 2.0% of the SID when the axis of the X-ray beam is perpendicular to the plane of the image receptor.

b. Means shall be provided to align the center of the X-ray field with the center of the image receptor to within 2.0% of the SID, or means shall be provided to both size and align the X-ray field such that the X-ray field at the plane of the image receptor does not extend beyond any edge of the image receptor. Compliance shall be determined with the axis of the X-ray beam perpendicular to the plane of the image receptor.

c. Subdivisions 4 a and b of this subsection may be met with a system that meets the requirements for a general purpose X-ray system as specified in subdivision 1 of this subsection or, when alignment means are also provided, may be met with either:

(1) An assortment of removable, fixed-aperture, beam-limiting devices sufficient to meet the requirement for each combination of image receptor size and SID for which the unit is designed with each such device having clear and permanent markings to indicate the image receptor size and SID for which it is designed; or

(2) A beam-limiting device having multiple fixed apertures sufficient to meet the requirement for each combination of image receptor size and SID for which the unit is designed. Permanent, clearly legible markings shall indicate the image receptor size and SID for which each aperture is designed and shall indicate which aperture is in position for use.

B. Radiation exposure control.

1. Exposure initiation. Means shall be provided to initiate the radiation exposure by a deliberate action on the part of the operator, such as the depression of a switch. Radiation exposure shall not be initiated without such an action. In addition, it shall not be possible to initiate an exposure when the timer is set to a "zero" or "off" position if either position is provided.

2. Exposure indication. Means shall be provided for visual indication observable at or from the operator's protected position whenever X-rays are produced. In addition, a signal audible to the operator shall indicate that the exposure has terminated.

3. Exposure termination. Means shall be provided to terminate the exposure at a preset time interval, preset product of current and time, a preset number of pulses, or a preset radiation exposure to the image receptor. Except for dental panoramic systems, termination of an exposure shall cause automatic resetting of the timer to its initial setting or to "zero."

a. Manual exposure control. An X-ray control shall be incorporated into each X-ray system such that an exposure can be terminated by the operator at any time except for:

(1) Exposure of two seconds or less; or

(2) During serial radiography when means shall be provided to permit completion of any single exposure of the series in process.

b. Automatic exposure controls. When an automatic exposure control is provided:

(1) Indication shall be made on the control panel when this mode of operation is selected;

(2) If the X-ray tube potential is equal to or greater than 50 kVp, the minimum exposure time for field emission equipment rated for pulsed operation shall be equal to or less than a time interval equivalent to two pulses;

(3) The minimum exposure time for all equipment other than that specified in subdivision 3 b (2) of this subsection shall be equal to or less than one-sixtieth (1/60) second or a time interval required to deliver five mAs, whichever is greater;

(4) Either the product of peak X-ray tube potential, current, and exposure time shall be limited to not more than 60 kW per exposure, or the product of X-ray tube current and exposure time shall be limited to not more than 600 mAs per exposure except that, when the X-ray tube potential is less than 50 kVp, the product of X-ray tube current and exposure time shall be limited to not more than 2000 mAs per exposure; and

(5) A visible signal shall indicate when an exposure has been terminated at the limits required by subdivision 3 b (4) of this subsection, and manual resetting shall be required before further automatically timed exposures can be made.

4. Exposure duration (timer) linearity. For systems having independent selection of exposure time settings, the average ratios (X_i) of exposure to the indicated timer setting, in units of $C\text{ kg}^{-1}\text{s}^{-1}$ (mR/s), obtained at any two clinically used timer settings shall not differ by more than 0.10 times their sum. This is written as:

$$(X_1 - X_2) \leq 0.1 (X_1 + X_2)$$

where X_1 and X_2 are the average $C\text{ kg}^{-1}\text{s}^{-1}$ (mR/s) values.

5. Exposure control location. The X-ray exposure control shall be so placed that the operator can view the patient while making any exposure.

6. Operator protection, except veterinary systems, bone densitometers, and other self-contained machines whose design was approved by the FDA.

a. Stationary systems. Stationary X-ray systems shall be required to have the X-ray exposure control permanently mounted behind a protected barrier so that the operator can remain behind that protected barrier during the entire exposure. Where it is impractical to stand behind a protected barrier, dental panoramic and podiatry X-ray systems may, as an alternative, be provided with means to allow the operator to be at least nine feet from the tube housing assembly during exposures.

b. Mobile and portable systems. Mobile and portable X-ray systems that are:

(1) Used continuously for greater than one week in the same location, i.e., a room or suite, shall meet the requirements of subdivision 6 a of this subsection;

(2) Used for less than one week at the same location shall be provided with either a protective barrier at least two meters (6.5 feet) high for operator protection during exposures, or means shall be provided to allow the operator to be at least 2.7 meters (9 feet) from the tube housing assembly during the exposure.

7. Operator protection for veterinary systems. All stationary, mobile or portable X-ray systems used for veterinary work shall be provided with either a two meter (6.5 feet) high protective barrier for operator protection during exposures, or shall be provided with means to allow the operator to be at least 2.7 meters (9 feet) from the tube housing assembly during exposures.

C. Source-to-skin distance. All mobile or portable radiographic systems shall be provided with means to limit the source-to-skin distance to equal to or greater than 30 centimeters, except for veterinary systems.

D. Reproducibility for Exposure and Time. When all technique factors are held constant, including control panel selections associated with automatic exposure control systems, the coefficient of variation of exposure for both manual and automatic

exposure control systems shall not exceed 0.10. This requirement applies to clinically used techniques.

E. Radiation from capacitor energy storage equipment in standby status. Radiation emitted from the X-ray tube when the system is fully charged and the exposure switch or timer is not activated shall not exceed a rate of 0.5 $\mu\text{C/kg}$ (2 milliroentgens) per hour at five centimeters from any accessible surface of the diagnostic source assembly, with the beam-limiting device fully open.

F. Accuracy. Deviation of measured technique factors from indicated values of kVp and exposure time shall not exceed the limits specified for that system by its manufacturer. In the absence of manufacturer's specifications, the deviation shall not exceed 10% of the indicated value for kVp and 10% for time.

G. mA/mAs linearity. The following requirements apply when the equipment is operated on a power supply as specified by the manufacturer for any fixed X-ray tube potential within the range of 40% to 100% of the maximum rated:

1. Equipment having independent selection of X-ray tube current (mA). The average ratios (X_i) of exposure to the indicated milliamperere-seconds product ($\text{C kg}^{-1} \text{ mAs}^{-1}$ (or mR/mAs)) obtained at any two consecutive tube current settings shall not differ by more than 0.10 times their sum:

$$X_1 - X_2 < 0.10 (X_1 + X_2)$$

where X_1 and X_2 are the average values obtained at each of two consecutive tube current settings, or at two settings differing by no more than a factor of two where the tube current selection is continuous.

2. Equipment having a combined X-ray tube current-exposure time product (mAs) selector, but not a separate tube current (mA) selector. The average ratios (X_i) of exposure to the indicated milliamperere-seconds product, in units of $\text{C kg}^{-1} \text{ mAs}^{-1}$ (or mR/mAs), obtained at any two consecutive mAs selector settings shall not differ by more than 0.10 times their sum:

$$X_1 - X_2 < 0.10 (X_1 + X_2)$$

where X_1 and X_2 are the average values obtained at any two mAs selector settings, or at two settings differing by no more than a factor of two where the mAs selector provides continuous selection.

3. Measuring compliance. Determination of compliance shall be based on four exposures taken within a time period of one hour, at each of the two settings. These two settings may include any two focal spot sizes except where one is equal to or less than 0.45 millimeters and the other is greater than 0.45 millimeters. For purposes of this requirement, focal spot size is the nominal focal spot size specified by the X-ray tube manufacturer.

H. Additional requirements. Diagnostic X-ray systems shall be required to comply with the following additional requirements.

1. Beam limitation for stationary and mobile general purpose X-ray systems.

a. There shall be provided a means of stepless adjustment of the size of the X-ray field. The minimum field size at an SID of 100 centimeters shall be equal to or less than five centimeters by five centimeters.

b. When a light localizer is used to define the X-ray field, it shall provide an average illumination of not less than 120 lux or 10 footcandles at 100 centimeters or at the maximum SID, whichever is less. The average illumination shall be based upon measurements made in the approximate center of each quadrant of the light field. Radiation therapy simulation systems manufactured on and after May 27, 1980, are exempt from this requirement.

2. Beam limitation and alignment on stationary general purpose X-ray systems equipped with PBL. If PBL is being used, the following requirements shall be met:

a. PBL shall prevent the production of X-rays when:

(1) Either the length or width of the X-ray field in the plane of the image receptor differs, except as permitted by subdivision 2 c of this subsection, from the corresponding image receptor dimensions by more than 3.0% of the

SID; or

(2) The sum of the length and width differences as stated in subdivision 2 a (1) of this subsection without regard to sign exceeds 4.0% of the SID;

b. Compliance with subdivision 2 a of this subsection shall be determined when the equipment indicates that the beam axis is perpendicular to the plane of the image receptor. Compliance shall be determined no sooner than five seconds after insertion of the image receptor;

c. The PBL system shall be capable of operation, at the discretion of the operator, such that the size of the field may be made smaller than the size of the image receptor through stepless adjustment of the field size. The minimum field size at an SID of 100 centimeters shall be equal to or less than five centimeters by five centimeters;

d. The PBL system shall be designed such that if a change in image receptor does not cause an automatic return to PBL function as described in subdivision 2 a of this subsection, then any change of image receptor size or SID must cause the automatic return.

3. Beam limitation for portable X-ray systems. Beam limitation for portable X-ray systems shall meet the beam limitation requirements of subdivisions A 1 or H 2 of this section.

I. Tube stands for portable X-ray systems. A tube stand or other mechanical support shall be used for portable X-ray systems, so that the X-ray tube housing assembly need not be hand held during exposures unless the system is specifically designed to be handheld.

J. Surveys. Radiation safety and equipment performance surveys shall be performed annually on all X-ray machines covered by this section in order to assure compliance with the regulations, except that bone densitometers and X-ray machines used in the practice of podiatry or dentistry shall be surveyed every three years. The surveys shall be performed by or under the direct supervision of a private or state inspector who is physically present at the facility during the inspection.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1630. Intraoral dental radiographic systems.

In addition to the provisions of 12VAC5-481-1590 and 12VAC5-481-1600, the requirements of 12VAC5-481-1630 apply to X-ray equipment and associated facilities used for dental radiography. Requirements for extraoral dental radiographic systems are covered in 12VAC5-481-1620. Only systems meeting the requirements of this section shall be used.

A. Source-to-skin distance (SSD). X-ray systems designed for use with an intraoral image receptor shall be provided with means to limit SSD, to not less than:

1. 18 centimeters if operable above 50 kVp; or
2. 10 centimeters if operable at 50 kVp only.

B. Beam limitation. Radiographic systems designed for use with an intraoral image receptor shall be provided with means to limit the X-ray beam such that the beam at the minimum SSD shall be containable in a circle having a diameter of no more than seven centimeters.

C. Radiation exposure control.

1. Exposure initiation.

a. Means shall be provided to initiate the radiation exposure by a deliberate action on the part of the operator, such as the depression of a switch. Radiation exposure shall not be initiated without such an action; and

b. It shall not be possible to make an exposure when the timer is set to a "zero" or "off" position if either position is provided.

2. Exposure indication. Means shall be provided for visual indication observable at or from the operator's protected position whenever X-rays are produced. In addition, a signal audible to the operator shall indicate that the exposure has

terminated.

3. Exposure termination.

a. Means shall be provided to terminate the exposure at a preset time interval, preset product of current and time, a preset number of pulses, or a preset radiation exposure to the image receptor.

b. An X-ray exposure control shall be incorporated into each X-ray system such that an exposure can be terminated by the operator at any time, except for exposures of two seconds or less.

c. Termination of an exposure shall cause automatic resetting of the timer to its initial setting or to "zero."

4. Exposure duration (timer) linearity. For systems having independent selection of exposure time settings, the average ratios (X_i) of exposure to the indicated timer setting, in units of $C\ kg^{-1}\ s^{-1}$ (mR/s), obtained at any two clinically used timer settings shall not differ by more than 0.10 times their sum. This is written as:

$$(X_1 - X_2) \leq 0.1 (X_1 + X_2)$$

where X_1 and X_2 are the average values.

5. Exposure control location and operator protection.

a. After September 20, 2006, stationary X-ray systems shall be required to have the X-ray exposure control permanently mounted behind a protected barrier, so that the operator can remain behind that protected barrier during the entire exposure. Where it is impractical to stand behind a protected barrier, the X-ray exposure shall be permanently mounted at least 2.7 meters (9 feet) from the tube housing assembly while making exposures. If an X-ray machine was installed prior to September 20, 2006, and if the X-ray exposure control is not permanently mounted behind a protected barrier, so that the operator can remain behind that protected barrier during the entire exposure, then dosimetry shall be required by all operators of the X-ray system.

b. Mobile and portable X-ray systems that are:

(1) Used for greater than one week in the same location, i.e., a room or suite, shall meet the requirements of subdivision 5 of this subsection;

(2) Used for less than one week in the same location shall be provided with either a protective barrier at least two meters (6.5 feet) high for operator protection, or means shall be provided to allow the operator to be at least 2.7 meters (9 feet) from the tube housing assembly while making exposures.

D. Reproducibility for Exposure and Time. When the equipment is operated on an adequate power supply as specified by the manufacturer, the estimated coefficient of variation of radiation exposures and times shall be no greater than 0.10, for any specific combination of selected technique factors.

E. mA/mAs linearity. The following requirements apply when the equipment is operated on a power supply as specified by the manufacturer for any fixed X-ray tube potential within the range of 40% to 100% of the maximum rated.

1. Equipment having independent selection of X-ray tube current (mA). The average ratios (X_i) of exposure to the indicated milliamperere-seconds product, in units of $C\text{ kg}^{-1}\text{ mAs}^{-1}$ (or mR/mAs), obtained at any two consecutive tube current settings shall not differ by more than 0.10 times their sum:

$$X_1 - X_2 < 0.10 (X_1 + X_2)$$

where X_1 and X_2 are the average values obtained at each of two consecutive tube current settings, or at two settings differing by no more than a factor of two where the tube current selection is continuous.

2. Equipment having a combined X-ray tube current-exposure time product (mAs) selector, but not a separate tube current (mA) selector. The average ratios (X_i) of exposure to the indicated milliamperere-seconds product, in units of $C\text{ kg}^{-1}\text{ mAs}^{-1}$ (or mR/mAs), obtained at any two consecutive mAs selector settings shall not differ by more than 0.10 times their sum:

$$X_1 - X_2 < 0.10 (X_1 + X_2)$$

where X_1 and X_2 are the average values obtained at any two mAs selector settings, or at two settings differing by no more than a factor of two where the mAs selector provides continuous selection.

3. Measuring compliance. Determination of compliance shall be based on four exposures taken within a time period of one hour, at each of the two settings. These two settings may include any two focal spot sizes except where one is equal to or less than 0.45 millimeters and the other is greater than 0.45 millimeters. For purposes of this requirement, focal spot size is the nominal focal spot size specified by the X-ray tube manufacturer.

F. Accuracy. Deviation of technique factors from indicated values for kVp and exposure time (if time is independently selectable) shall not exceed the limits specified for that system by its manufacturer. In the absence of manufacturer's specifications the deviation shall not exceed 10% of the indicated value for kVp and 10% for time.

G. kVp limitations. Dental X-ray machines with a nominal fixed kVp of less than 50 kVp shall not be used to make diagnostic dental radiographs of humans.

H. Administrative controls.

1. Patient and film holding devices shall be used when the techniques permit.
2. The tube housing and the PID shall not be hand held during an exposure.
3. The X-ray system shall be operated in such a manner that the useful beam at the patient's skin does not exceed the requirements of subsection B of this section.
4. Dental fluoroscopy without image intensification shall not be used.

I. Radiation safety and equipment performance surveys shall be performed every three years on all dental X-ray systems by or under the direct supervision of a private or state inspector who is physically present at the facility during the inspection in order to assure compliance with these regulations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1640. Computed tomography X-ray systems.

A. Reserved.

B. Requirements for equipment.

1. Termination of exposure.

a. Means shall be provided to terminate the X-ray exposure automatically by either de-energizing the X-ray source or shuttering the X-ray beam in the event of equipment failure affecting data collection. Such termination shall occur within an interval that limits the total scan time to no more than 110% of its preset value through the use of either a backup timer or devices that monitor equipment function.

b. A visible signal shall indicate when the X-ray exposure has been terminated through the means required by subdivision 1 a of this subsection.

c. The operator shall be able to terminate the X-ray exposure at any time during a scan, or series of scans under CT X-ray system control, of greater than one-half second duration.

2. Tomographic plane indication and alignment.

a. For any single tomogram system, means shall be provided to permit visual determination of the tomographic plane or a reference plane offset from the tomographic plane.

b. For any multiple tomogram system, means shall be provided to permit visual determination of the location of a reference plane. This reference plane can be offset from the location of the tomographic planes.

c. If a device using a light source is used to satisfy the requirements of subdivisions 2 a or b of this subsection, the light source shall provide illumination levels sufficient to permit visual determination of the location of the tomographic plane or reference plane under ambient light conditions of up

to 500 lux.

3. Beam-on and shutter status indicators and control switches.
 - a. The CT X-ray control and gantry shall provide visual indication whenever X-rays are produced and, if applicable, whether the shutter is open or closed.
 - b. Each emergency button or switch shall be clearly labeled as to its function.
4. Indication of CT conditions of operation. The CT X-ray system shall be designed such that the CT conditions of operation to be used during a scan or a scan sequence shall be indicated prior to the initiation of a scan or a scan sequence. On equipment having all or some of these conditions of operation at fixed values, this requirement may be met by permanent markings. Indication of CT conditions of operation shall be visible from any position from which scan initiation is possible.
5. Extraneous radiation. When data are not being collected for image production, the radiation adjacent to the tube port shall not exceed that permitted by subdivision 3 of 12VAC5-481-1600.
6. Maximum surface CTDI identification. The angular position where the maximum surface CTDI occurs shall be identified to allow for reproducible positioning of a CT dosimetry phantom.
7. Additional requirements applicable to CT X-ray Systems containing a gantry manufactured after September 3, 1985.
 - a. The total error in the indicated location of the tomographic plane or reference plane shall not exceed five millimeters.
 - b. If the X-ray production period is less than one-half second, the indication of X-ray production shall be actuated for at least one-half second. Indicators at or near the gantry shall be discernible from any point external to the patient opening where insertion of any part of the human body into the primary beam is possible.
 - c. The deviation of indicated scan increment versus actual increment shall not

exceed plus or minus one millimeter with any mass from 0 to 100 kilograms resting on the support device. The patient support device shall be incremented from a typical starting position to the maximum incremented distance or 30 centimeters, whichever is less, and then returned to the starting position. Measurement of actual versus indicated scan increment may be taken anywhere along this travel.

d. Premature termination of the X-ray exposure by the operator shall necessitate resetting of the CT conditions of operation prior to the initiation of another scan.

C. Facility design requirements.

1. Aural communication. Provision shall be made for two-way aural communication between the patient and the operator at the control panel.

2. Viewing systems.

a. Windows, mirrors, closed-circuit television, or an equivalent shall be provided to permit continuous observation of the patient during irradiation and shall be so located that the operator can observe the patient from the control panel.

b. When the primary viewing system is by electronic means, an alternate viewing system (which may be electronic) shall be available for use in the event of failure of the primary viewing system.

D. Surveys, calibrations, spot checks, and operating procedures.

1. Surveys.

a. All CT X-ray systems installed after September 20, 2006, and those systems not previously surveyed shall have a survey made by, or under the direct supervision of a private inspector who is physically present at the facility during the inspection. In addition, such surveys shall be done at least annually or after any change in the facility or equipment that might cause a significant increase in radiation hazard, whichever occurs first.

b. The registrant shall obtain a written report of the survey from the private inspector, and a copy of the report shall be sent to the agency within 60 days of the date of the survey.

2. Radiation calibrations.

a. The calibration of the radiation output of the CT X-ray system shall be performed by, or under the direction of, a private inspector who is physically present at the facility during such calibration.

b. The calibration of a CT X-ray system shall be performed at intervals specified by a private inspector and after any change or replacement of components that, in the opinion of the private inspector, could cause a change in the radiation output.

c. The calibration of the radiation output of a CT X-ray system shall be performed with a calibrated dosimetry system. The calibration of such system shall be traceable to a national standard. The dosimetry system shall have been calibrated within the preceding two years.

d. CT dosimetry phantom(s) shall be used in determining the radiation output of a CT X-ray system. Such phantom(s) shall meet the following specifications and conditions of use:

(1) CT dosimetry phantom(s) shall be right circular cylinders of polymethyl methacrylate of density 1.19 plus or minus 0.01 grams per cubic centimeter. The phantom(s) shall be at least 14 centimeters in length and shall have diameters of 32.0 centimeters for testing CT X-ray systems designed to image any section of the body and 16.0 centimeters for systems designed to image the head or for whole body scanners operated in the head scanning mode;

(2) CT dosimetry phantom(s) shall provide means for the placement of a dosimeter(s) along the axis of rotation and along a line parallel to the axis of rotation 1.0 centimeter from the outer surface and within the phantom. Means for the placement of dosimeters or alignment devices at other locations may

be provided;

(3) Any effects on the doses measured due to the removal of phantom material to accommodate dosimeters shall be accounted for through appropriate corrections to the reported data or included in the statement of maximum deviation for the values obtained using the phantom;

(4) All dose measurements shall be performed with the CT dosimetry phantom placed on the patient couch or support device without additional attenuation materials present.

e. The calibration shall be required for each type of head, body, or whole-body scan performed at the facility.

f. Calibration shall meet the following requirements:

(1) The dose profile along the center axis of the CT dosimetry phantom for the minimum, maximum, and midrange values of the nominal tomographic section thickness used by the registrant shall be measurable. Where less than three nominal tomographic thicknesses can be selected, the dose profile determination shall be performed for each available nominal tomographic section thickness;

(2) The CTDI along the two axes specified in subdivision 2 d (2) of this subsection shall be measured. The CT dosimetry phantom shall be oriented so that the measurement point 1.0 centimeter from the outer surface and within the phantom is in the same angular position within the gantry as the point of maximum surface CTDI identified. The CT conditions of operation shall correspond to typical values used by the registrant;

(3) The spot checks specified in subdivision 3 of this subsection shall be made.

g. Calibration procedures shall be in writing. Records of calibrations performed shall be maintained for inspection by the agency.

3. Spot checks.

- a. The spot-check procedures shall be in writing and shall have been developed by a private inspector.
 - b. The spot-check procedures shall incorporate the use of a CT dosimetry phantom that has a capability of providing an indication of contrast scale, noise, nominal tomographic section thickness, the resolution capability of the system for low and high contrast objects, and measuring the mean CTN for water or other reference material.
 - c. All spot checks shall be included in the calibration required by subdivision 2 of this subsection and at time intervals and under system conditions specified by a private inspector.
 - d. Spot checks shall include acquisition of images obtained with the CT dosimetry phantom(s) using the same processing mode and CT conditions of operation as are used to perform calibrations required by subdivision 2 of this subsection. The images shall be retained, until a new calibration is performed, in two forms as follows:
 - (1) Photographic copies of the images obtained from the image display device; and
 - (2) Images stored in digital form on a storage medium compatible with the CT X-ray system.
 - e. Written records of the spot checks performed shall be maintained for inspection by the agency.
4. Operating procedures.
- a. The CT X-ray system shall not be operated except by an individual who has been specifically trained in its operation.
 - b. Information shall be available at the control panel regarding the operation and calibration of the system. Such information shall include the following:
 - (1) Dates of the latest calibration and spot checks and the location within the facility where the results of those tests may be obtained;

(2) Instructions on the use of the CT dosimetry phantom(s) including a schedule of spot checks appropriate for the system, allowable variations for the indicated parameters, and the results of at least the most recent spot checks conducted on the system;

(3) The distance in millimeters between the tomographic plane and the reference plane if a reference plane is utilized; and

(4) A current technique chart available at the control panel that specifies for each routine examination the CT conditions of operation and the number of scans per examination.

c. If the calibration or spot check of the CT X-ray system identifies that a system operating parameter has exceeded a tolerance established by the private inspector, use of the CT X-ray system on patients shall be limited to those uses permitted by established written instructions of the private inspector.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-1650. Mammography.

A. Equipment standards. Only X-ray systems meeting the following standards shall be used.

1. System design. The X-ray system shall be specifically designed for mammography.
2. Image receptor. The image receptor systems and their individual components shall be specifically designed for or appropriate for mammography.
3. kVp/target/filter. The X-ray system shall have the capability of providing kVp/target/filter combinations compatible with the selected image receptor system.

4. Beam quality.

a. When used with screen-film image receptors, and when the contribution to filtration made by the compression device is included, the useful beam shall have a half-value layer (HVL):

(1) Between the values of: $((\text{measured kVp})/100)$ and $((\text{measured kVp})/100 + 0.1)$ millimeters aluminum for molybdenum targets;

(2) At least the value of $((\text{measured kVp})/100)$ millimeters aluminum for rhodium alloy targets.

b. For xeroradiography, the HVL of the useful beam with the compression device in place shall be at least 1.0 and not greater than 1.6 mm aluminum, measured at 49 kVp with a tungsten target tube.

5. Resolution. The combination of focal spot size, source-to-image receptor distance and magnification shall result in a resolution of at least 12 line pairs per millimeter (cycles/mm) measured when a resolution pattern is positioned 4.2 cm above all breast supports and when the resolution pattern is either perpendicular to or parallel with the chest wall edge of the image receptor support. The measurement shall be made with the kVp in the range of 25-30 and the mA shall be the highest available for the focal spot size selected. The resolution shall be at least 11 line pairs when a high-contrast resolution bar test pattern is orientated with the bars perpendicular to the anode-cathode axis, and a minimum resolution of 13 line pairs/mm when the bars are parallel to that axis. The bar pattern must be placed 4.5 cm above the breast support surface, centered with respect to the chest wall edge of the image receptor, and with the edge of the pattern within one cm of the chest wall edge of the image receptor. When more than one target material is provided, the measurement must be made using the appropriate focal spot for each target material.

6. Compression.

a. The X-ray system shall be capable of compressing the breast with a force of at least 25 pounds and shall be capable of maintaining this compression for

at least three minutes.

b. The chest wall edge of the compression paddle shall extend beyond the chest wall edge of the image receptor by no more than 2.0% of the Source-to-Image Receptor Distance with the compression paddle placed 4.2 cm above the breast support device. With the compression paddle in this position, the chest wall edge of the compression paddle shall not be visible in the acquired image.

7. System capabilities. A mammographic X-ray system utilizing screen-film image receptors shall have:

a. The capability of using anti-scatter grids that are:

(1) Integral to the X-ray system;

(2) Available for all image receptor sizes used;

b. The capability of automatic exposure control, for systems installed after September 20, 2006; and

c. The capability of displaying post-exposure mAs after an exposure made using an automatic exposure control device, for systems installed after September 20, 2006.

8. Milliampere-second read-out accuracy. For those mammographic X-ray systems equipped with automatic exposure control and post-exposure mAs read-out, the indicated mAs read-out shall be within 10% of the actual mAs delivered.

9. Transmission. For X-ray systems manufactured after September 5, 1978, the transmission of the primary beam through any image receptor support provided with the system shall be limited such that the exposure five centimeters from any accessible surface beyond the plane of the image receptor supporting device does not exceed 25.8 nC/kg (0.1 milliroentgen) for each activation of the tube. Exposure shall be measured with the system operated at the minimum SID for which it is designed. Compliance shall be determined at the maximum rated peak tube potential for the system and at the maximum rated product of tube current

and exposure time (mAs) for that peak tube potential. Compliance shall be determined by measurements averaged over an area of 100 square centimeters with no linear dimension greater than 20 centimeters.

10. Collimation.

a. All systems shall have beam-limiting devices that allow the entire chest wall edge of the X-ray field to extend to the chest wall edge of the image receptor and provide means to assure that the X-ray field does not extend beyond any edge of the image receptor by more than 2.0% of the SID.

b. Means for visually defining the perimeter of the X-ray field shall be provided. The total misalignment of the edges of the visually defined field with the respective edges of the X-ray field along either the length or width of the visually defined field shall not exceed 2.0% of the distance from the source to the center of the visually defined field when the surface upon which it appears is perpendicular to the axis of the X-ray beam.

11. Accuracy of kVp. Deviation of actual kVp from the indicated kVp shall not exceed the limits specified by the manufacturer of the X-ray system, or, the actual kVp shall be within plus or minus 2 kVp of the indicated kVp, whichever limit is more restrictive.

12. Automatic exposure control performance. In addition to 12VAC5-481-1620 D, mammographic systems in the AEC mode shall be able to maintain constant film density to within an optical density of plus or minus 0.3 of the average optical density over the kVp range used clinically, using phantoms of BR-12 or other breast equivalent material thicknesses of two centimeters to six centimeters. If the facility has established a technique chart that utilizes varying technical factors for different breast thicknesses, those adjustments in technique may be used when performing this test.

13. Radiation output minimum. At 28 kVp, with a focal spot meeting the requirements of subdivision A 5 of this section, the mammographic system shall be capable of sustaining a minimum output rate of $130 \mu\text{C/kg/sec}$

(500 mR/sec) for at least three seconds. This output shall be measured at a point 4.2 centimeters from the surface of the breast support device when the SID is at its maximum and the effect of compression paddle attenuation is included.

14. Screen-film contact. Cassettes shall not be used for mammography if poor contact of two or more large areas (>1 cm in diameter) or a section longer than 1 cm and >2 mm in width along the chest wall edge can be seen in a 40 mesh test.

15. Image quality. The mammographic X-ray imaging system shall be capable of providing an image of a 0.75 mm fiber, 0.32 mm speck group, and a 0.75 mm mass from the Conference of Radiation Control Program Directors NEXT '92 phantom (or equivalent) on the standard mammographic image receptor system in use at a facility. Mammograms shall not be taken on patients if this minimum is not met. Any fibers, speck groups and masses larger than those specified shall also be imaged.

16. Dose. The mean glandular dose for one craniocaudal view, measured with the phantom referenced in subdivision 15 of this subsection, based on exposure measured at the breast entrance location, and using dose conversion factors specified by the Health Care Financing Administration in their Medicare Mammography Survey Protocols, shall not exceed the following values:

- a. 2.0 mGy (200 millirads) for nongrid screen film systems;
- b. 3.0 mGy (300 millirads) for screen-film systems with grid.

17. Technique settings. The technique settings used for subdivisions 15 and 16 of this subsection shall be those used by the facility for its clinical images of a 50% adipose, 50% glandular, 4.2 cm compressed breast.

B. Quality assurance.

1. Quality assurance program required. The registrant shall have a written, ongoing equipment quality assurance program specific to mammographic imaging, covering all components of the diagnostic X-ray imaging system, to ensure consistently high-quality images with minimum patient exposure. Responsibilities under this requirement include providing qualified individuals who are to:

- a. Conduct equipment performance monitoring functions;
 - b. Analyze the monitoring results to determine if there are problems requiring correction;
 - c. Carry out or arrange for the necessary corrective actions when results of quality control tests including those specified in subdivision 3 of this subsection indicate the need; and
 - d. Maintain records for a minimum of two years documenting that actions required under subdivisions 1 a through c of this subsection have been completed.
2. Quality assurance program review. At intervals not to exceed 12 months, the registrant shall:
- a. Have the annual quality control tests specified in subdivision 3 of this subsection performed by a qualified individual and obtain the results of those tests, incorporating them into the records specified in subdivision 1 d of this subsection; and
 - b. Conduct a review of the effectiveness of the quality assurance program required in subdivision 1 of this subsection and maintain a written report of such review. Records of annual reviews shall be maintained for a minimum of two years and shall be available for agency review.
3. Equipment quality control tests. The registrant shall ensure that the following quality control tests are performed when applicable equipment or components are initially installed, or replaced or serviced (if such servicing affects test results), and performed thereafter at least as often as the frequency specified. The private inspector shall determine the corrective action interval.
- a. Processor performance by sensitometric means—daily, or day of use, prior to the first patient exposure. For any mammography registrant using film processors at multiple locations, such as a mobile service, each processor shall be subject to this requirement. Corrective action shall be taken when:

- (1) Deviations of 0.15 or more in optical density from established operating levels occur for readings of mid-density (MD) and density difference (DD) on the sensitometric control charts;
 - (2) Base plus fog (B+F) exceeds the established operating level by more than 0.03 in optical density.
- b. Resolution—upon tube installation or replacement and every 12 months.
 - c. Focal spot size—upon tube installation or tube replacement only or at least every 12 months, whichever occurs first.
 - d. Half-value layer—12 months.
 - e. kVp accuracy and reproducibility—12 months.
 - f. Output reproducibility, mA linearity, and mR/mAs—12 months.
 - g. Automatic exposure control reproducibility and performance (response to kVp and phantom thickness variations)—12 months.
 - h. Screen-film contact and screen artifact detection—six months.
 - i. Compression device performance (releases, level of force, etc)—six months.
 - j. Collimator alignment—12 months.
 - k. Primary/secondary barrier transmission—upon initial X-ray system installation and significant modification of the system or the facility.
 - l. Image quality (using a test "phantom," that simulates the composition of the breast and includes simulations of breast structures)—weekly for stationary systems, on each day of use for mobile systems, and upon significant service or modification of any mammographic system.
 - m. Densitometer accuracy check—every 12 months.
 - n. Glandular dose—every 12 months.
 - o. Image quality—every 12 months.
 - p. Artifacts—every 12 months.

4. Additional quality control requirements. The registrant shall perform the following observations and procedures according to the frequency noted and record the results. Corrections of problems noted shall be made and recorded. Records shall be maintained over the most recent two-year period.

- a. Retake Analysis—three months.
- b. Viewbox uniformity—six months.
- c. Darkroom integrity (safelight condition, light leaks, etc.)—six months.
- d. Screen cleaning—weekly.
- e. Fixer retention—three months.

C. Additional facility requirements.

1. Masks. Masks shall be provided on the viewboxes to block extraneous light from the viewer's eye when the illuminated surface of the viewbox is larger than the exposed area of the film.

2. Film processing.

- a. Film processors utilized for mammography shall be adjusted to and operated at the specifications recommended by the mammographic film manufacturer, or at other settings such that the sensitometric performance is at least equivalent.
- b. Clinical films and phantom image quality films shall be processed within 10 hours of exposure.
- c. Facilities shall offer to process films before the patient leaves the facility. If the patient chooses not to wait; of there is not developing capabilities, the patient will be notified within two business days if additional films are necessary.

3. Instruments and devices. An image quality phantom, sensitometer, and a calibrated densitometer shall be available to each facility in order to comply with the quality control test frequencies specified in subdivision B 3 of this section.

4. Operator qualifications. The operator of the X-ray machine shall be certified by

the American Registry of Radiologic Technologists and shall have had specialized training in mammography meeting the requirements set forth by the FDA under the MQSA of 1992.

5. Physician qualifications. The physician interpreting the mammograms shall be certified by the American Board of Radiology, the American Osteopathic Board of Radiology, or Board eligible, or equivalent, and shall have had specialized training in mammography and image interpretation.

6. Physicist qualifications. The person performing evaluation of mammographic system performance in accordance with these regulations shall meet the requirements set forth in 12VAC5-481-340 C.

7. Image retention. Clinical images shall be retained for a minimum of five years or 10 years if no other clinical images are obtained.

8. Retake rate. Corrective action shall be taken if the retake rate exceeds 5.0%. The retake rate shall be calculated as $(\text{repeated} + \text{rejected films}) / \text{total number of clinical films}$.

9. Darkroom fog. Darkroom fog levels shall not exceed 0.05 in optical density when sensitized mammographic film of the type used in the facility is exposed to darkroom conditions with safelight on for two minutes. Film shall be sensitized by exposing it to sufficient light from an appropriate intensifying screen or sensitometer so that after processing an optical density of at least 1.0 is achieved.

Facility qualifications. The registrant performing mammography shall be accredited by the American College of Radiology or another agency recognized as a certifying body or have their application pending. The registrant shall also be certified by the FDA or another agency recognized as an accrediting body under the MQSA of 1992 or have a provisional/interim certificate.

D. Additional state requirements.

1. When film developing is not available or the patient chooses not to wait, the patient shall be notified within two business days if another mammogram is

necessary. This requirement does not imply or require that a diagnostic opinion be made at the time of the mammogram. The interpreting physician may require that the mammogram be retaken if, in the opinion of the physician, the study is of inadequate quality.

2. Agency inspectors may conduct unannounced inspections during normal hours of business.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Part VII

Use of Radionuclides in the Healing Arts

Article 1

Purpose and Scope

12VAC5-481-1660. Purpose and scope.

Part VII (12VAC5-481-1660 et seq.) of this chapter establishes requirements and provisions for the production, preparation, compounding and use of radionuclides in the healing arts and for issuance of licenses authorizing the medical use of this material. These requirements and provisions provide for the protection of the public health and safety. The requirements and provisions of Part VII (12VAC5-481-1660 et seq.) of this chapter are in addition to, and not in substitution for, others in these regulations. The requirements and provisions of these regulations apply to applicants and licensees subject to Part VII (12VAC5-481-1660 et seq.) of this chapter unless specifically exempted.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 2

General Information

12VAC5-481-1670. General requirements.

The following regulations, Maintenance of records (10 CFR 35.5), Provisions for the protection of human research subjects (10 CFR 35.6), FDA, other Federal, and State requirements (10 CFR 35.7), and Implementation (10 CFR 35.10) are applicable in the Commonwealth of Virginia:

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1680. Licensing and exemptions.

The following regulations, License required (10 CFR 35.11(a) and (b)), Application for license, amendment, or renewal (10 CFR 35.12), Exemptions regarding Type A licenses of broad scope (10 CFR 35.15), License issuance (10 CFR 35.18), and Specific exemptions (10 CFR 35.19) are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1690. Notifications.

The following regulation, Notifications (10 CFR 35.14) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 3

General Administrative Requirements

12VAC5-481-1700. Authority and responsibilities for the radiation protection programs and changes.

The following regulations, Authority and responsibilities for the radiation protection programs (10 CFR 35.24), and Radiation Protection program changes (10 CFR 35.26) are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1710. Supervision.

The following regulation, Supervision (10 CFR 35.27) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1720. Written directives.

The following regulation, Written directives (10 CFR 35.40) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1730. Procedures for administrations requiring a written directive.

The following regulation, Procedures for administrations requiring a written directive (10 CFR 35.41) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1740. Suppliers for sealed sources or devices for medical use.

The following regulation, Suppliers for sealed sources or devices for medical use (10 CFR 35.49) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1750. Training for Radiation Safety Officer.

The following regulation, Training for Radiation Safety Officer (10 CFR 35.50) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1760. Training for an authorized medical physicist.

The following regulation, Training for an authorized medical physicist (10 CFR 35.51) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1770. Training for an authorized nuclear pharmacist.

The following regulation, Training for an authorized nuclear pharmacist (10 CFR 35.55) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1780. Training for experienced Radiation Safety Officer, teletherapy or medical physicist, authorized user, and pharmacist.

The following regulation, Training for experienced Radiation Safety Officer, teletherapy or medical physicist, authorized user, and pharmacist (10 CFR 35.57) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1790. Recentness of training.

The following regulation, Recentness of training (10 CFR 35.59) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 4**General Technical Requirements****12VAC5-481-1800. Possession, use, and calibration of instruments used to measure the activity of unsealed byproduct material.**

The following regulation, Possession, use, and calibration of instruments used to measure the activity of unsealed byproduct material (10 CFR 35.60) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1810. Calibration of survey instruments.

The following regulation, Calibration of survey instruments (10 CFR 35.61) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1820. Determination of dosages of unsealed byproduct material for medical use.

The following regulation, Determination of dosages of unsealed byproduct material for medical use (10 CFR 35.63) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1830. Authorization for calibration, transmission, and reference sources.

The following regulation, Authorization for calibration, transmission, and reference sources (10 CFR 35.65) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1840. Requirements for possession of sealed sources and brachytherapy sources.

The following regulation, Requirements for possession of sealed sources and brachytherapy sources (10 CFR 35.67) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1850. Labeling of vials and syringes.

The following regulation, Labeling of vials and syringes (10 CFR 35.69) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1860. Surveys of ambient radiation exposure rate.

The following regulation, Surveys of ambient radiation exposure rate (10 CFR 35.70) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1870. Release of individuals containing unsealed byproduct material or implants containing byproduct material.

The following regulation, Release of individuals containing unsealed byproduct material or implants containing byproduct material (10 CFR 35.75) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1880. Provision of mobile medical service.

The following regulation, Provision of mobile medical service (10 CFR 35.80) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1890. Decay-in-storage.

The following regulation, Decay-in-storage (10 CFR 35.92) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 5

Unsealed Byproduct Material – Written Directive Not Required

12VAC5-481-1900. Use of unsealed byproduct material for uptake, dilution, and excretion studies for which a written directive is not required.

The following regulation, Use of unsealed byproduct material for uptake, dilution, and excretion studies for which a written directive is not required (10 CFR 35.100) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1910. Training for uptake, dilution, and excretion studies.

The following regulation, Training for uptake, dilution, and excretion studies (10 CFR 35.190) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1920. Use of unsealed byproduct material for imaging and localization studies for which a written directive is not required.

The following regulation, Use of unsealed byproduct material for imaging and localization studies for which a written directive is not required (10 CFR 35.200) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1930. Permissible molybdenum-99 concentration.

The following regulation, Permissible molybdenum-99 concentration (10 CFR 35.204) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1940. Training for imaging and localization studies.

The following regulation, Training for imaging and localization studies (10 CFR 35.290) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 6

Unsealed Byproduct Material - Written Directive Required

12VAC5-481-1950. Use of unsealed by product material for which a written directive is required.

The following regulation, Use of unsealed by product material for which a written directive is required (10 CFR 35.300) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1960. Safety instruction.

The following regulation, Safety instruction (10 CFR 35.310) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1970. Safety precautions.

The following regulation, Safety precautions (10 CFR 35.315) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1980. Training for use of unsealed byproduct material for which a written directive is required.

The following regulation, Training for use of unsealed byproduct material for which a written directive is required (10 CFR 35.390) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-1990. Training for the oral administration of sodium iodide I-131 requiring a written directive in quantities less than or equal to 1.22 Gigabecquerels (33 millicuries).

The following regulation, Training for the oral administration of sodium iodide I-131 requiring a written directive in quantities less than or equal to 1.22 Gigabecquerels (33 millicuries) (10 CFR 35.392) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2000. Training for the oral administration of sodium iodide I-131 requiring a written directive in quantities greater than 1.22 Gigabecquerels (33 millicuries).

The following regulation, Training for the oral administration of sodium iodide I-131 requiring a written directive in quantities greater than 1.22 Gigabecquerels (33 millicuries) (10 CFR 35.394) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2001. Training for the parental administration of unsealed byproduct material requiring a written directive.

The following regulation, Training for the parenteral administration of unsealed byproduct material requiring a written directive (10 CFR 35.396) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 7

Manual Brachytherapy

12VAC5-481-2010. Manual Brachytherapy.

The following regulations, Use of sources for manual brachytherapy (10 CFR 35.400), Surveys after source implant and removal (10 CFR 35.404), Brachytherapy sources accountability (10 CFR 35.406), Safety instruction (10 CFR 35.410), Safety precautions

(10 CFR 35.415), Calibration measurements of brachytherapy sources (10 CFR 35.432), Decay of strontium-90 sources for ophthalmic treatment (10 CFR 35.433), Therapy-related computer systems (10 CFR 35.457), Training for use of manual brachytherapy sources (10 CFR 35.490), and Training for ophthalmic use of strontium-90 (10 CFR 35.491) are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 8

Sealed Sources for Diagnosis

12VAC5-481-2020. Use of sealed sources for diagnosis.

The following regulation, Use of sealed sources for diagnosis (10 CFR 35.500) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2030. Training for use of sealed sources for diagnosis.

The following regulation, Training for use of sealed sources for diagnosis (10 CFR 35.590) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 9.

Photon Emitting Remote Afterloader Units, Teletherapy Units, and Stereotactic
Radiosurgery Units

**12VAC5-481-2040. Photon Emitting Remote Afterloader Units, Teletherapy Units,
and Stereotactic Radiosurgery Units.**

The following regulations, Use of a sealed source in a remote afterloader unit, teletherapy unit, or gamma stereotactic radiosurgery unit (10 CFR 35.600), Surveys of patients and human research subjects treated with a remote afterloader unit (10 CFR 35.604), Installation, maintenance, adjustment, and repair (10 CFR 35.605), Safety procedures and instructions for remote afterloader units, teletherapy units, and gamma stereotactic radiosurgery units (10 CFR 35.610), Safety precautions for remote afterloader units, teletherapy units, and gamma stereotactic radiosurgery units (10 CFR 35.615), Dosimetry equipment (10 CFR 35.630), Full calibration measurements on teletherapy units (10 CFR 35.632), Full calibration measurements on remote afterloader units, (10 CFR 35.633), Full calibration measurements on gamma stereotactic radiosurgery units (10 CFR 35.635), Periodic spot-checks for teletherapy units (10 CFR 35.642), Periodic spot-checks for remote afterloader units (10 CFR 35.643), Periodic spot-checks for gamma stereotactic radiosurgery units (10 CFR 35.645), Additional technical requirements for mobile remote afterloader units (10 CFR 35.647), Radiation surveys, (10 CFR 35.652), Five-year inspection for teletherapy and gamma stereotactic radiosurgery units (10 CFR 35.655), Therapy-related computer systems (10 CFR 35.657), and Training for use of remote afterloader units, teletherapy units, and gamma stereotactic radiosurgery units (10 CFR 35.690) are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 10

Training and Experience Requirements

12VAC5-481-2050. (Repealed.)

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; repealed, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 11

Other Medical Uses of Byproduct Material or Radiation from Byproduct Material

12VAC5-481-2060. Other medical uses of byproduct material or radiation from byproduct materials.

The following regulation, Other medical uses of byproduct material or radiation from byproduct materials (10 CFR 35.1000) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 12

Records

12VAC5-481-2070. Records.

The following regulations, Records of authority and responsibilities for radiation protection programs (10 CFR 35.2024), Records of radiation protection program changes (10 CFR 35.2026), Records of written directives (10 CFR 35.2040), Records for procedures for administrations requiring a written directive (10 CFR 35.2041), Records of calibrations of instruments used to measure the activity of unsealed byproduct materials (10 CFR 35.2060), Records of radiation survey instrument calibrations (10 CFR 35.2061), Records of dosages of unsealed byproduct material for

medical use (10 CFR 35.2063), Records of leaks tests and inventory of sealed sources and brachytherapy sources (10 CFR 35.2067), Records of surveys for ambient radiation exposure rate (10 CFR 35.2070), Records of the release of individuals containing unsealed byproduct material or implants containing byproduct material (10 CFR 35.2075), Records of mobile medical services (10 CFR 35.2080), Records of decay-in-storage (10 CFR 35.2092), Records of molybdenum-99 concentrations (10 CFR 35.2204), Records of safety instruction (10 CFR 35.2310), Records of surveys after source implant and removal (10 CFR 35.2404), Records of brachytherapy source accountability (10 CFR 35.2406), Records of calibration measurements of brachytherapy sources (10 CFR 35.2432), Records of decay of strontium-90 sources for ophthalmic treatments (10 CFR 35.2433), Records of installation, maintenance, adjustment, and repair of remote afterloader units, teletherapy units, and gamma stereotactic radiosurgery units (10 CFR 35.2605), Records of safety procedures (10 CFR 35.2610), Records of dosimetry equipment used with remote afterloader units, teletherapy units, and gamma stereotactic radiosurgery units (10 CFR 35.2630), Records of teletherapy, remote afterloader, and gamma stereotactic radiosurgery full calibrations (10 CFR 35.2632), Records of periodic spot-checks for teletherapy units (10 CFR 35.2642), Records of periodic spot-checks for remote afterloader units (10 CFR 35.2643), Records of periodic spot-checks for gamma stereotactic radiosurgery units (10 CFR 35.2645), Records of additional technical requirements for mobile remote afterloader units (10 CFR 35.2647), Records of surveys of therapeutic treatment units (10 CFR 35.2652), and Records of 5-year inspection for teletherapy and gamma stereotactic radiosurgery units (10 CFR 35.2655) are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 13

Reports

12VAC5-481-2080. Reports.

The following regulations, Report and notification of a medical event (10 CFR 35.3045), Report and notification of a dose to an embryo/fetus or a nursing child (10 CFR 35.3047), and Report of a leaking source (10 CFR 35.3067), are applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part VIII

Radiation Safety Requirements For Analytical X-Ray Equipment

12VAC5-481-2090. Purpose and scope.

This part provides special requirements for analytical X-ray equipment. The requirements of this part are in addition to, and not in substitution for, applicable requirements in other parts of these regulations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2100. Equipment requirements.

A. Safety device. A device that prevents the entry of any portion of an individual's body into the primary X-ray beam path or that causes the beam to be shut off upon entry into its path shall be provided on all open-beam configurations. A registrant may apply to the agency for an exemption from the requirement of a safety device. Such application shall include:

1. A description of the various safety devices that have been evaluated;
2. The reason each of these devices cannot be used; and
3. A description of the alternative methods that will be employed to minimize the possibility of an accidental exposure, including procedures to assure that operators and others in the area will be informed of the absence of safety devices.

B. Warning devices.

1. Open-beam configurations shall be provided with a readily discernible indication of:

- a. X-ray tube "on-off" status located near the radiation source housing, if the primary beam is controlled in this manner; and/or
- b. Shutter "open-closed" status located near each port on the radiation source housing, if the primary beam is controlled in this manner.

2. An easily visible warning light labeled with the words "X-RAY ON," or words having a similar intent, shall be located:

- a. Near any switch that energizes an X-ray tube and shall be illuminated only when the tube is energized; or
- b. In the case of a radioactive source, near any switch that opens a housing shutter and shall be illuminated only when the shutter is open.

3. Warning devices shall be labeled so that their purpose is easily identified. On equipment installed after September 20, 2006, warning devices shall have fail-safe characteristics.

C. Ports. Unused ports on radiation source housings shall be secured in the closed position in a manner that will prevent casual opening.

D. Labeling. All analytical X-ray equipment shall be labeled with a readily discernible sign or signs bearing the radiation symbol and the words:

1. "CAUTION—HIGH INTENSITY X-RAY BEAM," or words having a similar intent, on the X-ray source housing; and

2. "CAUTION RADIATION—THIS EQUIPMENT PRODUCES RADIATION WHEN ENERGIZED," or words having a similar intent, near any switch that energizes an X-ray tube if the radiation source is an X-ray tube; or

3. "CAUTION—RADIOACTIVE MATERIAL", or words having a similar intent, on the source housing in accordance with 12VAC5-481-660 if the radiation source is a radionuclide.

E. Shutters. On open-beam configurations installed after September 20, 2006, each port on the radiation source housing shall be equipped with a shutter that cannot be opened unless a collimator or a coupling has been connected to the port.

F. Radiation source housing. Each radiation source housing shall be subject to the following requirements:

1. Each X-ray tube housing shall be equipped with an interlock that shuts off the tube if it is removed from the radiation source housing or if the housing is disassembled.

2. Each radioactive source housing or port cover or each X-ray tube housing shall be so constructed that, with all shutters closed, the radiation measured at a distance of five centimeters from its surface is not capable of producing a dose in excess of 2.5 millirems (0.025 mSv) in one hour. For systems utilizing X-ray tubes, this limit shall be met at any specified tube rating.

G. Generator cabinet. Each X-ray generator shall be supplied with a protective cabinet that limits leakage radiation measured at a distance of five centimeters from its surface such that it is not capable of producing a dose in excess of 0.25 millirem (2.5 μ Sv) in one hour.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2110. Area requirements.

A. Radiation Levels. The local components of an analytical X-ray system shall be located and arranged and shall include sufficient shielding or access control such that no radiation levels exist in any area surrounding the local component group that could result in a dose to an individual present therein in excess of the dose limits given in 12VAC5-481-640. For systems utilizing X-ray tubes, these levels shall be met at any specified tube rating.

B. Surveys.

1. Radiation surveys, as required by 12VAC5-481-750, of all analytical X-ray systems sufficient to show compliance with 12VAC5-481-2440 A shall be performed:

- a. Upon installation of the equipment, and at least once every 12 months thereafter;
- b. Following any change in the initial arrangement, number, or type of local components in the system;
- c. Following any maintenance requiring the disassembly or removal of a local component in the system;
- d. During the performance of maintenance and alignment procedures if the procedures require the presence of a primary X-ray beam when any local component in the system is disassembled or removed;
- e. Any time a visual inspection of the local components in the system reveals an abnormal condition; and
- f. Whenever personnel monitoring devices show a significant increase over the previous monitoring period or the readings are approaching the limits specified in 12VAC5-481-630.

2. Radiation survey measurements shall not be required if a registrant (or licensee) can demonstrate compliance with subsection A of this section to the satisfaction of the agency.

C. Posting. Each area or room containing analytical X-ray equipment shall be conspicuously posted with a sign or signs bearing the radiation symbol and the words "CAUTION—X-RAY EQUIPMENT" or words having a similar intent in accordance with 12VAC5-481-660.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2120. Operating requirements.

A. Procedures. Normal operating procedures shall be written and available to all analytical X-ray equipment workers. No individual shall be permitted to operate analytical X-ray equipment in any manner other than that specified in the procedures unless such individual has obtained written approval of the radiation safety officer.

B. Bypassing. No individual shall bypass a safety device or interlock unless such individual has obtained the approval of the radiation safety officer. Such approval shall be for a specified period of time. When a safety device or interlock has been bypassed, a readily discernible sign bearing the words "SAFETY DEVICE NOT WORKING", or words having a similar intent, shall be placed on the radiation source housing.

C. Repair or modification of X-ray tube systems. Except as specified in 12VAC5-481-2450 B, no operation involving removal of covers, shielding materials or tube housings or modifications to shutters, collimators, or beam stops shall be performed without ascertaining that the tube is off and will remain off until safe conditions have been restored. The main switch, rather than interlocks, shall be used for routine shutdown in preparation for repairs.

D. Radioactive source replacement, testing, or repair. Radioactive source housings shall be opened for source replacement, leak testing, or other maintenance or repair procedures only by individuals authorized to specifically conduct such procedures under a license issued by the Nuclear Regulatory Commission, an agreement state, or a

licensing state.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2130. Personnel requirements.

A. Instruction. No individual shall be permitted to operate or maintain analytical X-ray equipment unless such individual has received instruction in and demonstrated competence as to:

1. Identification of radiation hazards associated with the use of the equipment;
2. Significance of the various radiation warning, safety devices, and interlocks incorporated into the equipment, or the reasons they have not been installed on certain pieces of equipment and the extra precautions required in such cases;
3. Proper operating procedures for the equipment;
4. Recognition of symptoms of an acute localized exposure; and
5. Proper procedures for reporting an actual or suspected exposure.

B. Personnel monitoring.

1. Finger or wrist dosimetric devices shall be provided to and shall be used by:
 - a. Analytical X-ray equipment workers using systems having an open-beam configuration and not equipped with a safety device; and
 - b. Personnel maintaining analytical X-ray equipment if the maintenance procedures require the presence of a primary X-ray beam when any local component in the analytical X-ray system is disassembled or removed.
2. Reported dose values shall not be used for the purpose of determining compliance with 12VAC5-481-630 of these regulations unless evaluated by a private inspector.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Part IX

Radiation Safety Requirements For Particle Accelerators

Article 1

Purpose and Scope

12VAC5-481-2140. Purpose and scope.

A. This part establishes procedures for the registration and the use of particle accelerators.

B. In addition to the requirements of this part, all registrants are subject to the requirements of Parts I (12VAC5-481-10 et seq.), II (12VAC5-481-260 et seq.), III (12VAC5-481-380 et seq.), IV (12VAC5-481-600 et seq.), and X (12VAC5-481-2250 et seq.) of this chapter. Registrants engaged in industrial radiographic operations are subject to the requirements of Part V (12VAC5-481-1170 et seq.) of this chapter, and registrants engaged in the healing arts are subject to the requirements of Parts VI (12VAC5-481-1580 et seq.) and VII (12VAC5-481-1660 et seq.) of this chapter. Registrants whose operations result in the production of radioactive material are subject to the requirements of Part III (12VAC5-481-380 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 2

Registration Procedures

12VAC5-481-2150. Registration requirements.

No person shall receive, possess, use, transfer, own, or acquire a particle accelerator except as authorized in a registration issued pursuant to Part II (12VAC5-

481-260 et seq.) or III (12VAC5-481-380 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2160. General requirements for the issuance of a registration for particle accelerators.

In addition to the requirements of Part II (12VAC5-481-260 et seq.) or III (12VAC5-481-380 et seq.) of this chapter, a registration application for use of a particle accelerator will be approved only if the agency determines that:

1. The applicant is qualified by reason of training and experience to use the accelerator in question for the purpose requested in accordance with this part and Parts IV (12VAC5-481-600 et seq.) and X (12VAC5-481-2250 et seq.) of this chapter in such a manner as to minimize danger to public health and safety or property;
2. The applicant's proposed or existing equipment, facilities, and operating and emergency procedures are adequate to protect health and minimize danger to public health and safety or property;
3. The issuance of the registration will not be inimical to the health and safety of the public, and the applicant satisfies any applicable special requirement in 12VAC5-481-2170;
4. The applicant has appointed a radiation safety officer;
5. The applicant and the applicant's staff have substantial experience in the use of particle accelerators and training sufficient for application to its intended uses;
6. The applicant has established a radiation safety committee to approve, in advance, proposals for uses of particle accelerators, whenever deemed necessary by the agency; and
7. The applicant has an adequate training program for operators of particle

accelerators.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2170. Human use of particle accelerators.

In addition to the requirements of Part II (12VAC5-481-260 et seq.) of this chapter, a registration for use of a particle accelerator in the healing arts will be issued only if:

1. The applicant has appointed a medical committee of at least three members to evaluate all proposals for research, diagnostic, and therapeutic use of a particle accelerator whenever deemed necessary by the agency. Membership of the committee should include physicians expert in internal medicine, hematology, therapeutic radiology, and a person experienced in depth dose calculations and protection against radiation;
2. The individuals designated on the application as the users have substantial training and experience in deep therapy techniques or in the use of particle accelerators to treat humans; and
3. The individual designated on the application as the user is a physician.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 3

Radiation Safety Requirements for Use of Particle Accelerators

12VAC5-481-2180. Limitations.

A. No registrant shall permit any individual to act as an operator of a particle accelerator until such individual:

1. Has been instructed in radiation safety and shall have demonstrated an understanding thereof;
2. Has received copies of and instruction in this part and the applicable requirements of Parts IV (12VAC5-481-600 et seq.) and X (12VAC5-481-2250 et seq.) of this chapter, pertinent registration conditions and the registrant's operating and emergency procedures, and shall have demonstrated understanding thereof; and
3. Has demonstrated competence to use the particle accelerator, related equipment, and survey instruments that will be employed.

B. The radiation safety committee or the radiation safety officer shall have the authority to terminate the operations at a particle accelerator facility if such action is deemed necessary to minimize danger to public health and safety or property.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2190. Shielding and safety design requirements.

A. A private inspector, acceptable to the agency, shall be consulted in the design of a particle accelerator installation and called upon to perform a radiation survey when the accelerator is first capable of producing radiation.

B. Each particle accelerator installation shall be provided with such primary and secondary barriers as are necessary to assure compliance with 12VAC5-481-630.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2200. Particle accelerator controls and interlock systems.

A. Instrumentation, readouts, and controls on the particle accelerator control console shall be clearly identified and easily discernible.

B. Each entrance into a target room or other high radiation area shall be provided with a safety interlock that shuts down the machine under conditions of barrier penetration.

C. Each safety interlock shall be on a circuit that shall allow it to operate independently of all other safety interlocks.

D. All safety interlocks shall be designed so that any defect or component failure in the safety interlock system prevents operation of the accelerator.

E. When a safety interlock system has been tripped, it shall only be possible to resume operation of the accelerator by manually resetting controls at the position where the safety interlock has been tripped and, lastly, at the main control console.

F. A scram button or other emergency power cutoff switch shall be located and easily identifiable in all high radiation areas. Such a cutoff switch shall include a manual reset so that the accelerator cannot be restarted from the accelerator control console without resetting the cutoff switch.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2210. Warning devices.

A. Each location designated as a high radiation area, and each entrance to such location, shall be equipped with easily observable warning lights that operate when, and only when, radiation is being produced.

B. Except in facilities designed for human exposure, each high radiation area shall have an audible warning device which shall be activated for 15 seconds prior to the possible creation of such high radiation area. Such warning device shall be clearly discernible in all high radiation areas.

C. Barriers, temporary or otherwise, and pathways leading to high radiation areas shall be posted in accordance with 12VAC5-481-660.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2220. Operating procedures.

A. Particle accelerators, when not in operation, shall be secured to prevent unauthorized use.

B. The safety interlock system shall not be used to turn off the accelerator beam except in an emergency.

C. All safety and warning devices, including interlocks, shall be checked for proper operation at intervals not to exceed three months. Results of such tests shall be maintained at the accelerator facility for inspection by the agency.

D. Electrical circuit diagrams of the accelerator and the associated safety interlock systems shall be kept current and maintained for inspection by the agency and shall be available to the operator at each accelerator facility.

E. If, for any reason, it is necessary to intentionally bypass a safety interlock or interlocks, such action shall be:

1. Authorized by the radiation safety committee or radiation safety officer;
2. Recorded in a permanent log and a notice posted at the accelerator control console; and
3. Terminated as soon as possible.

F. A copy of the current operating and the emergency procedures shall be maintained at the accelerator control panel.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2230. Radiation monitoring requirements.

A. There shall be available at each particle accelerator facility appropriate portable monitoring equipment that is operable and has been appropriately calibrated for the radiations being produced at the facility. Such equipment shall be tested for proper operation daily and calibrated at intervals not to exceed one year and after each servicing and repair.

B. A radiation survey shall be performed and documented by a private inspector, acceptable to the agency, when changes have been made in shielding, operation, equipment, or occupancy of adjacent areas.

C. Radiation levels in all high radiation areas shall be continuously monitored. The monitoring devices shall be electrically independent of the accelerator control and safety interlock systems and capable of providing a readout at the control panel.

D. All area monitors shall be calibrated at intervals not to exceed one year and after each servicing and repair.

E. Whenever applicable, periodic surveys shall be made to determine the amount of airborne particulate radioactivity present.

F. Whenever applicable, periodic smear surveys shall be made to determine the degree of contamination.

G. All surveys shall be made in accordance with the written procedures established by a private inspector, acceptable to the agency, or the radiation safety officer.

H. Records of all radiation protection surveys, calibrations, and instrumentation tests shall be maintained at the accelerator facility.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2240. Ventilation systems.

A. Ventilation systems shall be provided to ensure that personnel entering any area where airborne radioactivity may be produced will not be exposed to airborne radioactive material in excess of those limits specified in 12VAC5-481-3690.

B. A registrant, as required in 12VAC5-481-3690 shall not vent, release, or otherwise discharge airborne radioactive material to an unrestricted area which exceeds the limits specified in 12VAC5-481-3690, except as authorized pursuant to 12VAC5-481-730. For purposes of this subsection concentrations may be averaged over a period not greater than one year. Every effort should be made to maintain releases of radioactive material to unrestricted areas as far below these limits as is reasonably achievable.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part X

Notices, Instructions, and Reports to Workers; Inspections

12VAC5-481-2250. Purpose and scope.

This part establishes requirements for notices, instructions and reports by licensees or registrants to individuals engaged in activities under a license or registration and options available to such individuals in connection with agency inspections of licensees or registrants to ascertain compliance with the provisions of the Act and regulations, orders, and licenses issued thereunder regarding radiological working conditions. The regulations in this part apply to all persons who receive, possess, use, own, or transfer sources of radiation registered with or licensed by the agency pursuant to Parts II (12VAC5-481-260 et seq.) and III (12VAC5-481-380 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2260. Posting of notices to workers.

A. Each licensee or registrant shall post current copies of the following documents:

1. The regulations in this part and in Part IV (12VAC5-481-600 et seq.) of this chapter;
2. The license, certificate of registration, conditions or documents incorporated into the license by reference and amendments thereto;
3. The operating procedures applicable to activities under the license or registration;
4. Any notice of violation involving radiological working conditions, proposed imposition of civil penalty, or order issued pursuant to Part I (12VAC5-481-10 et seq.) of this chapter, and any response from the licensee or registrant; and
5. Agency form "Notice to Employees" as required by these regulations.

B. If posting of a document specified in subdivisions A 1 through 3 of this section is not practicable, the licensee or registrant may post a notice that describes the document and states where it may be examined.

C. Agency documents posted pursuant to subdivision A 4 of this section shall be posted within two working days after receipt of the documents from the agency; the licensee's or registrant's response, if any, shall be posted within five working days after dispatch from the licensee or registrant. Such documents shall remain posted for a minimum of five working days or until action correcting the violation has been completed, whichever is later.

D. Documents, notices, or forms posted pursuant to this section shall appear in a sufficient number of places to permit individuals engaged in work under the license or registration to observe them on the way to or from any particular work location to which

the document applies, shall be conspicuous, and shall be replaced if defaced or altered.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2270. Instructions to workers.

A. All individuals likely to receive in a year an occupational dose in excess of 1 mSv (100 mrem):

1. Shall be kept informed of the storage, transfer, or use of sources of radiation in the licensee's or registrant's workplace;
2. Shall be instructed in the health protection problems associated with exposure to radiation or radioactive material to the individual and potential offspring, in precautions or procedures to minimize exposure, and in the purposes and functions of protective devices employed;
3. Shall be instructed in, and instructed to observe, to the extent within the worker's control, the applicable provisions of these regulations and licenses for the protection of personnel from exposures to radiation or radioactive material;
4. Shall be instructed of their responsibility to report promptly to the licensee or registrant any condition that may constitute, lead to, or cause a violation of the Act, these regulations, or license condition, or any unnecessary exposure to radiation or radioactive material;
5. Shall be instructed in the appropriate response to warnings made in the event of any unusual occurrence or malfunction that may involve exposure to radiation or radioactive material; and
6. Shall be advised as to the radiation exposure reports that workers shall be furnished pursuant to 12VAC5-481-2280.

B. The extent of these instructions shall be commensurate with potential radiological health protection problems present in the workplace.

C. The instructions listed in subsection A of this section shall be given at least annually to said individuals.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2280. Notifications and reports to individuals.

A. Radiation exposure data for an individual and the results of any measurements, analyses, and calculations of radioactive material deposited or retained in the body of an individual shall be reported to the individual as specified in this section. The information reported shall include data and results obtained pursuant to these regulations, orders, or license conditions, as shown in records maintained by the licensee or registrant pursuant to 12VAC5-481-1040. Each notification and report shall:

1. Be in writing;
2. Include appropriate identifying data such as the name of the licensee or registrant, the name of the individual, and the individual's identification number;
3. Include the individual's exposure information; and
4. Contain the following statement:

"This report is furnished to you under the provisions of Part X (12VAC5-481-2250 et seq.) of 12VAC5-481, Virginia Radiation Protection Regulations. You should preserve this report for further reference."

B. Each licensee shall make dose information available to workers as shown in records maintained by the licensee under the provisions of 12VAC5-481-1040. The licensee shall provide an annual report to each individual monitored under 12VAC5-481-760 of the dose received in that monitoring year if:

1. The individual's occupational dose exceeds 1 mSv (100 mrem) TEDE or 1 mSv (100 mrem) to any individual organ or tissue; or
2. The individual requests his annual dose report.

C. Each licensee or registrant shall furnish a written report of the worker's exposure to sources of radiation at the request of a worker formerly engaged in activities controlled by the licensee or registrant. The report shall include the dose record for each year the worker was required to be monitored pursuant to 12VAC5-481-760. Such report shall be furnished within 30 days from the date of the request, or within 30 days after the dose of the individual has been determined by the licensee or registrant, whichever is later. The report shall cover the period of time that the worker's activities involved exposure to sources of radiation and shall include the dates and locations of work under the license or registration in which the worker participated during this period.

D. When a licensee or registrant is required pursuant to 12VAC5-481-1100, 12VAC5-481-1110, or 12VAC5-481-1120 to report to the agency any exposure of an individual to sources of radiation, the licensee or the registrant shall also provide the individual a written report on the exposure data included therein. Such reports shall be transmitted at a time not later than the transmittal to the agency.

E. At the request of a worker who is terminating employment with the licensee or registrant in work involving exposure to radiation or radioactive material, during the current year, each licensee or registrant shall provide at termination to each such worker, or to the worker's designee, a written report regarding the radiation dose received by that worker from operations of the licensee or registrant during the current year or fraction thereof. If the most recent individual monitoring results are not available at that time, a written estimate of the dose shall be provided together with a clear indication that this is an estimate.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2290. Presence of representatives of licensees or registrants and workers during inspection.

A. Each licensee or registrant shall afford to the agency at all reasonable times opportunity to inspect materials, machines, activities, facilities, premises, and records pursuant to these regulations.

B. During an inspection, agency inspectors may consult privately with workers as specified in 12VAC5-481-2300. The licensee or registrant may accompany agency inspectors during other phases of an inspection.

C. If, at the time of inspection, an individual has been authorized by the workers to represent them during agency inspections, the licensee or registrant shall notify the inspectors of such authorization and shall give the workers' representative an opportunity to accompany the inspectors during the inspection of physical working conditions.

D. Each workers' representative shall be routinely engaged in work under control of the licensee or registrant and shall have received instructions as specified in 12VAC5-481-2270.

E. Different representatives of licensees or registrants and workers may accompany the inspectors during different phases of an inspection if there is no resulting interference with the conduct of the inspection. However, only one workers' representative at a time may accompany the inspectors.

F. With the approval of the licensee or registrant and the workers' representative, an individual who is not routinely engaged in work under control of the licensee or registrant, for example, a consultant to the licensee or registrant or to the workers' representative, shall be afforded the opportunity to accompany agency inspectors during the inspection of physical working conditions.

G. Notwithstanding the other provisions of 12VAC5-481-2290, agency inspectors are

authorized to refuse to permit accompaniment by any individual who deliberately interferes with a fair and orderly inspection. With regard to areas containing information classified by an agency of the United States government in the interest of national security, an individual who accompanies an inspector may have access to such information only if authorized to do so. With regard to any area containing proprietary information, the workers' representative for that area shall be an individual previously authorized by the licensee or registrant to enter that area.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2300. Consultation with workers during inspections.

A. Agency inspectors may consult privately with workers concerning matters of occupational radiation protection and other matters related to applicable provisions of these regulations and licenses to the extent the inspectors deem necessary for the conduct of an effective and thorough inspection.

B. During the course of an inspection, any worker may bring privately to the attention of the inspectors, either orally or in writing, any past or present condition that the worker has reason to believe may have contributed to or caused any violation of the Act, these regulations, or license condition, or any unnecessary exposure of an individual to sources of radiation under the licensee's or registrant's control. Any such notice in writing shall comply with the requirements of 12VAC5-481-2310 A.

C. The provisions of subsection B of this section shall not be interpreted as authorization to disregard instructions pursuant to 12VAC5-481-2270.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2310. Requests by workers for inspections.

A. Any worker or representative of workers believing that a violation of the Act, these regulations, or license conditions exists or has occurred in work under a license or registration with regard to radiological working conditions in which the worker is engaged may request an inspection by giving notice of the alleged violation to the agency. Any such notice shall be in writing, shall set forth the specific grounds for the notice, and shall be signed by the worker or representative of the workers. A copy shall be provided to the licensee or registrant by the agency no later than at the time of inspection except that, upon the request of the worker giving such notice, such worker's name and the name of individuals referred to therein shall not appear in such copy or on any record published, released, or made available by the agency, except for good cause shown.

B. If, upon receipt of such notice, the agency determines that the complaint meets the requirements set forth in subsection A of this section, and that there are reasonable grounds to believe that the alleged violation exists or has occurred, an inspection shall be made as soon as practicable to determine if such alleged violation exists or has occurred. Inspections pursuant to this section need not be limited to matters referred to in the complaint.

C. No licensee, registrant, or contractor or subcontractor of a licensee or registrant shall discharge or in any manner discriminate against any worker because such worker has filed any complaint or instituted or caused to be instituted any proceeding under these regulations or has testified or is about to testify in any such proceeding or because of the exercise by such worker on behalf of such worker or others of any option afforded by this part.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2320. Inspections not warranted; informal review.

A. Do the following:

1. If the agency determines, with respect to a complaint under 12VAC5-481-2310, that an inspection is not warranted because there are no reasonable grounds to believe that a violation exists or has occurred, the agency shall notify the complainant in writing of such determination. The complainant may obtain review of such determination by submitting a written statement of position with the agency. The agency will provide the licensee or registrant with a copy of such statement by certified mail, excluding, at the request of the complainant, the name of the complainant. The licensee or registrant may submit an opposing written statement of position with the agency. The agency will provide the complainant with a copy of such statement by certified mail.

2. Upon the request of the complainant, the agency may hold an informal conference in which the complainant and the licensee or registrant may orally present their views. An informal conference may also be held at the request of the licensee or registrant, but disclosure of the identity of the complainant will be made only following receipt of written authorization from the complainant. After considering all written and oral views presented, the agency shall affirm, modify, or reverse the determination of the agency and furnish the complainant and the licensee or registrant a written notification of the decision and the reason therefor.

B. If the agency determines that an inspection is not warranted because the requirements of 12VAC5-481-2310 A have not been met, the complainant shall be notified in writing of such determination. Such determination shall be without prejudice to the filing of a new complaint meeting the requirements of 12VAC5-481-2310 A.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Part XI

Licensing Requirements for Land Disposal of Radioactive Waste

Article 1

Purpose and Scope

12VAC5-481-2330. Purpose and scope.

A. The regulations in this part establish procedures, criteria, and terms and conditions upon which the agency issues licenses for the land disposal of wastes received from other persons. The requirements of this part are in addition to, and not in substitution for, other applicable requirements of these regulations.

B. The regulations in this part do not apply to disposal of byproduct material as defined in the definition of "byproduct material" in these regulations in quantities greater than 10,000 kilograms containing more than 185 MBq (5 mCi) of radium-226 or disposal of radioactive material as provided for in Part IV (12VAC5-481-600 et seq.) of this chapter.

C. This part establishes procedural requirements and performance objectives applicable to any method of land disposal. It establishes specific technical requirements for near-surface disposal of radioactive waste that involves disposal in the uppermost portion of the earth.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 2

General Regulatory Provisions

12VAC5-481-2340. License required.

A. No person may receive, possess, and dispose of waste received from other

persons at a land disposal facility unless authorized by a license issued by the agency pursuant to this part and Part III (12VAC5-481-380 et seq.) of this chapter.

B. Each person shall file an application with the agency pursuant to 12VAC5-481-440 and obtain a license as provided in this part before commencement of construction of a land disposal facility. Failure to comply with this requirement may be grounds for denial of a license.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2350. Content of application.

In addition to the requirements set forth in 12VAC5-481-450, an application to receive from others, possess, and dispose of wastes shall consist of general information, specific technical information, institutional information, and financial information as set forth in 12VAC5-481-2360 through 12VAC5-481-2400.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2360. General information.

The general information shall include each of the following:

1. Identity of the applicant including:

- a. The full name, address, telephone number, and description of the business or occupation of the applicant;
- b. If the applicant is a partnership, the name and address of each partner and the principal location where the partnership does business;
- c. If the applicant is a corporation or an unincorporated association, (i) the

state where it is incorporated or organized and the principal location where it does business, and (ii) the names and addresses of its directors and principal officers; and

d. If the applicant is acting as an agent or representative of another person in filing the application, all information required under this subsection must be supplied with respect to the other person.

2. Qualifications of the applicant:

a. The organizational structure of the applicant, both offsite and onsite, including a description of lines of authority and assignments of responsibilities, whether in the form of administrative directives, contract provisions, or otherwise;

b. The technical qualifications, including training and experience, of the applicant and members of the applicant's staff to engage in the proposed activities. Minimum training and experience requirements for personnel filling key positions described in subdivision 2 a of this section must be provided.

c. A description of the applicant's personnel training program; and

d. The plan to maintain an adequate complement of trained personnel to carry out waste receipt, handling, and disposal operations in a safe manner.

3. A description of:

a. The location of the proposed disposal site;

b. The general character of the proposed activities;

c. The types and quantities of waste to be received, possessed, and disposed of;

d. Plans for use of the land disposal facility for purposes other than disposal of wastes; and

e. The proposed facilities and equipment.

4. Proposed schedules for construction, receipt of waste, and first emplacement of waste at the proposed land disposal facility.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2370. Specific technical information.

The specific technical information shall include the following information needed for demonstration that the performance objectives and the applicable technical requirements of this part will be met:

1. A description of the natural and demographic disposal site characteristics as determined by disposal site selection and characterization activities. The description shall include geologic, geochemical, geotechnical, hydrologic, ecologic, archaeologic, meteorologic, climatologic, and biotic features of the disposal site and vicinity.
2. A description of the design features of the land disposal facility and the disposal units. For near-surface disposal, the description shall include those design features related to infiltration of water; integrity of covers for disposal units; structural stability of backfill, wastes, and covers; contact of wastes with standing water; disposal site drainage; disposal site closure and stabilization; elimination to the extent practicable of long-term disposal site maintenance; inadvertent intrusion; occupational exposures; disposal site monitoring; and adequacy of the size of the buffer zone for monitoring and potential mitigative measures.
3. A description of the principal design criteria and their relationship to the performance objectives.
4. A description of the design basis natural events or phenomena and their relationship to the principal design criteria.
5. A description of codes and standards that the applicant has applied to the design and that will apply to construction of the land disposal facilities.

6. A description of the construction and operation of the land disposal facility. The description shall include as a minimum the methods of construction of disposal units; waste emplacement; the procedures for and areas of waste segregation; types of intruder barriers; onsite traffic and drainage systems; survey control program; methods and areas of waste storage; and methods to control surface water and groundwater access to the wastes. The description shall also include a description of the methods to be employed in the handling and disposal of wastes containing chelating agents or other nonradiological substances that might affect meeting the performance objectives of this part.

7. A description of the disposal site closure plan, including those design features that are intended to facilitate disposal site closure and to eliminate the need for ongoing active maintenance.

8. An identification of the known natural resources at the disposal site, whose exploitation could result in inadvertent intrusion into the wastes after removal of active institutional control.

9. A description of the kind, amount, classification and specifications of the radioactive material proposed to be received, possessed, and disposed of at the land disposal facility.

10. A description of the quality control program for the determination of natural disposal site characteristics and for quality control during the design, construction, operation, and closure of the land disposal facility and the receipt, handling, and emplacement of waste. Audits and managerial controls must be included.

11. A description of the radiation safety program for control and monitoring of radioactive effluents to ensure compliance with the performance objective in 12VAC5-481-2490 and occupational radiation exposure to ensure compliance with the requirements of Part IV (12VAC5-481-600 et seq.) of this chapter and to control contamination of personnel, vehicles, equipment, buildings, and the disposal site. Both routine operations and accidents shall be addressed. The

program description must include procedures, instrumentation, facilities, and equipment.

12. A description of the environmental monitoring program to provide data to evaluate potential health and environmental impacts and the plan for taking corrective measures if migration is indicated.

13. A description of the administrative procedures that the applicant will apply to control activities at the land disposal facility.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2380. Technical analyses.

The specific technical information shall also include the following analyses needed to demonstrate that the performance objectives of this part will be met:

1. Pathways analyzed in demonstrating protection of the general population from releases of radioactivity shall include air, soil, groundwater, surface water, plant uptake, and exhumation by burrowing animals. The analyses shall clearly identify and differentiate between the roles performed by the natural disposal site characteristics and design features in isolating and segregating the wastes. The analyses shall clearly demonstrate that there is reasonable assurance that the exposures to humans from the release of radioactivity will not exceed the limits set forth in 12VAC5-481-2490.

2. Analyses of the protection of individuals from inadvertent intrusion shall include demonstration that there is reasonable assurance the waste classification and segregation requirements will be met and that adequate barriers to inadvertent intrusion will be provided.

3. Analyses of the protection of individuals during operations shall include assessments of expected exposures due to routine operations and likely

accidents during handling, storage, and disposal of waste. The analyses shall provide reasonable assurance that exposures will be controlled to meet the requirements of Part IV (12VAC5-481-600 et seq.) of this chapter.

4. Analyses of the long-term stability of the disposal site and the need for ongoing active maintenance after closure shall be based upon analyses of active natural processes such as erosion, mass wasting, slope failure, settlement of wastes and backfill, infiltration through covers over disposal areas and adjacent soils, and surface drainage of the disposal site. The analyses shall provide reasonable assurance that there will not be a need for ongoing active maintenance of the disposal site following closure.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2390. Institutional information.

The institutional information submitted by the applicant shall include:

1. A certification by the federal or state agency that owns the disposal site that the federal or state agency is prepared to accept transfer of the license when the provisions of 12VAC5-481-2460 are met and will assume responsibility for institutional control after site closure and post-closure observation and maintenance.
2. Where the proposed disposal site is on land not owned by the federal or a state government, the applicant shall submit evidence that arrangements have been made for assumption of ownership in fee by the federal or a state agency before the agency issues a license.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2400. Financial information.

The financial information shall be sufficient to demonstrate that the financial qualifications of the applicant are adequate to carry out the activities for which the license is sought and meet other financial assurance requirements of this part.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2410. Requirements for issuance of a license.

A license for the receipt, possession, and disposal of waste containing or contaminated with radioactive material will be issued by the agency upon finding that:

1. The issuance of the license will not constitute an unreasonable risk to the health and safety of the public;
2. The applicant is qualified by reason of training and experience to carry out the disposal operations requested in a manner that protects health and minimizes danger to life or property;
3. The applicant's proposed disposal site, disposal design, land disposal facility operations, including equipment, facilities, and procedures, disposal site closure, and post-closure institutional control are adequate to protect the public health and safety in that they provide reasonable assurance that the general population will be protected from releases of radioactivity as specified in the performance objective in 12VAC5-481-2490;
4. The applicant's proposed disposal site, disposal site design, land disposal facility operations, including equipment, facilities, and procedures, disposal site closure, and post-closure institutional control are adequate to protect the public health and safety in that they will provide reasonable assurance that individual inadvertent intruders are protected in accordance with the performance objective

in 12VAC5-481-2520;

5. The applicant's proposed land disposal facility operations, including equipment, facilities, and procedures, are adequate to protect the public health and safety in that they will provide reasonable assurance that the standards for radiation protection set out in Part IV (12VAC5-481-600 et seq.) of this chapter will be met;

6. The applicant's proposed disposal site, disposal site design, land disposal facility operations, disposal site closure, and post-closure institutional control are adequate to protect the public health and safety in that they will provide reasonable assurance that long-term stability of the disposed waste and the disposal site will be achieved and will eliminate to the extent practicable the need for ongoing active maintenance of the disposal site following closure;

7. The applicant's demonstration provides reasonable assurance that the applicable technical requirements of this part will be met;

8. The applicant's proposal for institutional control provides reasonable assurance that such control will be provided for the length of time found necessary to ensure the findings in subdivisions 3 through 6 of this section and that the institutional control meets the requirements of 12VAC5-481-2580; and

9. The financial or surety arrangements meet the requirements of this part.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2420. Conditions of licenses.

A. A license issued under this part, or any right thereunder, may be transferred, assigned, or in any manner disposed of, either voluntarily or involuntarily, directly or indirectly, through transfer of control of the license to any person, only if the agency finds, after securing full information, that the transfer is in accordance with the

provisions of the Act and gives its consent in writing in the form of a license amendment.

B. The licensee shall submit written statements under oath upon request of the agency, at any time before termination of the license, to enable the agency to determine whether the license should be modified, suspended, or revoked.

C. The license will be terminated only on the full implementation of the final closure plan as approved by the agency, including post-closure observation and maintenance.

D. The licensee shall be subject to the provisions of the Act now or hereafter in effect, and to all rules, regulations, and orders of the agency. The terms and conditions of the license are subject to amendment, revision, or modification, by reason of amendments to, or by reason of rules, regulations, and orders issued in accordance with the terms of the Act.

E. Each person licensed by the agency pursuant to the regulations in this part shall confine possession and use of materials to the locations and purposes authorized in the license.

F. The licensee shall not dispose of waste until the agency has inspected the land disposal facility and has found it to be in conformance with the description, design, and construction described in the application for a license.

G. The agency may incorporate in any license at the time of issuance, or thereafter, by appropriate rule, regulation or order, additional requirements and conditions with respect to the licensee's receipt, possession, and disposal of waste as it deems appropriate or necessary in order to:

1. Protect health or to minimize danger to life or property;
2. Require reports and the keeping of records, and to provide for inspections of activities under the license that may be necessary or appropriate to effectuate the purposes of the Act and regulations thereunder.

H. The authority to dispose of wastes expires on the date stated in the license. Any expiration date on a license applies only to the above ground activities and to the

authority to dispose of waste. Failure to renew the license shall not relieve the licensee of responsibility for implementing site closure, post-closure observation, and transfer of the license to the site owner.

I. Each licensee shall notify the agency in writing immediately following the filing of a voluntary or involuntary petition for bankruptcy under any Chapter of Title 11 (Bankruptcy) of the United States Code by or against:

1. The licensee;
2. An entity (as that term is defined in 11 USC §101(15)) controlling the licensee or listing the license or licensee as property of the estate; or
3. An affiliate (as that term is defined in 11 USC §101(2)) of the licensee.

J. The notification specified in this section shall indicate the bankruptcy court in which the petition for bankruptcy was filed and the date of the filing of the petition.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2430. Application for renewal or closure.

A. An application for renewal or an application for closure under 12VAC5-481-2440 must be filed at least 90 days prior to license expiration.

B. Applications for renewal of a license must be filed in accordance with 12VAC5-481-2350 through 12VAC5-481-2400. Applications for closure must be filed in accordance with 12VAC5-481-2440.

C. In any case in which a licensee has filed an application in proper form for renewal of a license, the license does not expire until the agency has taken final action on the application for renewal.

D. In determining whether a license will be renewed, the agency will apply the criteria set forth in 12VAC5-481-2410.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2440. Contents of application for site closure and stabilization.

A. Prior to final closure of the disposal site, or as otherwise directed by the agency, the applicant shall submit an application to amend the license for closure. This closure application shall include a final revision and specific details of the disposal site closure plan included as part of the license application submitted under subdivision 7 of 12VAC5-481-2370 that includes each of the following:

1. Any additional geologic, hydrologic, or other data pertinent to the long-term containment of emplaced wastes obtained during the operational period.
2. The results of tests, experiments, or any other analyses relating to backfill of excavated areas, closure and sealing, waste migration and interaction with emplacement media, or any other tests, experiments, or analysis pertinent to the long-term containment of emplaced waste within the disposal site.
3. Any proposed revision of plans for:
 - a. Decontamination and/or dismantlement of surface facilities;
 - b. Backfilling of excavated areas; or
 - c. Stabilization of the disposal site for post-closure care.
4. Any significant new information regarding the environmental impact of closure activities and long-term performance of the disposal site.

B. Upon review and consideration of an application to amend the license for closure submitted in accordance with subsection A of this section, the agency shall issue an amendment authorizing closure if there is reasonable assurance that the long-term performance objectives of this part will be met.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2450. Post-closure observation and maintenance.

The licensee shall observe, monitor, and carry out necessary maintenance and repairs at the disposal site until the site closure is complete and the license is transferred by the agency in accordance with 12VAC5-481-2460. Responsibility for the disposal site must be maintained by the licensee for five years. A shorter or longer time period for post-closure observation and maintenance may be established and approved as part of the site closure plan, based on site-specific conditions.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2460. Transfer of license.

Following closure and the period of post-closure observation and maintenance, the licensee may apply for an amendment to transfer the license to the disposal site owner.

The license shall be transferred when the agency finds:

1. That the closure of the disposal site has been made in conformance with the licensee's disposal site closure plan, as amended and approved as part of the license;
2. That reasonable assurance has been provided by the licensee that the performance objectives of this part are met;
3. That any funds and necessary records for care will be transferred to the disposal site owner;
4. That the post-closure monitoring program is operational for implementation by the disposal site owner; and
5. That the federal or state agency that will assume responsibility for institutional

control of the disposal site is prepared to assume responsibility and ensure that the institutional requirements found necessary under subdivision 8 of 12VAC5-481-2410 will be met.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2470. Termination of license.

A. Following any period of institutional control needed to meet the requirements found necessary under 12VAC5-481-2410, the licensee may apply for an amendment to terminate the license.

B. This application will be reviewed in accordance with the provisions of 12VAC5-481-450.

C. A license shall be terminated only when the agency finds:

1. That the institutional control requirements found necessary under 12VAC5-481-2410 8 have been met;
2. That any additional requirements resulting from new information developed during the institutional control period have been met; and
3. That permanent monuments or markers warning against intrusion have been installed.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 3

General Performance Objectives

12VAC5-481-2480. General requirement.

Land disposal facilities shall be sited, designed, operated, closed, and controlled after closure so that reasonable assurance exists that exposures to individuals are within the requirements established in the performance objectives in 12VAC5-481-2490 through 12VAC5-481-2520.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2490. Protection of the general population from releases of radioactivity.

Concentrations of radioactive material that may be released to the general environment in ground water, surface water, air, soil, plants, or animals shall not result in an annual dose exceeding an equivalent of 0.25 mSv (25 mrem) to the whole body, 0.75 mSv (75 mrem) to the thyroid, and 0.25 mSv (25 mrem) to any other organ of any member of the public. Reasonable effort should be made to maintain releases of radioactivity in effluents to the general environment ALARA.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2500. Protection of individuals from inadvertent intrusion.

Design, operation, and closure of the land disposal facility shall ensure protection of any individual inadvertently intruding into the disposal site and occupying the site or contacting the waste at any time after active institutional controls over the disposal site are removed.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2510. Protection of individuals during operations.

Operations at the land disposal facility shall be conducted in compliance with the standards for radiation protection set out in Part IV (12VAC5-481-600 et seq.) of this chapter, except for releases of radioactivity in effluents from the land disposal facility, that shall be governed by 12VAC5-481-2490. Every reasonable effort should be made to maintain radiation exposures ALARA.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2520. Stability of the disposal site after closure.

The disposal facility shall be sited, designed, used, operated, and closed to achieve long-term stability of the disposal site and to eliminate, to the extent practicable, the need for ongoing active maintenance of the disposal site following closure so that only surveillance, monitoring, or minor custodial care are required.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 4

Technical Requirements for Land Disposal Facilities

12VAC5-481-2530. Disposal site suitability requirements for land disposal.

Disposal site suitability for near-surface disposal. The primary emphasis in disposal

site suitability is given to isolation of wastes and to disposal site features that ensure that the long-term performance objectives are met.

1. The disposal site shall be capable of being characterized, modeled, analyzed and monitored.
2. Within the region where the facility is to be located, a disposal site should be selected so that projected population growth and future developments are not likely to affect the ability of the disposal facility to meet the performance objectives of this part.
3. Areas shall be avoided having known natural resources which, if exploited, would result in failure to meet the performance objectives of this part.
4. The disposal site shall be generally well drained and free of areas of flooding or frequent ponding. Waste disposal shall not take place in a 100-year flood plain, coastal high-hazard area or wetland, as defined in federal Executive Order 11988, "Floodplain Management Guidelines."
5. Upstream drainage areas shall be minimized to decrease the amount of runoff which could erode or inundate waste disposal units.
6. The disposal site shall provide sufficient depth to the water table that ground water intrusion, perennial or otherwise, into the waste will not occur. The agency will consider an exception to this requirement to allow disposal below the water table if it can be conclusively shown that disposal site characteristics will result in molecular diffusion being the predominant means of radionuclide movement and the rate of movement will result in the performance objectives being met. In no case will waste disposal be permitted in the zone of fluctuation of the water table.
7. The hydrogeologic unit used for disposal shall not discharge ground water to the surface within the disposal site.
8. Areas shall be avoided where tectonic processes such as faulting, folding, seismic activity, or vulcanism may occur with such frequency and extent to significantly affect the ability of the disposal site to meet the performance objectives of this part or may preclude defensible modeling and prediction of

long-term impacts.

9. Areas shall be avoided where surface geologic processes such as mass wasting, erosion, slumping, landsliding, or weathering occur with such frequency and extent to significantly affect the ability of the disposal site to meet the performance objectives of this part, or may preclude defensible modeling and prediction of long-term impacts.

10. The disposal site must not be located where nearby facilities or activities could adversely impact the ability of the site to meet the performance objectives of this part or significantly mask the environmental monitoring program.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2540. Disposal site design for land disposal.

Disposal site design for near-surface disposal.

1. Site design features shall be directed toward long-term isolation and avoidance of the need for continuing active maintenance after site closure.
2. The disposal site design and operation shall be compatible with the disposal site closure and stabilization plan and lead to disposal site closure that provides reasonable assurance that the performance objectives will be met.
3. The disposal site shall be designed to complement and improve, where appropriate, the ability of the disposal site's natural characteristics to assure that the performance objectives will be met.
4. Covers shall be designed to minimize to the extent practicable water infiltration, to direct percolating or surface water away from the disposed waste, and to resist degradation by surface geologic processes and biotic activity.
5. Surface features shall direct surface water drainage away from disposal units

at velocities and gradients that will not result in erosion that will require ongoing active maintenance in the future.

6. The disposal site shall be designed to minimize to the extent practicable the contact of water with waste during storage, the contact of standing water with waste during disposal, and the contact of percolating or standing water with wastes after disposal.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2550. Land disposal facility operation and disposal site closure.

Near-surface disposal facility operation and disposal site closure.

1. Wastes designated as Class A pursuant to these regulations shall be segregated from other wastes by placing in disposal units which are sufficiently separated from disposal units for the other waste classes so that any interaction between Class A wastes and other wastes will not result in the failure to meet the performance objectives of this part. This segregation is not necessary for Class A wastes if they meet the stability requirements of these regulations.

2. Wastes designated as Class C pursuant to these regulations shall be disposed of so that the top of the waste is a minimum of 5 meters below the top surface of the cover or must be disposed of with intruder barriers that are designed to protect against an inadvertent intrusion for at least 500 years.

3. Except as provided in subdivision 12 of this subsection, only waste classified as Class A, B, or C shall be acceptable for near-surface disposal. All waste shall be disposed of in accordance with requirements of 4 through 11 of this subsection.

4. Wastes shall be emplaced in a manner that maintains the package integrity

during emplacement, minimizes the void spaces between packages, and permits the void spaces to be filled.

5. Void spaces between waste packages shall be filled with earth or other material to reduce future subsidence within the fill.

6. Waste shall be placed and covered in a manner that limits the radiation dose rate at the surface of the cover to levels that at a minimum will permit the licensee to comply with all provisions of 12VAC5-481-640 at the time the license is transferred pursuant to 12VAC5-481-2460.

7. The boundaries and locations of each disposal unit shall be accurately located and mapped by means of a land survey. Near-surface disposal units shall be marked in such a way that the boundaries of each unit can be easily defined. Three permanent survey marker control points, referenced to United States Geological Survey (USGS) or National Geodetic Survey (NGS) survey control stations, shall be established on the site to facilitate surveys. The USGS or NGS control stations shall provide horizontal and vertical controls as checked against USGS or NGS record files.

8. A buffer zone of land shall be maintained between any buried waste and the disposal site boundary and beneath the disposed waste. The buffer zone shall be of adequate dimensions to carry out environmental monitoring activities specified in 12VAC5-481-2560 C and take mitigative measures if needed.

9. Closure and stabilization measures as set forth in the approved site closure plan shall be carried out as each disposal unit is filled and covered.

10. Active waste disposal operations shall not have an adverse effect on completed closure and stabilization measures.

11. Only wastes containing or contaminated with radioactive material shall be disposed of at the disposal site.

12. Proposals for disposal of waste that is not generally acceptable for near-surface disposal because the waste form and disposal methods must be different and, in general, more stringent than those specified for Class C waste, may be

submitted to the agency for approval.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2560. Environmental monitoring.

A. At the time a license application is submitted, the applicant shall have conducted a preoperational monitoring program to provide basic environmental data on the disposal site characteristics. The applicant shall obtain information about the ecology, meteorology, climate, hydrology, geology including geophysics and geotechnical engineering, geochemistry, and seismology of the disposal site. For those characteristics that are subject to seasonal variation, data must cover at least a 12-month period.

B. During the land disposal facility site construction and operation, the licensee shall maintain an environmental monitoring program. Measurements and observations must be made and recorded to provide data to evaluate the potential health and environmental impacts during both the construction and the operation of the facility and to enable the evaluation of long-term effects and the need for mitigative measures. The monitoring system must be capable of providing early warning of releases of waste from the disposal site before they leave the site boundary.

C. After the disposal site is closed, the licensee responsible for post-operational surveillance of the disposal site shall maintain a monitoring system based on the operating history and the closure and stabilization of the disposal site. The monitoring system must be capable of providing early warning of releases of waste from the disposal site before they leave the site boundary.

D. The licensee shall have plans for taking corrective measures if the environmental monitoring program detects migration of waste which would indicate that the

performance objectives may not be met.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2570. Alternative requirements for design and operations.

The agency may, upon request or on its own initiative, authorize provisions other than those set forth in 12VAC5-481-2540 through 12VAC5-481-2560 for the segregation and disposal of waste and for the design and operation of a land disposal facility on a specific basis, if it finds reasonable assurance of compliance with the performance objectives of this part.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2571. Waste classification.

A. Considerations. Determination of the classification of radioactive waste involves two considerations. First, consideration must be given to the concentration of long-lived radionuclides (and their shorter-lived precursors) whose potential hazard will persist long after such precautions as institutional controls, improved waste form, and deeper disposal have ceased to be effective. These precautions delay the time when long-lived radionuclides could cause exposures. In addition, the magnitude of the potential dose is limited by the concentration and availability of the radionuclide at the time of exposure. Second, consideration must be given to the concentration of shorter-lived radionuclides for which requirements on institutional controls, waste form, and disposal methods are effective.

B. Classes of waste.

1. Class A waste is waste that is usually segregated from other waste classes at

the disposal site. The physical form and characteristics of Class A waste must meet the minimum requirements set forth in 12VAC5-481-2572 A. If Class A waste also meets the stability requirements set forth in 12VAC5-481-2572 B, it is not necessary to segregate the waste for disposal.

2. Class B waste is waste that must meet more rigorous requirements on waste form to ensure stability after disposal. The physical form and characteristics of Class B waste must meet both the minimum and stability requirements set forth in 12VAC5-481-2572.

3. Class C waste is waste that not only must meet more rigorous requirements on waste form to ensure stability but also requires additional measures at the disposal facility to protect against inadvertent intrusion. The physical form and characteristics of Class C waste must meet both the minimum and stability requirements set forth 12VAC5-481-2572.

4. Waste that is not generally acceptable for near-surface disposal is waste for which form and disposal methods must be different, and in general more stringent, than those specified for Class C waste. In the absence of specific requirements in this part, such waste must be disposed of in a geologic repository as defined in 10 CFR Part 60 or 63 unless proposals for disposal of such waste in a disposal site licensed pursuant to this part are approved by the agency.

C. Classification determined by long-lived radionuclides. If radioactive waste contains only radionuclides listed in Table 2, classification shall be determined as follows:

1. If the concentration does not exceed 0.1 times the value in Table 2, the waste is Class A.
2. If the concentration exceeds 0.1 times the value in Table 2 but does not exceed the value in Table 3, the waste is Class C.
3. If the concentration exceeds the value in Table 2, the waste is not generally acceptable for near-surface disposal.

4. For wastes containing mixtures of radionuclides listed in Table 2, the total concentration shall be determined by the sum of fractions rule described in subsection G of this section.

Table 2
Long Lived Radionuclides Waste Concentration

Radionuclide	Concentration curies per cubic meter
C-14	8
C-14 in activated metal	80
Ni-59 in activated metal	220
Nb-94 in activated metal	0.2
Tc-99	3
I-129	0.08
Alpha emitting transuranic nuclides with half-life greater than 5 years	¹ 100
Pu-241	¹ 3,500
Cm-242	¹ 20,000

¹Units are nanocuries per gram.

D. Classification determined by short-lived radionuclides. If radioactive waste does not contain any of the radionuclides listed in Table 2, classification shall be determined based on the concentrations shown in Table 3. However, as specified in subsection F of this section, if radioactive waste does not contain any nuclides listed in either Table 2 or 3, it is Class A.

1. If the concentration does not exceed the value in Column 1, the waste is Class A.
2. If the concentration exceeds the value in Column 1, but does not exceed the value in Column 2, the waste is Class B.
3. If the concentration exceeds the value in Column 2, but does not exceed the value in Column 3, the waste is Class C.
4. If the concentration exceeds the value in Column 3, the waste is not generally acceptable for near-surface disposal.
5. For wastes containing mixtures of the nuclides listed in Table 3, the total

concentration shall be determined by the sum of fractions rule described in subsection G of this section.

Table 3
Short Lived Radionuclide Waste Concentration

Radionuclide	Concentration, curies per cubic meter		
	Col. 1	Col. 2	Col. 3
Total of all nuclides with less than 5 year half-life	700	(1)	(1)
H-3	40	(1)	(1)
Co-60	700	(1)	(1)
Ni-63	3.5	70	700
Ni-63 in activated metal	35	700	7000
Sr-90	0.04	150	7000
Cs-137	1	44	4600

¹There are no limits established for these radionuclides in Class B or C wastes. Practical considerations such as the effects of external radiation and internal heat generation on transportation, handling, and disposal will limit the concentrations for these wastes. These wastes shall be Class B unless the concentrations of other nuclides in Table 3 determine the waste to the Class C independent of these nuclides.

E. Classification determined by both long- and short-lived radionuclides. If radioactive waste contains a mixture of radionuclides, some of which are listed in Table 2, and some of which are listed in Table 3, classification shall be determined as follows:

1. If the concentration of a nuclide listed in Table 2 does not exceed 0.1 times the value listed in Table 2, the class shall be that determined by the concentration of nuclides listed in Table 3.
2. If the concentration of a nuclide listed in Table 2 exceeds 0.1 times the value listed in Table 2 but does not exceed the value in Table 2, the waste shall be Class C, provided the concentration of nuclides listed in Table 3 does not exceed the value shown in Column 3 of Table 3.

F. Classification of wastes with radionuclides other than those listed in Tables 2 and 3. If radioactive waste does not contain any nuclides listed in either Table 2 or 3, it is Class A.

G. The sum of the fractions rule for mixtures of radionuclides. For determining classification for waste that contains a mixture of radionuclides, it is necessary to determine the sum of fractions by dividing each nuclide's concentration by the appropriate limit and adding the resulting values. The appropriate limits must all be taken from the same column of the same table. The sum of the fractions for the column must be less than 1.0 if the waste class is to be determined by that column. Example: A waste contains Sr-90 in a concentration of 50 Ci/m³ and Cs-137 in a concentration of 22 Ci/m³. Since the concentrations both exceed the values in Column 1, Table 2, they must be compared to Column 2 values. For Sr-90 fraction $50/150=0.33$; for Cs-137 fraction, $22/44=0.5$; the sum of the fractions= 0.83 . Since the sum is less than 1.0, the waste is Class B.

H. Determination of concentrations in wastes. The concentration of a radionuclide may be determined by indirect methods such as use of scaling factors that relate the inferred concentration of one radionuclide to another that is measured, or radionuclide material accountability, if there is reasonable assurance that the indirect methods can be correlated with actual measurements. The concentration of a radionuclide may be averaged over the volume of the waste, or weight of the waste if the units are expressed as nanocuries per gram.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2572. Waste characteristics.

A. The following requirements are minimum requirements for all classes of waste and are intended to facilitate handling at the disposal site and provide protection of health and safety of personnel at the disposal site.

1. Waste must not be packaged for disposal in cardboard or fiberboard boxes.
2. Liquid waste must be solidified or packaged in sufficient absorbent material to

absorb twice the volume of the liquid.

3. Solid waste containing liquid shall contain as little freestanding and noncorrosive liquid as is reasonably achievable, but in no case shall the liquid exceed 1.0% of the volume.

4. Waste must not be readily capable of detonation or of explosive decomposition or reaction at normal pressures and temperatures, or of explosive reaction with water.

5. Waste must not contain, or be capable of generating, quantities of toxic gases, vapors, or fumes harmful to persons transporting, handling, or disposing of the waste. This does not apply to radioactive gaseous waste packaged in accordance with subdivision 7 of this subsection.

6. Waste must not be pyrophoric. Pyrophoric materials contained in waste shall be treated, prepared, and packaged to be nonflammable.

7. Waste in a gaseous form must be packaged at a pressure that does not exceed 1.5 atmospheres at 20°C. Total activity must not exceed 100 curies per container.

8. Waste containing hazardous, biological, pathogenic, or infectious material must be treated to reduce to the maximum extent practicable the potential hazard from the nonradiological materials.

B. The requirements in this section are intended to provide stability of the waste. Stability is intended to ensure that the waste does not structurally degrade and affect overall stability of the site through slumping, collapse, or other failure of the disposal unit and thereby lead to water infiltration. Stability is also a factor in limiting exposure to an inadvertent intruder, since it provides a recognizable and nondispersible waste.

1. Waste must have structural stability. A structurally stable waste form will generally maintain its physical dimensions and its form, under the expected disposal conditions such as weight of overburden and compaction equipment, the presence of moisture, and microbial activity, and internal factors such as radiation effects and chemical changes. Structural stability can be provided by

the waste form itself, processing the waste to a stable form, or placing the waste in a disposal container or structure that provides stability after disposal.

2. Notwithstanding the provisions in subdivision A 2 and A 3 of this section, liquid wastes, or wastes containing liquid, must be converted into a form that contains as little freestanding and noncorrosive liquid as is reasonably achievable, but in no case shall the liquid exceed 1.0% of the volume of the waste when the waste is in a disposal container designed to ensure stability, or 0.5% of the volume of the waste for waste processed to a stable form.

3. Void spaces within the waste and between the waste and its package must be reduced to the extent practicable.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2573. Labeling.

Each package of waste must be clearly labeled to identify whether it is Class A waste, Class B waste, or Class C waste, in accordance with 12VAC5-481-2571.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2580. Institutional requirements.

A. Land ownership. Disposal of waste received from other persons may be permitted only on land owned in fee by the federal or a state government.

B. Institutional control. The land owner or custodial agency shall conduct an institutional control program to physically control access to the disposal site following transfer of control of the disposal site from the disposal site operator. The institutional control program shall also include, but not be limited to, conducting an environmental

monitoring program at the disposal site, periodic surveillance, minor custodial care, and other requirements as determined by the agency; and administration of funds to cover the costs for these activities. The period of institutional controls will be determined by the agency, but institutional controls may not be relied upon for more than 100 years following transfer of control of the disposal site to the owner.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2590. Alternative requirements for waste classification and characteristics.

The agency licensing a low-level disposal facility may, upon request or on its own initiative, authorize other provisions for the classification and characteristics of waste on a specific basis, if, after evaluation of the specific characteristics of the waste, disposal site, method of disposal, it finds reasonable assurance of compliance with the performance objectives specified in this part.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 5

Financial Assurances

12VAC5-481-2600. Applicant qualifications and assurances.

Each applicant shall show that it either possesses the necessary funds or has reasonable assurance of obtaining the necessary funds, or by a combination of the two, to cover the estimated costs of conducting all licensed activities over the planned operating life of the project, including costs of construction and disposal.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2610. Funding for disposal site closure and stabilization.

A. The applicant shall provide assurances prior to the commencement of operations that sufficient funds will be available to carry out disposal site closure and stabilization, including: (i) decontamination or dismantlement of land disposal facility structures; and (ii) closure and stabilization of the disposal site so that following transfer of the disposal site to the site owner the need for ongoing active maintenance is eliminated to the extent practicable and only minor custodial care, surveillance, and monitoring are required. These assurances shall be based on agency-approved cost estimates reflecting the agency-approved plan for disposal site closure and stabilization. The applicant's cost estimates must take into account total costs that would be incurred if an independent contractor were hired to perform the closure and stabilization work.

B. In order to avoid unnecessary duplication and expense, the agency will accept financial sureties that have been consolidated with earmarked financial or surety arrangements established to meet requirements of federal or other state agencies (and/or local governmental bodies) for such decontamination, closure, and stabilization. The agency will accept these arrangements only if they are considered adequate to satisfy the requirements of this section and that the portion of the surety that covers the closure of the disposal site is clearly identified and committed for use in accomplishing these activities.

C. The licensee's financial or surety arrangement shall be submitted annually for review by the agency to assure that sufficient funds will be available for completion of the closure plan.

D. The amount of the licensee's financial or surety arrangement shall change in accordance with changes in the predicted costs of closure and stabilization. Factors affecting closure and stabilization cost estimates include inflation, increases in the amount of disturbed land, changes in engineering plans, closure and stabilization that

has already been accomplished, and any other conditions affecting costs. The financial or surety arrangement shall be sufficient at all times to cover the costs of closure and stabilization of the disposal units that are expected to be used before the next license renewal.

E. The financial or surety arrangement shall be either open-ended or be written for a specified period of time and shall be automatically renewed unless the person who issues the surety notifies the agency, the beneficiary (the site owner), and the principal (the licensee) not less than 90 days prior to the renewal date of its intention not to renew. In such a situation, the licensee must submit a replacement surety within 30 days after notification of cancellation. If the licensee fails to provide a replacement surety acceptable to the agency, the beneficiary may collect on the original surety.

F. Proof of forfeiture shall not be necessary to collect the surety so that, in the event that the licensee could not provide an acceptable replacement surety within the required time, the surety shall be automatically collected prior to its expiration. The conditions described above shall be clearly stated on any surety instrument.

G. Financial or surety arrangements generally acceptable to the agency include surety bonds, cash deposits, certificates of deposit, deposits of government securities, escrow accounts, irrevocable letters or lines of credit, trust funds, and combinations of the above or such other types of arrangements as may be approved by the agency. Self-insurance, or any arrangement that essentially constitutes self-insurance, will not satisfy the surety requirement for private sector applicants.

H. The licensee's financial or surety arrangement shall remain in effect until the closure and stabilization program has been completed and approved by the agency, and the license has been transferred to the site owner.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2620. Financial assurances for institutional controls.

A. Prior to the issuance of the license, the applicant shall provide for agency approval, a binding arrangement, between the applicant and the disposal site owner that ensures that sufficient funds will be available to cover the costs of monitoring and any required maintenance during the institutional control period. The binding arrangement shall be reviewed periodically by the agency to ensure that changes in inflation, technology, and disposal facility operations are reflected in the arrangements.

B. Subsequent changes to the binding arrangement specified in subsection A of this section relevant to institutional control shall be submitted to the agency for prior approval.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 6

Records, Reports, Tests, and Inspections

12VAC5-481-2630. Maintenance of records, reports, and transfers.

A. Each licensee shall maintain any records and make any reports in connection with the licensed activities as may be required by the conditions of the license or by the rules, regulations, and orders of the agency.

B. Records that are required by these regulations or by license conditions shall be maintained for a period specified by the appropriate regulations or by license condition. If a retention period is not otherwise specified, these records must be maintained and transferred to the officials specified in subsection D of this section as a condition of license termination unless the agency otherwise authorizes their disposition.

C. Records that shall be maintained pursuant to this part may be the original or a reproduced copy or microfilm if this reproduced copy or microfilm is capable of producing copy that is clear and legible at the end of the required retention period.

D. Notwithstanding subsections A through C of this section, copies of records of the location and the quantity of wastes contained in the disposal site must be transferred upon license termination to the chief executive of the nearest municipality, the chief executive of the county in which the facility is located, the county zoning board or land development and planning agency, the state governor, and other state, local and federal governmental agencies as designated by the agency at the time of license termination.

E. Following receipt and acceptance of a shipment of waste, the licensee shall record the date of disposal of the waste, the location in the disposal site, the condition of the waste packages as received, any discrepancies between materials listed on the manifest and those received, and any evidence of leaking or damaged packages or radiation or contamination levels in excess of limits specified in United States Department of Transportation and agency regulations. The licensee shall briefly describe any repackaging operations of any of the waste packages included in the shipment, plus any other information required by the agency as a license condition.

F. Each licensee authorized to dispose of waste received from other persons shall file a copy of its financial report or a certified financial statement annually with the agency in order to update the information base for determining financial qualifications.

G. Do the following:

1. Each licensee authorized to dispose of waste received from other persons, pursuant to this part, shall submit annual reports to the agency. Reports shall be submitted by the end of the first calendar quarter of each year for the preceding year.

2. The reports shall include:

- a. Specification of the quantity of each of the principal contaminants released to unrestricted areas in liquid and in airborne effluents during the preceding year,

- b. The results of the environmental monitoring program,

- c. A summary of licensee disposal unit survey and maintenance activities,

- d. A summary, by waste class, of activities and quantities of radionuclides disposed of,
 - e. Any instances in which observed site characteristics were significantly different from those described in the application for a license, and
 - f. Any other information the agency may require.
3. If the quantities of waste released during the reporting period, monitoring results, or maintenance performed are significantly different from those predicted, the report must cover this specifically.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2640. Tests on land disposal facilities.

Each licensee shall perform, or permit the agency to perform, any tests the agency deems appropriate or necessary for the administration of the regulations in this part, including, but not limited to, tests of:

1. Wastes;
2. Facilities used for the receipt, storage, treatment, handling or disposal of wastes;
3. Radiation detection and monitoring instruments;
4. Other equipment and devices used in connection with the receipt, possession, handling, treatment, storage, or disposal of waste; or
5. Environmental sampling or testing.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2650. Agency inspections of land disposal facilities.

A. Each licensee shall afford to the agency at all reasonable times opportunity to inspect waste not yet disposed of, and the premises, equipment, operations, and facilities in which wastes are received, possessed, handled, treated, stored, or disposed of.

B. Each licensee shall make available to the agency for inspection, upon reasonable notice, records kept by it pursuant to these regulations. Authorized representatives of the agency may copy and take away copies of, for the agency's use, any record required to be kept pursuant to these regulations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Part XII

Licensing and Radiation Safety Requirements for Irradiators

Article 1

Purpose and Scope

12VAC5-481-2660. Purpose and scope.

The following regulation, Purpose and scope (10 CFR 36.1) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 2

Specific Licensing Requirements

12VAC5-481-2670. Application for a specific license.

The following regulation, Application for a specific license (10 CFR 36.11) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2680. Specific licenses for irradiators.

The following regulation, Specific licenses for irradiators (10 CFR 36.13) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2690. Start of construction.

The following regulation, Start of construction (10 CFR 36.15) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2700. Applications for exemptions.

The following regulation, Applications for exemptions (10 CFR 36.17) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2710. Request for written statements.

The following regulation, Request for written statements (10 CFR 36.19) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 3**Design and Performance Requirements for Irradiators****12VAC5-481-2720. Performance criteria for sealed sources.**

The following regulation, Performance criteria for sealed sources (10 CFR 36.21) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2730. Access control.

The following regulation, Access control (10 CFR 36.23) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2740. Shielding.

The following regulation, Shielding (10 CFR 36.25) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2750. Fire protection.

The following regulation, Fire protection (10 CFR 36.27) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2760. Radiation monitors.

The following regulation, Radiation monitors (10 CFR 36.29) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006;

amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2770. Control of source movement.

The following regulation, Control of source movement (10 CFR 36.31) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2780. Irradiator pools.

The following regulation, Irradiator pools (10 CFR 36.33) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2790. Source rack protection.

The following regulation, Source rack protection (10 CFR 36.35) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2800. Power failures.

The following regulation, Power failures (10 CFR 36.37) is applicable in the

Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2810. Design requirements.

The following regulation, Design requirements (10 CFR 36.39) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2820. Construction monitoring and acceptance testing.

The following regulation, Construction monitoring and acceptance testing (10 CFR 36.41) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 4

Operation of Irradiators

12VAC5-481-2830. Training.

The following regulation, Training (10 CFR 36.51) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2840. Operating and emergency procedures.

The following regulation, Operating and emergency procedures (10 CFR 36.53) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2850. Personnel monitoring.

The following regulation, Personnel monitoring (10 CFR 36.55) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2860. Radiation surveys.

The following regulation, Radiation surveys (10 CFR 36.57) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2870. Detection of leaking sources.

The following regulation, Detection of leaking sources (10 CFR 36.58) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2880. Inspection and maintenance.

The following regulation, Inspection and maintenance (10 CFR 36.61) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2890. Pool water purity.

The following regulation, Pool water purity (10 CFR 36.63) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2900. Attendance during operation.

The following regulation, Attendance during operation (10 CFR 36.65) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2910. Entering and leaving the radiation room.

The following regulation, Entering and leaving the radiation room (10 CFR 36.67) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2920. Irradiation of explosive or flammable materials.

The following regulation, Irradiation of explosive or flammable materials (10 CFR 36.69) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 5

Records

12VAC5-481-2930. Records and retention periods.

The following regulation, Records and retention periods (10 CFR 36.81) is applicable

in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2940. Reports.

The following regulation, Reports (10 CFR 36.83) is applicable in the Commonwealth of Virginia

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part XIII

Transportation of Radioactive Material

Article 1

Purpose and Scope

12VAC5-481-2950. Purpose and scope.

The regulations in this part apply to any licensee authorized by specific or general license issued by the agency to receive, possess, use, or transfer licensed material, if the licensee delivers that material to a carrier for transport, transports the material outside the site of usage as specified in the agency license, or transports that material on public highways. No provision of this part authorizes possession of licensed material.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 2

General Regulatory Provisions

12VAC5-481-2960. Requirement for license.

No person shall transport radioactive material or deliver radioactive material to a carrier for transport except as authorized in a general or specific license issued by the agency or as exempted in 12VAC5-481-2970.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-2970. Exemptions.

A. Common and contract carriers, freight forwarders, and warehouse workers that are subject to the requirements of the United States Department of Transportation (DOT) in 49 CFR Part 170 through 49 Part CFR 189 or the United States Postal Service in the Postal Service Domestic Mail Manual (DMM), Section C-023.9.0, and the United States Postal Service, are exempt from the requirements of this part to the extent that they transport or store radioactive material in the regular course of their carriage for others or storage incident thereto. Common and contract carriers that are not subject to the requirements of the DOT or United States Postal Service are subject to 12VAC5-481-2960 and other applicable requirements of these regulations.

B. A licensee is exempt from all the requirements of this part with respect to shipment or carriage of the following low-level materials:

1. NARM and ores containing naturally occurring radionuclides that are not intended to be processed for use of these radionuclides, provided the activity concentration of the material does not exceed 10 times the values specified in Table A-2 of 12VAC5-481-3770.

2. Materials for which the activity concentration is not greater than the activity concentration values specified in Table A-2 of 12VAC5-481-3770, or for which the consignment activity is not greater than the limit for an exempt consignment found in Table A-2 of 12VAC5-481-3770.

C. Fissile material meeting one of the following requirements are exempt from classification as fissile material and from the fissile material package standards of 10 CFR 71.55 and 71.59, but are subject to all other requirements of 10 CFR 71, except as noted.

1. Individual package containing two grams or less fissile material.

2. Individual or bulk packaging containing 15 grams or less of fissile material provided the package has at least 200 grams of solid nonfissile material for every gram of fissile material. Lead, beryllium, graphite, and hydrogenous material enriched in deuterium may be present in the package but must not be included in determining the required mass for solid nonfissile material.

3. Low concentrations of solid fissile material commingled with solid nonfissile material, provided that there is at least 2,000 grams of solid nonfissile material for every gram of fissile material, and there is no more than 180 grams of fissile material distributed within 360 kg of contiguous nonfissile material. Lead, beryllium, graphite, and hydrogenous material enriched in deuterium may be present in the package but must not be included in determining the required mass of solid nonfissile material.

4. Uranium enriched in uranium-235 to a maximum of 1.0% by weight, and with total plutonium and uranium-233 content of up to 1.0% of the mass of uranium-235, provided that the mass of any beryllium, graphite, and hydrogenous material enriched in deuterium constitutes less than 5.0% of the uranium mass.

5. Liquid solutions of uranyl nitrate enriched in uranium-235 to a maximum of 2.0% by mass, with a total plutonium and uranium-233 content not exceeding 0.002% of the mass of uranium, and with a minimum nitrogen to uranium atomic ratio (N/U) of 2. The material must be contained in at least a DOT Type A

package.

6. Packages containing, individually, a total plutonium mass of not more than 1,000 grams, of which not more than 20% by mass may consist of plutonium-239, plutonium-241, or any combination of these radionuclides.

D. Any physician licensed by the Commonwealth of Virginia to dispense drugs in the practice of medicine is exempt from this section with respect to transport by the physician of radioactive material for use in the practice of medicine provided the physician is an authorized user under Part VII (12VAC5-481-1660 et seq.).

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-2980. Transportation of licensed material.

A. Each licensee who transports licensed material outside the site of usage, as specified in the agency license, or where transport is on public highways, or who delivers licensed material to a carrier for transport, shall:

1. Comply with the applicable requirements, appropriate to the mode of transport, of the regulations of the DOT; particularly the regulations of the DOT in the following areas:

- a. Packaging – 49 CFR Part 173: Subparts A and B and I.
- b. Marking and labeling – 49 CFR Part 172: Subpart D, 172.400 through 172.407 and 172.436 through 172.441.
- c. Placarding – 49 CFR Part 172: Subpart F, especially §§172.500 through 172.519, 172.556, and Appendices B and C.
- d. Accident reporting – 49 CFR Part 171: §§171.15 and 171.16.
- e. Shipping papers and emergency information – 49 CFR Part 172: Subpart C and Subpart G.

- f. Hazardous material employee training – 49 CFR Part 172: Subpart H.
 - g. Hazardous material shipper/carrier registration – 49 CFR Part 107: Subpart G.
 - h. Security plans – 49 CFR Part 172: Subpart I.
2. The licensee shall also comply with applicable DOT regulations pertaining to the following modes of transportation:
- a. Rail – 49 CFR Part 174: Subparts A through D and K.
 - b. Air – 49 CFR Part 175.
 - c. Vessel – 49 CFR Part 176: Subparts A through F and M.
 - d. Public Highway – 49 CFR Part 177 and Parts 390 through 397.
3. Assure that any special instructions needed to safely open the package are sent to or have been made available to the consignee in accordance with 12VAC5-481-900.

B. If, for any reason, the regulations of the DOT are not applicable to a shipment of licensed material, the licensee shall conform to the standards and requirements of 49 CFR Parts 107, 171 through 180, and 390 through 397, appropriate to the mode of transport to the same extent as if the shipment was subject to the regulations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 3

General Licenses

12VAC5-481-2990. General licenses for carriers.

A. A general license is hereby issued to any common or contract carrier not exempt under 12VAC5-481-2970 to receive, possess, transport, and store radioactive material

in the regular course of their carriage for others or storage incident thereto, provided the transportation and storage is in accordance with the applicable requirements, appropriate to the mode of transport, of the United States Department of Transportation insofar as such requirements relate to the loading and storage of packages, placarding of the transporting vehicle, and incident reporting. Notification of an incident shall be filed with, or made to, the agency as prescribed in 49 CFR, regardless of or in addition to notification made to the United States Department of Transportation or other agencies.

B. A general license is hereby issued to any private carrier to transport radioactive material, provided the transportation is in accordance with the applicable requirements, appropriate to the mode of transport, of the United States Department of Transportation insofar as such requirements relate to the loading and storage of packages, placarding of the transporting vehicle, and incident reporting. Notification of an incident shall be filed with, or made to, the agency as prescribed in 49 CFR, regardless of or in addition to notification made to the United States Department of Transportation or other agencies.

C. Persons who transport radioactive material pursuant to the general licenses in subsection A or B of this section are exempt from the requirements of Parts IV (12VAC5-481-600 et seq.) and X (12VAC5-481-2250 et seq.) of this chapter to the extent that they transport radioactive material.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3000. General license: NRC-approved packages.

A. A general license is hereby issued to any licensee to transport, or to deliver to a carrier for transport, licensed material in a package for which a license, certificate of compliance (CoC), or other approval has been issued by the NRC.

B. This general license applies only to a licensee who:

1. Has a copy of the specific license, CoC, or other approval by the NRC of the package and has the drawings and other documents referenced in the approval relating to the use and maintenance of the packaging and to the actions to be taken prior to shipment;
2. Complies with the terms and conditions of the license, certificate, or other approval by the NRC, as applicable, and the applicable requirements of Part XIII (12VAC5-481-2950 et seq.) of this chapter;
3. Prior to the licensee's first use of the package, submits in writing to the NRC the licensee's name and license number and the package identification number specified in the package approval using the appropriate method listed in 10 CFR 71.1(a); and
4. Has a quality assurance program that complies with 12VAC5-481-3130.

C. The general license in subsection A of this section applies only when the package approval authorizes use of the package under this general license.

D. For a Type B or fissile material package, the design of which was approved by the NRC before April 1, 1996, the general license is subject to the additional restrictions of 12VAC5-481-3010.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3010. Previously approved packages.

A Type B(U) package, a Type B(M) package or a fissile material package, previously approved by the NRC but without the designation "-85" in the identification number of the NRC CoC, may be used under the general license of 12VAC5-481-3000 with the following additional conditions:

1. Fabrication of the package is satisfactorily completed by April 1, 1999, as demonstrated by application of its model number in accordance with 10 CFR 71.85(c);
2. A package used for a shipment to a location outside the United States is subject to multilateral approval except approved under special arrangement in accordance with United States Department of Transportation regulations at 49 CFR 173.403; and
3. A serial number that uniquely identifies each packaging that conforms to the approved design is assigned to and legibly and durably marked on the outside of each packaging.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3020. General License: United States Department of Transportation specification container.

A. A general license is issued to any licensee to transport, or to deliver to a carrier for transport, licensed material in a specification container for fissile material or for a Type B quantity of radioactive material as specified in 49 CFR Parts 173 and 178.

B. This general license applies only to a licensee who:

1. Has a copy of the specification;
2. Complies with the terms and conditions of the specification and the applicable requirements of this part; and
3. Has a quality assurance program that complies with 12VAC5-481-3130.

C. The general license in subsection A of this section is subject to the limitation that the specification container may not be used for a shipment to a location outside the United States except by multilateral approval as defined in 49 CFR 173.403.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3030. General License: use of foreign approved package.

A. A general license is issued to any licensee to transport, or to deliver to a carrier for transport, licensed material in a package the design of which has been approved in a foreign national competent authority certificate that has been revalidated by the DOT as meeting the applicable requirements of 49 CFR 171.12.

B. This general license applies only to international shipments.

C. This general license applies only to a licensee who:

1. Has a copy of the applicable certificate, the revalidation, and the drawings and other documents referenced in the certificate relating to the use and maintenance of the packaging and to the actions to be taken prior to shipment;
2. Complies with the terms and conditions of the certificate and revalidation, and with the applicable requirements of this part; and
3. The licensee has a quality assurance program that complies with 12VAC5-481-3130.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3040. General license: fissile material.

A. A general license is issued to any licensee to transport fissile material, or to deliver fissile material to a carrier for transport, if the material is shipped in accordance

with this section. The fissile material need not be contained in a package that meets the standards of 10 CFR Part 71, Subparts E and F; however, the material must be contained in a Type A package. The Type A package must also meet the DOT requirements of 49 CFR 173.417(a).

B. The general license applies only to a licensee who has a quality assurance program that complies with 12VAC5-481-3130.

C. The general license applies only when a package's contents:

1. Contain no more than a Type A quantity of radioactive material; and
2. Contain less than 500 total grams of beryllium, graphite, or hydrogenous material enriched in deuterium.

D. The general license applies only to packages containing fissile material that are labeled with a CSI that:

1. Has been determined in accordance with subsection E of this section;
2. Has a value less than or equal to 10; and
3. For a shipment of multiple packages containing fissile material, the sum of the CSIs must be less than or equal to 50 (for shipment on a nonexclusive use conveyance) and less than or equal to 100 (for shipment on an exclusive use conveyance).

E. The value for the CSI must be greater than or equal to the number calculated by the following equation:

1. The calculated CSI must be rounded up to the first decimal place;
2. The values of X, Y, and Z used in the CSI equation must be taken from Tables 5 or 6, as appropriate;
3. If Table 5 is used to obtain the value of X, then the values for the terms in the equation for uranium-233 and plutonium must be assumed to be zero; and
4. Table 4 values for X, Y, and Z must be used to determine the CSI if:

- a. Uranium-233 is present in the package;
- b. The mass of plutonium exceeds one percent of the mass of uranium-235;
- c. The uranium is of unknown uranium-235 enrichment or greater than 24 weight percent enrichment; or
- d. Substances having a moderating effectiveness (i.e., an average hydrogen density greater than H₂O) (e.g., certain hydrocarbon oils or plastics) are present in any form, except as polyethylene used for packing or wrapping.

Table 4

Mass Limits for General License Packages Containing Mixed Quantities of Fissile Material or Uranium-235 of Unknown Enrichment

Fissile material	Fissile material mass mixed with moderating substances having an average hydrogen density less than or equal to H ₂ O (grams)	Fissile material mass mixed with moderating substances having an average hydrogen density greater than H ₂ O ^a (grams)
U-235 (X)	60	38
U-233 (Y)	43	27
Pu-239 or Pu-241 (Z)	37	24

^aWhen mixtures of moderating substances are present, the lower mass limits shall be used if more than 15 percent of the moderating substance has an average hydrogen density greater than H₂O.

Table 5

Mass Limits for General License Packages Containing Uranium-235 of Known Enrichment

Uranium enrichment in weight percent of U-235 not exceeding	Fissile material mass of U-235 (X) (grams)
24	60
20	63
15	67
11	72
10	76
9.5	78
9	81

8.5	82
8	85
7.5	88
7	90
6.5	93
6	97
5.5	102
5	108
4.5	114
4	120
3.5	132
3	150
2.5	180
2	246
1.5	408
1.35	480
1	1,020
0.92	1,800

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3050. (Repealed.)

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; repealed, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3051. General license: plutonium-beryllium special form material.

A. A general license is issued to any licensee to transport fissile material in the form

of plutonium-beryllium (Pu-Be) special form sealed sources, or to deliver Pu-Be sealed sources to a carrier for transport, if the material is shipped in accordance with this section. This material need not be contained in a package that meets the standards of Subparts E and F of 10 CFR Part 71; however, the material must be contained in a Type A package. The Type A package must also meet the DOT requirements of 49 CFR 173.417(a).

B. The general license applies only to a licensee who has a quality assurance program that complies with 12VAC5-481-3130.

C. The general license applies only when a package's contents:

1. Contain no more than a Type A quantity of radioactive material; and
2. Contain less than 1,000 grams of plutonium, provided that: plutonium-239, plutonium-241, or any combination of these radionuclides, constitutes less than 240 grams of the total quantity of plutonium in the package.

D. The general license applies only to packages labeled with a CSI that:

1. Has been determined in accordance with subsection E of this section;
2. Has a value less than or equal to 100; and
3. For a shipment of multiple packages containing Pu-Be sealed sources, the sum of the CSIs must be less than or equal to 50 (for shipment on a nonexclusive use conveyance) and less than or equal to 100 (for shipment on an exclusive use conveyance).

E. The value for the CSI must be greater than or equal to the number calculated by the following equation:

<input type="checkbox"/>

The calculated CSI must be rounded up to the first decimal place.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 4

Operating Controls and Procedures

12VAC5-481-3060. Assumptions as to unknown properties of fissile material.

When the isotopic abundance, mass, concentration, degree of irradiation, degree of moderation, or other pertinent property of fissile material in any package is not known, the licensee shall package the fissile material as if the unknown properties have credible values that will cause the maximum neutron multiplication.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3070. Preliminary determinations.

Prior to the first use of any packaging for the shipment of radioactive material:

1. The licensee shall ascertain that there are no cracks, pinholes, uncontrolled voids, or other defects which could significantly reduce the effectiveness of the packaging;
2. Where the maximum normal operating pressure will exceed 35 kilopascal (5 lbf/in²) gauge, the licensee shall test the containment system at an internal pressure at least 50% higher than the maximum normal operating pressure to verify the capability of that system to maintain its structural integrity at that pressure;
3. The licensee shall determine that the packaging has been fabricated in accordance with the design approved by the NRC; and
4. The licensee shall conspicuously and durably mark the packaging with its model number, serial number, gross weight, and a package identification number as assigned by the NRC.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3080. Routine determinations.

Prior to each shipment of licensed material, the licensee shall determine that:

1. The package is proper for the contents to be shipped;
2. The package is in unimpaired physical condition except for superficial defects such as marks or dents;
3. Each closure device of the packaging, including any required gasket, is properly installed and secured and free of defects;
4. Any system for containing liquid is adequately sealed and has adequate space or other specified provision for expansion of the liquid;
5. Any pressure relief device is operable and set in accordance with written procedures;
6. The package has been loaded and closed in accordance with written procedures;
7. For fissile material, any moderator or neutron absorber, if required, is present and in proper condition;
8. Any structural part of the package that could be used to lift or tie down the package during transport is rendered inoperable for that purpose unless it satisfies design requirements specified in 10 CFR 71.45;
9. The level of nonfixed radioactive contamination on the external surfaces of each package offered for shipment is ALARA and within the limits specified in 49 CFR 173.443;
10. External radiation levels around the package and around the vehicle, if applicable, will not exceed the limits specified in 10 CFR 71.47 at any time during

transportation; and

11. Accessible package surface temperatures will not exceed the limits specified in 10 CFR 71.43(g) at any time during transportation.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3090. Air transport of plutonium.

Notwithstanding the provisions of any general licenses and notwithstanding any exemptions stated directly in this part or included indirectly by citation of the DOT regulations, as may be applicable, the licensee shall assure that plutonium in any form is not transported by air, or delivered to a carrier for air transport, unless:

1. The plutonium is contained in a medical device designed for individual human application;
2. The plutonium is contained in a material in which the specific activity is less than or equal to the activity concentration values for plutonium specified in Table A-2 of 12VAC5-481-3770 and in which the radioactivity is essentially uniformly distributed;
3. The plutonium is shipped in a single package containing no more than an A₂ quantity of plutonium in any isotope or form and is shipped in accordance with 12VAC5-481-2980;
4. The plutonium is shipped in a package specifically authorized, in the CoC, issued by the NRC, for the shipment of plutonium by air and the licensee requires, through special arrangement with the carrier, compliance with 49 CFR 175.704, the DOT regulations applicable to the air transport of plutonium.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3091. Opening instructions.

Before delivery of a package to a carrier for transport, the licensee shall ensure that any special instructions needed to safely open the package have been sent to, or otherwise made available to, the consignee for the consignee's use in accordance with 12VAC5-481-900.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3100. Shipment records.

Each licensee shall maintain for a period of three years after shipment a record of each shipment of licensed material not exempt under 12VAC5-481-2970, showing, where applicable:

1. Identification of the packaging by model number and serial number;
2. Verification that the packaging, as shipped, had no significant defect;
3. Volume and identification of coolant;
4. Type and quantity of licensed material in each package, and the total quantity of each shipment;
5. Date of the shipment;
6. Name and address of the transferee;
7. Address to which the shipment was made; and
8. Results of the determinations required by 12VAC5-481-3080 and by the conditions of the package approval.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3110. Reports.

The licensee shall report to the agency within 30 days:

1. Any instance in which there is significant reduction in the effectiveness of any packaging during use;
2. Details of any defects with safety significance in the packaging after first use, with the means employed to repair the defects and prevent their recurrence; or
3. Instances in which the conditions of approval in the CoC were not observed in making a shipment.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3120. Advance notification of transport of nuclear waste.

A. Prior to the transport of any nuclear waste outside of the confines of the licensee's facility or other place of use or storage, or prior to the delivery of any nuclear waste to a carrier for transport, each licensee shall provide advance notification of such transport to the governor, or governor's designee, and the agency.

B. Advance notification is required only when:

1. The nuclear waste is required to be in Type B packaging for transportation;
2. The nuclear waste is being transported through Virginia enroute to a disposal facility or to a collection point for transport to a disposal facility; and
3. The quantity of licensed material in a single package exceeds:
 - a. 3000 times the A_1 value of the radionuclides as specified in 12VAC5-481-

3770;

b. 3000 times the A_2 value of the radionuclides as specified in 12VAC5-481-

3770; or

c. 1000 terabecquerel (27,000 curies).

C. Each advance notification required by subsection A of this section shall contain the following information:

1. The name, address, and telephone number of the shipper, carrier, and receiver of the shipment;
2. A description of the nuclear waste contained in the shipment as required by 49 CFR 172.202 and 172.203(d);
3. The point of origin of the shipment and the seven-day period during which departure of the shipment is estimated to occur;
4. The seven-day period during which arrival of the shipment at state boundaries is estimated to occur;
5. The destination of the shipment, and the seven-day period during which arrival of the shipment is estimated to occur; and
6. A point of contact with a telephone number for current shipment information.

D. The notification required by subsection A of this section shall be made in writing to the office of the governor, or governor's designee, and to the agency. A notification delivered by mail must be postmarked at least seven days before the beginning of the seven-day period during which departure of the shipment is estimated to occur. A notification delivered by messenger must reach the office of the governor, or governor's designee and the agency, at least four days before the beginning of the seven-day period during which departure of the shipment is estimated to occur. A copy of the notification shall be retained by the licensee for three years.

E. The licensee shall notify the governor, or governor's designee, and the agency of any changes to schedule information provided pursuant to subsection A of this section. Such notification shall be by telephone to a responsible individual in the office of the

governor, or governor's designee, and the agency. The licensee shall maintain for three years a record of the name of the individual contacted.

F. Each licensee who cancels a nuclear waste shipment, for which advance notification has been sent, shall send a cancellation notice, identifying the advance notification that is being canceled, to the governor, or governor's designee, and to the agency. A copy of the notice shall be retained by the licensee for three years.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 5

Quality Assurance

12VAC5-481-3130. Quality assurance.

A. Quality assurance requirements apply to the design, purchase, fabrication, handling, shipping, storing, cleaning, assembly, inspection, testing, operation, maintenance, repair, and modification of components of packaging that are important to safety. Quality assurance comprises all those planned and systematic actions necessary to provide adequate confidence that a system or component will perform satisfactorily in service. Quality assurance includes quality control, which comprises those quality assurance actions related to control of the physical characteristics and quality of the material or component to predetermined requirements. The licensee, certificate holder, and applicant for a CoC are responsible for the quality assurance requirements as they apply to design, fabrication, testing, and modification of packaging. Each licensee is responsible for the quality assurance provision that applies to its use of packaging for the shipment of licensed material subject to this chapter.

B. Each licensee, certificate holder and applicant for a CoC shall establish, maintain, and execute a quality assurance program satisfying each of that applicable criteria of

this section, 10 CFR Part 71, Subpart H and satisfying any specific provisions that are applicable to the licensee's activities including procurement of packaging. The licensee, certificate holder, and applicant for CoC shall execute the applicable criteria in a graded approach to an extent that is commensurate with the quality assurance requirement's importance to safety.

C. Before the use of any package for the shipment of licensed material subject to this rule, each licensee shall obtain NRC approval of its quality assurance program.

D. A program for transport container inspection and maintenance limited to radiographic exposure devices, source changers, or packages transporting these devices and meeting the requirements of 12VAC5-481-1270, is deemed to satisfy the requirements of 12VAC5-481-3000 and subsection B of this section.

E. The licensee, certificate holder, and applicant for a CoC shall be responsible for the establishment and execution of the quality assurance program. The licensee, certificate holder, and applicant for a CoC may delegate to others, such as contractors, agents, or consultants, the work of establishing and executing the quality assurance program, or any part of the quality assurance program, but shall retain responsibility for the program. The licensee shall clearly establish and delineate, in writing, the authority and duties of persons and organizations performing activities affecting the safety-related functions of structures, systems, and components. These activities include performing the functions associated with attaining quality objectives and the quality assurance functions. While the term licensee is used in these criteria, the requirements are applicable to whatever design, fabrication, assembly, and testing of the package is accomplished with respect to a package before the time a package is issued.

F. The quality assurance functions are:

1. Assuring that an appropriate quality assurance program is established and effectively executed; and
2. Verifying, by procedures such as checking, auditing, and inspection, that activities affecting the safety-related functions have been performed correctly.

G. The persons and organizations performing quality assurance functions must have

sufficient authority and organizational freedom to:

1. Identify quality problems;
2. Initiate, recommend, or provide solutions; and
3. Verify implementation of solutions.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part XIV

Radiation Safety Requirements for Wireline Service Operations and Subsurface Tracer Studies

Article 1

Purpose and Scope

12VAC5-481-3140. Purpose.

The regulations in this part establish radiation safety requirements for using sources of radiation for wireline service operations including mineral-logging, radioactive markers, and subsurface tracer studies. The requirements of this part are in addition to, and not in substitution for, the requirements of Parts I (12VAC5-481-10 et seq.), II (12VAC5-481-260 et seq.), III (12VAC5-481-380 et seq.), IV (12VAC5-481-600 et seq.), and X (12VAC5-481-2250 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3150. Scope.

The regulations in this part apply to all licensees or registrants who use sources of radiation for wireline service operations including mineral-logging, radioactive markers, or subsurface tracer studies.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3151. Licensing.

A. The agency will approve an application for a specific license for the use of licensed material in well logging if the applicant meets the following requirements:

1. The applicant satisfies the general requirements specified in 12VAC5-481-440 and 12VAC5-481-450.
2. The applicant shall develop a program for training logging supervisors and logging assistants and submit to the agency a description of this program that specifies:
 - a. Initial training;
 - b. On-the-job training;
 - c. Annual safety reviews provided by the licensee;
 - d. Means the applicant will use to demonstrate the logging supervisor's knowledge and understanding of and ability to comply with the agency's regulations and licensing requirements and the applicant's operating and emergency procedures; and
 - e. Means the applicant will use to demonstrate the logging assistant's knowledge and understanding of and ability to comply with the applicant's operating and emergency procedures.
3. The applicant shall submit to the agency written operating and emergency procedures as described in 12VAC5-481-3280 or an outline or summary of the procedures that includes the important radiation safety aspects of the

procedures.

4. The applicant shall establish and submit to the agency its program for annual inspections of the job performance of each logging supervisor to ensure that the agency's regulations, license requirements, and the applicant's operating and emergency procedures are followed. Inspection records shall be retained for three years after each annual internal inspection.

5. The applicant shall submit a description of its overall organizational structure as it applies to the radiation safety responsibilities in well logging, including specified delegations of authority and responsibility.

6. If an applicant wants to perform leak testing of sealed sources, the applicant shall identify the manufacturers and the model numbers of the leak test kits to be used. If the applicant wants to analyze its own wipe samples, the applicant shall establish procedures to be followed and submit a description of these procedures to the agency. The description must include the following:

- a. Instruments to be used;
- b. Methods of performing the analysis; and
- c. Pertinent experience of the person who will analyze the wipe samples.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 2

Prohibition

12VAC5-481-3160. Agreement with well owner.

No licensee shall perform wireline service operations with a sealed source(s) unless, prior to commencement of the operation, the licensee has a written agreement with the well operator, well owner, drilling contractor, or land owner that:

1. In the event a sealed source is lodged downhole, a reasonable effort at

recovery will be made;

2. No person may attempt to recover a sealed source in a manner which, in the licensee's opinion, could result in its rupture; and

3. In the event a decision is made to abandon the sealed source downhole, the requirements of 12VAC5-481-3370 C shall be met.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 3

Equipment Control

12VAC5-481-3170. Limits on levels of radiation.

Sources of radiation shall be used, stored, and transported in such a manner that the transportation requirements of Part XIII (12VAC5-481-2950 et seq.) of this chapter and the dose limitation requirements of Part IV (12VAC5-481-600 et seq.) of this chapter are met.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3180. Storage precautions.

A. Each source of radiation, except accelerators, shall be provided with a storage or transport container. The container shall be provided with a lock, or tamper seal for calibration sources, to prevent unauthorized removal of, or exposure to, the source of radiation.

B. Sources of radiation shall be stored in a manner that will minimize danger from explosion or fire.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3190. Transport precautions.

Transport containers shall be physically secured to the transporting vehicle to prevent accidental loss, tampering, or unauthorized removal.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3200. Radiation survey instruments.

A. The licensee or registrant shall maintain sufficient calibrated and operable radiation survey instruments at each field station to make physical radiation surveys as required by this part and by Part IV (12VAC5-481-600 et seq.). Instrumentation shall be capable of measuring 0.001 mSv (0.1 mrem) per hour through at least 0.5 mSv (50 mrem) per hour.

B. Each radiation survey instrument shall be calibrated:

1. At intervals not to exceed six months and after each instrument servicing;
2. For linear scale instruments, at two points located approximately 25% and 75% of full-scale on each scale; for logarithmic scale instruments, at midrange of each decade, and at two points of at least one decade; and for digital instruments, at appropriate points; and
3. So that accuracy within 20% of the true radiation level can be demonstrated on each scale.

C. Calibration records shall be maintained for a period of three years.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3210. Leak testing of sealed sources.

A. Requirements. Each licensee using sealed sources of radioactive material shall have the sources tested for leakage. Records of leak test results shall be kept in units of becquerels (microcuries) and maintained for three years after the leak test is performed.

B. Method of Testing. Tests for leakage shall be performed only by persons specifically authorized to perform such tests by the agency, the NRC, or another agreement state. The test sample shall be taken from the surface of the source, source holder, or from the surface of the device in which the source is stored or mounted and on which one might expect contamination to accumulate. The test sample shall be analyzed for radioactive contamination, and the analysis shall be capable of detecting the presence of 185 Bq (0.0005 μ Ci) of radioactive material on the test sample.

C. Interval of Testing. Each sealed source (except an energy compensated source (ECS)) shall be tested at intervals not to exceed six months. Each ECS that is not exempt in subsection E of this section must be tested at intervals not to exceed three years. In the absence of a certificate from a transferor indicating that a test has been made prior to the transfer, the sealed source shall not be put into use until tested. If, for any reason, it is suspected that a sealed source may be leaking, it shall be removed from service immediately and tested for leakage as soon as practical.

D. Leaking or Contaminated Sources. If the test reveals the presence of 185 Bq (0.005 μ Ci) or more of leakage or contamination, the licensee shall immediately withdraw the source from use and shall cause it to be decontaminated, repaired, or disposed of in accordance with these regulations. The licensee shall check the equipment associated with the leaking source for radioactive contamination and, if contaminated, have it decontaminated or disposed of in accordance with these regulations. A report describing the equipment involved, the test results, and the

corrective action taken shall be filed with the agency within five days of receiving the test results.

E. Exemptions. The following sources are exempted from the periodic leak test requirements of subsections A through D of this section:

1. Hydrogen-3 sources;
2. Sources of radioactive material with a half-life of 30 days or less;
3. Sealed sources of radioactive material in gaseous form;
4. Sources of beta- or gamma-emitting radioactive material with an activity of 3.7 MBq (100 μ Ci) or less; and
5. Sources of alpha-emitting radioactive material with an activity of 0.37 MBq (10 μ Ci) or less.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3220. Physical inventory.

Each licensee or registrant shall conduct a semi-annual physical inventory to account for all sources of radiation. Records of inventories shall be maintained for three years from the date of the inventory and shall include the quantities and kinds of sources of radiation, the location the date of the inventory, and the name of the individual conducting the inventory.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3230. Utilization records.

Each licensee or registrant shall maintain current records, which shall be kept available for three years from the date of the recorded event, showing the following information for each source of radiation:

1. Make, model number, and a serial number or a description of each source of radiation used;
2. The identity of the well-logging supervisor responsible for the source and the logging assistant present;
3. Locations where used and dates of use; and
4. In the case of tracer materials and radioactive markers, the utilization record shall indicate the radionuclide and activity used in a particular well.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3240. Design, performance, and certification criteria for sealed sources used in downhole operations.

A. Each sealed source, except those containing radioactive material in gaseous form, and ECSs used in downhole operations, shall meet the following minimum criteria:

1. Be of doubly encapsulated construction;
2. Contain radioactive material whose chemical and physical forms are as insoluble and nondispersible as practical; and
3. Certified by one of the following methods:
 - a. For a sealed source manufactured on or before July 14, 1989, a licensee may use the sealed source, for use in well-logging applications if it meets the requirements of USASI N5.10-1968, "Classification of Sealed Radioactive Sources," or the requirements in subdivision 3 b or c of this subsection;

b. For a sealed source manufactured after July 1989, a licensee may use the sealed source, for use in well-logging applications if it meets the oil well-logging requirements of ANSI/HPS N43.6-1997, "Sealed Radioactive Sources-Classification"; or

c. For a sealed source manufactured after July 14, 1989, a licensee may use the sealed source, for use in well-logging applications, if the sealed source's prototype has been tested and found to maintain its integrity after each of the following tests:

(1) Temperature. The test source must be held at -40°C for 20 minutes, 600°C for 1 hour, and then be subject to a thermal shock test with a temperature drop from 600°C to 20°C within 15 seconds.

(2) Impact test. A 5 kg steel hammer, 2.5 cm in diameter, must be dropped from a height of 1 m onto the test source.

(3) Vibrations test. The test source must be subject to a vibration from 25 Hz to 500 Hz at 5 g amplitude for 30 minutes.

(4) Puncture test. A 1 gram hammer and pin, 0.3 cm pin diameter, must be dropped from a height of 1 m onto the test source.

(5) Pressure test. The test source must be subject to an external pressure of 1.695×10^7 pascals (24,600 pounds per square inch absolute).

B. Certification documents shall be maintained for inspection by the agency for a period of two years after source disposal. If the source is abandoned downhole, the certification documents shall be maintained until the agency authorizes disposition.

C. Energy Compensated Source (ECS). Licensee use of an ECS, which may contain no greater than 3.7 MBq (100 μCi), is exempt from this part, except the following:

1. For well-logging applications with a surface casing for protecting fresh water aquifers, use of the ECS is only subject to the requirements of 12VAC5-481-3210, 12VAC5-481-3220 and 12VAC5-481-3230.

2. For well-logging applications without a surface casing for protecting fresh

water aquifers, use of the ECS is only subject to the requirements of 12VAC5-481-3160, 12VAC5-481-3210, 12VAC5-481-3220, 12VAC5-481-3230, subsection D of this section and 12VAC5-481-3370.

3. ECSs must be registered with the NRC under 10 CFR 32.210 or with an agreement state.

D. Use of a sealed source in a well without a surface casing. The licensee may use a sealed source in a well without a surface casing for protecting fresh water aquifers only if the licensee follows a procedure for reducing the probability of the source becoming lodged in the well. The procedure must be approved by the agency pursuant to 12VAC5-481-3151 A 3.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3241. Tritium neutron generator target sources.

A. Use of a tritium neutron generator target source, containing quantities not exceeding 1,110 GBq (30 curies) and in a well with a surface casing to protect fresh water aquifers, is subject to the requirements of this part except 12VAC5-481-3160, 12VAC5-481-3240 and 12VAC5-481-3370.

B. Use of a tritium neutron generator target source, containing quantities exceeding 1,110 GBq (30 curies) or in a well without a surface casing to protect fresh water aquifers, is subject to the requirements of this part except 12VAC5-481-3240.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3250. Labeling.

A. Each source, source holder, or logging tool containing radioactive material shall bear a durable, legible, and clearly visible marking or label, that has, as a minimum, the standard radiation caution symbol, without the conventional color requirement, and the following wording:

DANGER or CAUTION
RADIOACTIVE MATERIAL

This labeling shall be on the smallest component transported as a separate piece of equipment.

B. Each transport container shall have permanently attached to it a durable, legible, and clearly visible label which has, as a minimum, the standard radiation caution symbol and the following wording:

DANGER or CAUTION
RADIOACTIVE MATERIAL
NOTIFY CIVIL AUTHORITIES (OR NAME OF COMPANY)

C. Uranium sinker bars used in well-logging applications shall be legibly impressed with the following words:

CAUTION
RADIOACTIVE DEPLETED URANIUM
NOTIFY CIVIL AUTHORITIES (OR NAME OF COMPANY) IF FOUND

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3260. Inspection and maintenance.

A. Each licensee shall visually check source holders, logging tools, and source handling tools, for defects before each use to ensure that the equipment is in good

working condition and that required labeling is present. If defects are found, the equipment must be removed from service until repaired, and a record must be made listing: the date of check, name of inspector, equipment involved, defects found, and repairs made. These records must be retained for three years after the defect is found.

B. Each licensee or registrant shall conduct, at intervals not to exceed six months, a program of inspection and maintenance of source holders, logging tools, source handling tools, storage containers, transport containers, and injection tools to assure proper labeling and physical condition. Records of inspection and maintenance shall be maintained for a period of three years.

C. If any inspection conducted pursuant to subsection B of this section reveals damage to labeling or components critical to radiation safety, the device shall be removed from service until repairs have been made.

D. If a sealed source is stuck in the source holder, the licensee shall not perform any operation, such as drilling, cutting, or chiseling, on the source holder unless the licensee is specifically approved by the agency, NRC, or another agreement state to perform this operation.

E. The repair, opening, or modification of any sealed source shall be performed only by persons specifically authorized to do so by the agency, the NRC, or another agreement state.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3261. Radioactive markers.

The licensee may use radioactive markers in wells only if the individual markers contain quantities of licensed material not exceeding the quantities specified in 12VAC5-481-3730. The use of markers is subject only to the requirements of 12VAC5-

481-3220.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 4

Requirements for Personal Safety

12VAC5-481-3270. Training requirements.

A. No licensee shall permit any individual to act as a logging supervisor as defined in this part until such individual has:

1. Received instruction in the following and demonstrated an understanding thereof:

a. Fundamentals of radiation safety including:

- (1) Characteristics of radiation;
- (2) Units of radiation dose and quantity of radioactivity;
- (3) Hazards of exposure to radiation;
- (4) Levels of radiation from licensed material;
- (5) Methods of controlling radiation dose (time, distance, and shielding); and
- (6) Radiation safety practices, including prevention of contamination, and methods of decontamination;

b. Radiation detection instruments including:

- (1) Use, operation, calibration, and limitations of radiation survey instruments;
- (2) Survey techniques; and
- (3) Use of personnel monitoring equipment;

c. Equipment to be used including:

- (1) Operation of equipment, including source handling equipment and remote handling tools;

- (2) Storage, control, and disposal of licensed material; and
- (3) Maintenance of equipment;
- d. The requirements of pertinent Virginia regulations; and
- e. Case histories of accidents in well logging;

2. Received copies of and instruction in the regulations contained in this part and the applicable sections of Parts I (12VAC5-481-10 et seq.), IV (12VAC5-481-600 et seq.), and X (12VAC5-481-2250 et seq.) of this chapter or their equivalent, conditions of appropriate license, and the licensee's operating and emergency procedures, and demonstrated an understanding thereof;

3. Demonstrated competence to use sources of radiation, related handling tools, and radiation survey instruments which will be used on the job by a field evaluation; and

4. Demonstrated understanding of subdivisions 1 and 2 of this subsection by successfully passing a written test.

B. No licensee or registrant shall permit any individual to act as a logging assistant until such individual has:

1. Received instruction in the applicable sections of Parts I (12VAC5-481-10 et seq.), IV (12VAC5-481-600 et seq.) and X (12VAC5-481-2250 et seq.) of this chapter or their equivalent;

2. Received copies of, and instruction in the licensee's operating and emergency procedures;

3. Demonstrated understanding of subdivisions 1 and 2 of this subsection by successfully passing a written or oral test; and

4. Demonstrated competence to use, under the personal supervision of the logging supervisor, the sources of radiation, related handling tools, and radiation survey instruments that will be used on the job.

C. The licensee shall provide safety reviews at least once during each calendar year.

D. The licensee shall maintain employee training records for three years following termination of the individual's employment.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3280. Operating and emergency procedures.

The licensee's or registrant's operating and emergency procedures shall include instructions in at least the following:

1. Handling and use of sources of radiation to be employed so that no individual is likely to be exposed to radiation doses in excess of the standards established in Part IV (12VAC5-481-600 et seq.) of this chapter;
2. Methods and occasions for conducting radiation surveys;
3. Methods and occasions for locking and securing sources of radiation;
4. Personnel monitoring and the use of personnel monitoring equipment;
5. Transportation to temporary jobsites and field stations, including the packaging and placing of sources of radiation in vehicles, placarding of vehicles, and securing sources of radiation during transportation;
6. Minimizing exposure of individuals in the event of an accident;
7. Procedure for notifying proper personnel in the event of an accident;
8. Maintenance of records;
9. Use, inspection and maintenance of source holders, logging tools, source handling tools, storage containers, transport containers, and injection tools;
10. Procedure to be followed in the event a sealed source is lodged downhole;
11. Procedures to be used for picking up, receiving, and opening packages containing radioactive material;

12. For the use of tracers, decontamination of the environment, equipment, and personnel;
13. Maintenance of records generated by logging personnel at temporary jobsites;
14. Notifying proper persons in the event of an accident; and
15. Actions to be taken if a sealed source is ruptured, including actions to prevent the spread of contamination and minimize inhalation and ingestion of radioactive material and actions to obtain suitable radiation survey instruments as required by 12VAC5-481-3200.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3290. Personnel monitoring.

A. No licensee shall permit any individual to act as a logging supervisor or a logging assistant unless each such individual wears either a film badge, OSL or TLD. Each film badge, OSL or TLD shall be assigned to and worn by only one individual. Film badges must be replaced at least monthly and OSLs or TLDs replaced at least quarterly. After replacement, each film badge, OSL or TLD must be promptly processed.

B. Personnel monitoring records shall be maintained for inspection until the agency authorizes disposition.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Article 5

Precautionary Procedures in Logging and Subsurface Tracer Studies

12VAC5-481-3300. Security.

A. A logging supervisor must be physically present at a temporary job site whenever licensed materials are being handled or are not stored and locked in a vehicle or storage place. The logging supervisor may leave the job site to obtain assistance if a source becomes lodged in a well.

B. During well logging, except when radiation sources are below ground or in shipping or storage containers, the logging supervisor or other individual designated by the logging supervisor must maintain direct surveillance of the operation to prevent unauthorized entry into a restricted area as defined in 12VAC5-481-10.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3310. Handling tools.

The licensee shall provide and require the use of tools that will assure remote handling of sealed sources other than low-activity calibration sources.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3320. Subsurface tracer studies.

A. Protective gloves and other appropriate protective clothing and equipment shall be used by all personnel handling radioactive tracer material. Precautions shall be taken to avoid ingestion or inhalation of radioactive material.

B. No licensee shall cause the injection of radioactive material into potable aquifers without prior written authorization from the agency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3330. Particle accelerators.

No licensee or registrant shall permit above-ground testing of particle accelerators, designed for use in well-logging, which results in the production of radiation, except in areas or facilities so controlled or shielded that the requirements of 12VAC5-481-630 and 12VAC5-481-640, as applicable, are met.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 6**Radiation Surveys and Records****12VAC5-481-3340. Radiation surveys and contamination control.**

A. Radiation surveys or calculations shall be made and recorded for each area where radioactive materials are used and stored.

B. Radiation surveys shall be made and recorded for the radiation levels in occupied positions and on the exterior of each vehicle used to transport radioactive material. Such surveys shall include each source of radiation or combination of sources to be transported in the vehicle.

C. If the sealed source assembly is removed from the logging tool before departing the jobsite, the logging tool detector shall be energized, or a survey meter used, to assure that the logging tool is free of contamination.

D. Radiation surveys shall be made and recorded at the jobsite or well-head for each tracer operation, except those using hydrogen-3, carbon-14, and sulfur-35. These surveys shall include measurements of radiation levels before and after the operation.

E. Records required pursuant to subsections A through D of this section shall include the dates, the identification of individual(s) making the survey, the identification of survey instrument(s) used, and an exact description of the location of the survey. Records of these surveys shall be maintained for three years after completion of the survey.

F. If the licensee detects evidence that a sealed source has ruptured or licensed materials have caused contamination, the licensee shall initiate immediately the emergency procedures required by 12VAC5-481-3280 and contact the agency immediately.

G. During efforts to recover a sealed source lodged in the well, the licensee shall continuously monitor, with an appropriate radiation detection instrument or a logging tool with a radiation detector, the circulating fluids from the well, if any, to check for contamination resulting from damage to the sealed source.

H. If contamination results from the use of licensed material in well logging, the licensee shall decontaminate all work area equipment and personnel before release from the site or release for unrestricted use.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3350. Documents and records required at field stations.

Each licensee shall maintain the following documents and records for the specific devices and sources used at the field station:

1. Appropriate license, certificate of registration, or equivalent document(s);
2. Operating and emergency procedures;
3. Copy of Part IV (12VAC5-481-600 et seq.), Part X (12VAC5-481-2250 et seq.) and this part;

4. Records of the latest survey instrument calibrations pursuant to 12VAC5-481-3200;
5. Records of the latest leak test results pursuant to 12VAC5-481-3210;
6. Records of physical inventories required pursuant to 12VAC5-481-3220;
7. Utilization records required pursuant to 12VAC5-481-3230;
8. Records of inspection and maintenance required pursuant to 12VAC5-481-3260;
9. Survey records required pursuant to 12VAC5-481-3340; and
10. Training records required pursuant to 12VAC5-481-3270.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3360. Documents and records required at temporary jobsites.

Each licensee or registrant conducting operations at a temporary jobsite shall have the following documents and records available at that site for inspection by the agency:

1. Operating and emergency procedures;
2. Survey records required pursuant to 12VAC5-481-3340 for the period of operation at the site;
3. Evidence of current calibration for the radiation survey instruments in use at the site;
4. When operating in the state under reciprocity, a copy of the appropriate license, certificate of registration, or equivalent document(s); and
5. Shipping papers for the transportation of radioactive material.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Article 7

Notification

12VAC5-481-3370. Notification of incidents, abandonment, and lost sources.

A. Notification of incidents and sources lost in other than downhole logging operations shall be made in accordance with appropriate provisions of Part IV (12VAC5-481-600 et seq.) of this chapter.

B. Whenever a sealed source or device containing radioactive material is lodged downhole, the licensee shall:

1. Monitor at the surface for the presence of radioactive contamination with a radiation survey instrument or logging tool during logging tool recovery operations; and

2. Notify the agency immediately by telephone and subsequently, within 30 days, by confirmatory letter if the licensee knows or has reason to believe that a sealed source has been ruptured. This letter shall identify the well or other location, describe the magnitude and extent of the escape of radioactive material, assess the consequences of the rupture, and explain efforts planned or being taken to mitigate these consequences.

C. When it becomes apparent that efforts to recover the radioactive source will not be successful, the licensee shall:

1. Advise the well-operator of the regulations of the Virginia Department of Mines, Minerals, and Energy; Division of Gas and Oil, regarding abandonment and an appropriate method of abandonment, that shall include:

- a. The immobilization and sealing in place of the radioactive source with a cement plug,

- b. The setting of a whipstock or other deflection device, and

- c. The mounting of a permanent identification plaque at the surface of the

well, containing the appropriate information required by subsection D of this section;

2. Notify the agency by telephone, giving the circumstances of the loss, and request approval of the proposed abandonment procedures; and

3. File a written report with the agency within 30 days of the abandonment. The licensee shall send a copy of the report to the Virginia Department of Mines, Minerals, and Energy; Division of Gas and Oil. The report shall contain the following information:

a. Date of occurrence;

b. A description of the well logging source involved, including the radionuclide and its quantity, chemical, and physical form;

c. Surface location and identification of the well;

d. Results of efforts to immobilize and seal the source in place;

e. A brief description of the attempted recovery effort;

f. Depth of the source;

g. Depth of the top of the cement plug;

h. Depth of the well;

i. Any other information, such as a warning statement, contained on the permanent identification plaque; and

j. The names of state agencies receiving a copy of this report.

D. Whenever a sealed source containing radioactive material is abandoned downhole, the licensee shall provide a permanent plaque for posting the well or well-bore. This plaque shall:

1. Be constructed of long-lasting material, such as stainless steel or monel; and

2. Contain the following information engraved on its face:

a. The word "CAUTION";

b. The radiation symbol without the conventional color requirement;

- c. The date of abandonment;
- d. The name of the well operator or well owner;
- e. The well name and well identification number(s) or other designation;
- f. The sealed source(s) by radionuclide and activity;
- g. The source depth and the depth to the top of the plug; and
- h. An appropriate warning, depending on the specific circumstances of each abandonment.

E. The licensee shall immediately notify the agency by telephone and subsequently by confirming letter if the licensee knows or has reason to believe that radioactive material has been lost in or to an underground potable aquifer. Such notice shall designate the well location and shall describe the magnitude and extent of loss of radioactive material, assess the consequences of such loss, and explain efforts planned or being taken to mitigate these consequences.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Part XV

Therapeutic Radiation Machines

12VAC5-481-3380. Purpose and scope.

A. This part establishes requirements, for which the registrant is responsible, for use of therapeutic radiation machines. The provisions of this part are in addition to, and not in substitution for, other applicable provisions of these regulations.

B. The use of therapeutic radiation machines shall be by, or under the supervision of, a licensed practitioner of the healing arts who meets the training/experience criteria established by 12VAC5-481-3390 C.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3390. General administrative requirements for facilities using therapeutic radiation machines.

A. Administrative controls. The registrant shall be responsible for directing the operation of the therapeutic radiation machines that have been registered with the agency and reporting misadministrations within 10 days. The registrant or the registrant's agent shall ensure that the requirements of Part XV (12VAC5-481-3380 et seq.) of this chapter are met in the operation of the therapeutic radiation machine(s).

B. A therapeutic radiation machine that does not meet the provisions of these regulations shall not be used for irradiation of patients.

C. Training for external beam radiation therapy authorized users. The registrant for any therapeutic radiation machine subject to 12VAC5-481-3420 or 12VAC5-481-3430 shall require the authorized user to be a physician who:

1. Is certified in:

- a. Radiology or therapeutic radiology by the American Board of Radiology;
- b. Radiation oncology by the American Osteopathic Board of Radiology;
- c. Radiology, with specialization in radiotherapy, as a British "Fellow of the Faculty of Radiology" or "Fellow of the Royal College of Radiology"; or
- d. Therapeutic radiology by the Canadian Royal College of Physicians and Surgeons;

or

2. Is in the active practice of therapeutic radiology, and has completed 200 hours of instruction in basic radiation techniques applicable to the use of an external beam radiation therapy unit, 500 hours of supervised work experience, and a minimum of three years of supervised clinical experience.

- a. To satisfy the requirement for instruction, the classroom and laboratory

training shall include:

- (1) Radiation physics and instrumentation;
- (2) Radiation protection;
- (3) Mathematics pertaining to the use and measurement of ionization radiation; and
- (4) Radiation biology.

b. To satisfy the requirement for supervised work experience, training shall be under the supervision of an authorized user and shall include:

- (1) Review of the full calibration measurements and periodic quality assurance checks;
- (2) Evaluation of prepared treatment plans and calculation of treatment times/patient treatment settings;
- (3) Using administrative controls to prevent miss-administrations;
- (4) Implementing emergency procedures to be followed in the event of the abnormal operation of an external beam radiation therapy unit or console; and
- (5) Checking and using radiation survey meters.

c. To satisfy the requirement for a period of supervised clinical experience, training shall include one year in a formal training program approved by the Residency Review Committee for Radiology of the Accreditation Council for Graduate Medical Education or the Committee on Postdoctoral Training of the American Osteopathic Association and an additional two years of clinical experience in therapeutic radiology under the supervision of an authorized user. The supervised clinical experience shall include:

- (1) Examining individuals and reviewing their case histories to determine their suitability for external beam radiation therapy treatment, and any limitations/contraindications;
- (2) Selecting proper dose and how it is to be administered;
- (3) Calculating the external beam radiation therapy doses and collaborating

with the authorized user in the review of patients' progress and consideration of the need to modify originally prescribed doses and/or treatment plans as warranted by patients' reaction to radiation; and

(4) Post-administration follow-up and review of case histories.

3. Notwithstanding the requirements of subdivisions 1 and 2 of this subsection, the registrant for any therapeutic radiation machine subject to 12VAC5-481-3420 may also submit the training of the prospective authorized user physician for agency review on a case-by-case basis.

4. A physician shall not act as an authorized user for any therapeutic radiation machine until such time as said physician's training has been reviewed and approved by the agency.

D. Training for radiation therapy physicist. The registrant for any therapeutic radiation machine subject to 12VAC5-481-3420 and 12VAC5-481-3430 shall require the radiation therapy physicist to:

1. Be registered with the agency, under the provisions of Part II (12VAC5-481-260 et seq.) of this chapter, as a provider of radiation services in the area of calibration and surveys of external beam radiation therapy units; and

2. Shall meet the requirements of 12VAC5-481-340 B 2.

E. Qualifications of operators.

1. Individuals who will be operating a therapeutic radiation machine for medical use shall be American Registry of Radiologic Technologists (ARRT) Registered Radiation Therapy Technologists. Individuals who are not ARRT Registered Radiation Therapy Technologists shall submit evidence that they have satisfactorily completed a radiation therapy technologist training program that complies with the requirements of the Joint Review Committee on Education in Radiologic Technology.

2. The names and training of all personnel currently operating a therapeutic radiation machine shall be kept on file at the facility. Information on former

operators shall be retained for a period of at least two years beyond the last date they were authorized to operate a therapeutic radiation machine at that facility.

F. Written safety procedures and rules shall be developed by a radiation therapy physicist and shall be available in the control area of a therapeutic radiation machine, including any restrictions required for the safe operation of the particular therapeutic radiation machine. The operator shall be able to demonstrate familiarity with these rules.

G. Individuals shall not be exposed to the useful beam except for medical therapy purposes and unless such exposure has been ordered in writing by a licensed practitioner of the healing arts who is specifically identified on the Certificate of Registration. This provision specifically prohibits deliberate exposure of an individual for training, demonstration or other nonhealing-arts purposes.

H. Visiting authorized user. Notwithstanding the provisions of subsection G of this section, a registrant may permit any physician to act as a visiting authorized user under the term of the registrant's Certificate of Registration for up to 60 days per calendar year under the following conditions:

1. The visiting authorized user has the prior written permission of the registrant's management and, if the use occurs on behalf of an institution, the institution's radiation safety committee; and
2. The visiting authorized user meets the requirements established for authorized user(s) in subdivisions 1 and 2 of this subsection; and
3. The registrant maintains copies of all records specified by this subsection for five years from the date of the last visit.

I. All individuals associated with the operation of a therapeutic radiation machine shall be instructed in and shall comply with the provisions of the registrant's quality management program. In addition to the requirements of Part XV of this chapter, these individuals are also subject to the requirements of 12VAC5-481-640, 12VAC5-481-680, and 12VAC5-481-760.

J. Information and maintenance record and associated information. The registrant

shall maintain the following information in a separate file or package for each therapeutic radiation machine, for inspection by the agency:

1. Report of acceptance testing;
2. Records of all surveys, calibrations, and periodic quality assurance checks of the therapeutic radiation machine required by Part XV of this chapter, as well as the name(s) of person(s) who performed such activities;
3. Records of maintenance and/or modifications performed on the therapeutic radiation machine after September 20, 2006, as well as the name(s) of person(s) who performed such services;
4. Signature of person authorizing the return of therapeutic radiation machine to clinical use after service, repair, or upgrade.

K. Records retention. All records required by Part XV of this chapter shall be retained until disposal is authorized by the agency unless another retention period is specifically authorized in Part XV of this chapter. All required records shall be retained in an active file from at least the time of generation until the next agency inspection. Any required record generated prior to the last agency inspection may be microfilmed or otherwise archived as long as a complete copy of said record can be retrieved until such time as the agency authorizes final disposal.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3400. General technical requirements for facilities using therapeutic radiation machines.

A. Surveys.

1. The registrant shall ensure that radiation surveys of all new facilities, and existing facilities not previously surveyed are performed with an operable radiation measurement survey instrument calibrated in accordance with 12VAC5-

481-3440. The radiation survey shall be performed by, or under the direction of, a radiation therapy physicist or a private inspector and shall verify that, with the therapeutic radiation machine in a "BEAM-ON" condition, with the largest clinically available treatment field and with a scattering phantom in the useful beam of radiation:

- a. Radiation levels in restricted areas are not likely to cause personnel exposures in excess of the limits specified in 12VAC5-481-640; and
- b. Radiation levels in unrestricted areas do not exceed the limits specified in 12VAC5-481-720.

2. In addition to the requirements of 12VAC5-481-3400 A 1, a radiation survey shall also be performed prior to any subsequent medical use and:

- a. After making any change in the treatment room shielding;
- b. After making any change in the location of the therapeutic radiation machine within the treatment room;
- c. After relocating the therapeutic radiation machine; or
- d. Before using the therapeutic radiation machine in a manner that could result in increased radiation levels in areas outside the external beam radiation therapy treatment room.

3. The survey record shall indicate all instances where the facility, in the opinion of the radiation therapy physicist or a private inspector, is in violation of applicable regulations. The survey record shall also include: the date of the measurements; the reason the survey is required; the manufacturer's name; the model number and serial number of the therapeutic radiation machine; the instrument(s) used to measure radiation levels; a plan of the areas surrounding the treatment room that were surveyed; the measured dose rate at several points in each area expressed in microsieverts or millirems per hour; the calculated maximum level of radiation over a period of one week for each restricted and unrestricted area; and the signature of the individual responsible for conducting the survey;

4. If the results of the surveys required by subdivision 1 or 2 of this subsection indicate any radiation levels in excess of the respective limit specified in subdivision 1 of this subsection, the registrant shall lock the control in the "OFF" position and not use the unit:

a. Except as may be necessary to repair, replace, or test the therapeutic radiation machine, the therapeutic radiation machine shielding, or the treatment room shielding; or

b. Until the registrant has received a specific exemption from the agency.

B. Modification of radiation therapy unit or room before beginning a treatment program. If the survey required by subsection A of this section indicates that an individual in an unrestricted area may be exposed to levels of radiation greater than those permitted by 12VAC5-481-720, before beginning the treatment program the registrant shall:

1. Either equip the unit with beam direction interlocks or add additional radiation shielding to ensure compliance with 12VAC5-481-720;

2. Perform the survey required by subsection A of this section again; and

3. Include in the report required by subsection D of this section the results of the initial survey, a description of the modification made to comply with subdivision 1 of this subsection, and the results of the second survey; or

4. Request and receive a registration amendment under 12VAC5-481-720 that authorizes radiation levels in unrestricted areas greater than those permitted by 12VAC5-481-720.

C. Dosimetry equipment.

1. The registrant shall have a calibrated dosimetry system available for use. The system shall have been calibrated by the National Institute for Standards and Technology (NIST) or by an American Association of Physicists in Medicine (AAPM) Accredited Dosimetry Calibration Laboratory (ADCL). The calibration shall have been performed within the previous 24 months and after any servicing.

that may have affected system calibration.

- a. For beams with energies greater than one MV (1 MeV), the dosimetry system shall have been calibrated for Cobalt-60;
- b. For beams with energies equal to or less than one MV (1 MeV), the dosimetry system shall have been calibrated at an energy (energy range) appropriate for the radiation being measured;

2. The registrant shall have available for use a dosimetry system for quality assurance check measurements. To meet this requirement, the system may be compared with a system that has been calibrated in accordance with subdivision C 1 of this section. This comparison shall have been performed within the previous 12 months and after each servicing that may have affected system calibration. The quality assurance check system may be the same system used to meet the requirement in subdivision C 1 of this section;

3. The registrant shall maintain a record of each dosimetry system calibration, intercomparison, and comparison for the duration of the license and/or registration. For each calibration, intercomparison, or comparison, the record shall include: the date; the model numbers and serial numbers of the instruments that were calibrated, inter-compared, or compared as required by subdivisions C 1 and 2 of this section; the correction factors that were determined; the names of the individuals who performed the calibration, intercomparison, or comparison; and evidence that the intercomparison was performed by, or under the direct supervision and in the physical presence of, a radiation therapy physicist.

D. Reports of external beam radiation therapy surveys and measurements. The registrant for any therapeutic radiation machine subject to 12VAC5-481-3420 or 12VAC5-481-3430 shall furnish a copy of the records required in subsections A and B of this section to the agency within 30 days following completion of the action that initiated the record requirement.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3410. Quality management program.

The facility shall implement a quality management program. The facility shall include in the quality management program notification of a misadministration, a recordable event, and recording written directives.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3420. Therapeutic radiation machines of less than 500 kV.

A. Leakage radiation. When the X-ray tube is operated at its maximum rated tube current for the maximum kV, the leakage air kerma rate shall not exceed the value specified at the distance specified for that classification of therapeutic radiation machine:

1. 5-50 kV Systems. The leakage air kerma rate measured at any position five centimeters from the tube housing assembly shall not exceed one mGy (100 mrad) in any one hour.
2. >50 and <500 kV Systems. The leakage air kerma rate measured at a distance of one meter from the target in any direction shall not exceed one cGy (1 rad) in any one hour. This air kerma rate measurement may be averaged over areas no larger than 100 square centimeters. In addition, the air kerma rate at a distance of five centimeters from the surface of the tube housing assembly shall not exceed 30 cGy (30 rad) per hour. >
3. For each therapeutic radiation machine, the registrant shall determine, or obtain from the manufacturer, the leakage radiation existing at the positions specified in subdivisions A 1 and 2 of this section for the specified operating

conditions. Records on leakage radiation measurements shall be maintained at the installation for inspection by the agency.

B. Permanent beam limiting devices. Permanent diaphragms or cones used for limiting the useful beam shall provide at least the same degree of attenuation as required for the tube housing assembly.

C. Adjustable or removable beam limiting devices.

1. All adjustable or removable beam limiting devices, diaphragms, cones or blocks shall not transmit more than 5.0% of the useful beam for the most penetrating beam used;

2. When adjustable beam limiting devices are used, the position and shape of the radiation field shall be indicated by a light beam.

D. Filter system. The filter system shall be so designed that:

1. Filters cannot be accidentally displaced at any possible tube orientation;

2. For equipment installed after September 20, 2006, an interlock system prevents irradiation if the proper filter is not in place;

3. The air kerma rate escaping from the filter slot shall not exceed one cGy (1 rad) per hour at one meter under any operating conditions; and

4. Each filter shall be marked as to its material of construction and its thickness.

E. Tube immobilization.

1. The X-ray tube shall be so mounted that it cannot accidentally turn or slide with respect to the housing aperture; and

2. The tube housing assembly shall be capable of being immobilized for stationary portal treatments.

F. Source marking. The tube housing assembly shall be so marked that it is possible to determine the location of the source to within five millimeters, and such marking shall be readily accessible for use during calibration procedures.

G. Beam block. Contact therapy tube housing assemblies shall have a removable shield of material, equivalent in attenuation to 0.5 millimeters of lead at 100 kV, which

can be positioned over the entire useful beam exit port during periods when the beam is not in use.

H. Timer. A suitable irradiation control device shall be provided to terminate the irradiation after a pre-set time interval.

1. A timer with a display shall be provided at the treatment control panel. The timer shall have a pre-set time selector and an elapsed time or time remaining indicator;
2. The timer shall be a cumulative timer that activates with an indication of "BEAM-ON" and retains its reading after irradiation is interrupted or terminated. After irradiation is terminated and before irradiation can be reinitiated, it shall be necessary to reset the elapsed time indicator;
3. The timer shall terminate irradiation when a preselected time has elapsed, if any dose monitoring system present has not previously terminated irradiation;
4. The timer shall permit accurate pre-setting and determination of exposure times as short as one second;
5. The timer shall not permit an exposure if set at zero;
6. The timer shall not activate until the shutter is opened when irradiation is controlled by a shutter mechanism unless calibration includes a timer error correction to compensate for mechanical lag; and
7. Timer shall be accurate to within 1.0% of the selected value or one second, whichever is greater.

I. Control panel functions. The control panel, in addition to the displays required by other provisions in this section, shall have:

1. An indication of whether electrical power is available at the control panel and if activation of the X-ray tube is possible;
2. An indication of whether X-rays are being produced;
3. A means for indicating X-ray tube potential and current;
4. The means for terminating an exposure at any time;

5. A locking device which will prevent unauthorized use of the therapeutic radiation machine; and

6. For therapeutic radiation machines manufactured after September 20, 2006, a positive display of specific filter(s) in the beam.

J. Multiple tubes. When a control panel may energize more than one X-ray tube:

1. It shall be possible to activate only one X-ray tube at any time;

2. There shall be an indication at the control panel identifying which X-ray tube is activated; and

3. There shall be an indication at the tube housing assembly when that tube is energized.

K. Target-to-skin distance (TSD). There shall be a means of determining the central axis TSD to within one centimeter and of reproducing this measurement to within two millimeters thereafter.

L. Shutters. Unless it is possible to bring the X-ray output to the prescribed exposure parameters within five seconds after the X-ray "ON" switch is energized, the beam shall be attenuated by a shutter having a lead equivalency not less than that of the tube housing assembly. In addition, after the unit is at operating parameters, the shutter shall be controlled by the operator from the control panel. An indication of shutter position shall appear at the control panel.

M. Low filtration X-ray tubes. Each therapeutic radiation machine equipped with a beryllium or other low-filtration window shall be clearly labeled as such upon the tube housing assembly and shall be provided with a permanent warning device on the control panel that is activated when no additional filtration is present, to indicate that the dose rate is very high.

N. Facility design requirements for therapeutic radiation machines capable of operating in the range 50 kV to 500 kV. In addition to adequate shielding to meet requirements of 12VAC5-481-3450, the treatment room shall meet the following design requirements:

1. Aural communication. Provision shall be made for continuous two-way aural communication between the patient and the operator at the control panel;
2. Viewing systems. Provision shall be made to permit continuous observation of the patient during irradiation and the viewing system shall be so located that the operator can observe the patient from the control panel. The therapeutic radiation machine shall not be used for patient irradiation unless at least one viewing system is operational.

O. Additional requirements. Treatment rooms that contain a therapeutic radiation machine capable of operating above 150 kV shall meet the following additional requirements:

1. All protective barriers shall be fixed except for entrance doors or beam interceptors;
2. The control panel shall be located outside the treatment room or in a totally enclosed booth, which has a ceiling, inside the room;
3. Interlocks shall be provided such that all entrance doors, including doors to any interior booths, shall be closed before treatment can be initiated or continued. If the radiation beam is interrupted by any door opening, it shall not be possible to restore the machine to operation without closing the door and reinitiating irradiation by manual action at the control panel; and
4. When any door referred to in subdivision 3 of this subsection is opened while the X-ray tube is activated, the air kerma rate at a distance of one meter from the source shall be reduced to less than one mGy (100 mrad) per hour.

P. Full calibration measurements.

1. Full calibration of a therapeutic radiation machine subject to this section shall be performed by, or under the direct supervision of, a radiation therapy physicist:
 - a. Before the first medical use following installation or reinstallation of the therapeutic radiation machine;
 - b. At intervals not exceeding one year; and

c. Before medical use under the following conditions:

(1) Whenever quality assurance check measurements indicate that the radiation output differs by more than 5.0% from the value obtained at the last full calibration and the difference cannot be reconciled; and

(2) Following any component replacement, major repair, or modification of components that could significantly affect the characteristics of the radiation beam.

d. Notwithstanding the requirements of subdivision 1 c of this subsection:

(1) Full calibration of therapeutic radiation machines with multienergy capabilities is required only for those modes and/or energies that are not within their acceptable range; and

(2) If the repair, replacement or modification does not affect all energies, full calibration shall be performed on the affected energy that is in most frequent clinical use at the facility. The remaining energies may be validated with quality assurance check procedures against the criteria in subdivision 1 c (1) of this subsection.

2. To satisfy the requirement of subdivision 1 of this subsection, full calibration shall include all measurements recommended for annual calibration by NCRP Report 69, "Dosimetry of X-ray and Gamma Ray Beams for Radiation Therapy in the Energy Range 10 keV to 50 MeV" (1981).

3. The registrant shall maintain a record of each calibration for the duration of the registration. The record shall include: the date of the calibration; the manufacturer's name, model number, and serial number for both the therapeutic radiation machine and the X-ray tube; the model numbers and serial numbers of the instruments used to calibrate the therapeutic radiation machine; and the signature of the radiation therapy physicist responsible for performing the calibration.

Q. Periodic quality assurance checks.

1. Periodic quality assurance checks shall be performed on therapeutic radiation machines subject to this section, which are capable of operation at greater than or equal to 50 kV.
2. To satisfy the requirement of subdivision 1 of this subsection, quality assurance checks shall meet the following requirements:
 - a. The registrant shall perform quality assurance checks in accordance with written procedures established by the radiation therapy physicist.; and
 - b. The quality assurance check procedures shall specify the frequency at which tests or measurements are to be performed. The quality assurance check procedures shall specify that the quality assurance check shall be performed during the calibration specified in subdivision P 1 of this section. The acceptable tolerance for each parameter measured in the quality assurance check, when compared to the value for that parameter determined in the calibration specified in subdivision P 1 of this section, shall be stated.
3. The cause for a parameter exceeding a tolerance set by the radiation therapy physicist shall be investigated and corrected before the system is used for patient irradiation;
4. Whenever a quality assurance check indicates a significant change in the operating characteristics of a system, as specified in the radiation therapy physicist's quality assurance check procedures, the system shall be recalibrated as required in subdivision P 1 of this section;
5. The registrant shall use the dosimetry system described in 12VAC5-481-3400 C 2 to make the quality assurance check required in subdivision 2 of this subsection;
6. The registrant shall have the radiation therapy physicist review and sign the results of each radiation output quality assurance check within one month of the date that the check was performed;
7. The registrant shall ensure that safety quality assurance checks of therapeutic

radiation machines subject to this section are performed at intervals not to exceed one month;

8. Notwithstanding the requirements of subdivisions 4 and 7 of this subsection, the registrant shall ensure that no therapeutic radiation machine is used to administer radiation to humans unless the quality assurance checks required by subdivisions 6 and 7 of this subsection have been performed within the 30-day period immediately prior to said administration;

9. To satisfy the requirement of subdivision 7 of this subsection, safety quality assurance checks shall ensure proper operation of:

- a. Electrical interlocks at each external beam radiation therapy room entrance;
- b. The "BEAM-ON" and termination switches;
- c. Beam condition indicator lights on the access door(s), control console, and in the radiation therapy room;
- d. Viewing systems;
- e. If applicable, electrically operated treatment room doors from inside and outside the treatment room;

10. The registrant shall maintain a record of each quality assurance check required by subdivisions 1 and 7 of this subsection for three years. The record shall include: the date of the quality assurance check; the manufacturer's name, the model number, and serial number of the therapeutic radiation machine; the manufacturer's name; the model number and serial number for the instrument(s) used to measure the radiation output of the therapeutic radiation machine; and the signature of the individual who performed the periodic quality assurance check.

R. Operating procedures.

1. The therapeutic radiation machine shall not be used for irradiation of patients unless the requirements of subsections P and Q of this section have been met;

2. Therapeutic radiation machines shall not be left unattended unless secured pursuant to subdivision 1 5 of this section;
3. When a patient must be held in position for radiation therapy, mechanical supporting or restraining devices shall be used;
4. The tube housing assembly shall not be held by an individual during operation unless the assembly is designed to require such holding and the peak tube potential of the system does not exceed 50 kV. In such cases, the holder shall wear protective gloves and apron of not less than 0.5 millimeters lead equivalency at 100 kV;
5. A copy of the current operating and emergency procedures shall be maintained at the therapeutic radiation machine control console; and
6. No individual other than the patient shall be in the treatment room during exposures from therapeutic radiation machines operating above 150 kV. At energies less than or equal to 150 kV, any individual, other than the patient, in the treatment room shall be protected by a barrier sufficient to meet the requirements of 12VAC5-481-640.

S. Possession of survey instrument(s). Each facility location authorized to use a therapeutic radiation machine in accordance with this section shall possess appropriately calibrated portable monitoring equipment. As a minimum, such equipment shall include a portable radiation measurement survey instrument capable of measuring dose rates over the range 10 mSv (1 mrem) per hour to 10 mSv (1000 mrem) per hour. The survey instrument(s) shall be operable and calibrated in accordance with 12VAC5-481-3440.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3430. Therapeutic radiation machines -- photon therapy systems

(500 kV and above) and electron therapy systems (500 kV and above).

A. Possession of survey instrument(s). Each facility location authorized to use a therapeutic radiation machine in accordance with this section shall possess appropriately calibrated portable monitoring equipment. As a minimum, such equipment shall include a portable radiation measurement survey instrument capable of measuring dose rates over the range 10 mSv (1 mrem) per hour to 10 mSv (1000 mrem) per hour. The survey instrument(s) shall be operable and calibrated in accordance with 12VAC5-481-3440.

B. Leakage radiation outside the maximum useful beam in photon and electron modes.

1. The absorbed dose due to leakage radiation (excluding neutrons) at any point outside the maximum sized useful beam, but within a circular plane of radius two meters which is perpendicular to and centered on the central axis of the useful beam at the nominal treatment distance (i.e. patient plane), shall not exceed a maximum of 0.2% and an average of 0.1% of the absorbed dose on the central axis of the beam at the nominal treatment distance. Measurements shall be averaged over an area not exceeding 100 square centimeters at a minimum of 16 points uniformly distributed in the plane;

2. Except for the area defined in subdivision 1 of this subsection, the absorbed dose due to leakage radiation (excluding neutrons) at one meter from the electron path between the electron source and the target or electron window shall not exceed 0.5% of the absorbed dose on the central axis of the beam at the nominal treatment distance. Measurements shall be averaged over an area not exceeding 100 square centimeters;

3. For equipment manufactured after September 20, 2006, the neutron absorbed dose outside the useful beam shall be in compliance with International Electrotechnical Commission (IEC) Document 601-2-1 (most current revision); and

4. For each therapeutic radiation machine, the registrant shall determine, or

obtain from the manufacturer, the leakage radiation existing at the positions specified in subdivisions 1 through 3 of this subsection for the specified operating conditions. Records on leakage radiation measurements shall be maintained at the installation for inspection by the agency.

C. Leakage radiation through beam limiting devices.

1. Photon radiation. All adjustable or interchangeable beam limiting devices shall attenuate the useful beam such that at the nominal treatment distance, the maximum absorbed dose anywhere in the area shielded by the beam limiting device(s) shall not exceed 2.0% of the maximum absorbed dose on the central axis of the useful beam measured in a 10 centimeter by 10 centimeter radiation field, or for multileaf collimators, shall not exceed manufacturer's specifications;

2. Electron radiation. All adjustable or interchangeable electron applicators shall attenuate the radiation, including but not limited to photon radiation generated by electrons incident on the beam limiting device and electron applicator and other parts of the radiation head, such that the absorbed dose in a plane perpendicular to the central axis of the useful beam at the nominal treatment distance shall not exceed:

a. A maximum of 2.0% and average of 0.5% of the absorbed dose on the central axis of the useful beam at the nominal treatment distance. This limit shall apply beyond a line seven centimeters outside the periphery of the useful beam; and

b. A maximum of 10% of the absorbed dose on the central axis of the useful beam at the nominal treatment distance. This limit shall apply beyond a line two centimeters outside the periphery of the useful beam.

3. Measurement of leakage radiation.

a. Photon radiation. Measurements of leakage radiation through the beam limiting devices shall be made with the beam limiting devices closed and any residual aperture blocked by at least two-tenth value layers of suitable absorbing material. In the case of overlapping beam limiting devices, the

leakage radiation through each set shall be measured independently at the depth of maximum dose. Measurements shall be made using a radiation detector of area not exceeding 10 square centimeters;

b. Electron radiation. Measurements of leakage radiation through the electron applicators shall be made with the electron beam directed into the air and using a radiation detector of area up to but not exceeding one square centimeter suitably protected against radiation which has been scattered from material beyond the radiation detector. Measurements shall be made using one centimeter of water equivalent build up material.

D. Filters/wedges.

1. Each wedge filter that is removable from the system shall be clearly marked with an identification number. For removable wedge filters, the nominal wedge angle shall appear on the wedge or wedge tray (if permanently mounted to the tray). If the wedge or wedge tray is significantly damaged, the wedge transmission factor shall be redetermined;

2. If the absorbed dose rate information required by subsection I of this section relates exclusively to operation with a field flattening filter or beam scattering foil in place, such foil or filter shall be removable only by the use of tools;

3. For equipment manufactured after September 20, 2006, that utilizes wedge filters, interchangeable field flattening filters, or interchangeable beam scattering foils:

a. Irradiation shall not be possible until a selection of a filter or a positive selection to use "no filter" has been made at the treatment control panel, either manually or automatically;

b. An interlock system shall be provided to prevent irradiation if the filter selected is not in the correct position;

c. A display shall be provided at the treatment control panel showing the wedge filter(s), interchangeable field flattening filter(s), and/or interchangeable beam scattering foil(s) in use; and

d. An interlock shall be provided to prevent irradiation if any filter and/or beam scattering foil selection operation carried out in the treatment room does not agree with the filter and/or beam scattering foil selection operation carried out at the treatment control panel.

E. Stray radiation in the useful beam. For equipment manufactured after September 20, 2006, the registrant shall determine during acceptance testing, or obtain from the manufacturer, data sufficient to ensure that X-ray stray radiation in the useful electron beam, absorbed dose at the surface during X-ray irradiation and stray neutron radiation in the useful X-ray beam are in compliance with International Electrotechnical Commission (IEC) Document 601-2-1 (most current revision).

F. Beam monitors. All therapeutic radiation machines subject to this section shall be provided with redundant beam monitoring systems. The sensors for these systems shall be fixed in the useful beam during treatment to indicate the dose monitor unit rate.

1. Equipment manufactured after September 20, 2006, shall be provided with at least two independently powered integrating dose meters. Alternatively, common elements may be used if the production of radiation is terminated upon failure of any common element.

2. Equipment manufactured on or before September 20, 2006, shall be provided with at least one radiation detector. This detector shall be incorporated into a useful beam monitoring system;

3. The detector and the system into which that detector is incorporated shall meet the following requirements:

a. Each detector shall be removable only with tools and, if movable, shall be interlocked to prevent incorrect positioning;

b. Each detector shall form part of a beam monitoring system from whose readings in dose monitor units the absorbed dose at a reference point can be calculated;

c. Each beam monitoring system shall be capable of independently

monitoring, interrupting, and terminating irradiation; and

d. For equipment manufactured after September 20, 2006, the design of the beam monitoring systems shall ensure that the:

(1) Malfunctioning of one system shall not affect the correct functioning of the other system(s); and

(2) Failure of either system shall terminate irradiation or prevent the initiation of radiation.

e. Each beam monitoring system shall have a legible display at the treatment control panel. For equipment manufactured after September 20, 2006, each display shall:

(1) Maintain a reading until intentionally reset;

(2) Have only one scale and no electrical or mechanical scale multiplying factors;

(3) Utilize a design such that increasing dose is displayed by increasing numbers; and

(4) In the event of power failure, the beam monitoring information required in subdivision 3 e (3) of this subsection displayed at the control panel at the time of failure shall be retrievable in at least one system for a 20 minute period of time.

G. Beam symmetry.

1. Bent-beam linear accelerators subject to this section shall be provided with auxiliary device(s) to monitor beam symmetry;

2. The device(s) referenced in subdivision 1 of this subsection shall be able to detect field asymmetry greater than 10%; and

3. The device(s) referenced in subdivision 1 of this subsection shall be configured to terminate irradiation if the specifications in subdivision 2 of this subsection cannot be maintained.

H. Selection and display of dose monitor units.

1. Irradiation shall not be possible until a new selection of a number of dose monitor units has been made at the treatment control panel;
2. The preselected number of dose monitor units shall be displayed at the treatment control panel until reset manually for the next irradiation;
3. After termination of irradiation, it shall be necessary to reset the dosimeter display before subsequent treatment can be initiated; and
4. For equipment manufactured after September 20, 2006, after termination of irradiation, it shall be necessary for the operator to reset the preselected dose monitor units before irradiation can be initiated.

I. Air kerma rate/absorbed dose rate. For equipment manufactured after September 20, 2006, a system shall be provided from whose readings the air kerma rate or absorbed dose rate at a reference point can be calculated. (The radiation detectors specified in subsection F of this section may form part of this system.) In addition:

1. The dose monitor unit rate shall be displayed at the treatment control panel;
2. If the equipment can deliver under any conditions an air kerma rate or absorbed dose rate at the nominal treatment distance more than twice the maximum value specified by the manufacturer, a device shall be provided that terminates irradiation when the air kerma rate or absorbed dose rate exceeds a value twice the specified maximum. The dose rate at which the irradiation will be terminated shall be a record maintained by the registrant;
3. If the equipment can deliver under any fault condition(s) an air kerma rate or absorbed dose rate at the nominal treatment distance more than 10 times the maximum value specified by the manufacturer, a device shall be provided to prevent the air kerma rate or absorbed dose rate anywhere in the radiation field from exceeding twice the specified maximum value and to terminate irradiation if the excess absorbed dose at the nominal treatment distance exceeds 4 Gy (400 rad); and
4. For each therapeutic radiation machine, the registrant shall determine, or

obtain from the manufacturer, the maximum value(s) specified in subdivisions 2 and 3 of this subsection for the specified operating conditions. Records of these maximum value(s) shall be maintained at the installation for inspection by the agency.

J. Termination of irradiation by the beam monitoring system or systems during stationary beam radiation therapy.

1. Each primary system shall terminate irradiation when the preselected number of dose monitor units has been detected by the system;

2. If the original design of the equipment included a secondary dose monitoring system, that system shall be capable of terminating irradiation when not more than 15% or 40 dose monitor units above the preselected number of dose monitor units set at the control panel has been detected by the secondary dose monitoring system; and

3. For equipment manufactured after September 20, 2006, an indicator on the control panel shall show which monitoring system has terminated irradiation.

K. Termination of irradiation. It shall be possible to terminate irradiation and equipment movement or go from an interruption condition to termination condition at any time from the operator's position at the treatment control panel.

L. Interruption of irradiation. If a therapeutic radiation machine has an interrupt mode, it shall be possible to interrupt irradiation and equipment movements at any time from the treatment control panel. Following an interruption it shall be possible to restart irradiation by operator action without any reselection of operating conditions. If any change is made of a preselected value during an interruption, irradiation and equipment movements shall be automatically terminated.

M. Timer. A suitable irradiation control device shall be provided to terminate the irradiation after a pre-set time interval.

1. A timer shall be provided which has a display at the treatment control panel. The timer shall have a pre-set time selector and an elapsed time indicator;

2. The timer shall be a cumulative timer that activates with an indication of "BEAM-ON" and retains its reading after irradiation is interrupted or terminated. After irradiation is terminated and before irradiation can be reinitiated, it shall be necessary to reset the elapsed time indicator;

3. The timer shall terminate irradiation when a preselected time has elapsed, if the dose monitoring systems have not previously terminated irradiation.

N. Selection of radiation type. Equipment capable of both X-ray therapy and electron therapy shall meet the following additional requirements:

1. Irradiation shall not be possible until a selection of radiation type (X-rays or electrons) has been made at the treatment control panel;

2. The radiation type selected shall be displayed at the treatment control panel before and during irradiation;

3. An interlock system shall be provided to ensure that the equipment can principally emit only the radiation type that has been selected;

4. An interlock system shall be provided to prevent irradiation with X-rays, except to obtain an image, when electron applicators are fitted;

5. An interlock system shall be provided to prevent irradiation with electrons when accessories specific for X-ray therapy are fitted; and

6. An interlock system shall be provided to prevent irradiation if any selected operations carried out in the treatment room do not agree with the selected operations carried out at the treatment control panel.

O. Selection of energy. Equipment capable of generating radiation beams of different energies shall meet the following requirements:

1. Irradiation shall not be possible until a selection of energy has been made at the treatment control panel;

2. The nominal energy value selected shall be displayed at the treatment control panel until reset manually for the next irradiation. After termination of irradiation, it shall be necessary to reset the nominal energy value selected before

subsequent treatment can be initiated;

3. Irradiation shall not be possible until the appropriate flattening filter or scattering foil for the selected energy is in its proper location; and

4. For equipment manufactured after September 20, 2006, the selection of energy shall be in compliance with International Electrotechnical Commission (IEC) Document 601-2-1.

P. Selection of stationary beam radiation therapy or moving beam radiation therapy.

Therapeutic radiation machines capable of both stationary beam radiation therapy and moving beam radiation therapy shall meet the following requirements:

1. Irradiation shall not be possible until a selection of stationary beam radiation therapy or moving beam radiation therapy has been made at the treatment control panel;

2. The mode of operation shall be displayed at the treatment control panel;

3. An interlock system shall be provided to ensure that the equipment can operate only in the mode that has been selected;

4. An interlock system shall be provided to prevent irradiation if any selected parameter in the treatment room does not agree with the selected parameter at the treatment control panel;

5. Moving beam radiation therapy shall be controlled to obtain the selected relationships between incremental dose monitor units and incremental movement. For equipment manufactured after September 20, 2006:

a. An interlock system shall be provided to terminate irradiation if the number of dose monitor units delivered in any 10 degrees of rotation or one cm of linear motion differs by more than 20% from the selected value;

b. Where angle terminates the irradiation in moving beam radiation therapy, the dose monitor units delivered shall differ by less than 5.0% from the dose monitor unit value selected;

c. An interlock shall be provided to prevent motion of more than five degrees

or one cm beyond the selected limits during moving beam radiation therapy;

d. An interlock shall be provided to require that a selection of direction be made at the treatment control panel in all units that are capable of both clockwise and counter-clockwise moving beam radiation therapy.

e. Moving beam radiation therapy shall be controlled with both primary position sensors and secondary position sensors to obtain the selected relationships between incremental dose monitor units and incremental movement.

6. Where the beam monitor system terminates the irradiation in moving beam radiation therapy, the termination of irradiation shall be as required by 12VAC5-481-3430 J; and

7. For equipment manufactured after September 20, 2006, an interlock system shall be provided to terminate irradiation if movement:

a. Occurs during stationary beam radiation therapy; or

b. Does not start or stops during moving beam radiation therapy unless such stoppage is a pre-planned function.

Q. Facility design requirements for therapeutic radiation machines operating above 500 kV. In addition to shielding adequate to meet requirements of 12VAC5-481-3450, the following design requirements are made:

1. Protective barriers. All protective barriers shall be fixed, except for access doors to the treatment room or movable beam interceptors;

2. Control panel. In addition to other requirements specified in Part XV (12VAC5-481-3380 et seq.) of this chapter, the control panel shall also:

a. Be located outside the treatment room;

b. Provide an indication of whether electrical power is available at the control panel and if activation of the radiation is possible;

c. Provide an indication of whether radiation is being produced; and

d. Include an access control (locking) device that will prevent unauthorized

use of the therapeutic radiation machine;

3. Viewing systems. Windows, mirrors, closed-circuit television or an equivalent viewing system shall be provided to permit continuous observation of the patient following positioning and during irradiation and shall be so located that the operator may observe the patient from the treatment control panel. The therapeutic radiation machine shall not be used for patient irradiation unless at least one viewing system is operational;

4. Aural communications. Provision shall be made for continuous aural communication between the patient and the operator at the control panel. The therapeutic radiation machine shall not be used for irradiation of patients unless continuous aural communication is possible;

5. Room entrances. Treatment room entrances shall be provided with warning lights in a readily observable position near the outside of all access doors, which will indicate when the useful beam is "ON" and when it is "OFF";

6. Entrance interlocks. Interlocks shall be provided such that all access controls are activated before treatment can be initiated or continued. If the radiation beam is interrupted by any access control, it shall not be possible to restore the machine to operation without resetting the access control and reinitiating irradiation by manual action at the control panel;

7. Beam interceptor interlocks. If the shielding material in any protective barrier requires the presence of a beam interceptor to ensure compliance with 12VAC5-481-720, interlocks shall be provided to prevent the production of radiation, unless the beam interceptor is in place, whenever the useful beam is directed at the designated barrier(s);

8. Emergency cutoff switches. At least one emergency power cutoff switch shall be located in the radiation therapy room and shall terminate all equipment electrical power including radiation and mechanical motion. This switch is in addition to the termination switch required by subsection K of this section. All emergency power cutoff switches shall include a manual reset so that the

therapeutic radiation machine cannot be restarted from the unit's control console without resetting the emergency cutoff switch;

9. Safety interlocks. All safety interlocks shall be designed so that any defect or component failure in the safety interlock system prevents or terminates operation of the therapeutic radiation machine; and

10. Surveys for residual radiation. Surveys for residual activity shall be conducted on all therapeutic radiation machines capable of generating photon and electron energies above 10 MV prior to machining, removing from treatment room, or working on therapeutic radiation machine components which may have become activated due to photo-neutron production.

R. Radiation therapy physicist support.

1. The services of a radiation therapy physicist shall be required in facilities having therapeutic radiation machines with energies of 500 kV and above. The radiation therapy physicist shall be responsible for:

a. Full calibration(s) required by subsection T of this section and surveys required by 12VAC5-481-3400 A;

b. Supervision and review of dosimetry;

c. Beam data acquisition and transfer for computerized dosimetry, and supervision of its use;

d. Quality assurance, including quality assurance check review required by subdivision U 5 of this section.

e. Consultation with the authorized user in treatment planning, as needed; and

f. Performance of calculations/assessments regarding misadministrations.

2. If the radiation therapy physicist is not a full-time employee of the registrant, the operating procedures required by subsection S of this section shall also specifically address how the radiation therapy physicist is to be contacted for problems or emergencies, as well as the specific actions, if any, to be taken until

the radiation therapy physicist can be contacted.

S. Operating procedures.

1. No individual, other than the patient, shall be in the treatment room during treatment or during any irradiation for testing or calibration purposes;
2. Therapeutic radiation machines shall not be made available for medical use unless the requirements of 12VAC5-481-3400 A, and subsections T and U of this section have been met;
3. Therapeutic radiation machines, when not in operation, shall be secured to prevent unauthorized use;
4. When adjustable beam limiting devices are used, the position and shape of the radiation field shall be indicated by a light field.
5. If a patient must be held in position during treatment, mechanical supporting or restraining devices shall be used; and
6. A copy of the current operating and emergency procedures shall be maintained at the therapeutic radiation machine control console.

T. Acceptance testing, commissioning and full calibration measurements.

1. Acceptance testing, commissioning and full calibration of a therapeutic radiation machine subject to this section shall be performed by, or under the direct supervision of, a radiation therapy physicist.
2. Acceptance testing and commissioning shall be performed in accordance with "AAPM Code of Practice for Radiotherapy Accelerators: Report of AAPM Radiation Therapy Task Group 45" and shall be conducted before the first medical use following installation or reinstallation of the therapeutic radiation machine.
3. Full calibration shall include measurement of all parameters required by Table II of "Comprehensive QA for Radiation Oncology: Report of AAPM Radiation Therapy Committee Task Group 40" and shall be performed in accordance with "AAPM Code of Practice for Radiotherapy Accelerators: Report of AAPM

Radiation Therapy Task Group 45". Although it shall not be necessary to complete all elements of a full calibration at the same time, all parameters (for all energies) shall be completed at intervals not exceeding 12 calendar months, unless a more frequent interval is required in Table II.

4. The radiation therapy physicist shall perform all elements of a full calibration necessary to determine that all parameters are within acceptable limits:

a. Whenever quality assurance check measurements indicate that the radiation output differs by more than 5.0% from the value obtained at the last full calibration and the difference cannot be reconciled. Therapeutic radiation machines with multienergy and/or multimode capabilities shall only require measurements for those modes and/or energies that are not within their acceptable range; and

b. Following any component replacement, major repair, or modification of components that could significantly affect the characteristics of the radiation beam. If the repair, replacement or modification does not affect all modes and/or energies, measurements shall be performed on the effected mode/energy that is in most frequent clinical use at the facility. The remaining energies/modes may be validated with quality assurance check procedures against the criteria in subdivision 4 a of this subsection.

5. The registrant shall maintain a record of each calibration in an auditable form for the duration of the registration. The record shall include: the date of the calibration; the manufacturer's name, model number and serial number for the therapeutic radiation machine; the model numbers and serial numbers of the instruments used to calibrate the therapeutic radiation machine; and the signature of the radiation therapy physicist responsible for performing the calibration.

U. Periodic quality assurance checks.

1. Periodic quality assurance checks shall be performed on all therapeutic radiation machines subject to this section at intervals not to exceed those

specified in "Comprehensive QA for Radiation Oncology: Report of AAPM Radiation Therapy Committee Task Group 40";

2. To satisfy the requirement of subdivision 1 of this subsection, quality assurance checks shall include determination of central axis radiation output and a representative sampling of periodic quality assurance checks contained in "Comprehensive QA for Radiation Oncology: Report of AAPM Radiation Therapy Committee Task Group 40". Representative sampling shall include all referenced periodic quality assurance checks in an interval not to exceed 12 consecutive calendar months;

3. The registrant shall use a dosimetry system that has been inter-compared within the previous 12 months with the dosimetry system described in 12VAC5-481-3400 C 1 to make the periodic quality assurance checks required in subdivision 2 of this subsection;

4. The registrant shall perform periodic quality assurance checks required by subdivision 1 of this subsection in accordance with procedures established by the radiation therapy physicist;

5. The registrant shall review the results of each periodic radiation output check according to the following procedures:

a. The authorized user and radiation therapy physicist shall be immediately notified if any parameter is not within its acceptable tolerance. The therapeutic radiation machine shall not be made available for subsequent medical use until the radiation therapy physicist has determined that all parameters are within their acceptable tolerances;

b. If all quality assurance check parameters appear to be within their acceptable ranges, the quality assurance check shall be reviewed and signed by either the authorized user or radiation therapy physicist within three treatment days; and

c. The radiation therapy physicist shall review and sign the results of each radiation output quality assurance check at intervals not to exceed one

month.

6. Therapeutic radiation machines subject to this section shall have safety quality assurance checks listed in "Comprehensive QA for Radiation Oncology: Report of AAPM Radiation Therapy Committee Task Group 40" performed at intervals not to exceed one week;

7. To satisfy the requirement of subdivision 6 of this subsection, safety quality assurance checks shall ensure proper operation of:

a. Electrical interlocks at each external beam radiation therapy room entrance;

b. Proper operation of the "BEAM-ON", interrupt and termination switches;

c. Beam condition indicator lights on the access doors, control console, and in the radiation therapy room;

d. Viewing systems;

e. Electrically operated treatment room door(s) from inside and outside the treatment room;

f. At least one emergency power cutoff switch. If more than one emergency power cutoff switch is installed and not all switches are tested at once, each switch shall be tested on a rotating basis. Safety quality assurance checks of the emergency power cutoff switches may be conducted at the end of the treatment day in order to minimize possible stability problems with the therapeutic radiation machine.

8. The registrant shall promptly repair any system identified in subdivision 7 of this subsection that is not operating properly; and

9. The registrant shall maintain a record of each quality assurance check required by subdivisions 1 and 7 of this subsection for three years. The record shall include: the date of the quality assurance check; the manufacturer's name, model number, and serial number of the therapeutic radiation machine; the manufacturer's name, model number and serial number for the instrument(s)

used to measure the radiation output of the therapeutic radiation machine; and the signature of the individual who performed the periodic quality assurance check.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3440. Calibration of survey instruments.

A. The registrant shall ensure that the survey instruments used to show compliance with Part XV (12VAC5-481-3380 et seq.) of this chapter have been calibrated before first use, at intervals not to exceed 12 months, and following repair.

B. To satisfy the requirements of subsection A of this section, the registrant shall:

1. Calibrate all required scale readings up to 10 mSv (1000 mrem) per hour with an appropriate radiation source that is traceable to the National Institute of Standards and Technology (NIST);
2. Calibrate at least two (2) points on each scale to be calibrated. These points should be at approximately 1/3 and 2/3 of full-scale; and

C. To satisfy the requirements of subsection B of this section, the registrant shall:

1. Consider a point as calibrated if the indicated dose rate differs from the calculated dose rate by not more than 10%; and
2. Consider a point as calibrated if the indicated dose rate differs from the calculated dose rate by not more than 20% if a correction factor or graph is conspicuously attached to the instrument.

D. The registrant shall retain a record of each calibration required in subsection A of this section for three years. The record shall include:

1. A description of the calibration procedure; and
2. A description of the source used and the certified dose rates from the source,

and the rates indicated by the instrument being calibrated, the correction factors deduced from the calibration data, the signature of the individual who performed the calibration, and the date of calibration.

E. The registrant may obtain the services of individuals licensed by the agency, the NRC, or another agreement state to perform calibrations of survey instruments. Records of calibrations that contain information required by subsection D of this section shall be maintained by the registrant.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3450. Shielding and safety design requirements.

A. Each therapeutic radiation machine subject to 12VAC5-481-3420 or 12VAC5-481-3430 shall be provided with such primary and/or secondary barriers as are necessary to ensure compliance with 12VAC5-481-640 and 12VAC5-481-720.

B. Facility design information for all new installations of a therapeutic radiation machine or installations of a therapeutic radiation machine of higher energy into a room not previously approved for that energy shall be submitted for agency approval prior to actual installation of the therapeutic radiation machine.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

Part XVI

Regulation and Licensing of Technologically Enhanced Naturally Occurring Radioactive Materials (TENORM)

12VAC5-481-3460. Purpose.

This part establishes radiation protection standards for the possession, use, transfer, and disposal of Technologically Enhanced Naturally Occurring Radioactive Materials (TENORM).

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3470. Scope.

A. These regulations apply to any person who receives, owns, possesses, uses, processes, transfers, distributes, or disposes of TENORM.

B. The regulations in this part address the introduction of TENORM into products in which neither the TENORM, nor the radiation emitted from the TENORM, is considered to be beneficial to the products.

C. The manufacture and distribution of products containing TENORM, in which the TENORM and/or its emitted radiation is considered to be a beneficial attribute, are licensed under the provisions of Part III (12VAC5-481-380 et seq.) of this chapter.

D. This part does not apply to radionuclides for which NRC retains exclusive jurisdiction.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3480. Exemptions.

A. Persons who receive, own, possess, use, process, transfer, distribute, or dispose of TENORM are exempt from the requirements of this part (12VAC5-481-3460 et seq.) of this chapter with respect to any combination of radium-226 and radium-228 if the materials contain, or are contaminated at, concentrations less than 185 Bq/kg (5 pCi/gm) excluding natural background. This does not apply to consumer or retail

products that are discussed in 12VAC5-481-3560 C and 12VAC5-481-3570. Using purposeful dilution to render TENORM waste exempt shall not be allowed without prior agency approval.

B. Persons who receive products or materials containing TENORM distributed in accordance with a specific license issued by the agency pursuant to 12VAC5-481-3540 1, or to an equivalent license issued by another licensing state, are exempt from these regulations with regard to those products or materials.

C. The distribution, including custom blending, possession, and use of fertilizers containing TENORM, is exempt from the requirements of this part.

D. TENORM waste regulated by CERCLA (The Comprehensive Environmental Response, Compensation, and Liability Act) or RCRA (Resources Conservation and Recovery Act) are exempt from this part.

E. The transportation and storage incident to transportation are governed by other parts of these regulations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3490. Standards for radiation protection for TENORM.

A. No person licensed under 12VAC5 481-3530 or 12VAC5-481-3540 shall conduct operations, use, or transfer TENORM in a manner such that a member of the public will receive an annual total effective dose equivalent in excess of 1mSv (100 mrem) per year from all licensed sources including TENORM.

B. Persons subject to a license under this part shall comply with radiation protection standards set out in Part IV (12VAC5-481-600 et seq.) of this chapter.

C. Doses from indoor radon and its progeny shall not be included in total effective dose equivalent calculations.

D. No person shall release TENORM for unrestricted use in such a manner that the reasonably maximally exposed individual will receive an annual total effective dose equivalent from the released TENORM in excess of 1mSv (100 mrem) per year excluding natural background.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3500. Protection of Workers During Operations.

Each person subject to a specific license under Part XVI of this chapter shall conduct operations in compliance with the standards for radiation protection set out in other parts of these regulations.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3510. Release for unrestricted use.

Each person subject to a license under this part shall:

1. Not transfer or release for unrestricted use facilities or equipment contaminated with TENORM in excess of levels in Table 6.

Table 6. Acceptable Surface Contamination Levels ¹ for TENORM.			
	AVERAGE ^{2,3,6}	MAXIMUM ^{2,4,6}	REMOVABLE ^{2,3,5,6}
Alpha	5,000 dpm/100 cm ²	15,000 dpm/100 cm ²	1,000 dpm/100 cm ²
Beta-gamma	5,000 dpm/100 cm ²	15,000 dpm/100 cm ²	1,000 dpm/100 cm ²

¹Where surface contamination by both alpha and beta-gamma emitting nuclides exists, the limits established for alpha and beta-gamma emitting nuclides should apply independently.

²As used in this table, dpm (disintegrations per minute) means the rate of emission by radioactive material as determined by correcting the counts per minute observed by an appropriate detector for background, efficiency, and geometric factors associated with the instrumentation.

³Measurements of average contamination level should not be averaged over more than one square meter. For objects of less surface area, the average should be derived for each object.

⁴The maximum contamination level applies to an area of not more than 100 cm².

⁵The amount of removable radioactive material per 100 cm² of surface area should be determined by wiping that area with dry filter or soft absorbent paper, applying moderate pressure, and assessing the amount of radioactive material on the wipe with an appropriate instrument of known efficiency. When removable contamination on objects of surface area A (where A is less than 100 sq. cm) is determined, the entire surface should be wiped and the contamination level multiplied by 100/A to convert a "per 100 sq. cm" basis.

⁶The average and minimum radiation levels associated with surface contamination resulting from beta-gamma emitters should not exceed 0.2 mrad/hr (2 Gy/hr) at 1 cm, respectively, measured through not more than 7 milligrams per square centimeter of total absorber.

2. Not transfer or release for unrestricted use equipment contaminated with TENORM in excess of a surface gamma radiation level of 200 µrem/hr at 1 cm excluding natural background; and

3. Not transfer land for unrestricted use where the concentration of radium-226 or radium-228 in soil averaged over any 100 square meters exceeds the background level by more than 185 Bq/kg (5 pCi/gm), averaged over any 15 cm layer of soil below the surface, unless compliance with 12VAC5-481-3490 B through D can be demonstrated.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3520. Disposal and transfer of waste for disposal.

A. Each person subject to a license under this part shall manage and dispose of wastes containing TENORM:

1. By transfer of the wastes for disposal to a facility licensed under requirements for uranium or thorium byproduct materials in either 40 CFR Part 192 or 10 CFR Part 40 Appendix R;
2. By transfer of the wastes for disposal to a disposal facility licensed by the NRC, or another agreement state; or
3. In accordance with alternate methods authorized by the agency upon application or upon the agency's initiative, consistent with 12VAC5-481-3490 and where applicable the Clean Water Act, Safe Drinking Water Act and other requirements of the United States Environmental Protection Agency for disposal of such wastes.

B. Equipment contaminated with TENORM in excess of levels specified in Table 6 of this part, which is to be disposed of as waste, shall be disposed of:

1. So as to prevent any reintroduction into commerce or unrestricted use; and
2. Within disposal areas specifically designed to meet the criteria of subsection A of this section.

C. Transfers of waste containing TENORM for disposal shall be made only to a person specifically authorized by the NRC, or another agreement state, to receive such waste.

D. Records of disposal, including manifests, shall be maintained pursuant to the provisions of Part IV (12VAC5-481-600 et seq.) of this chapter.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3530. General license.

A. Subject to the requirements of 12VAC5-481-3490 through 12VAC5-481-3520 and 12VAC5-481-3540, a general license is hereby issued to possess, own, use, transfer,

distribute or dispose of TENORM without regard to quantity.

B. This general license does not authorize the manufacturing of products containing TENORM in concentrations greater than those specified in 12VAC5-481-3480 A nor the receipt and disposal of wastes from other persons.

C. The decontamination of equipment, facilities, and land shall be performed only by persons specifically licensed by the agency, NRC or another agreement state to conduct such work. However, employees or contractors under control and supervision of a general licensee can perform routine maintenance on equipment, facilities, and land owned or controlled by the general licensee. Maintenance that provides a different pathway for exposure than is found in daily operations and that increases the potential for additional exposure is not considered routine.

D. Any person subject to the general license issued by this section shall notify the agency. Such notification shall include:

1. Name and address of the licensee;
2. Location and description of the facility or operation; and
3. Description of the TENORM including estimates of the amount and extent of TENORM.

E. Transfer of material or real property.

1. The transfer of TENORM not exempt from these regulations from one general licensee to another general licensee is authorized if:

- a. The equipment and facilities contaminated with TENORM are to be used by the recipient for the same purpose; or
- b. The transfer of control or ownership of land contaminated with TENORM includes an annotation of the deed records, or notice to owners of surface and mineral rights, to indicate the presence of TENORM.

2. Transfers not made in accordance with subdivision 1 of this subsection require prior approval by the agency.

3. Transfers made under subdivision 1 of this subsection do not relieve the

general licensee who makes the transfer from the responsibilities of assessing the extent of TENORM contamination or material present, informing the general licensee receiving the TENORM of these assessments, and maintaining records required by this chapter.

4. A general licensee intending to transfer material or real property for unrestricted use shall document compliance with the requirements of 12VAC5-481-3510.

F. Distribution of TENORM products between general licensees. The distribution of TENORM products not exempt from these regulations from one general licensee to another general licensee is authorized provided the product is accompanied by labels or manifests which identify the type and amount of TENORM.

G. The agency may, by written notice, require any person authorized by a general license to apply for and obtain a specific license. The notice shall state the reason or reasons for requiring a specific license.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3540. Specific Licenses.

Unless otherwise exempt, a specific license is required to:

1. Manufacture and distribute any material or product containing TENORM unless authorized by 12VAC5-481-3530 F, exempted under the provisions of 12VAC5-481-3480, or licensed under the provisions of Part III (12VAC5-481-380 et seq.) of this chapter;
2. Except as provided in 12VAC5-481-3530 C, decontaminate equipment or land not otherwise exempted under the provisions of 12VAC5-481-3480 or facilities contaminated with TENORM in excess of the levels set forth in 12VAC5-481-

3510, as applicable; for purposes of this subsection, the term "decontaminate" shall not include maintenance that incidentally results in removal of contamination;

3. Receive TENORM from other persons for disposal.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3550. Filing application for specific licenses.

A. Applications for specific licenses shall be filed in a manner and on a form prescribed by the agency.

B. The agency may at any time after the filing of the original application, and before the expiration of the license, require further statements in order to enable the agency to determine whether the application should be granted or denied or whether a license should be modified or revoked.

C. Each application shall be signed by the applicant or licensee or a person duly authorized to act for and on the licensee's behalf.

D. An application for a license may include a request for a license authorizing one or more activities.

E. Each application for a specific license shall be accompanied by a fee of \$50.

F. In an application, the applicant may incorporate by reference information contained in previous applications, statements, or reports filed with the agency provided such references are clear and specific.

G. Applications and documents submitted to the agency may be made available for public inspection.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3560. Requirements for the issuance of specific licenses.

A. A license application will be approved if the agency determines that:

1. The applicant is qualified by reason of training and experience to use the TENORM in question for the purpose requested in accordance with these rules in such a manner as to protect the public health and safety or property;
2. The applicant's proposed equipment, facilities, and procedures are adequate to protect the public health and safety or property;
3. The issuance of the license will not be inimical to the health and safety of the public;
4. The applicant satisfied all applicable special requirements in this part;
5. The applicant has met the financial surety requirements of 12VAC5-481-450 C; and
6. The applicant has adequately addressed the following items in the application:
 - a. Procedures and equipment for monitoring and protecting workers;
 - b. An evaluation of the radiation levels and concentrations of contamination expected during normal operations;
 - c. Operating and emergency procedures, including procedures for waste reduction and quality assurance of items released for unrestricted use; and
 - d. A method for managing the radioactive material removed from contaminated equipment and facilities.

B. An application for a specific license to decontaminate equipment, land, or facilities contaminated with TENORM in excess of the levels set forth in 12VAC5-481-3480 A, 12VAC5-481-3510 2, or Table 6, as applicable, and to dispose of the resulting waste will be approved if:

1. The applicant satisfies the general requirements specified in subsection A of this section; and
2. The applicant has adequately addressed the following items in the application:

- a. Procedures and equipment for monitoring and protection of workers;
- b. An evaluation of the radiation levels and concentrations of contamination expected during normal operations;
- c. Operating and emergency procedures, including procedures for waste reduction and quality assurance of items released for unrestricted use; and
- d. Method of disposing of the TENORM removed from contaminated equipment, facilities, and/or land.

C. An application for a specific license to transfer materials or manufacture or distribute products containing TENORM to persons exempted from these regulations pursuant to 12VAC5-481-3530 B will be approved if:

1. The applicant satisfies the general requirements specified in subsection A of this section;
2. The TENORM is not contained in any food, beverage, cosmetic, drug, or other commodity designed for ingestion or inhalation by, or application to, a human being; and
3. The applicant submits sufficient information relating to the design, manufacture, prototype testing, quality control procedures, labeling or marking, and conditions of handling, storage, use, and disposal of the TENORM material or product to demonstrate that the material or product will meet the safety criteria set forth in 12VAC5-481-3570. The information shall include:
 - a. A description of the material or product and its intended use or uses;
 - b. The type, quantity, and concentration of TENORM in each material or product;
 - c. The chemical and physical form of the TENORM in the material or product, and changes in chemical and physical form that may occur during the useful life of the material or product;
 - d. An analysis of the solubility in water and body fluids of the TENORM in the material or product;

- e. The details of manufacture and design of the material or product relating to containment and shielding of the TENORM and other safety features under normal and severe conditions of handling, storage, use, reuse, and disposal of the material or product;
- f. The degree of access of human beings to the material or product during normal handling, use, and disposal;
- g. The total quantity of TENORM expected to be distributed annually in the material or product;
- h. The expected useful life of the material or product;
- i. The proposed method of labeling or marking each unit of the material or product with identification of the manufacturer or initial transferor of the product and the radionuclides and quantity of TENORM in the material or product;
- j. The procedures for prototype testing of the material or product to demonstrate the effectiveness of the containment, shielding, and other safety features under both normal and severe conditions of handling, storage, use, reuse, and disposal;
- k. The results of the prototype testing of the material or product, including any change in the form of the TENORM contained in it, the extent to which the TENORM may be released to the environment, any change in radiation levels, and any other changes in safety features;
- l. The estimated external radiation doses and dose commitments relevant to the safety criteria in 12VAC5-481-3570 and the basis for such estimates;
- m. A determination that the probabilities with respect to doses referred to in 12VAC5-481-3570 meet the safety criteria;
- n. The quality control procedures to be followed in the production of production lots of the material or product, and the quality control standards the material or product will be required to meet; and

o. Any additional information, including experimental studies and tests, required by the agency to facilitate a determination of the radiation safety of the material or product.

D. Notwithstanding the provisions of subdivision 2 of 12VAC5-481-3570, the agency may deny an application for a specific license if the end uses of the product are frivolous or cannot be reasonably foreseen.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3570. Safety Criteria for Products.

An applicant for a license under 12VAC5-481-3560 C shall demonstrate that the product is designed and will be manufactured so that:

1. In normal use and disposal of a single exempt item, and in normal handling and storage of the quantities of exempt items likely to accumulate in one location during marketing, distribution, installation, and servicing of the product, it is unlikely that the TEDE in any one year, to a suitable sample of the group of individuals expected to be most highly exposed to radiation or radioactive material from the product will exceed the doses in Column I of 12VAC5-481-3580.
2. In use and disposal of a single exempt item and in handling and storage of the quantities of exempt items likely to accumulate in one location during marketing, distribution, installation, and servicing of the product, the probability is low (not more than one failure per year for each 10,000 exempt units distributed) that the containment, shielding, or other safety features of the product would fail under such circumstances that a person would receive an external radiation dose or dose commitment in excess of the dose to the appropriate organ as specified in

Column II of the table in 12VAC5-481-3580 and the probability is negligible (not more than one such failure per year for each one millions exempt units distributed) that a person would receive an external radiation dose or dose commitment in excess of the dose to the appropriate organ as specified in Column III of the table in 12VAC5-481-3580. It is the intent of this paragraph that as the magnitude of the potential dose increases above that permitted under normal conditions, the probability that any individual will receive such a dose must decrease. The probabilities have been expressed in general terms to emphasize the approximate nature of the estimates that are to be made. The above values may be used a guidelines in estimating compliance with the criteria.

3. It is unlikely that there will be a significant reduction in the effectiveness of the containment, shielding, or other safety features of the product from wear and abuse likely to occur in normal handling and use of the product during its useful life.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3580. Table of organ doses.

Part of Body	Column I (rem)	Column II (rem)	Column III (rem)	Column IV (rem)
Whole body; head and trunk; active blood-forming organs; gonads; or lens of eye	0.001	0.01	0.5	15
Hands and forearms; feet and ankles; localized areas of skin averaged over areas no larger than 1 square centimeter	0.015	0.15	7.5	200
Other organs	0.003	0.03	1.5	50

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3590. Issuance of Specific Licenses.

A. Upon a determination that an application meets the requirements of these regulations, the agency will issue a specific license authorizing the proposed activity in such form and containing such conditions and limitations as it deems appropriate or necessary.

B. The agency may incorporate in any license at the time of issuance, or thereafter by amendment, such additional requirements and conditions with respect to the licensee's receipt, possession, use, and transfer of TENORM subject to this part as it deems appropriate or necessary in order to:

1. Protect public health and safety or property;
2. Require such reports and the keeping of such records, and to provide for such inspections of activities under the license as may be appropriate or necessary; and
3. Prevent loss, theft, or loss of control of TENORM subject to this part.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3600. Conditions of specific licenses issued under 12VAC5-481-3560.

A. General terms and conditions.

1. Each license issued pursuant to this part shall be subject to all the provisions of the Act, now or hereafter in effect, and to all rules, regulations, and orders of

the agency.

2. No license issued or granted under this part and no right to possess or utilize TENORM granted by any license issued pursuant to this part shall be transferred, assigned, or in any manner disposed of, either voluntarily or involuntarily, directly or indirectly, through transfer of control of any license to any person unless the agency shall, after securing full information, find that the transfer is in accordance with the provisions of the Act, and shall give its consent in writing.

3. Each person licensed by the agency pursuant to this part shall confine use and possession of the TENORM licensed to the locations and purposes authorized in the license.

4. Each person licensed by the agency pursuant to this part is subject to the general license provisions of 12VAC5-481-3500, 12VAC5-481-3510, and 12VAC5-481-3520.

5. Each licensee shall:

a. Notify the agency, in writing, immediately following the filing of a voluntary or involuntary petition for bankruptcy under any Chapters of Title II (Bankruptcy) of the United States Code (11 USC) by or against a licensee, an entity (as that term is defined in 11 USC §101 (15)) controlling a licensee or listing the license or licensee as property of the estate; or an affiliate (as that term is defined in 11 USC §101 (2)) of the licensee.

b. Indicate in their bankruptcy notification the bankruptcy court in which the petition for bankruptcy was filed; and the date of the filing of the petition.

B. Quality control, labeling, and reports of transfer. Each person licensed under 12VAC5-481-3560 C shall:

1. Carry out adequate control procedures in the manufacture of the product to assure that each production lot meets the quality control standards approved by the agency;

2. Label or mark each unit so that the manufacturer, processor, producer, or initial transferor of the material or product and the TENORM in the product can be identified; and
3. Maintain records identifying, by name and address, each person to whom TENORM is transferred for use under 12VAC5-481-3480 B or the equivalent regulations of another licensing state, and stating the kinds, quantities, and uses of TENORM transferred. An annual summary report stating the total quantity of each radionuclide transferred under the specific license shall be filed with the agency. Each report shall cover the year ending December 31, and shall be filed within 90 days thereafter. If no transfers of TENORM have been made pursuant to 12VAC5-481-3560 C during the reporting period, the report shall so indicate.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3610. Expiration and termination of specific licenses.

A. Except as provided in subdivision D 6 of this section and 12VAC5-481-3620 B, each specific license shall expire at the end of the specified day in the month and year stated therein.

B. Each licensee shall notify the agency in writing and request termination of the license when the licensee decides to terminate all activities involving TENORM authorized under the license. This notification and request for termination of the license must include the reports and information specified in subdivision D 4 of this section. The licensee is subject to the provisions of subsections D and E of this section, as applicable.

C. No less than 30 days before the expiration date specified in a specific license, the licensee shall either:

1. Submit an application for license renewal under 12VAC5-481-3620; or
2. Notify the agency in writing, under subsection B of this section, if the licensee decides to discontinue all activities involving TENORM.

D. If a licensee does not submit an application for license renewal under 12VAC5-481-3620, the licensee shall, on or before the expiration date specified in the license:

1. Terminate use of TENORM;
2. Remove TENORM contamination consistent with the requirements of 12VAC5-481-3510.
3. Properly dispose of TENORM; and
4. Submit a report of disposal of TENORM and radiation surveys to confirm the absence of TENORM or to establish the levels of residual TENORM contamination. The licensee shall, as appropriate:

- a. Report levels of radiation in units of microroentgens per hour of beta and gamma radiation at one centimeter and gamma radiation at one meter from surfaces and report levels of radioactivity in units of disintegrations per minute (or microcuries) per 100 square centimeters removable and fixed on surfaces, microcuries or Becquerel per milliliter in water, and picocuries or becquerels per gram in contaminated solids such as soils or concrete; and
- b. Specify the instruments used and certify that each instrument is properly calibrated and tested.

5. If levels of residual activity are less than those established in 12VAC5-481-3510, the licensee shall so certify. If the agency determines that this certification and the information submitted under subdivision 4 of this subsection is adequate and surveys confirm the findings, the agency will notify the licensee in writing that the license is terminated.

6. If levels of residual TENORM are not in conformance with criteria established in 12VAC5-481-3510, the license continues in effect beyond the expiration date, if necessary, with respect to possession of residual TENORM until the agency

notifies the licensee in writing that the license is terminated. During this time, the licensee is subject to the provisions of subsection E of this section. In addition to the information submitted under subdivision 4 of this subsection, the licensee shall submit a plan, if appropriate, for decontaminating the location(s) and disposing of this subsection of the residual TENORM.

E. Each licensee who possesses residual TENORM under subdivision D 6 of this section, following the expiration date specified in the license, shall:

1. Be limited to actions involving TENORM related to preparing the locations for release for unrestricted use; and
2. Continue to control entry to restricted areas until the locations are suitable for release for unrestricted use and the agency notifies the licensee in writing that the license is terminated.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3620. Renewal of specific licenses.

A. Applications for renewal of specific licenses shall be filed in accordance with 12VAC5-481-3550.

B. In any case in which a licensee, not less than 30 days prior to expiration of an existing license, has filed an application in proper form for renewal or for a new license authorizing the same activities, such existing license shall not expire until final action by the agency.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3630. Amendment of specific licenses at request of licensee.

Applications for amendment of a license shall be filed in accordance with 12VAC5-481-3550 and shall specify the respects in which the licensee desires the license to be amended and the grounds for such amendment.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3640. Agency action on applications to renew and amend specific licenses.

In considering an application by a licensee to renew or amend the license, the agency will apply the criteria set forth in 12VAC5-481-3560.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3650. Modification and revocation of specific licenses.

A. The terms and conditions of all licenses shall be subject to amendment, revision, or modification or the license may be suspended or revoked by reason of amendments to the Act, or by reason of rules, regulations, and orders issued by the agency.

B. Any license may be revoked, suspended, or modified, in whole or in part, for any material false statement in the application or any statement of fact required under provisions of the Act, or because of conditions revealed by such application or statement of fact or any report, record, or inspection or other means which would warrant the agency to refuse to grant a license on an original application, or for violation of, or failure to observe any of the terms and conditions of the Act, or of the license, or of any rule, regulation, or order of the agency.

C. Except in cases of willfulness or those in which the public health, interest or

safety requires otherwise, the agency shall not modify, suspend or revoke a license prior to the institution of proceedings unless facts or conduct that may warrant such action shall have been called to the attention of the licensee in writing and the licensee shall have been accorded an opportunity to demonstrate or achieve compliance with all lawful requirements.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; amended, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3660. Reciprocal recognition of specific licenses.

Subject to these regulations, any person who holds a specific license from an agreement state or a licensing state, and issued by the agency having jurisdiction where the licensee maintains an office for directing the licensed activity and at which radiation safety records are normally maintained, is hereby granted a general license to conduct the activities authorized in such licensing document within this state for a period not in excess of 180 days in any calendar year provided that:

1. The licensing document does not limit the activity authorized by such document to specified installations or locations;
2. The out-of-state licensee notifies the agency in writing at least three days prior to engaging in such activity. Such notification shall indicate the location, period, and type of proposed possession and use within the State, and shall be accompanied by a copy of the pertinent licensing document. If, for a specific case, the three-day period would impose an undue hardship on the out-of-state licensee, the licensee may, upon application to the agency, obtain permission to proceed sooner. The agency may waive the requirement for filing additional written notifications during the remainder of the calendar year following the receipt of the initial notification from a person engaging in activities under the general license provided in subdivision 1 of this section;

- 3. The out-of-state licensee complies with all applicable regulations of the agency and with all the terms and conditions of the licensing document, except any such terms and conditions which may be inconsistent with applicable regulations of the agency;
- 4. The out-of-state licensee supplies such other information as the agency may request; and
- 5. The out-of-state licensee shall not transfer or dispose of TENORM possessed or used under the general license provided in subsection A of this section, except by transfer to a person:
 - a. Specifically licensed by the agency or by another licensing state to receive such TENORM; or
 - b. Exempt from the requirements for a license for such TENORM under 12VAC5-481-3480.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006.

12VAC5-481-3670. (Repealed.)

Historical Notes

Derived from Virginia Register Volume 22, Issue 25, eff. September 20, 2006; repealed, Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

Part XVII

Schedules

12VAC5-481-3680. Assigned protection factors for respirators.

	Operating mode	Assigned Protection Factors
I. Air Purifying Respirators (Particulate ^b only) ^c :		
Filtering facepiece disposable ^d	Negative Pressure	(d)

Facepiece, half ^e	Negative Pressure	10
Facepiece, full	Negative Pressure	100
Facepiece, half	Powered air-purifying respirators	50
Facepiece, full	Powered air-purifying respirators	1000
Helmet/hood	Powered air-purifying respirators	1000
Facepiece, loose-fitting	Powered air-purifying respirators	25

II. Atmosphere supplying respirators (particulate, gases and vapors^f):

1. Air-line respirator:

Facepiece, half	Demand	10
Facepiece, half	Continuous Flow	50
Facepiece, half	Pressure Demand	50
Facepiece, full	Demand	100
Facepiece, full	Continuous Flow	1000
Facepiece, full	Pressure Demand	1000
Helmet/hood	Continuous Flow	1000
Facepiece, loose-fitting	Continuous Flow	25
Suit	Continuous Flow	(g)

2. Self-contained breathing Apparatus (SCBA):

Facepiece, full	Demand	^h 100
Facepiece, full	Pressure Demand	ⁱ 10,000
Facepiece, full	Demand, Recirculating	^h 100
Facepiece, full	Positive Pressure Recirculating	ⁱ 10,000

III. Combination Respirators:

Any combination of air-purifying and atmosphere-supplying respirators

Assigned protection factor for type and mode of operation as listed above.

^aThese assigned protection factors apply only in a respiratory protection program that meets the requirements of this section. They are applicable only to airborne radiological

hazards and may not be appropriate to circumstances when chemical or other respiratory hazards exist instead of, or in addition to, radioactive hazards. Selection and use of respirators for such circumstances must also comply with Department of Labor regulations.

Radioactive contaminants for which the concentration values in Table 1, Column 3 of 12VAC5-481-3690 are based on internal dose due to inhalation may, in addition, present external exposure hazards at higher concentrations. Under these circumstances, limitations on occupancy may have to be governed by external dose limits.

^bAir purifying respirators with APF <100 must be equipped with particulate filters that are at least 95% efficient. Air purifying respirators with APF = 100 must be equipped with particulate filters that are at least 99% efficient. Air purifying respirators with APFs >100 must be equipped with particulate filters that are at least 99.97% efficient.

^cThe licensee may apply to VDH for the use of an APF greater than 1 for absorbent cartridges as protection against airborne radioactive gases and vapors (e.g., radioiodine).

^dLicensees may permit individuals to use this type of respirator who have not been medically screened or fit tested on the device provided that no credit be taken for their use in estimating intake or dose. It is also recognized that it is difficult to perform an effective positive or negative pressure pre-use user seal check on this type of device. All other respiratory protection program requirements listed in 12VAC5-481-820 apply. An assigned protection factor has not been assigned for these devices. However, an APF equal to 10 may be used if the licensee can demonstrate a fit factor of at least 100 by use of a validated or evaluated, qualitative or quantitative fit test.

^eUnder-chin type only. No distinction is made in this section between elastomeric half-masks with replaceable cartridges and those designed with the filter medium as an integral part of the facepiece (e.g., disposable or reusable disposable). Both types are acceptable so long as the seal area of the latter contains some substantial type of seal-enhancing material such as rubber or plastic, the two or more suspension straps are

adjustable, the filter medium is at least 95 percent efficient and all other requirements of this section are met.

^fThe assigned protection factors for gases and vapors are not applicable to radioactive contaminants that present an absorption or submersion hazard. For tritium oxide vapor, approximately one-third of the intake occurs by absorption through the skin so that an overall protection factor of 3 is appropriate when atmosphere-supplying respirators are used to protect against tritium oxide. Exposure to radioactive noble gases is not considered a significant respiratory hazard, and protective actions for these contaminants should be based on external (submersion) dose considerations.

^gNo NIOSH approval schedule is currently available for atmosphere supplying suits. This equipment may be used in an acceptable respiratory protection program as long as all the other minimum program requirements, with the exception of fit testing, are met (i.e., 12VAC5-481-820).

^hThe licensee should implement institutional controls to assure that these devices are not used in areas immediately dangerous to life or health (IDLH).

ⁱThis type of respirator may be used as an emergency device in unknown concentrations for protection against inhalation hazards. External radiation hazards and other limitations to permitted exposure such as skin absorption shall be taken into account in these circumstances. This device may not be used by any individual who experiences perceptible outward leakage of breathing gas while wearing the device.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3690. Annual Limits on Intake (ALI) and Derived Air Concentrations (DACs) of radionuclides for occupational exposure; effluent concentrations; concentration.

The following regulation, Annual Limits on Intake (ALI)s and Derived Air

Concentrations (DACs) of Radionuclides for Occupational Exposure; Effluent Concentrations; Concentrations for Release to Sewerage, 10 CFR Part 20 - Appendix B, is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3700. Quantities of licensed materials requiring labeling.

Radionuclide	Abbreviation	Quantity (μCi)
Hydrogen-3	H-3	1,000
Beryllium-7	Be-7	1,000
Beryllium-10	Be-10	1
Carbon-11	C-11	1,000
Carbon-14	C-14	100
Fluorine-18	F-18	1,000
Sodium-22	Na-22	10
Sodium-24	Na-24	100
Magnesium-28	Mg-28	100
Aluminum-26	Al-26	10
Silicon-31	Si-31	1,000
Silicon-32	Si-32	1
Phosphorus-32	P-32	10
Phosphorus-33	P-33	100
Sulfur-35	S-35	100
Chlorine-36	Cl-36	10
Chlorine-38	Cl-38	1,000
Chlorine-39	Cl-39	1,000
Argon-39	Ar-39	1,000
Argon-41	Ar-41	1,000
Potassium-40	K-40	100
Potassium-42	K-42	1,000
Potassium-43	K-43	1,000

Potassium-44	K-44	1,000
Potassium-45	K-45	1,000
Calcium-41	Ca-41	100
Calcium-45	Ca-45	100
Calcium-47	Ca-47	100
Scandium-43	Sc-43	1,000
Scandium-44m	Sc-44m	100
Scandium-44	Sc-44	100
Scandium-46	Sc-46	10
Scandium-47	Sc-47	100
Scandium-48	Sc-48	100
Scandium-49	Sc-49	1,000
Titanium-44	Ti-44	1
Titanium-45	Ti-45	1,000
Vanadium-47	V-47	1,000
Vanadium-48	V-48	100
Vanadium-49	V-49	1,000
Chromium-48	Cr-48	1,000
Chromium-49	Cr-49	1,000
Chromium-51	Cr-51	1,000
Manganese-51	Mn-51	1,000
Manganese-52m	Mn-52m	1,000
Manganese-52	Mn-52	100
Manganese-53	Mn-53	1,000
Manganese-54	Mn-54	100
Manganese-56	Mn-56	1,000
Iron-52	Fe-52	100
Iron-55	Fe-55	100
Iron-59	Fe-59	10
Iron-60	Fe-60	1
Cobalt-55	Co-55	100
Cobalt-56	Co-56	10
Cobalt-57	Co-57	100
Cobalt-58m	Co-58m	1,000

Cobalt-58	Co-58	100
Cobalt-60m	Co-60m	1,000
Cobalt-60	Co-60	1
Cobalt-61	Co-61	1,000
Cobalt-62m	Co-62m	1,000
Nickel-56	Ni-56	100
Nickel-57	Ni-57	100
Nickel-59	Ni-59	100
Nickel-63	Ni-63	100
Nickel-65	Ni-65	1,000
Nickel-66	Ni-66	10
Copper-60	Cu-60	1,000
Copper-61	Cu-61	1,000
Copper-64	Cu-64	1,000
Copper-67	Cu-67	1,000
Zinc-62	Zn-62	100
Zinc-63	Zn-63	1,000
Zinc-65	Zn-65	10
Zinc-69m	Zn-69m	100
Zinc-69	Zn-69	1,000
Zinc-71m	Zn-71m	1,000
Zinc-72	Zn-72	100
Gallium-65	Ga-65	1,000
Gallium-66	Ga-66	100
Gallium-67	Ga-67	1,000
Gallium-68	Ga-68	1,000
Gallium-70	Ga-70	1,000
Gallium-72	Ga-72	100
Gallium-73	Ga-73	1,000
Germanium-66	Ge-66	1,000
Germanium-67	Ge-67	1,000
Germanium-68	Ge-68	10
Germanium-69	Ge-69	1,000
Germanium-71	Ge-71	1,000

Germanium-75	Ge-75	1,000
Germanium-77	Ge-77	1,000
Germanium-78	Ge-78	1,000
Arsenic-69	As-69	1,000
Arsenic-70	As-70	1,000
Arsenic-71	As-71	100
Arsenic-72	As-72	100
Arsenic-73	As-73	100
Arsenic-74	As-74	100
Arsenic-76	As-76	100
Arsenic-77	As-77	100
Arsenic-78	As-78	1,000
Selenium-70	Se-70	1,000
Selenium-73m	Se-73m	1,000
Selenium-73	Se-73	100
Selenium-75	Se-75	100
Selenium-79	Se-79	100
Selenium-81m	Se-81m	1,000
Selenium-81	Se-81	1,000
Selenium-83	Se-83	1,000
Bromine-74m	Br-74m	1,000
Bromine-74	Br-74	1,000
Bromine-75	Br-75	1,000
Bromine-76	Br-76	100
Bromine-77	Br-77	1,000
Bromine-80m	Br-80m	1,000
Bromine-80	Br-80	1,000
Bromine-82	Br-82	100
Bromine-83	Br-83	1,000
Bromine-84	Br-84	1,000
Krypton-74	Kr-74	1,000
Krypton-76	Kr-76	1,000
Krypton-77	Kr-77	1,000
Krypton-79	Kr-79	1,000

Krypton-81	Kr-81	1,000
Krypton-83m	Kr-83m	1,000
Krypton-85m	Kr-85m	1,000
Krypton-85	Kr-85	1,000
Krypton-87	Kr-87	1,000
Krypton-88	Kr-88	1,000
Rubidium-79	Rb-79	1,000
Rubidium-81m	Rb-81m	1,000
Rubidium-81	Rb-81	1,000
Rubidium-82m	Rb-82m	1,000
Rubidium-83	Rb-83	100
Rubidium-84	Rb-84	100
Rubidium-86	Rb-86	100
Rubidium-87	Rb-87	100
Rubidium-88	Rb-88	1,000
Rubidium-89	Rb-89	1,000
Strontium-80	Sr-80	100
Strontium-81	Sr-81	1,000
Strontium-83	Sr-83	100
Strontium-85m	Sr-85m	1,000
Strontium-85	Sr-85	100
Strontium-87m	Sr-87m	1,000
Strontium-89	Sr-89	10
Strontium-90	Sr-90	0.1
Strontium-91	Sr-91	100
Strontium-92	Sr-92	100
Yttrium-86m	Y-86m	1,000
Yttrium-86	Y-86	100
Yttrium-87	Y-87	100
Yttrium-88	Y-88	10
Yttrium-90m	Y-90m	1,000
Yttrium-90	Y-90	10
Yttrium-91m	Y-91m	1,000
Yttrium-91	Y-91	10

Yttrium-92	Y-92	100
Yttrium-93	Y-93	100
Yttrium-94	Y-94	1,000
Yttrium-95	Y-95	1,000
Zirconium-86	Zr-86	100
Zirconium-88	Zr-88	10
Zirconium-89	Zr-89	100
Zirconium-93	Zr-93	1
Zirconium-95	Zr-95	10
Zirconium-97	Zr-97	100
Niobium-88	Nb-88	1,000
Niobium-89m (66 min)	Nb-89m	1,000
Niobium-89 (122 min)	Nb-89	1,000
Niobium-90	Nb-90	100
Niobium-93m	Nb-93m	10
Niobium-94	Nb-94	1
Niobium-95m	Nb-95m	100
Niobium-95	Nb-95	100
Niobium-96	Nb-96	100
Niobium-97	Nb-97	1,000
Niobium-98	Nb-98	1,000
Molybdenum-90	Mo-90	100
Molybdenum-93m	Mo-93m	100
Molybdenum-93	Mo-93	10
Molybdenum-99	Mo-99	100
Molybdenum-101	Mo-101	1,000
Technetium-93m	Tc-93m	1,000
Technetium-93	Tc-93	1,000
Technetium-94m	Tc-94m	1,000
Technetium-94	Tc-94	1,000
Technetium-96m	Tc-96	1,000
Technetium-96	Tc-96	100
Technetium-97m	Tc-97m	100
Technetium-97	Tc-97	1,000

Techneium-98	Tc-98	10
Techneium-99m	Tc-99m	1,000
Techneium-99	Tc-99	100
Techneium-101	Tc-101	1,000
Techneium-104	Tc-104	1,000
Ruthenium-94	Ru-94	1,000
Ruthenium-97	Ru-97	1,000
Ruthenium-103	Ru-103	100
Ruthenium-105	Ru-105	1,000
Ruthenium-106	Ru-106	1
Rhodium-99m	Rh-99m	1,000
Rhodium-99	Rh-99	100
Rhodium-100	Rh-100	100
Rhodium-101m	Rh-101m	1,000
Rhodium-101	Rh-101	10
Rhodium-102m	Rh-102m	10
Rhodium-102	Rh-102	10
Rhodium-103m	Rh-103m	1,000
Rhodium-105	Rh-105	100
Rhodium-106m	Rh-106m	1,000
Rhodium-107	Rh-107	1,000
Palladium-100	Pd-100	100
Palladium-101	Pd-101	1,000
Palladium-103	Pd-103	100
Palladium-107	Pd-107	10
Palladium-109	Pd-109	100
Silver-102	Ag-102	1,000
Silver-103	Ag-103	1,000
Silver-104m	Ag-104m	1,000
Silver-104	Ag-104	1,000
Silver-105	Ag-105	100
Silver-106m	Ag-106m	100
Silver-106	Ag-106	1,000
Silver-108m	Ag-108m	1

Silver-110m	Ag-110m	10
Silver-111	Ag-111	100
Silver-112	Ag-112	100
Silver-115	Ag-115	1,000
Cadmium-104	Cd-104	1,000
Cadmium-107	Cd-107	1,000
Cadmium-109	Cd-109	1
Cadmium-113m	Cd-113m	0.1
Cadmium-113	Cd-113	100
Cadmium-115m	Cd-115m	10
Cadmium-115	Cd-115	100
Cadmium-117m	Cd-117m	1,000
Cadmium-117	Cd-117	1,000
Indium-109	In-109	1,000
Indium-110 (69.1 min.)	In-110	1,000
Indium-110 (4.9h)	In-110	1,000
Indium-111	In-111	100
Indium-112	In-112	1,000
Indium-113m	In-113m	1,000
Indium-114m	In-114m	10
Indium-115m	In-115m	1,000
Indium-115	In-115	100
Indium-116m	In-116m	1,000
Indium-117m	In-117m	1,000
Indium-117	In-117	1,000
Indium-119m	In-119m	1,000
Tin-110	Sn-110	100
Tin-111	Sn-111	1,000
Tin-113	Sn-113	100
Tin-117m	Sn-117m	100
Tin-119m	Sn-119m	100
Tin-121m	Sn-121m	100
Tin-121	Sn-121	1,000
Tin-123m	Sn-123m	1,000

Tin-123	Sn-123	10
Tin-125	Sn-125	10
Tin-126	Sn-126	10
Tin-127	Sn-127	1,000
Tin-128	Sn-128	1,000
Antimony-115	Sb-115	1,000
Antimony-116m	Sb-116m	1,000
Antimony-116	Sb-116	1,000
Antimony-117	Sb-117	1,000
Antimony-118m	Sb-118m	1,000
Antimony-119	Sb-119	1,000
Antimony-120 (16 min.)	Sb-120	1,000
Antimony-120 (5.76d)	Sb-120	100
Antimony-122	Sb-122	100
Antimony-124m	Sb-124m	1,000
Antimony-124	Sb-124	10
Antimony-125	Sb-125	100
Antimony-126m	Sb-126m	1,000
Antimony-126	Sb-126	100
Antimony-127	Sb-127	100
Antimony-128 (10.4 min.)	Sb-128	1,000
Antimony-128 (9.01h)	Sb-128	100
Antimony-129	Sb-129	100
Antimony-130	Sb-130	1,000
Antimony-131	Sb-131	1,000
Tellurium-116	Te-116	1,000
Tellurium-121m	Te-121m	10
Tellurium-121	Te-121	100
Tellurium-123m	Te-123m	10
Tellurium-123	Te-123	100
Tellurium-125m	Te-125m	10
Tellurium-127m	Te-127m	10
Tellurium-127	Te-127	1,000
Tellurium-129m	Te-129m	10

Tellurium-129	Te-129	1,000
Tellurium-131m	Te-131m	10
Tellurium-131	Te-131	100
Tellurium-132	Te-132	10
Tellurium-133m	Te-133m	100
Tellurium-133	Te-133	1,000
Tellurium-134	Te-134	1,000
Iodine-120m	I-120m	1,000
Iodine-120	I-120	100
Iodine-121	I-121	1,000
Iodine-123	I-123	100
Iodine-124	I-124	10
Iodine-125	I-125	1
Iodine-126	I-126	1
Iodine-128	I-128	1,000
Iodine-129	I-129	1
Iodine-130	I-130	10
Iodine-131	I-131	1
Iodine-132m	I-132m	100
Iodine-132	I-132	100
Iodine-133	I-133	10
Iodine-134	I-134	1,000
Iodine-135	I-135	100
Xenon-120	Xe-120	1,000
Xenon-121	Xe-121	1,000
Xenon-122	Xe-122	1,000
Xenon-123	Xe-123	1,000
Xenon-125	Xe-125	1,000
Xenon-127	Xe-127	1,000
Xenon-129m	Xe-129m	1,000
Xenon-131m	Xe-131m	1,000
Xenon-133m	Xe-133m	1,000
Xenon-133	Xe-133	1,000
Xenon-135m	Xe-135m	1,000

Xenon-135	Xe-135	1,000
Xenon-138	Xe-138	1,000
Cesium-125	Cs-125	1,000
Cesium-127	Cs-127	1,000
Cesium-129	Cs-129	1,000
Cesium-130	Cs-130	1,000
Cesium-131	Cs-131	1,000
Cesium-132	Cs-132	100
Cesium-134m	Cs-134m	1,000
Cesium-134	Cs-134	10
Cesium-135m	Cs-135m	1,000
Cesium-135	Cs-135	100
Cesium-136	Cs-136	10
Cesium-137	Cs-137	10
Cesium-138	Cs-138	1,000
Barium-126	Ba-126	1,000
Barium-128	B-128	100
Barium-131m	Ba-131m	1,000
Barium-131	Ba-131	100
Barium-133m	Ba-133m	100
Barium-133	Ba-133	100
Barium-135m	Ba-135m	100
Barium-139	Ba-139	1,000
Barium-140	Ba-140	100
Barium-141	Ba-141	1,000
Barium-142	Ba-142	1,000
Lanthanum-131	La-131	1,000
Lanthanum-132	La-132	100
Lanthanum-135	La-135	1,000
Lanthanum-137	La-137	10
Lanthanum-138	La-138	100
Lanthanum-140	La-140	100
Lanthanum-141	La-141	100
Lanthanum-142	La-142	1,000

Lanthanum-143	La-143	1,000
Cerium-134	Ce-134	100
Cerium-135	Ce-135	100
Cerium-137m	Ce-137m	100
Cerium-137	Ce-137	1,000
Cerium-139	Ce-139	100
Cerium-141	Ce-141	100
Cerium-143	Ce-143	100
Cerium-144	Ce-144	1
Praseodymium-136	Pr-136	1,000
Praseodymium-137	Pr-137	1,000
Praseodymium-138m	Pr-138m	1,000
Praseodymium-139	Pr-139	1,000
Praseodymium-142m	Pr-142m	1,000
Praseodymium-142	Pr-142	100
Praseodymium-143	Pr-143	100
Praseodymium-144	Pr-144	1,000
Praseodymium-145	Pr-145	100
Praseodymium-147	Pr-147	1,000
Neodymium-136	Nd-136	1,000
Neodymium-138	Nd-138	100
Neodymium-139m	Nd-139m	1,000
Neodymium-139	Nd-139	1,000
Neodymium-141	Nd-141	1,000
Neodymium-147	Nd-147	100
Neodymium-149	Nd-149	1,000
Neodymium-151	Nd-151	1,000
Promethium-141	Pm-141	1,000
Promethium-143	Pm-143	100
Promethium-144	Pm-144	10
Promethium-145	Pm-145	10
Promethium-146	Pm-146	1
Promethium-147	Pm-147	10
Promethium-148m	Pm-148m	10

Promethium-148	Pm-148	10
Promethium-149	Pm-149	100
Promethium-150	Pm-150	1,000
Promethium-151	Pm-151	100
Samarium-141m	Sm-141m	1,000
Samarium-141	Sm-141	1,000
Samarium-142	Sm-142	1,000
Samarium-145	Sm-145	100
Samarium-146	Sm-146	1
Samarium-147	Sm-147	100
Samarium-151	Sm-151	10
Samarium-153	Sm-153	100
Samarium-155	Sm-155	1,000
Samarium-156	Sm-156	1,000
Europium-145	Eu-145	100
Europium-146	Eu-146	100
Europium-147	Eu-147	100
Europium-148	Eu-148	10
Europium-149	Eu-149	100
Europium-150 (12.62h)	Eu-150	100
Europium-150 (34.2y)	Eu-150	1
Europium-152m	Eu-152m	100
Europium-152	Eu-152	1
Europium-154	Eu-154	1
Europium-155	Eu-155	10
Europium-156	Eu-156	100
Europium-157	Eu-157	100
Europium-158	Eu-158	1,000
Gadolinium-145	Gd-145	1,000
Gadolinium-146	Gd-146	10
Gadolinium-147	Gd-147	100
Gadolinium-148	Gd-148	0.001
Gadolinium-149	Gd-149	100
Gadolinium-151	Gd-151	10

Gadolinium-152	Gd-152	100
Gadolinium-153	Gd-153	10
Gadolinium-159	Gd-159	100
Terbium-147	Tb-147	1,000
Terbium-149	Tb-149	100
Terbium-150	Tb-150	1,000
Terbium-151	Tb-151	100
Terbium-153	Tb-153	1,000
Terbium-154	Tb-154	100
Terbium-155	Tb-155	1,000
Terbium-156m (5.0h)	Tb-156m	1,000
Terbium-156m (24.4h)	Tb-156m	1,000
Terbium-156	Tb-156	100
Terbium-157	Tb-157	10
Terbium-158	Tb-158	1
Terbium-160	Tb-160	10
Terbium-161	Tb-161	100
Dysprosium-155	Dy-155	1,000
Dysprosium-157	Dy-157	1,000
Dysprosium-159	Dy-159	100
Dysprosium-165	Dy-165	1,000
Dysprosium-166	Dy-166	100
Holmium-155	Ho-155	1,000
Holmium-157	Ho-157	1,000
Holmium-159	Ho-159	1,000
Holmium-161	Ho-161	1,000
Holmium-162m	Ho-162m	1,000
Holmium-162	Ho-162	1,000
Holmium-164m	Ho-164m	1,000
Holmium-164	Ho-164	1,000
Holmium-166m	Ho-166m	1
Holmium-166	Ho-166	100
Holmium-167	Ho-167	1,000
Erbium-161	Er-161	1,000

Erbium-165	Er-165	1,000
Erbium-169	Er-169	100
Erbium-171	Er-171	100
Erbium-172	Er-172	100
Thulium-162	Tm-162	1,000
Thulium-166	Tm-166	100
Thulium-167	Tm-167	100
Thulium-170	Tm-170	10
Thulium-171	Tm-171	10
Thulium-172	Tm-172	100
Thulium-173	Tm-173	100
Thulium-175	Tm-175	1,000
Ytterbium-162	Yb-162	1,000
Ytterbium-166	Yb-166	100
Ytterbium-167	Yb-167	1,000
Ytterbium-169	Yb-169	100
Ytterbium-175	Yb-175	100
Ytterbium-177	Yb-177	1,000
Ytterbium-178	Yb-178	1,000
Lutetium-169	Lu-169	100
Lutetium-170	Lu-170	100
Lutetium-171	Lu-171	100
Lutetium-172	Lu-172	100
Lutetium-173	Lu-173	10
Lutetium-174m	Lu-174m	10
Lutetium-174	Lu-174	10
Lutetium-176m	Lu-176m	1,000
Lutetium-176	Lu-176	100
Lutetium-177m	Lu-177m	10
Lutetium-177	Lu-177	100
Lutetium-178m	Lu-178m	1,000
Lutetium-178	Lu-178	1,000
Lutetium-179	Lu-179	1,000
Hafnium-170	Hf-170	100

Hafnium-172	Hf-172	1
Hafnium-173	Hf-173	1,000
Hafnium-175	Hf-175	100
Hafnium-177m	Hf-177m	1,000
Hafnium-178m	Hf-178m	0.1
Hafnium-179m	Hf-179m	10
Hafnium-180m	Hf-180m	1,000
Hafnium-181	Hf-181	10
Hafnium-182m	Hf-182m	1,000
Hafnium-182	Hf-182	0.1
Hafnium-183	Hf-183	1,000
Hafnium-184	Hf-184	100
Tantalum-172	Ta-172	1,000
Tantalum-173	Ta-173	1,000
Tantalum-174	Ta-174	1,000
Tantalum-175	Ta-175	1,000
Tantalum-176	Ta-176	100
Tantalum-177	Ta-177	1,000
Tantalum-178	Ta-178	1,000
Tantalum-179	Ta-179	100
Tantalum-180m	Ta-180m	1,000
Tantalum-180	Ta-180	100
Tantalum-182m	Ta-182m	1,000
Tantalum-182	Ta-182	10
Tantalum-183	Ta-183	100
Tantalum-184	Ta-184	100
Tantalum-185	Ta-185	1,000
Tantalum-186	Ta-186	1,000
Tungsten-176	W-176	1,000
Tungsten-177	W-177	1,000
Tungsten-178	W-178	1,000
Tungsten-179	W-179	1,000
Tungsten-181	W-181	1,000
Tungsten-185	W-185	100

Tungsten-187	W-187	100
Tungsten-188	W-188	10
Rhenium-177	Re-177	1,000
Rhenium-178	Re-178	1,000
Rhenium-181	Re-181	1,000
Rhenium-182 (12.7h)	Re-182	1,000
Rhenium-182 (64.0h)	Re-182	100
Rhenium-184m	Re-184m	10
Rhenium-184	Re-184	100
Rhenium-186m	Re-186m	10
Rhenium-186	Re-186	100
Rhenium-187	Re-187	1,000
Rhenium-188m	Re-188m	1,000
Rhenium-188	Re-188	100
Rhenium-189	Re-189	100
Osmium-180	Os-180	1,000
Osmium-181	Os-181	1,000
Osmium-182	Os-182	100
Osmium-185	Os-185	100
Osmium-189m	Os-189m	1,000
Osmium-191m	Os-191m	1,000
Osmium-191	Os-191	100
Osmium-193	Os-193	100
Osmium-194	Os-194	1
Iridium-182	Ir-182	1,000
Iridium-184	Ir-184	1,000
Iridium-185	Ir-185	1,000
Iridium-186	Ir-186	100
Iridium-187	Ir-187	1,000
Iridium-188	Ir-188	100
Iridium-189	Ir-189	100
Iridium-190m	Ir-190m	1,000
Iridium-190	Ir-190	100
Iridium-192 (73.8d)	Ir-192	1

Iridium-192m (1.4 min.)	Ir-192m	10
Iridium-194m	Ir-194m	10
Iridium-194	Ir-194	100
Iridium-195m	Ir-195m	1,000
Iridium-195	Ir-95	1,000
Platinum-186	Pt-186	1,000
Platinum-188	Pt-188	100
Platinum-189	Pt-189	1,000
Platinum-191	Pt-191	100
Platinum-193m	Pt-193m	100
Platinum-193	Pt-193	1,000
Platinum-195m	Pt-195m	100
Platinum-197m	Pt-197m	1,000
Platinum-197	Pt-197	100
Platinum-199	Pt-199	1,000
Platinum-200	Pt-200	100
Gold-193	Au-193	1,000
Gold-194	Au-194	100
Gold-195	Au-195	10
Gold-198m	Au-198m	100
Gold-198	Au-198	100
Gold-199	Au-199	100
Gold-200m	Au-200m	100
Gold-200	Au-200	1,000
Gold-201	Au-201	1,000
Mercury-193m	Hg-193m	100
Mercury-193	Hg-193	1,000
Mercury-194	Hg-194	1
Mercury-195m	Hg-195m	100
Mercury-195	Hg-195	1,000
Mercury-197m	Hg-197m	100
Mercury-197	Hg-197	1,000
Mercury-199m	Hg-199m	1,000
Mercury-203	Hg-203	100

Thallium-194m	TI-194m	1,000
Thallium-194	TI-194	1,000
Thallium-195	TI-195	1,000
Thallium-197	TI-197	1,000
Thallium-198m	TI-198m	1,000
Thallium-198	TI-198	1,000
Thallium-199	TI-199	1,000
Thallium-200	TI-200	1,000
Thallium-201	TI-201	1,000
Thallium-202	TI-202	100
Thallium-204	TI-204	100
Lead-195m	Pb-195m	1,000
Lead-198	Pb-198	1,000
Lead-199	Pb-199	1,000
Lead-200	Pb-200	100
Lead-201	Pb-201	1,000
Lead-202m	Pb-202m	1,000
Lead-202	Pb-202	10
Lead-203	Pb-203	1,000
Lead-205	Pb-205	100
Lead-209	Pb-209	1,000
Lead-210	Pb-210	0.01
Lead-211	Pb-211	100
Lead-212	Pb-212	1
Lead-214	Pb-214	100
Bismuth-200	Bi-200	1,000
Bismuth-201	Bi-201	1,000
Bismuth-202	Bi-202	1,000
Bismuth-203	Bi-203	100
Bismuth-205	Bi-205	100
Bismuth-206	Bi-206	100
Bismuth-207	Bi-207	10
Bismuth-210m	Bi-210m	0.1
Bismuth-210	Bi-210	1

Bismuth-212	Bi-212	10
Bismuth-213	Bi-213	10
Bismuth-214	Bi-214	100
Polonium-203	Po-203	1,000
Polonium-205	Po-205	1,000
Polonium-207	Po-207	1,000
Polonium-210	Po-210	0.1
Astatine-207	At-207	100
Astatine-211	At-211	10
Radon-220	Rn-220	1
Radon-222	Rn-222	1
Francium-222	Fr-222	100
Francium-223	Fr-223	100
Radium-223	Ra-223	0.1
Radium-224	Ra-224	0.1
Radium-225	Ra-225	0.1
Radium-226	Ra-226	0.1
Radium-227	Ra-227	1,000
Radium-228	Ra-228	0.1
Actinium-224	Ac-224	1
Actinium-225	Ac-225	0.01
Actinium-226	Ac-226	0.1
Actinium-227	Ac-227	0.001
Actinium-228	Ac-228	1
Thorium-226	Th-226	10
Thorium-227	Th-227	0.01
Thorium-228	Th-228	0.001
Thorium-229	Th-229	0.001
Thorium-230	Th-230	0.001
Thorium-231	Th-231	100
Thorium-232	Th-232	100
Thorium-234	Th-234	10
Thorium-natural		100
Protactinium-227	Pa-227	10

Protactinium-228	Pa-228	1
Protactinium-230	Pa-230	0.1
Protactinium-231	Pa-231	0.001
Protactinium-232	Pa-232	1
Protactinium-233	Pa-233	100
Protactinium-234	Pa-234	100
Uranium-230	U-230	0.01
Uranium-231	U-231	100
Uranium-232	U-232	0.001
Uranium-233	U-233	0.001
Uranium-234	U-234	0.001
Uranium-235	U-235	0.001
Uranium-236	U-236	0.001
Uranium-237	U-237	100
Uranium-238	U-238	100
Uranium-239	U-239	1,000
Uranium-240	U-240	100
Uranium-natural		100
Neptunium-232	Np-232	100
Neptunium-233	Np-233	1,000
Neptunium-234	Np-234	100
Neptunium-235	Np-235	100
Neptunium-236 (1.15x10 ⁵ y)	Np-236	0.001
Neptunium-236 (22.5h)	Np-236	1
Neptunium-237	Np-237	0.001
Neptunium-238	Np-238	10
Neptunium-239	Np-239	100
Neptunium-240	Np-240	1,000
Plutonium-234	Pu-234	10
Plutonium-235	Pu-235	1,000
Plutonium-236	Pu-236	0.001
Plutonium-237	Pu-237	100
Plutonium-238	Pu-238	0.001
Plutonium-239	Pu-239	0.001

Plutonium-240	Pu-240	0.001
Plutonium-241	Pu-241	0.01
Plutonium-242	Pu-242	0.001
Plutonium-243	Pu-243	1,000
Plutonium-244	Pu-244	0.001
Plutonium-245	Pu-245	100
Americium-237	Am-237	1,000
Americium-238	Am-238	100
Americium-239	Am-239	1,000
Americium-240	Am-240	100
Americium-241	Am-241	0.001
Americium-242m	Am-242m	0.001
Americium-242	Am-242	10
Americium-243	Am-243	0.001
Americium-244m	Am-244m	100
Americium-244	Am-244	10
Americium-245	Am-245	1,000
Americium-246m	Am-246m	1,000
Americium-246	Am-246	1,000
Curium-238	Cm-238	100
Curium-240	Cm-240	0.1
Curium-241	Cm-241	1
Curium-242	Cm-242	0.01
Curium-243	Cm-243	0.001
Curium-244	Cm-244	0.001
Curium-245	Cm-245	0.001
Curium-246	Cm-246	0.001
Curium-247	Cm-247	0.001
Curium-248	Cm-248	0.001
Curium-249	Cm-249	1,000
Berkelium-245	Bk-245	100
Berkelium-246	Bk-246	100
Berkelium-247	Bk-247	0.001
Berkelium-249	Bk-249	0.1

Berkelium-250	Bk-250	10
Californium-244	Cf-244	100
Californium-246	Cf-246	1
Californium-248	Cf-248	0.01
Californium-249	Cf-249	0.001
Californium-250	Cf-250	0.001
Californium-251	Cf-251	0.001
Californium-252	Cf-252	0.001
Californium-253	Cf-253	0.1
Californium-254	Cf-254	0.001
Einsteinium-250	Es-250	100
Einsteinium-251	Es-251	100
Einsteinium-253	Es-253	0.1
Einsteinium-254m	Es-254m	1
Einsteinium-254	Es-254	0.01
Fermium-252	Fm-252	1
Fermium-253	Fm-253	1
Fermium-254	Fm-254	10
Fermium-255	Fm-255	1
Fermium-257	Fm-257	0.01
Mendelevium-257	Md-257	10
Mendelevium-258	Md-258	0.01

Any radionuclide other than alpha emitter radionuclides not listed above, or mixtures of beta emitters of unknown composition 0.01

Any alpha-emitting radionuclide not listed above or mixtures of alpha-emitters of unknown composition 0.001

¹The quantities listed above were derived by taking 1/10 of the most restrictive ALI listed in table 1, columns 1 and 2 of 10 CFR Part 20, Appendix B, rounding to the nearest factor of 10, and arbitrarily constraining the values listed between 0.001 and 1,000 μ Ci. Values of 100 μ Ci have been assigned for radionuclides having a radioactive half-life in excess of 10^9 years (except rhenium, 1000 μ Ci) to take into account their low specific activity.

NOTE: For purposes of 10 CFR 20.1902(e), 10 CFR 20.1905(a), and 10 CFR

20.2201(a) where there is involved a combination of radionuclides in known amounts, the limit for the combination should be derived as follows: determine, for each radionuclide in the combination, the ratio between the quantity present in the combination and the limit otherwise established for the specific radionuclide when not in combination. The sum of such ratios for all radionuclides in the combination may not exceed "1" (i.e., "unity").

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3710. Requirements for transfers of low-level radioactive waste intended for disposal at licensed land disposal facilities and manifests.

A. Manifest.

1. A waste generator, waste collector, or waste processor that transports, or offers for transportation, low-level radioactive waste intended for ultimate disposal at a licensed low-level radioactive waste land disposal facility must prepare a manifest reflecting information requested on applicable NRC Forms 540 (Uniform Low-Level Radioactive Waste Manifest (Shipping Paper)) and 541 (Uniform Low-Level Radioactive Waste Manifest (Container and Waste Description)) and, if necessary, on an applicable NRC Form 542 (Uniform Low-Level Radioactive Waste Manifest (Manifest Index and Regional Compact Tabulation)). NRC Forms 540 and 540A must be completed and must physically accompany the pertinent low-level waste shipment.

2. Upon agreement between shipper and consignee, NRC Forms 541, 541A, 542, and 542A may be completed, transmitted, and stored in electronic media with the capability for producing legible, accurate, and complete records on the respective forms.

3. Licensees are not required by the agency, the NRC, or another agreement

state to comply with the manifesting requirements of this subpart when they ship:

- a. Low-level radioactive waste for processing and expect its return, such as for storage under their license, prior to disposal at a licensed land disposal facility;
- b. Low-level radioactive waste that is being returned to the licensee that is the waste generator or generator; or
- c. Radioactively contaminated material to a waste processor that becomes the processor's residual waste.

4. For guidance in completing the forms required under subdivision 1 of this subsection, refer to the instructions that accompany the forms. Copies of manifests required by this subpart may be legible carbon copies, photocopies, or computer printouts that reproduce the data in the format of the uniform manifest.

5. NRC Forms 540, 540A, 541, 541A, 542, and 542A, and the accompanying instructions, in hard copy, may be obtained from the Information and Records Management Branch, Office of Information Resources Management, U.S. Nuclear Regulatory Commission, Washington, DC 20555-0001, telephone (800) 368-5642. The forms are available online at <http://www.nrc.gov/reading-rm/doc-collections/forms>.

6. This section includes information requirements of the DOT, as codified in 49 CFR Part 172. Information on hazardous, medical, or other waste, required to meet Environmental Protection Agency (EPA) regulations, as codified in 40 CFR Part 259, 261 or elsewhere, is not addressed in this section and must be provided on the required EPA forms. However, the required EPA forms must accompany the uniform low-level radioactive waste manifest required by this section.

B. General information. The shipper of the radioactive waste must provide the following information on the uniform manifest:

1. The name, facility address, and telephone number of the licensee shipping the waste;

2. An explicit declaration indicating whether the shipper is acting as a waste generator, waste collector, waste processor, or a combination of these identifiers for purposes of the manifested shipment; and

3. The name, address, and telephone number, or the name and EPA identification number for the carrier transporting the waste.

C. Shipment information. The shipper of the radioactive waste must provide the following information regarding the waste shipment on the uniform manifest:

1. The date of the waste shipment;

2. The total number of packages or disposal containers;

3. The total disposal volume and disposal weight in the shipment;

4. The total radionuclide activity in the shipment;

5. The activity of each of the radionuclides H-3, C-14, Tc-99, and I-129 contained in the shipment; and

6. The total masses of U-233, U-235, and plutonium in special nuclear material and the total mass of uranium and thorium in source material.

D. Disposal container and waste information. The shipper of the radioactive waste must provide the following information on the uniform manifest regarding the waste and each disposal container of waste in the shipment:

1. An alphabetic or numeric identification that uniquely identifies each disposal container in the shipment;

2. A physical description of the disposal container, including the manufacturer and model of any high integrity container;

3. The volume displaced by the disposal container;

4. The gross weight of the disposal container, including the waste;

5. For waste consigned to a disposal facility, the maximum radiation level at the surface of each disposal container;

6. A physical and chemical description of the waste;

7. The total weight percentage of chelating agent for any waste containing more than 0.1% chelating agent by weight, plus the identity of the principal chelating agent;

8. The approximate volume of waste within a container;

9. The sorbing or solidification media, if any, and the identity of the solidification media vendor and brand name;

10. The identities and activities of individual radionuclides contained in each container, the masses of U-233, U-235, and plutonium in special nuclear material, and the masses of uranium and thorium in source material. For discrete waste types, such as activated materials, contaminated equipment, mechanical filters, sealed source or devices, and wastes in solidification or stabilization media, the identities and activities of individual radionuclides associated with or contained on these waste types within a disposal container must be reported; and

11. The total radioactivity within each container.

E. Uncontainerized waste information. The shipper of the radioactive waste must provide the following information on the uniform manifest regarding a waste shipment delivered without a disposal container:

1. The approximate volume and weight of the waste;

2. A physical and chemical description of the waste;

3. The total weight percentage of chelating agent if the chelating agent exceeds 0.1% by weight, plus the identity of the principal chelating agent;

4. For waste consigned to a disposal facility, the classification of the waste according to 12VAC5-481-2571. Waste not meeting the structural stability requirements of 12VAC5-481-2572 must be identified;

5. The identities and activities of individual radionuclides contained in the waste, the masses of U-233, U-235, and plutonium in special nuclear material, and the masses of uranium and thorium in source material; and

6. For wastes consigned to a disposal facility, the maximum radiation levels at the surface of the waste.

F. Multigenerator disposal container information.

1. This subsection applies to disposal containers enclosing mixtures of waste originating from different generators. The origin of the low-level radioactive waste resulting from a waste processor's activities may be attributable to one or more generators, including waste generators. This subsection also applies to mixtures of wastes shipped in an uncontainerized form, for which portions of the mixture within the shipment originate from different generators.

2. For homogeneous mixtures of waste, such as incinerator ash, the shipper must provide the waste description applicable to the mixture and the volume of the waste attributed to each generator.

3. For heterogeneous mixtures of waste, such as the combined products from a large compactor, the shipper must identify each generator contributing waste to the disposal container and for discrete waste types, such as activated materials, contaminated equipment, mechanical filters, sealed source or devices, and wastes in solidification or stabilization media, the identities and activities of individual radionuclides contained on these waste types within the disposal container. For each generator, the shipper must provide the following:

- a. The volume of waste within the disposal container;
- b. A physical and chemical description of the waste, including the solidification agent, if any;
- c. The total weight percentage of chelating agents for any disposal container containing more than 0.1 percent chelating agent by weight, plus the identity of the principal chelating agent;
- d. The sorbing or solidification media, if any, and the identity of the solidification media vendor and brand name if the media is claimed to meet stability requirements in 12VAC5-481-2572; and

e. Radionuclide identities and activities contained in the waste, the masses of U-233, U-235, and plutonium in special nuclear material, and the masses of uranium and thorium in source material, if contained in the waste.

G. Certification. An authorized representative of the waste generator, waste processor, or waste collector must certify by signing and dating the shipment manifest that the transported materials are properly classified, described, packaged, marked, and labeled and are in proper condition for transportation according to the applicable regulations of the DOT and the agency, NRC or another agreement state. A waste collector, in signing the certification, is certifying that nothing has been done to the collected waste that would invalidate the waste generator's certification.

H. Control and tracking; transfers. A licensee that transfers radioactive waste to a land disposal facility or a licensed waste collector must comply with subdivisions 1 through 9 of this subsection. A licensee that transfers waste to a licensed waste processor for waste treatment or repackaging must comply with subdivisions 4 through 9 of this subsection. A licensee shall:

1. Prepare all wastes so that the waste is classified according to 12VAC5-481-2571, and meets the waste characteristics requirements in 12VAC5-481-2572;
2. Label each disposal container of waste, or transport package if potential radiation hazards preclude labeling of the individual disposal container, to identify whether it is Class A waste, Class B waste, Class C waste, or greater than Class C waste, according to 12VAC5-481-2571;
3. Conduct a quality assurance program to ensure compliance with 12VAC5-481-2571 and 12VAC5-481-2572. The program must include management evaluation of audits;
4. Prepare the uniform low-level radioactive waste manifest as required by this part;
5. Forward a copy or electronically transfer the uniform low-level radioactive waste manifest to the intended consignee so that receipt of the manifest precedes the low-level radioactive waste shipment or the manifest is delivered to

the consignee with the waste at the time the waste is transferred to the consignee, or both;

6. Include NRC Form 540, and Form 540A if required, with the shipment regardless of the option chosen in subdivision 5 of this subsection;

7. Receive acknowledgment of the receipt of the shipment in the form of a signed copy of NRC Form 540;

8. Retain a copy of or electronically store the uniform low-level radioactive waste manifest and documentation of acknowledgment of receipt as the record of transfer of licensed material as required by Part I (12VAC5-481-10 et seq.), Part III (12VAC5-481-380 et seq.), Part IV (12VAC5-481-600 et seq.) and Part X (12VAC5-481-2250 et seq.); and

9. For any shipment or any part of a shipment for which acknowledgment of receipt has not been received within the times set forth in this part, conduct an investigation according to subsection L of this section.

I. Control and tracking; prepackaged waste. A waste collector licensee that handles only prepackaged waste must:

1. Acknowledge receipt of the waste from the shipper within one week of receipt by returning a signed copy of NRC Form 540;

2. Prepare a new manifest to reflect consolidated shipments that meet the requirements of this section. The waste collector must ensure that, for each container of waste in the shipment, the manifest identifies the generator of that container of waste;

3. Forward a copy or electronically transfer the uniform low-level radioactive waste manifest to the intended consignee so that receipt of the manifest precedes the low-level radioactive waste shipment or the manifest is delivered to the consignee with the waste at the time the waste is transferred to the consignee, or both;

4. Include NRC Form 540, and 540A if required, with the shipment regardless of

the option chosen in subdivision 4 of this subsection;

5. Receive acknowledgment of the receipt of the shipment in the form of a signed copy of NRC Form 540;

6. Retain a copy of or electronically store the uniform low-level radioactive waste manifest and documentation of acknowledgment of receipt as the record of transfer of licensed material as required under Part I (12VAC5-481-10 et seq.), Part III (12VAC5-481-380 et seq.), Part IV (12VAC5-481-600 et seq.) and Part X (12VAC5-481-2250 et seq.);

7. For any shipment or any part of a shipment for which acknowledgment of receipt has not been received within the times set forth in this section, conduct an investigation according to subsection L of this section; and

8. Notify the shipper and the agency when any shipment, or part of a shipment, has not arrived within 60 days after receipt of an advance manifest, unless notified by the shipper that the shipment has been canceled.

J. Control and tracking; treatment or repackaging. A licensed waste processor that treats or repackages waste must:

1. Acknowledge receipt of the waste from the shipper within one week of receipt by returning a signed copy of NRC Form 540;

2. Prepare a new manifest that meets the requirements of this section. Preparation of the new manifest reflects that the waste processor is responsible for meeting these requirements. For each container of waste in the shipment, the manifest must identify the waste generators, the preprocessed waste volume, and the other information as required under subsection F of this section;

3. Prepare all wastes so that the waste is classified according to 12VAC5-481-2571, and meets the waste characteristics requirements in 12VAC5-481-2572;

4. Label each package of waste to identify whether it is Class A waste, Class B waste, or Class C waste, in accordance with 12VAC5-481-2571 and 12VAC5-481-2572;

5. Conduct a quality assurance program to ensure compliance with 12VAC5-481-2571 and 12VAC5-481-2572. The program must include management evaluation of audits;
 6. Forward a copy or electronically transfer the uniform low-level radioactive waste manifest to the intended consignee so that receipt of the manifest precedes the low-level radioactive waste shipment or the manifest is delivered to the consignee with the waste at the time the waste is transferred to the consignee, or both;
 7. Include NRC Form 540, and Form 540A if required, with the shipment regardless of the option chosen in subdivision 6 of this subsection;
 8. Receive acknowledgment of the receipt of the shipment in the form of a signed copy of NRC Form 540;
 9. Retain a copy of or electronically store the uniform low-level radioactive waste manifest and documentation of acknowledgment of receipt as the record of transfer of licensed material as required by Part I (12VAC5-481-10 et seq.), Part III (12VAC5-481-380 et seq.), Part IV (12VAC5-481-600 et seq.) and Part X (12VAC5-481-2250 et seq.);
 10. For any shipment or any part of a shipment for which acknowledgment of receipt has not been received within the times set forth in this part, conduct an investigation according to subsection L; and
 11. Notify the shipper and the agency when any shipment, or part of a shipment, has not arrived within 60 days after receipt of an advance manifest, unless notified by the shipper that the shipment has been canceled.
- K. Control and tracking; land disposal facility. A land disposal facility operator shall:
1. Acknowledge receipt of the waste within one week of receipt by returning, as a minimum, a signed copy of NRC Form 540 to the shipper. The shipper to be notified is the licensee that last possessed the waste and transferred the waste to the operator. If any discrepancy exists between materials listed on the uniform

low-level radioactive waste manifest and materials received, copies or electronic transfer of the affected forms must be returned indicating the discrepancy;

2. Maintain copies of all completed manifests and electronically store the information required by 12VAC5-481-2630, until the agency terminates the license; and

3. Notify the shipper and the agency when any shipment, or part of a shipment, has not arrived within 60 days after receipt of an advance manifest, unless notified by the shipper that the shipment has been canceled.

L. Investigation. A shipment or part of a shipment for which acknowledgment is not received within the times set forth in this part must:

1. Be investigated by the shipper if the shipper has not received notification or receipt within 20 days after transfer; and

2. Be traced and reported. The investigation must include tracing the shipment and filing a report with the agency. A licensee that conducts a trace investigation must file a written report with the agency within two weeks of completing the investigation.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3720. Exempt concentrations schedule.

Element (atomic number)	Isotope	Col. I	Col. II
		Gas Concentration $\mu\text{Ci}/\text{ml}^1$	Liquid and Solid Concentration $\mu\text{Ci}/\text{ml}^2$
Antimony (51)	Sb-122		3×10^{-4}
	Sb-124		2×10^{-4}
	Sb-125		1×10^{-3}
Argon (18)	A-37	1×10^{-3}	
	A-41	4×10^{-7}	

Arsenic (33)	As-73		5×10^{-3}
	As-74		5×10^{-4}
	As-76		2×10^{-4}
	As-77		8×10^{-4}
Barium (56)	Ba-131		2×10^{-3}
	Ba-140		3×10^{-4}
Beryllium (4)	Be-7		2×10^{-2}
Bismuth (83)	Bi-206		4×10^{-4}
Bromine (35)	Br-82	4×10^{-7}	3×10^{-3}
Cadmium (48)	Cd-109		2×10^{-3}
	Cd-115M		3×10^{-4}
	Cd-115		3×10^{-4}
Calcium (20)	Ca-45		9×10^{-5}
	Ca-47		5×10^{-4}
Carbon (6)	C-14	1×10^{-6}	8×10^{-3}
Cerium (58)	Ce-141		9×10^{-4}
	Ce-143		4×10^{-4}
	Ce-144		1×10^{-4}
Cesium (55)	Cs-131		2×10^{-2}
	Cs-134m		6×10^{-2}
	Cs-134		9×10^{-5}
Chlorine (17)	Cl-38	9×10^{-7}	4×10^{-3}
Chromium (24)	Cr-51		2×10^{-2}
Cobalt (27)	Co-57		5×10^{-3}
	Co-58		1×10^{-3}
	Co-60		5×10^{-4}
Copper (29)	Cu-64		3×10^{-3}
Dysprosium (66)	Dy-165		4×10^{-3}
	Dy-166		4×10^{-4}
Erbium (68)	Er-169		9×10^{-4}

	Er-171		1×10^{-3}
Europium (63)	Eu-152 (9.2 hrs)		6×10^{-4}
	Eu-155		2×10^{-3}
Fluorine (9)	F-18	2×10^{-6}	8×10^{-3}
Gadolinium (64)	Gd-153		2×10^{-3}
	Gd-159		8×10^{-4}
Gallium (31)	Ga-72		4×10^{-4}
Germanium (32)	Ge-71		2×10^{-2}
Gold (79)	Au-196		2×10^{-3}
	Au-198		5×10^{-4}
	Au-199		2×10^{-3}
Hafnium (72)	Hf-81		7×10^{-4}
Hydrogen (1)	H-3	5×10^{-6}	3×10^{-2}
Indium (49)	In-113M		1×10^{-2}
	In-114M		2×10^{-4}
Iodine (53)	I-126	3×10^{-9}	2×10^{-5}
	I-131	3×10^{-9}	2×10^{-5}
	I-132	8×10^{-8}	6×10^{-4}
	I-133	1×10^{-8}	7×10^{-5}
	I-134	2×10^{-7}	1×10^{-3}
Iridium (77)	Ir-190		2×10^{-3}
	Ir-192		4×10^{-4}
	Ir-194		3×10^{-4}
Iron (26)	Fe-55		8×10^{-3}
	Fe-59		6×10^{-4}
Krypton (36)	Kr-85M	1×10^{-6}	
	Kr-85	3×10^{-6}	
Lanthanum (57)	La-140		2×10^{-4}
Lead (82)	Pb-203		4×10^{-3}

Lutetium (71)	Lu-177	1×10^{-3}
Manganese (25)	Mn-52	3×10^{-4}
	Mn-54	1×10^{-3}
	Mn-56	1×10^{-3}
Mercury (80)	Hg-197M	2×10^{-3}
	Hg-197	3×10^{-3}
	Hg-203	2×10^{-4}
Molybdenum (42)	Mo-99	2×10^{-3}
Neodymium (60)	Nd-147	6×10^{-4}
	Nd-149	3×10^{-3}
Nickel (28)	Ni-65	1×10^{-3}
Niobium (Columbium) (41)	Nb-95	1×10^{-3}
	Nb-97	9×10^{-3}
Osmium (76)	Os-185	7×10^{-4}
	Os-191M	3×10^{-2}
	Os-191	2×10^{-3}
	Os-193	6×10^{-4}
Palladium (46)	Pd-103	3×10^{-3}
	Pd-109	9×10^{-4}
Phosphorus (15)	P-32	2×10^{-4}
Platinum (78)	Pt-191	1×10^{-3}
	Pt-193M	1×10^{-2}
	Pt-197M	1×10^{-2}
	Pt-197	1×10^{-3}
Potassium (19)	K-42	3×10^{-3}
Praseodymium (59)	Pr-142	3×10^{-4}
	Pr-143	5×10^{-4}
Promethium (61)	Pm-147	2×10^{-3}
	Pm-149	4×10^{-4}
Rhenium (75)	Re-183	6×10^{-3}

	Re-186		9×10^{-4}
	Re-188		6×10^{-4}
Rhodium (45)	Rh-103M		1×10^{-1}
	Rh-105		1×10^{-3}
Rubidium (37)	Rb-86		7×10^{-4}
Ruthenium (44)	Ru-97		4×10^{-4}
	Ru-103		8×10^{-4}
	Ru-105		1×10^{-3}
	Ru-106		1×10^{-4}
Samarium (62)	Sm-153		8×10^{-4}
Scandium (21)	Sc-46		4×10^{-4}
	Sc-47		9×10^{-4}
	Sc-48		3×10^{-4}
Selenium (34)	Se-75		3×10^{-3}
Silicon (14)	Si-31		9×10^{-3}
Silver (47)	Ag-105		1×10^{-3}
	Ag-110M		3×10^{-4}
	Ag-111		4×10^{-4}
Sodium (11)	Na-24		2×10^{-3}
Strontium (38)	Sr-85		1×10^{-4}
	Sr-89		1×10^{-4}
	Sr-91		7×10^{-4}
	Sr-92		7×10^{-4}
Sulfur (16)	S-35	9×10^{-8}	6×10^{-4}
Tantalum (73)	Ta-182		4×10^{-4}
Technetium (43)	Tc-96M		1×10^{-1}
	Tc-96		1×10^{-3}
Tellurium (52)	Te-125M		2×10^{-3}
	Te-125M		6×10^{-4}
	Te-127		3×10^{-3}

	Te-129M		3×10^{-4}
	Te-131M		6×10^{-4}
	Te-132		3×10^{-4}
Terbium (65)	Tb-160		4×10^{-4}
Thallium (81)	Tl-200		4×10^{-3}
	Tl-201		3×10^{-3}
	Tl-202		1×10^{-3}
	Tl-204		1×10^{-3}
Thulium (69)	Tm-170		5×10^{-4}
	Tm-171		5×10^{-3}
Tin (50)	Sn-113		9×10^{-4}
	Sn-125		2×10^{-4}
Tungsten (Wolfram) (74)	W-181		4×10^{-3}
	W-187		7×10^{-4}
Vanadium (23)	V-48		3×10^{-4}
Xenon (54)	Xe-131M	4×10^{-6}	
	Xe-133	3×10^{-6}	
	Xe-135	1×10^{-6}	
Ytterbium (70)	Yb-175		1×10^{-3}
Yttrium (39)	Y-90		2×10^{-4}
	Y-91M		3×10^{-2}
	Y-91		3×10^{-4}
	Y-92		6×10^{-4}
	Y-93		3×10^{-4}
Zinc (30)	Zn-65		1×10^{-3}
	Zn-69M		7×10^{-4}
	Zn-69		2×10^{-2}
Zirconium (40)	Zr-95		6×10^{-4}
	Zr-97		2×10^{-4}
Beta and/or gamma emitting radioactive material not listed above with half-life less		1×10^{-10}	1×10^{-6}

than three years

Footnotes:

¹Values are given only for those materials normally used as gases.

²μCi/gm for solids.

NOTE 1: Many radioisotopes disintegrate into isotopes that are also radioactive. In expressing the concentrations, the activity stated is that of the parent isotope and takes into account the daughters.

NOTE 2: For purposes of 12VAC5-481-400 A where there is involved a combination of isotopes, the limit for the combination should be derived as follows:

Determine for each isotope in the product the ratio between the concentration present in the product and the exempt concentration for the specific isotope when not in combination. The sum of such ratios may not exceed "1" (i.e., unity).

Example:

Equation showing the relationship described in Note 2 for two example isotopes

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3730. Exempt quantities.

Radioactive material	Microcuries
Antimony 122 (Sb 122)	100
Antimony 124 (Sb 124)	10
Antimony 125 (Sb 125)	10
Arsenic 73 (As 73)	100
Arsenic 74 (As 74)	10
Arsenic 76 (As 76)	10
Arsenic 77 (as 77)	100
Barium 131 (Ba 131)	10
Barium 133 (Ba 133)	10

Barium 140 (Ba 140)	10
Bismuth 210 (Bi 210)	1
Bromine 82 (Br 82)	10
Cadmium109 (Cd 109)	10
Cadmium 115m (Cd 115m)	10
Cadmium115 (Cd 115)	100
Calcium 45 (Ca 45)	10
Calcium 47 (Ca 47)	10
Carbon 14 (C 14)	100
Cerium 141 (Ce 141)	100
Cerium 143 (Ce 143)	100
Cerium 144 (Ce 144)	1
Cesium 129 (Cs 129)	100
Cesium 131 (Cs 131)	1,000
Cesium 134m (Cs 134m)	100
Cesium 134 (Cs 134)	1
Cesium 135 (Cs 135)	10
Cesium 136 (Cs 136)	10
Cesium 137 (Cs 137)	10
Chlorine 36 (Cl 36)	10
Chlorine 38 (Cl 38)	10
Chromium 51 (Cr 51)	1,000
Cobalt 57 (Co 57)	100
Cobalt 58m (Co 58m)	10
Cobalt 58 (Co 58)	10
Cobalt 60 (Co 60)	1
Copper 64 (Cu 64)	100
Dysprosium 165 (Dy 165)	10
Dysprosium 166(Dy 166)	100
Erbium 169 (Er 169)	100
Erbium 171 (Er 171)	100
Europium 152 9.2 h (Eu 152 9.2 h)	100
Europium 152 13 yr (Eu 152 13 yr)	1
Europium 154 (Eu 154)	1

Europium 155(Eu 155)	10
Fluorine 18 (F 18)	1,000
Gadolinium 153 (Gd 153)	10
Gadolinium 159 (Gd 159)	100
Gallium 67 (Ga 67)	100
Gallium 72 (Ga 72)	10
Germanium 68 (Ge 68)	10
Germanium 71 (Ga 71)	100
Gold 195 (Au 195)	10
Gold 198 (Au 198)	100
Gold 199 (Au 199)	100
Hafnium 181 (Hf 181)	10
Holmium 166 (Ho 166)	100
Hydrogen 3 (H3)	1,000
Indium 111 (In 111)	100
Indium 113m (In 113m)	100
Indium 114m(In 114m)	10
Indium 115m(In 115m)	100
Indium 115 (In 115)	10
Iodine 123 (I 123)	100
Iodine 125 (I 125)	1
Iodine 126 (I 126)	1
Iodine 129 (I 129)	0,1
Iodine 131 (I 131)	1
Iodine 132 (I 132)	10
Iodine 133 (I 133)	1
Iodine 134 (I 134)	10
Iodine 135 (I 135)	10
Iridium 192 (Ir 192)	10
Iridium 194 (Ir 194)	100
Iron 52 (Fe 52)	10
Iron 55 (Fe 55)	100
Iron 59 (Fe 59)	10
Krypton 85 (Kr 85)	100

Krypton 87 (Kr 87)	10
Lanthanum 140 (La 140)	10
Lutetium 177 (Lu 177)	100
Manganese 52 (Mn 52)	10
Manganese 54 (Mn 54)	10
Manganese 56 (Mn 56)	10
Mercury 197m (Hg 197m)	100
Mercury 197 (Hg 197)	100
Mercury 203 (Hg 203)	10
Molybdenum 99 (Mo 99)	100
Neodymium 147 (Nd 147)	100
Neodymium 149 (Nd 149)	100
Nickel 59 (Ni 59)	100
Nickel 63 (Ni 63)	10
Nickel 65 (Ni 65)	100
Niobium 93m (Nb 93m)	10
Niobium 95 (Nb 95)	10
Niobium 97 (Nb 97)	10
Osmium 185 (Os 185)	10
Osmium 191m (Os 191)	100
Osmium 191 (Os 191)	100
Osmium 193 (Os 193)	100
Palladium 103 (Pd 103)	100
Palladium 109 (Pd 109)	100
Phosphorus 32 (P 32)	10
Platinum 191 (Pt 191)	100
Platinum 193m (Pt 193m)	100
Platinum 193 (Pt 193)	100
Platinum 197m (Pt 197m)	100
Platinum 197 (Pt 197)	100
Polonium 210 (Po 210)	0.1
Potassium 42 (K 42)	10
Potassium 43 (K 43)	10
Praseodymium 142 (Pr 142)	100

Praseodymium 143 (Pr 143)	100
Promethium 147 (Pm 147)	10
Promethium 149 (Pm 149)	10
Rhenium 186 (Re 186)	100
Rhenium 188 (Re 188)	100
Rhodium 103m (Rh 103m)	100
Rhodium 105 (Rh 105)	100
Rubidium 81 (Rb81)	10
Rubidium 86 (R86)	10
Rubidium 87 (Rb87)	10
Ruthenium 97 (Ru 97)	100
Ruthenium 103 (Ru 103)	10
Ruthenium 105(Ru 105)	10
Ruthenium 106(Ru 106)	1
Samarium 151(Sm 151)	10
Samarium 153(Sm 153)	100
Scandium 46 (Sc 46)	10
Scandium 47 (Sc 47)	100
Scandium 48 (Sc 48)	10
Selenium 75 (Se 75)	10
Silicon 31 (Si 31)	100
Silver 105 (Ag 105)	10
Silver 110m (Ag 110m)	1
Silver 111 (Ag 111)	100
Sodium 22 (Na 22)	10
Sodium 24 (Na 24)	10
Strontium 85 (Sr 85)	10
Strontium 89 (Sr 89)	1
Strontium 90 (Sr 90)	0.1
Strontium 91 (Sr 91)	10
Strontium 92 (Sr 92)	10
Sulphur 35 (S 35)	100
Tantalum 182 (Ta 182)	10
Technetium 96 (Tc 96)	10

Techneium 97m (Tc 97m)	100
Techneium 97 (Tc 97)	100
Techneium 99m (Tc 99m)	100
Techneium 99 (Tc 99)	10
Tellurium 125 m (Te 125 m)	10
Tellurium 127m (Te 127m)	10
Tellurium 127 (Te 127)	100
Tellurium 129m (Te 129m)	10
Tellurium 129 (Te 129)	100
Tellurium 131m (Te 131m)	10
Tellurium 132 (Te 132)	10
Terbium 160 (Tb 160)	10
Thallium 200 (Tl 200)	100
Thallium 201 (Tl 201)	100
Thallium 202 (Tl 202)	100
Thallium 204 (Tl 204)	10
Thulium 170 (Tm 170)	10
Thulium 171 (Tm 171)	10
Tin 113 (Sn 113)	10
Tin 125 (Sn 125)	10
Tungsten 181 (W 181)	10
Tungsten 185 (W 185)	10
Tungsten 187 (W 187)	100
Vanadium 48 (V 48)	10
Xenon 131m (Xe 131m)	1,000
Xenon 133 (Xe 133)	100
Xenon 135 (Xe 135)	100
Ytterbium 175 (Yb 175)	100
Yttrium 87 (Y 87)	10
Yttrium 88 (Y 88)	10
Yttrium 90 (Y 90)	10
Yttrium 91 (Y91)	10
Yttrium 92 (Y92)	100
Yttrium 93 (Y93)	100

Zinc 65 (Zn 65)	10
Zinc 69m (Zn 69m)	100
Zinc 69 (Zn 69)	1,000
Zirconium 93 (Zr 93)	10
Zirconium 95 (Zr 95)	10
Zirconium 97 (Zr 97)	10
Any radioactive material not listed above other than alpha emitting radioactive materials	0.1

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3740. Quantities of radioactive materials requiring consideration of the need for an emergency plan for responding to a release.

Radioactive material ¹	Release fraction	Quantity (curies)
Actinium-228	0.001	4,000
Americium-241	.001	2
Americium-242	.001	2
Americium-243	.001	2
Antimony-124	.01	4,000
Antimony-126	.01	6,000
Barium-133	.01	10,000
Barium-140	.01	30,000
Bismuth-207	.01	5,000
Bismuth-210	.01	600
Cadmium-109	.01	1,000
Cadmium-113	.01	80
Calcium-45	.01	20,000
Californium-252	.001	g (20 mg)
Carbon-14 (non-carbon dioxide)	.01	50,000
Cerium-141	.01	10,000
Cerium-144	.01	300

Cesium-134	.01	2,000
Cesium-137	.01	3,000
Chlorine-36	.5	100
Chromium-51	.01	300,000
Cobalt-60	.001	5,000
Copper-64	.01	200,000
Curium-242	.001	60
Curium-243	.001	3
Curium-244	.001	4
Curium-245	.001	2
Europium-152	.01	500
Europium-154	.01	400
Europium-155	.01	3,000
Germanium-68	.01	2,000
Gadolinium-153	.01	5,000
Gold-198	.01	30,000
Hafnium-172	.01	400
Hafnium-181	.01	7,000
Holmium-166m	.01	100
Hydrogen-3	.5	20,000
Iodine-125	.5	10
Iodine-131	.5	10
Indium-114m	.01	1,000
Iridium-192	.001	40,000
Iron-55	.01	40,000
Iron-59	.01	7,000
Krypton-85	1.0	6,000,000
Lead-210	.01	8
Manganese-56	.01	60,000
Mercury-203	.01	10,000
Molybdenum-99	.01	30,000
Neptunium-237	.001	2
Nickel-63	.01	20,000
Niobium-94	.01	300

Phosphorus-32	.5	100
Phosphorus-33	.5	1,000
Polonium-210	.01	10
Potassium-42	.01	9,000
Promethium-145	.01	4,000
Promethium-147	.01	4,000
Radium-226	.001	100
Ruthenium-106	.01	200
Samarium-151	.01	4,000
Scandium-46	.01	3,000
Selenium-75	.01	10,000
Silver-110m	.01	1,000
Sodium-22	.01	9,000
Sodium-24	.01	10,000
Strontium-89	.01	3,000
Strontium-90	.01	90
Sulfur-35	.5	900
Technitium-99	.01	10,000
Technitium-99m	.01	400,000
Tellurium-127m	.01	5,000
Tellurium-129m	.01	5,000
Terbium-160	.01	4,000
Thulium-170	.01	4,000
Tin-113	.01	10,000
Tin-123	.01	3,000
Tin-126	.01	1,000
Titanium-44	.01	100
Vanadium-48	.01	7,000
Xenon-133	1.0	900,000
Yttrium-91	.01	2,000
Zinc-65	.01	5,000
Zirconium-93	.01	400
Zirconium-95	.01	5,000
Any other beta-gamma emitter	.01	10,000

Mixed fission products	.01	1,000
Mixed corrosion products	.01	10,000
Contaminated equipment beta-gamma	.001	10,000
Irradiated material, any form other than solid noncombustible	.01	1,000
Irradiated material, solid noncombustible	.001	10,000
Mixed radioactive waste, beta-gamma	.01	1,000
Packaged mixed waste, beta-gamma ²	.001	10,000
Any other alpha emitter	.001	2
Contaminated equipment, alpha	.0001	20
Packaged waste, alpha ²	.0001	20
Combinations of radioactive materials listed above ¹		

¹For combinations of radioactive materials, consideration of the need for an emergency plan is required if the sum of the ratios of the quantity of each radioactive material authorized to the quantity listed for that material in this section exceeds one.

²Waste packaged in Type B containers does not require an emergency plan.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3750. Quantities for use with decommissioning.

Materials	Microcuries
Americium-241	.01
Antimony-122	100
Antimony-124	10
Antimony-125	10
Arsenic-73	100
Arsenic-74	10
Arsenic-76	10
Arsenic-77	100
Barium-131	10

Barium-133	10
Barium-140	10
Bismuth-210	1
Bromine-82	10
Cadmium-109	10
Cadmium-115m	10
Cadmium-115	100
Calcium-45	10
Calcium-47	10
Carbon-14	100
Cerium-141	100
Cerium-143	100
Cerium-144	1
Cesium-131	1,000
Cesium-134m	100
Cesium-134	1
Cesium-135	10
Cesium-136	10
Cesium-137	10
Chlorine-36	10
Chlorine-38	10
Chromium-51	1,000
Cobalt-55	100
Cobalt-56	10
Cobalt-57	100
Cobalt-58m	10
Cobalt-58	10
Cobalt-60	1
Copper-64	100
Dysprosium-165	10
Dysprosium-166	100
Erbium-169	100
Erbium-171	100
Europium-152 9.2h	100

Europium-152 13 yr	1
Europium-154	1
Europium-155	10
Fluorine-18	1,000
Gadolinium-153	10
Gadolinium-159	100
Gallium-72	10
Germanium-71	100
Gold-198	100
Gold-199	100
Hafnium-181	10
Holmium-166	100
Hydrogen-3	1,000
Indium-113m	100
Indium-114m	10
Indium-115m	100
Indium-115	10
Iodine-125	1
Iodine-126	1
Iodine-129	0.1
Iodine-131	1
Iodine-132	10
Iodine-133	1
Iodine-134	10
Iodine-135	10
Iridium-192	10
Iridium-194	100
Iron-55	100
Iron-59	10
Krypton-85	100
Krypton-87	10
Lanthanum-140	10
Lutetium-177	100
Manganese-52	10

Manganese-54	10
Manganese-56	10
Mercury-197m	100
Mercury-197	100
Mercury-203	10
Molbdenum-99	100
Neodymium-147	100
Neodymium-149	100
Nickel-59	100
Nickel-63	10
Nickel-65	100
Niobium-93m	10
Niobium-95	10
Niobium-97	10
Osmium-185	10
Osmium-191m	100
Osmium-191	100
Osmium-193	100
Palladium-103	100
Palladium-109	100
Phosphorus-32	10
Platinum-191	100
Platinum-193m	100
Platinum-193	100
Platinum-197m	100
Platinum-197	100
Plutonium-239	.01
Polonium-210	0.1
Potassium-42	10
Praseodymium-142	100
Praseodymium-143	100
Promethium-147	10
Promethium-149	10
Radium-226	.01

Rhenium-186	100
Rhenium-188	100
Rhodium-103m	100
Rhodium-105	100
Rubidium-86	10
Rubidium-87	10
Ruthenium-97	100
Ruthenium-103	10
Ruthenium-105	10
Ruthenium-106	1
Samarium-151	10
Samarium-153	100
Scandium-46	10
Scandium-47	100
Scandium-48	10
Seleium-75	10
Silicon-31	100
Silver-105	10
Silver-110m	1
Silver-111	100
Sodium-24	10
Strontium-85	10
Strontium-89	1
Strontium-90	0.1
Strontium-91	10
Strontium-92	10
Sulphur-35	100
Tantalum-182	10
Technetium-96	10
Technetium-97m	100
Technetium-97	100
Technetium-99m	100
Technetium-99	10
Tellurium-125m	10

Tellurium127m	10
Tellurium-127	100
Tellurium129m	10
Tellurium-129	100
Tellurium-131m	10
Tellurium-132	10
Terbium-160	10
Thallium-200	100
Thallium-201	100
Thallium-202	100
Thallium-204	10
Thorium (natural) ¹	100
Thulium-170	10
Thulium-171	10
Tin-113	10
Tin-125	10
Tungsten-181	10
Tungsten-185	10
Tungsten-187	100
Uranium (natural) ²	100
Uranium-233	.01
Uranium-234--Uranium-235	.01
Vandium-48	10
Xenon-131m	1,000
Xenon-133	100
Xenon-135	100
Ytterbium-175	100
Yttrium-90	10
Yttrium-91	10
Yttrium-92	100
Yttrium-93	100
Zinc-65	10
Zinc-69m	100
Zinc-69	1,000

Zirconium-93	10
Zirconium-95	10
Zirconium-97	10
Any alpha emitting radionuclide not listed above or mixtures of alpha emitters of unknown composition	.01
Any radionuclide other than alpha emitting radio-nuclides, not listed above or mixtures of beta emitters of unknown composition	.1

¹Based on alpha disintegration rate of Th-232, Th-230 and their daughter products.

²Based on alpha disintegration rate of U-238, U-234, and U-235.

Note: For purposes of §20.2003, where there is involved a combination of isotopes in known amounts, the limit for the combination should be derived as follows: Determine, for each isotope in the combination, the ratio between the quantity present in the combination and the limit otherwise established for the specific isotope when not in combination. The sum of such ratios for all the isotopes in the combination may not exceed "1" (i.e., "unity").

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3760. Limits for broad scopes.

Radioactive material	Col. I curies	Col. II curies
Antimony-122	1	0.01
Antimony-124	1	0.01
Antimony-125	1	0.01
Arsenic-73	10	0.1
Arsenic-74	1	0.01
Arsenic-76	1	0.01
Arsenic-77	10	0.1
Barium-131	10	0.1
Barium-140	1	0.01

Beryllium-7	10	0.1
Bismuth-210	0.1	0.001
Bromine-82	10	0.1
Cadmium-109	1	0.01
Cadmium-115m	1	0.01
Cadmium-115	10	0.1
Calcium-45	1	0.01
Calcium-47	10	0.1
Carbon-14	100	1
Cerium-141	10	0.1
Cerium-143	10	0.1
Cerium-144	0.1	0.001
Cesium-131	100	1
Cesium-134m	100	1
Cesium-134	0.1	0.001
Cesium-135	1	0.01
Cesium-136	10	0.1
Cesium-137	0.1	0.001
Chlorine-36	1	0.01
Chlorine-38	100	1
Chromium-51	100	1
Cobalt-57	10	0.1
Cobalt-58m	100	1
Cobalt-58	1	0.01
Cobalt-60	0.1	0.001
Copper-64	10	0.1
Dysprosium-165	100	1
Dysprosium-166	10	0.1
Erbium-169	10	0.1
Erbium-171	10	0.1
Europium-152 9.2 h	10	0.1
Europium-152 13 y	0.1	0.001
Europium-154	0.1	0.001
Europium-155	1	0.01

Fluorine-18	100	1
Gadolinium-153	1	0.01
Gadolinium-159	10	0.1
Gallium-72	10	0.1
Germanium-71	100	1
Gold-198	10	0.1
Gold-199	10	0.1
Hafnium-181	1	0.01
Holmium-166	10	0.1
Hydrogen-3	100	1
Indium-113m	100	1
Indium-114m	1	0.01
Indium-115m	100	1
Indium-115	1	0.01
Iodine-125	0.1	0.001
Iodine-126	0.1	0.001
Iodine-129	0.1	0.001
Iodine-131	0.1	0.001
Iodine-132	10	0.1
Iodine-133	1	0.01
Iodine-134	10	0.1
Iodine-135	1	0.01
Iridium-192	1	0.01
Iridium-194	10	0.1
Iron-55	10	0.1
Iron-59	1	0.01
Krypton-85	100	1
Krypton-87	10	0.1
Lanthanum-140	1	0.01
Lutetium-177	10	0.1
Manganese-52	1	0.01
Manganese-54	1	0.01
Manganese-56	10	0.1
Mercury-197m	10	0.1

Mercury-197	10	0.1
Mercury-203	1	0.01
Molybdenum-99	10	0.1
Neodymium-147	10	0.1
Neodymium-149	10	0.1
Nickel-59	10	0.1
Nickel-63	1	0.01
Nickel-65	10	0.1
Niobium-93m	1	0.01
Niobium-95	1	0.01
Niobium-97	100	1
Osmium-185	1	0.01
Osmium-191m	100	1
Osmium-191	10	0.1
Osmium-193	10	0.1
Palladium-103	10	0.1
Palladium-109	10	0.1
Phosphorus-32	1	0.01
Platinum-191	10	0.1
Platinum-193m	100	1
Platinum-193	10	0.1
Platinum-197m	100	1
Platinum-197	100	.1
Polonium-210	0.01	0.0001
Potassium-42	1	0.01
Praseodymium-142	10	0.1
Praseodymium-143	10	0.1
Promethium-147	1	0.01
Promethium-149	10	0.1
Radium-226	0.01	0.0001
Rhenium-186	10	0.1
Rhenium-188	10	0.1
Rhodium-103m	1,000	10
Rhodium-105	10	0.1

Rubidium-86	1	0.01
Rubidium-87	1	0.01
Ruthenium-97	100	1
Ruthenium-103	1	0.01
Ruthenium-105	10	0.1
Ruthenium-106	0.1	0.001
Samarium-151	1	0.01
Samarium-153	10	0.1
Scandium-46	1	0.01
Scandium-47	10	0.1
Scandium-48	1	0.01
Selenium-75	1	0.01
Silicon-31	10	0.1
Silver-105	1	0.01
Silver-110m	0.1	0.001
Silver-111	10	0.1
Sodium-22	0.1	0.001
Sodium-24	1	0.01
Strontium-85m	1,000	10
Strontium-85	1	0.01
Strontium-89	1	0.01
Strontium-90	0.01	0.0001
Strontium-91	10	0.1
Strontium-92	10	0.1
Sulphur-35	10	0.1
Tantalum-182	1	0.01
Technetium-96	10	0.1
Technetium-97m	10	0.1
Technetium-97	10	0.1
Technetium-99m	100	1
Technetium-99	1	0.01
Tellurium-125m	1	0.01
Tellurium-127m	1	0.01
Tellurium-127	10	0.1

Tellurium-129m	1	0.01
Tellurium-129	100	1
Tellurium-131m	10	0.1
Tellurium-132	1	0.01
Terbium-160	1	0.01
Thallium-200	10	0.1
Thallium-201	10	0.1
Thallium-202	10	0.1
Thallium-204	1	0.01
Thulium-170	1	0.01
Thulium-171	1	0.01
Tin-113	1	0.01
Tin-125	1	0.01
Tungsten-181	1	0.01
Tungsten-185	1	0.01
Tungsten-187	10	0.1
Vandadium-48	1	0.01
Xenon-131m	1,000	10
Xenon-133	100	1
Xenon-135	100	1
Ytterbium-175	10	0.1
Yttrium-90	1	0.01
Yttrium-91	1	0.01
Yttrium-92	10	0.1
Yttrium-93	1	0.01
Zinc-65	1	0.01
Zinc-69m	10	0.1
Zinc-69	100	1
Zirconium-93	1	0.01
Zirconium-95	1	0.01
Zirconium-97	1	0.01
Any radioactive material other than alpha emitting radioactive material not listed above	0.1	0.001

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3770. Determination of A₁ and A₂.

The following regulation, Determination of A₁ and A₂ (10 CFR Part 71, Appendix A) is applicable in the Commonwealth of Virginia.

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.

12VAC5-481-3780. Nationally tracked source thresholds.

The terabecquerel (TBq) values are the regulatory standard. The curie (Ci) values specified are obtained by converting from the TBq value. The curie values are provided for practical usefulness only and are rounded after conversion.

Radioactive material	Category 1 (TBq)	Category 1 (Ci)	Category 2 (TBq)	Category 2 (Ci)
Actinium-227	20	540	0.2	5.4
Americium-241	60	1,600	0.6	16
Americium-241/Be	60	1,600	0.6	16
Californium-252	20	540	0.2	5.4
Cobalt-60	30	810	0.3	8.1
Curium-244	50	1,400	0.5	14
Cesium-137	100	2,700	1	27
Gadolinium-153	1,000	27,000	10	270
Iridium-192	80	2,200	0.8	22
Plutonium-238	60	1,600	0.6	16
Plutonium-239/Be	60	1,600	0.6	16
Polonium-210	60	1,600	0.6	16
Promethium-147	40,000	1,100,000	400	11,000

Radium-226	40	1,100	0.4	11
Selenium-75	200	5,400	2	54
Strontium-90	1,000	27,000	10	270
Thorium-228	20	540	0.2	5.4
Thorium-229	20	540	0.2	5.4
Thulium-170	20,000	540,000	200	5,400
Ytterbium-169	300	8,100	3	81

Statutory Authority

§32.1-229 of the Code of Virginia.

Historical Notes

Derived from Virginia Register Volume 24, Issue 18, eff. June 12, 2008.
