


Serial# 423050

3H Efficiency

Total # pts : 953
Valid # pts : 30
Mean : 64.50
SD : 0.28

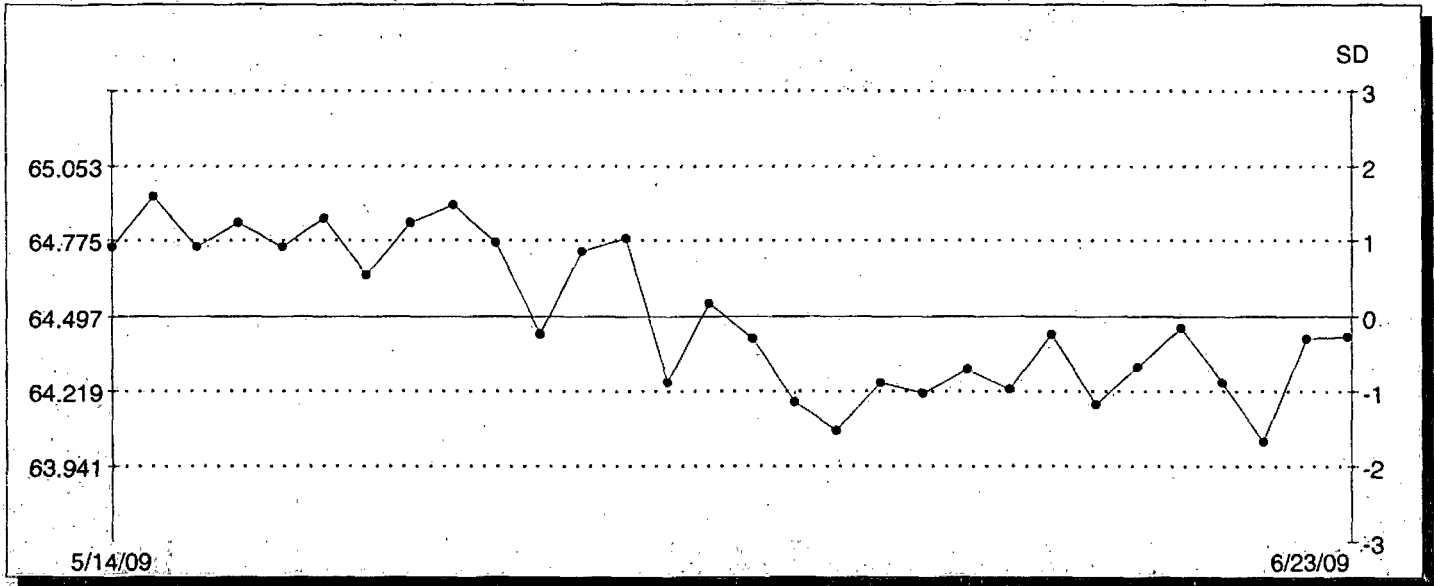

Handwritten signature or initials

Serial# 423050

3H Efficiency

Total # pts : 953
Valid # pts : 30
Mean : 64.50
SD : 0.28

Date	Value	Valid Pt
May 14, 2009	64.75	X
May 15, 2009	64.94	X
May 18, 2009	64.75	X
May 19, 2009	64.84	X
May 20, 2009	64.75	X
May 21, 2009	64.86	X
May 23, 2009	64.65	X
May 28, 2009	64.85	X
May 29, 2009	64.91	X
May 30, 2009	64.77	X
Jun 01, 2009	64.43	X
Jun 03, 2009	64.74	X
Jun 04, 2009	64.79	X
Jun 05, 2009	64.25	X
Jun 05, 2009	64.54	X
Jun 06, 2009	64.41	X
Jun 07, 2009	64.18	X
Jun 08, 2009	64.07	X
Jun 09, 2009	64.25	X
Jun 09, 2009	64.21	X
Jun 10, 2009	64.30	X
Jun 12, 2009	64.22	X
Jun 12, 2009	64.43	X
Jun 13, 2009	64.17	X
Jun 14, 2009	64.30	X
Jun 15, 2009	64.45	X
Jun 18, 2009	64.25	X
Jun 19, 2009	64.03	X
Jun 20, 2009	64.41	X
Jun 23, 2009	64.42	X