


Room 1220 Scoping Survey

Contents

Page	
2	Floor Plan
3	Hood wipe results
4	List of objects surveyed
5	Object wipe results

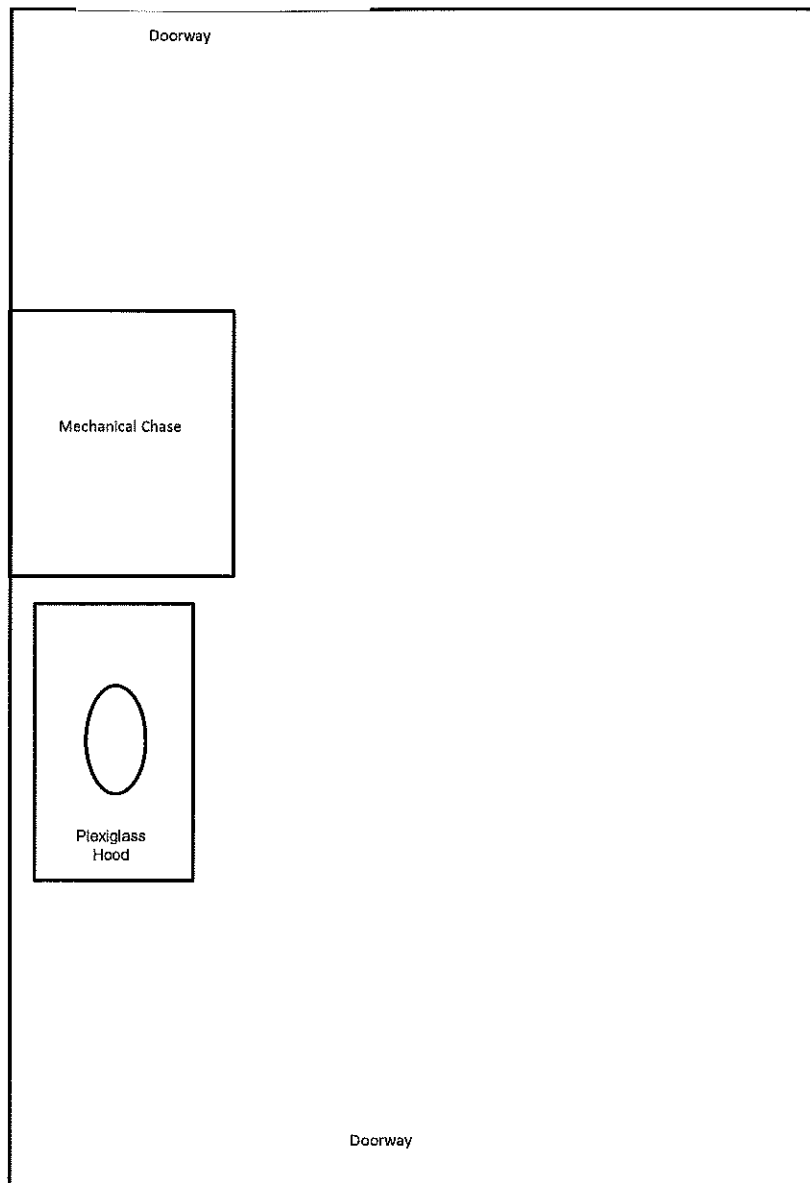

Floor Plan Room 1220

RSA Laboratories
 A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**

Customer: **Chemtura**

Customer Samp No. **N/A**

Location: **1220 Hood 04**

4' Plexiglas® Hood

RSA Lab Sample No. **N/A**

Project: **Lab Decommissioning**

Date Collected: **3/10/2011**

Samp. Description: **Survey Wipes**

Date Counted: **3/10/2011**

Matrix: **Wipes**

C-14 LLD dpm= 39.94

RSA ID#	CUST. ID#	Location	C-14 CPM	dpm/100 cm sq
BG		BACKGROUND	34.30	
1		Left Side	12.90	14.20
2		Left back	4.20	4.70
3		Right Back	9.50	10.40
4		Right Back	9.80	10.80
5		Counter Left	4.10	4.50
6		Counter Right	18.90	20.90
7		Sill	2.90	3.20
8		Ceiling Left	10.40	11.40
9		Ceiling Right	4.60	5.00
10		Glas Left	11.40	12.50
11		Glass Right	9.40	10.30
C-14		QC C-14	107840.50	134397.40
BL		QC Blank	10.00	10.90

Object # Description

288 Tool Box
289 Table
290 Dewar
291 Flammable Cabinet
292 HPLC
293 HPLC
294 HPLC
295 Refrigerator RF-27
296 Phone

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1


Report No. **N/A**Customer: **Chemtura**Customer Samp No. **N/A**Location: **1220 Objects**RSA Lab Sample No. **N/A**Project: **Lab Decommissioning**Date Collected: **02/02/2011 - 02/11/2011**Samp. Description: **Survey Wipes**Date Counted: **02/02/2011 -02/15/2011**Matrix: **Wipes****C-14 LLD dpm= 41.55**

RSA ID#	CUST. ID#	Location	C-14 CPM	dpm/100 cm sq
	BG	BACKGROUND	37.40	
1		Object 288	10.70	11.60
2		Object 289 Left Top	19.90	21.50
3		Object 289 Right Top	13.90	15.00
4		Object 289 Shelf	6.80	7.70
5		Object 290	4.60	4.90
6		Object 291 Top	3.30	3.60
7		Object 291 Right Side	12.10	13.10
8		Object 291 Left Side	15.10	16.30
9		Object 291 Front	1.20	1.30
10		Object 291 Left Inside	5.30	5.70
11		Object 291 Shelf	9.50	10.20
12		Object 291 Right Inside	12.70	13.70
13		Object 291 Bottom	19.20	20.80
14		Object 291 Door Inside	8.70	9.40
15		Object 292	13.40	14.60
16		Object 293	0.00	0.00
17		Object 294	9.00	9.80
18		Object 295 Top	15.60	16.80
19		Object 295 L Side	15.30	16.40
20		Object 295 R Side	5.00	5.40
21		Object 295 Front	10.90	11.80
22		Object 295 Inside Left	10.30	11.10
23		Object 295 Back	14.30	15.40
C14		QC C-14	124732.50	134904.30
24		Object 295 Inside Right	13.80	14.80
25		Object 295 Bottom	18.00	19.40
26		Object 295 Inside Door	6.70	7.20
27		Object 296	16.10	17.40
BL		QC Blank	9.90	10.70
27		Object 289 Right Top Post Decon	12.90	13.90
28		Object 289 Left Top Post Decon	29.70	32.10
29		Object 289 Right Shelf Post Decon	0.00	0.00
30		Object 289 Left Shelf Post Decon	21.30	23.70

Room 1221 Scoping Survey

Contents


Page	
2	Floor Plan
3	Drawing of a typical 8-foot fume hood
4	Wipe test data for Hood 17
5	List of objects surveyed
6-7	Object wipe results

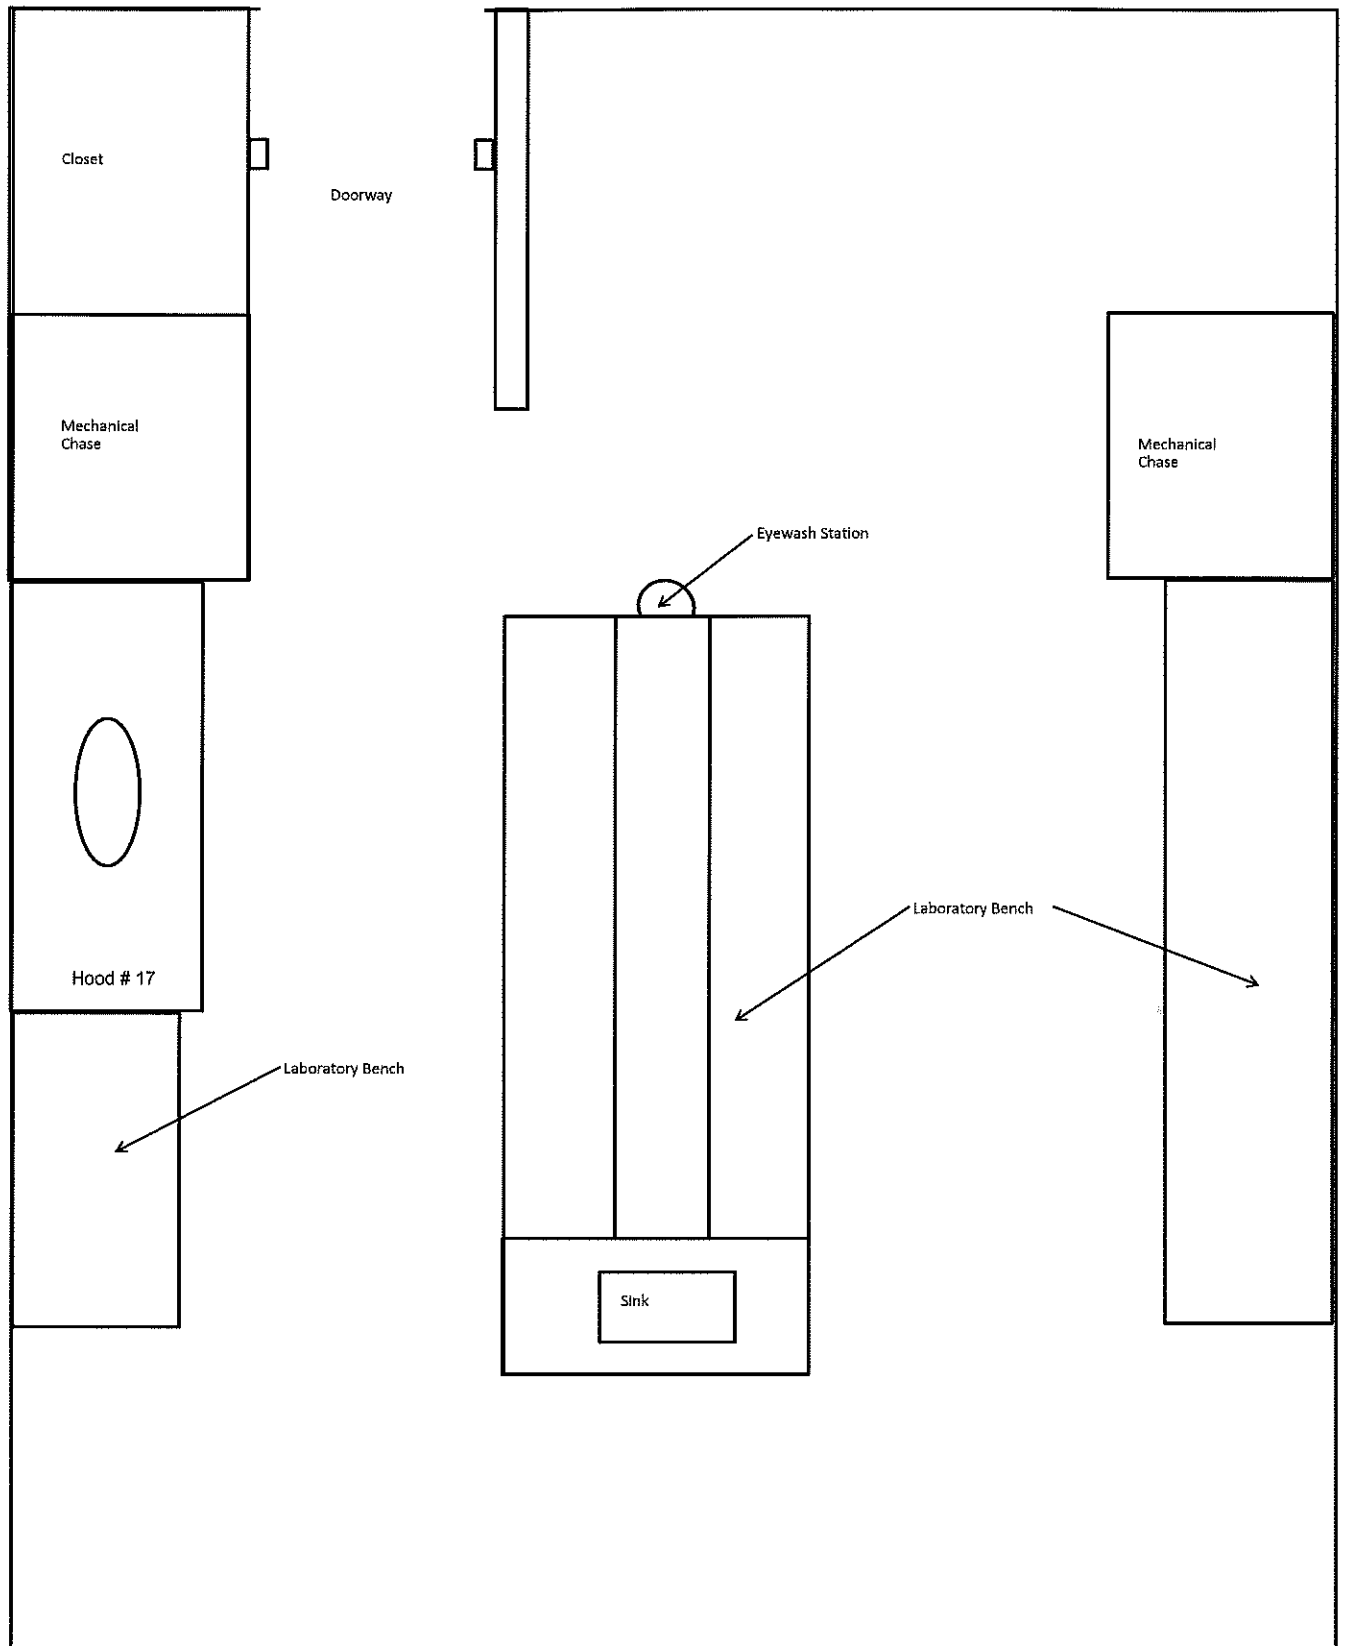


Floor Plan Room 1221

19 Pendleton Drive
 Hebron, CT 06248
 (860) 228-0487

8 Foot fume hood

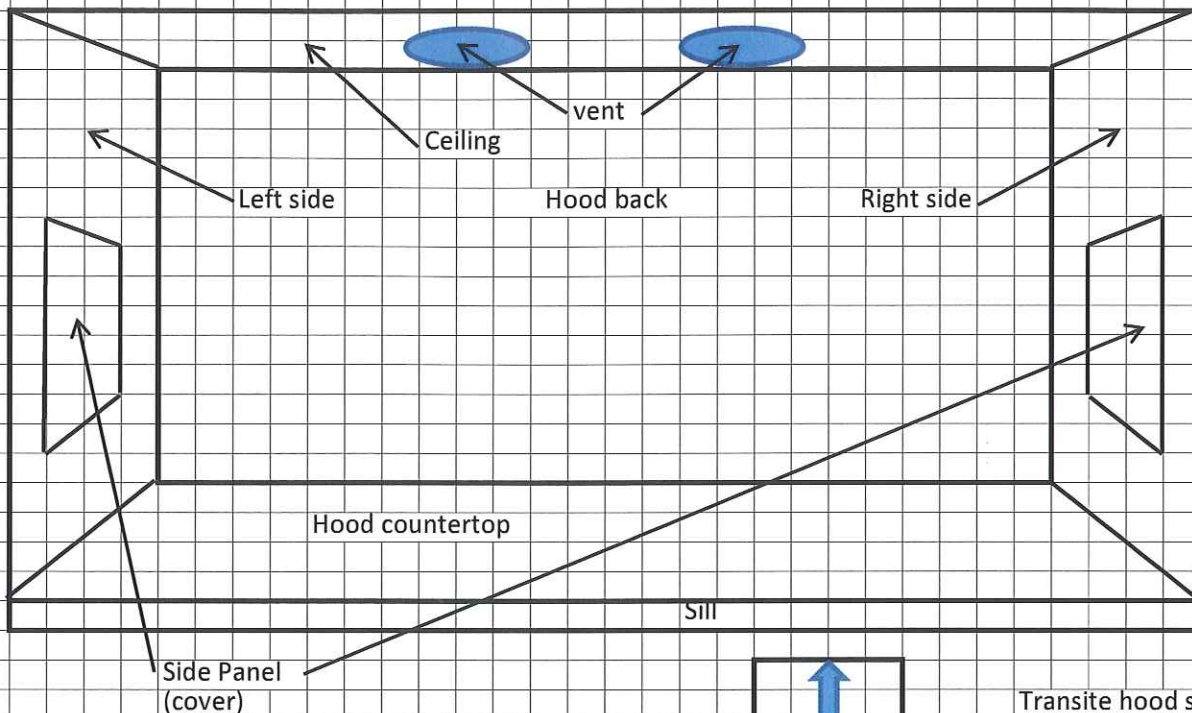

Transite hood side view

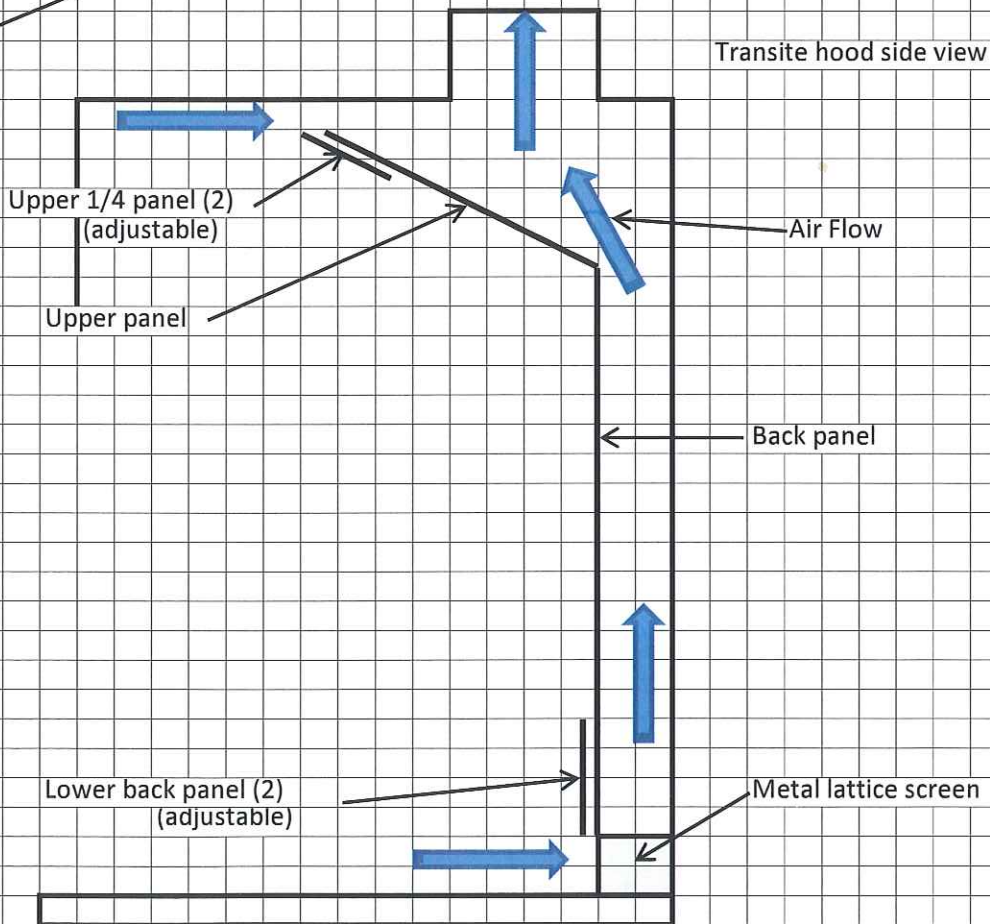

The following are removable

- 1 Upper 1/4 panel
- 2 Upper panel
- 3 Back panel
- 4 Lower Back panel
- 5 Side panel
- 6 Metal lattice screen

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**Customer Samp No. **N/A**RSA Lab Sample No. **N/A**Date Collected: **3/9/2011**Date Counted: **3/9/2011**Customer: **Chemtura**Location: **1221 Hood 17**Project: **Lab Decommissioning**Samp. Description: **Survey Wipes**Matrix: **Wipes****C-14 LLD dpm= 39.94**

RSA ID#	CUST. ID#	Location	C-14 CPM	dpm/100 cm sq
	BG	BACKGROUND	34.30	
1		Left Side	0.00	0.00
2		Hood Back Upper Left	0.00	0.00
3		Hood Back Upper Right	10.80	11.90
4		Hood Back Lower Left	10.10	11.10
5		Hood Back Lower Right	12.70	14.00
6		Right Side	14.00	15.30
7		Counter Left	10.70	11.80
8		Counter Right	18.30	20.10
9		Sill	0.90	1.00
10		Ceiling Right	9.00	9.90
11		Ceiling Left	8.90	9.80
12		Glass Left	14.50	15.90
13		Glass Right	10.60	11.50
14		Screen	4.00	4.40
15		Lower Back Left Front	20.90	23.00
16		Lower Back Left Back	3.60	4.00
17		Lower Back Right Front	0.00	0.00
18		Lower Back Right Back	0.00	0.00
19		Back Panel Left Front	7.90	8.60
20		Back Panel Left Back	13.10	14.30
21		Back Panel Right Front	7.60	8.40
22		Back Panel Left Front	12.40	13.60
C-14		QC C-14	114435.80	134219.80
23		Upper Panel Left Front	10.00	11.30
24		Upper Panel Left Back	14.70	16.20
25		Upper Panel Right Front	16.00	17.50
26		Upper Panel Left Front	12.20	13.30
27		Upper 1/4 Left Front	10.00	11.00
28		Upper 1/4 Left Back	3.30	3.60
29		Upper 1/4 Right Front	8.60	9.40
30		Upper 1/4 Right Back	21.30	23.60
31		Left Cover	14.30	15.50
32		Right Cover	6.40	7.00
BL		QC Blank	10.10	11.00

Object #	Description
298	File Cabinet
299	File Cabinet
300	File Cabinet
301	File Cabinet
302	File Cabinet
303	File Cabinet
304	File Cabinet
305	File Cabinet
306	Table
307	Flammable Cab
308	File Cabinet
309	Oven
310	Phone
311	Centrifuge
312	Refrigerator RF-24
313	Freezer - 07

RSA Laboratories
 A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 2

Report No. **N/A**

Customer: **Chemtura**

Customer Samp No. **N/A**

Location: **1221 Objects**

RSA Lab Sample No. **N/A**

Project: **Lab Decommissioning**

Date Collected: **1/0/1900**

Samp. Description: **Survey Wipes**

Date Counted: **1/0/1900**

Matrix: **Wipes**


C-14 LLD dpm= 38.20

RSA ID#	CUST. ID#	Location	C-14 CPM	dpm/100 cm sq
BG		BACKGROUND	31.10	
62		Object 298	19.60	21.40
63		Object 299	12.80	13.90
64		Object 300	11.80	12.90
65		Object 301	17.30	18.90
66		Object 302	10.50	11.50
67		Object 303	24.70	26.90
68		Object 304	0.00	0.00
69		Object 305	11.30	12.40
70		Object 306	11.40	12.50
71		Object 307 Top	11.30	12.40
72		Object 307 Right Side	14.30	15.60
73		Object 307 Left Side	0.00	0.00
74		Object 307 Front	12.10	13.20
75		Object 307 Left Inside	10.10	11.00
76		Object 307 Shelf	21.10	23.00
77		Object 307 Right Inside	12.20	13.20
78		Object 307 Bottom	16.50	18.00
79		Object 307 Inside Door	17.90	19.50
80		Object 308	6.30	6.90
81		Object 309 Top	13.20	14.40
82		Object 309 Right Side	12.60	13.70
83		Object 309 Left Side	17.80	19.40
84		Object 309 Front	2.80	3.10
C-14		QC C-14	124756.20	134973.70
85		Object 309 Left Inside	12.50	13.70
86		Object 309 Back	12.50	13.70
87		Object 309 Right Inside	14.80	16.30
88		Object 309 Bottom	14.20	15.50
89		Object 309 Inside Door	5.70	6.30
90		Object 310	13.90	15.20
91		Object 311	10.50	11.50
92		Object 312 Top	11.00	12.00
93		Object 312 Right Side	29.90	32.60
94		Object 312 Left Side	17.40	18.90
95		Object 312 Front	18.00	19.60

Room 1222 Scoping Survey


Contents

Page	
2	Floor Plan
3	Drawing of a typical 6-foot fume hood
4	Drawing of a typical 8-foot fume hood
5	Wipe test data for Hood 20
6	Wipe test data for Hood 20A




19 Pendleton Drive
 Hebron, CT 06248
 (860) 228-0487

6 Foot fume hood

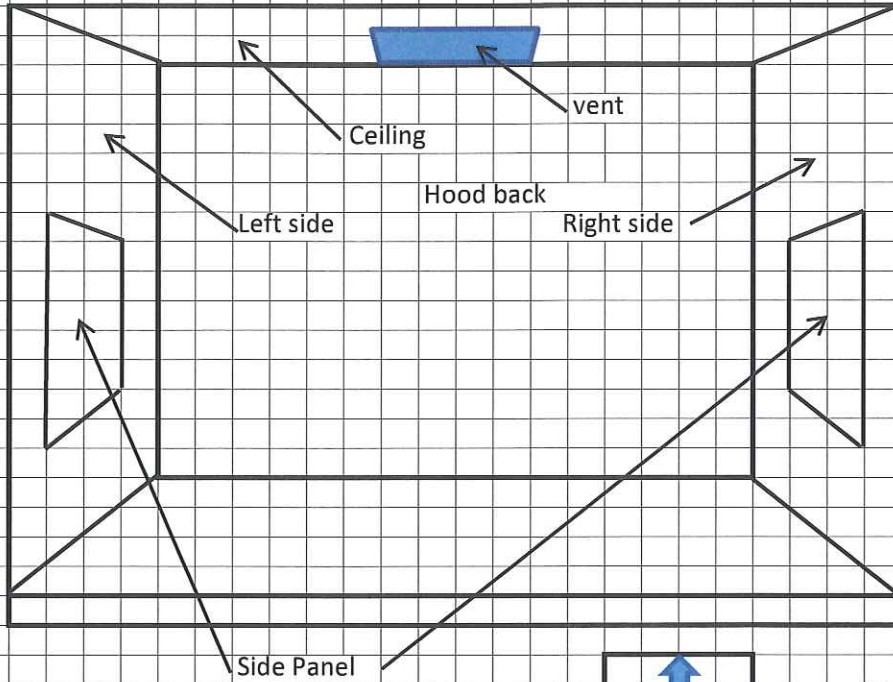

Transite hood side view

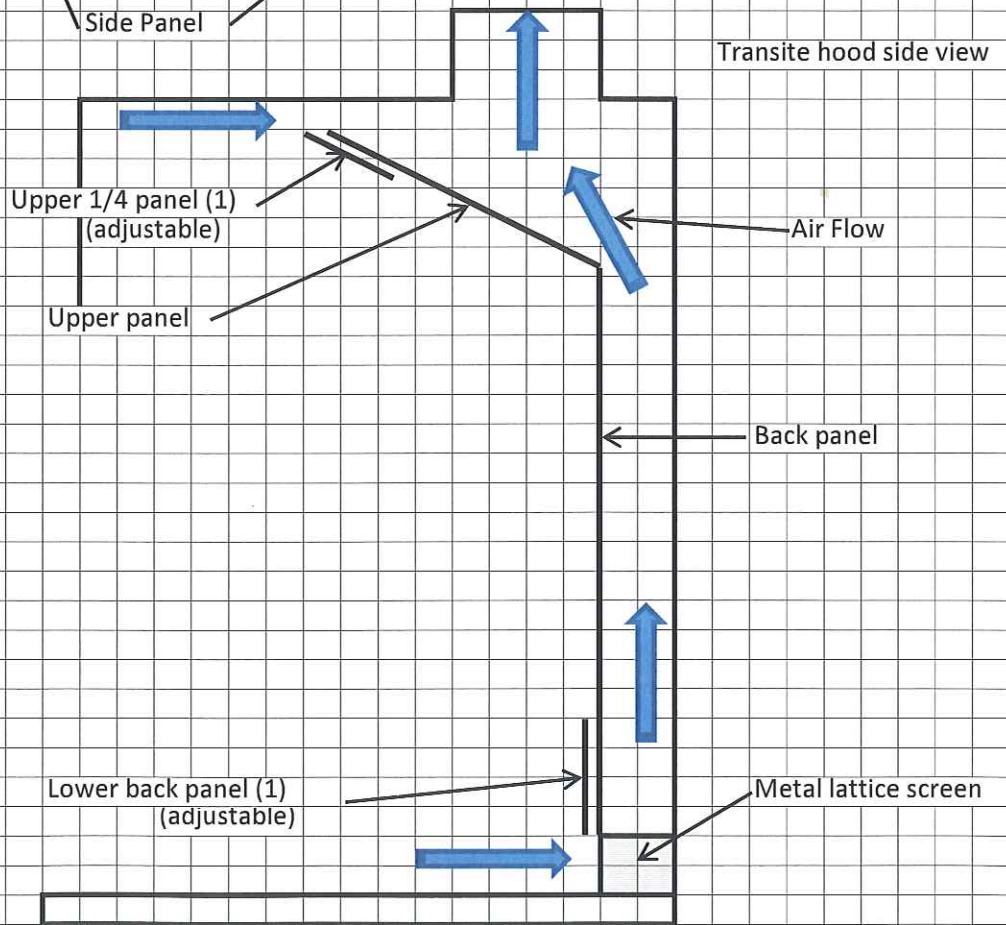


The following are removable


- 1 Upper 1/4 panel
- 2 Upper panel
- 3 Back panel
- 4 Lower Back panel
- 5 Side panel
- 6 Metal lattice screen

19 Pendleton Drive
 Hebron, CT 06248
 (860) 228-0487

8 Foot fume hood

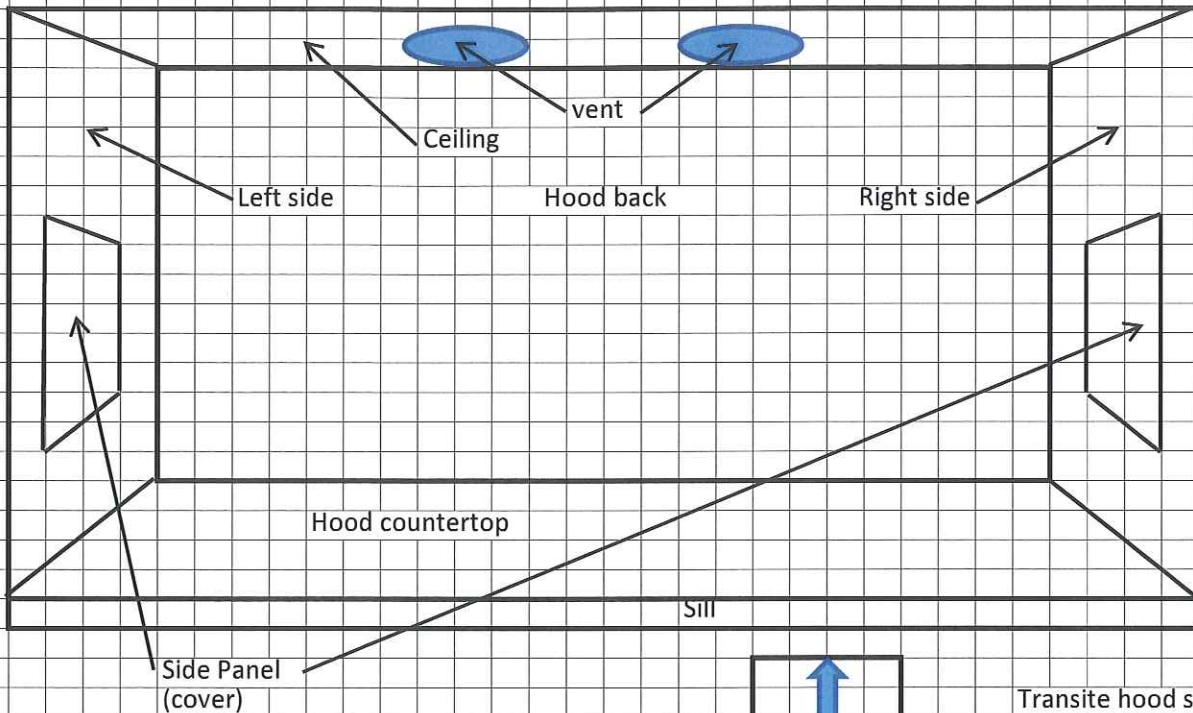

Transite hood side view

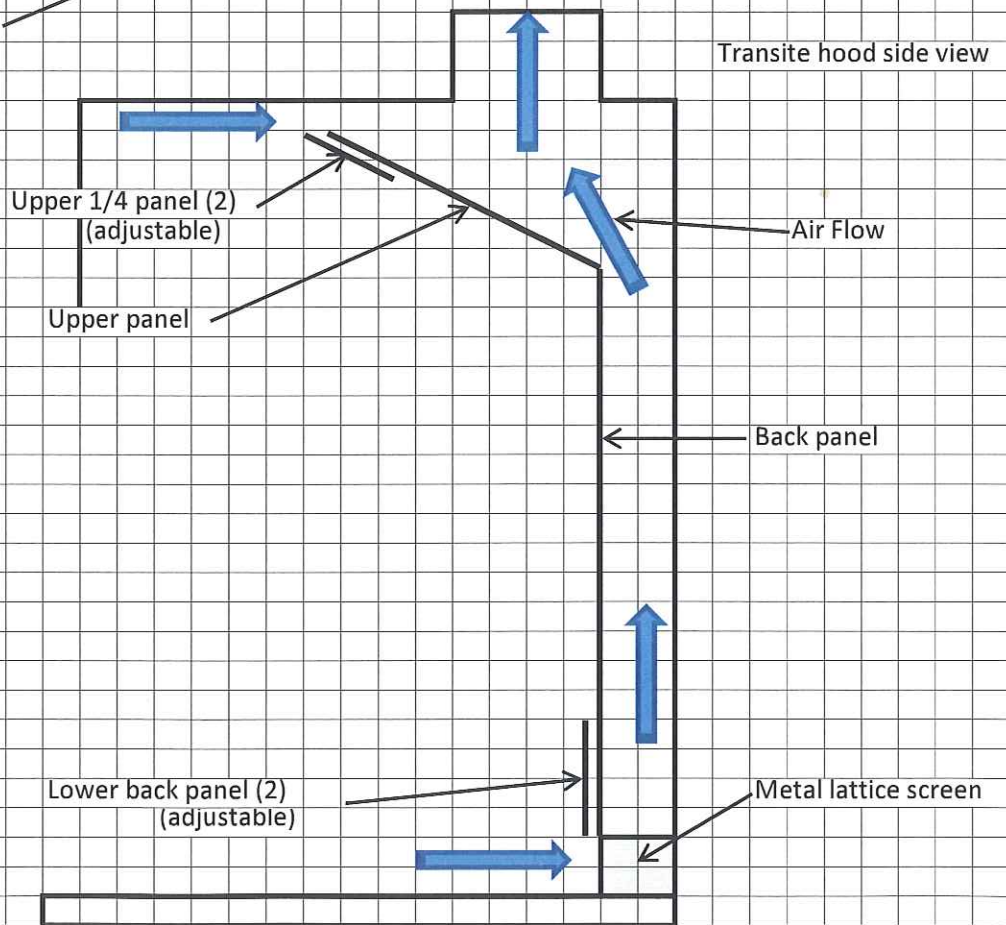

The following are removable

- 1 Upper 1/4 panel
- 2 Upper panel
- 3 Back panel
- 4 Lower Back panel
- 5 Side panel
- 6 Metal lattice screen

RSA Laboratories
 A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**

Customer: **Chemtura**

Customer Samp No. **N/A**

Location: **1222 Hood 20**

RSA Lab Sample No. **N/A**

Project: **Lab Decommissioning**

Date Collected: **02/17/2011 - 02/28/2011**

Samp. Description: **Survey Wipes**

Date Counted: **02/17/2011 - 02/28/2011**

Matrix: **Wipes**

C-14 LLD dpm= 39.35

RSA ID#	CUST. ID#	Location	C-14 CPM	dpm/100 cm sq
	BG	BACKGROUND	33.20	
1		Left Side	11.10	11.90
2		Right Side	9.60	10.40
3		Lower Back Left Front	10.00	10.80
4		Lower Back Left Back	3.70	4.00
5		Lower Back Right Front	11.00	11.80
6		Lower Back Right Back	15.40	16.70
7		Hood Back Left	8.20	8.80
8		Hood Back Right	3.20	3.50
9		Glass Left	2.00	2.10
10		Glass Right	12.70	13.90
11		Left Upper Panel Front	4.50	4.90
12		Left Upper Panel Back	11.50	12.60
13		Right Upper Panel Front	0.00	0.00
14		Right Upper Panel Back	10.90	11.80
15		Left Upper 1/4 panel Front	15.20	16.40
16		Left Upper 1/4 panel Back	11.40	12.40
17		Right Upper 1/4 panel Front	15.90	17.20
18		Right Upper 1/4 panel Back	15.00	16.20
19		Left Cover	0.00	0.00
20		Right Cover	15.10	16.30
21		Left Counter	11.60	12.50
22		Right Counter	21.90	23.70
23		Screen	99.90	112.30
24		Hood Back Upper Left	14.10	15.30
25		Hood Back Upper Right	26.60	28.70
26		Hood Back Lower Left	13.50	14.70
27		Hood Back Lower Right	41.10	44.40
28		Ceiling Left	20.60	23.90
29		Ceiling Right	39.20	42.60
C-14		QC C-14	125295.70	135557.40
BL		QC Blank	23.80	25.80

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**Customer: **Chemtura**Customer Samp No. **N/A**Location: **1222 Hood 20A**RSA Lab Sample No. **N/A**Project: **Lab Decommissioning**Date Collected: **2/18/2011**Samp. Description: **Survey Wipes**Date Counted: **2/18/2011**Matrix: **Wipes****C-14 LLD dpm= 40.98**

RSA ID#	CUST. ID#	Location			C-14 CPM	dpm/100 cm sq
BG		BACKGROUND			36.30	
1		Left Side			26.00	28.10
2		Right Side			14.00	15.10
3		Counter Left			17.50	18.90
4		Counter Right			15.10	16.30
5		Sill			21.10	23.00
6		Lower Back Front			8.70	9.50
7		Lower Back Back			5.30	5.70
8		Upper Panel Front			29.70	32.20
9		Upper Panel Back			0.90	0.90
10		Upper 1/4 Front			12.30	13.40
11		Upper 1/4 Back			20.30	22.00
12		Back Panel left front			9.70	10.50
13		Back Panel right front			17.52	18.90
14		Back Panel left back			22.20	24.00
15		Back Panel right back			17.00	18.50
16		Glass Left			29.60	32.00
17		Glass Right			15.90	17.20
18		Hood Back Upper Left			13.30	14.40
19		Hood Back Upper Right			1.00	1.10
20		Hood Back Lower Left			2.30	2.50
21		Hood Back Lower Right			4.30	4.70
22		Left Ceiling			15.70	17.20
23		Right Ceiling			15.30	16.70
C-14		QC C-14			121523.20	134205.70
24		Screen			9.50	10.90
25		Left Cover			18.30	19.80
26		Right Cover			1.50	1.60
BL		QC Blank			0.00	0.00