



SOUTHWEST RESEARCH INSTITUTE®

5220 Culebra Road, P.O. Drawer 28510
Institute Quality Systems
Institute Calibration Laboratory
Phone: 210-522-5215 Fax 210-522-4834



Calibration Laboratory
Certificate #0972-01

Certificate of Calibration

Cost Center / Customer: DIV20 / DON BANNON

Mail Stop: B57

Manufacturer/Model: ORION / 920A

Description: PH/ION METER

Serial Number: 039518

Asset Number: 017640

Procedure: PH METERS - 23 DEC 09

Work Order: 303103468

Date Issued: 9-Sep-2011

Date Calibrated: 9-Sep-2011

*** Date Due :** 9-Mar-2012

**** Results:** FOUND-LEFT

Temperature: 72.0 °F

Humidity: 45 %RH

Barometer: N/A

This certificate documents traceability to the National Institute of Standards and Technology (NIST) and the International System of Units (SI). The Laboratory quality system conforms to ISO/IEC 17025, 2005, ANSI/NCCL Z540-1-1994 and relevant requirements of the ISO 9000-2000 standard. This certificate shall not be reproduced, except in full, without the written approval of the Southwest Research Institute Calibration Laboratory. This certificate shall not be used to claim product endorsement by Southwest Research Institute, American Association for Laboratory Accreditation (A2LA) or any agency of the U. S. Government. Results of this calibration relate only to the instrument described above at the time of calibration and does not imply any long term stability of the instrument.

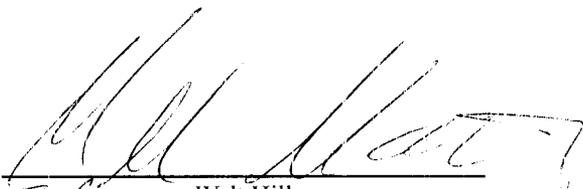
*Determined by the customer, does not imply the instrument will remain within tolerance as any number of factors may cause an out-of-tolerance condition before this date. **Data type found in this certificate or attached measurement report must be interpreted as: Found-left - adjustment and/or repair was not performed, As-found - data is before unit is adjusted and/or repaired, As-left - data is after adjusted and/or repaired was performed. The customer has sole responsibility for determination of in-/out-of-tolerance or compliance/noncompliance.


Measurement uncertainty calculated in accordance with the method described in the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM), for a confidence level of approximately 95 percent using a coverage factor of $k=2$.

Remarks: MILLIVOLTS CALIBRATED ONLY.

Standards Used

<u>Asset #</u>	<u>Manufacturer</u>	<u>Model</u>	<u>Description</u>	<u>Cal Date</u>	<u>Due Date</u>
006413	FLUKE	5520A/SC1100	MULTI-PRODUCT CALIBRATOR	3-May-2011	3-May-2012


Walt Hill
Laboratory Manager


Clint Rowe
Metrology Technician

Southwest Research Institute
Calibration Laboratory
Measurement Report

Work Order:	303103468	Mfr:	Orion	Technician:	CER
Asset No.:	017640	Model:	720A	Type Data:	Found-left
Serial No.:	039518	Type:	pH Meter	Cal Date:	9-Sep-11

Remarks: millivolts calibrated only.

Function/Range	Test Point	TI Reading	Difference	± Limit	± Uncertainty	Result	% Limit
mVolts Input 1	mVolts 0.0	mVolts 0.0	mVolts 0.0	mVolts 0.5	mVolts 0.24	Pass	0%
	1000.0	1000.2	0.2	1.0	0.24	Pass	20%
	-1000.0	-1000.2	-0.2	1.0	0.24	Pass	20%
mVolts Input 2	mVolts 0.0	mVolts 0.0	mVolts 0.0	mVolts 0.5	mVolts 0.24	Pass	0%
	1000.0	1000.2	0.2	1.0	0.24	Pass	20%
	-1000.0	-1000.2	-0.2	1.0	0.24	Pass	20%

END OF REPORT