

Radiological Survey Sheet

Job Location Pfizer, Inc. Groton, Ct. 06340 118 N / No 6 Page 1 of 6
 Survey Purpose Radiologic Survey of Equipment LAA decom m Date 10-3-12
 Performed by E. GAILOR E Gailor
 (Print) (Sign)

| | | | | |
|-------------------------------|-----------------------------|-----------------------------|------------------------|-------------------------------|
| Instrument (Model/S/N) | Packard Tri-Carb S/N 431521 | Packard Tri-Carb S/N 431520 | Ludlum 2241-2 163603 | Wallac Model 1409 S/N 4061042 |
| Det. (Model/SN) | Internal | Internal | Ludlum 43-68 PR 149613 | Internal |
| Type Rad. | β | β | β | β |
| Cal. Due: | 03/05/2013 | 03/05/2013 | 04/17/2013 | 09/15/2012 |
| Check Instruments Used | ✓ | | ✓ | |

| No. | Time | Locations | See attached LSC printout for Total Activity (cpm/100 cm ²) |
|-----|------|--------------|---|
| 1. | 0845 | BACKGROUND | |
| 2. | | door | |
| 3. | | 1st floor | |
| 4. | | UPPER WALL | |
| 5. | | LOWER " | |
| 6. | | CAB DOORS | |
| 7. | | " TOP SHELVE | |
| 8. | | " 2nd " | |
| 9. | | " 3rd " | |
| 10. | | SINK AREA | |
| 11. | | UPPER WALL | |
| 12. | | LOWER " | |
| 13. | | UPPER " | |
| 14. | | LOWER " | |
| 15. | | UPPER " | |
| 16. | | LOWER " | |
| 17. | | UPPER " | |
| 18. | | LOWER " | |

Radiological Survey Continuation Sheet


Page 2 of 6

Date 10-3-12

| No. | Time | Locations | See attached LSC printout for Total Activity (cpm/100 cm ²) |
|-----|------|------------|---|
| 19 | 0845 | UPPER WALL | |
| 20 | | LOWER " | |
| 21 | | UPPER " | |
| 22 | | LOWER " | |
| 23 | | UPPER " | |
| 24 | | LOWER " | |
| 25 | | UPPER " | |
| 26 | | LOWER " | |
| 27 | | UPPER " | |
| 28 | | LOWER " | |
| 29 | | UPPER " | |
| 30 | | LOWER " | |
| 31 | | UPPER " | |
| 32 | | LOWER " | |
| 33 | | UPPER " | |
| 34 | | LOWER " | |
| 35 | | UPPER " | |
| 36 | | LOWER " | |
| 37 | | FLOOR | |
| 38 | | " | |
| 39 | | " | |
| 40 | | " | |
| 41 | | " | |
| 42 | | " | |
| 43 | | " | |
| 44 | | " | |
| 45 | ✓ | " | |

118N / NO6

Pg 4 of 6
10-3-12

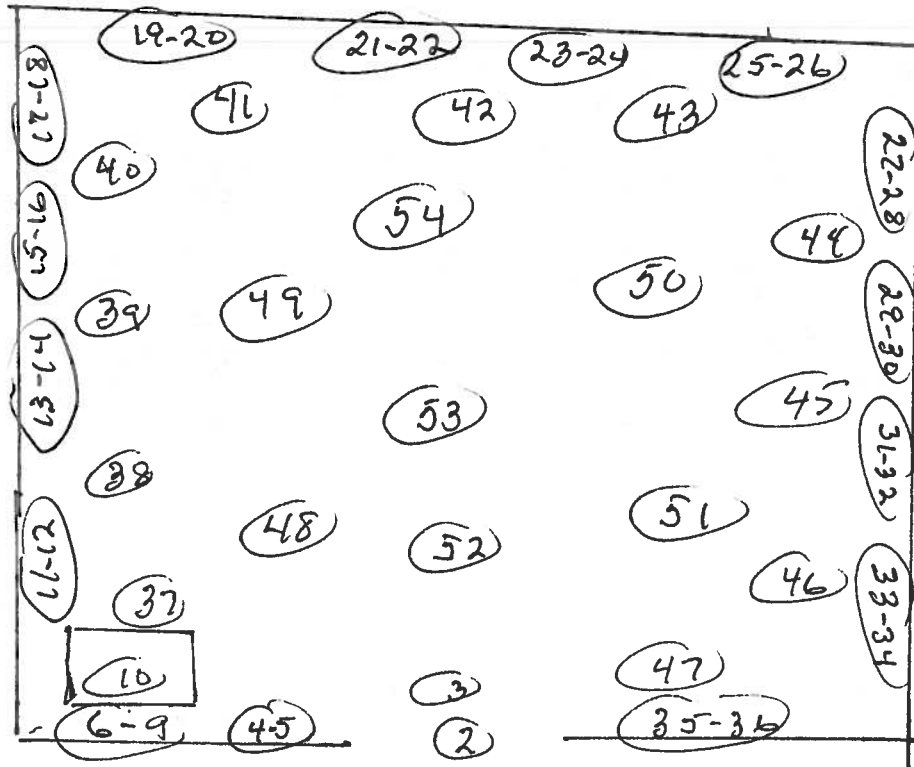

O = wipe location

- 100% of leach surfaces were surveyed using 43-68. NO READINGS
AN EXCESS OF NORMAL BACKGROUND LEVELS WERE NOTED.

Assay Definition-

Assay Description:
Equipment Swipes

Assay Type: CPM
Report Name: Report1
Output Data Path: C:\Packard\Tricarb\Results\Ed Gailor\Eds Monthly Swipes
Raw Results Path: C:\Packard\Tricarb\Results\Ed Gailor\Eds Monthly Swipes\20121003_1131\20121003_1131.results
RTF File Name: C:\Packard\Tricarb\Results\Ed Gailor\Eds Monthly Swipes\Ed's Monthly Swipes.rtf
Assay File Name: C:\Packard\TriCarb\Assays\Eds Monthly Swipes.lsa

Count Conditions-

Nuclide: Triple
Quench Indicator: tSIE/AEC
External Std Terminator (sec): 5 sec
Pre-Count Delay (min): 0.00
Quench Set: n/a
Count Time (min): 1.00
Count Mode: Normal
Assay Count Cycles: 1 Repeat Sample Count: 1
#Vials/Sample: 1 Calculate % Reference: Off

Background Subtract: On - Manual
Low CPM Threshold: Off
2 Sigma % Terminator: Off

| Regions | LL | UL | Bkg Subtract |
|---------|------|--------|--------------|
| A | 0.0 | 18.6 | 0.00 |
| B | 18.6 | 156.0 | 0.00 |
| C | 0.0 | 2000.0 | 0.00 |

Count Corrections-

Static Controller: On Luminescence Correction: On
Colored Samples: n/a Heterogeneity Monitor: n/a
Coincidence Time (nsec): 18 Delay Before Burst (nsec): 75

Half Life-

Half Life Correction: Off

| Regions | Half Life | Units | Reference Date | Reference Time |
|---------|-----------|-------|----------------|----------------|
| A | | | | |
| B | | | | |
| C | | | | |

Cycle 1 Results

| S# | CPMA | CPMB | CPMC | MESSAGES |
|----|------|------|------|----------|
| 1 | 9 | 7 | 20 | |
| 2 | 4 | 7 | 19 | |
| 3 | 12 | 7 | 27 | |
| 4 | 6 | 8 | 18 | |
| 5 | 11 | 9 | 27 | |
| 6 | 7 | 10 | 27 | |
| 7 | 10 | 3 | 16 | |
| 8 | 8 | 7 | 19 | |
| 9 | 13 | 11 | 33 | |
| 10 | 15 | 8 | 26 | |

Protocol# 4 - Eds Monthly Swipes.lsa

| | | | |
|----|----|----|----|
| 11 | 14 | 7 | 26 |
| 12 | 15 | 9 | 34 |
| 13 | 8 | 5 | 17 |
| 14 | 11 | 9 | 24 |
| 15 | 4 | 5 | 13 |
| 16 | 7 | 7 | 26 |
| 17 | 10 | 9 | 28 |
| 18 | 12 | 7 | 26 |
| 19 | 17 | 7 | 31 |
| 20 | 11 | 8 | 26 |
| 21 | 7 | 12 | 28 |
| 22 | 12 | 8 | 26 |
| 23 | 9 | 6 | 19 |
| 24 | 14 | 3 | 20 |
| 25 | 7 | 6 | 22 |
| 26 | 8 | 3 | 23 |
| 27 | 21 | 10 | 34 |
| 28 | 11 | 5 | 20 |
| 29 | 9 | 4 | 18 |
| 30 | 13 | 8 | 29 |
| 31 | 6 | 7 | 29 |
| 32 | 8 | 6 | 23 |
| 33 | 9 | 5 | 24 |
| 34 | 4 | 6 | 14 |
| 35 | 7 | 2 | 14 |
| 36 | 10 | 5 | 20 |
| 37 | 14 | 5 | 25 |
| 38 | 9 | 6 | 20 |
| 39 | 3 | 7 | 15 |
| 40 | 10 | 9 | 23 |
| 41 | 11 | 9 | 30 |
| 42 | 12 | 13 | 29 |
| 43 | 9 | 9 | 26 |
| 44 | 13 | 7 | 22 |
| 45 | 6 | 9 | 23 |
| 46 | 7 | 11 | 21 |
| 47 | 18 | 6 | 25 |
| 48 | 0 | 7 | 9 |
| 49 | 3 | 14 | 22 |
| 50 | 5 | 13 | 22 |
| 51 | 3 | 8 | 17 |
| 52 | 7 | 9 | 22 |
| 53 | 16 | 8 | 31 |
| 54 | 10 | 6 | 23 |