




UNITED STATES  
NUCLEAR REGULATORY COMMISSION  
REGION IV  
1600 EAST LAMAR BLVD  
ARLINGTON, TEXAS 76011-4511

# EMAIL

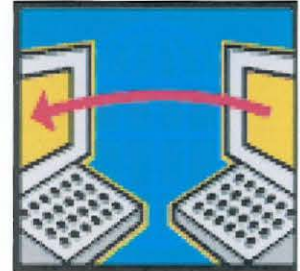

**Name:** LTC David J. Phillips, Ph.D. License: 46-02645-03  
**Organization:** Department of the Army Docket: 030-03368  
Madigan Army Medical Center Control: 581363  
**Phone:** 253-968-4300  
**E-mail Address:** david.j.phillips48.mil@mail.mil  
**From:** Jacqueline D. Cook  
**Date:** December 30, 2013  
**Subject:** Application dated July 10, 2013, for License Amendment  
**Pages:** 2

Dr. Phillips:

Per your application dated July 10, 2013, the items on the next page are deficiencies which require your response. **Please respond to this e-mail if at all possible by Tuesday, January 14, 2014.** If you are unable to respond by this due date, please don't hesitate to contact me so we can discuss an extension to the date. Our fax number is (817) 200-1263. You may respond by e-mail in pdf format if you'd like. My email address is [Jackie.Cook@nrc.gov](mailto:Jackie.Cook@nrc.gov). When responding to this e-mail, please include the license, docket and control numbers located at the top of this page.

Thanking you in advance for your cooperation, assistance, and prompt response in this matter.

/RA/  
Jacqueline D. Cook  
Senior Health Physicist

**PUBLIC**

- Immediate Release  
 Normal Release

**NON-PUBLIC**

- A.3 Sensitive-Security Related  
 A.7 Sensitive Internal  
 Other: \_\_\_\_\_

Reviewer: Joe Date: 12/30/13

1. Currently on materials license cover letters we send to you and other correspondence, on the attention line, it specifies MCHJ-PVR (Health Physics Office); however, in Item 2 of the NRC Form 313, amendment application dated July 10, 2013, it specifies MCHJ-CLY-R (Health Physics Service).

Please clarify this discrepancy.

2. Please provide procedures required by 10 CFR 35.610, Safety procedures and instructions for remote afterloader units, teletherapy units, and gamma stereotactic radiosurgery units. (<http://www.nrc.gov/reading-rm/doc-collections/cfr/part035/part035-0610.html>)
3. Please note that in Item 10.c. on page B-5, you discuss calibration records (certificates); however, Item 8.27, Item 10: Installation, Maintenance, Adjustment, Repair, and Inspection of Therapy Devices Containing Sealed Sources of NUREG-1556, Vol. 9, Rev. 2 requests a copy of the manufacturer's training certification and an outline of the training in procedures to be followed if you requested an employee who is trained by the manufacturer to be authorized to perform the aforementioned activities. However since you are contracting with the manufacturer to provide these aforementioned activities, no response is necessary.

**PUBLIC**

- Immediate Release  
 Normal Release

**NON-PUBLIC**

- A.3 Sensitive-Security Related  
 A.7 Sensitive Internal  
 Other:

Reviewer: JAN Date: 12/30/13