

Fax: 734-662-9224

Ludlum 14C PR 200414
Check Source 0.9mR/h
Serial # 194297
Bkgd = 0.01mR/hr

OPDYKE DIAGNOSTIC CENTER, P.C.
719 S. OPDYKE ROAD
AUBURN HILLS, MI 48326

AREA SURVEY/WIPE TEST DIAGRAM

NUCLEAR DEPARTMENT DIAGRAM


p.1

248 333 9404

Opdyke Family Medical



o
u
t
s
i
d
e

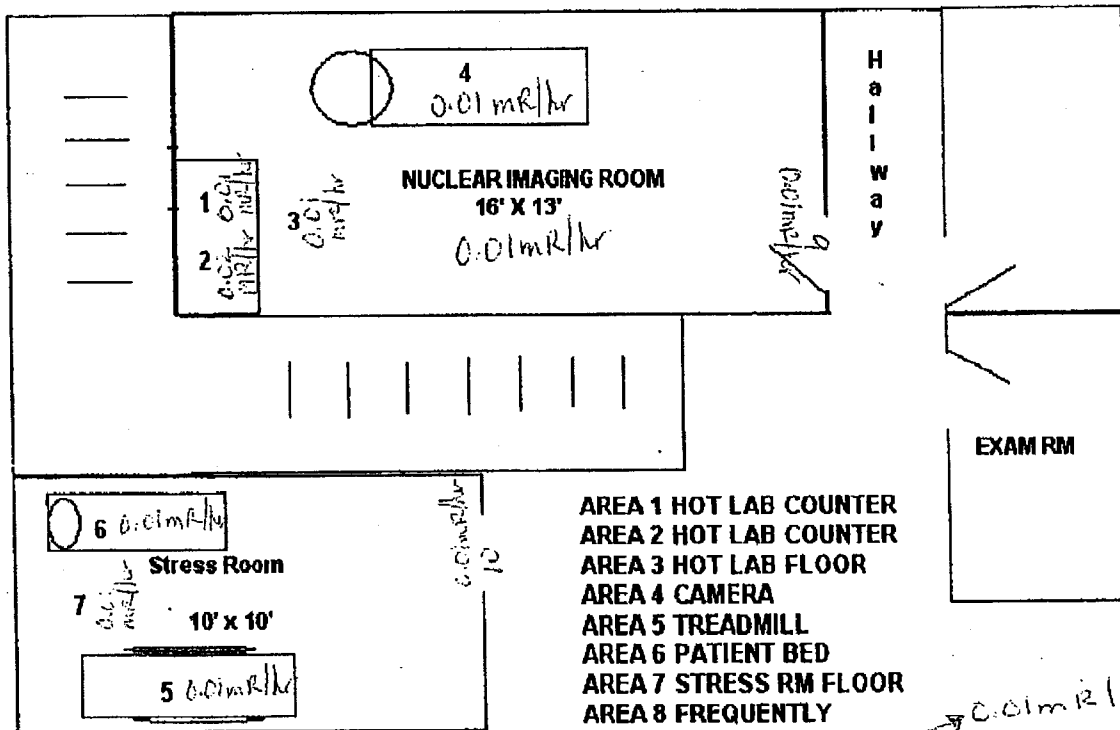

Closeout wipes

1. 39 dpm
2. 43 dpm
3. 38 dpm
4. 40 dpm
5. 33 dpm
6. 33 dpm
7. 35 dpm
8. 43 dpm
9. 38 dpm
10. 40 dpm
11. 40 dpm

Wipes:
Bkgd: 181cpm

Sources that were removed
from Nuclear Lab
Co⁵⁷ Flood } 0.4mR/hr
Co⁵⁷ Flood } 38dpm
Co⁵⁷ Flood }

Ammo box w/ sources
0.6mR/hr
39dpm

- AREA 1 HOT LAB COUNTER
- AREA 2 HOT LAB COUNTER
- AREA 3 HOT LAB FLOOR
- AREA 4 CAMERA
- AREA 5 TREADMILL
- AREA 6 PATIENT BED
- AREA 7 STRESS RM FLOOR
- AREA 8 FREQUENTLY TOUCHED OBJECTS (keyboards, doorknobs)

- Area 9 Doorway in Nuclear Room
- Area 10 Doorway in Stress Lab
- Area 11 Floor in front of camera

RECEIVED MAR 10 2016

Control #590299

Frank
ATTN: 630-515-1071