

Fax: 734-662-9224

Ludlum 14C PR 200414  
Check Source 0.9mR/hr  
Serial # 194297  
Bkgd = 0.01mR/hr

OPDYKE DIAGNOSTIC CENTER, P.C.  
719 S. OPDYKE ROAD  
AUBURN HILLS, MI 48326

AREA SURVEY/WIPE TEST DIAGRAM

NUCLEAR DEPARTMENT DIAGRAM


p.1

248 333 9404

Opdyke Family Medical



o  
u  
t  
s  
i  
d  
e

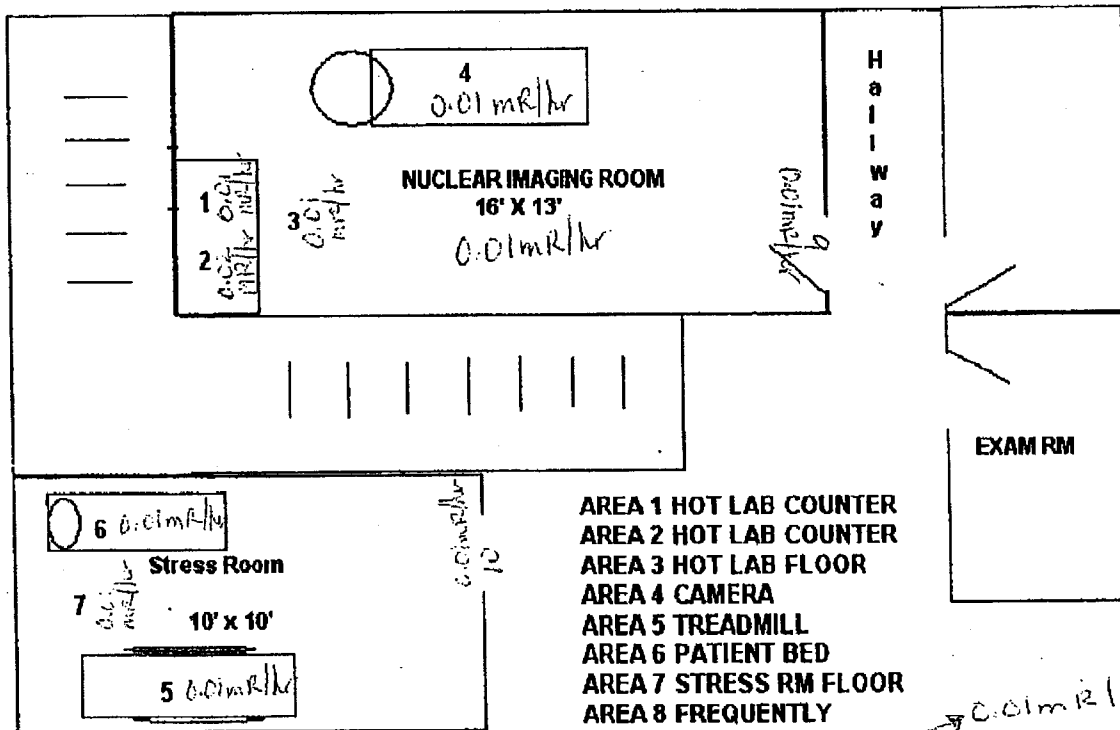

Closeout wipes

1. 39 dpm
2. 43 dpm
3. 38 dpm
4. 40 dpm
5. 33 dpm
6. 33 dpm
7. 35 dpm
8. 43 dpm
9. 38 dpm
10. 40 dpm
11. 40 dpm

Wipes:  
Bkgd: 1810cpm

Sources that were removed  
from Nuclear Lab  
Co<sup>57</sup> Flood } 0.4 mR/hr  
Co<sup>57</sup> Flood } 38 dpm  
Co<sup>57</sup> Flood }

Ammo box w/ sources  
0.6 mR/hr  
39 dpm

- AREA 1 HOT LAB COUNTER
- AREA 2 HOT LAB COUNTER
- AREA 3 HOT LAB FLOOR
- AREA 4 CAMERA
- AREA 5 TREADMILL
- AREA 6 PATIENT BED
- AREA 7 STRESS RM FLOOR
- AREA 8 FREQUENTLY TOUCHED OBJECTS (keyboards, doorknobs)

- Area 9 Doorway in Nuclear Room
- Area 10 Doorway in Stress Lab
- Area 11 Floor in front of camera

RECEIVED MAR 10 2016

Control #590299

Frank  
ATTN: 630-515-1071