

Br. 3



**BrachyTherapy**  
501 Locust Ave., Suite 1  
Charlottesville, VA 22902  
USA  
tel +1 434-977-8495  
fax +1 434-244-7181  
www.varian.com

April 26, 2016

Mr. Stephen Hammann  
U.S. NRC Region I  
2100 Renaissance Blvd., Suite 100  
King of Prussia, PA 19406-2713

Re: NRC license 45-30957-01  
Docket No. 030-36666

Dear Mr. Hammann:

I write to amend the HDR Service organization chart. This was originally submitted as ATT 5 to correspondence 24 November 2014 during license renewal. A copy of that letter and the earlier org chart are attached for reference.

The new organization chart is enclosed and shows HDR service operations reporting to Mr. Stephen Hotz with no changes below his position.

Very truly yours,


A handwritten signature in black ink that reads "Richard G. Piccolo".

Richard G. Piccolo, CHP  
Varian BrachyTherapy RSO

Encl: Org chart - 26 April 2016  
Earlier org chart - Oct 2014  
Cover letter referencing ATT 5 - Nov 2014

590813  
NMSS/RGN1 MATERIALS-002


## Brachytherapy Service - North America

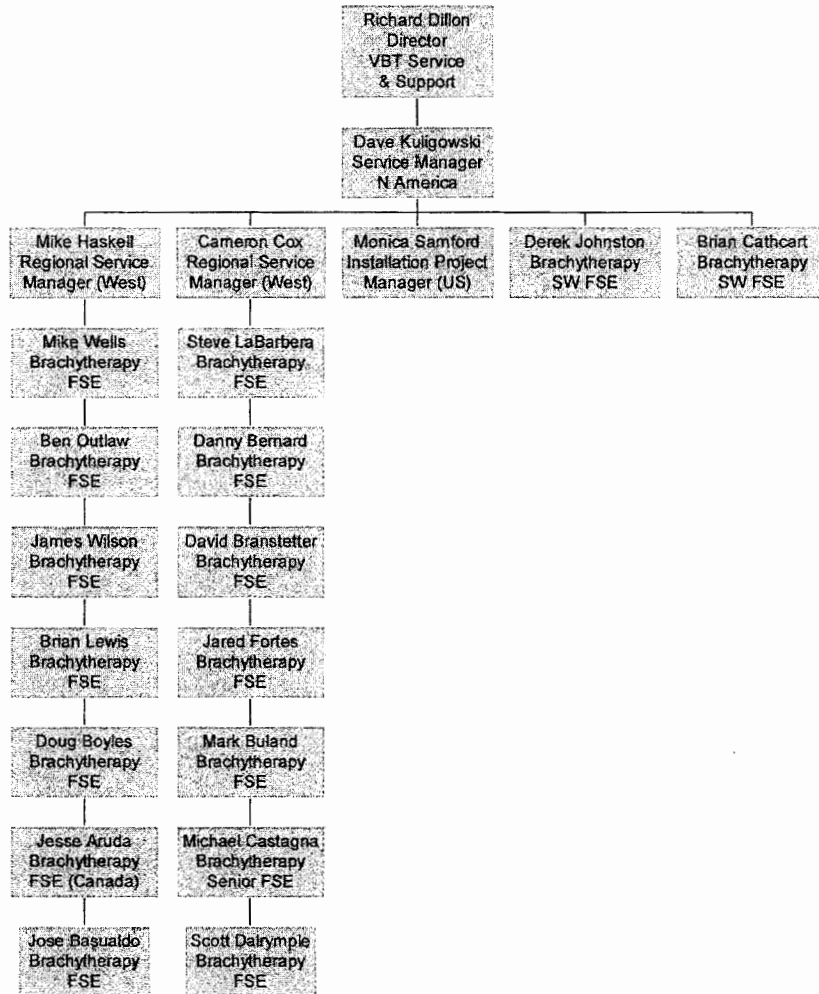

Richard Dillon  
 Director, Brachytherapy Service & Support  
 October 1<sup>st</sup> 2014

# Varian Medical Systems, Inc. – U.S. HDR Field Service Operations

---

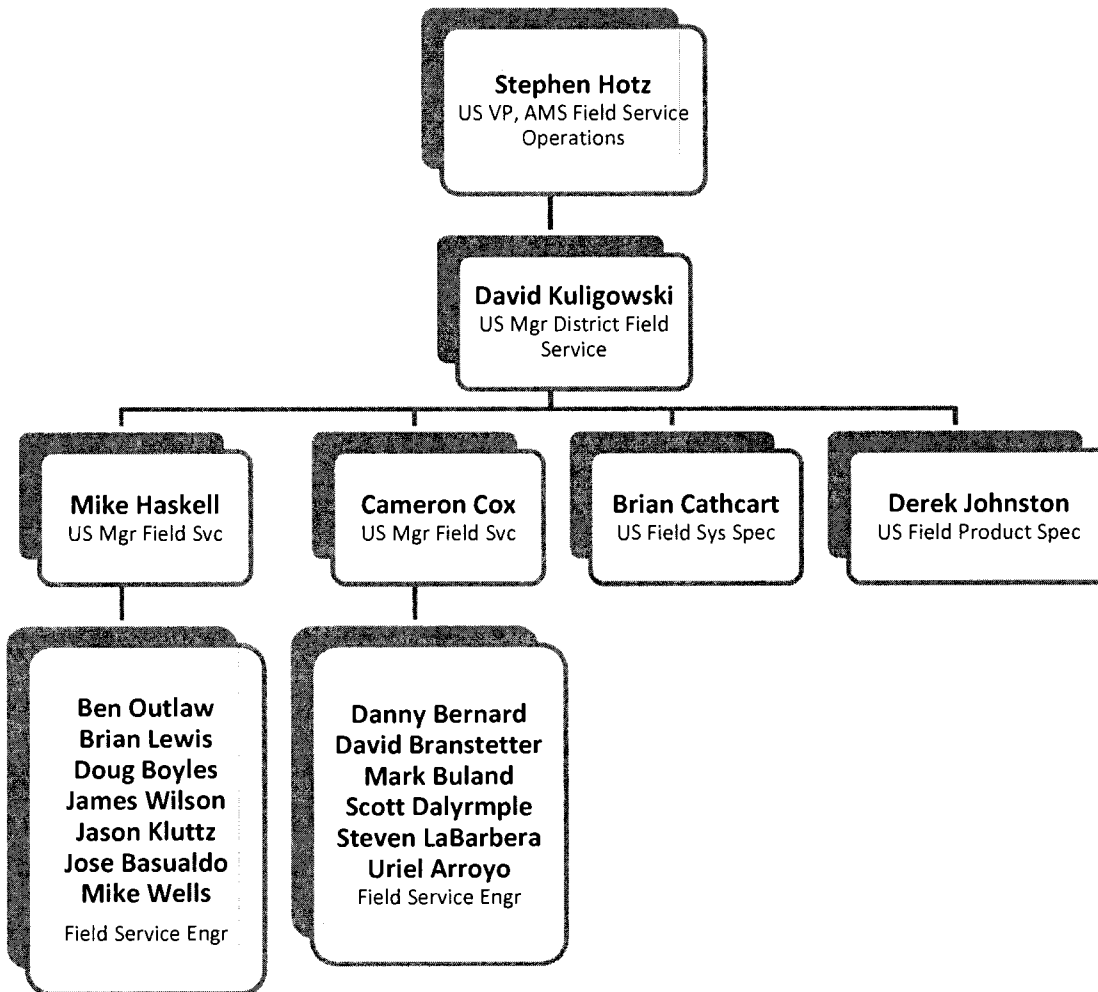



**BrachyTherapy**  
501 Locust Ave., Suite 1  
Charlottesville, VA 22902  
USA  
tel +1 434-977-8495  
fax +1 434-244-7181  
www.varian.com

November 24, 2014

Ms. Kathy Modes  
DNMS  
U.S. NRC Region I  
2100 Renaissance Blvd., Suite 100  
King of Prussia, PA 19406-2713

Re: NRC license 45-30957-01  
Docket No. 030-36666  
RAI – License Renewal

Dear Ms. Modes:

The amended license renewal is enclosed under this cover. The signed Form 313, sent on October 17, 2014, is not included in this mailing. The bases for the changes were our two telephone conversations. The bulk of the changes are contained in the document that addresses NRC Form 313 Item 3 and Items 5-13. Five attachments are included that are referenced within the larger. Emergency procedures are in Sections 10.6.23, 10.6.24 and 10.6.25 starting page 14.

Very truly yours,

A handwritten signature in black ink that reads "Richard G. Piccolo".

Richard G. Piccolo, CHP  
Varian BrachyTherapy RSO

Encl: RAI – Items 3 and 5-13  
ATT 1 – SS&D front pages  
ATT 2 – RSO Delegation of Authority  
ATT 3 – Radiation Safety Organization Chart  
ATT 4 – T & E for Named AU  
ATT 5 – Field Service Organization Chart



**ACKNOWLEDGEMENT - RECEIPT OF CORRESPONDENCE**

<b>Name and Address of Applicant and/or Licensee</b>  Richard G. Piccolo Radiation Safety Officer Varian Medical Systems, Inc. 501 Locust Avenue Charlottesville, VA 22902	<b>License Number(s)</b> 45-30957-01
	<b>Mail Control Number(s)</b> 590813
	<b>Licensing and/or Technical Reviewer or Branch</b> Decommissioning and Technical Support Branch

This is to acknowledge receipt of your:  Letter and/or  Application Dated: April 26, 2016

The initial processing, which included an administrative review, has been performed.  
 Amendment  Termination  New License  Renewal

There were no administrative omissions identified during our initial review.

This is to acknowledge receipt of your application for renewal of the material(s) license identified above. Your application is deemed timely filed, and accordingly, the license will not expire until final action has been taken by this office.

Your application for a new NRC license did not include your taxpayer identification number. Please fill out NRC Form 531, Request for Taxpayer Identification Number, located at the following link:  
<http://www.nrc.gov/reading-rm/doc-collections/forms/nrc531.pdf>  
 Send the completed NRC Form 531, by facsimile, to the following number: (301) 415-5387

The following administrative omissions have been identified:  
 [Empty box for listing omissions]

A copy of your action has been e-mailed to our License Fee and Accounts Receivable Branch, in our Headquarters office in Rockville, MD. You will be contacted separately if there is a fee issue involved.

Your application has been assigned the above listed MAIL CONTROL NUMBER. When calling to inquire about this action, please refer to this control number. Your application has been forwarded to a technical reviewer. Please note that the technical review, which is normally completed within 180 days for a renewal application (90 days for all other requests), may identify additional omissions or require additional information. If you have any questions concerning the processing of your application, our contact information is listed below:

**Region I**  
**U. S. Nuclear Regulatory Commission**  
**Division of Nuclear Materials Safety**  
**2100 Renaissance Boulevard, Suite 100**  
**King of Prussia, PA 19406-2713**  
**(610) 337-5260, (610) 337-5313,**  
**(610) 337-5398, (610) 337-5513 or (610) 337-5239**