

L-9



Consolidated Medical
Plaza Suite 101
Ave. Gautier Benitez 201
Caguas, Puerto Rico
Tel (787) 744-5278

La fuente Town Center
704 Marginal Suite 11104
Guayama, Puerto Rico
Tel (787) 866-5278

Calle Jose C. Vazquez #120
Frente al Hospital Menonita
Aibonito, Puerto Rico
Tel (787) 991-7000

To : Lester Tripp
Health Physicist, Medical Branch
Division of Nuclear Materials Safety
U.S. Nuclear Regulatory Commission
Region I
2100 Renaissance Blvd, Suite 200
King of Prussia, PA 19406-2713

From : Hiram Rivera Luna, MD, RSO
License Number: 52-17273-01
Docket Number: 03012483

Mail Control Number: 591088 (Reference) RLS

Subject : Amendment to License No. 52-17273-01
Request to release old facilities for unrestricted use

Date : November 9, 2016

This is a request for an amendment to license No. 52-17273-01 to remove the old facility located at La Fuente Town Center, Suite 11104, 706 Marginal, Guayama, PR as one of our authorized location and to release it for unrestricted use.


We include the results of the radiation **area survey** and wipe test demonstrating safe levels in all spaces within the facility as well as in the main sewage clean-out pipe. Please note that the radiopharmaceuticals used in the mentioned facility were Technetium-99m (given daily), Gallium-67 (last given on August 18, 2016), Iodine-131 (last given on August 16, 2016) and Indium-111 (last given in 2014). All doses were supplied by a radiopharmacy as unit doses.

We also notify that all sealed sources in the old location were moved to the new facilities. No radioactive material are stored in the old facilities.

You can contact me at Telephones 787-378-3901 or 787-744-5278 or Fax 787-744-5433 or email hrivera@nuscan.com if you have any question or suggestion. Thanks for your attention in this matter.

592323

REC'D IN LAT. 11/09/2016

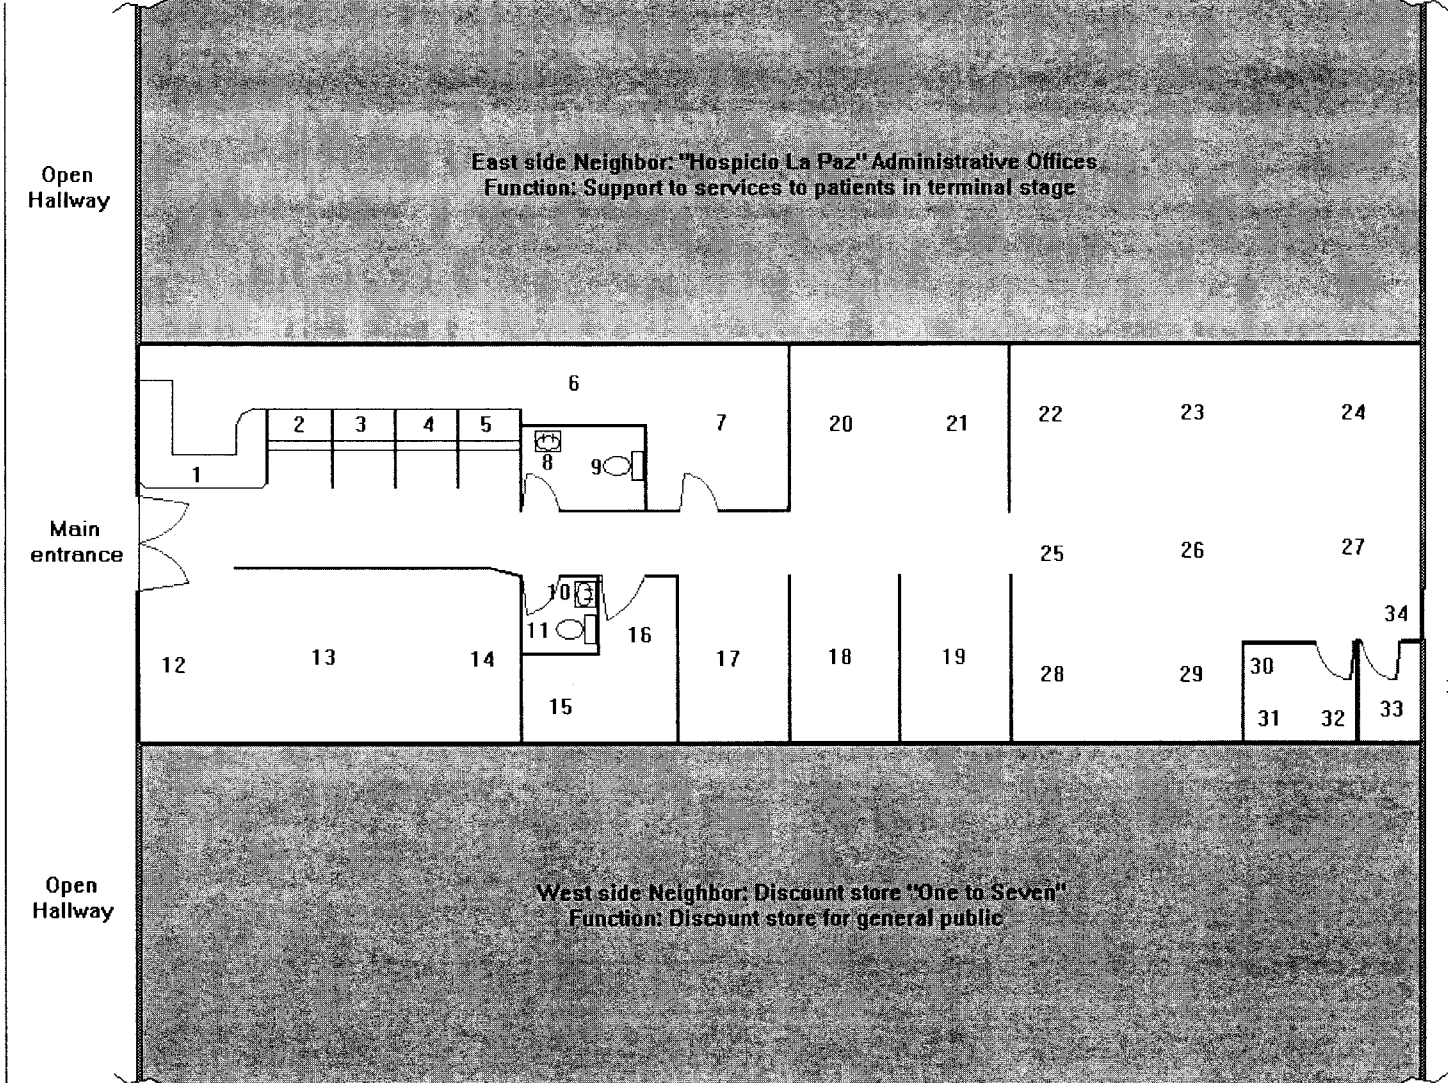

Open Hallway

East side Neighbor: "Hospicio La Paz" Administrative Offices
Function: Support to services to patients in terminal stage

Public parking

Main entrance

Open Hallway

West side Neighbor: Discount store "One to Seven"
Function: Discount store for general public



Consolidated Medical
Plaza Suite 101
Ave. Gautier Benitez 201
Caguas, Puerto Rico
Tel (787) 744-5278

La fuente Town Center
704 Marginal Suite 11104
Guayama, Puerto Rico
Tel (787) 866-5278

Calle Jose C. Vazquez #120
Frente al Hospital Menonita
Aibonito, Puerto Rico
Tel. (787) 991-7000

**Surface survey of Nuscan-Guayama Facility
prior to release for unrestricted use**

Date: September 26, 2016

Label	Location	Background	Wipe cpm Count		Activity in nCi
			Gross	Net	
1	Front desk	224	267	43	0.030
2	Interview desk 1	224	204	0	0.000
3	Interview desk 2	224	291	67	0.046
4	Interview desk 3	224	249	25	0.017
5	Interview desk 4	224	236	12	0.008
6	Reception hallway	224	226	2	0.001
7	Printers and server room	224	194	0	0.000
8	Bathroom 1 washbasin	224	231	7	0.005
9	Bathroom 1 toilet	224	230	6	0.004
10	Bathroom 2 washbasin	224	231	7	0.005
11	Bathroom 2 toilet	224	201	0	0.000
12	Waiting area 1	224	233	9	0.006
13	Waiting area 2	224	249	25	0.017
14	Waiting area 3	224	210	0	0.000
15	Storage room area 1	224	243	19	0.013
16	Storage room area 2	224	232	8	0.006
17	Ultrasound exam room 1	224	226	2	0.001
18	Ultrasound exam room 2	224	224	0	0.000
19	Ultrasound exam room 3	224	253	29	0.020
20	Densitometry room area 1	224	236	12	0.008
21	Densitometry room area 2	224	224	0	0.000
22	Nuclear Medicine area 1	224	230	6	0.004
23	Nuclear Medicine area 2	224	229	5	0.003
24	Nuclear Medicine area 3	224	244	20	0.014
25	Nuclear Medicine area 4	224	228	4	0.003
26	Nuclear Medicine area 5	224	206	0	0.000
27	Nuclear Medicine area 6	224	225	1	0.001
28	Nuclear Medicine area 7	224	243	19	0.013
29	Nuclear Medicine area 8	224	232	8	0.006
30	Hot room area 1	224	226	2	0.001
31	Hot room area 2	224	253	29	0.020
32	Hot room area 3	224	210	0	0.000
33	Electrical Room	224	267	43	0.030
34	Posterior Emergency Exit	224	268	44	0.030
35	Sewage clean-out access	224	241	17	0.012

Counter: Captus 3000 S/N 900983

**Area survey of Nuscan-Guayama Facility
prior to release for unrestricted use**

Date: September 26, 2016

Label	Location	Area Survey mR/hr
1	Front desk	0.00
2	Interview desk 1	0.00
3	Interview desk 2	0.00
4	Interview desk 3	0.00
5	Interview desk 4	0.00
6	Reception hallway	0.00
7	Printers and server room	0.00
8	Bathroom 1 handwash	0.01
9	Bathroom 1 toilet	0.01
10	Bathroom 2 handwash	0.00
11	Bathroom 2 toilet	0.01
12	Waiting area 1	0.00
13	Waiting area 2	0.00
14	Waiting area 3	0.00
15	Storage room area 1	0.00
16	Storage room area 2	0.00
17	Ultrasound exam room 1	0.01
18	Ultrasound exam room 2	0.01
19	Ultrasound exam room 3	0.00
20	Densitometry room area 1	0.01
21	Densitometry room area 2	0.00
22	Nuclear Medicine area 1	0.00
23	Nuclear Medicine area 2	0.01
24	Nuclear Medicine area 3	0.01
25	Nuclear Medicine area 4	0.00
26	Nuclear Medicine area 5	0.00
27	Nuclear Medicine area 6	0.01
28	Nuclear Medicine area 7	0.00
29	Nuclear Medicine area 8	0.00
30	Hot room area 1	0.01
31	Hot room area 2	0.00
32	Hot room area 3	0.01
33	Electrical Room	0.01
34	Posterior Emergency Exit	0.00
35	Sewage clean-out access	0.01

GM Survey Meter: Ludlum model 14 C General Purpose Analog Ratemeter with internal GM
Range: 0.0 - 2000 mR/hr



ACKNOWLEDGEMENT - RECEIPT OF CORRESPONDENCE

Name and Address of Applicant and/or Licensee Hiram Rivera Luna, M.D. Radiation Safety Officer P.O. Box 6960 Caguas, PR 00726-6960	Date November 17, 2016
	License Number(s) 52-17273-01
	Mail Control Number(s) 592323
	Licensing and/or Technical Reviewer or Branch Lester Tripp
	<input checked="" type="checkbox"/> Memo

This is to acknowledge receipt of your: Letter and/or Application Dated: November 9, 2016

The initial processing, which included an administrative review, has been performed.
 Amendment Termination New License Renewal

There were no administrative omissions identified during our initial review.

This is to acknowledge receipt of your application for renewal of the material(s) license identified above. Your application is deemed timely filed, and accordingly, the license will not expire until final action has been taken by this office.

Your application for a new NRC license did not include your taxpayer identification number. Please complete and submit NRC Form 531, Request for Taxpayer Identification Number, located at the following link: <http://www.nrc.gov/reading-rm/doc-collections/forms/nrc531.pdf>
 Follow the instructions on the form for submission.

The following administrative omissions have been identified:

Your application has been assigned the above listed MAIL CONTROL NUMBER. When calling to inquire about this action, please refer to this control number. Your application has been forwarded to a technical reviewer. Please note that the technical review, which is normally completed within 180 days for a renewal application (90 days for all other requests), may identify additional omissions or require additional information. If you have any questions concerning the processing of your application, our contact information is listed below:

Region I
 U. S. Nuclear Regulatory Commission
 Division of Nuclear Materials Safety
 2100 Renaissance Boulevard, Suite 100
 King of Prussia, PA 19406-2713
 (610) 337-5260, (610) 337-5313,
 (610) 337-5398, (610) 337-5239