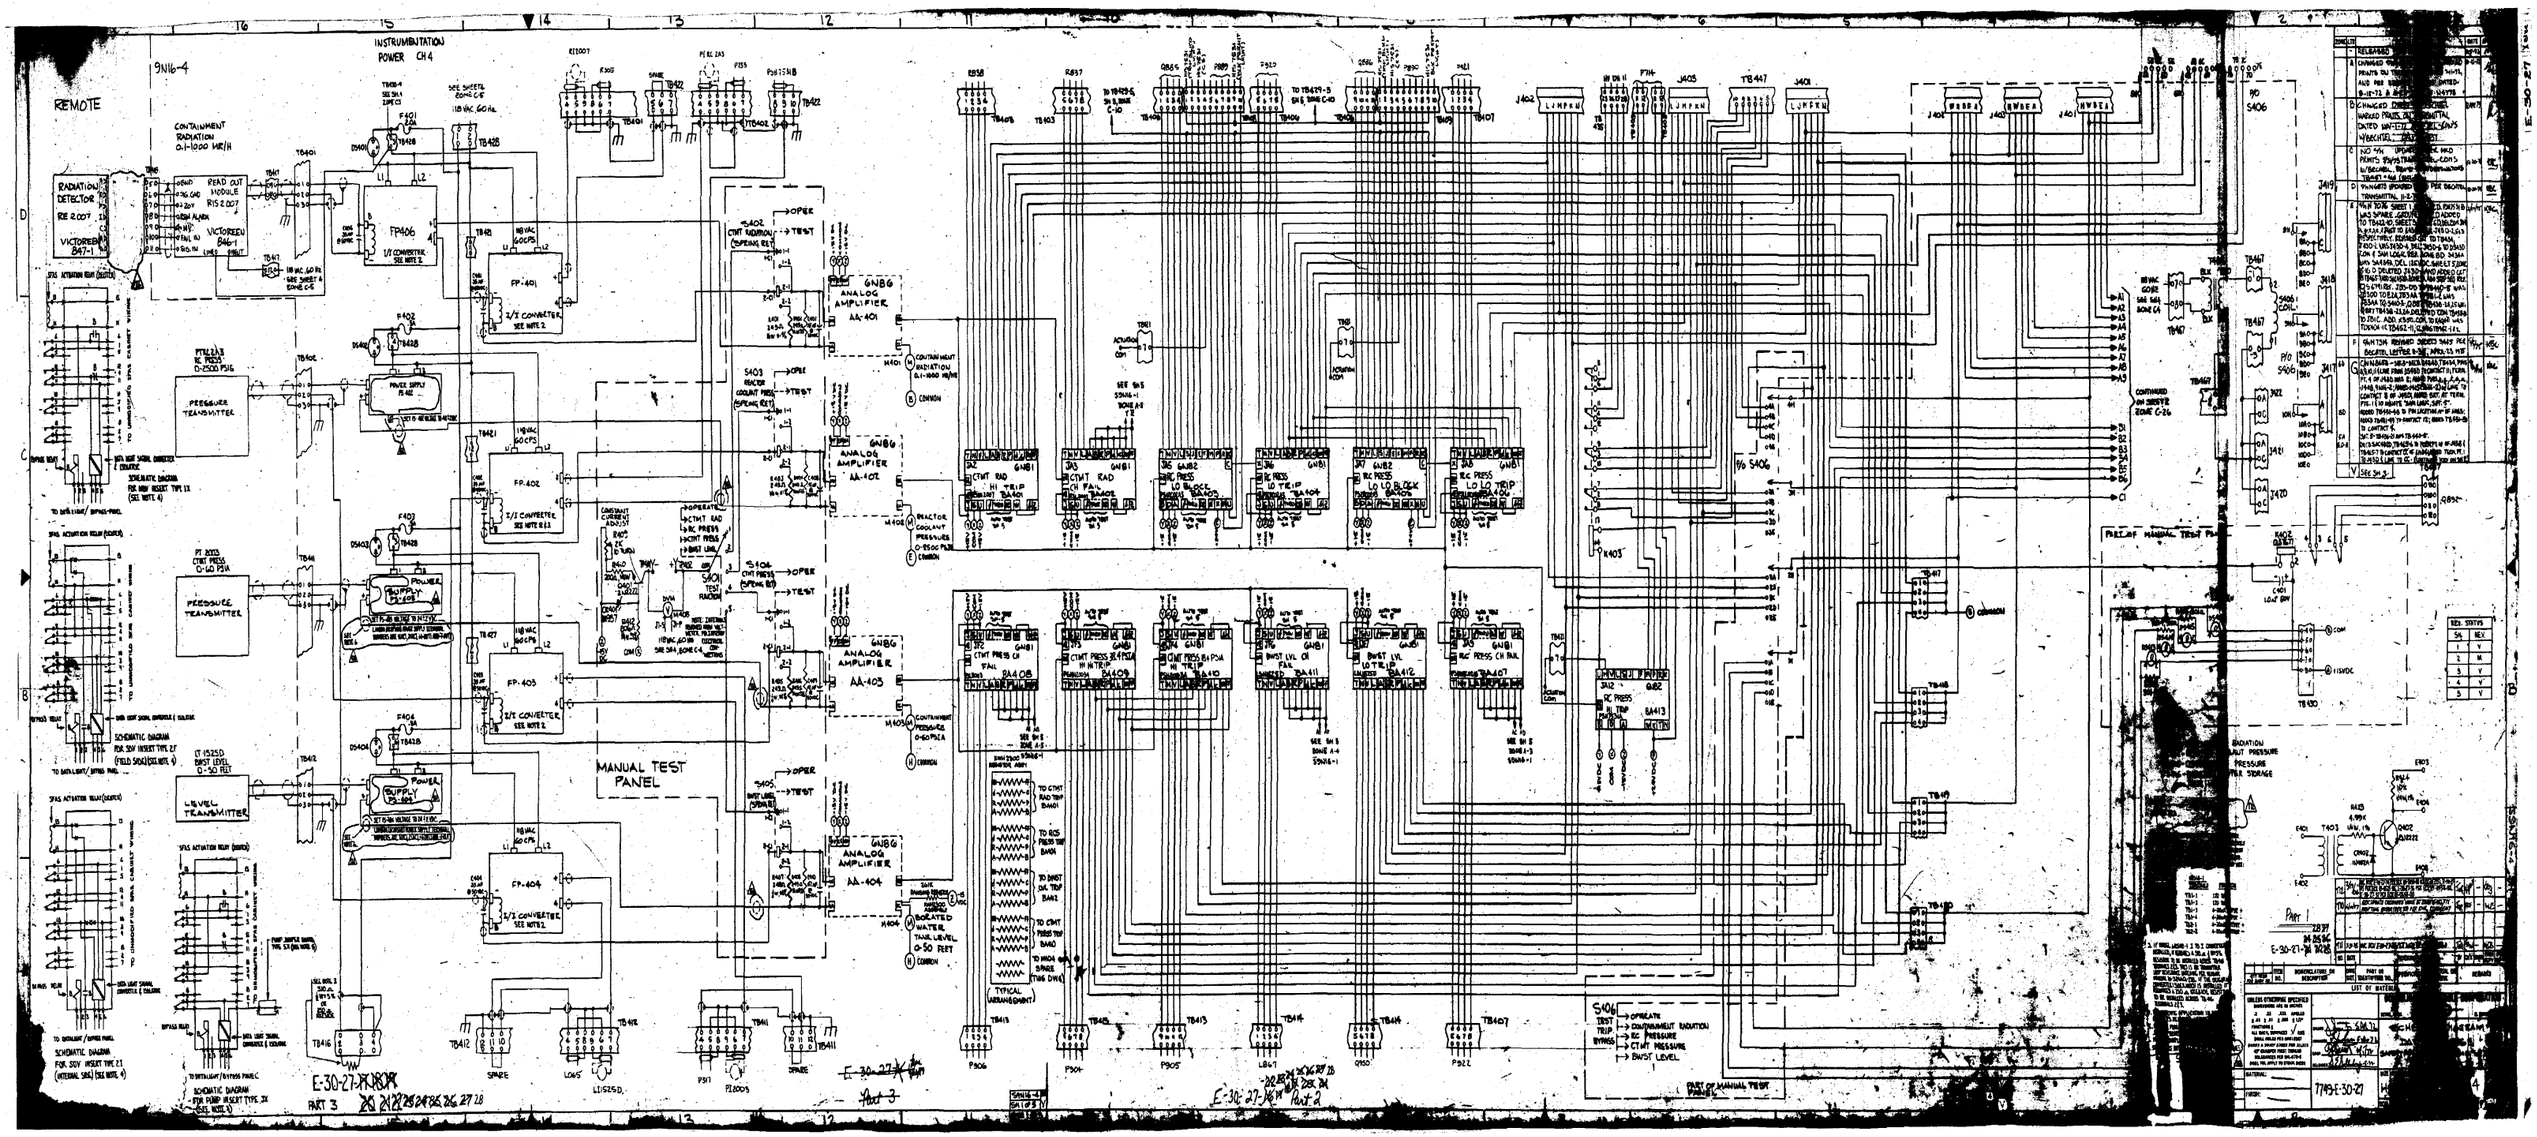

INSTRUMENTATION POWER CH4
9N16-4
REMOTE
CONTAINMENT RADIATION 0.1-1000 MR/H
RADIATION DETECTOR RE 2007
READ OUT MODULE RIS 2007
VICTOREEN 846-1
PRESSURE TRANSMITTER
PRESSURE TRANSMITTER
LEVEL TRANSMITTER
MANUAL TEST PANEL
ANALOG AMPLIFIER AA-401
ANALOG AMPLIFIER AA-402
ANALOG AMPLIFIER AA-403
ANALOG AMPLIFIER AA-404
CONTAINMENT RADIATION 0.1-1000 MR/HR
REACTOR COOLANT PRESSURE 0-2500 PSIA
CONTAINMENT PRESSURE 0-60 PSIA
BORATED WATER TANK LEVEL 0-50 FEET
TYPICAL WARRANGEMENT
PART OF MANUAL TEST PANEL
E-30-27
PART 3
Part 2
Part 1
7749-E-30-27