



May 30, 2017

UNITED STATES NUCLEAR REGULATORY COMMISSION
Region III, Materials Licensing Section
2443 Warrenville Road, Suite 210
Lisle, IL 60532-4351

Re: Amendment to license #21-18659-01

Please amend our license to remove the Gamma Camera Room #1313 (formerly x-ray room B), from the Radiology Department. No radioactive materials were present in the area as of 5/16/2017. A close out survey and wipe are enclosed for your review.

Sincerely

Gerald J. Barbini
President and CEO


Enc 4

RECEIVED JUN 06 2017



Allegan General Hospital

CARDIO MD ROOM (#1313) SURVEY LOCATIONS

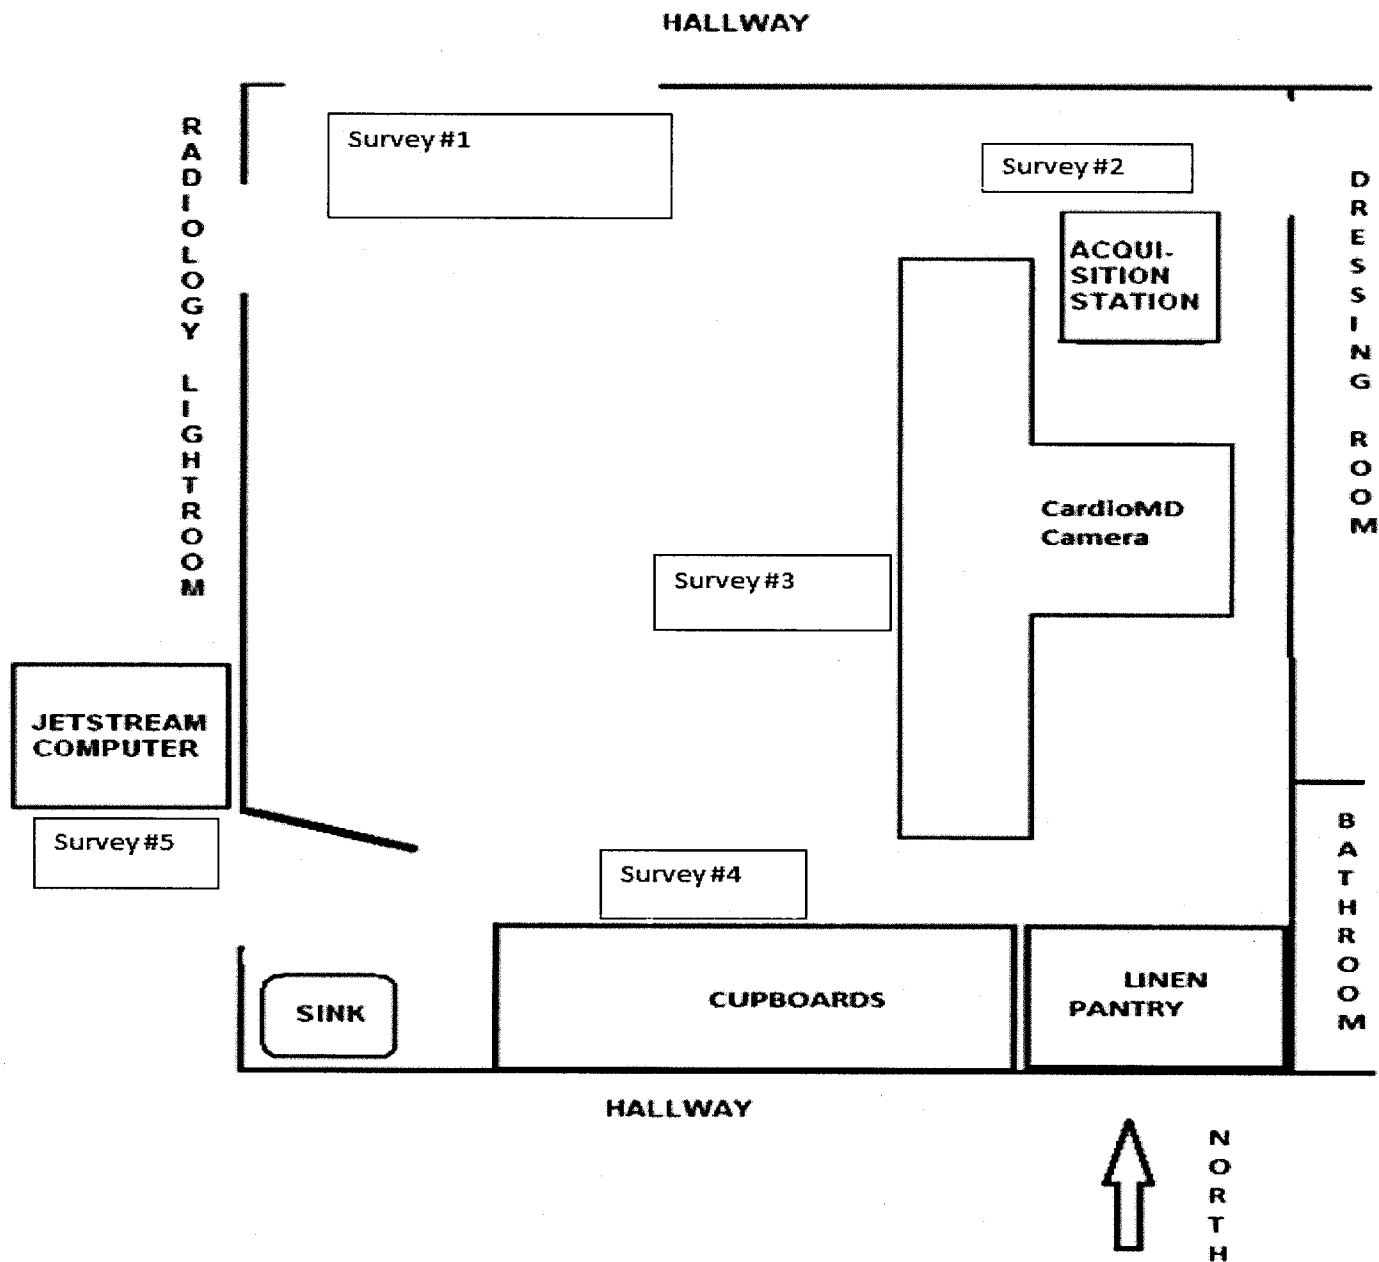

CLOSE OUT AREA SURVEY

CARDIO MD ROOM (#1313)


May 16, 2017

#1 Entry Door	0.01 mr/hr
#2 Acquisition Station	0.01 mr/hr
#3 Floor at Camera	0.01 mr/hr
#4 Counter	0.01 mr/hr
#5 JetStream Computer	0.01 mr/hr
Background	0.01 mr/hr

INSTRUMENT: B-14C

SN: 279391

CHECK SOURCE: (mr/hr): 2.0

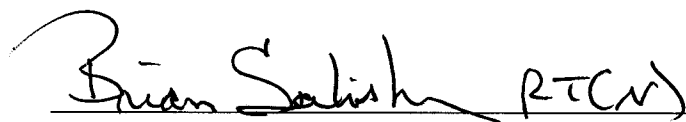 (R.T.C.M.)

Technologist

Wipe History

	Net Counting Rate		Net Activity	
#5 CARDIO MD JETSTREAM COMPUTER		05/16/2017 10:34	60 sec	Trigger: 2000 dpm
Background		309.0 cpm		
Full Spectrum	3.000 cpm		4.615 dpm	
#4 CARDIO MD COUNTERTOP		05/16/2017 10:33	60 sec	Trigger: 2000 dpm
Background		309.0 cpm		
Full Spectrum	61.00 cpm		93.85 dpm	
#3 CARDIO MD FLOOR @ CAMERA		05/16/2017 10:20	60 sec	Trigger: 2000 dpm
Background		309.0 cpm		
Full Spectrum	33.00 cpm		50.77 dpm	
#2 CARDIO MD ACQ STATION		05/16/2017 10:15	60 sec	Trigger: 2000 dpm
Background		309.0 cpm		
Full Spectrum	66.00 cpm		101.5 dpm	
#1 CARDIO MD ENTRY DOOR		05/16/2017 10:12	60 sec	Trigger: 2000 dpm
Background		309.0 cpm		
Full Spectrum	22.00 cpm		33.85 dpm	

Blair Sabatini (RTCW)

 Allegan General Hospital

555 Linn Street • Allegan, Michigan • 49010

PRESORTED
FIRST CLASS



U.S. POSTAGE PITNEY BOWES



ZIP 49010 \$ 000.42³
02 1W
0001394814 JUN 01 2017

UNITED STATES NUCLEAR
REGULATORY COMMISSION
Region III, Materials Licensing Section
2443 Warrenville Road, Suite 210
Lisle, IL 60532

RECEIVED JUN 06 2017

DAJ2SMB 60532

