

REGULATORY INFORMATION DISTRIBUTION SYSTEM (RIDS)

ACCESSION NBR: 8707220647 DOC. DATE: 87/07/17 NOTARIZED: NO DOCKET #
 FACIL: 50-250 Turkey Point Plant, Unit 3, Florida Power and Light C 05000250
 50-251 Turkey Point Plant, Unit 4, Florida Power and Light C 05000251
 AUTH. NAME WOODY, C. O. AUTHOR AFFILIATION Florida Power & Light Co.
 RECIP. NAME RECIP. AFFILIATION Document Control Branch (Document Control Desk)


SUBJECT: Forwards results of spike sample analysis performed under NRC Confirmatory Measurements Program, per 870430 request. Results analyzed according to sample provided & corrected to 870111.


DISTRIBUTION CODE: IE35D COPIES RECEIVED: LTR 1 ENCL 1 SIZE: 2
 TITLE: Emergency Preparedness-Appraisal/Confirmatory Action Ltr/Exercise Rep

NOTES:

	RECIPIENT ID CODE/NAME	COPIES LTTR ENCL		RECIPIENT ID CODE/NAME	COPIES LTTR ENCL	
	PD2-2 LA	1	0	PD2-2 PD	1	1
	McDONALD, D	1	1			
INTERNAL:	ARM/DAF/LFMB	1	0	NRR/DREP/EPB	1	1
	NRR/PMAS/ILRB	1	1	REG-FILE 02	1	1
	RGN2 FILE 01	1	1	RGN2/DRSS/EPRPB	1	1
EXTERNAL:	LPDR	1	1	NRC PDR	1	1
	NSIC	1	1			

TOTAL NUMBER OF COPIES REQUIRED: LTTR 12 ENCL 10

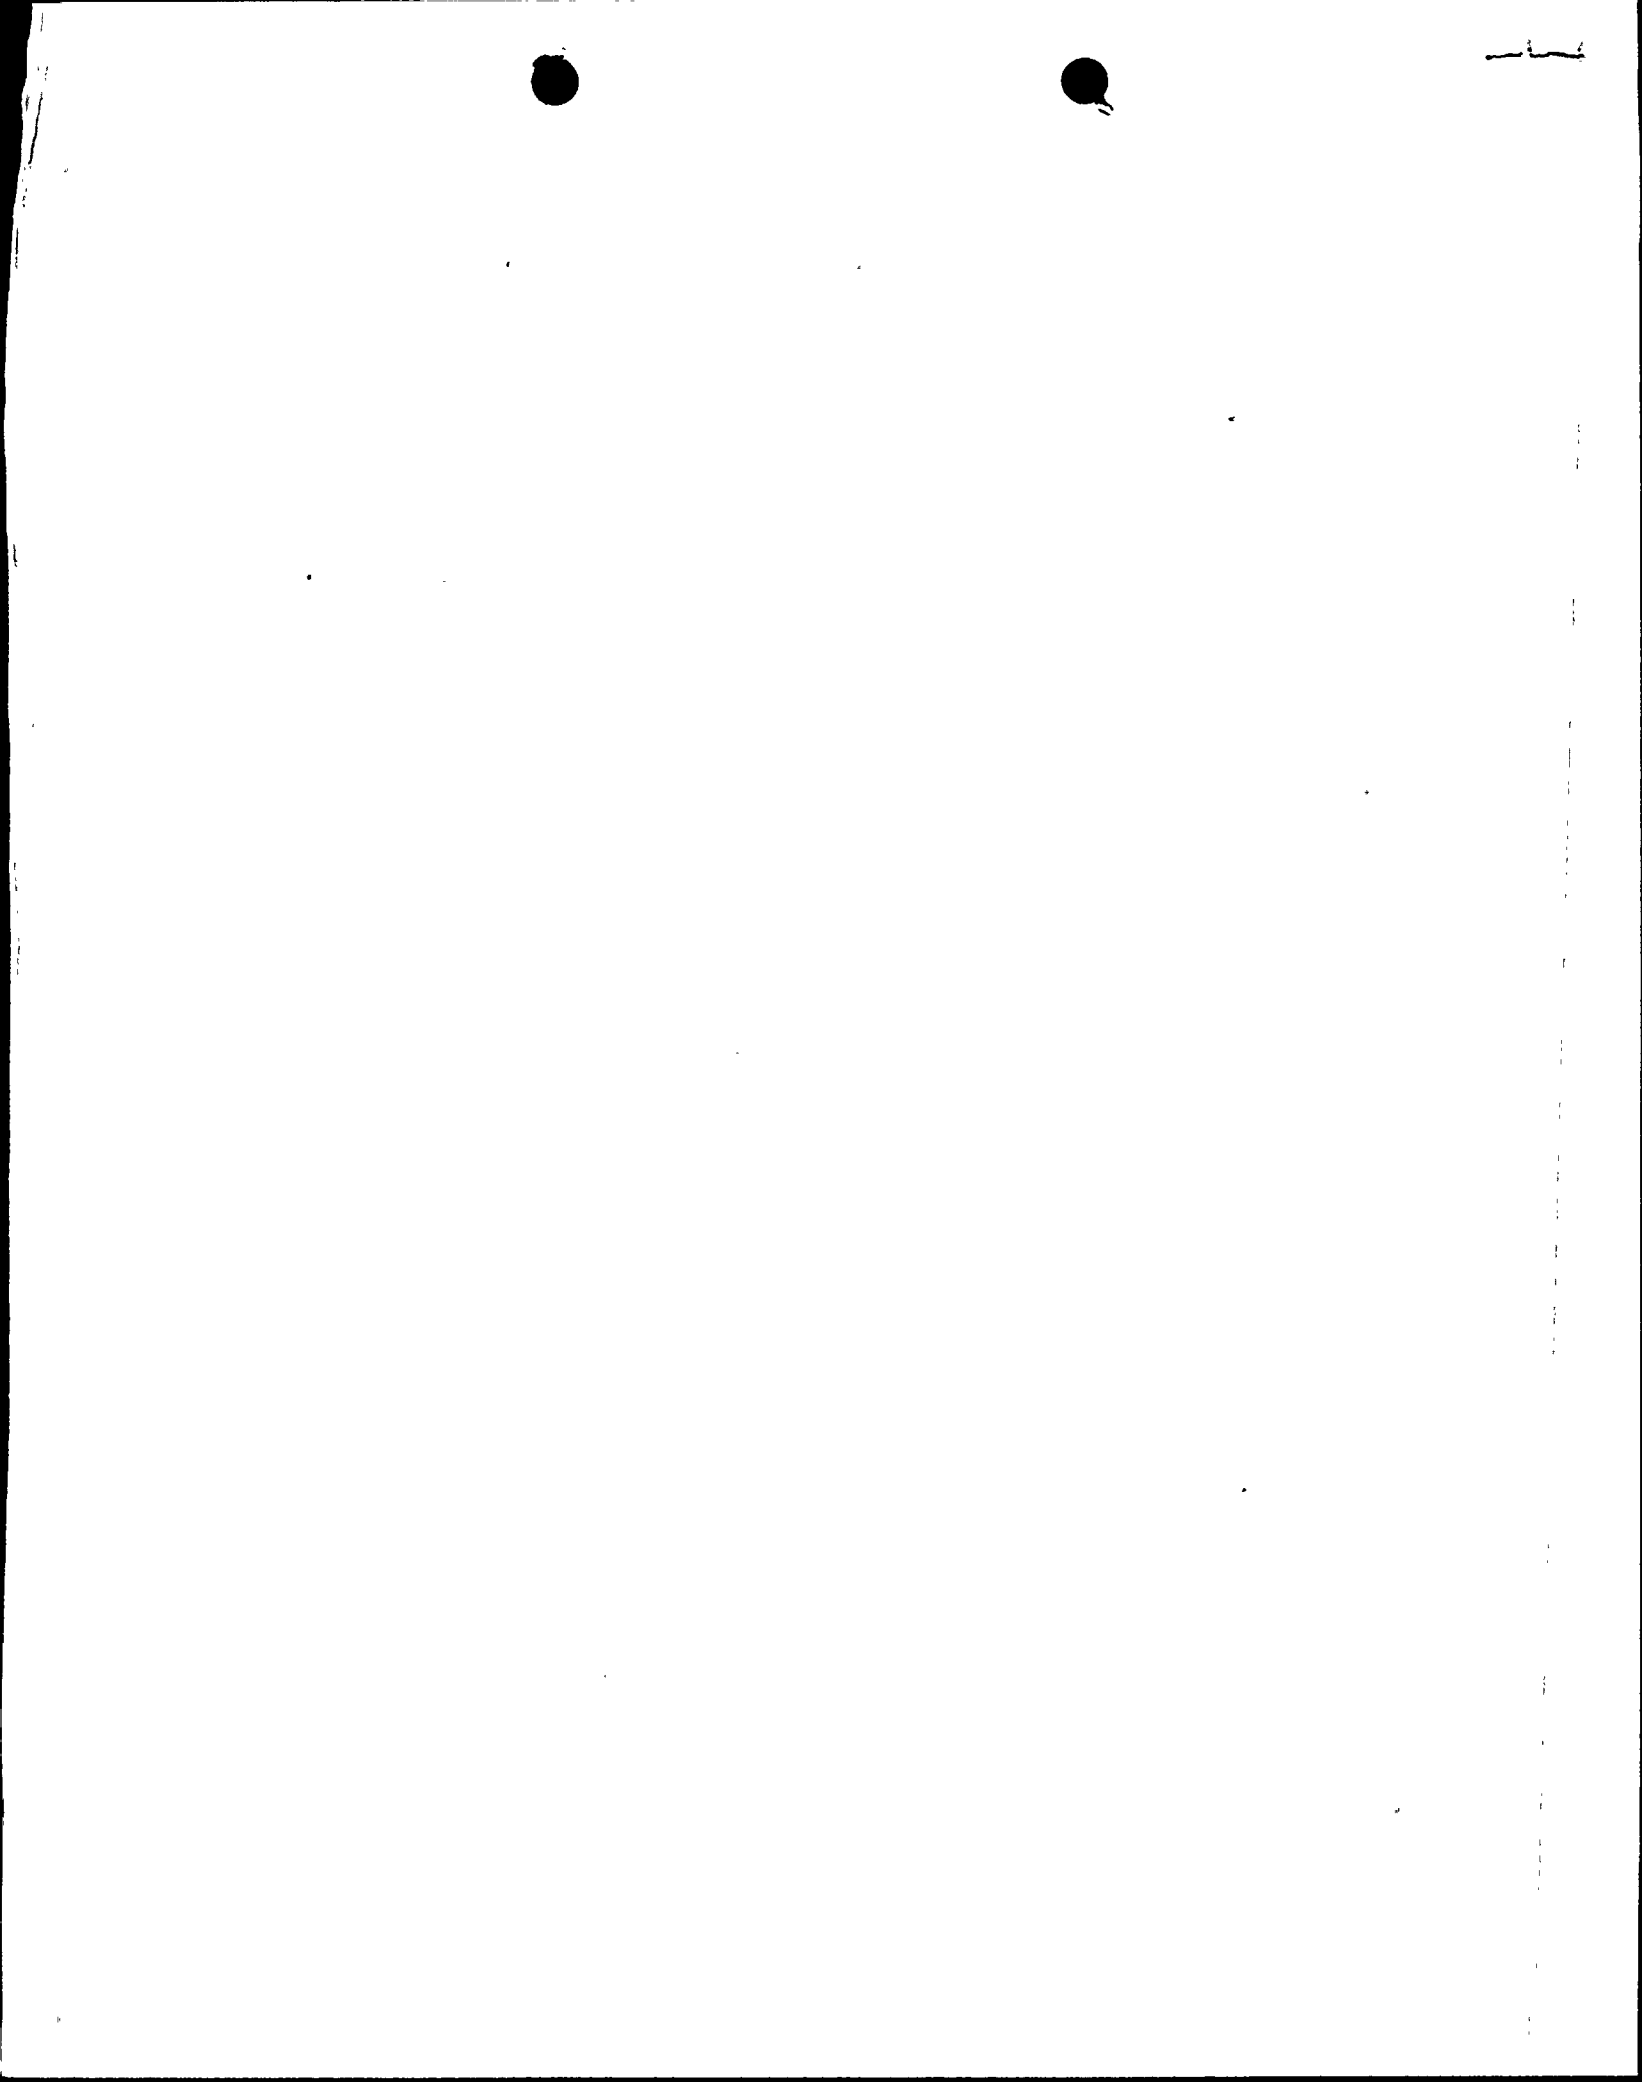

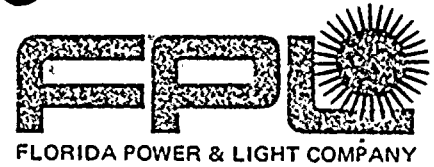

JULY 17 1987

L-87-302

U. S. Nuclear Regulatory Commission
Attn: Document Control Desk
Washington, D. C. 20555

Gentlemen:

Re: Turkey Point Units 3 and 4
Docket Nos. 50-250 and 50-251
Results of the NRC Confirmatory
Measurements Program Samples

In response to a NRC request dated April 30, 1987 Florida Power & Light has obtained the results of the spike sample analysis performed under the subject program.

The sample received by Turkey Point Plant was analyzed in accordance with the instructions that accompanied the sample. The results are corrected to January 11, 1987 and attached to this letter.

Should there be any additional questions, please contact us.

Very truly yours,

C. O. Woody
Group Vice President
Nuclear Energy


COW/SDF/gp

Attachment

cc: Dr. J. Nelson Grace, Regional Administrator, Region II, USNRC
Senior Resident Inspector, USNRC, Turkey Point Plant

FE 25
11

8707220647 870717
PDR ADDCK 05000250
PDR

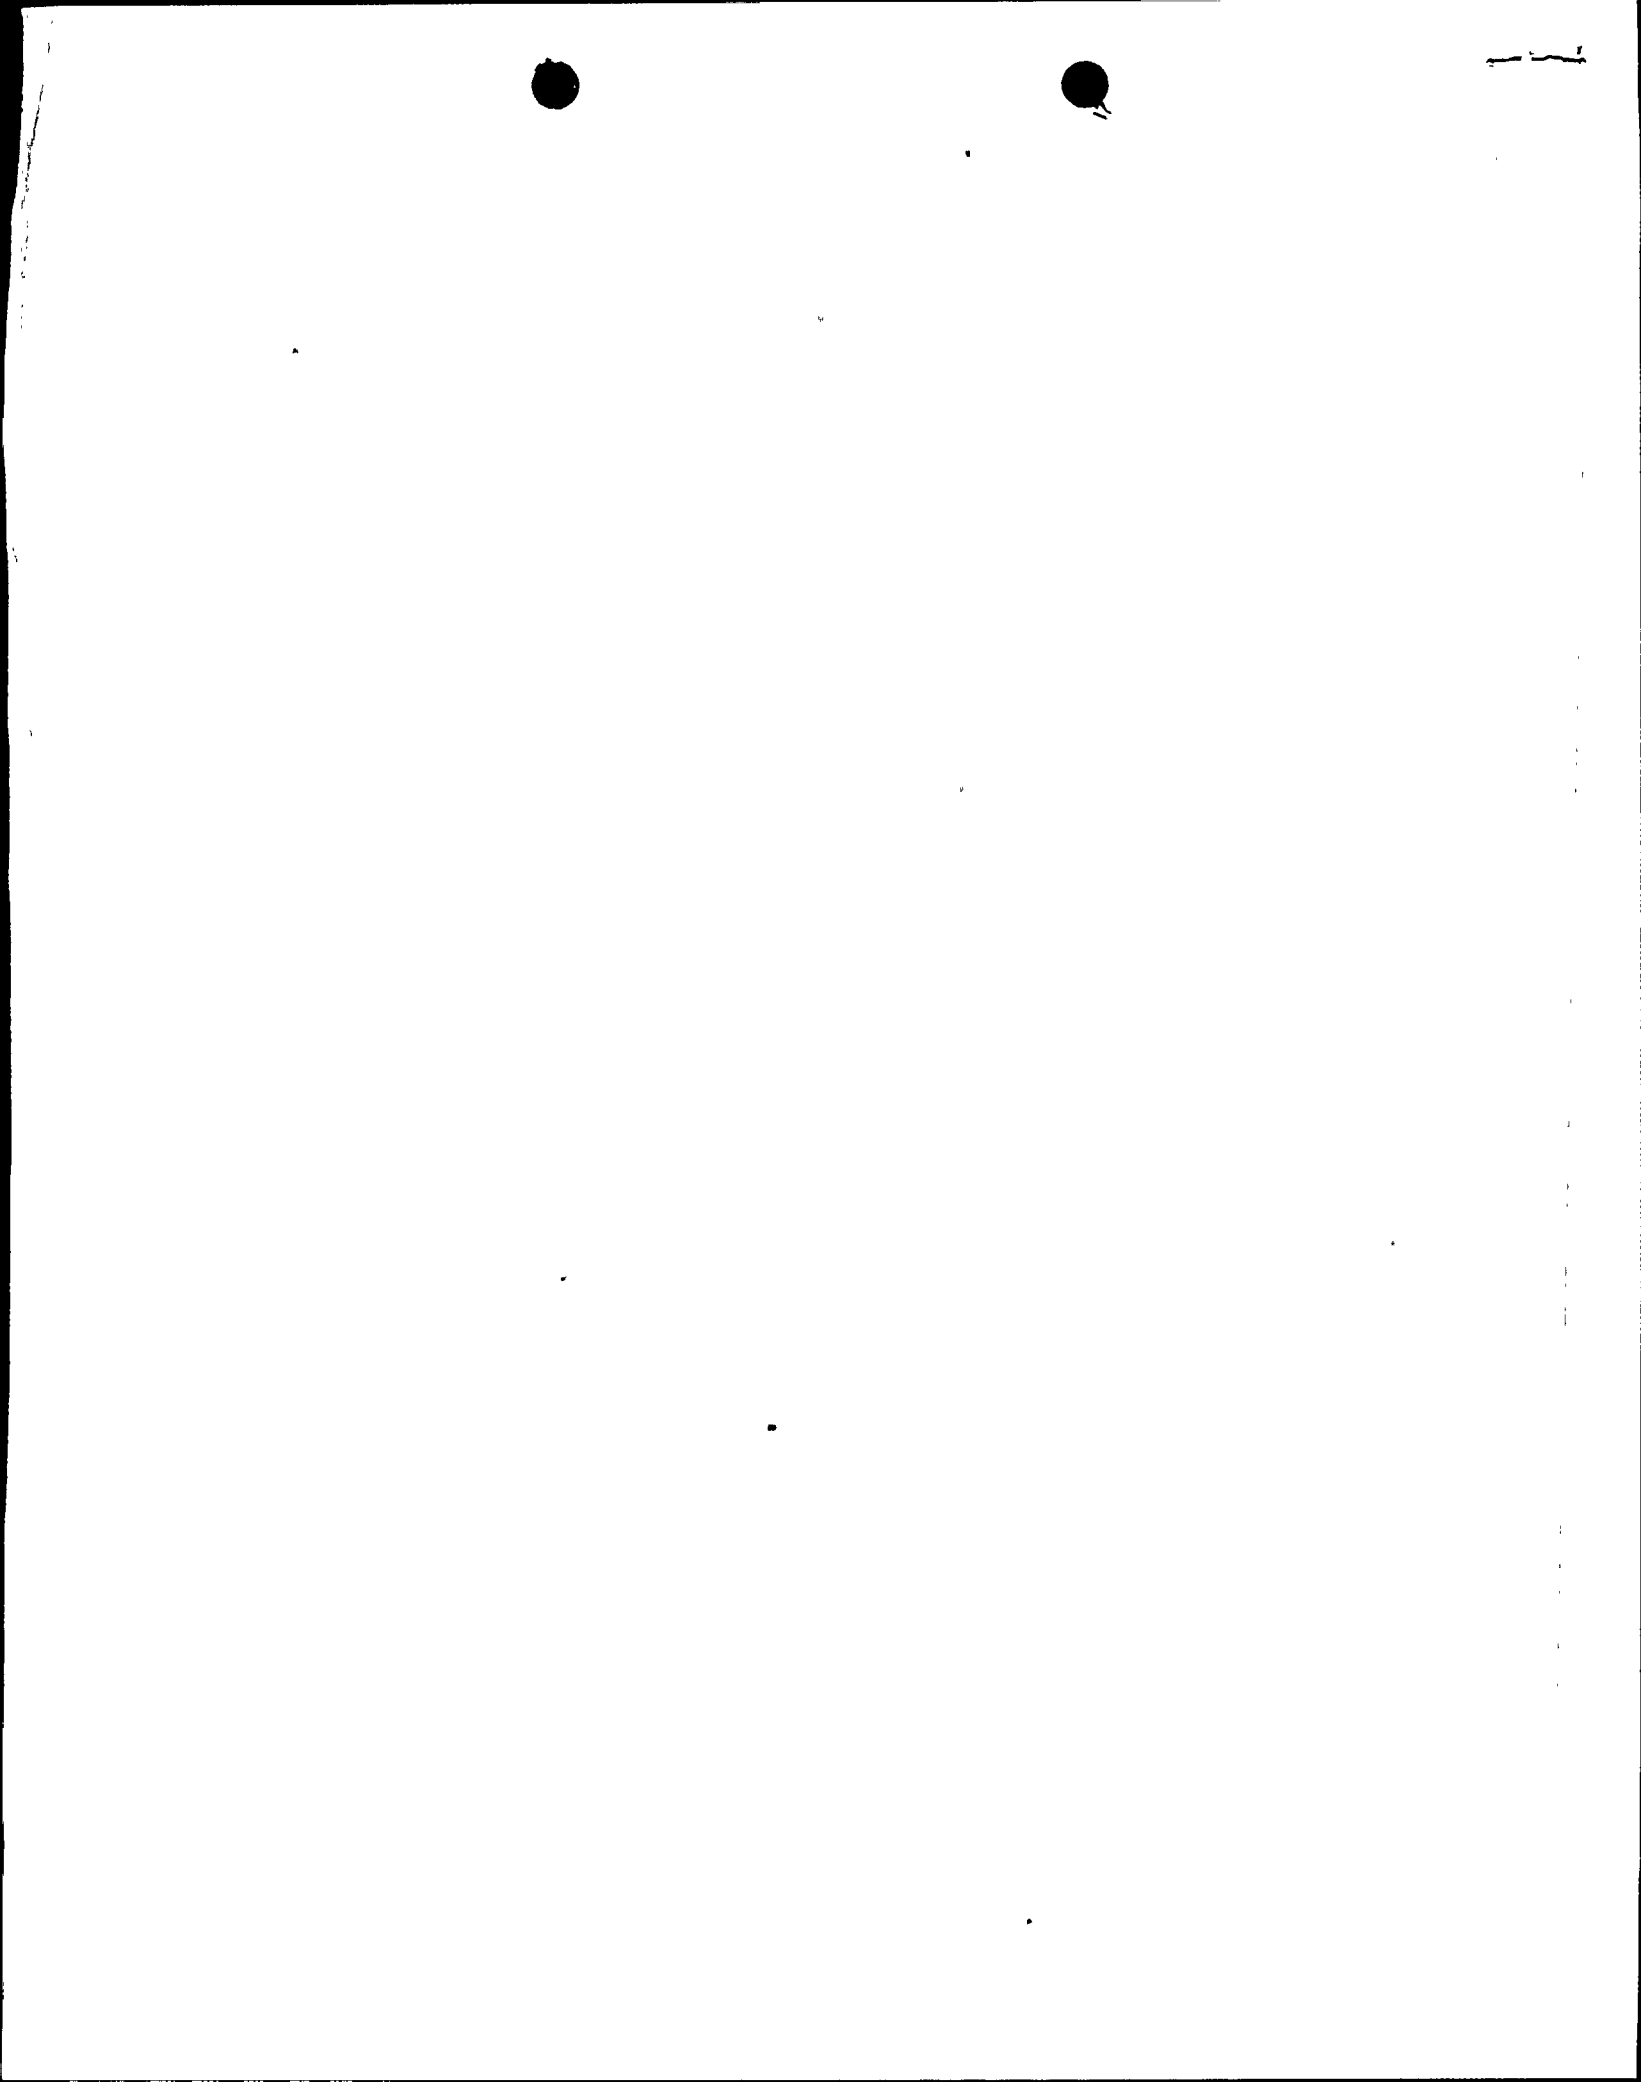

ATTACHMENT

Re: Turkey Point Units 3 and 4
Docket Nos. 50-250 and 50-251
Results of the NRC Confirmatory
Measurements Program Samples

Sample Analyses Results

<u>Isotope</u>	<u>Activity ($\mu\text{Ci/ml}$)</u>
Fe-55	$1.72 \text{ E-}05 \pm 1.72 \text{ E-}06$
Sr-89	$3.35 \text{ E-}05 \pm 3.35 \text{ E-}06$
Sr-90	$3.91 \text{ E-}06 \pm 3.91 \text{ E-}07$
H-3	$5.95 \text{ E-}05 \pm 2.38 \text{ E-}06$

