



## Medical Events Subcommittee Report

Ronald D. Ennis, M.D.  
Advisory Committee for the Medical  
Uses of Isotopes  
September 20, 2018

1



## Subcommittee Members

- Ronald D. Ennis, M.D. (Chair)
- Richard Green
- Darlene Metter, M.D.
- Michael O'Hara, Ph.D.
- John Suh, M.D.
- Michael Sheetz

2



## Process

- This year, rather than review the details of specific cases, we are reporting on our overview of events over last 3.5 years to discern common themes within each section of 10 CFR Part 35 and across the sections, to inform a discussion of possible ways to decrease medical events (MEs).
- We reviewed the last three reports of this subcommittee (FYs 2014-16) as well as the spring report of Dr. Howe for FY 2017

3



## Summary

- Two overarching themes emerged
  - Performance of a time out immediately prior to administration of radioactive byproduct material, as is done in surgery and other settings, could have prevented some MEs
  - Lack of recent or frequent performance of the specific administration appears to be a contributing factor in a number of cases

4

**Medical Events Summary**

|               | 2014     | 2015     | 2016     | 2017     | Total     |
|---------------|----------|----------|----------|----------|-----------|
| <b>Cause</b>  |          |          |          |          |           |
| Wrong drug*   | 0        | 3        | 3        | 0        | 6         |
| Wrong dosage  | 5        | 0        | 3        | 3        | 11        |
| Wrong patient | 1        | 1        | 2        | 0        | 4         |
| <b>Total</b>  | <b>6</b> | <b>4</b> | <b>8</b> | <b>3</b> | <b>21</b> |

\* In most cases wrong drug was also wrong dosage  
21 events over 4 years

5

**How Can These Events Be Prevented?**

- Wrong drug: Time out - confirm the order, compare to the prescription
- Wrong dosage: If a dose calibrator is available – measure the activity
- Wrong patient: Time out - Verify patients by two means of identification
- 10/21 preventable if time out had been used

**Medical Event Summary**

|                               | 2014     | 2015     | 2016     | 2017     | Total     |
|-------------------------------|----------|----------|----------|----------|-----------|
| WD not done or incorrectly    | 0        | 1        | 0        | 2        | 3         |
| Error in delivery (#capsules) | 2        | 3        | 1        | 1        | 7         |
| Wrong dose                    | 0        | 2        | 3        | 0        | 5         |
| Equipment                     | 1        | 1        | 0        | 0        | 2         |
| Unauthorized clinic           | 0        | 0        | 1        | 0        | 1         |
| Wrong patient                 | 1        | 0        | 0        | 1        | 2         |
| <b>Total</b>                  | <b>4</b> | <b>7</b> | <b>5</b> | <b>4</b> | <b>20</b> |

Time out could prevent 10-17/20

7

**Medical Event Summary**

|   | 2014 | 2015 | 2016 | 2017 | Total |
|---|------|------|------|------|-------|
| Applicator issue (e.g. movement during implant)     | 1    | 1    | 1    | 0    | 3     |
| Wrong site implanted (e.g. penile bulb)             | 3    | 1    | 1    | 1    | 6     |
| Activity/prescription error (e.g. air kerma vs mCi) | 1    | 2    | 0    | 1    | 4     |
| Prostate Dose                                       | 0    | 4    | 18   | 5    | 27    |

### 35.400 Manual Brachytherapy

#### Medical Event Summary

|   | 2014 | 2015 | 2016 | 2018 | Total   |
|---|------|------|------|------|---------|
| Total ME                                  | 5    | 8    | 20   | 7    | 40      |
| "Time out" may have prevented             | 1    | 2    | 0    | 1    | 4 (10%) |
| Lack of experience may have played a role | 3    | 1    | 1    | 1    | 6 (15%) |

9

### 35.400 Manual Brachytherapy

Many MEs in this category are no longer categorized as MEs due to change from dose- to activity-based definition.

Lack of experience possibly plays a role in the true MEs of this type, but hard to assess to what degree in each case.

In approximately 25% of cases, a "time out" or enhanced retraining prior to performance of an uncommon procedure might have prevented the ME.

10

### 35.600 Use of a sealed source in a remote afterloader unit, teletherapy unit, or gamma stereotactic unit

#### Medical Event Summary

|                            | 2014 | 2015 | 2016 | 2017       |
|----------------------------|------|------|------|------------|
| <u>Cause</u>               |      |      |      |            |
| Wrong position             | 3    | 6    | 1    | 2          |
| Wrong reference length     | 2    | 3    | 0    | 2          |
| Wrong plan                 | 1    | 3    | 1    | 0          |
| Wrong dose/source strength | 2    | 0    | 0    | 0          |
| Machine malfunction        | 2    | 2    | 3    | 2          |
| <u>Software failure</u>    | 0    | 0    | 0    | 2 (9 pts)  |
| Total                      | 10   | 14   | 5    | 8 (14 pts) |

37 events over 4 years

11

### 35.600 Use of a sealed source in a remote afterloader unit, teletherapy unit, or gamma stereotactic unit

#### Medical Event Summary

|                 | 2014 | 2015 | 2016 | 2017       |
|-----------------|------|------|------|------------|
| <u>Location</u> |      |      |      |            |
| Breast          | 1    | 1    | 0    | 0          |
| Gynecological   | 5    | 9    | 2    | 7 (14 pts) |
| Skin            | 2    | 1    | 1    | 0          |
| Bronchus        | 1    | 2    | 0    | 0          |
| Prostate        | 0    | 0    | 2    | 0          |
| <u>Brain</u>    | 1    | 1    | 0    | 1          |
| Total           | 10   | 14   | 5    | 8 (14 pts) |

GYN tumors most common site of ME

12



### 35.600 Use of a sealed source in a remote afterloader unit, teletherapy unit, or gamma stereotactic unit

#### MEs that may have been prevented by "timeout" (wrong plans or dose)

- 2014 3/10 events
  - 2015 3/14 events
  - 2016 1/5 events
  - 2017 0/8 events
- Total 6/37 (16.2%)

13



### 35.600 Use of a sealed source in a remote afterloader unit, teletherapy unit, or gamma stereotactic unit

#### MEs caused by "infrequent user"

This is difficult to determine based on information on NMED. If assumption is made about wrong position as surrogate for "infrequent" user

- 2014 3/10 events
  - 2015 6/14 events
  - 2016 1/5 events
  - 2017 2/8 events
- Total 12/37 (32.4%)

14



### 35.1000 Radioactive Seed Localization

#### Medical Events Summary

|   | 2014 | 2015 | 2016 | 2017 |
|---|------|------|------|------|
| Total Medical Events                        | 1    | 1    | 0    | 2    |
| Cause:                                      |      |      |      |      |
| Delayed seed removal (patient intervention) | 1    | 1    |      |      |
| Lost seed                                   |      |      |      | 1    |
| Wrong implant site                          |      |      |      | 1    |



### 35.1000 Gamma Knife® Perfexion™ and Icon™

#### Medical Events Summary

|   | 2014 | 2015 | 2016 | 2017 |
|---|------|------|------|------|
| Total Medical Events  | 1    | 8    | 3    | 0    |
| Cause:  |      |      |      |      |
| Patient positioning system misalignment by vendor (same site) |      | 8    |      |      |
| Patient setup error   |      |      | 2    |      |
| Patient movement  |      |      | 1    |      |
| Wrong site (treatment plan)                                   | 1    |      |      |      |

### 35.1000 Y-90 Theraspheres

#### Medical Events Summary


|  | 2014 | 2015 | 2016 | 2017 |
|--|------|------|------|------|
| Total Medical Events                                 | 9    | 8    | 13   | 15   |
| Cause:   |      |      |      |      |
| > 20% residual activity remaining in delivery device | 6    | 7    | 9    | 7    |
| Delivery device setup error                          |      |      | 1    | 2    |
| Wrong dose (treatment plan calculation error)        | 1    |      | 1    | 4    |
| Wrong site (catheter placement error)                | 1    | 1    | 2    | 2    |
| Wrong site (shunting)                                | 1    |      |      |      |

### 35.1000 Y-90 SirSpheres

#### Medical Events Summary

|  | 2014 | 2015 | 2016 | 2017 |
|--|------|------|------|------|
| Total Medical Events   | 15   | 10   | 13   | 8    |
| Cause:   |      |      |      |      |
| > 20% residual activity remaining in delivery device not due to stasis | 10   | 2    | 9    | 7    |
| Wrong site (shunting)  | 2    | 4    |      |      |
| Delivery device setup error  | 1    | 3    |      |      |
| Wrong dose (treatment plan calculation error)                          | 1    | 1    | 2    |      |
| Wrong site (catheter placement error)                                  | 1    |      | 2    | 1    |

### Overview Y-90 Microsphere ME 2014 - 2017

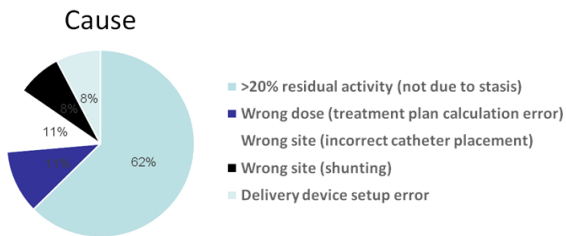

### Actions to Prevent 35.1000 Y-90 Microsphere Medical Events

- Review mechanics of Y-90 microsphere delivery device and setup procedures
- Confirm all data and calculations in treatment plan
- Perform "Time Out" to assure all elements of treatment are in accordance with Written Directive

 **U.S.NRC 35.1000 Medical Events That May Have Been Prevented by “Time Out”**  
United States Nuclear Regulatory Commission  
 Protecting People and the Environment

|              | RSL              | Perfexion/Icon    | Y-90<br>Microspheres |
|--------------|------------------|-------------------|----------------------|
| 2014         | 1/2              | 1/1               | 3/24                 |
| 2015         | 0/1              | 0/8               | 2/18                 |
| 2016         | 0/1              | 2/3               | 3/26                 |
| 2017         | 0                | 0                 | 3/23                 |
| <b>Total</b> | <b>1/4 (25%)</b> | <b>3/12 (25%)</b> | <b>11/91 (12%)</b>   |

 **U.S.NRC 35.1000 Medical Events That May Have Been Attributed to Lack of Experience or Infrequent User**  
United States Nuclear Regulatory Commission  
 Protecting People and the Environment

|              | RSL             | Perfexion/Icon    | Y-90<br>Microspheres |
|--------------|-----------------|-------------------|----------------------|
| 2014         | 0/2             | 0/1               | 1/24                 |
| 2015         | 0/1             | 0/8               | 3/18                 |
| 2016         | 0/1             | 2/3               | 1/26                 |
| 2017         | 0               | 0                 | 2/23                 |
| <b>Total</b> | <b>0/4 (0%)</b> | <b>2/12 (17%)</b> | <b>7/91 (8%)</b>     |

 **U.S.NRC Possible Elements of a “Time Out”**  
United States Nuclear Regulatory Commission  
 Protecting People and the Environment

- Identity of patient via two identifiers (e.g. name and DOB)
- Procedure to be performed
- Isotope
- Activity
- Dosage
- Others as applicable
  - units of activity (LDR prostate)
  - anatomic location
  - patient name on treatment plan
  - treatment plan independent second check has been performed
  - reference length (HDR)
  - Implant site location (RSL)

23

 **U.S.NRC Possible Elements of Refresher for Infrequent Procedure**  
United States Nuclear Regulatory Commission  
 Protecting People and the Environment

- Take review course from professional society
- Read review articles
- Speak to colleague with experience
- Do dry run of procedure with the team
- Review mechanics of device set up and procedure

24

## Recommendation for Action

The subcommittee recommends the NRC issue an Information Notice alerting AUs to the themes identified herein

25

## Acronyms

- 10 CFR – Title 10 of the *Code of Federal Regulations*
- AUs – authorized users
- DOB – date of birth
- FY – Fiscal Year
- Gy – Gray
- gyn – gynecological
- HDR – high dose-rate

26

## Acronyms

- LDR – low dose rate
- mCi – milliCurie
- ME – Medical Event
- RSL – radioactive seed localization
- Y – Yttrium

27