



Veterans
Administration

In Reply Refer To:

December 22, 1981

Mr. David Skov
U. S. Nuclear Regulatory Commission
1450 Maria Lane, Suite 210
Walnut Creek, CA 94596

Gentlemen:

Submitted herewith is a copy of our Capintec dose calibrator linearity test which was conducted on 4-27-81. This test record was inadvertently placed in a filing cabinet rather than with the other dose calibrator records. Thus, it was unavailable during your recent inspection. Please accept my apologies.

Sincerely,

A handwritten signature in cursive script that reads "L. W. Wetterau".

L. W. WETTERAU
Radiation Safety Officer
Nuclear Medicine Ultrasound Service

Enclosure

8204150505 820216
PDR FOIA
NELSON82-11 PDR

DEC 29 11 12 AM '81


RECEIVED
DEC 29 11 12 AM '81

Linearity Check for Capintec Dose Calibrator

4-27-81

46 5490

KE SEMI-LOGARITHMIC 3 CYCLES X 70 DIVISIONS
KEUFEL & ESSER CO. MADE IN U.S.A.

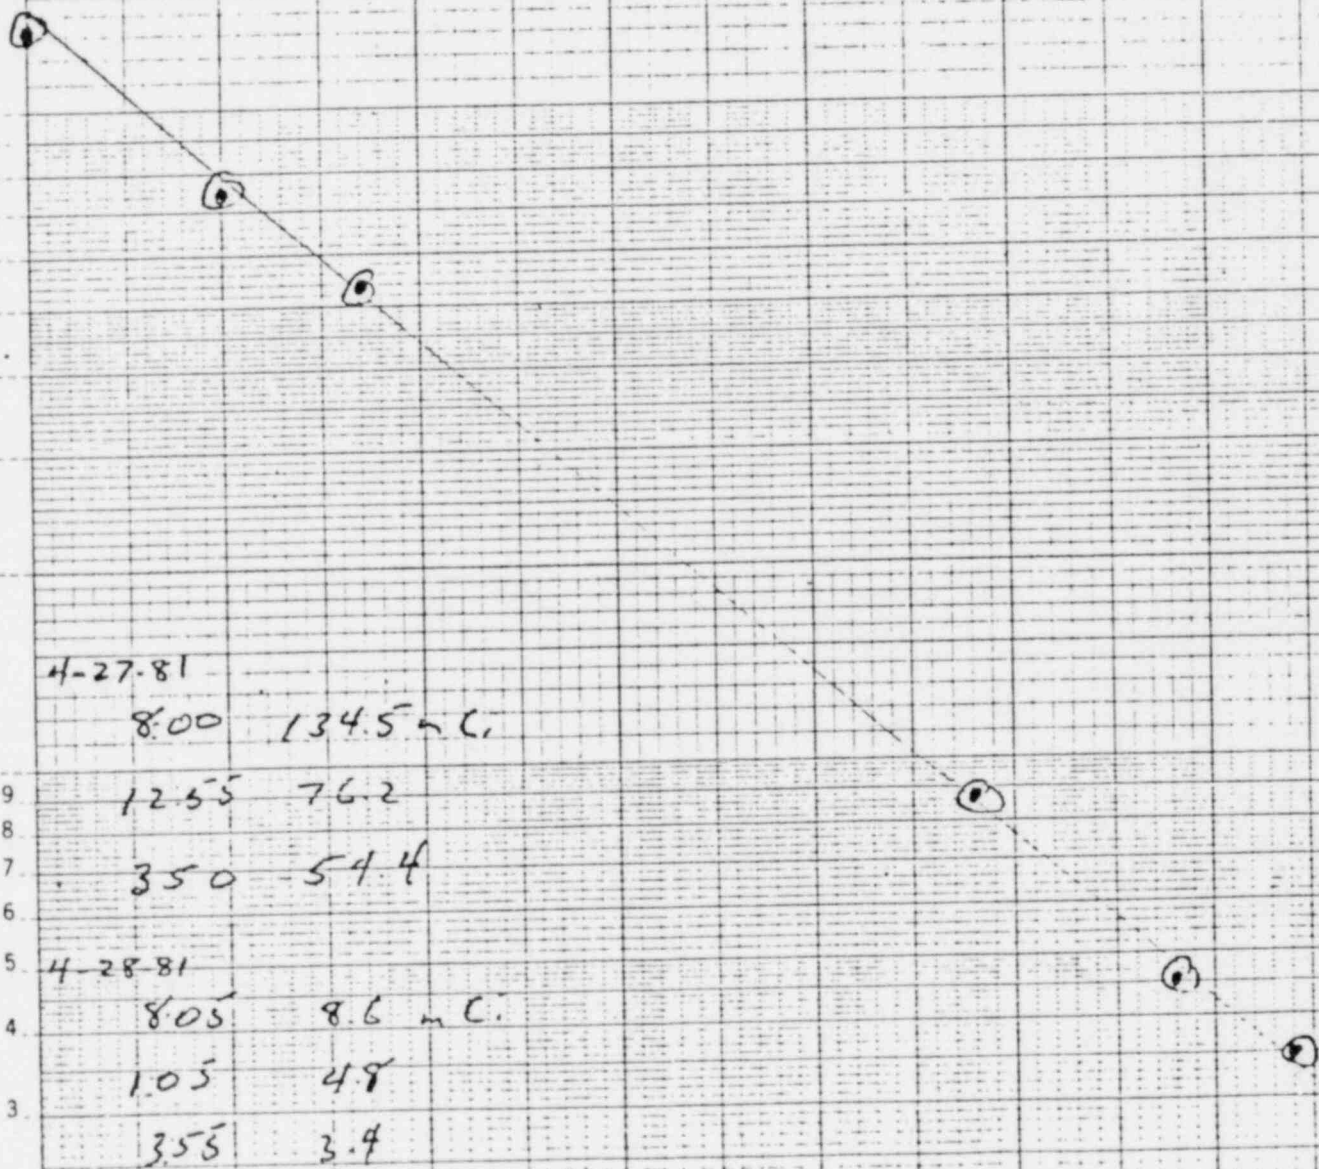

4-27-81

8.00 134.5 mCi

12.55 76.2

350 54.4

4-28-81

8.05 8.6 mCi

1.05 4.8

3.55 3.4

Within $\pm 3\%$

5

10

15

20

25

30

35