

Appendix

NOTICE OF VIOLATION

Industrial Gamma Inspection

License No. 24-19850-01

As a result of the inspection conducted on October 1, 1982, and in accordance with the NRC Enforcement Policy, 47 FR 9987 (March 9, 1982), the following violations were identified:

1. 10 CFR 34.28(b) requires that the licensee conduct a program for inspection and maintenance of radiographic exposure devices, storage containers and source changers at intervals not to exceed three months. Records of these inspections and maintenance shall be kept for two years.

Contrary to this requirement, you have failed to maintain records of your quarterly maintenance and inspections performed during 1981 and to October 1, 1982.

This is a Severity Level V violation (Supplement VI).

2. 10 CFR 34.24 requires that each survey instrument used to conduct physical radiation surveys be calibrated at intervals not to exceed three months and after each instrument servicing.

Contrary to this requirement, during the period from June 7, 1982, to July 21, 1982, you conducted physical radiation surveys with a survey instrument which was calibrated more than three months prior to the date of use.

This is a Severity Level IV violation (Supplement VI).

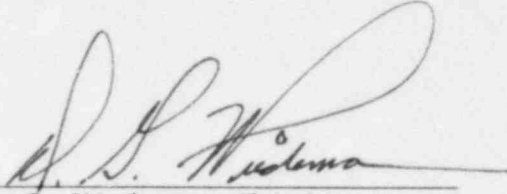
3. 10 CFR 20.401(b) requires that you maintain records showing the results of monitoring required by 10 CFR 20.205(b) and (c), "Procedures for picking up, receiving, and opening packages."

Contrary to this requirement, you failed to maintain records of the monitoring you performed during 1981 and 1982 of incoming packages containing more than Type A Quantities of iridium-192.

This is a Severity Level V violation (Supplement IV).

Pursuant to the provisions of 10 CFR 2.201, you are required to submit to this office within thirty days of the date of this Notice a written statement or explanation in reply, including for each item of noncompliance: (1) corrective action taken and the results achieved; (2) corrective action to be taken to avoid further noncompliance; and (3) the date when full compliance will be achieved. Consideration may be given to extending your response time for good cause shown.

10-13-82
Dated


D. G. Wiedeman, Chief
Materials Radiation Protection
Section 1