

Appendix

NOTICE OF VIOLATION

Oak Hill Hospital

License No. 24-16612-01

As a result of the inspection conducted on September 28 and 29, 1982, and in accordance with the NRC Enforcement Policy, 47 FR 9987 (March 9, 1982), the following violations were identified:

1. 10 CFR 35.14(e)(1)(i) requires that sealed sources used as calibration or reference sources be tested for leakage and/or contamination at intervals not to exceed six months.

Contrary to the above, a review of records and statements of licensee representatives indicated that this requirement was not met. Specifically, your 1 millicurie cesium-137 source Serial No. NSH1318, purchased on February 9, 1976 was used from June 30, 1981 to September 28, 1982. The last recorded leak test was performed on February 2, 1981.

This is a Severity Level V violation (Supplement VI).

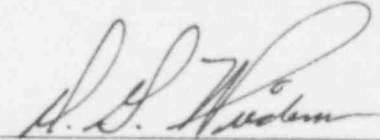
2. License Condition No. 15 requires that all licensed material be possessed and used in accordance with statements, representations, and procedures contained in application dated June 20, 1980. Item 10b of the application states that the procedures described in Appendix D, Section 2, of the NRC Medical Licensing Guide will be used for calibration of the dose calibrator. Appendix D, Section 2, requires quarterly linearity tests.

Contrary to the above, the NRC inspector learned from statements of licensee representatives, and a review of records that this requirement was not met. Specifically, quarterly linearity tests were not performed from April 1982, to the day of the inspection September 28, 1982.

This is a Severity Level V violation (Supplement VI).

Pursuant to the provisions of 10 CFR 2.201, you are required to submit to this office within thirty days of the date of this Notice a written statement or explanation in reply, including for each item of noncompliance: (1) corrective action taken and the results achieved; (2) corrective action to be taken to avoid further noncompliance; and (3) the date when full compliance will be achieved. Consideration may be given to extending your response time for good cause shown.

10-18-82
Dated


D. G. Wiedeman, Chief
Materials Radiation Protection
Section 1