

NOV 07 1985

License No. 29-16796-02  
Docket No. 030-14993  
Control No. 104478

Sharlin Radiological Associates, P.A.  
ATTN: Frank Gingerelli, M.D.  
35 Pangborn Place  
Hackensack, New Jersey 07601

Gentlemen:

Please find enclosed an amendment to your NRC Material License.

Please review the enclosed document carefully and be sure that you understand all conditions. If there are any errors or questions, please notify the Region I Material Licensing Section, (215) 337-5239, so that we can provide appropriate corrections and answers.

Please be advised that you must conduct your program involving licensed radioactive materials in accordance with the conditions of your NRC license, representations made in your license application, and NRC regulations. In particular, please note the items in the enclosed, "Requirements for Materials Licensees."

Since serious consequences to employees and the public can result from failure to comply with NRC requirements, the NRC expects licensees to pay meticulous attention to detail and to achieve the high standard of compliance which the NRC expects of its licensees.

You will be periodically inspected by NRC. A fee may be charged for inspections in accordance with 10 CFR Part 170. Failure to conduct your program safely and in accordance with NRC regulations, license conditions, and representations made in your license application and supplemental correspondence with NRC will result in prompt and vigorous enforcement action against you. This could include issuance of a notice of violation, or in case of serious violations, an imposition of a civil penalty or an order suspending, modifying or revoking your license as specified in the General Policy and Procedures for NRC Enforcement Actions, 10 CFR Part 2, Appendix C.

8512160008 851107  
REQ1 LIC30  
29-16796-0 PDR

OFFICIAL RECORD COPY

ML 29-16796-02/LTR - 0001.0.0  
10/28/85

ML10

We wish you success in operating a safe and effective licensed program.


Sincerely,

Jenny M. Johansen, M.S.  
Nuclear Materials Safety Section B  
Division of Radiation Safety  
and Safeguards

Enclosures:

1. Amendment No. 04
2. Requirements for Materials Licensees
3. 10 CFR Parts 2, 19, 20, 30, 35, and 170
4. Notice to All Teletherapy Licensees

RI:DRSS  
Johansen/k1

10/29/85 

OFFICIAL RECORD COPY

ML 29-16796-02/LTR - 0002.0.0  
10/28/85

BETWEEN: William O. Miller, Chief  
License Fee Management Branch  
Office of Administration

John E. Glenn, Chief  
Nuclear Materials Section B  
Division of Engineering and  
Technical Programs

LICENSE FEE TRANSMITTAL

No Fee  
Needed - Teletherapy Survey

A. REGION I

1. APPLICATION ATTACHED

Applicant/Licensee: Sharlin Radiological Associates, P.A.

Application Dated: 9/20/85

Control No.: 104478

License No.: 29-16796-02

2. FEE ATTACHED

Amount: 0

Check No.: 0

3. COMMENTS

02300

3/89

LMS-03

Signed Brionda Platchek

Date 10/10/85

B. LICENSE FEE MANAGEMENT BRANCH

1. Fee Category and Amount: 7A no fee due to

2. Correct Fee Paid. Application may be processed for: survey  
report

Amendment ✓

Renewal \_\_\_\_\_

License \_\_\_\_\_

**FEE EXEMPT**

Signed Jo Jackson

Date 10/31/85

LEONARD S. ROSEN, M.D., F.A.C.R.  
DANIEL S. CUKIER, M.D., M.A.C.R.  
DAVID N. BRAMWIT, M.D., M.A.C.R.  
FRANK GINGERELLI, M.D., M.A.C.R.  
STEPHEN Z. KAUFMAN, M.D., M.A.C.R., D.A.B.N.M.  
JAE N. KIM, M.D., PH.D., M.A.C.R., D.A.B.N.M.

HERBERT S. SHARLIN, M.D., F.A.C.R.  
CONSULTANT

DIAGNOSTIC RADIOLOGY  
XERORADIOGRAPHY  
THERAPEUTIC RADIOLOGY  
LINEAR ACCELERATOR  
COBALT TELETHERAPY  
NUCLEAR MEDICINE

SHARLIN RADIOLOGICAL ASSOCIATES, P.A.

35 PANGBORN PLACE  
HACKENSACK, N. J. 07601  
TELEPHONE (201) 342-7558

September 20, 1985

United States Nuclear Regulatory Commission  
Region I  
631 Park Avenue  
King of Prussia, PA 19406

Attn: John Glenn, Ph.D.

Dear Dr. Glenn:

Please find the enclosed radiation protection survey performed on our Cobalt-60 Teletherapy unit following replacement of the source. This report is submitted as a requirement by condition 18 of our license (29-16796-02). In accordance with Section 20.201 of 10 CFR Part 20.

Should you require further information, please do not hesitate to contact me.

Sincerely,

RECEIVED BY LFMB	
Date	10-21-85
Log	Oct 10
By	<i>[Signature]</i>
Orig. To	AMD / 7A <i>[initials]</i>
FG/mm	Action Compl.

*[Signature]*  
Frank Gingerelli, M.D.  
Sharlin Radiological Assoc., P.A.  
35 Pangborn Place  
Hackensack, N.J. 07601

enclosure

cc: U.S.N.R.C.  
c/o Document Management Branch  
Washington, D.C. 20555

**FEE EXEMPT**

**"OFFICIAL RECORD COPY"**

**ML10 104478**

**OCT 08 1985**

*251/99/21*  
*22pp*

RECEIVED  
'85 OCT 21 AM 1:00  
U.S.N.R.C.  
DOC. MGMT. BRANCH

SHARLIN RADIOLOGICAL ASSOCIATES, P.A.  
35 Pangborn Place  
Hackensack, New Jersey 07601

RADIATION SAFETY SURVEY

NRC License # 29-16796-02

THERATRON 80

Source Manufacturer:	Neutron Products, Inc.
Model Number :	NPI-20-6000W
Serial Number :	T-788
Source Installed :	September 13, 1985
Curie Content :	6410 curies on September 13, 1985
Date of Survey :	September 16, 1985

I. Beam Output Calibration

The exposure rate was measured on September 16, 1985 for the range of field sizes and for the range of distances used in treatment in compliance with 10 CFR 35.21. A Capintec model 192 electrometer with 6cc probe was used for the calibration. The Capintec Electrometer was last calibrated on March 9, 1984 at K & S Associates, Inc., 1854 Airline Drive, Nashville, Tennessee. A copy of the calibration report is also appended.

II. Teletherapy HEAD Survey - Beam "Off"

The head survey was made with the beam in the "off" position at 1 meter from the source. A Victoreen Survey Model # 471A, Serial # 319, was used to perform this survey. Please see attached calibration certificate specifying calibration method and date. Table I specifies the maximum and average radiation levels surrounding the head. The head is in compliance with NCRP Report # 33, since the average exposure rate at 1 meter does not exceed 2.0 mR/hr., and the maximum exposure rate at 1 meter does not exceed 10.0 mR/hr..

III. Limits of BEAM ORIENTATION

Electrical and mechanical interlocks are installed so that the primary beam can not be directed off the beam absorber. The limit the primary beam is permitted away from the center line of the integral beam stopper is less than 5 degrees + or -.

Conversion from rads/min to RHM (Roetgens per hour at 1 meter) for a 10 x 10 field and 20 x 20 field at 80cm SAD.

1) 10cm x 10cm field at 80.0cm SAD = 163.7 rads/min.

$$\frac{163.7 \text{ rads/min} \times \left(\frac{80}{100}\right)^2 \times 60 \text{ min/hr}}{(.967)(.989)} = 6573 \text{ RHM}$$

where .967 = F (rads/R) water  
.989 = Aeg

2) 20cm x 20cm field at 80.0cm SAD = 170.6 rads/min.

$$\frac{170.6 \text{ rads/min} \times \left(\frac{80}{100}\right)^2 \times 60 \text{ min/hr}}{(.967)(.989)} = 6850 \text{ RHM}$$

TELETHERAPY HEAD SURVEY  
(Source in "OFF" position.  
Measurements taken one meter  
from source)

Top View - Showing orientation  
of Views A through D

Position No.	Radiation Level (mR/hr)
View A	
1	3.2
2	1.1
3	3.6
4	1.0 (shield installed)

View B	
5	1.3
6	2.2
7	0.5
8	0.2

View C	
9	1.5
10	1.7

View D	
11	0.2
12	0.4
13	2.3
14	3.6

Average value 1.6



Maximum value 3.6

Instrument used \_\_\_\_\_  
Victoreen 471A


Curies 6410  
&  
Date 9/13/85

Manufacturer's  
name & model #  
of teletherapy  
unit AECL


Theratron 80

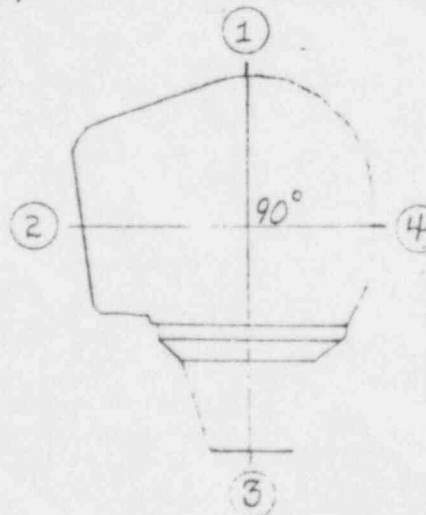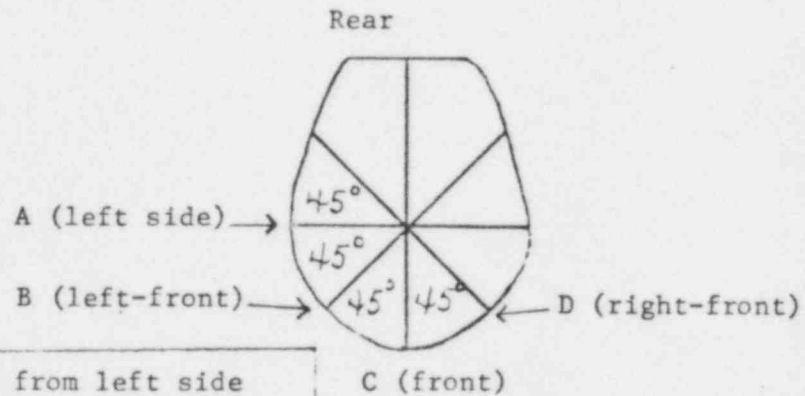


View B - Vertical from left-front

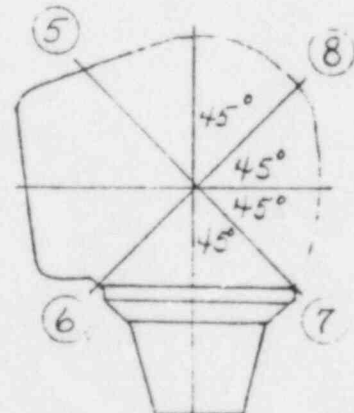

View C - Vertical from front

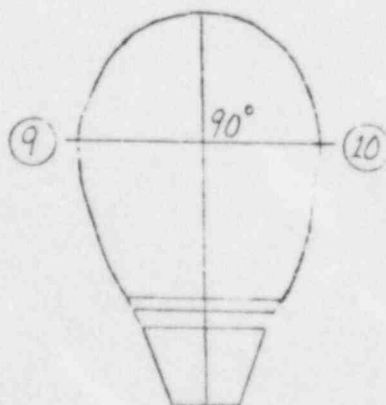

View D - Vertical from right-front

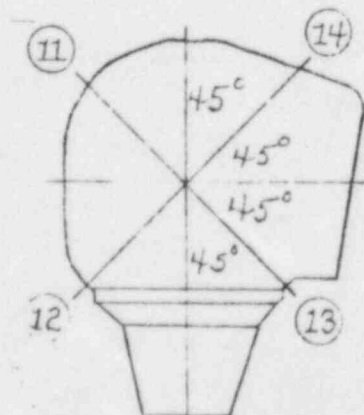

#### IV. Room Protection Survey


The room protection survey was made with a Victoreen Model 471A Survey Meter as described in Part II. The beam was directed against a lucite phantom with a 20cm x 20cm field size at 80.0cm SAD, 70.0cm SSD.

Each barrier was surveyed at  $30^{\circ}$  increments of the gantry angle with the beam intercepted by the beam absorber. Figure II illustrates the gantry angle with respect to the room. For example, when the gantry angle is set on  $90^{\circ}$ , the beam will be directed towards Barrier D (intercepted by the beam absorber).

Table II specifies the maximum readings and corresponding orientation of the beam. The dose rates were measured one foot from side barriers, and one foot on the roof.

<u>Location</u>	<u>Description</u>
A	Treatment room door
B	Control area
C	Hallway
D	Patient waiting room
E	Outside
F	Outside
G	Outside
H	Patient dressing rooms (1/2 level up)
I	Roof (fenced in area)
J	Boiler room (1/2 level down)
K	Roof (unfenced area)

Note: Room is located on ground level, no basement.

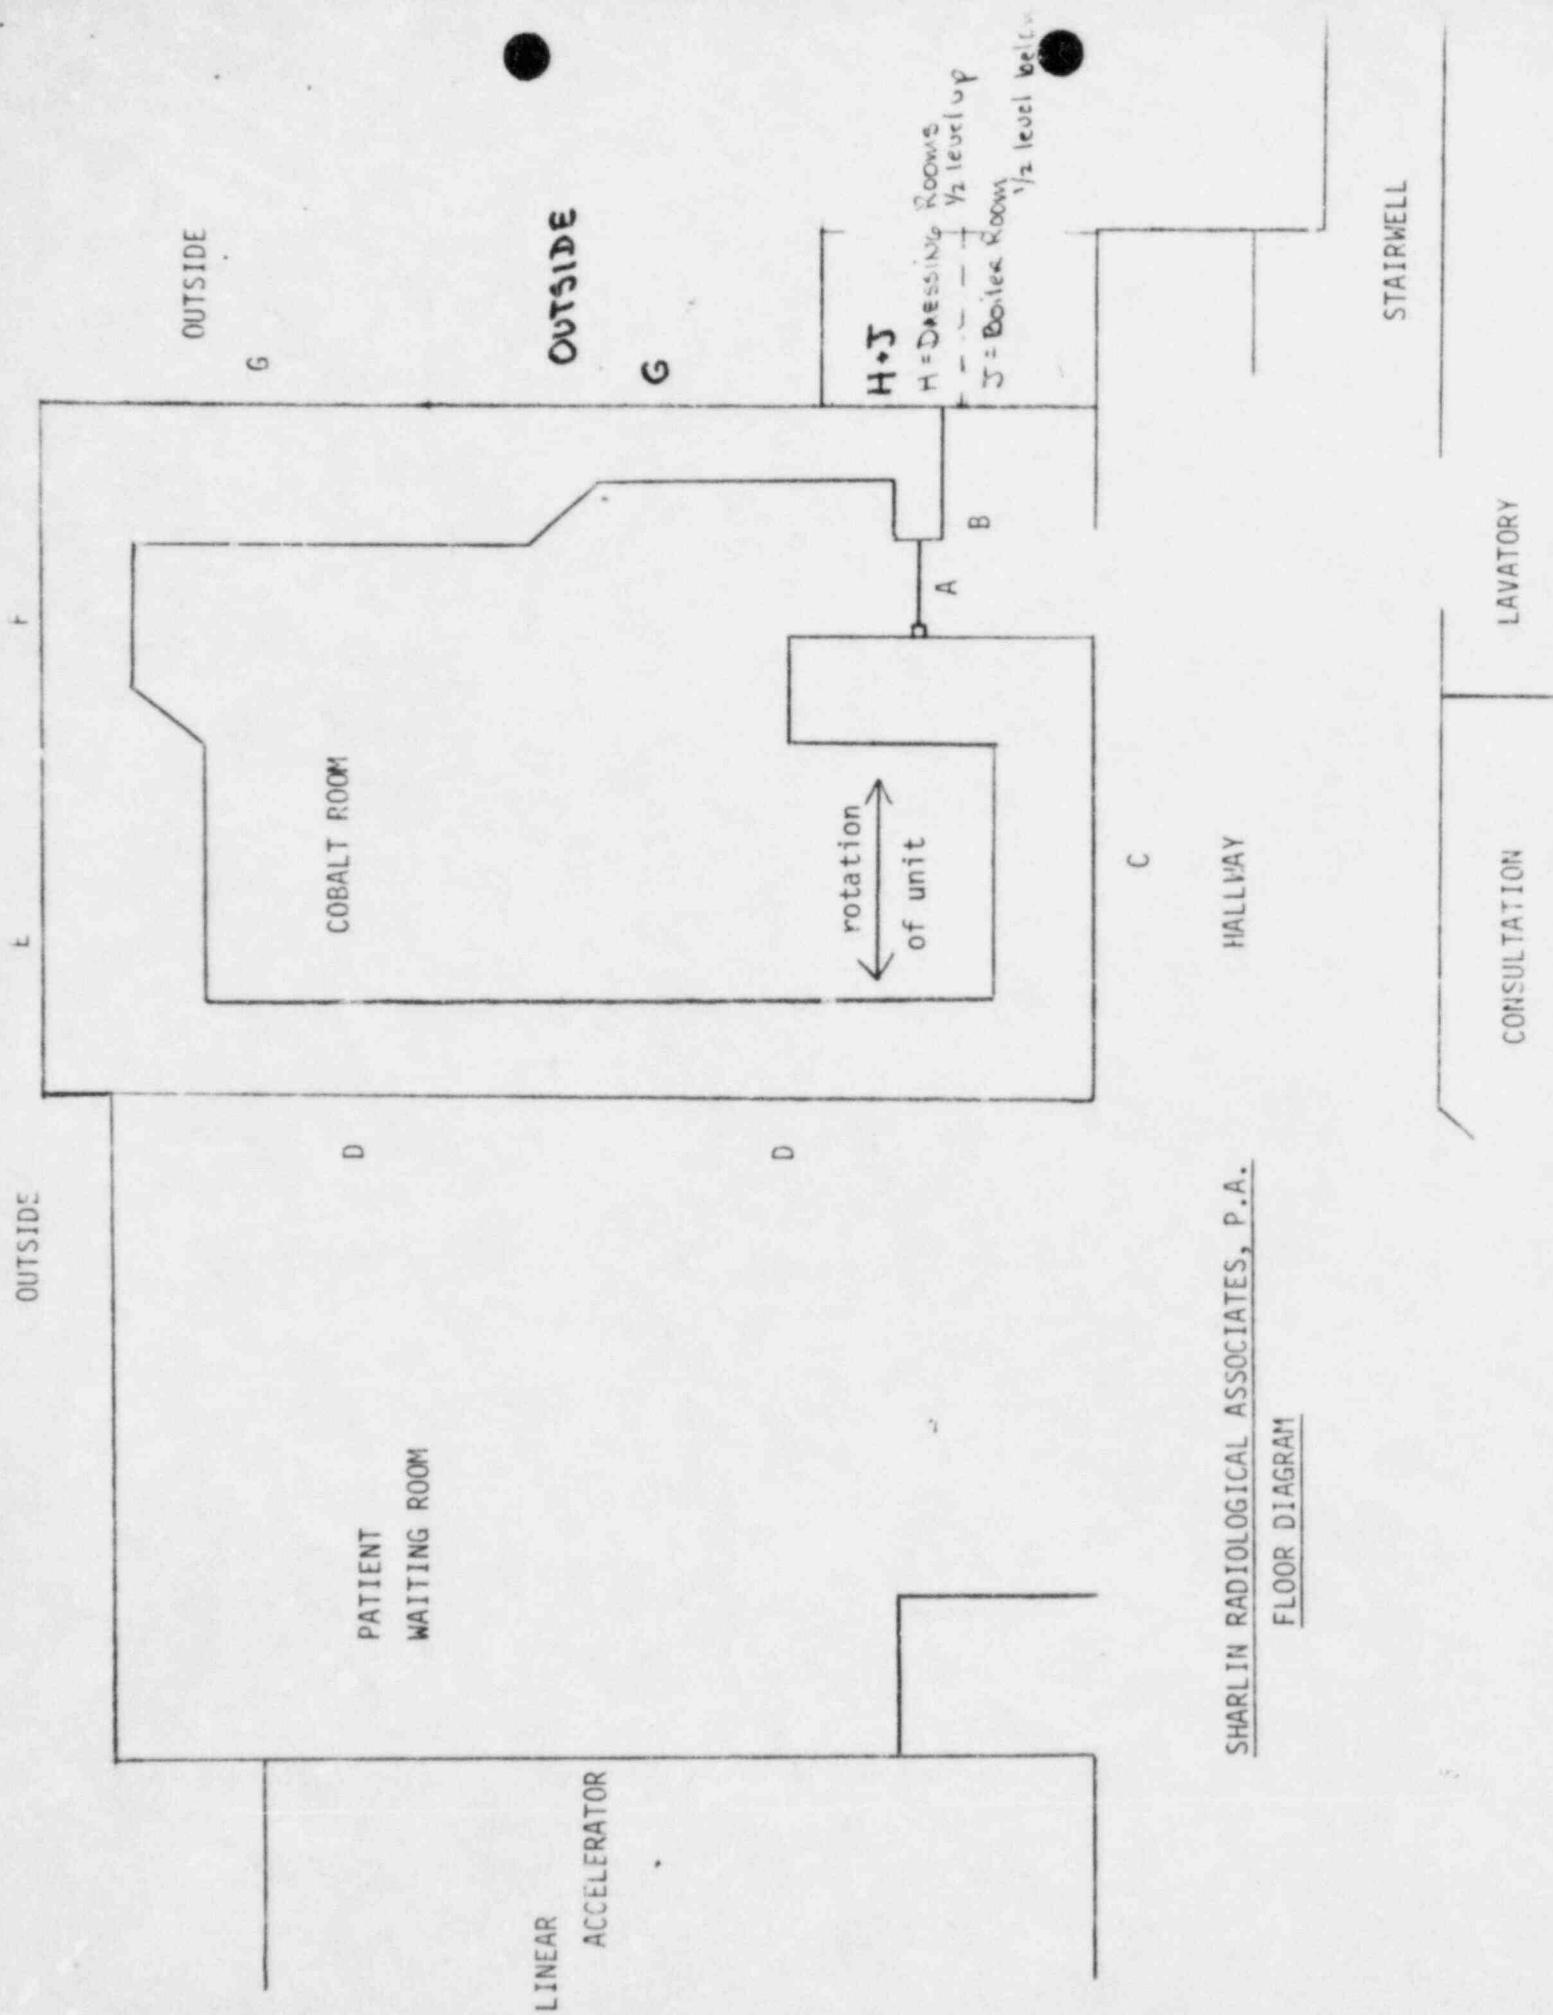

SHARLIN RADIOLOGICAL ASSOCIATES, P.A.

FLOOR DIAGRAM

FIGURE II

Beam Interlock Diagram

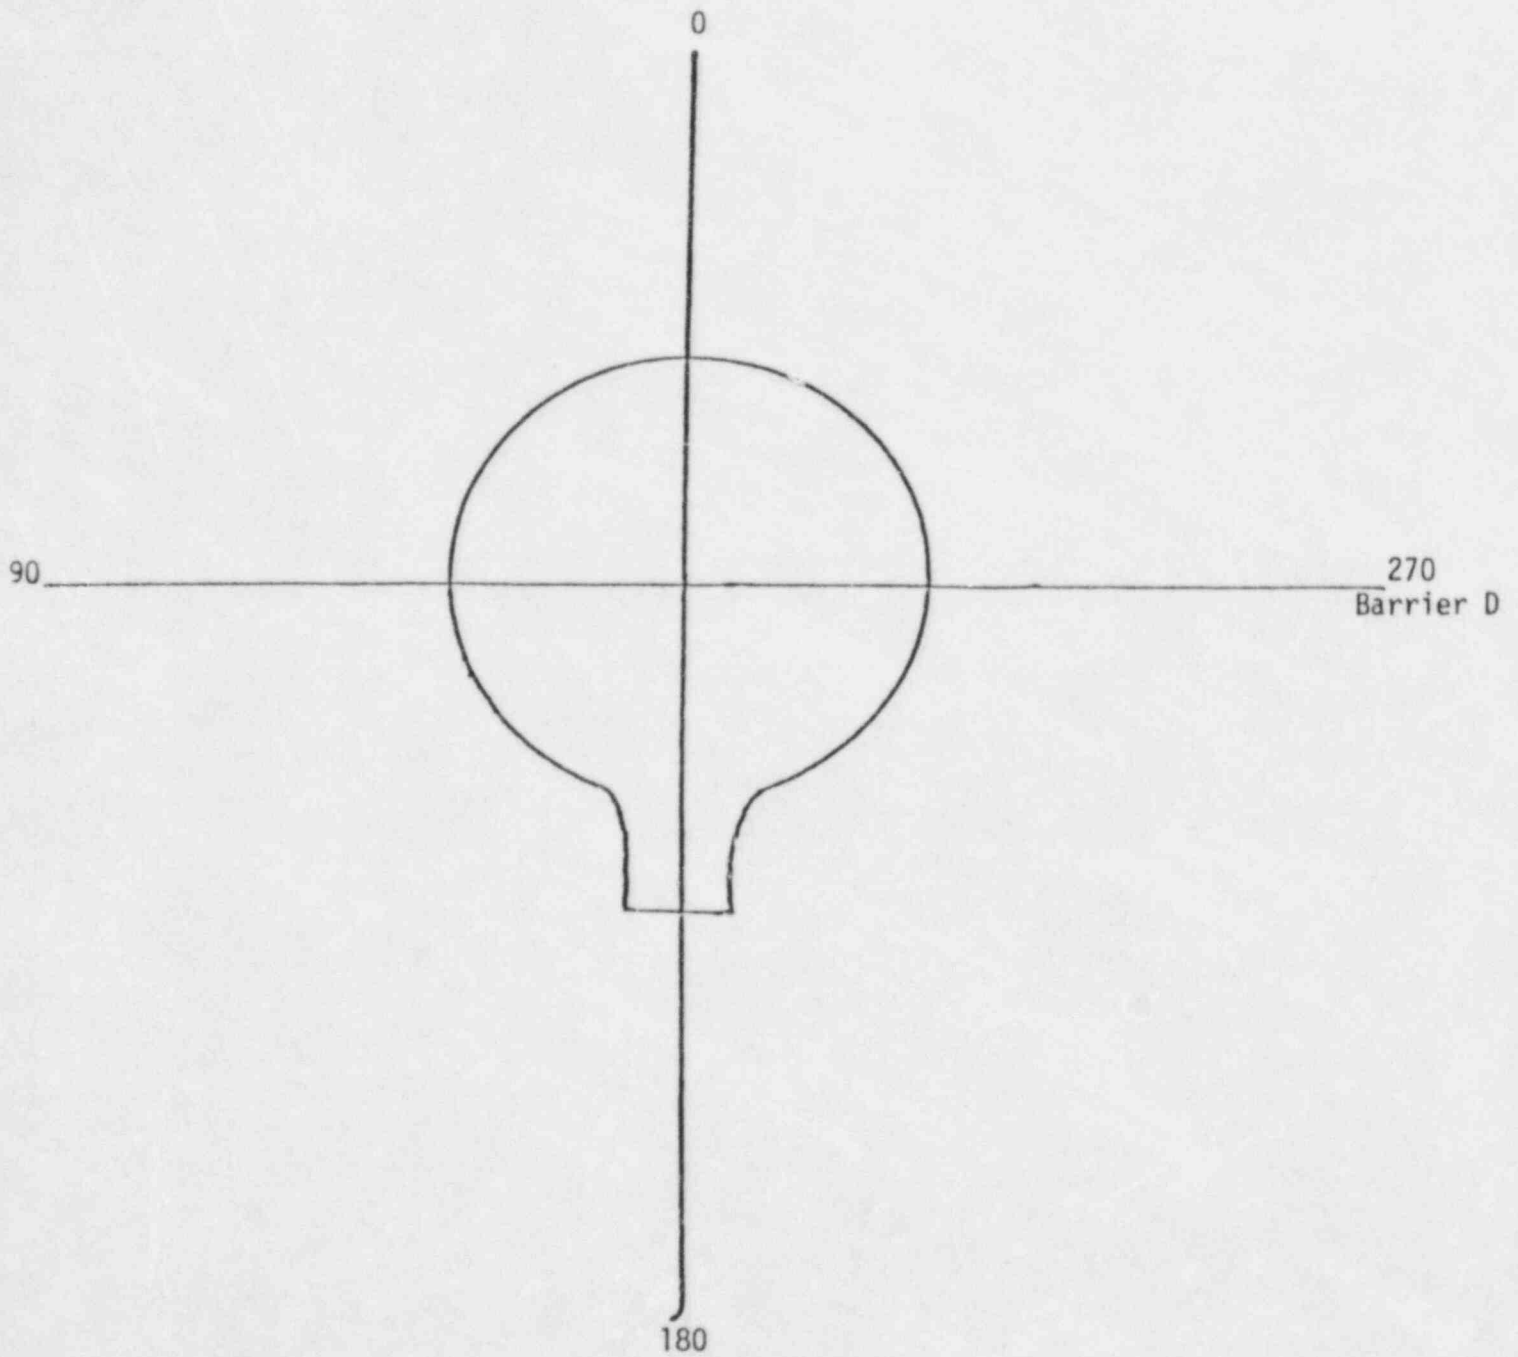


TABLE II  
MAXIMUM DOSE RATES

<u>Location</u>	<u>Area</u>	<u>Beam Orientation</u>	<u>mR/hr.</u>
A	Restricted	240 <sup>0</sup>	2.7
B	Restricted	300 <sup>0</sup>	1.6
C	Non-Restricted	*	<0.5
D	Non-Restricted	90 <sup>0</sup>	1.2
E	Non-Restricted	*	<0.5
F	Non-Restricted	*	<0.5
G	Non-Restricted	240 <sup>0</sup> & 300 <sup>0</sup>	9.2
H	Non-Restricted	*	<0.5
I	Restricted	150 <sup>0</sup>	25.0
J	Non-Restricted	*	<0.5
K	Non-Restricted	150 <sup>0</sup>	4.0

\*Detectable level less than 0.5 mR/hr  
in any orientation.

Beam orientation specifies the gantry angle (as illustrated in Figure II), with beam directed against the beam absorber.

In order for the room to comply with 10 CFR 20.105 (b), the average dose rate in one hour shall not exceed 2 mR/hr. in unrestricted areas. NCRP Report # 33 recommends that weekly permissible doses should be less than 100 mR/week in restricted areas and 10 mR/week in unrestricted areas. Refer to Table III for average dose rates and maximum weekly doses at each barrier. The average dose rate was calculated based on using fractional beam "on" times.

No more than 5 patients are treated in any one hour, therefore the amount of time the beam would be on in any given hour is 11 minutes. (See assumptions and calculations below.) The average hourly dose rate would then be 18% of the instantaneous maximum dose rate found in Table II. The maximum dose per week at each barrier is calculated employing a workload of 5.4 hours/week of beam "on" time. (See assumptions and calculations below.)

30 patients per day are treated  
5 days per week, 200 rads average per patient  
Average treatment time per patient  
= 200 rads delivered to a depth of  
10cm (Field Size 10 x 10) 80 SSD  
Output = 167.5 rads/min., DD% = 55.6

$$\frac{200}{(167.5)(55.6)} = 2.15 \text{ min. per treatment (Avg. patient)}$$

The results listed in Table III show that the teletherapy room is in compliance with 10 CFR 20.105 (b) and NCRP Report # 33.

TABLE III

<u>LOCATION</u>	<u>MAXIMUM mR/nour</u>	<u>OCCUPANCY FACTOR</u>	<u>AVERAGE mR/hour</u>	<u>MAXIMUM mR/week</u>	<u>MPD mR/week</u>
A	2.7	1	0.5	14.6	100
B	1.6	1	0.3	8.6	100
C	<0.5	1	<0.1	<0.6	10
D	1.2	1	0.2	6.5	10
E	<0.5	1/16	<0.1	<0.2	10
F	<0.5	1/16	<0.1	<0.2	10
G	9.2	1/16	1.7	3.1	10
H	<0.5	1	<0.1	<0.5	10
I	25	<< 1/16	4.6	<8.5	100
J	<0.5	1/16	<0.1	<0.2	10
K	4.0	<< 1/16	0.7	<1.4	10

\*Note: All areas become unrestricted and measure less than 0.5 mR/hr with beam in off position.

#### V. Timer Accuracy

The timer on the control panel of the teletherapy unit in the control area was tested against a calibrated stop watch and found to be accurate within two-tenths of a second for a trial of 60 seconds.

#### VI. Electrical and Mechanical Interlocks

The door to the teletherapy room was opened slightly when the machine was operating in the beam "on" mode and the interlock was found to be operational in that the source immediately moved to the "off" position. The emergency stop bar on the control panel was also activated in the beam "on" mode and the source returned to the beam "off" position. In both cases, door opened and emergency stop bar activated, the unit would not operate in the beam "on" position unless the control panel was reset. The "on" and "off" positions of the source were cross checked with the Primalert 10 radiation monitor which is tested daily with a test source provided by the manufacturer.

When the timer was switched "off" while the beam was in the "on" position, the source returned to the "off" position. (cross-checked with Primalert 10)

Electrical and mechanical beam stops were tested and found to restrict the operation of the unit to only be directed at the beam absorber as specified in Section III.

VII. Warning Signs, Indicator Lights, and NRC Posting Requirements

Beam "on-off" indicator lights on the control panel, in the treatment room (2 locations), and above the treatment door function correctly in both the beam "on" and the beam "off" modes. (cross-checked with Primalert 10) Appropriate warning signs are posted on the treatment room door. NRC-3 and emergency instructions with phone numbers to reach radiologists, physicists and repair technicians are posted as well. Also, posted are instructions where N.R.C. license and regulations are kept.

The roof area that is restricted above the treatment room has a chain link fence around it on three sides and a stone wall on the fourth side. The fence is approximately six feet high and the stone wall is approximately seven feet high. There is no way to get onto any area of the roof of the entire building without either using a ladder or going out a window. Two signs stating "Caution Radiation Area", including the radiation symbol are attached to the fence at eye level. These two signs are approximately 8" x 12" in size and are located on the only two sides that one can climb from the other areas of the roof.

Also, there are two other signs located next to the above signs stating "CAUTION, DO NOT ENTER AREA, CHECK WITH COBALT TECHNICIAN TO REQUEST PERMISSION TO ENTER". These signs measure 16" x 12". No one is to be within the fenced area while the Cobalt 60 machine is "on". All personnel involved are aware of this.

VIII. Radiation Monitor

A Nuclear Associates Model 05-433 "Primalert 10" radiation monitor with Model 05-440 "Primapak" battery back-up unit has been installed within the teletherapy room, is checked daily, and in good working order.

Surveyors:

Bruce D. Bucher  
Bruce D. Bucher

Robert A. Sasso  
Robert A. Sasso, M.S.

# SHARLIN RADIOLOGICAL ASSOCIATES. P.A.

35 PANGBORN PLACE  
HACKENSACK, N. J. 07601

TELEPHONE (201) 342-7558

COBALT - 60 OUTPUTS

MONTH OF: September, 1985

FIELD SIZE	80 SSD*	80 SAD
4 X 4	-	-
5 X 5	158.2	157.5
6 X 6	160.5	159.1
7 X 7	162.8	160.8
8 X 8	163.9	161.2
9 X 9	166.0	162.7
10 X 10	167.5	163.7
11 X 11	168.8	164.4
12 X 12	170.0	165.0
13 X 13	171.5	166.0
14 X 14	173.0	167.0
15 X 15	174.1	167.5
16 X 16	175.2	168.1
17 X 17	176.6	169.1
18 X 18	178.0	170.2
19 X 19	178.6	170.4
20 X 20	179.1	170.6
21 X 21	179.8	170.9
22 X 22	180.5	171.2
23 X 23	181.2	171.6
24 X 24	182.0	172.1
25 X 25	182.7	172.4
26 X 26	183.4	172.7
27 X 27	183.7	172.7
28 X 28	183.9	172.7
29 X 29	184.0	172.7
30 X 30	184.2	172.7

\*NOTE: SSD Outputs include backscatter factor  
Lucite Tray Factor=1.03  
Calibration = 163.7 Rads/Min. at 80.0cm for 10X10 Field  
for 9/16/85

*Robert A. Sasso*  
Radiologist

Model No.	Serial No.	Date Calibrated	Calibration Technique	Recommended Date For Recalibration
471A	319	3-20-85	137 CS	3-20-86
<p>FREQUENCY OF RECALIBRATION MAY VARY DEPENDING ON LOCAL, STATE OR FEDERAL REQUIREMENTS.</p>				

Register No. REP 2193 Tom Kraw Calibration Lab.

VICTOREEN, INC.  
10101 Woodland, Avenue. Cleveland, Ohio 44104  
A Sheller-Globe Corporation Subsidiary

# *K & S Associates, Inc.*

*Radiological Consultants*

*Medical - Industrial*

ACCREDITED DOSIMETRY CALIBRATION LABORATORY

## Calibration Report

Institution/Facility: Sharlin Radiological Date: March 26, 1984  
Associates, P.A. Report: 283  
35 Pangborn Place  
Hackensack, New Jersey 07601

Instrument: Capintec 192, SN 60F318  
Capintec PR06C, SN CII0.6799  
  
  
Test No.: 84043

The responsibility for calibration results provided by K & S Associates, Inc. and its employees extends only to the time the instruments leave the K & S laboratory facility. Constancy tests are highly recommended. It is the responsibility of the instrument user to assure himself that his interpretation of the information contained herein is consistent with the interpretation intended.

CALIBRATION FACTORS:

R/RDG: Roentgen/reading calibration factors apply to the chamber-electrometer-readout system as a unit, with scales, switch settings and output mode specified. To obtain the exposure in roentgens at the reference point\*, in the absence of the chamber, the calibration factor is applied directly to the instrument reading corrected for temperature and pressure:

$$\text{Exposure} = \text{RDG} \times \text{R/RDG} \times \text{TPC}$$

where TPC = temperature-pressure correction

R/C: Roentgen/coulomb calibration factors apply to the ion chamber alone. To obtain the exposure in roentgens at the reference point\*, in the absence of the chamber, an appropriately calibrated (coulomb/reading) electrometer must be used.

$$\text{Exposure} = \text{RDG} \times \text{R/C} \times \text{C/RDG} \times \text{TPC}$$

where C/RDG = calibration factor of electrometer  
TPC = temperature-pressure correction

TEMPERATURE-PRESSURE CORRECTION FACTOR:

For chambers open to the atmosphere, the instrument readings were normalized to 760 millimeters of mercury and 22 degrees Celsius. Use of the chamber at other pressures and temperatures requires correction by the following multiplicative factor:

$$\frac{T + 273.15}{295.15} \times \frac{760}{P}$$

where T is the temperature in degrees Celsius, and P is the chamber pressure in millimeters of mercury.

No corrections were made for air humidity.

CALIBRATION CONDITIONS:

Unless otherwise indicated, the calibration field size is 10 cm x 10 cm for Co-60 and 10 cm diameter circle for x-rays. Stem effect was not investigated; the calibration factor applies only to the field size stated.

During calibration the chamber was centered in the beam with the stem perpendicular to the beam direction, except for end-window chambers which are calibrated with the stem parallel to the beam direction.

\*The exposure reference point is at the geometrical center of the chamber volume, except when stated otherwise in the calibration report.

The exposure rate at the calibration position was measured with a transfer-quality ionization chamber which has a calibration that is directly traceable to the National Bureau of Standards.

#### BEAM QUALITY:

X-ray beam quality is described in terms of the first half-value thickness in millimeters of aluminum or copper. The ratio of the first to the second half-value thickness (homogeneity coefficient-H.C.) and the kilovoltage are also given.

The half-value thicknesses were determined under "good geometry" narrow beam conditions with high purity certified aluminum or copper attenuators. The focus-attenuator distance was approximately 50 cm, and the focus-chamber distance was approximately 100 cm.

#### ATMOSPHERIC COMMUNICATION:

All chambers are tested for communication to the atmosphere prior to calibration.

#### CALIBRATION ACCURACY CLASSIFICATION:

The accuracy of the calibration factors stated in this report are described in terms of classifications and represent the maximum deviation from the national dosimetry standard.

The classifications assigned by the ADCL are based on the precision of the laboratory and on the precision, accuracy, and reproducibility of the instrument or system submitted for calibration.

	Cobalt-60	Cesium-137	X-rays
CLASS I	+/- 0.5 %	+/- 0.5 %	+/- 1.0 %
CLASS II	+/- 0.5 %	+/- 0.5 %	+/- 2.0 %
CLASS III	+/- 1.0 %	+/- 1.0 %	+/- 2.0 %
CLASS III A	+/- 2.0 %	+/- 2.0 %	+/- 2.0 %
CLASS IV	-	+/- 5.0 %	+/- 5.0 %
CLASS V	-	+/- 10.0 %	+/- 10.0 %

# ELECTROMETER CALIBRATION REPORT

3-9-84  
 DATE

## INSTRUMENT:

Mfr: Capintec  
 Model No. 192  
 Serial No. 60F318

## SUBMITTED BY:

Sharlin Radiological  
Associates  
Hackensack, New Jersey

## SCALES, SWITCH POSITIONS, CONDITIONS:

COMPENSATION FACTOR: 1.00; PROBE SELECTOR: (see below);  
 METER RANGE: NORMAL OR EXTENDED; EXPOSURE LEVEL: (see below);  
 MODE: TOTAL

POLARIZING POTENTIAL: -300 V (indicates + 0301 V)

LEAKAGE: + 3.3 x 10<sup>-14</sup> A

LINEARITY: within +/- 0.1% of full scale or the precision of the reading, whichever is greater

## CHARGE CALIBRATION FACTOR:

PROBE SELECTOR	EXPOSURE LEVEL	FACTOR (C/unit of reading)
B	MEDIUM	2.162 x 10 <sup>-10</sup> C/RDG
B	HIGH	2.159 x 10 <sup>-10</sup> C/RDG
ELECTROMETER	MEDIUM	0.990 C/RDG
ELECTROMETER	HIGH	0.988 C/RDG

COMMENTS: \_\_\_\_\_  
 \_\_\_\_\_  
 \_\_\_\_\_

Reviewed by: Robert A. Hagg Log: E-2 Page(s) 204  
 Title: Associate Director Log: \_\_\_\_\_ Page(s) \_\_\_\_\_  
 Checked by: TWS Log: \_\_\_\_\_ Page(s) \_\_\_\_\_

## ELECTROMETER CALIBRATION

### CALIBRATION FACTORS:

C/RDG: This factor is given in coulomb/unit of reading of the electrometer on the indicated switch settings and scales. To obtain the corrected charge in coulomb, the calibration factor is applied directly to the instrument reading of the appropriate scale:

$$\text{Coulomb} = \text{TRUE RDG} \times \text{C/RDG}$$

### POLARIZING POTENTIAL:

Polarizing potential was measured using a calibrated digital voltmeter and is reported as the potential of the thimble with respect to the circuit low or guard.

### ELECTROMETER LEAKAGE:

Electrometer leakage is indicated in ampere for the indicated setting, and is the net charge in coulomb divided by the time interval in seconds.

### LINEARITY:

Linearity is specified as a percentage of the full scale. If the electrometer is nonlinear on a portion of the scale, a linearity correction factor is given. To correct for nonlinearity, the linearity correction factor is applied to the reading as follows:

$$\text{TRUE RDG} = \text{RDG} \times \text{Linearity Correction Factor}$$

#### ION COLLECTION EFFICIENCY:

The ion collection efficiency ( $A_{ion}$ )<sup>1</sup> stated in this report is based on measurements of the currents (or charges) produced in a Cobalt-60 beam with the stated exposure rate and polarizing potential and has been calculated using the two voltage method of Boag<sup>2</sup> and Greening<sup>3</sup> for continuous radiation.

$$A_{ion} = \frac{((V_1/V_2)^2 - \text{Ratio})}{((V_1/V_2)^2 - 1)}$$

where  $V_1$  = full polarizing potential

$V_2$  = reduced polarizing potential

Ratio = the current (or charge) at  $V_1$   
divided by the current  
(or charge) at  $V_2$

#### REFERENCES

1. Task Group 21, Radiation Therapy Committee, American Association of Physicists in Medicine, "A protocol for the determination of absorbed dose from high-energy photon and electron beams" Med. Phys., Vol. 10, p. 742 (1983).
2. Boag, J. W., Radiation Dosimetry, 2nd ed., edited by F. Attix and W. Roesch (Academic, New York, 1966), Vol. II.
3. Greening, J. R., Phys. Med. Biol., Vol. 9, p. 143 (1964).

## DOSIMETER SYSTEM CALIBRATION

3-9-84

## ELECTROMETER:

Mfgr: CapintecModel No. 192Serial No. 60F318

## SUBMITTED BY:

Sharlin RadiologicalAssociatesHackensack, New Jersey

## CHAMBER:

Mfgr: CapintecModel No. PR06CSerial No. C110, 6799ORIENTATION: "C" in serial no.

## SCALES, SWITCH POSITIONS, CONDITIONS:

toward sourceCOMPENSATION FACTOR: 1.00; PROBE SELECTOR: B;METER RANGE: NORMAL or EXTENDED; EXPOSURE LEVEL: MEDIUM;MODE: TOTALPOLARIZING POTENTIAL -300 VSYSTEM LEAKAGE:  $1 \times 10^{-14}$  A

Beam Quality			Exposure Rate (R/min)	SCD (cm)	CALIBRATION FACTOR	Class
HVT (mm)	H.C.	kVp				
5.10 Al	0.76	100	13.4	50	1.005 R/ RDG	II
*Co-60	-	-	58.4	74	1.057 R/RDG	II

Discharge Test Reading (refer to instruction manual) NA % of full scaleCOMMENTS: \* with polystyrene buildup capReviewed by: Thomas W. SlaneyTitle: DirectorChecked by: R.F.Log C-4 Page(s) 125Log T-4 Page(s) 117Log          Page(s)         Log          Page(s)

IONIZATION CHAMBER CALIBRATION

3-9-84

CHAMBER:

SUBMITTED BY:

Mfgr: Capintec Sharlin Radiological  
Model No. PRO6C (0.6 ml. AE plastic) Associates  
Serial No. CII0.6799 Hackensack, New Jersey

ORIENTATION/CONDITIONS: "C" in serial number toward source  
\_\_\_\_\_  
\_\_\_\_\_

ION COLLECTION EFFICIENCY ( $A_{ion}$ ): 0.999

POLARIZING POTENTIAL: -314 V CHAMBER LEAKAGE:  $-1 \times 10^{-14}$  A

Beam Quality		kVp	Exposure Rate (R/min)	SCD (cm)	CALIBRATION FACTOR	Class
HVT (mm)	H.C.					
5.10 Al	0.76	100	13.4	50	$4.650 \times 10^9$ R/C	II
*Co-60	-	-	58.4	74	$4.887 \times 10^9$ R/C	II

COMMENTS: \* with polystyrene buildup cap  
\_\_\_\_\_  
\_\_\_\_\_

Reviewed by: Robert A. Hagg Log C-4 Page(s) 125  
Title: Associate Director Log T-4 Page(s) 117  
Checked by: TLW Log \_\_\_\_\_ Page(s) \_\_\_\_\_