

Raymond W. Gize, M.D.  
Diagnostic Radiologist

PUBLIC/PDR  
030-32941  
Philip D. Godsey, M.D.  
Diagnostic Radiologist

January 12, 1998

U.S. Nuclear Regulatory Commission  
Region III  
801 Warrenville Road  
Lisle, IL 60532

RE: License #13-26451-01


To whom it may concern:

Hoosier Radiology, P.C. no longer provides Nuclear Medicine examinations at 2520 Lake Avenue, Fort Wayne, Indiana. This decision was made by the Board of Directors based upon the lack of procedure volume experienced by this corporation. The equipment was removed on December 12, 1997 by the manufacturer, G.E. Medical Systems.

Enclosed you will find documentation for the final surveys and swipe tests which were performed prior to the removal of the equipment. All sealed sources yet remain onsite in a restricted area and are checked on a weekly basis until proper disposal can take place.

Considering these facts, please contact myself or Ken Dyson, RT,CNMT regarding the necessary procedures required henceforth.

Sincerely

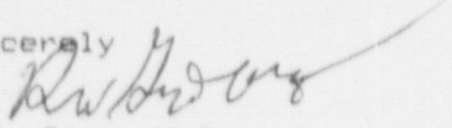  
R.W. Gize, M.D.  
President

c.: Shirley Crutchfield



9802040065 980112  
PDR ADOCK 03032941  
C PDR

Main Office  
2520 Lake Avenue • P.O. Box 5778  
Fort Wayne, Indiana 46895-5778  
(219) 424-6161 • Fax (219) 424-5746

PM: 1-19-98

RECEIVED

JAN 22 1998

REGION III

JAN 22 1998

ml  
3104

PDR ADOCK

Report date: 1/12/98

Subject: Nuclear Medicine  
Sealed sources

#1	Co 57	6.06 mci as of 11/1/92 47.11 uci as of 1/1/98 1,885 days of decay
#2	Co 57	6.18 mci as of 10/16/96 1,982 uci as of 1/1/98 440 days of decay
#3	Cs 137	220.8 uci as of 12/1/92 196.8 uci as of 1/1/98 1,885 days of decay
#4	Co 57	4.7 mci as of 12/16/93 107.7 uci as of 1/1/98 1,475 days of decay (circular flood)


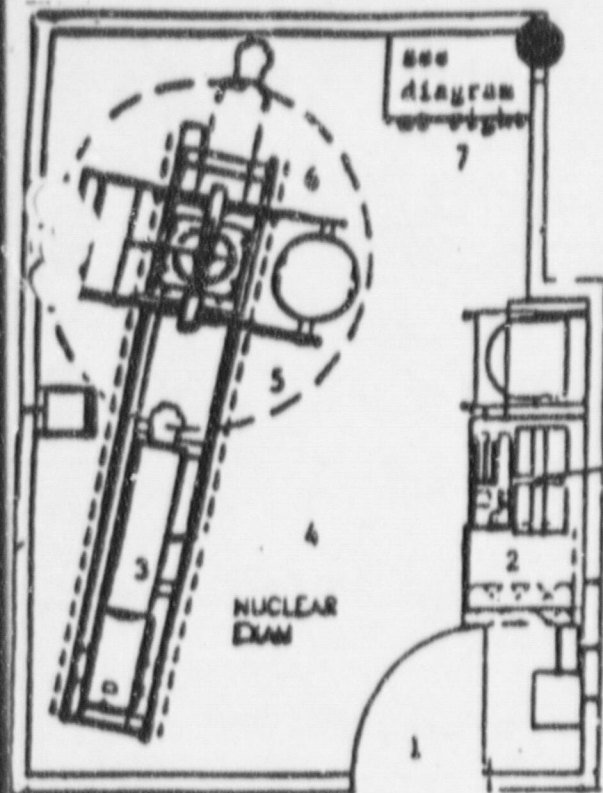


EXHIBIT 8.1

WIPE TESTING FOR THE MONTH OF Dec, 1997  
Instrument Ludlum Model 2600

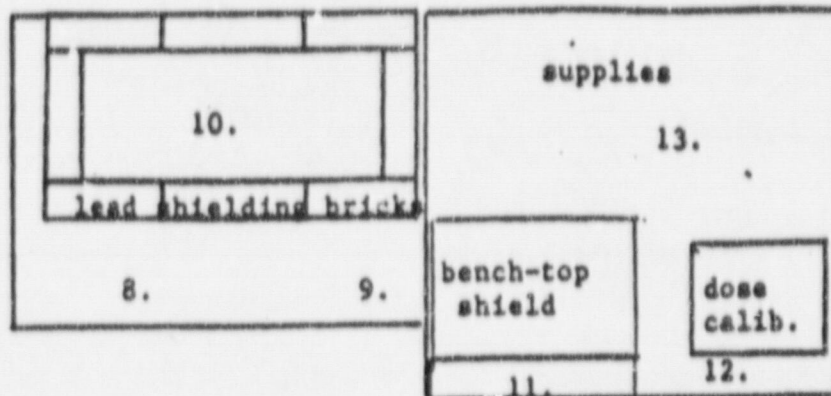

~~WELL COUNTER EFFICIENCY CALCULATIONS PER MINUTE~~

~~WELL COUNTER EFFICIENCY CALCULATIONS PER MINUTE~~


See Attachment 10.12 for Well Counter Efficiency calculations.

date	1	2	3	4	5	6	7	8	9	10	11	12	13	RM	init
12-3-97	39	44	38	37	41	42	40	45	36	37	42	43	36	39	KD
12-9-97	41	42	37	39	40	44	46	41	37	42	38	36	44	43	KD
12-11-97	36	41	39	43	40	37	41	42	38	39	44	42	37	40	KD


Re-wipes:


Final  
Survey  
to depart



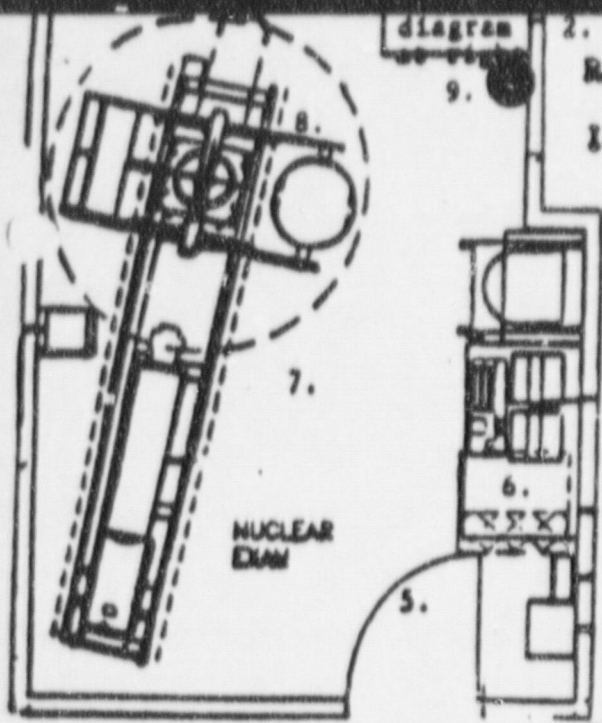

2. RADIATION SURVEY FOR THE MONTH OF Dec, 1997  
 Instrument Ludlum Model 3

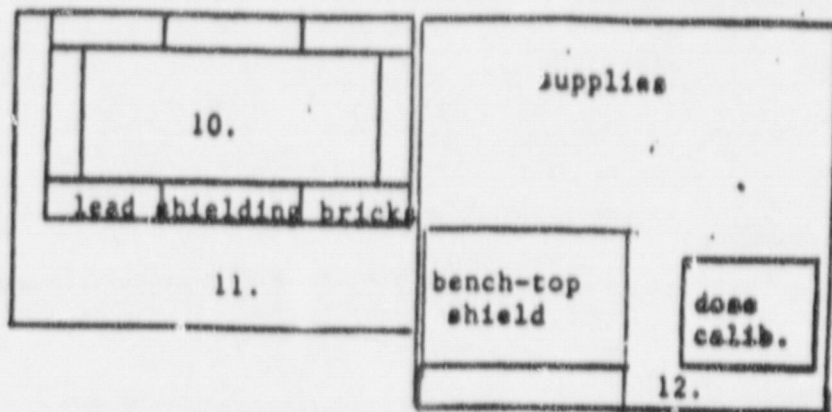

mR/hr at location

date	*	1	2	3	4	5	6	7	8	9	10	11	12	** init
1	***	.02	.02	.02	.02	.02	.02	.02	.02	.02	2.0	0.5	0.5	
2					NO	PAT								
3	1.0	.02	.02	.02	.02	.02	.02	.02	.02	.02	0.1	0.1	0.1	-KA
4					NO	PAT								
5					NO	PAT								
6														
7														
8					NO	PAT								
9	1.0	.02	.02	.02	.02	.02	.02	.02	.02	.02	0.1	0.1	0.1	✓ KD
10	1.0	.02	.02	.02	.02	.02	.02	.02	.02	.02	0.1	0.1	0.1	✓ KD
11	1.0	.02	.02	.02	.02	.02	.02	.02	.02	.02	0.1	0.1	0.1	✓ KD
12														
13														
14														
15														
16														
17														
18														
19														
20														
21														
22														
23														
24														
25														
26														
27														
28														
29														
30														

Final Survey  
 12/14/97  
 PWB

...Immediately notify KSO if you find unexpectedly high or low level.  
 \* Survey meter che. before use \*\* Survey meter che.

DATE: 1/26/98

## CORRESPONDENCE CLARIFICATION SHEET

REVIEWER:

John Madera ~~FRANKER~~ Bill R.

LICENSEE:

HOOSIER Radiology, P.C.

LICENSE NUMBER:

13-26451-01

The following correspondence has been received from the above licensee and it is not clear what action(s) is(are) required: Please review this correspondence and indicate which of the following applies, and please return to Debbie Hersey, as soon as possible.

☐ Additional Information to Control No. \_\_\_\_\_  
Process in as a new action, additional information, and no fee required.

☐ Process as new licensing action. Review has already been started on Control No. \_\_\_\_\_ and this information cannot be combined with current in-house action.

☐ Can be combined with Control No. \_\_\_\_\_. Review has not been started.

☐ Appears to be a(n) \_\_\_\_\_.

☒ Appears to be information for the license file file it.

☐ Licensee is adding Nuclear Pharmacists.  
Amendment is necessary \_\_\_\_\_. Amendment is not necessary \_\_\_\_\_.  
(Information for license file)

☐ Licensee is adding authorized users.  
A check is included \_\_\_\_\_. No check is included \_\_\_\_\_.  
Amendment is necessary \_\_\_\_\_. Amendment is not necessary \_\_\_\_\_.  
(Information for the license file)

☒ Other: Location Change

Thank You For Your Help!!!

02/02/95

WANTS TO TERMINATE, BUT STILL HAS RADIOACTIVE MATERIAL.PLEASE FILE IN LICENSE FILE.

1/24/98 - CALLED KEN DYSON AND TOLD HIM WE CANNOT TERMINATE THE LICENSE BECAUSE HE STILL HAD SERVED SOURCES CONTAINING RADIOACTIVE MATERIAL.  
(OVER)