



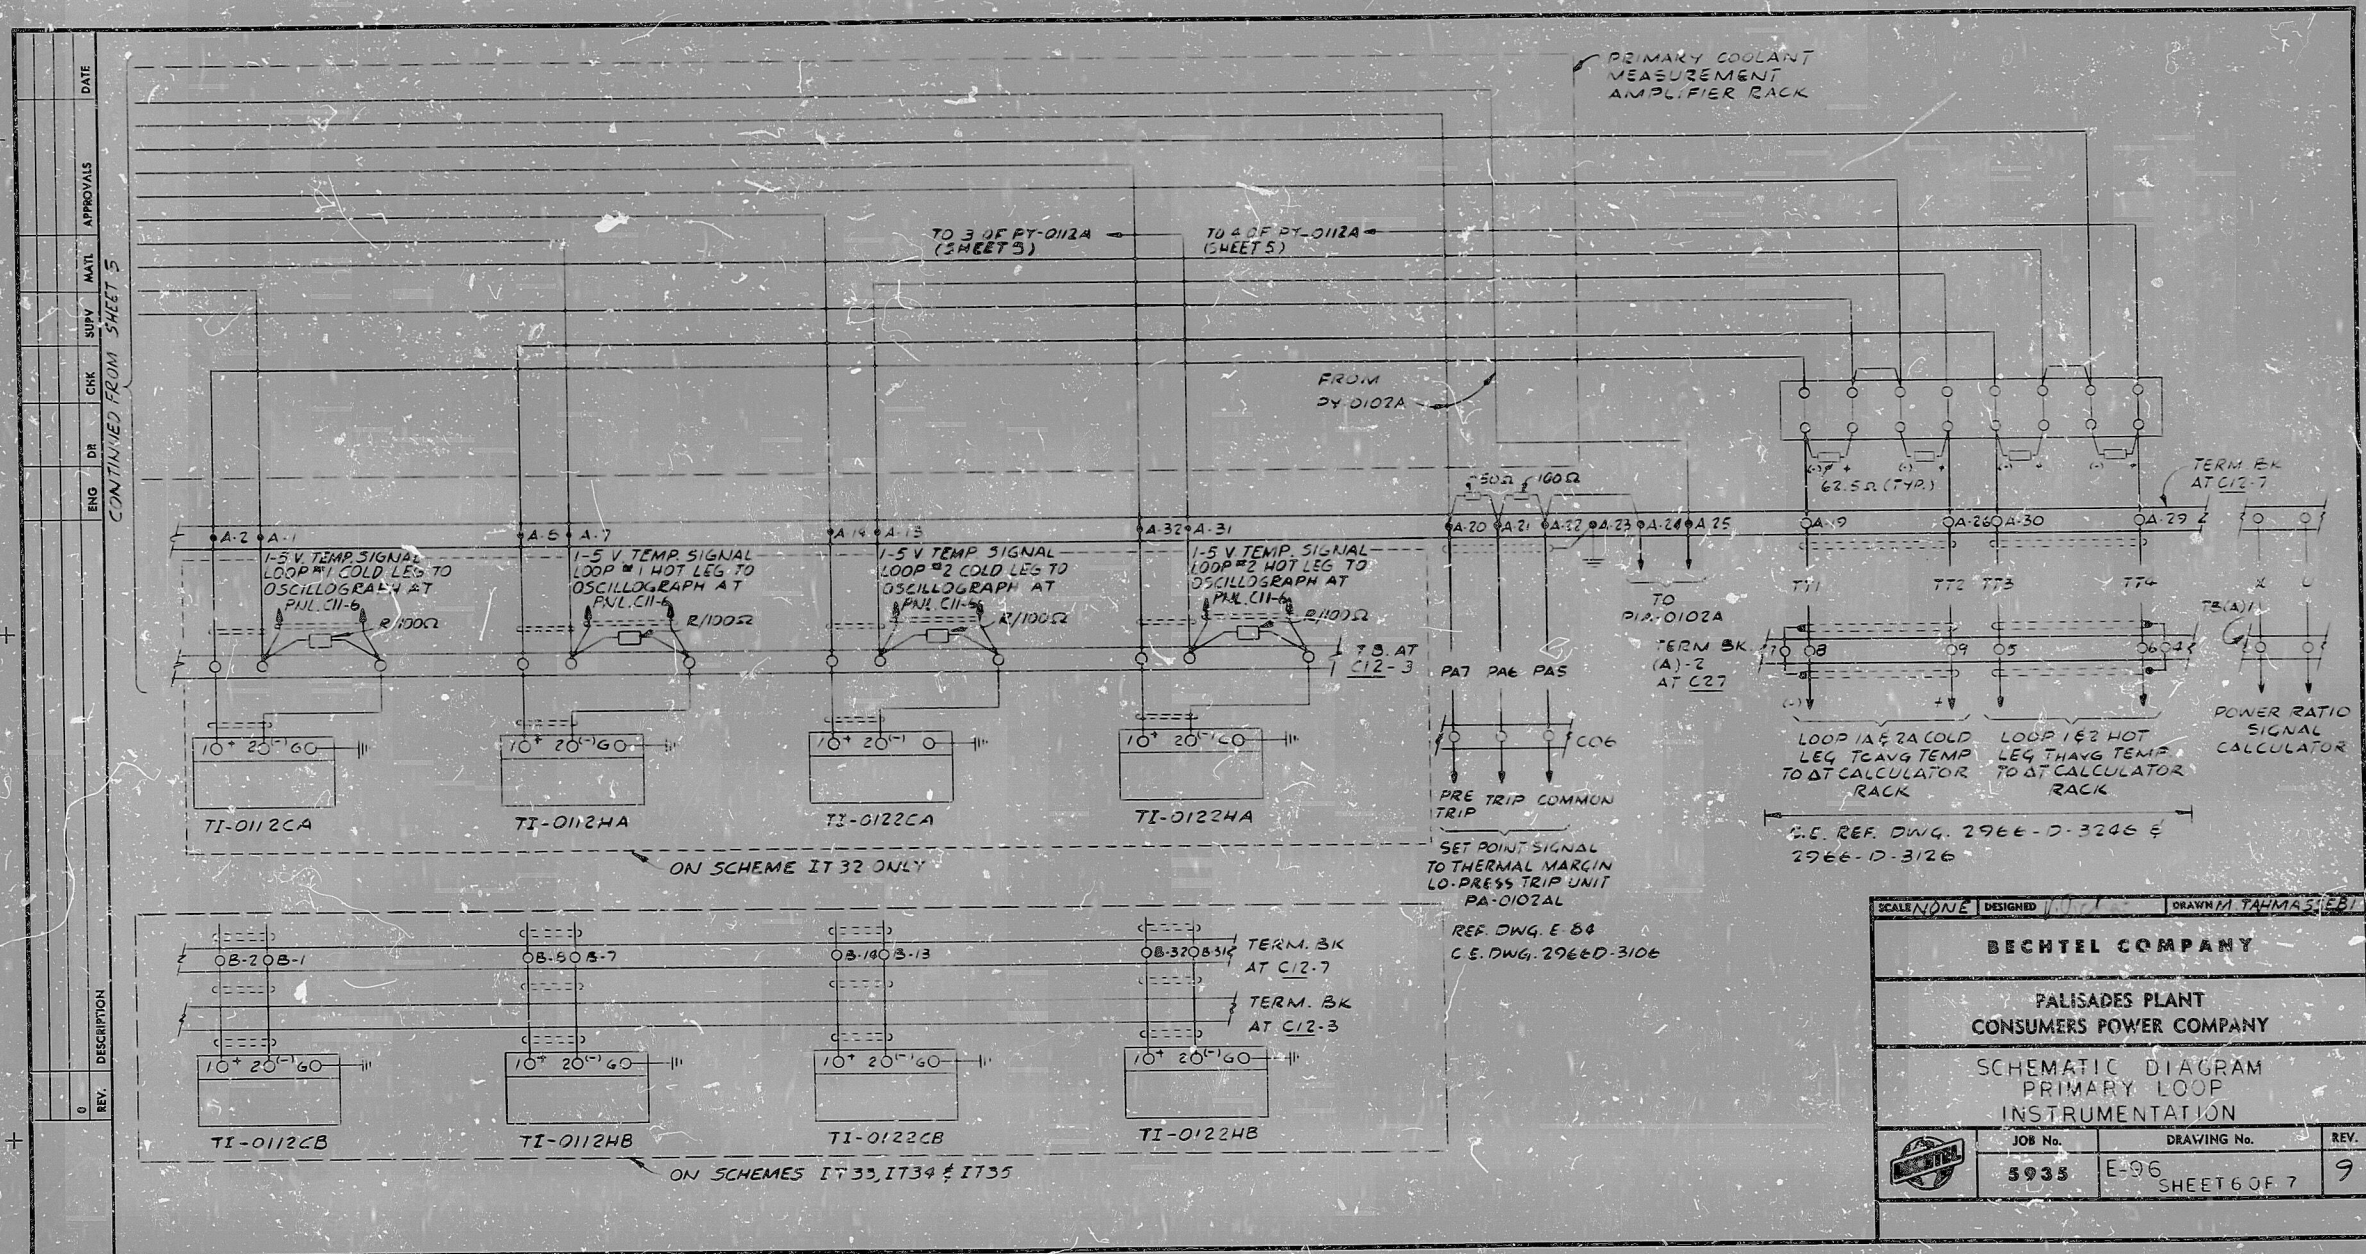

950CE 96 9 6 SCH DIAGM PRIMARY LOOP INST

741

Temp

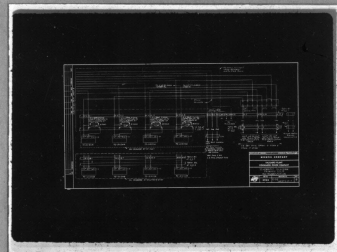

8101130513