


(Smear) (CPM/100 cm ²)					
Direct Count (CPM/Direct Frisk)					
No.	α	β	No.	α	β
1	Ø	30	26		
2	2	37	27		
3	3	35	28		
4	1	46	29		
5	Ø	32	30		
6	Ø	39	31		
7	Ø	32	32		
8	Ø	33	33		
9	Ø	30	34		
10	1	45	35		
11	Ø	44	36		
12	1	37	37		
13			38		
14			39		
15			40	N	
16			41		A
17			42		
18			43		
19	N		44		
20		A	45		
21			46		
22			47		
23			48		
24			49		
25			50		

circle one

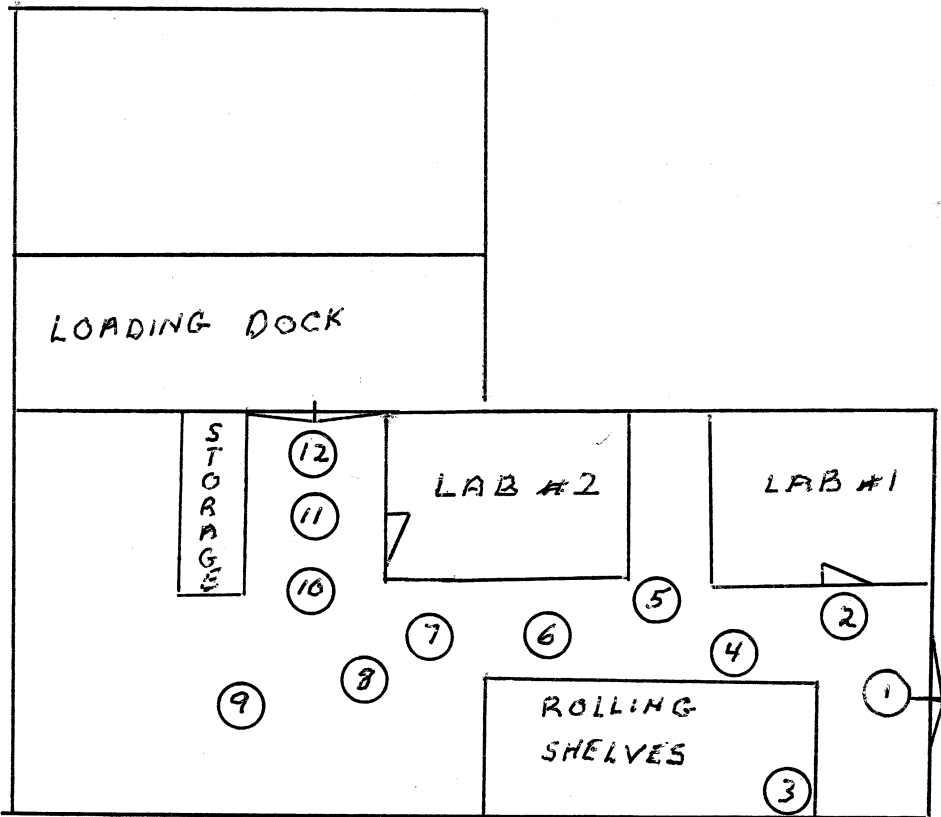

Comments	Surveyed By:	Date:	Instrument	Serial #	α Eff.	β Eff.	α Bkg.	β Bkg.	γ Bkg.	Cal. Due	Key	
SCAN FLOOR AVG 400	Larry Paulus	11/29/07	2929	142645	-	-	-	-	-	9/21/08		
MAX 800 CPM		11/29/07	44-10-1	PA156519	0.349	0.182	0.4	36.7	-	2/21/08	■ A/S Location	
		11/28/07	2360	184938	-	-	-	-	-	2/14/08	*- Boundary	
ALPHA AND BETA		11/29/07	43-37	PR178371	0.066	0.175	3	450	-	2/14/08	○ Smear	
BACKGROUND = CPM											□ Dose Rate /hr	
	Reviewed By:	Date:									* Direct Reading CPM/direct frisk	
	Nicholas Bernier	6/4/12	Original survey mis placed									△ Grab Sample