


MATERIALS LICENSE

Pursuant to the Atomic Energy Act of 1954, as amended, the Energy Reorganization Act of 1974 (Public Law 93-438), and Title 10, Code of Federal Regulations, Chapter I, Parts 30, 31, 32, 33, 34, 35, 36, 37, 39, 40, 70 and 71, and in reliance on statements and representations heretofore made by the licensee, a license is hereby issued authorizing the licensee to receive, acquire, possess, and transfer byproduct, source, and special nuclear material designated below; to use such material for the purpose(s) and at the place(s) designated below; to deliver or transfer such material to persons authorized to receive it in accordance with the regulations of the applicable Part(s). This license shall be deemed to contain the conditions specified in Section 183 of the Atomic Energy Act of 1954, as amended, and is subject to all applicable rules, regulations, and orders of the Nuclear Regulatory Commission now or hereafter in effect and to any conditions specified below.

<p style="text-align: center;">Licensee</p> <p>1. Mid-America Isotopes, Inc.</p> <p>2. 706 E. Liberty Ln. Ashland, MO 65010</p>		<p>In accordance with letter dated April 11, 2024,</p>	<p>4. Expiration Date: June 30, 2036</p>
		<p>3. License No.: 24-26241-01MD is amended in its entirety to read as follows:</p>	<p>5. Docket No.: 030-31896 Reference No.:</p>
<p>6. Byproduct, source, and/or special nuclear material</p> <p>A. Molybdenum-99</p> <p>B. Technetium-99m</p> <p>C. Iodine-131</p> <p>D. Xenon-133</p>	<p>7. Chemical and/or physical form</p> <p>A. Any</p> <p>B. Any</p> <p>C. Any</p> <p>D. Any</p>	<p>8. Maximum amount that licensee may possess at any one time under this license</p> <p>A. 90 curies total</p> <p>B. 90 curies total</p> <p>C. 1.99 curies total</p> <p>D. 2 curies total</p>	<p>9. Authorized use</p> <p>A. Preparation and distribution of radioactive drugs, including compounding of iodine-131 and redistribution of used and unused molybdenum-99/technetium-99m generators, to authorized recipients in accordance with 10 CFR 32.72. Preparation and distribution of radioactive drugs and radiochemicals, including compounding of iodine-131 and redistribution of used and unused molybdenum-99/technetium-99m generators, to authorized recipients for non-medical use.</p> <p>B. Same as Item 9.A.</p> <p>C. Same as Item 9.A.</p> <p>D. Same as Item 9.A.</p>

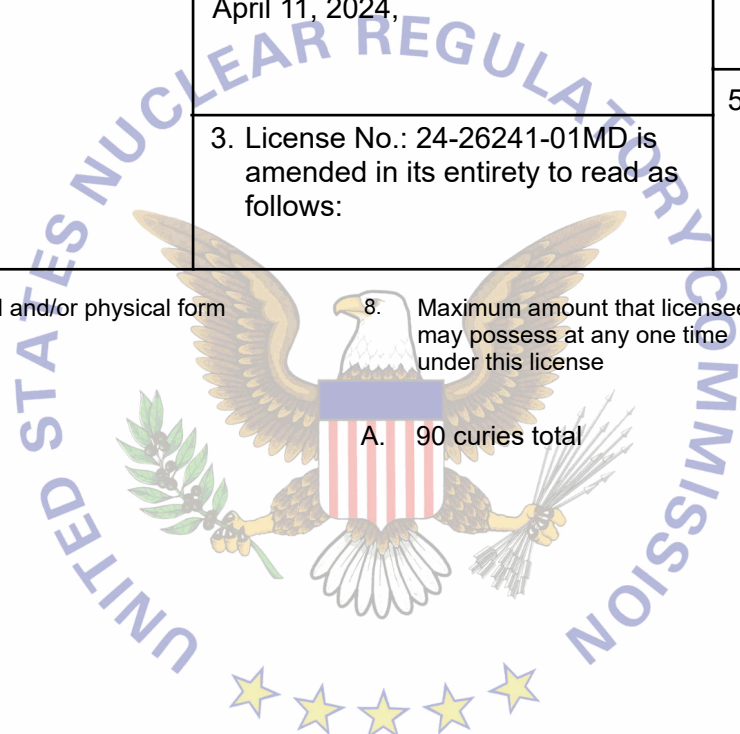

**MATERIALS LICENSE
SUPPLEMENTARY SHEET**

License No.:
24-26241-01MD

Docket or Reference No.:
030-31896

Amendment No. 26

- | | | | |
|--|----------------------------------|--|---|
| 6. Byproduct, source, and/or special nuclear material | 7. Chemical and/or physical form | 8. Maximum amount that licensee may possess at any one time under this license | 9. Authorized use |
| E. Any byproduct material with Atomic Numbers 1 through 83 with Exceptions | E. Any | E. 1.5 curies per source and 2 curies total | E. Same as Item 9.A. |
| F. Any byproduct material permitted by 10 CFR 31.11 | F. Prepackaged Kits | F. 60 millicuries total | F. Redistribution to specific licensees or general licensees pursuant to 10 CFR 31.11, provided the packaging and labeling remain unchanged. |
| G. Any byproduct material permitted by 10 CFR 35.65 | G. Sealed Sources | G. 60 millicuries total | G. Calibration and checking of the licensee's own instruments. Redistribution of sealed sources initially distributed by a manufacturer licensed pursuant to 10 CFR 32.74 to authorized recipients and to authorized recipients for non-medical use. |
| H. Any byproduct material permitted in 10 CFR 35.400 | H. Sealed Sources | H. 500 millicuries total | H. Redistribution of sealed sources initially distributed by a manufacturer licensed pursuant to 10 CFR 32.74. Redistribution of sealed sources that have been registered either with NRC under 10 CFR 32.210 or with an Agreement State and have been distributed in accordance with an NRC or Agreement State specific license authorizing distribution to persons specifically authorized by an NRC or Agreement State license to receive, possess, and use the sources. |
| I. Any byproduct material permitted by 10 CFR 35.500 | I. Sealed Sources | I. 5.5 curies total | I. Same as Item 9.H. |




**MATERIALS LICENSE
SUPPLEMENTARY SHEET**

License No.:
24-26241-01MD

Docket or Reference No.:
030-31896

Amendment No. 26

- | | | | |
|--|--|---|--|
| <p>6. Byproduct, source, and/or special nuclear material</p> | <p>7. Chemical and/or physical form</p> | <p>8. Maximum amount that licensee may possess at any one time under this license</p> | <p>9. Authorized use</p> |
| <p>J. Uranium- depleted in Uranium-235</p> | <p>J. Metal</p> | <p>J. 201 kilograms total</p> | <p>J. Shielding for molybdenum-99/technetium-99m generators.</p> |
| <p>K. Molybdenum-99</p> | <p>K. Liquid NorthStar Mo-99/Tc-99m to be used in the RadioGenix® System</p> | <p>K. 7.5 curies per source vessel, not to exceed 30 curies total</p> | <p>K. For use of the NorthStar RadioGenix™ System Model 1.1 for preparation and distribution of radioactive drugs and radiochemicals for medical use in accordance with 10 CFR 32.72 and for non-medical use to authorized recipients.</p> |
| <p>L. Germanium-68</p> | <p>L. Any</p> | <p>L. 100 millicuries total</p> | <p>L. For use of the Eckert and Ziegler GalliaPharm™ and IRE Galli-Eo® Ge-68/Ga-68 generators to prepare Ga-68 radiopharmaceuticals for imaging and localization studies.</p> |
| <p>M. Gallium-68</p> | <p>M. Any</p> | <p>M. 100 millicuries total</p> | <p>M. For preparation and distribution of radioactive drugs in accordance with 10 CFR 32.72 and radiochemicals for non-medical use to authorized recipients.</p> |

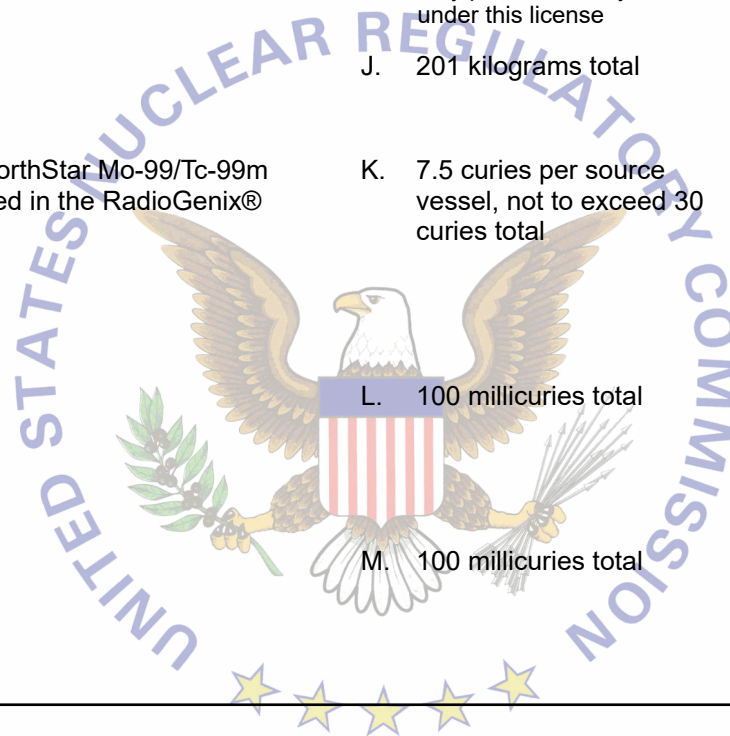

**MATERIALS LICENSE
SUPPLEMENTARY SHEET**

License No.:
24-26241-01MD

Amendment No. 26

Docket or Reference No.:
030-31896

CONDITIONS

10. Licensed material shall be used or stored at the licensee's facilities located at 706 E. Liberty Ln., Ashland, Missouri, 65010.
11. The Radiation Safety Officer (RSO) for this license is Jon W. Woodward, R.Ph.
12. Licensed material shall only be used by, or under the supervision of:
- A. A pharmacist working or designated as an authorized nuclear pharmacist in accordance with 10 CFR 32.72(b)(2)(i) or (4).
- B. Authorized Nuclear Pharmacists for all licensed material except Item 6.K.:
- | | | |
|---------------------------|------------------------------------|---------------------------------------|
| William A. Boerger, R.Ph. | Andrew N. Borrock, Pharm.D., R.Ph. | Scott C. Brower, R.Ph. |
| Bynum L. Kimmons, R.Ph. | William C. McHugh, Ph.D., R.Ph. | William Brent McHugh, Pharm.D., R.Ph. |
| David Osterberg, R.Ph. | Glen Palmer, R.Ph. | Jon W. Woodward, R.Ph. |
- C. William Brent McHugh, Pharm.D., R.Ph. and Jon W. Woodward, R.Ph. for the elution of Tc-99m from the RadioGenix™ System.
13. A. Sealed sources and detector cells shall be tested for leakage and/or contamination at intervals not to exceed the intervals specified in the certificate of registration issued by the U.S. Nuclear Regulatory Commission under 10 CFR 32.210 or by an Agreement State. In the absence of a registration certificate, sealed sources shall be tested for leakage and/or contamination at intervals not to exceed six months, or at such other intervals as specified.
- B. Notwithstanding Paragraph A of this Condition, sealed sources designed to primarily emit alpha particles shall be tested for leakage and/or contamination at intervals not to exceed three months.

**MATERIALS LICENSE
SUPPLEMENTARY SHEET**License No.:
24-26241-01MD

Amendment No. 26

Docket or Reference No.:
030-31896

- C. In the absence of a certificate from a transferor indicating that a leak test has been made within the intervals specified in the certificate of registration issued by the U.S. Nuclear Regulatory Commission under 10 CFR 32.210 or by an Agreement State, prior to the transfer, a sealed source received from another person shall not be put into use until tested and the test results received.
- D. Sealed sources need not be tested if they contain only hydrogen-3; or they contain only a radioactive gas; or the half-life of the isotope is 30 days or less; or they contain not more than 100 microcuries of beta- and/or gamma-emitting material or not more than 10 microcuries of alpha-emitting material.
- E. Sealed sources need not be tested if they are in storage and are not being used. However, when they are removed from storage for use or transferred to another person, and have not been tested within the required leak test interval, they shall be tested before use or transfer. No sealed source shall be stored for a period of more than 10 years without being tested for leakage and/or contamination.
- F. The leak test shall be capable of detecting the presence of 185 becquerels (0.005 microcuries) of radioactive material on the test sample. If the test reveals the presence of 185 becquerels (0.005 microcuries) or more of removable contamination, a report shall be filed with the U.S. Nuclear Regulatory Commission in accordance with 10 CFR 30.50(c)(2), and the source shall be removed immediately from service and decontaminated, repaired, or disposed of in accordance with Commission regulations.
- G. Tests for leakage and/or contamination, including leak test sample collection and analysis, shall be performed by the licensee or other persons specifically licensed by the U.S. Nuclear Regulatory Commission or an Agreement State to perform such services.
- H. Records of leak test results shall be kept in units of becquerels (microcuries) and shall be maintained for three years.
14. Sealed sources containing licensed material shall not be opened or sources removed from source holders by the licensee, except as specifically authorized.

**MATERIALS LICENSE
SUPPLEMENTARY SHEET**License No.:
24-26241-01MDDocket or Reference No.:
030-31896

Amendment No. 26

15. The licensee shall conduct a physical inventory every six months, or at other intervals approved by the U.S. Nuclear Regulatory Commission, to account for all sealed sources and/or devices received and possessed under the license. Records of inventories shall be maintained for three years from the date of each inventory, and shall include the radionuclides, quantities, manufacturer's name and model numbers, and the date of the inventory.
16. The licensee is authorized to hold radioactive material with a physical half-life of less than or equal to 120 days for decay-in-storage before disposal in ordinary trash provided:
- A. Before disposal as ordinary trash, the waste shall be surveyed at the container surface with the appropriate survey instrument set on its most sensitive scale and with no interposed shielding to determine that its radioactivity cannot be distinguished from background. All radiation labels shall be removed or obliterated, except for radiation labels on materials that are within containers and that will be managed as biomedical waste after they have been released from the licensee.
 - B. A record of each such disposal permitted under this license condition shall be retained for three years. The record must include the date of disposal, the date on which the byproduct material was placed in storage, the radionuclides disposed, the survey instrument used, the background dose rate, the dose rate measured at the surface of each waste container, and the name of the individual who performed the disposal.
17. Except for maintaining labeling as required by 10 CFR Part 20, or Part 71, the licensee shall obtain authorization from the U.S. Nuclear Regulatory Commission before making any changes in the sealed source, device, or source-device combination that would alter the description or specifications as indicated in the respective certificate of registration issued either by the U.S. Nuclear Regulatory Commission pursuant to 10 CFR 32.210 or by an Agreement State.

**MATERIALS LICENSE
SUPPLEMENTARY SHEET**License No.:
24-26241-01MD

Amendment No. 26

Docket or Reference No.:
030-31896

18. The licensee is authorized to retrieve, receive and dispose of radioactive waste from its customers, limited to radiopharmacy-supplied syringes and vials and their contents.
19. This license does not authorize distribution to persons exempt from licensing.
20. Notwithstanding the requirements of 10 CFR 30.35(a)(1), the licensee is exempt from the requirement to have a decommissioning funding plan needed for the possession and use of Ge-68/Ga-68 medical use generators (Eckert and Ziegler GalliaPharm™ and IRE Galli-Eo® generators), based on the commitments between the licensee and manufacturer (Eckert and Ziegler for the GalliaPharm™) and between the licensee and distributor (Cardinal Health for the Galli-Eo®). The licensee shall return the generators to the manufacturer/distributor in accordance with the generator return agreements described in the letters dated June 3, 2021 (ML21159A136) and June 17, 2021 (ML21172A011).
21. The licensee applied for and is authorized to revise its radiation safety program to:
- A. Permit revisions to existing RadioGenix® System radiation safety programs to conform to future changes in licensing guidance and additional safety recommendations from the manufacturer.
 - B. Permit individuals who have received training resulting from safety and operational changes to the RadioGenix® System to use the RadioGenix® System after these changes are made by the manufacturer.

**MATERIALS LICENSE
SUPPLEMENTARY SHEET**License No.:
24-26241-01MD

Amendment No. 26

Docket or Reference No.:
030-31896

22. Except as specifically provided otherwise in this license, the licensee shall conduct its program in accordance with the statements, representations, and procedures contained in the documents, including any enclosures, listed below. This license condition applies only to those statements, representations, and procedures that are required to be submitted in accordance with the regulations. The U.S. Nuclear Regulatory Commission's regulations shall govern unless the statements, representations, and procedures in the licensee's application and correspondence impose on the licensee requirements that are more restrictive than or in addition to the regulations.

- A. Letter dated December 27, 2020 (ML21006A384)
- B. Letter dated March 22, 2021 (ML21083A125)
- C. Letter dated June 3, 2021 (ML21159A136)
- D. Letter dated June 17, 2021 (ML21172A011)
- E. Letter dated August 31, 2023 (ML23249A157)
- F. Letter dated April 21, 2024 (ML24128A086)
- G. Letter dated May 18, 2024 (ML24143A065)



FOR THE U.S. NUCLEAR REGULATORY COMMISSION

Date: June 20, 2024

By: _____

Frank P. D. Tran
Region 3